

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030717.D
 Acq On : 22 Aug 2022 16:13
 Operator : JC/MD
 Sample : N4267-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	122948	131496	12.25%	1.548%
2	1.666	91	95	106	rVB	100194	123825	11.54%	1.457%
3	2.306	194	200	208	rBV	219428	340830	31.76%	4.011%
4	2.514	231	234	236	rBV2	644	885	0.08%	0.010%
5	2.788	274	279	289	rVB6	2628	5518	0.51%	0.065%
6	2.947	298	305	314	rVV	9350	20664	1.93%	0.243%
7	3.008	314	315	318	rVB2	532	451	0.04%	0.005%
8	3.276	357	359	362	rBV2	244	320	0.03%	0.004%
9	3.544	400	403	405	rBV2	292	367	0.03%	0.004%
10	4.050	483	486	488	rBV2	305	359	0.03%	0.004%
11	4.233	513	516	519	rBV2	368	505	0.05%	0.006%
12	4.318	528	530	532	rVB2	428	331	0.03%	0.004%
13	4.343	532	534	537	rVB2	339	336	0.03%	0.004%
14	4.398	540	543	544	rBV	322	337	0.03%	0.004%
15	4.465	544	554	567	rBV	97195	279146	26.01%	3.285%
16	4.818	610	612	617	rVB2	802	987	0.09%	0.012%
17	4.861	617	619	621	rBV	472	589	0.05%	0.007%
18	4.922	625	629	632	rVV	549	586	0.05%	0.007%
19	5.062	637	652	670	rBV	147012	446757	41.63%	5.258%
20	5.196	672	674	676	rVV2	372	349	0.03%	0.004%
21	5.233	676	680	686	rVB3	647	1328	0.12%	0.016%
22	5.477	719	720	724	rVV	432	465	0.04%	0.005%
23	5.562	726	734	743	rVB5	3339	9736	0.91%	0.115%
24	5.641	743	747	751	rBV2	518	977	0.09%	0.011%
25	5.727	758	761	762	rBV	803	611	0.06%	0.007%
26	5.769	765	768	769	rBV2	415	406	0.04%	0.005%
27	5.800	772	773	778	rBV2	373	577	0.05%	0.007%
28	5.977	789	802	816	rBV2	361968	1073109	100.00%	12.629%
29	6.379	866	868	872	rVB	357	450	0.04%	0.005%
30	6.440	875	878	879	rBV	309	437	0.04%	0.005%
31	6.544	891	895	897	rBV3	645	855	0.08%	0.010%
32	6.684	915	918	921	rVB	436	440	0.04%	0.005%
33	6.769	921	932	949	rBV	292227	704927	65.69%	8.296%
34	6.885	949	951	956	rVV2	795	1103	0.10%	0.013%
35	6.934	958	959	963	rBV3	574	830	0.08%	0.010%
36	7.111	981	988	998	rBV4	11558	28767	2.68%	0.339%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030717.D
 Acq On : 22 Aug 2022 16:13
 Operator : JC/MD
 Sample : N4267-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1037	rBV	228191	495854	46.21%	5.836%
38	7.488	1046	1050	1051	rBV2	1015	1148	0.11%	0.014%
39	7.574	1062	1064	1068	rVB2	386	360	0.03%	0.004%
40	7.647	1074	1076	1078	rVB	419	335	0.03%	0.004%
41	7.665	1078	1079	1082	rBV	482	497	0.05%	0.006%
42	7.775	1094	1097	1098	rVV2	363	348	0.03%	0.004%
43	7.873	1112	1113	1118	rBV2	346	379	0.04%	0.004%
44	7.934	1118	1123	1130	rBV3	2371	4773	0.44%	0.056%
45	8.068	1142	1145	1146	rBV	537	418	0.04%	0.005%
46	8.257	1173	1176	1177	rBV2	571	486	0.05%	0.006%
47	8.275	1177	1179	1181	rVB	545	441	0.04%	0.005%
48	8.330	1181	1188	1197	rBV	153596	258037	24.05%	3.037%
49	8.415	1200	1202	1203	rVV2	718	486	0.05%	0.006%
50	8.476	1207	1212	1220	rVB4	1464	3009	0.28%	0.035%
51	8.653	1234	1241	1252	rBV	539989	843577	78.61%	9.928%
52	8.793	1262	1264	1268	rVB3	455	541	0.05%	0.006%
53	8.830	1268	1270	1273	rBV2	372	479	0.04%	0.006%
54	8.952	1285	1290	1300	rBV	112745	165283	15.40%	1.945%
55	9.086	1310	1312	1315	rVB2	390	348	0.03%	0.004%
56	9.202	1330	1331	1335	rVB2	438	326	0.03%	0.004%
57	9.281	1340	1344	1346	rBV3	1909	2571	0.24%	0.030%
58	9.384	1356	1361	1374	rBV	434859	616331	57.43%	7.254%
59	9.622	1398	1400	1403	rVB2	506	483	0.05%	0.006%
60	9.665	1406	1407	1410	rVV2	435	475	0.04%	0.006%
61	9.708	1410	1414	1419	rVV2	1920	2869	0.27%	0.034%
62	9.799	1427	1429	1431	rBV	471	366	0.03%	0.004%
63	9.823	1431	1433	1436	rBV	475	496	0.05%	0.006%
64	9.866	1439	1440	1442	rBV	627	348	0.03%	0.004%
65	10.055	1465	1471	1478	rBV	603965	809539	75.44%	9.527%
66	10.311	1509	1513	1514	rBV3	825	815	0.08%	0.010%
67	10.421	1527	1531	1534	rBV2	399	631	0.06%	0.007%
68	10.537	1547	1550	1552	rVV	377	347	0.03%	0.004%
69	10.604	1558	1561	1563	rBV2	421	607	0.06%	0.007%
70	10.738	1579	1583	1585	rBV2	370	593	0.06%	0.007%
71	10.805	1591	1594	1595	rVB2	440	401	0.04%	0.005%
72	10.957	1616	1619	1620	rBV2	551	411	0.04%	0.005%
73	10.976	1620	1622	1623	rVB2	739	510	0.05%	0.006%
74	11.085	1636	1640	1643	rVV2	453	765	0.07%	0.009%
75	11.195	1652	1658	1665	rBV	443730	570957	53.21%	6.720%
76	11.500	1706	1708	1710	rVB2	803	600	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
 Data File : VX030717.D
 Acq On : 22 Aug 2022 16:13
 Operator : JC/MD
 Sample : N4267-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.695	1737	1740	1743	rBV	450	864	0.08%	0.010%
78	11.768	1746	1752	1755	rVV2	710	976	0.09%	0.011%
79	11.841	1762	1764	1766	rVB2	378	325	0.03%	0.004%
80	11.945	1779	1781	1784	rBV2	294	381	0.04%	0.004%
81	12.024	1789	1794	1805	rVB	639352	762579	71.06%	8.975%
82	12.323	1837	1843	1850	rBV	592996	752824	70.15%	8.860%
83	12.518	1873	1875	1878	rBV2	612	590	0.05%	0.007%
84	12.768	1912	1916	1919	rBV3	1353	2008	0.19%	0.024%
85	12.811	1919	1923	1925	rVB	289	320	0.03%	0.004%
86	12.945	1941	1945	1948	rBV	594	663	0.06%	0.008%
87	13.481	2030	2033	2034	rBV2	359	354	0.03%	0.004%
88	13.597	2046	2052	2053	rBV3	428	635	0.06%	0.007%
89	13.701	2066	2069	2072	rBV2	475	451	0.04%	0.005%
90	13.780	2079	2082	2083	rBV3	470	426	0.04%	0.005%
91	13.871	2095	2097	2100	rBV2	364	463	0.04%	0.005%
92	13.951	2109	2110	2112	rBV2	396	374	0.03%	0.004%
93	14.134	2136	2140	2145	rBV2	1597	1900	0.18%	0.022%
94	14.201	2149	2151	2152	rBV	560	459	0.04%	0.005%
95	14.335	2172	2173	2176	rBV2	654	432	0.04%	0.005%
96	14.725	2235	2237	2238	rBV2	603	394	0.04%	0.005%
97	14.877	2260	2262	2263	rBV2	885	601	0.06%	0.007%
98	14.938	2270	2272	2274	rBV2	707	522	0.05%	0.006%
99	15.219	2316	2318	2321	rBV	666	548	0.05%	0.006%
100	15.597	2378	2380	2384	rVB2	1233	919	0.09%	0.011%


Sum of corrected areas: 8496904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030717.D
Acq On : 22 Aug 2022 16:13
Operator : JC/MD
Sample : N4267-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

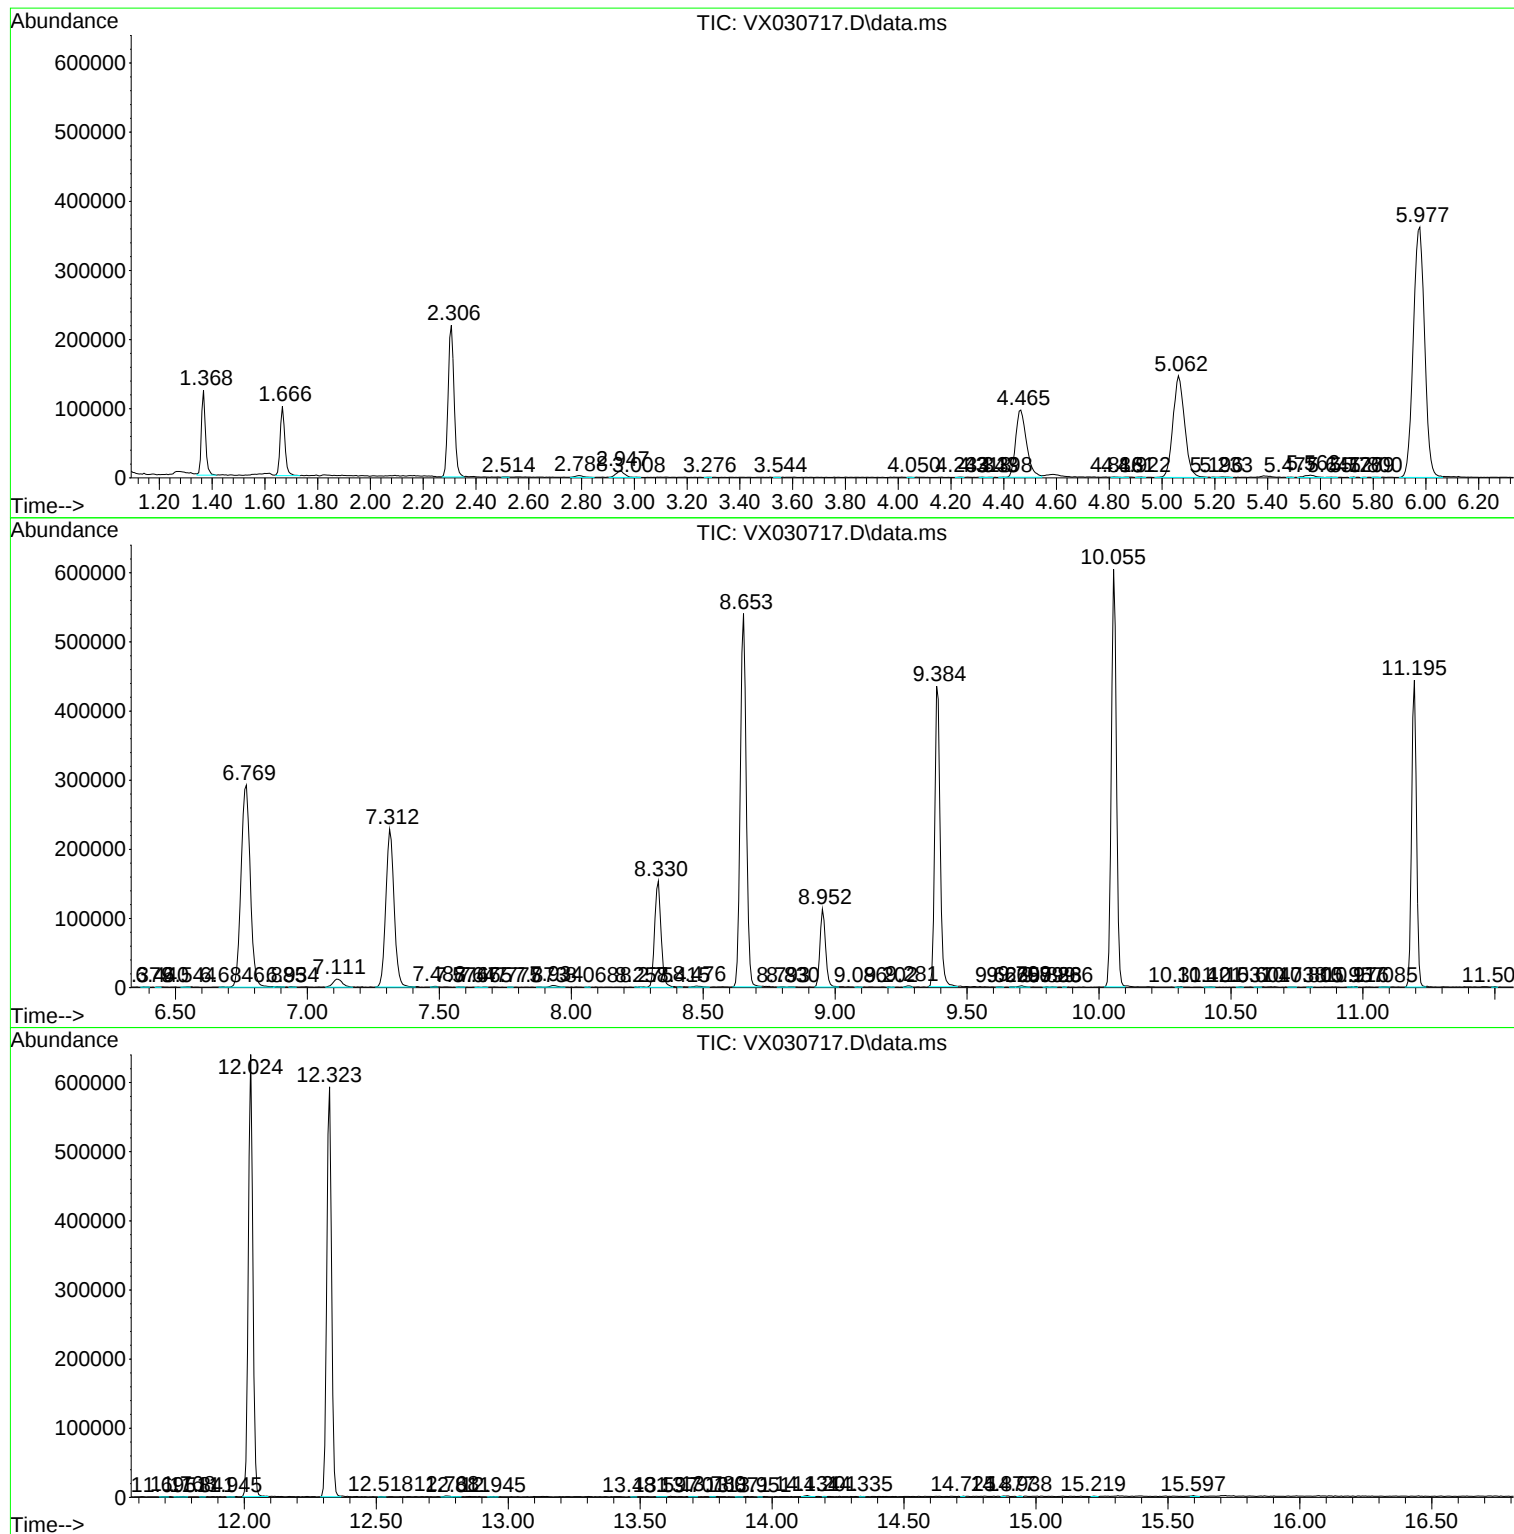

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030717.D
Acq On : 22 Aug 2022 16:13
Operator : JC/MD
Sample : N4267-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030717.D
Acq On : 22 Aug 2022 16:13
Operator : JC/MD
Sample : N4267-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc