
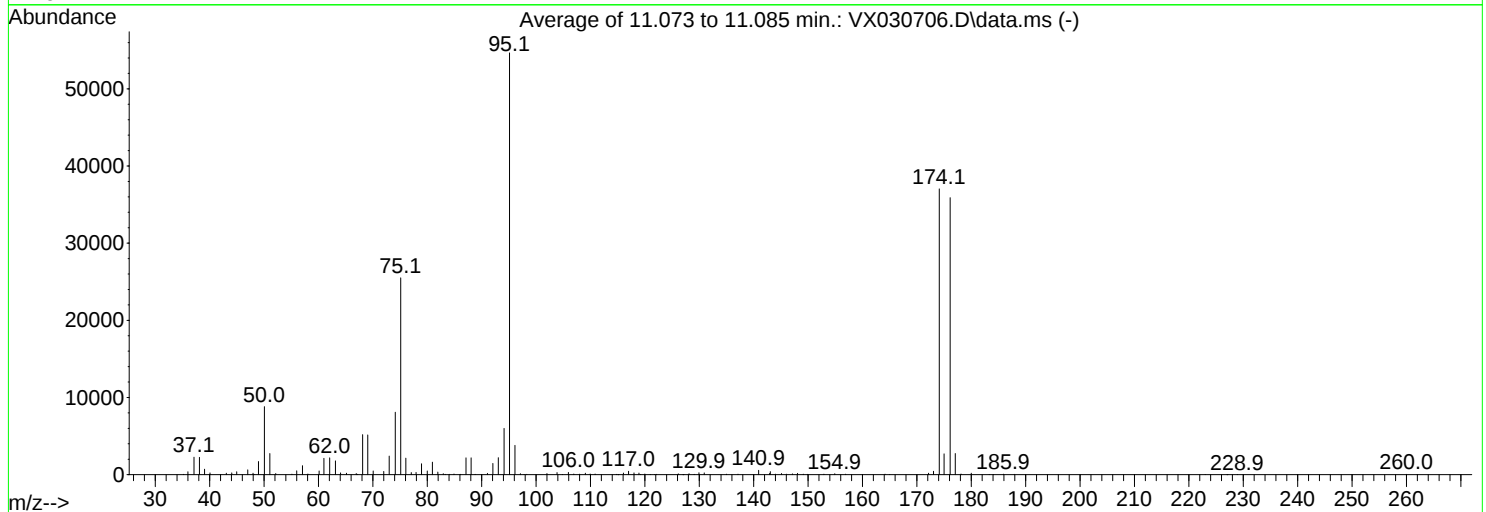


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082222\
Data File : VX030706.D
Acq On : 22 Aug 2022 08:47
Operator : JC/MD
Sample : BFB684
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB684

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Title : VOC Analysis
Last Update : Tue Aug 23 02:05:32 2022

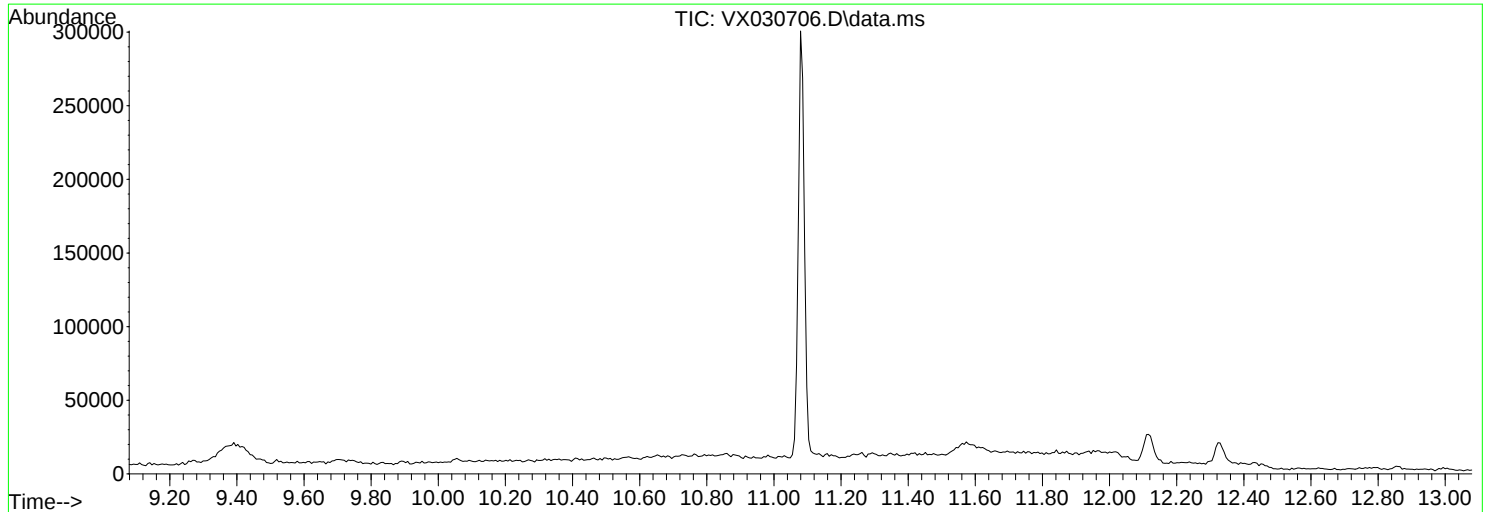

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	8804	PASS
75	95	30	80	46.7	25506	PASS
95	95	100	100	100.0	54667	PASS
96	95	5	9	6.9	3787	PASS
173	174	0.00	2	1.2	445	PASS
174	95	50	120	67.7	37029	PASS
175	174	5	9	7.3	2688	PASS
176	174	95	101	96.9	35888	PASS
177	176	5	9	7.6	2728	PASS

m/z	Abundance
36.00	72.0
37.10	65.0
38.90	138.0
40.10	407.0
41.00	317.0
43.10	143.0
44.10	676.0
45.00	107.0
46.90	87.0
48.10	64.0
48.90	80.0
49.90	131.0
50.90	108.0
55.10	220.0
56.10	203.0
57.10	213.0
61.00	71.0
62.80	64.0
64.20	215.0
65.90	60.0
69.20	154.0
71.10	154.0
72.90	186.0
74.20	240.0
75.20	137.0
76.10	137.0
77.10	130.0
78.30	60.0
81.20	132.0
84.10	96.0
86.10	79.0
91.10	213.0
93.80	58.0
95.10	141.0
95.70	54.0
97.20	61.0
102.00	93.0
104.90	87.0
108.00	115.0
108.90	318.0
111.10	69.0
115.10	109.0
118.00	80.0
119.20	94.0
120.00	57.0
126.20	88.0
127.10	239.0
128.10	1276.0
129.10	246.0
131.20	153.0
133.00	151.0
145.20	206.0
146.10	96.0
146.90	202.0
180.00	454.0
182.00	561.0
184.10	205.0
192.10	64.0
223.10	100.0
224.90	204.0
227.00	131.0
257.90	66.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

m/z	Abundance
36.00	370.0
37.10	1937.0
38.00	1939.0
39.10	731.0
40.00	754.0
41.00	277.0
42.00	76.0
43.00	346.0
44.00	917.0
45.00	376.0
47.00	594.0
47.90	255.0
49.00	1642.0
50.10	7185.0
51.10	2157.0
52.20	156.0
55.10	313.0
56.00	639.0
57.10	978.0
58.10	79.0
60.10	318.0
61.00	2066.0
62.00	1793.0
63.10	1276.0
64.00	361.0
65.20	161.0
67.00	208.0
68.10	4611.0
69.00	3977.0
70.10	342.0
71.00	110.0
71.90	154.0
73.00	2019.0
74.10	6876.0
75.10	20592.0
76.10	1876.0
77.10	387.0
78.00	312.0
78.90	1054.0
80.00	377.0
80.90	1234.0
81.90	248.0
83.10	112.0
84.10	160.0
86.10	76.0
87.10	1876.0
88.00	1729.0
88.80	156.0
91.00	270.0
92.00	1030.0
93.10	1539.0
94.10	4189.0
95.10	41360.0
96.10	2591.0
97.20	155.0
102.00	273.0
103.90	109.0
104.80	70.0
106.00	201.0
106.90	66.0
107.90	145.0
108.90	249.0
109.90	95.0
111.20	106.0
115.10	230.0
116.00	166.0
117.00	293.0
118.00	272.0
118.90	252.0
120.10	82.0
122.10	53.0
126.20	73.0
126.90	229.0
128.10	1331.0
129.10	161.0
130.10	116.0
130.80	162.0
133.10	110.0
140.90	421.0
142.90	431.0
145.10	464.0
146.00	166.0
146.90	150.0
148.00	111.0
152.90	101.0
156.90	55.0
164.20	114.0
172.10	96.0
173.20	256.0
174.10	23008.0
175.00	1691.0
176.10	21968.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

177.10	1730.0
178.10	106.0
180.00	698.0
182.10	482.0
183.30	56.0
184.00	196.0
185.90	73.0
223.10	146.0
224.90	192.0
227.00	107.0
262.00	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

m/z	Abundance
35.20	71.0
36.10	609.0
37.10	2741.0
38.10	2905.0
39.10	1223.0
40.00	615.0
41.10	362.0
43.10	307.0
44.10	887.0
45.00	520.0
47.10	1105.0
48.20	340.0
49.00	1797.0
50.10	11103.0
51.10	3577.0
52.10	171.0
55.20	282.0
56.00	752.0
57.00	1622.0
58.10	124.0
60.10	548.0
61.10	2593.0
62.10	3096.0
63.10	2269.0
63.90	533.0
65.10	258.0
67.20	146.0
68.10	6068.0
69.10	6494.0
69.90	340.0
70.20	308.0
71.10	120.0
72.00	567.0
73.00	3398.0
74.10	10346.0
75.10	31816.0
76.10	2853.0
77.10	461.0
77.90	357.0
79.00	1768.0
80.00	613.0
81.00	2042.0
81.90	356.0
82.90	262.0
84.00	144.0
84.90	97.0
86.00	155.0
87.10	2316.0
88.10	2766.0
91.10	547.0
92.00	1990.0
93.00	2610.0
94.10	7384.0
95.10	66616.0
96.10	4662.0
97.10	206.0
97.80	59.0
102.10	158.0
103.80	314.0
104.90	109.0
106.00	439.0
107.00	119.0
108.00	192.0
109.10	259.0
110.00	81.0
110.80	107.0
111.30	84.0
114.90	115.0
116.10	278.0
117.10	363.0
118.10	347.0
118.90	375.0
120.00	141.0
121.80	67.0
126.20	246.0
127.00	281.0
128.20	1622.0
129.00	347.0
129.90	320.0
130.90	269.0
137.20	88.0
140.90	700.0
143.10	498.0
144.00	144.0
145.20	250.0
146.00	152.0
147.10	213.0
148.00	175.0
149.10	131.0
152.90	81.0
154.90	223.0
156.80	67.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

164.10	62.0
172.20	251.0
173.00	608.0
174.10	42480.0
175.00	2854.0
176.10	41600.0
177.00	3262.0
178.10	66.0
180.10	641.0
182.10	530.0
184.00	245.0
185.90	88.0
222.90	94.0
225.00	119.0
227.10	164.0
228.90	59.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

m/z	Abundance
35.20	79.0
36.10	346.0
37.10	2280.0
38.20	1902.0
39.20	567.0
40.10	532.0
41.10	262.0
43.00	321.0
44.00	902.0
44.90	575.0
47.00	453.0
48.00	321.0
49.00	1881.0
50.10	8516.0
51.10	2779.0
52.10	109.0
55.20	273.0
56.00	713.0
57.00	1500.0
58.00	69.0
60.10	572.0
61.00	1880.0
62.10	1669.0
63.10	1805.0
64.10	413.0
65.20	139.0
66.90	222.0
68.10	4884.0
69.10	5434.0
70.10	439.0
70.90	137.0
72.00	499.0
73.10	2371.0
74.10	7743.0
75.10	24520.0
76.00	2107.0
77.00	338.0
77.90	216.0
78.90	1430.0
80.00	430.0
80.90	1573.0
82.00	395.0
83.30	131.0
84.00	140.0
84.90	134.0
86.10	144.0
87.10	2317.0
88.10	2029.0
91.00	319.0
92.10	1352.0
93.10	2476.0
94.10	6436.0
95.10	56448.0
96.10	4107.0
97.00	211.0
98.30	115.0
101.90	295.0
103.90	359.0
104.90	128.0
105.90	247.0
106.90	79.0
108.10	202.0
109.00	275.0
110.00	68.0
110.90	147.0
114.80	109.0
116.00	191.0
116.90	625.0
117.90	293.0
119.20	345.0
119.90	205.0
121.00	50.0
122.20	76.0
126.10	226.0
127.10	211.0
128.20	1262.0
129.00	370.0
129.90	311.0
131.00	247.0
133.10	153.0
135.00	178.0
137.00	128.0
140.90	574.0
143.00	684.0
144.00	60.0
145.00	367.0
146.10	174.0
147.10	125.0
148.10	203.0
149.10	69.0
149.90	136.0
154.90	167.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

157.00	96.0
165.00	53.0
172.20	239.0
173.00	471.0
174.10	45600.0
175.00	3520.0
176.10	44096.0
177.10	3191.0
178.10	105.0
180.00	569.0
182.00	619.0
184.10	231.0
187.90	106.0
192.00	56.0
222.90	98.0
224.90	206.0
227.00	148.0
260.00	131.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684