

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082223\
Data File : VX037162.D
Acq On : 22 Aug 2023 19:19
Operator : JC/MD
Sample : 04051-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20230816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	26	30	58	rBV	45434	220089	16.31%	6.128%
2	2.324	197	203	213	rBV3	45649	89294	6.62%	2.486%
3	5.391	690	706	720	rBV	46414	140110	10.39%	3.901%
4	5.556	722	733	745	rVV2	48408	134310	9.96%	3.740%
5	5.958	789	799	814	rBV	59996	160655	11.91%	4.473%
6	6.763	922	931	944	rBV	95601	228492	16.94%	6.362%
7	7.128	981	991	1005	rBV	624667	1349098	100.00%	37.565%
8	8.652	1234	1241	1250	rBV	201524	326762	24.22%	9.099%
9	10.055	1465	1471	1481	rBV	244616	321543	23.83%	8.953%
10	11.079	1634	1639	1652	rBV	214145	275812	20.44%	7.680%
11	12.024	1788	1794	1803	rBV	270704	345171	25.59%	9.611%




Sum of corrected areas: 3591336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082223\
Data File : VX037162.D
Acq On : 22 Aug 2023 19:19
Operator : JC/MD
Sample : 04051-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20230816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

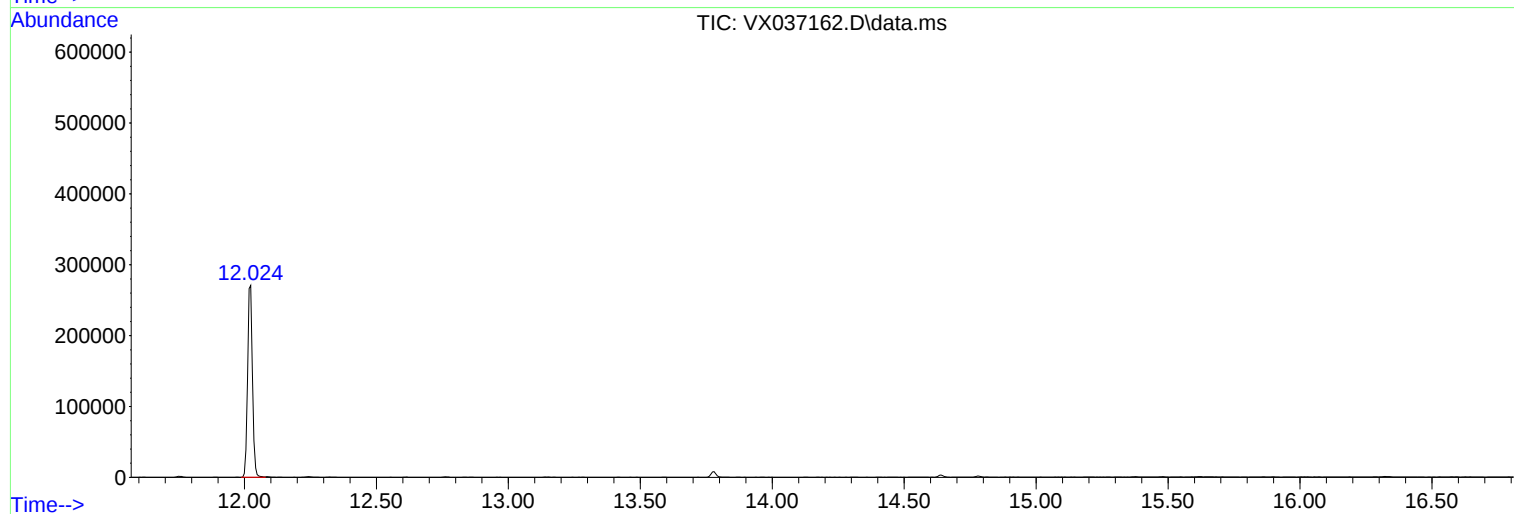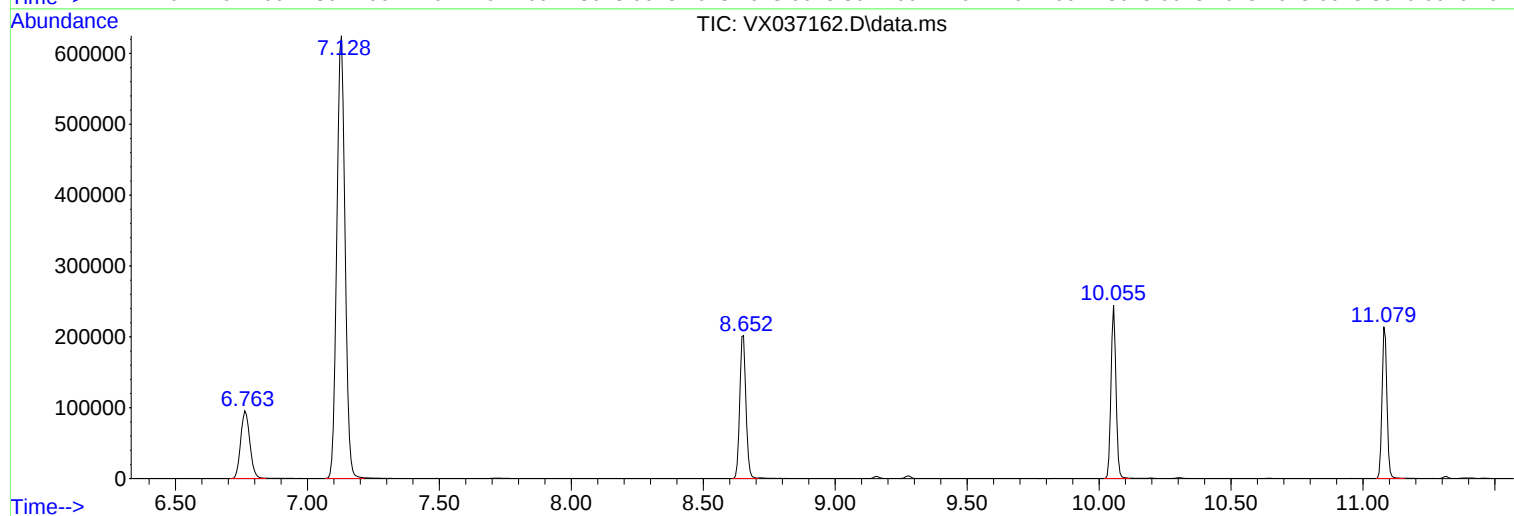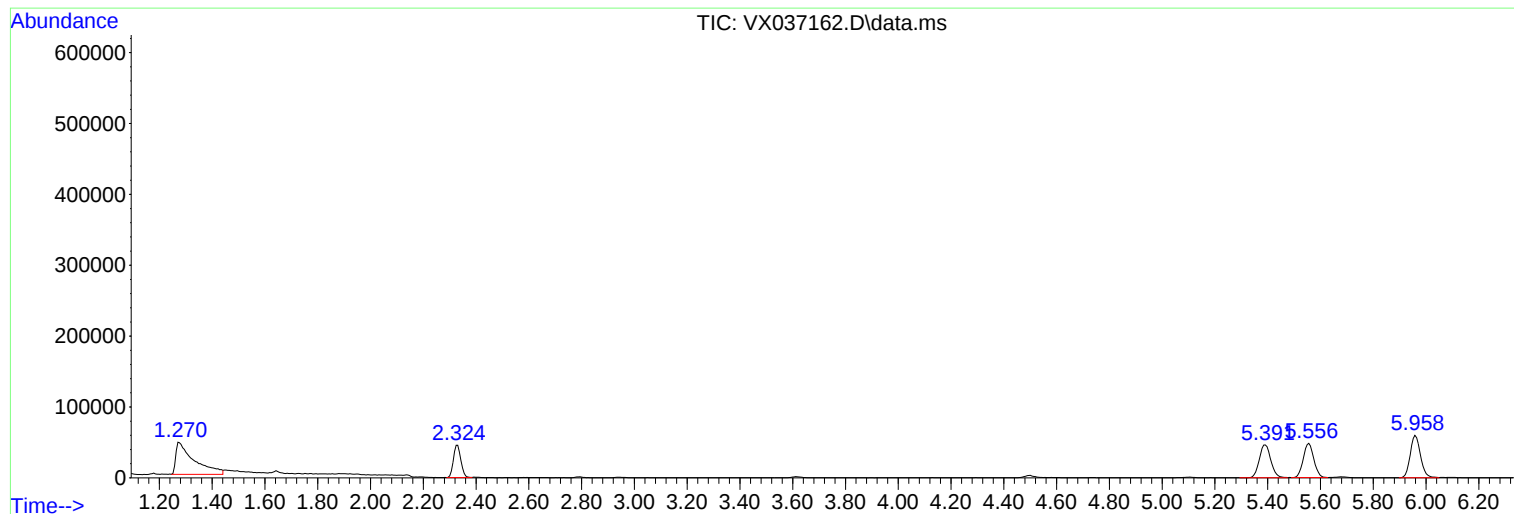

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082223\
Data File : VX037162.D
Acq On : 22 Aug 2023 19:19
Operator : JC/MD
Sample : 04051-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20230816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082223\
Data File : VX037162.D
Acq On : 22 Aug 2023 19:19
Operator : JC/MD
Sample : 04051-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20230816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------