
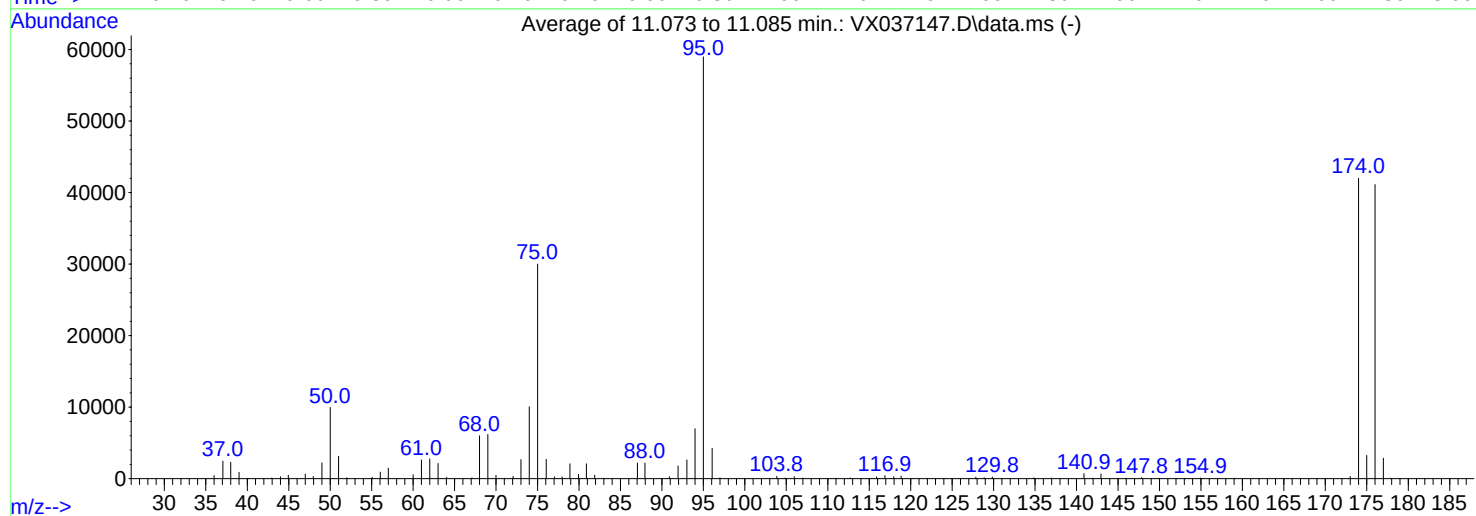


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082223\
 Data File : VX037147.D
 Acq On : 22 Aug 2023 12:01
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260
 Last Update : Fri Aug 18 09:30:38 2023

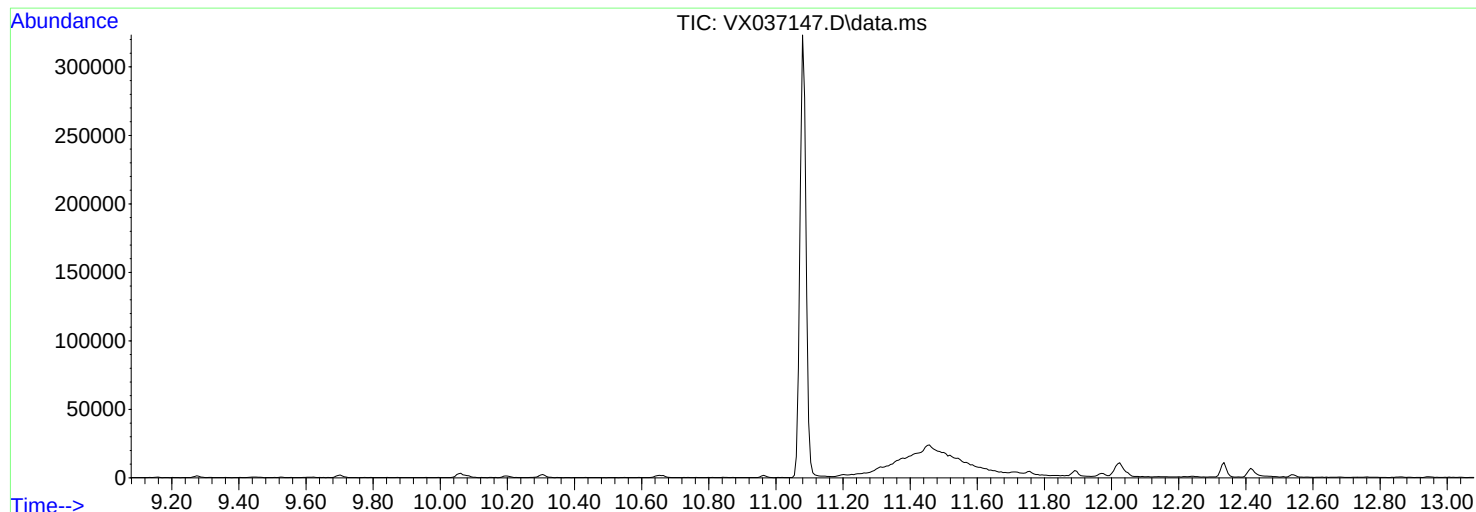

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	9947	PASS
75	95	30	60	50.9	30008	PASS
95	95	100	100	100.0	58973	PASS
96	95	5	9	7.2	4218	PASS
173	174	0.00	2	0.7	304	PASS
174	95	50	100	71.2	41997	PASS
175	174	5	9	7.7	3251	PASS
176	174	95	101	97.9	41117	PASS
177	176	5	9	6.9	2854	PASS