

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082225\
 Data File : VX047502.D
 Acq On : 22 Aug 2025 16:46
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: Aug 25 01:30:44 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	244196	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	502580	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	499075	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	249141	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	210374	61.556	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	123.120%#
35) Dibromofluoromethane	5.397	113	178757	54.803	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.600%
50) Toluene-d8	8.653	98	622818	53.422	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	106.840%
62) 4-Bromofluorobenzene	11.079	95	253759	58.983	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	117.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082225\
Data File : VX047502.D
Acq On : 22 Aug 2025 16:46
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: Aug 25 01:30:44 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




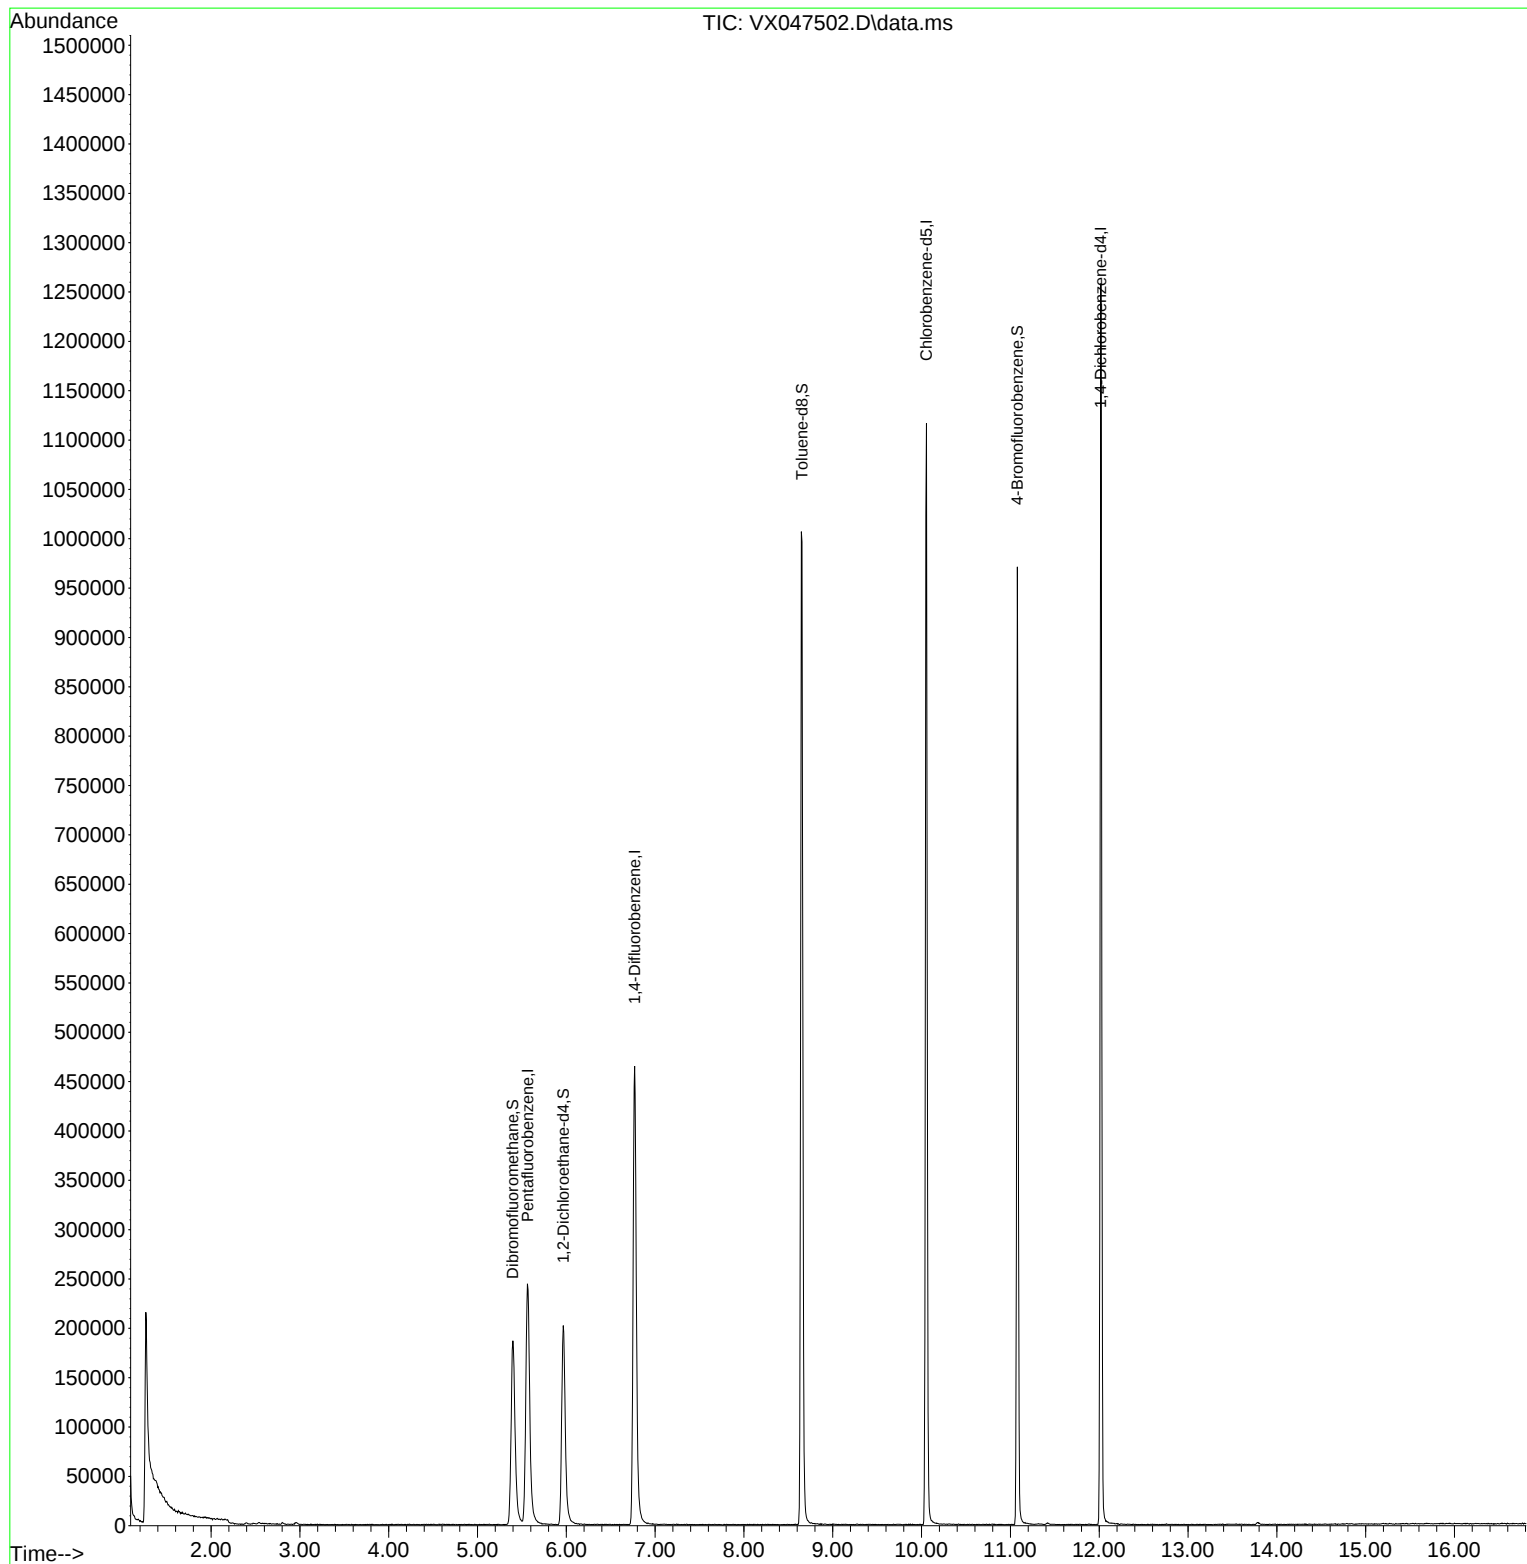


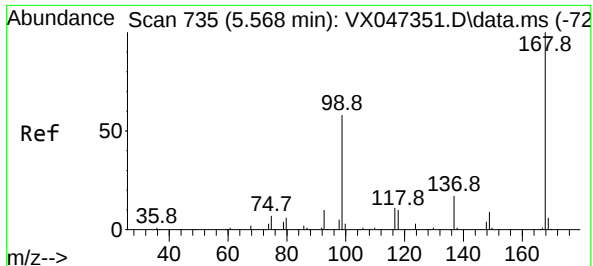

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 244196
Ion Ratio Lower Upper
168 100
99 60.6 47.9 71.9

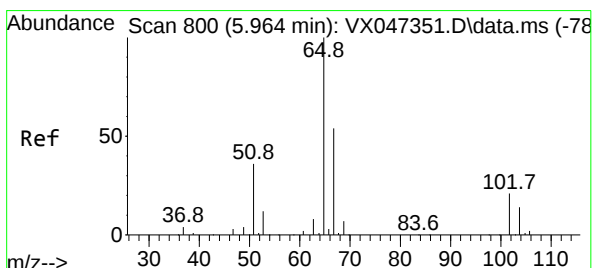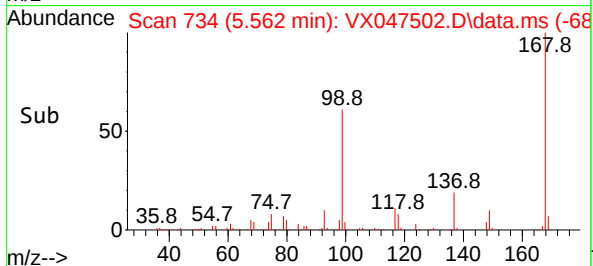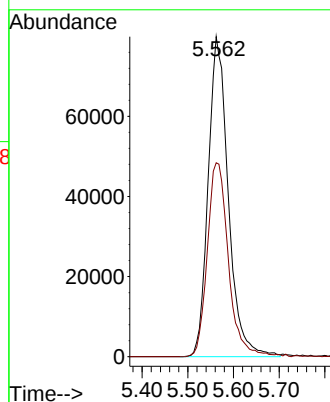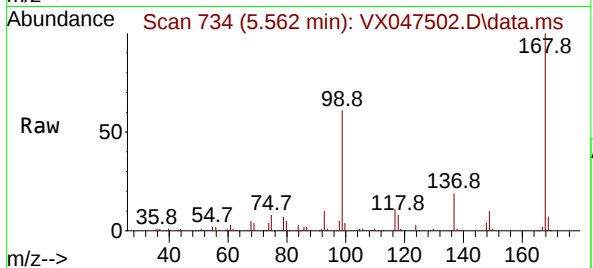

#33
1,2-Dichloroethane-d4
Concen: 61.556 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46

Tgt Ion: 65 Resp: 210374
Ion Ratio Lower Upper
65 100
67 52.7 0.0 106.0


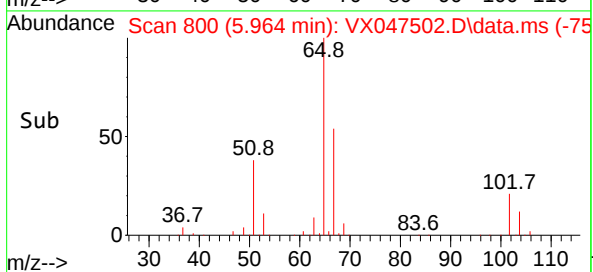
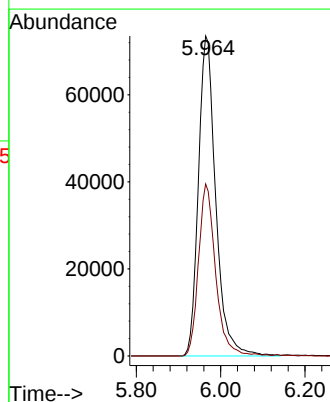
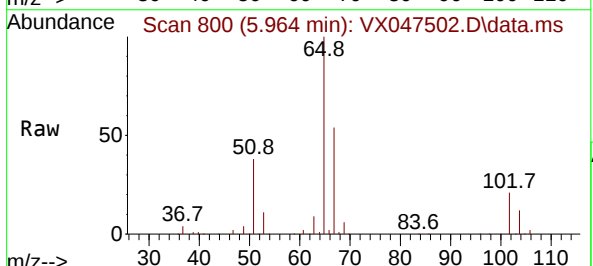


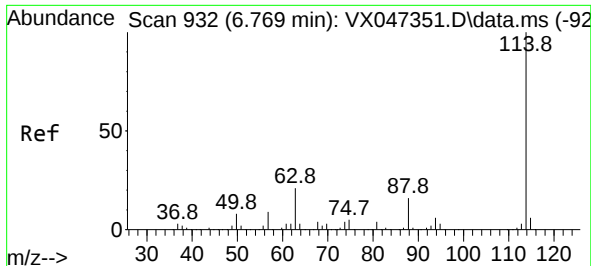

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 502580
Ion Ratio Lower Upper
114 100
63 22.4 0.0 42.4
88 16.5 0.0 33.0

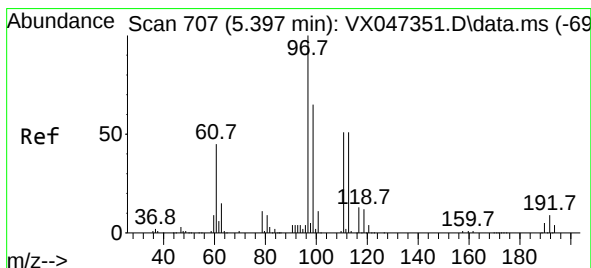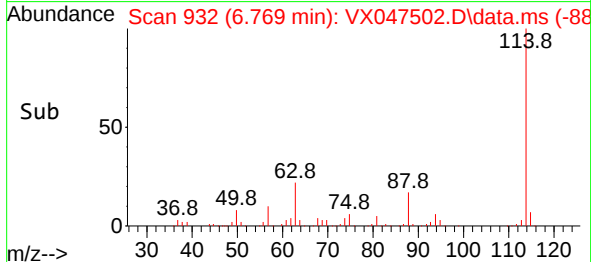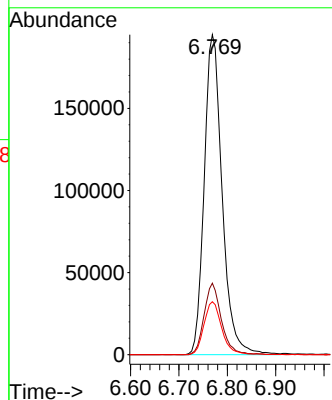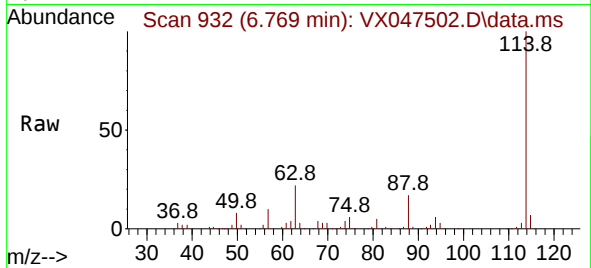

#35
Dibromofluoromethane
Concen: 54.803 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46

Tgt Ion:113 Resp: 178757
Ion Ratio Lower Upper
113 100
111 102.6 81.4 122.2
192 17.9 14.1 21.1


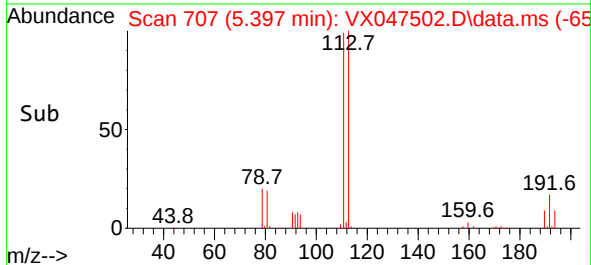
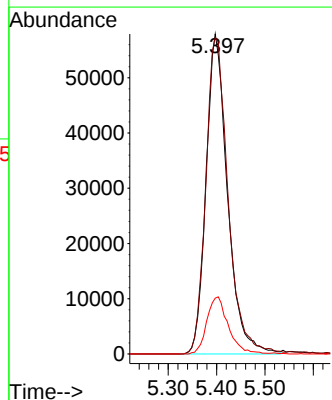
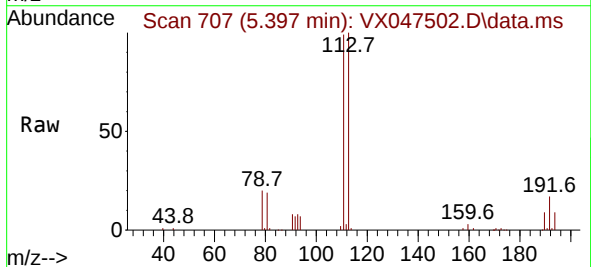


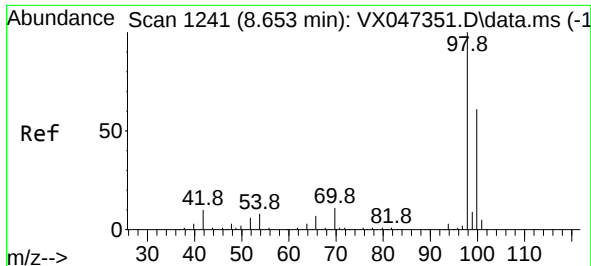

#50
Toluene-d8
Concen: 53.422 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 622818
Ion Ratio Lower Upper
98 100
100 65.7 53.9 80.9

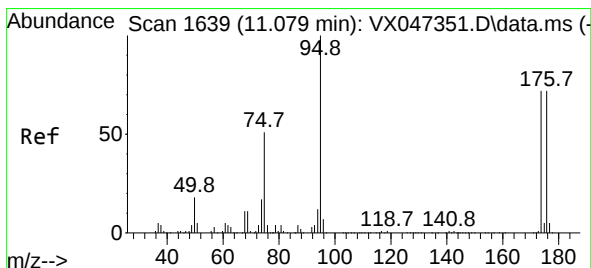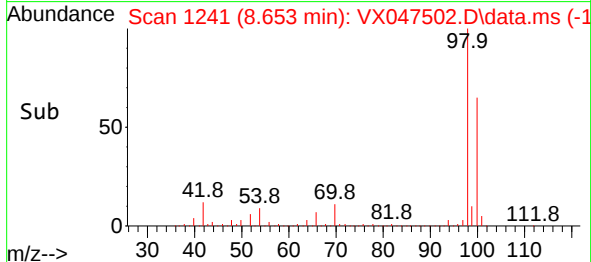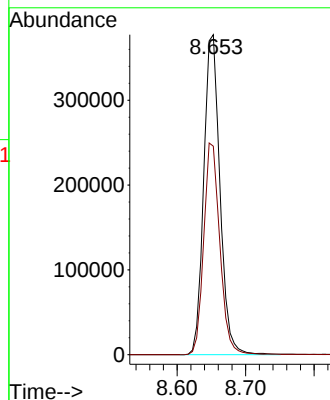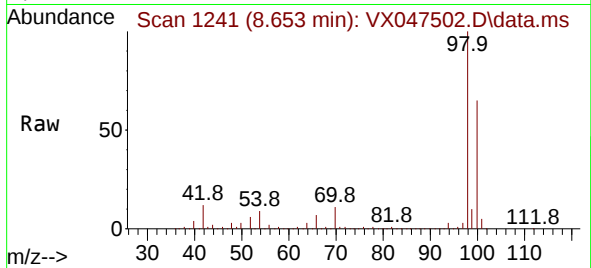

#62
4-Bromofluorobenzene
Concen: 58.983 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46

Tgt Ion: 95 Resp: 253759
Ion Ratio Lower Upper
95 100
174 73.8 0.0 148.0
176 71.2 0.0 145.4


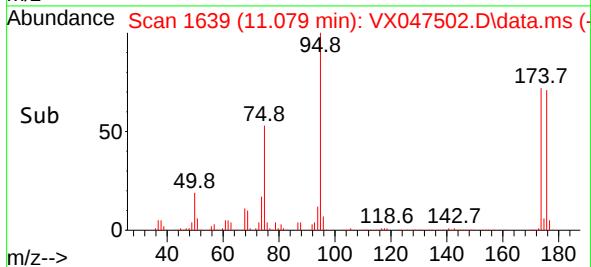
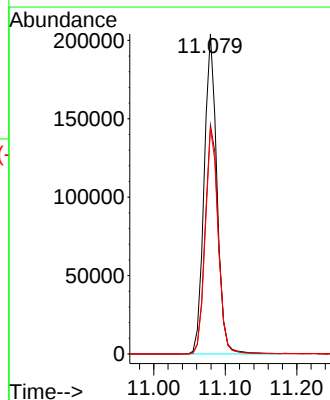
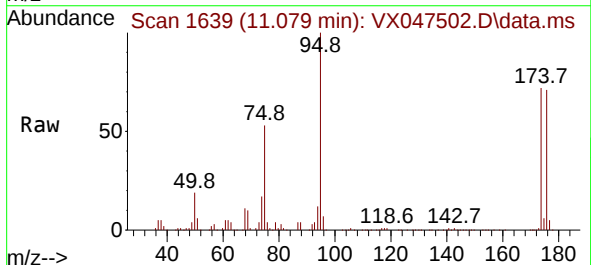


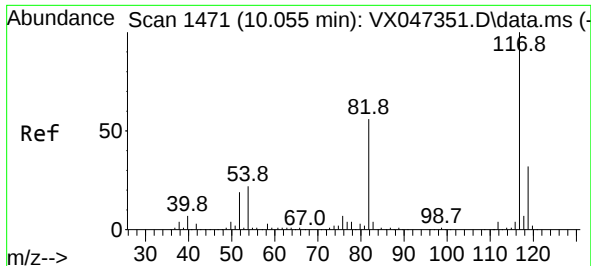

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 499075
Ion Ratio Lower Upper
117 100
82 56.4 45.0 67.4
119 32.6 25.8 38.8

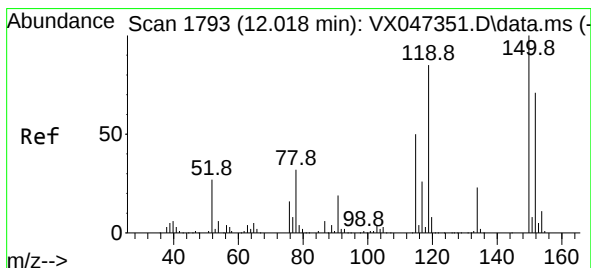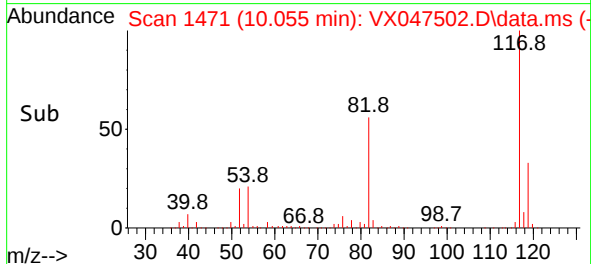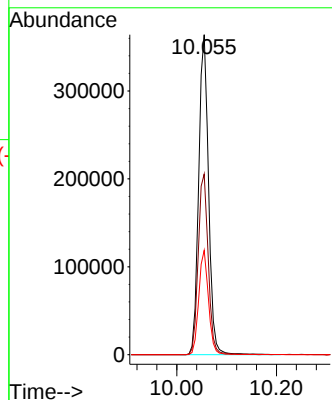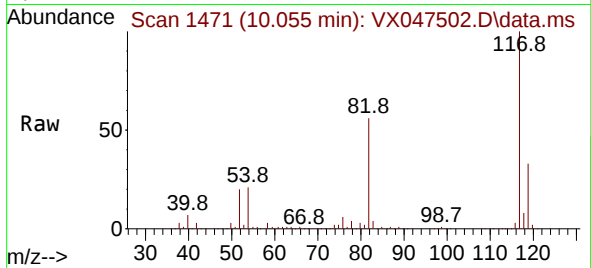

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX047502.D
Acq: 22 Aug 2025 16:46

Tgt Ion:152 Resp: 249141
Ion Ratio Lower Upper
152 100
115 62.1 44.6 133.8
150 158.3 0.0 349.8

