

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082318\
 Data File : VX004229.D
 Acq On : 23 Aug 2018 16:19
 Operator : JC/MD
 Sample : J4295-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 OUTFALL

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	75	80	92	rBV	1255040	1692368	95.35%	13.476%
2	1.166	93	95	108	rVB3	41513	64046	3.61%	0.510%
3	1.483	144	147	153	rVB	77474	87507	4.93%	0.697%
4	1.605	160	167	169	rBV5	10534	21999	1.24%	0.175%
5	1.636	169	172	177	rVB	15088	19032	1.07%	0.152%
6	1.995	227	231	238	rVB	13671	19796	1.12%	0.158%
7	2.349	284	289	299	rBV	18582	32406	1.83%	0.258%
8	2.447	299	305	313	rVB	151699	253005	14.25%	2.015%
9	2.886	372	377	386	rVB2	9961	20454	1.15%	0.163%
10	3.154	413	421	432	rVB3	13864	44740	2.52%	0.356%
11	3.416	458	464	472	rVB3	7889	18819	1.06%	0.150%
12	3.513	474	480	488	rVB2	12278	27704	1.56%	0.221%
13	3.672	499	506	516	rVB2	17673	43845	2.47%	0.349%
14	4.099	568	576	587	rVB2	16666	42693	2.41%	0.340%
15	4.355	606	618	621	rBV2	17068	46021	2.59%	0.366%
16	4.708	667	676	696	rVB	27741	81944	4.62%	0.653%
17	5.501	790	806	822	rBV2	207426	609002	34.31%	4.850%
18	5.659	822	832	848	rVB	303258	867225	48.86%	6.906%
19	6.068	888	899	915	rBV	221948	577665	32.55%	4.600%
20	6.860	1020	1029	1048	rVB	469305	1092399	61.55%	8.699%
21	7.366	1101	1112	1119	rBV5	8281	22590	1.27%	0.180%
22	7.458	1119	1127	1135	rVB2	15526	35957	2.03%	0.286%
23	7.555	1135	1143	1148	rBV	21800	43242	2.44%	0.344%
24	7.665	1156	1161	1167	rVB	17142	30170	1.70%	0.240%
25	8.653	1317	1323	1327	rBV	56880	89583	5.05%	0.713%
26	8.714	1327	1333	1341	rVB	1154100	1774957	100.00%	14.134%
27	9.500	1455	1462	1470	rVB2	14455	21650	1.22%	0.172%
28	9.586	1470	1476	1480	rBV	31145	44181	2.49%	0.352%
29	10.116	1552	1563	1572	rBV	918945	1263994	71.21%	10.065%
30	10.250	1580	1585	1591	rBV	38468	53648	3.02%	0.427%
31	10.360	1596	1603	1610	rVV	108899	151744	8.55%	1.208%
32	10.433	1610	1615	1620	rVV5	11736	18531	1.04%	0.148%
33	10.701	1655	1659	1665	rBV2	38905	60645	3.42%	0.483%
34	10.829	1675	1680	1689	rBV	20691	33020	1.86%	0.263%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082318\
Data File : VX004229.D
Acq On : 23 Aug 2018 16:19
Operator : JC/MD
Sample : J4295-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OUTFALL

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260

35	10.915	1689	1694	1705	rVB	21343	31389	1.77%	0.250%
36	11.140	1725	1731	1739	rBV	993448	1248262	70.33%	9.940%
37	11.360	1760	1767	1772	rBV	13136	18954	1.07%	0.151%
38	11.433	1775	1779	1782	rBV	31653	49420	2.78%	0.394%
39	11.506	1787	1791	1794	rVV	21598	32126	1.81%	0.256%
40	11.536	1794	1796	1806	rVB	14065	20374	1.15%	0.162%
41	11.671	1814	1818	1822	rVB	18004	23496	1.32%	0.187%
42	11.811	1835	1841	1847	rVB	62003	82093	4.63%	0.654%
43	11.896	1851	1855	1860	rBV	17227	22778	1.28%	0.181%
44	11.981	1866	1869	1873	rBV2	15447	18264	1.03%	0.145%
45	12.079	1879	1885	1891	rBV	1266464	1520779	85.68%	12.110%
46	12.140	1891	1895	1900	rVB	17491	23187	1.31%	0.185%
47	12.274	1912	1917	1920	rBV	27074	37221	2.10%	0.296%
48	12.378	1929	1934	1942	rVB4	8715	19983	1.13%	0.159%
49	12.914	2017	2022	2030	rBV2	15723	21391	1.21%	0.170%
50	13.658	2137	2144	2151	rBV4	9597	17871	1.01%	0.142%
51	13.835	2168	2173	2180	rVB	24119	34982	1.97%	0.279%
52	14.694	2308	2314	2321	rBV	18516	28823	1.62%	0.230%


Sum of corrected areas: 12557975

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX082318\
Data File : VX004229.D
Acq On : 23 Aug 2018 16:19
Operator : JC/MD
Sample : J4295-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OUTFALL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

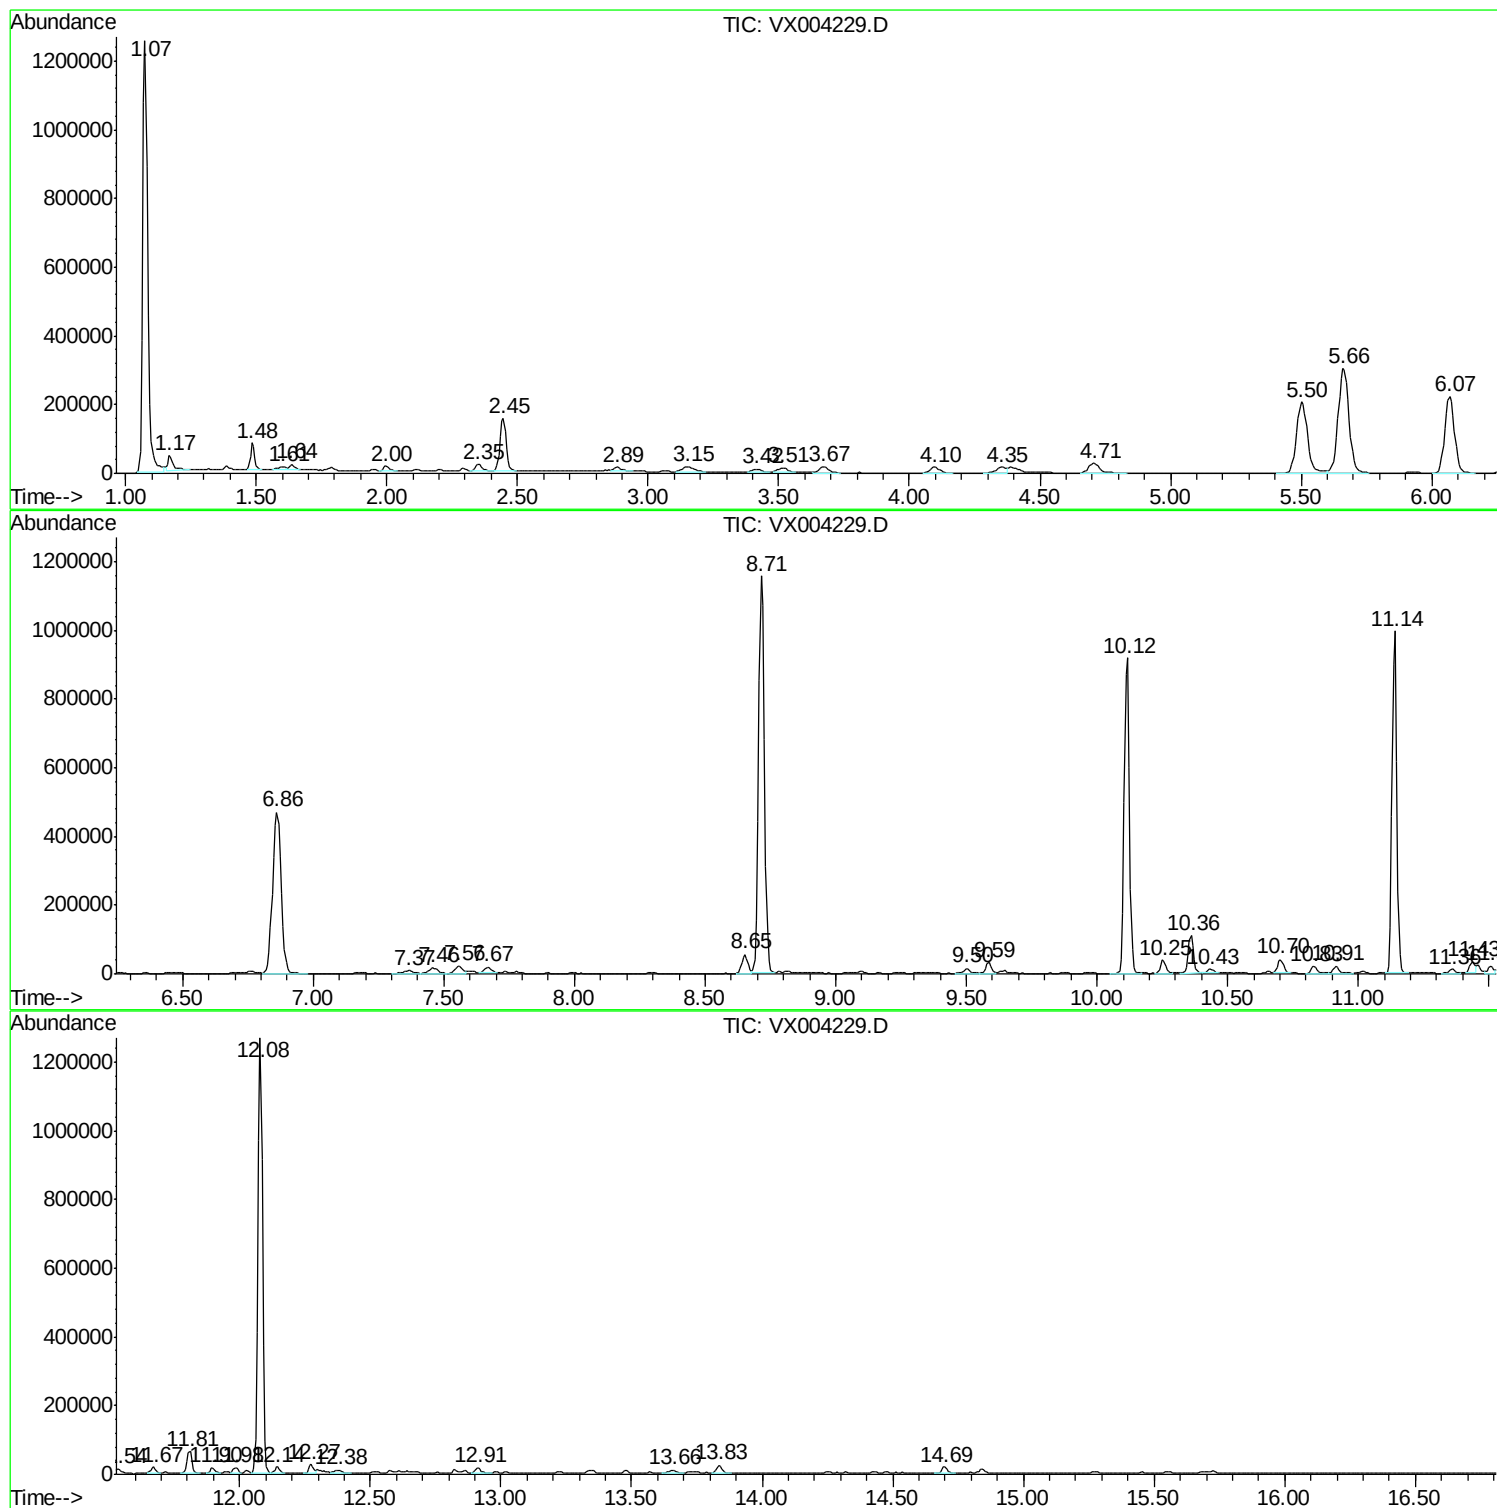

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX082318\
Data File : VX004229.D
Acq On : 23 Aug 2018 16:19
Operator : JC/MD
Sample : J4295-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OUTFALL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX082318\
Data File : VX004229.D
Acq On : 23 Aug 2018 16:19
Operator : JC/MD
Sample : J4295-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OUTFALL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc