

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082319\
 Data File : VX011795.D
 Acq On : 23 Aug 2019 14:06
 Operator : JC/SP
 Sample : K4388-19
 Misc : 5.77g/5mL/100uL/10mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 T6-E3-(0)

Quant Time: Aug 26 02:27:54 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082219W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 23 01:48:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	457040	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	613355	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	552735	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	299886	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.05	65	206841	45.05	ug/l	0.00
Spiked Amount			Recovery	=	90.10%	
35) Dibromofluoromethane	5.49	113	167731	42.29	ug/l	0.00
Spiked Amount			Recovery	=	84.58%	
50) Toluene-d8	8.71	98	696206	50.33	ug/l	0.00
Spiked Amount			Recovery	=	100.66%	
62) 4-Bromofluorobenzene	11.13	95	253817	46.42	ug/l	0.00
Spiked Amount			Recovery	=	92.84%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX082319\
Data File : VX011795.D
Acq On : 23 Aug 2019 14:06
Operator : JC/SP
Sample : K4388-19
Misc : 5.77a/5mL/100uL/10mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
T6-E3-(0)

Quant Time: Aug 26 02:27:54 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082219W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 23 01:48:12 2019
Response via : Initial Calibration

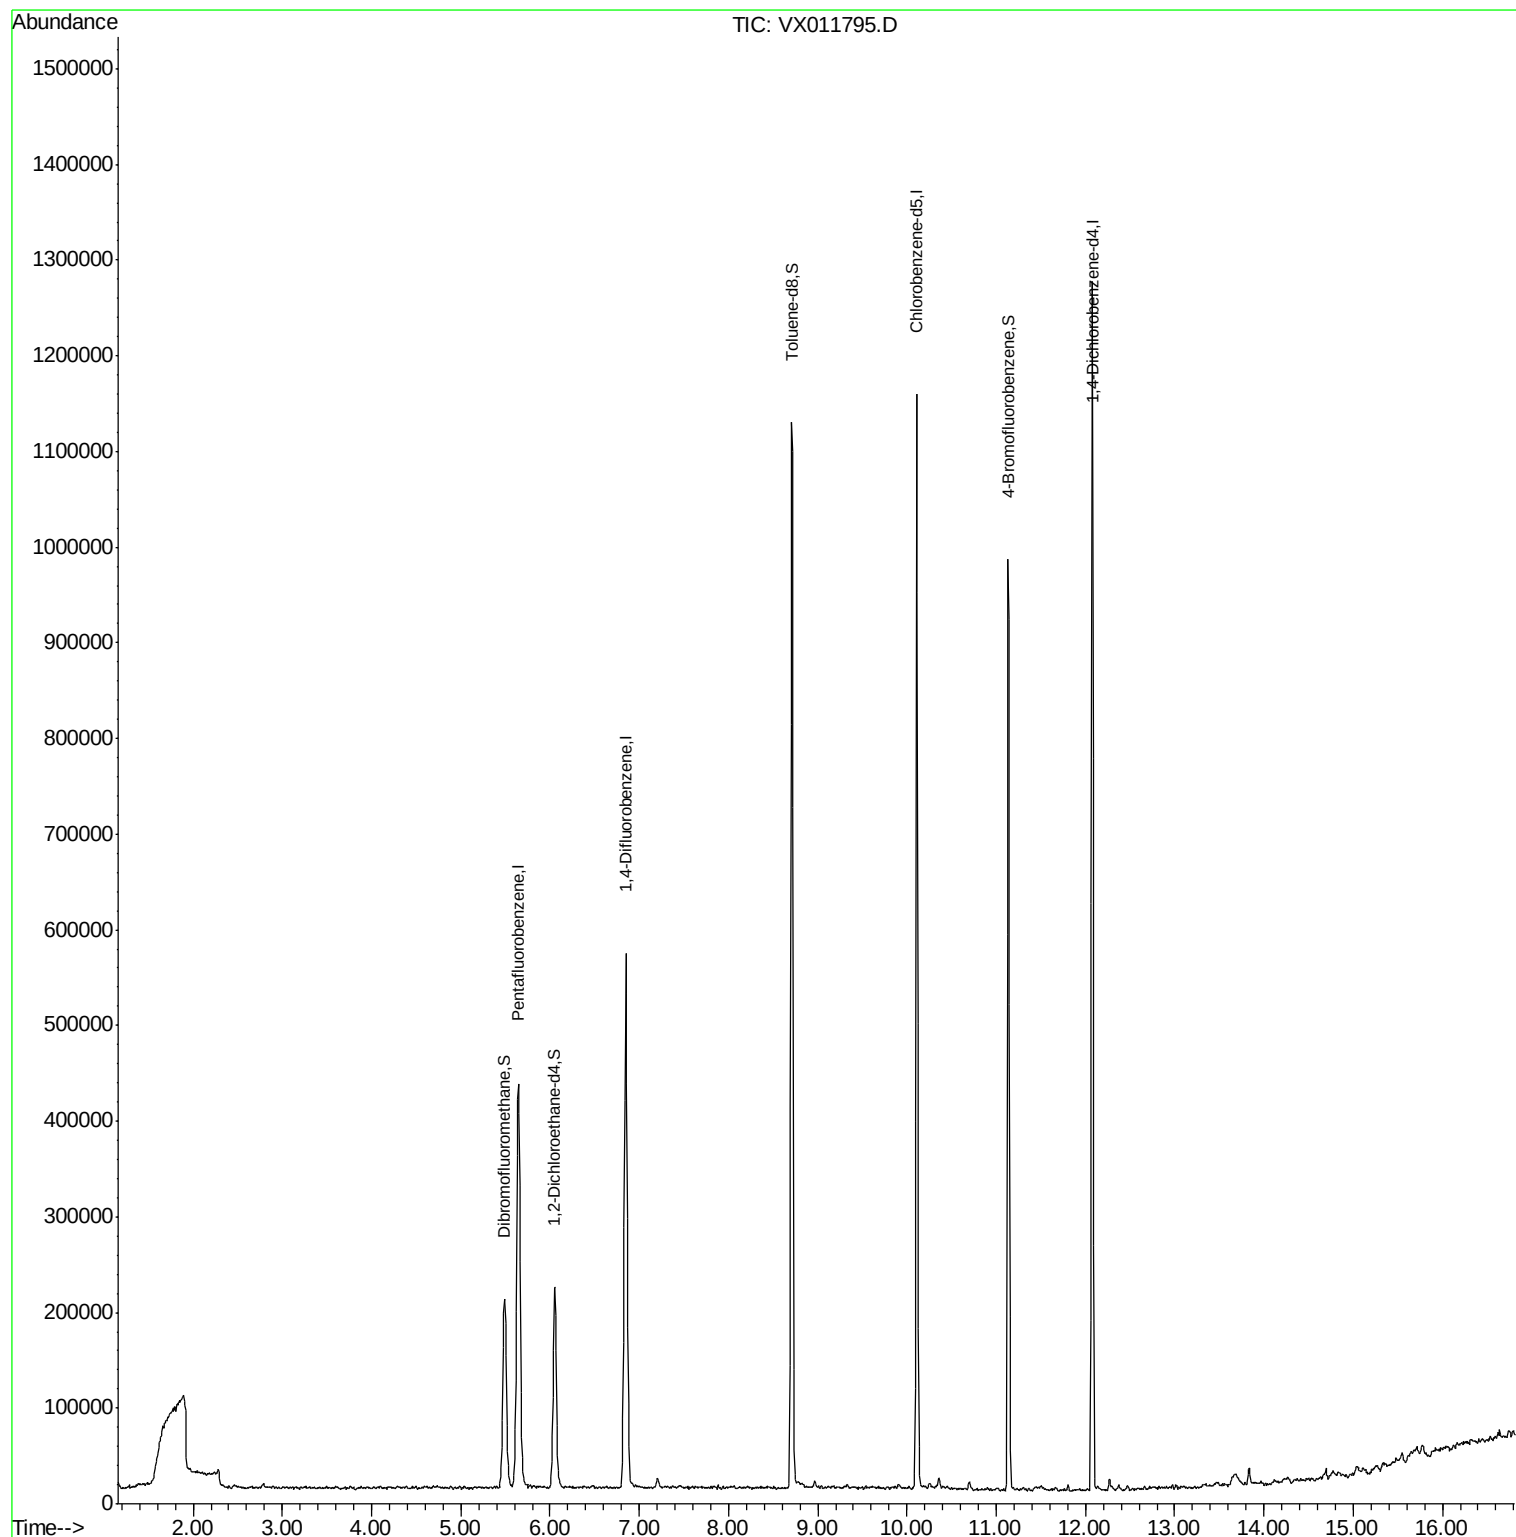

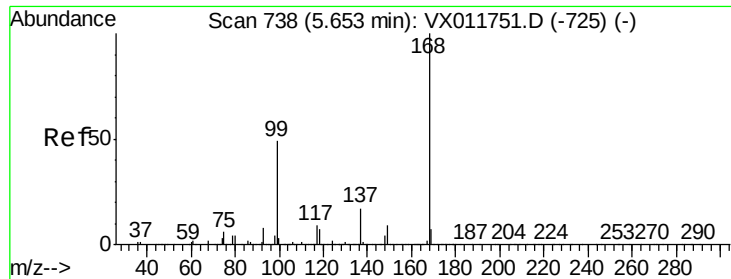

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 737

Delta R.T. -0.01 min

Lab File: VX011795.D

Acq: 23 Aug 2019 14:06

Instrument :

MSVOA_X

ClientSampleId :


T6-E3-(0)

Tot Ion:168 Resp: 457040

Ion Ratio Lower Upper




168 100

99 46.2 39.4 59.2

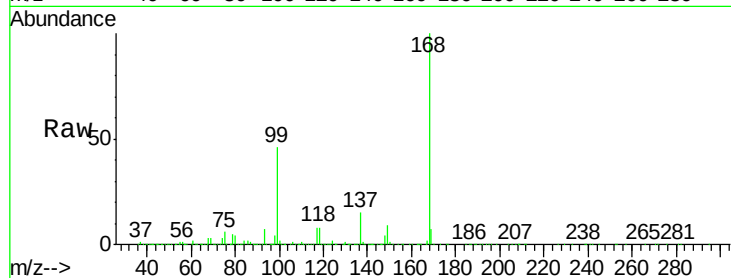

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

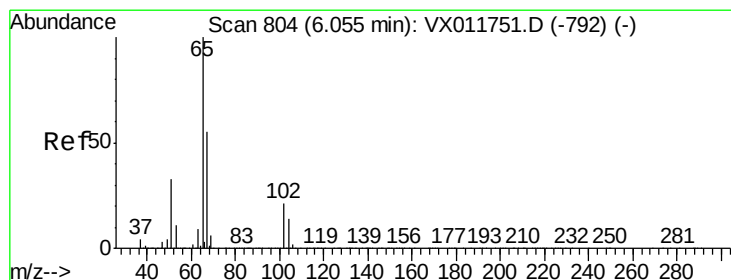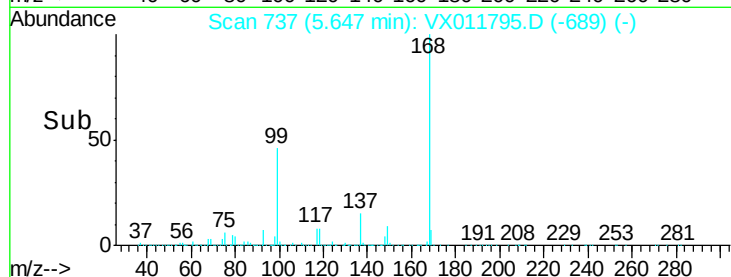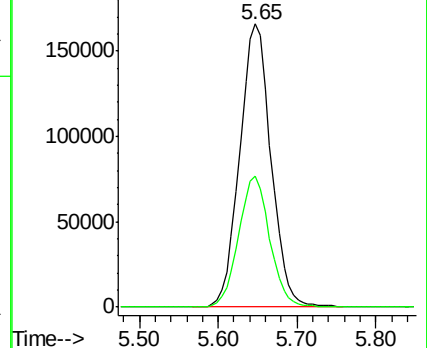

#33

1,2-Dichloroethane-d4

Concen: 45.051 ug/l

RT: 6.05 min Scan# 803

Delta R.T. -0.01 min

Lab File: VX011795.D


Acq: 23 Aug 2019 14:06

Tgt Ion: 65 Resp: 206841

Ion Ratio Lower Upper



65 100


67 53.1 0.0 107.8

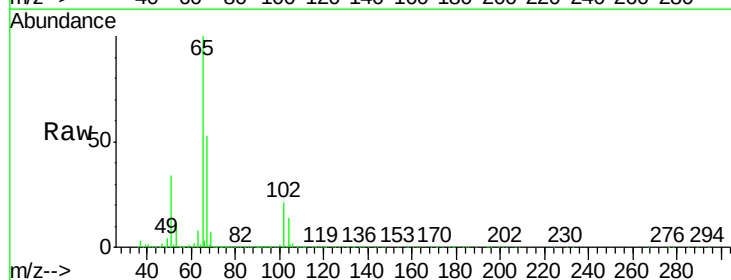

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

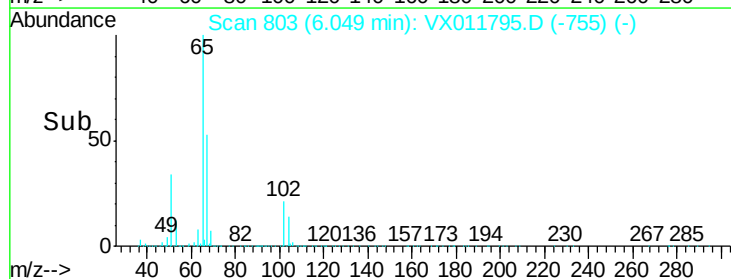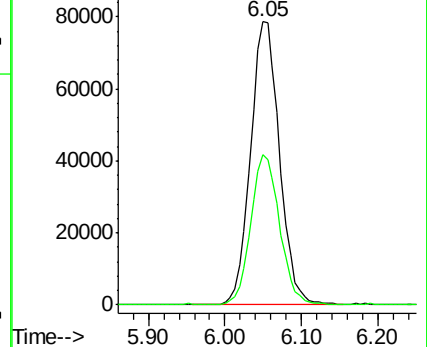


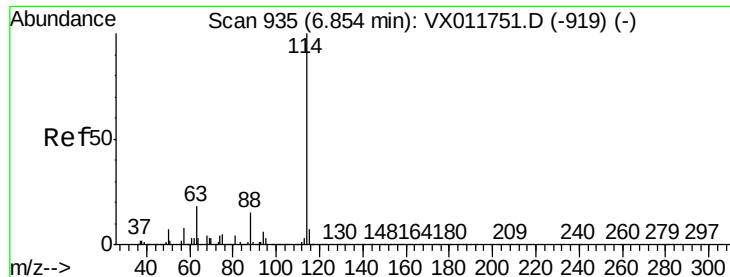




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.85 min Scan# 934
Delta R.T. -0.01 min
Lab File: VX011795.D
Acq: 23 Aug 2019 14:06

Instrument :
MSVOA_X
ClientSampleId :
T6-E3-(0)

Tot Ion	Ratio	Lower	Upper
114	100		
63	18.3	0.0	36.8
88	15.6	0.0	30.2

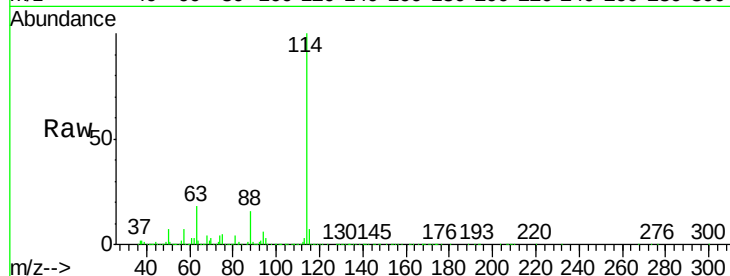


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

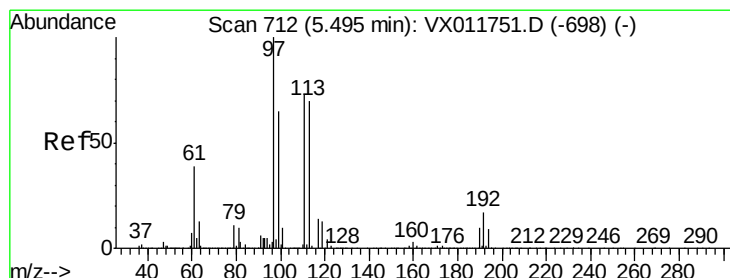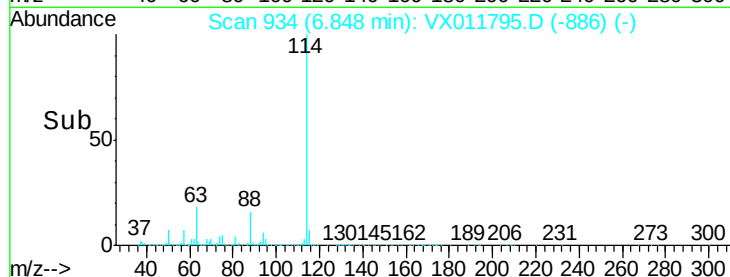
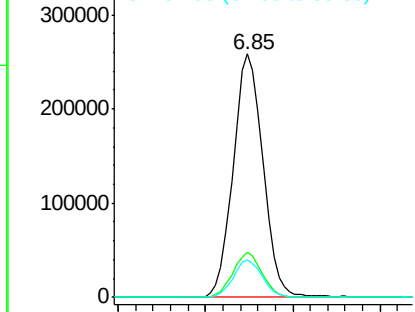



#35
Dibromofluoromethane
Concen: 42.290 ug/l
RT: 5.49 min Scan# 711
Delta R.T. -0.01 min
Lab File: VX011795.D
Acq: 23 Aug 2019 14:06

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.9	81.0	121.4
192	26.2	19.9	29.9

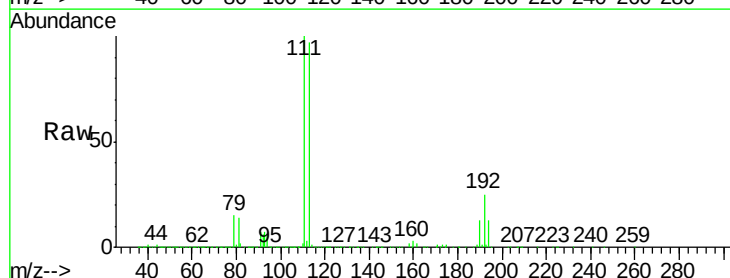

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



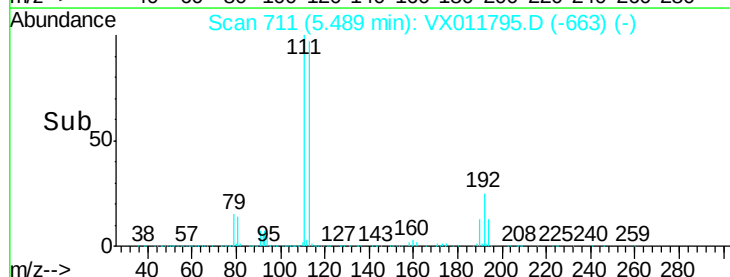
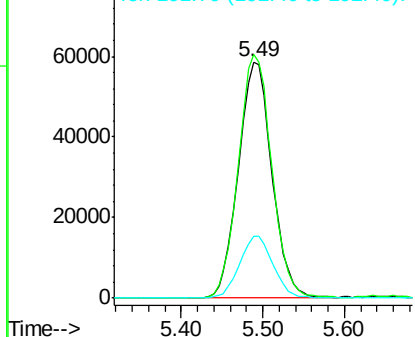


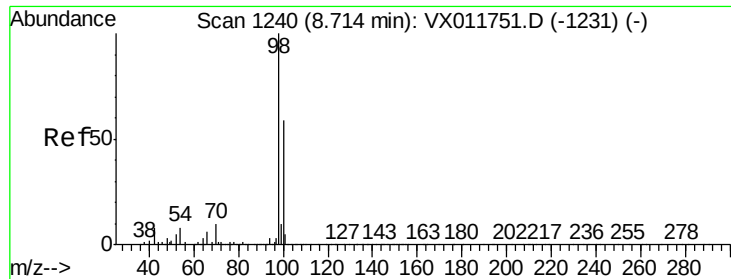

#50
Toluene-d8
Concen: 50.325 ug/l
RT: 8.71 min Scan# 1239
Delta R.T. -0.01 min
Lab File: VX011795.D
Acq: 23 Aug 2019 14:06




Instrument :
MSVOA_X
ClientSampleId :
T6-E3-(0)


Tot Ion: 98 Resp: 696206
Ion Ratio Lower Upper
98 100
100 65.3 52.1 78.1

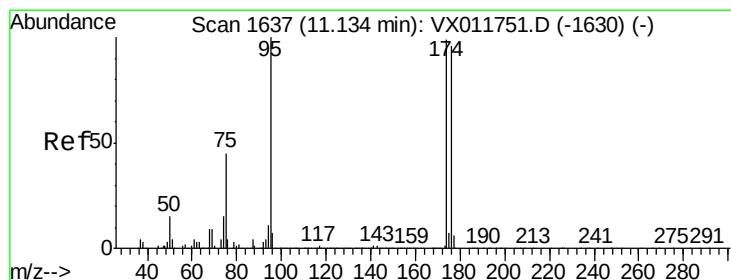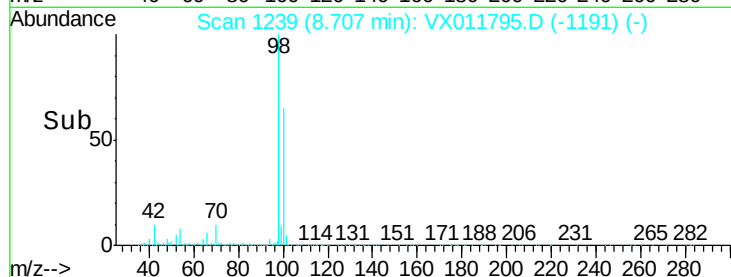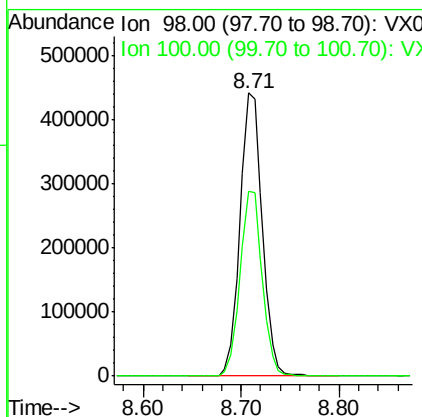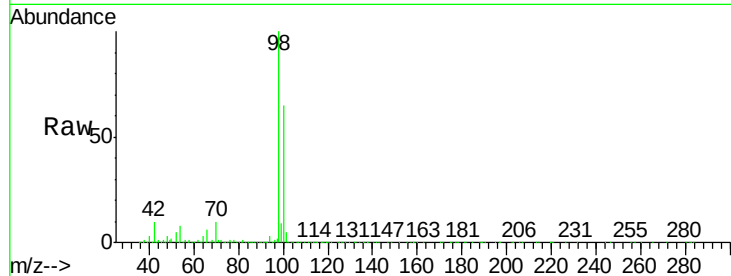

#62
4-Bromofluorobenzene
Concen: 46.418 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX011795.D
Acq: 23 Aug 2019 14:06

Tgt Ion: 95 Resp: 253817
Ion Ratio Lower Upper
95 100
174 102.4 0.0 197.4
176 100.1 0.0 194.4


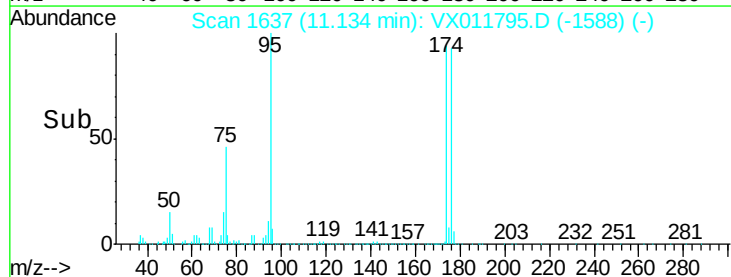
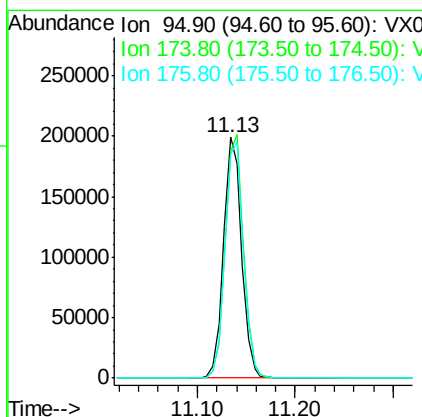
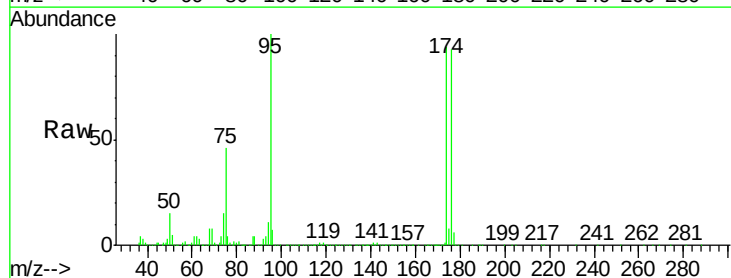


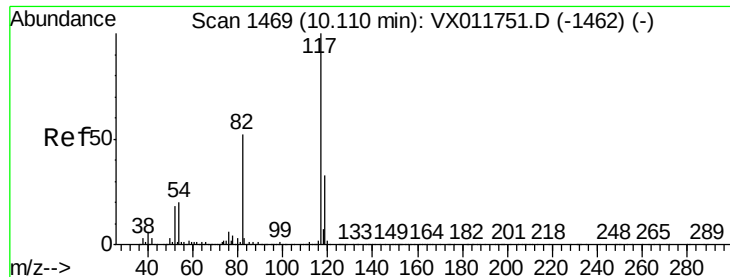

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX011795.D
Acq: 23 Aug 2019 14:06

Instrument :
MSVOA_X
ClientSampled :
T6-E3-(0)

Tot Ion:117 Resp: 552735
Ion Ratio Lower Upper
117 100
82 50.8 41.7 62.5
119 32.3 26.2 39.2

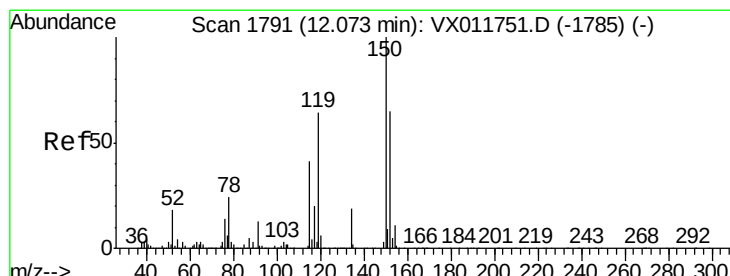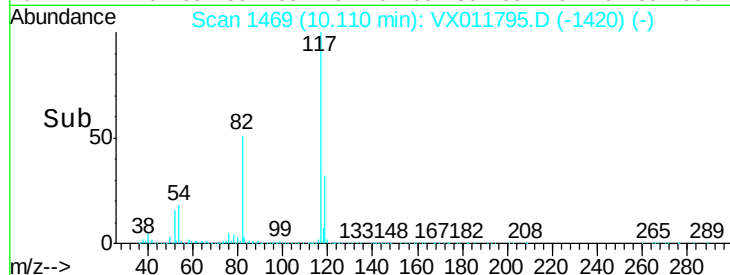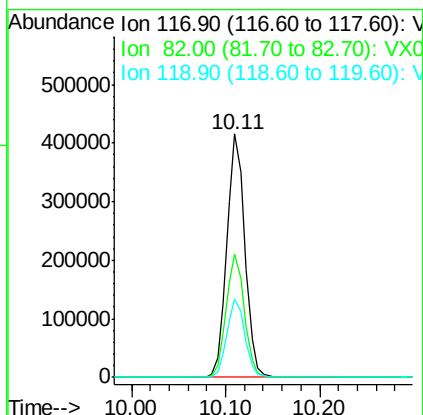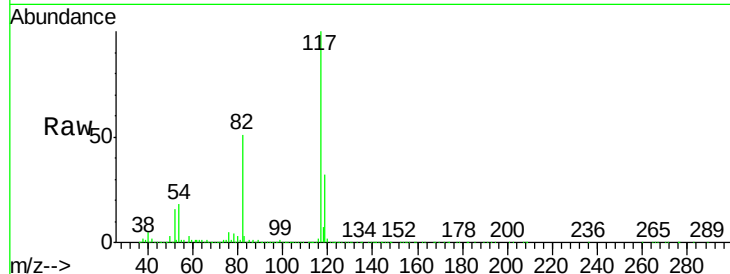

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.01 min
Lab File: VX011795.D
Acq: 23 Aug 2019 14:06

Tgt Ion:152 Resp: 299886
Ion Ratio Lower Upper
152 100
115 51.6 37.3 111.8
150 154.6 0.0 343.0

