



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082324\
Data File : VX043092.D
Acq On : 23 Aug 2024 07:55
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082224W.M
Title : SW846 8260
Last Update : Fri Aug 23 08:42:59 2024

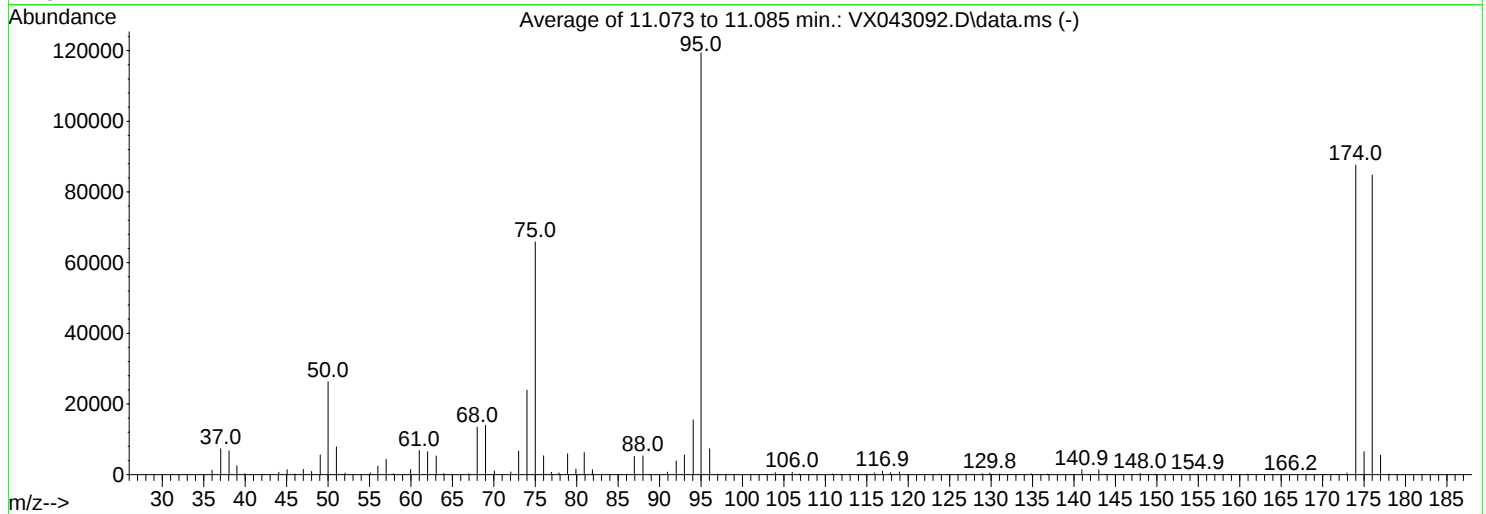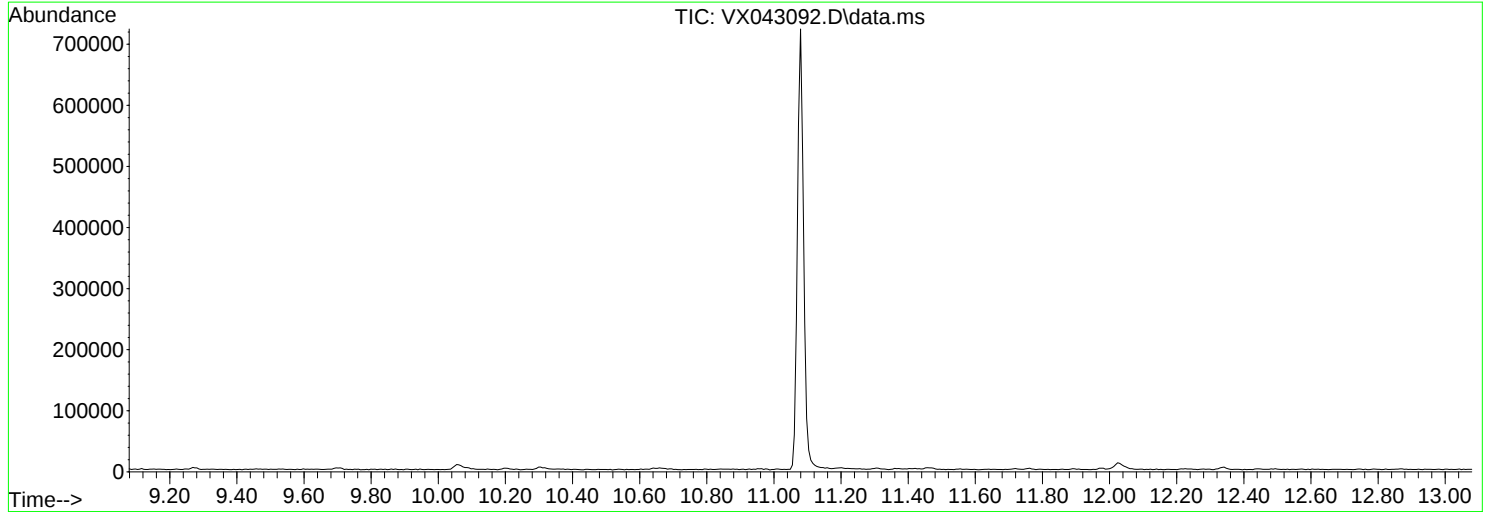

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	26328	PASS
75	95	30	60	55.2	65853	PASS
95	95	100	100	100.0	119379	PASS
96	95	5	9	6.1	7323	PASS
173	174	0.00	2	0.6	511	PASS
174	95	50	100	73.4	87637	PASS
175	174	5	9	7.4	6484	PASS
176	174	95	101	96.8	84811	PASS
177	176	5	9	6.5	5533	PASS