

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082418\
 Data File : VX004250.D
 Acq On : 24 Aug 2018 16:42
 Operator : JC/MD
 Sample : J4270-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BU-03-082318

Quant Time: Aug 25 00:30:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 23 05:39:44 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	298239	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	477111	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	438447	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	261292	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.07	65	204008	52.48	ug/l	0.00
Spiked Amount			Recovery	=	104.96%	
35) Dibromofluoromethane	5.50	113	175032	49.31	ug/l	0.00
Spiked Amount			Recovery	=	98.62%	
50) Toluene-d8	8.71	98	674464	50.34	ug/l	0.00
Spiked Amount			Recovery	=	100.68%	
62) 4-Bromofluorobenzene	11.14	95	242005	48.41	ug/l	0.00
Spiked Amount			Recovery	=	96.82%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	1223	0.61	ug/l	# 86
5) Bromomethane	1.64	94	1336	Below Cal		93
6) Chloroethane	1.78	64	2014	1.61	ug/l	# 51
10) Methyl Iodide	2.51	142	752	4.45	ug/l	98
11) Tert butyl alcohol	3.08	59	714	0.86	ug/l	# 87
13) Acrolein	2.29	56	149	0.75	ug/l	# 1
15) Acrylonitrile	3.15	53	778	0.38	ug/l	# 81
16) Acetone	2.45	43	12548	Below Cal		93
17) Carbon Disulfide	2.56	76	1511	0.97	ug/l	96
18) Methyl Acetate	2.78	43	6360	1.10	ug/l	97
20) Methylene Chloride	2.85	84	76096	20.34	ug/l	98
25) 2-Butanone	4.71	43	3071	Below Cal	#	79
29) Tetrahydrofuran	5.17	42	1553	0.93	ug/l	94
30) Chloroform	5.21	83	6515	1.03	ug/l	94
36) 1,1-Dichloropropene	5.66	75	19308	3.60	ug/l	# 49
38) Carbon Tetrachloride	5.66	117	25676	5.09	ug/l	# 16
39) Methylcyclohexane	7.46	83	1553	0.25	ug/l	90
43) Isopropyl Acetate	6.46	43	171156	21.12	ug/l	99
47) Bromodichloromethane	7.90	83	1452	0.29	ug/l	# 91
48) Methyl methacrylate	7.68	41	7606	1.75	ug/l	# 21
51) 4-Methyl-2-Pentanone	8.65	43	1429	0.24	ug/l	# 33
59) 2-Hexanone	9.55	43	11877	2.64	ug/l	# 55
68) m/p-Xylenes	10.36	106	2091	0.30	ug/l	93
76) 1,2,3-Trichloropropane	11.14	75	115091	21.66	ug/l	# 37
81) trans-1,4-Dichloro-2-buten	11.14	75	115091	70.27	ug/l	# 10
84) 1,2,4-Trimethylbenzene	11.81	105	4359	0.30	ug/l	93
94) Hexachlorobutadiene	13.78	225	277	Below Cal		76
95) Naphthalene	13.83	128	24969	1.46	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX082418\
Data File : VX004250.D
Acq On : 24 Aug 2018 16:42
Operator : JC/MD
Sample : J4270-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BU-03-082318

Quant Time: Aug 25 00:30:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 23 05:39:44 2018
Response via : Initial Calibration

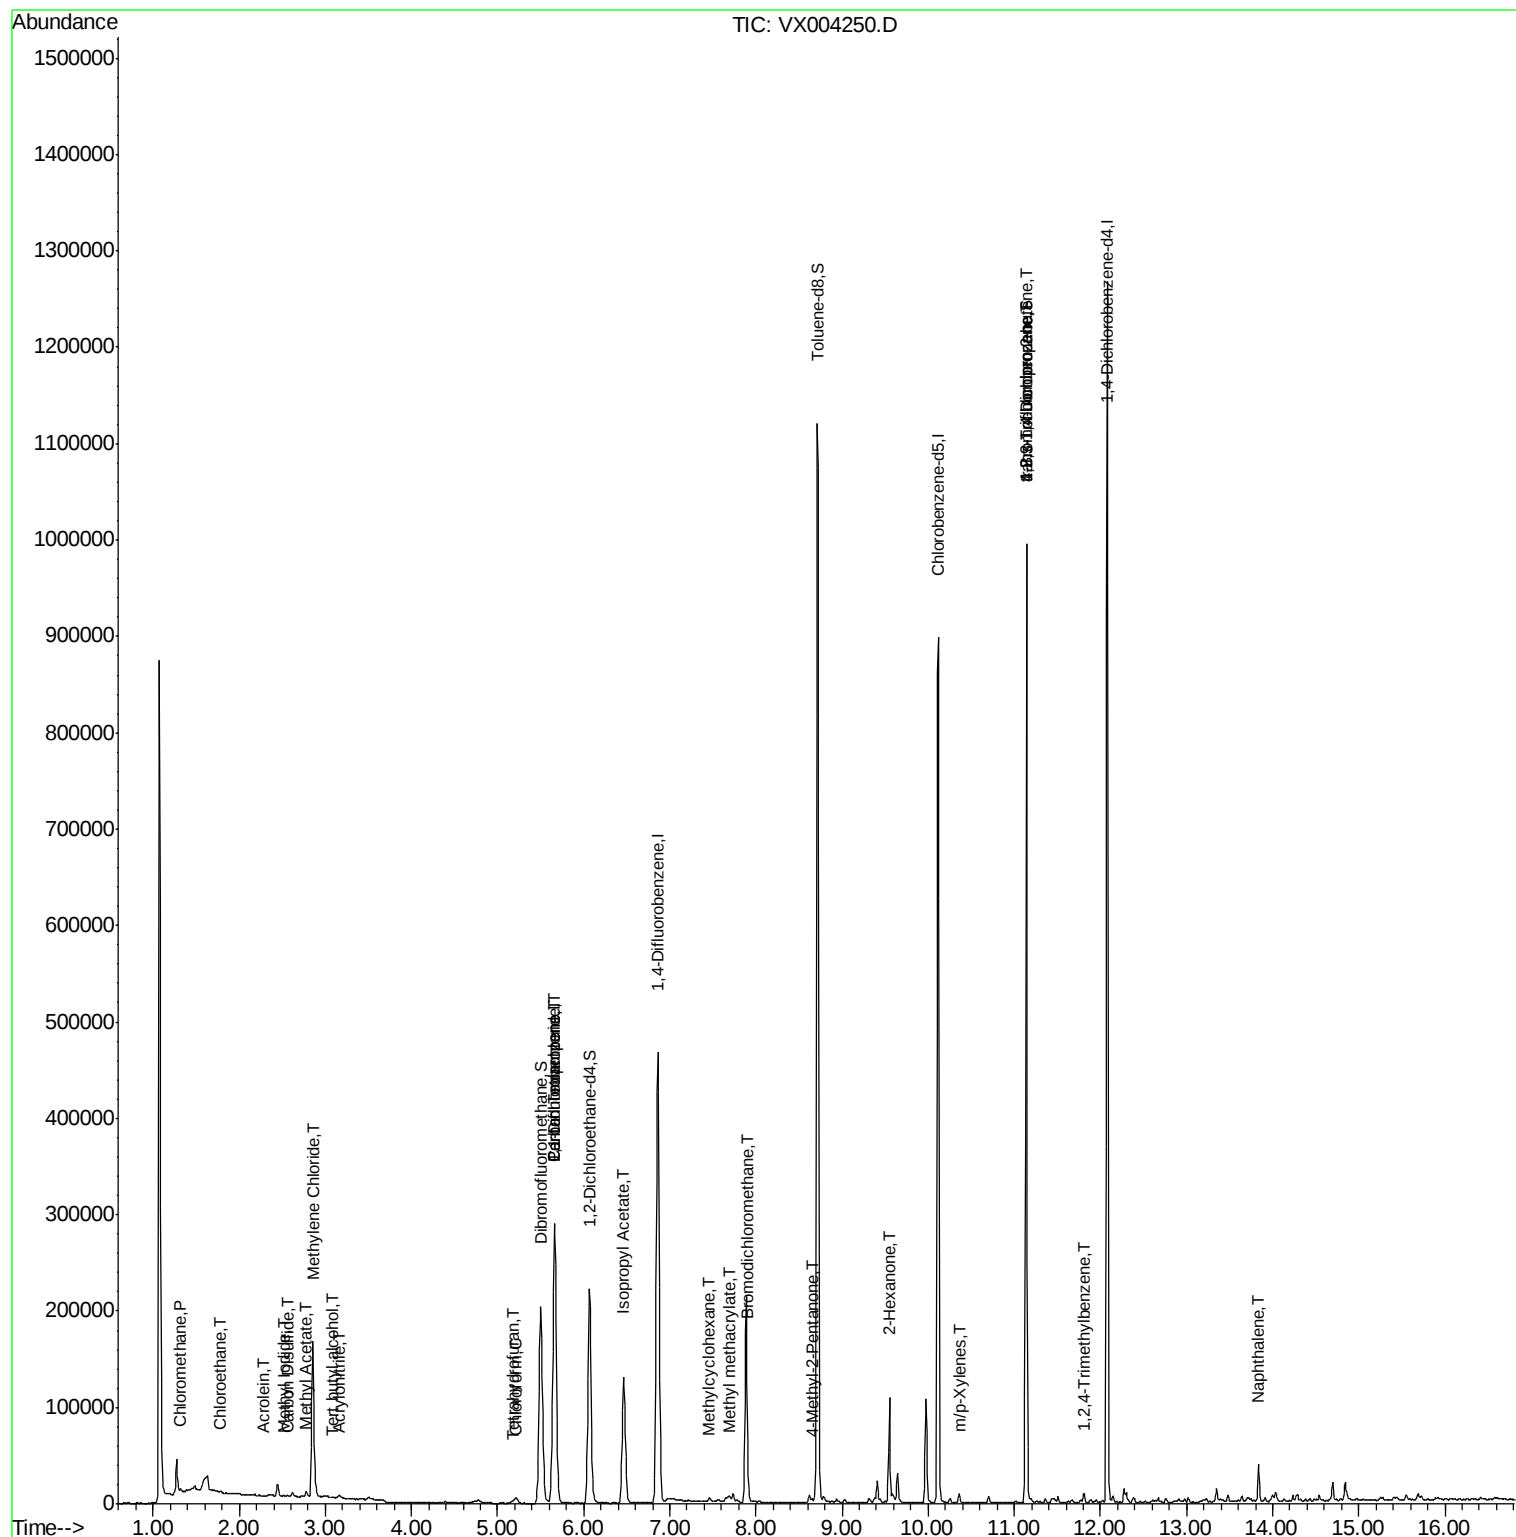



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.66 min Scan# 832

Delta R.T. -0.00 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :


BU-03-082318

Tot Ion:168 Resp: 298239

Ion Ratio Lower Upper

168 100

99 50.9 39.9 59.9

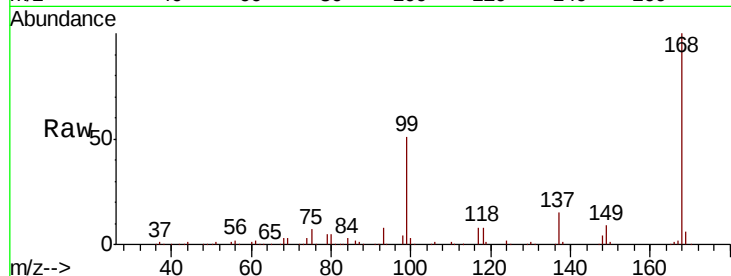

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

120000

100000

80000

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80



#3

Chloromethane

Concen: 0.61 ug/l

RT: 1.32 min Scan# 120

Delta R.T. -0.01 min

Lab File: VX004250.D


Acq: 24 Aug 2018 16:42

Tgt Ion: 50 Resp: 1223

Ion Ratio Lower Upper

50 100

52 24.9 26.2 39.2#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.32

1000

800

600


400


200

0

Time-->

1.30 1.32 1.34 1.36



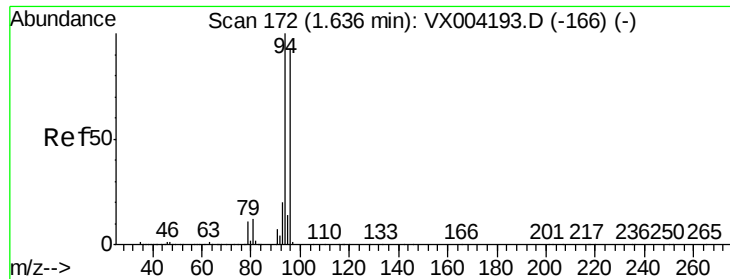

#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 172

Delta R.T. 0.00 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :


BU-03-082318

Tot Ion: 94 Resp: 1336

Ion Ratio Lower Upper

94 100

96 86.0 74.5 111.7

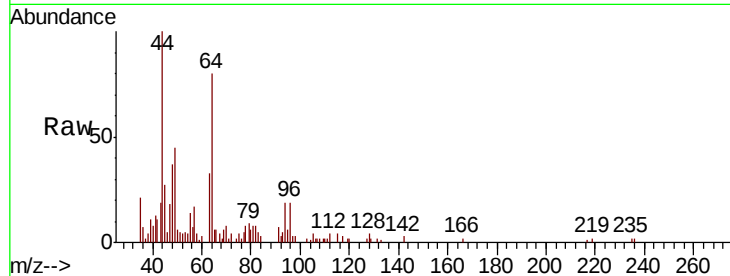

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.64

800



600

400

200

0

Time--> 1.55 1.60 1.65 1.70 1.75

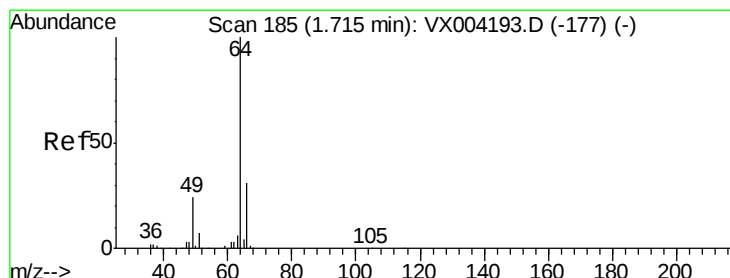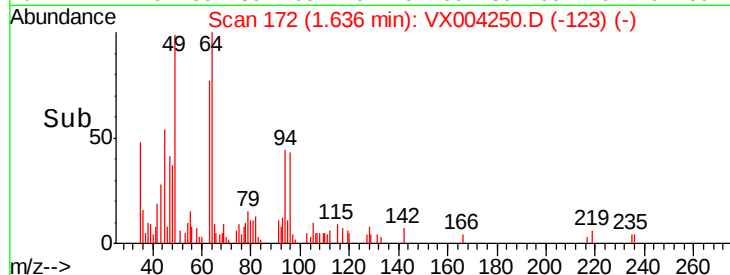

#6

Chloroethane

Concen: 1.61 ug/l

RT: 1.78 min Scan# 196

Delta R.T. 0.07 min

Lab File: VX004250.D


Acq: 24 Aug 2018 16:42

Tgt Ion: 64 Resp: 2014

Ion Ratio Lower Upper

64 100

66 4.1 24.6 36.8#

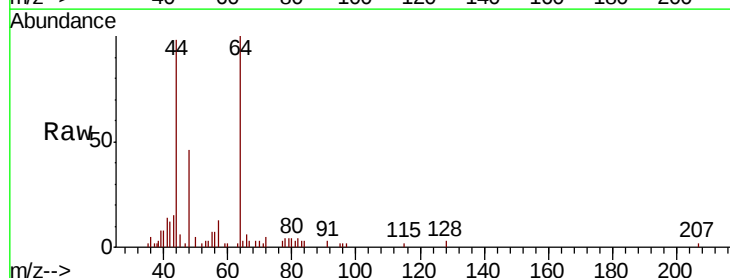

Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

1.78


3000


2000

1000

0

Time--> 1.75 1.80 1.85









#10
Methyl Iodide
Concen: 4.45 ug/l
RT: 2.51 min Scan# 315
Delta R.T. 0.00 min
Lab File: VX004250.D
Acq: 24 Aug 2018 16:42




Instrument :
MSVOA_X
ClientSampled :
BU-03-082318


Tot Ion:142 Resp: 752
Ion Ratio Lower Upper
142 100
127 41.2 33.8 50.6
141 15.0 11.4 17.0

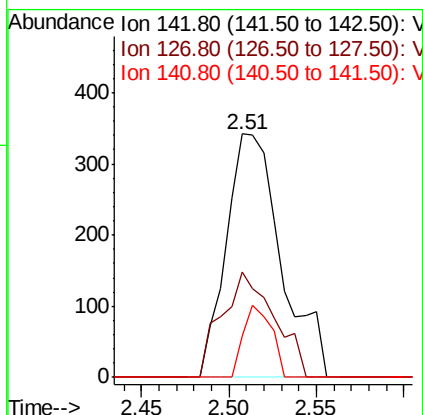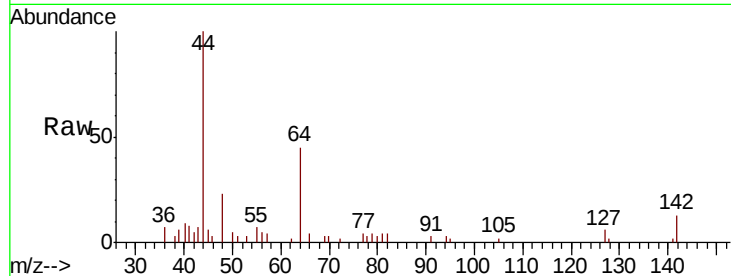

#11
Tert butyl alcohol
Concen: 0.86 ug/l
RT: 3.08 min Scan# 409
Delta R.T. -0.00 min
Lab File: VX004250.D
Acq: 24 Aug 2018 16:42

Tgt Ion: 59 Resp: 714
Ion Ratio Lower Upper
59 100
57 15.1 8.2 12.4#

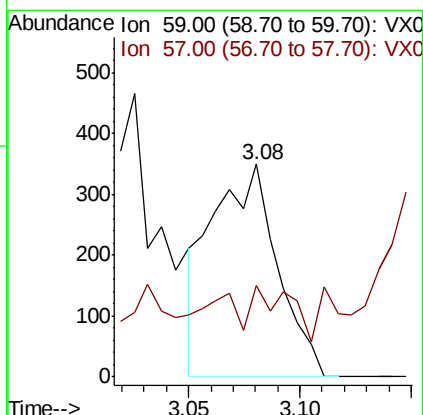

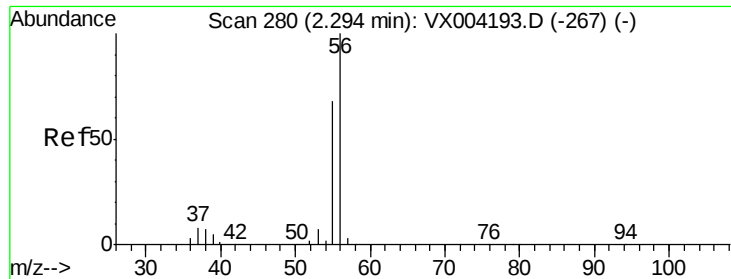

#13

Acrolein

Concen: 0.75 ug/l

RT: 2.29 min Scan# 279

Delta R.T. -0.01 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampled :





BU-03-082318

Tot Ion: 56 Resp: 149

Ion Ratio Lower Upper

56 100

55 152.3 54.7 82.1#

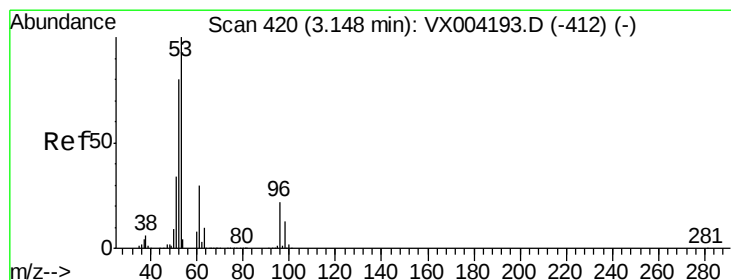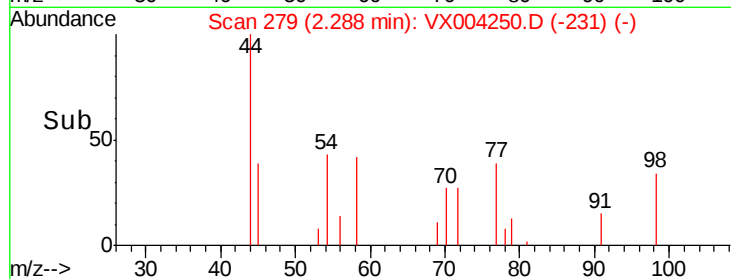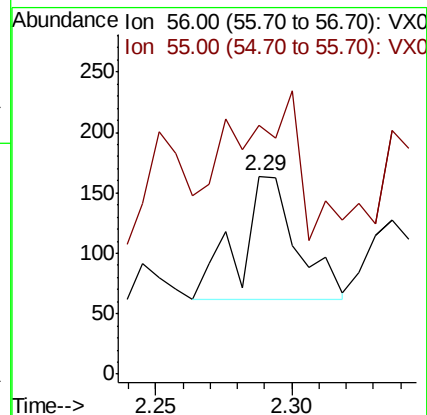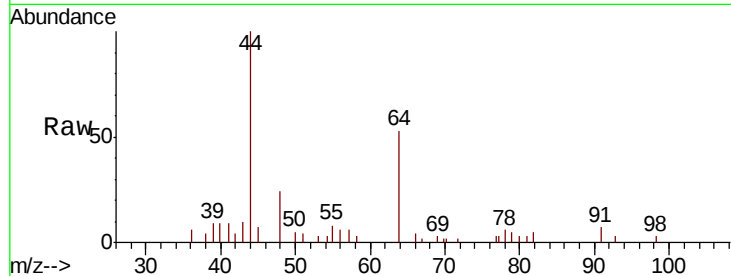

#15

Acrylonitrile

Concen: 0.38 ug/l

RT: 3.15 min Scan# 421

Delta R.T. 0.01 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42




Tgt Ion: 53 Resp: 778


Ion Ratio Lower Upper

53 100

52 82.5 65.2 97.8

51 0.0 28.2 42.2#

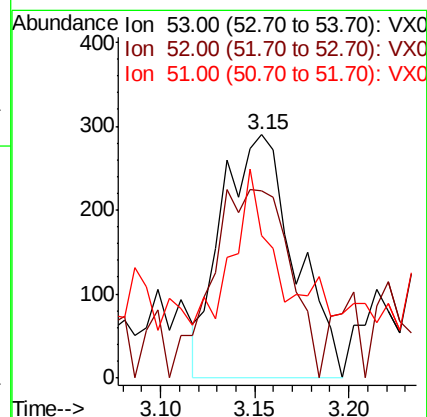

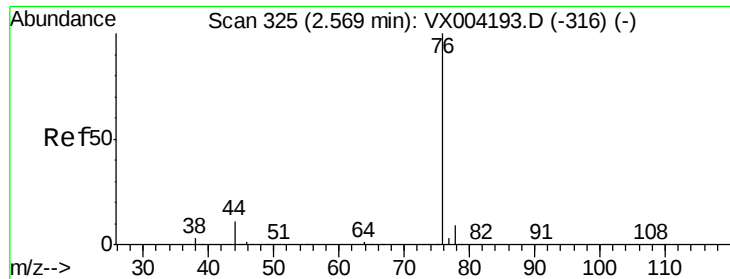

#17

Carbon Disulfide

Concen: 0.97 ug/l

RT: 2.56 min Scan# 324

Delta R.T. -0.01 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :


BU-03-082318

Tot Ion: 76 Resp: 1511

Ion Ratio Lower Upper




76 100

78 7.5 7.0 10.6

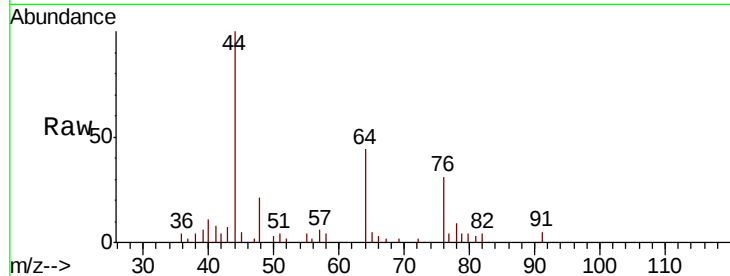

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

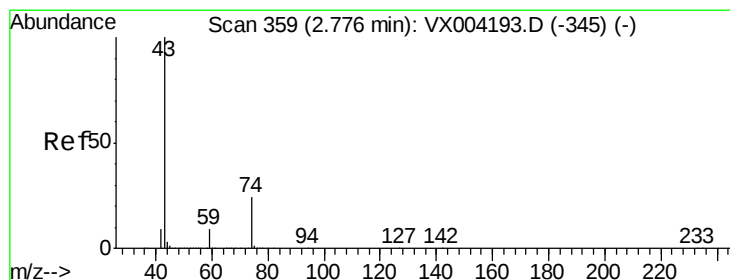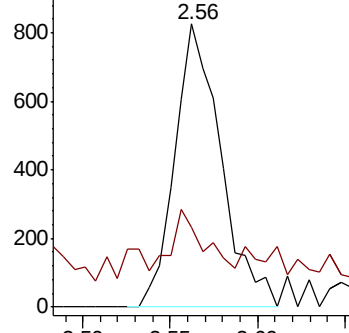

#18

Methyl Acetate

Concen: 1.10 ug/l

RT: 2.78 min Scan# 359

Delta R.T. -0.00 min

Lab File: VX004250.D


Acq: 24 Aug 2018 16:42

Tgt Ion: 43 Resp: 6360

Ion Ratio Lower Upper



43 100


74 25.7 19.4 29.2

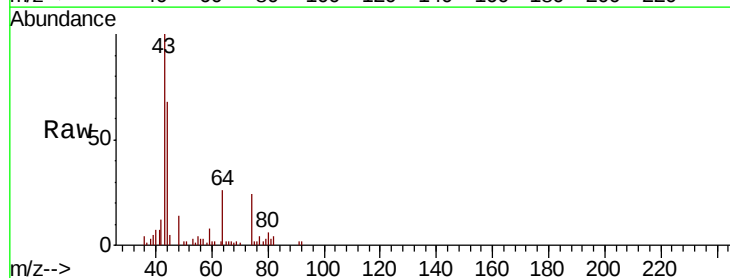

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

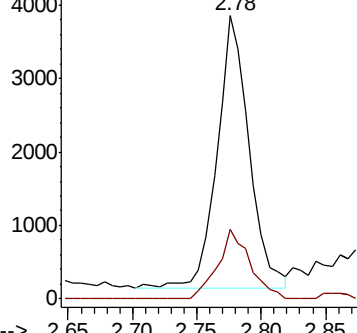

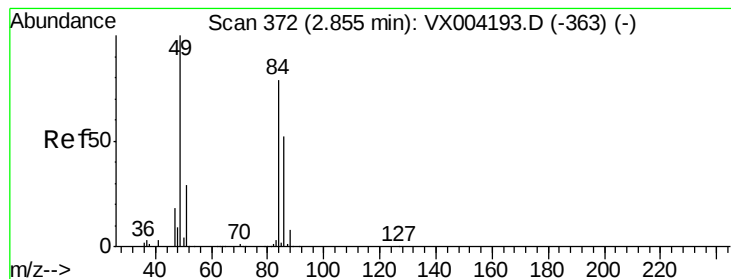

#20

Methylene Chloride

Concen: 20.34 ug/l

RT: 2.85 min Scan# 372

Delta R.T. -0.00 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :

BU-03-082318

Tot Ion: 84 Resp: 76096


Ion Ratio Lower Upper

84 100

49 124.8 101.2 151.8

51 39.8 29.5 44.3

86 67.1 52.3 78.5






Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

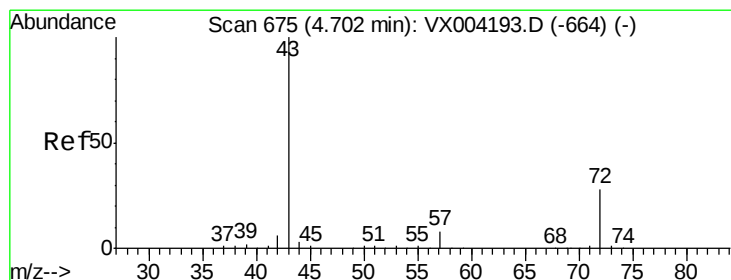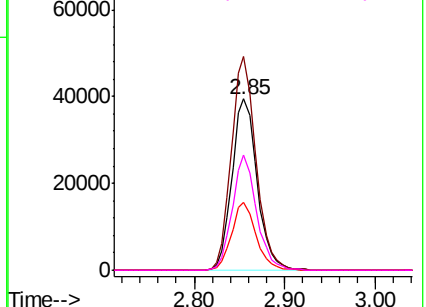

#25

2-Butanone

Concen: Below Cal

RT: 4.71 min Scan# 676

Delta R.T. 0.01 min

Lab File: VX004250.D


Acq: 24 Aug 2018 16:42

Tgt Ion: 43 Resp: 3071

Ion Ratio Lower Upper



43 100


72 38.3 22.0 33.0#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

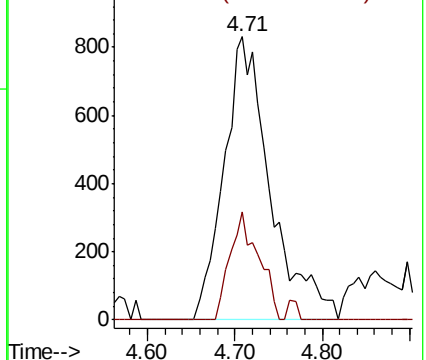



#29

Tetrahydrofuran

Concen: 0.93 ug/l

RT: 5.17 min Scan# 751

Delta R.T. 0.01 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampled :

BU-03-082318





Tot Ion: 42 Resp: 1553

Ion Ratio Lower Upper

42 100

72 41.0 37.4 56.0

71 41.0 34.5 51.7

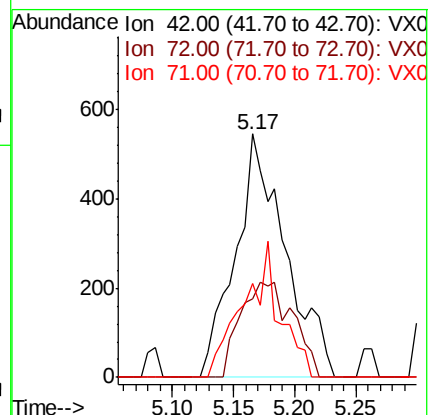

#30

Chloroform

Concen: 1.03 ug/l

RT: 5.21 min Scan# 759

Delta R.T. -0.00 min

Lab File: VX004250.D




Acq: 24 Aug 2018 16:42


Tgt Ion: 83 Resp: 6515

Ion Ratio Lower Upper

83 100

85 60.8 52.6 79.0


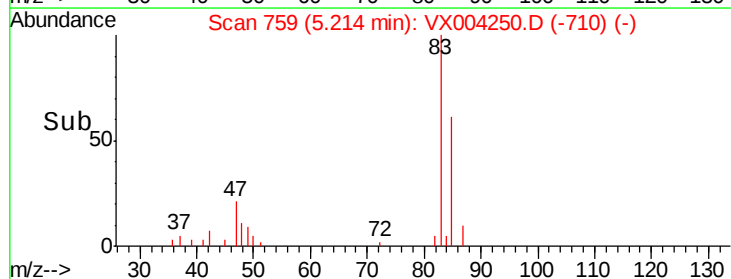
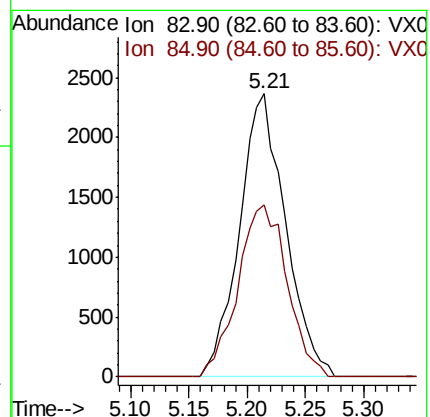



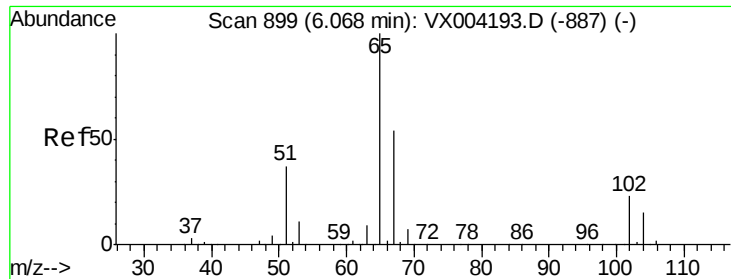

#33
 1,2-Dichloroethane-d4
 Concen: 52.48 ug/l
 RT: 6.07 min Scan# 899
 Delta R.T. -0.00 min
 Lab File: VX004250.D
 Acq: 24 Aug 2018 16:42




Instrument :
 MSVOA_X
 ClientSampleId :
 BU-03-082318


Tot Ion: 65 Resp: 204008
 Ion Ratio Lower Upper
 65 100
 67 53.5 0.0 106.8

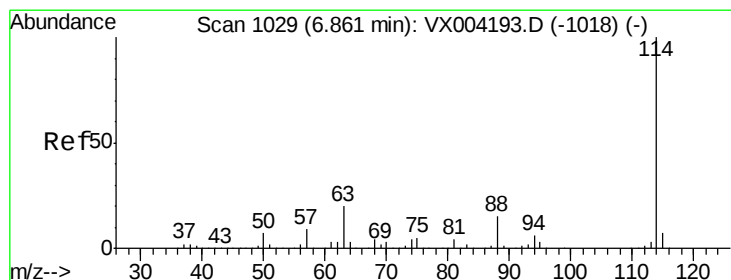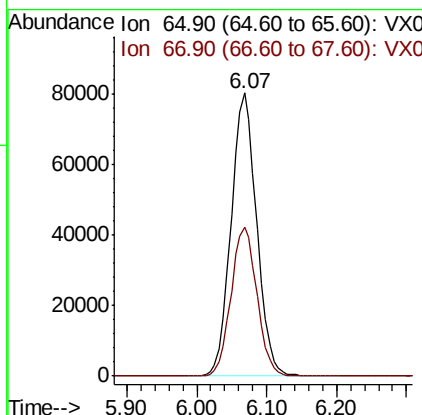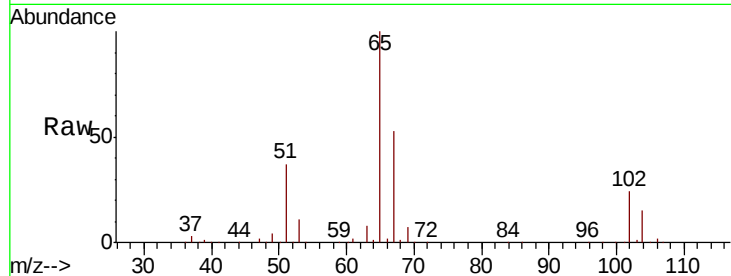

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.86 min Scan# 1029
 Delta R.T. -0.00 min
 Lab File: VX004250.D
 Acq: 24 Aug 2018 16:42

Tgt Ion: 114 Resp: 477111
 Ion Ratio Lower Upper
 114 100
 63 19.5 0.0 39.0
 88 15.4 0.0 30.4

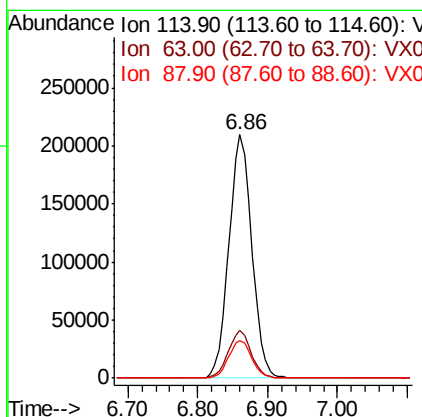

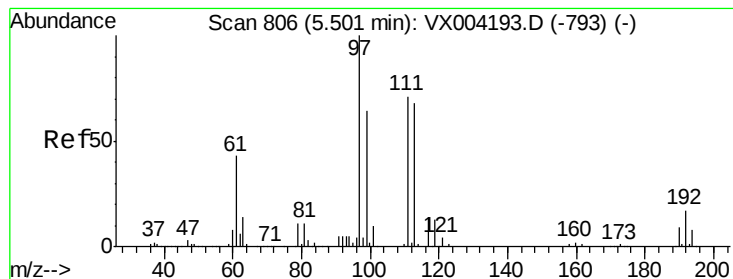

#35

Dibromofluoromethane

Concen: 49.31 ug/l

RT: 5.50 min Scan# 806

Delta R.T. -0.00 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :

BU-03-082318





Tot Ion:113 Resp: 175032

Ion Ratio Lower Upper

113 100

111 100.5 82.4 123.6

192 24.2 19.4 29.2

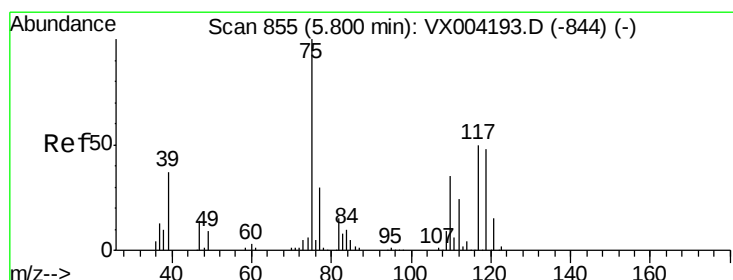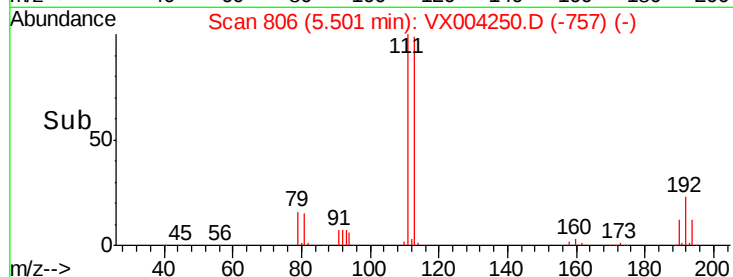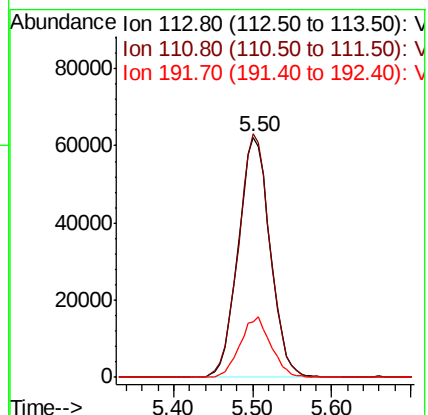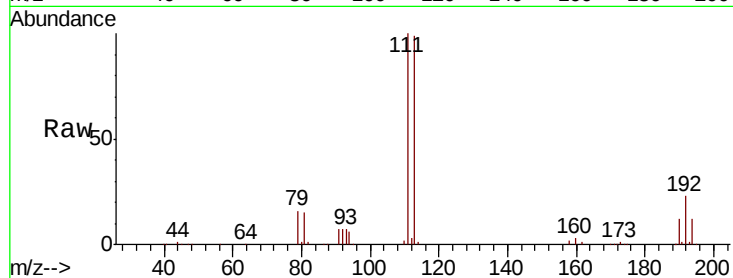

#36

1,1-Dichloropropene

Concen: 3.60 ug/l

RT: 5.66 min Scan# 832

Delta R.T. -0.14 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42




Tgt Ion: 75 Resp: 19308


Ion Ratio Lower Upper

75 100

110 9.0 18.0 54.0#

77 0.1 24.6 36.8#

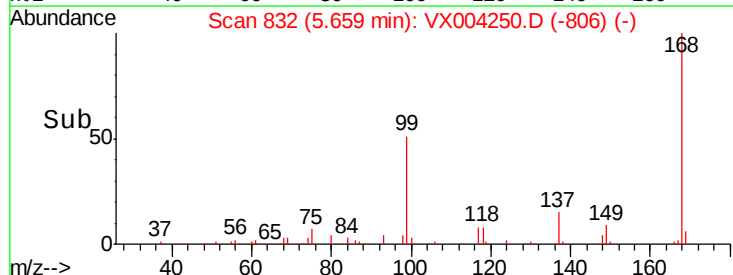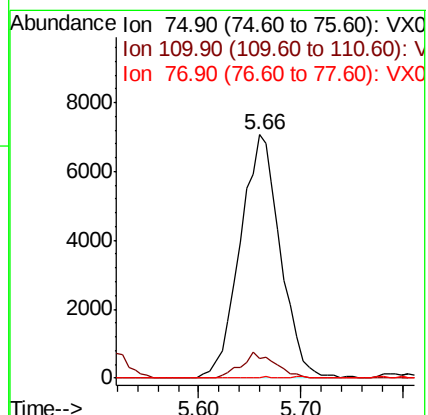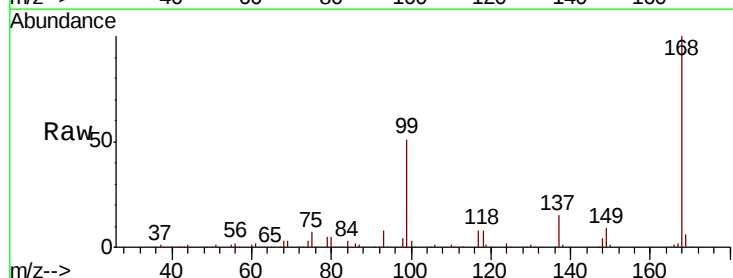



#38

Carbon Tetrachloride

Concen: 5.09 ug/l

RT: 5.66 min Scan# 832

Delta R.T. -0.12 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :

BU-03-082318


Tot Ion:117 Resp: 25676

Ion Ratio Lower Upper

117 100

119 6.4 78.8 118.2#




121 0.0 24.9 37.3#

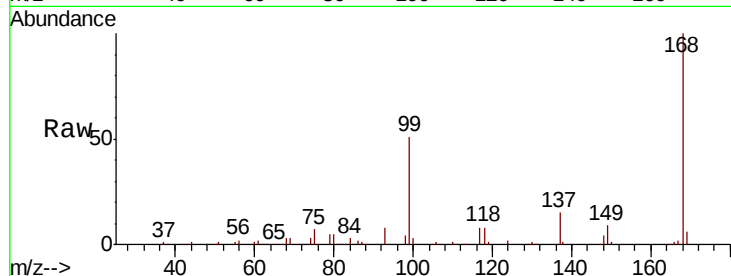

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

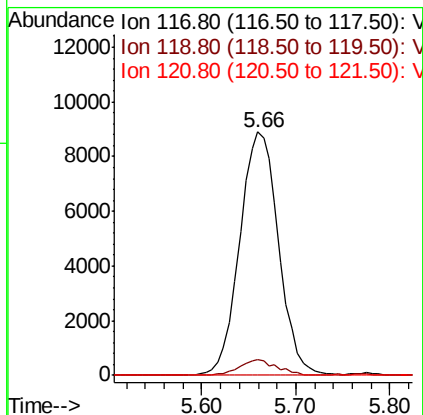

#39

Methylcyclohexane

Concen: 0.25 ug/l

RT: 7.46 min Scan# 1128

Delta R.T. 0.01 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42


Tgt Ion: 83 Resp: 1553

Ion Ratio Lower Upper

83 100

55 70.2 61.0 91.4



98 39.8 39.6 59.4




Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0

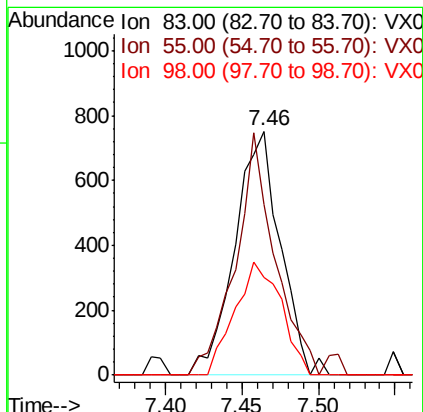







#43

Isopropyl Acetate
 Concen: 21.12 ug/l
 RT: 6.46 min Scan# 964
 Delta R.T. -0.00 min
 Lab File: VX004250.D
 Acq: 24 Aug 2018 16:42

Instrument :
 MSVOA_X
 ClientSampleId :
 BU-03-082318




Tot Ion	43	Resp	171156
Ion Ratio	Lower	Upper	
43	100		
61	21.0	17.0	25.4
87	14.1	11.4	17.2

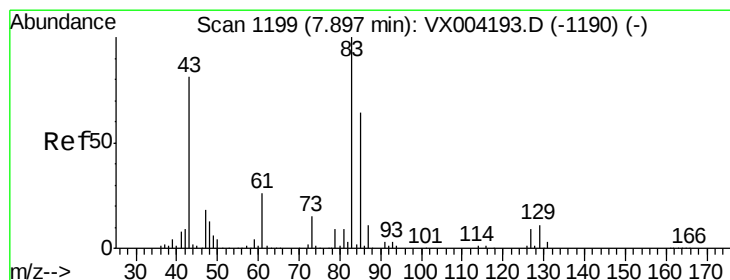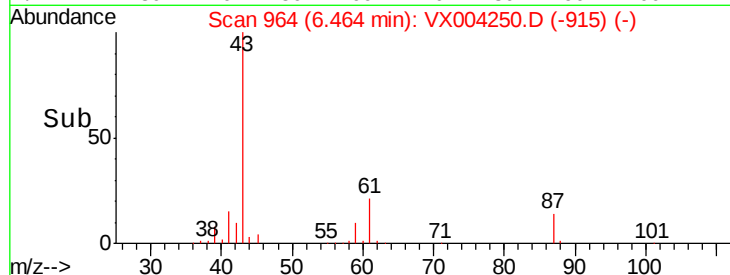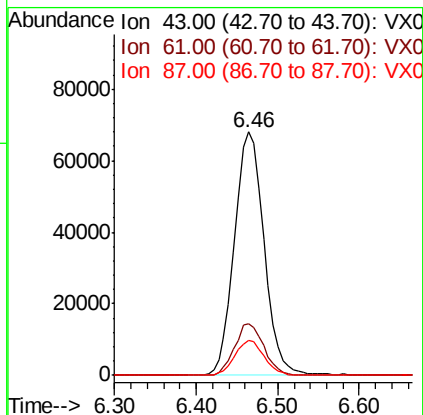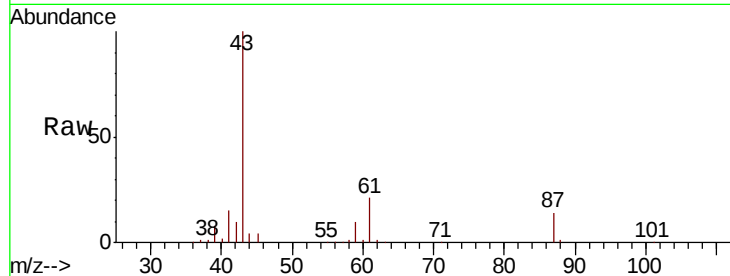


#47

Bromodichloromethane
 Concen: 0.29 ug/l
 RT: 7.90 min Scan# 1200
 Delta R.T. 0.01 min
 Lab File: VX004250.D
 Acq: 24 Aug 2018 16:42

Tgt Ion	83	Resp	1452
Ion Ratio	Lower	Upper	
83	100		
85	58.4	50.9	76.3
127	0.0	7.3	10.9#

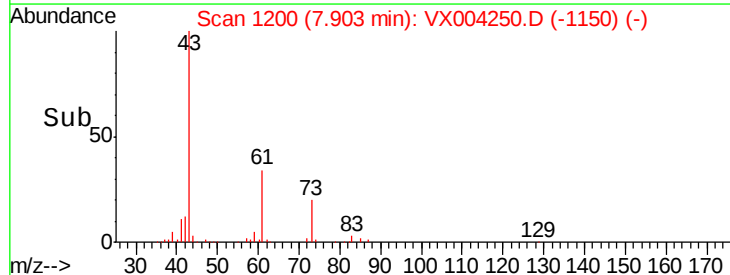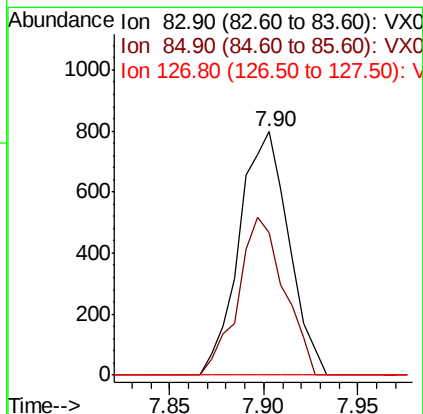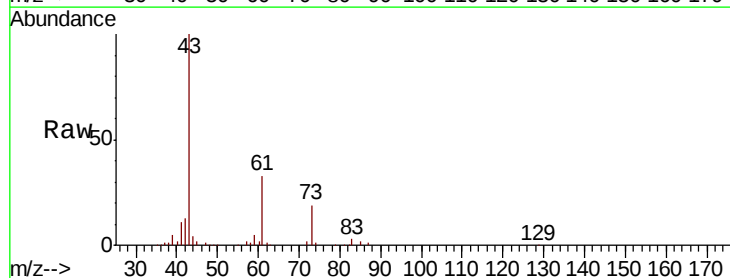

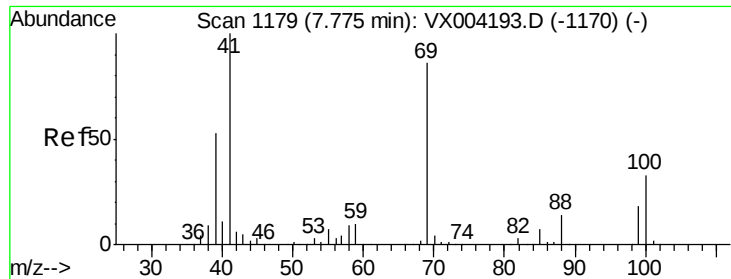

#48

Methvl methacrylate

Concen: 1.75 ug/l

RT: 7.68 min Scan# 1164

Delta R.T. -0.09 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :

BU-03-082318


Tot Ion: 41 Resp: 7606

Ion Ratio Lower Upper

41 100

69 0.0 70.2 105.4#




39 14.7 42.7 64.1#

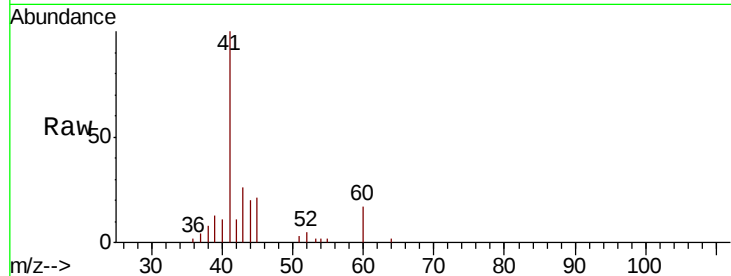

Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

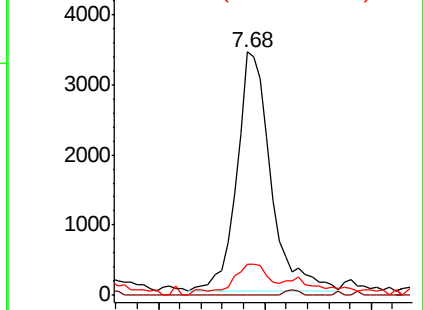

#50

Toluene-d8

Concen: 50.34 ug/l

RT: 8.71 min Scan# 1333

Delta R.T. -0.00 min

Lab File: VX004250.D


Acq: 24 Aug 2018 16:42

Tgt Ion: 98 Resp: 674464

Ion Ratio Lower Upper



98 100


100 66.4 52.9 79.3



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

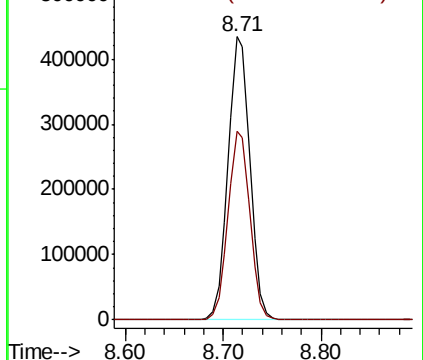

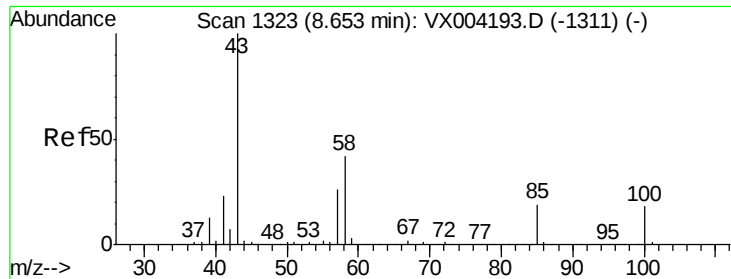

#51

4-Methyl-2-Pentanone

Concen: 0.24 ug/l

RT: 8.65 min Scan# 1323

Delta R.T. -0.00 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :





BU-03-082318

Tot Ion: 43 Resp: 1429

Ion Ratio Lower Upper

43 100

58 83.6 33.1 49.7#

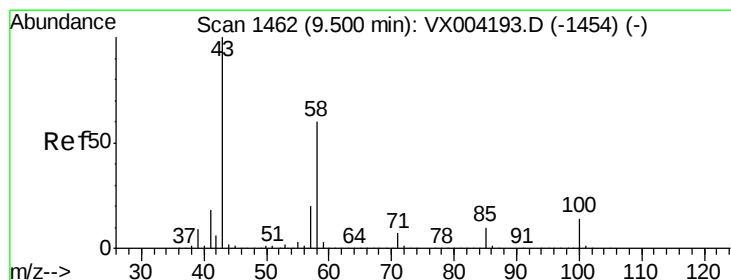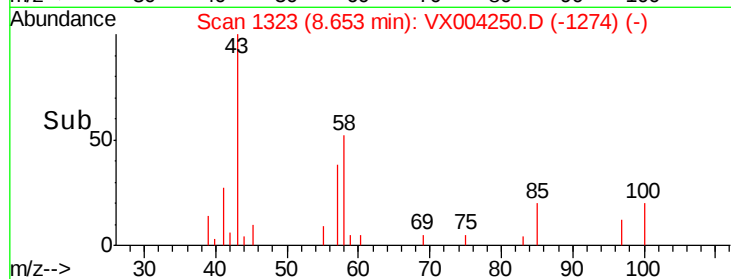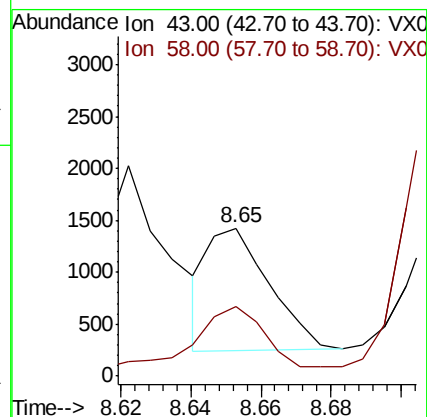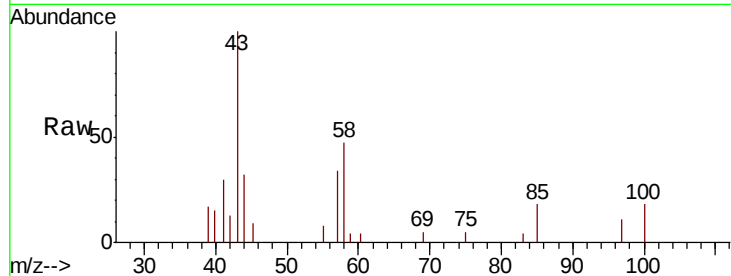

#59

2-Hexanone

Concen: 2.64 ug/l

RT: 9.55 min Scan# 1470

Delta R.T. 0.05 min

Lab File: VX004250.D




Acq: 24 Aug 2018 16:42


Tgt Ion: 43 Resp: 11877

Ion Ratio Lower Upper

43 100

58 24.6 29.0 87.0#



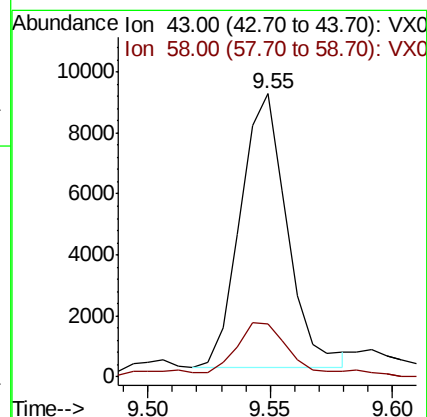





#62
4-Bromofluorobenzene
Concen: 48.41 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. -0.00 min
Lab File: VX004250.D
Acq: 24 Aug 2018 16:42




Instrument :
MSVOA_X
ClientSampleId :
BU-03-082318


Tot Ion	95	Resp	242005
Ion	Ratio	Lower	Upper
95	100		
174	93.9	0.0	185.2
176	87.1	0.0	178.6

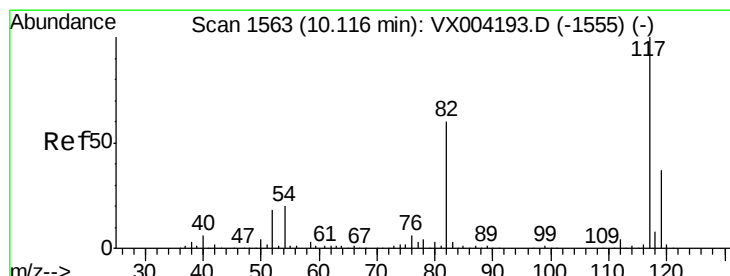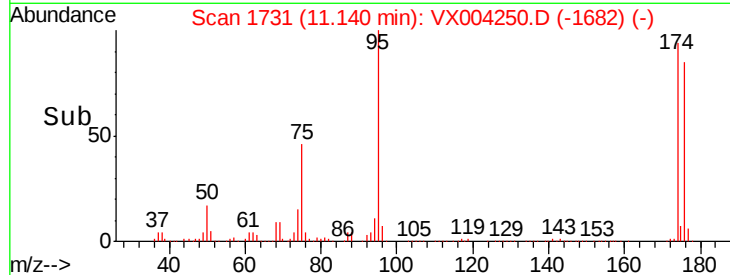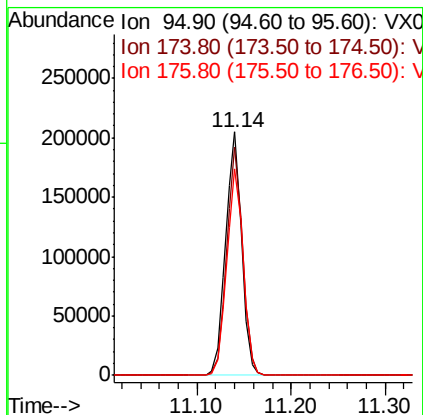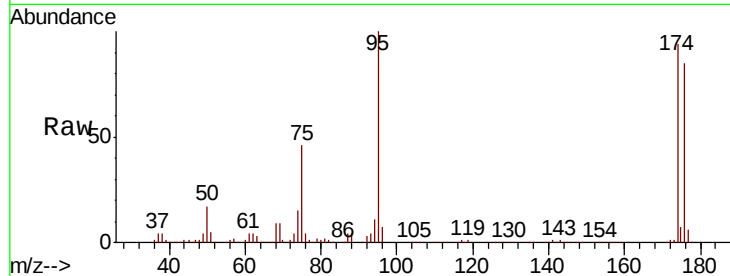

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. -0.00 min
Lab File: VX004250.D
Acq: 24 Aug 2018 16:42

Tgt Ion	117	Resp	438447
Ion	Ratio	Lower	Upper
117	100		
82	51.5	47.8	71.6
119	32.7	29.3	43.9

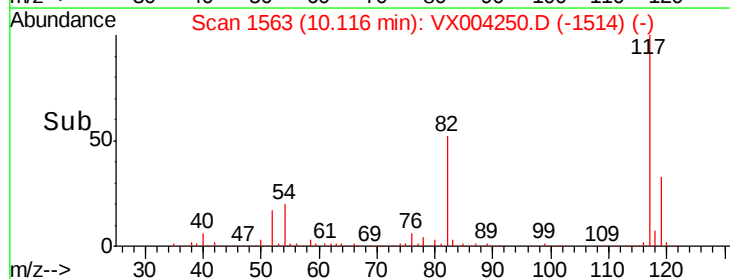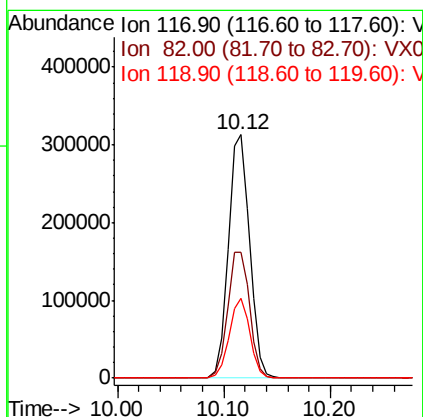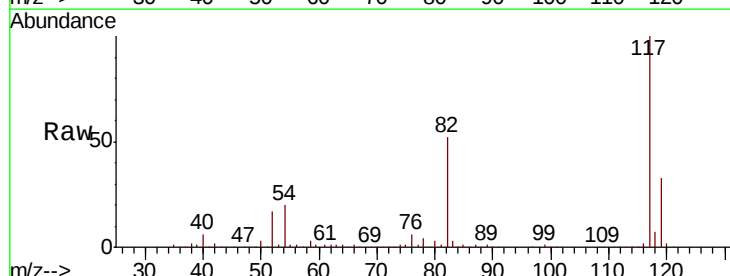


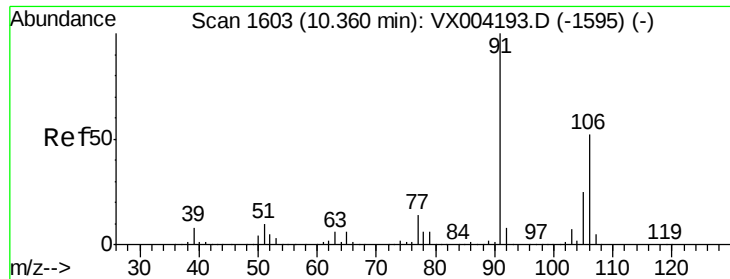




#68
m/p-Xvlenes
Concen: 0.30 ug/l
RT: 10.36 min Scan# 1603
Delta R.T. -0.00 min
Lab File: VX004250.D
Acq: 24 Aug 2018 16:42

Instrument :
MSVOA_X
ClientSampleId :
BU-03-082318

Tot Ion:106 Resp: 2091
Ion Ratio Lower Upper
106 100
91 206.7 157.1 235.7

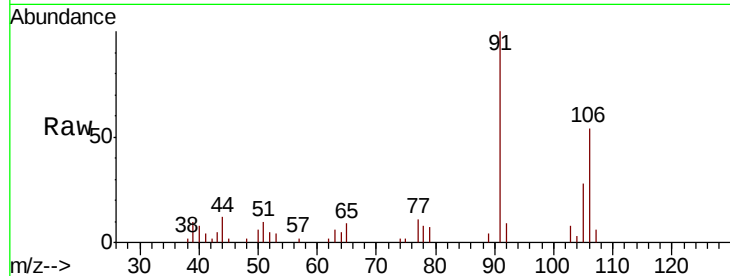


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0

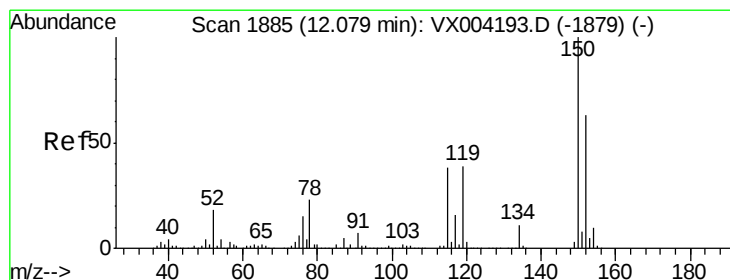
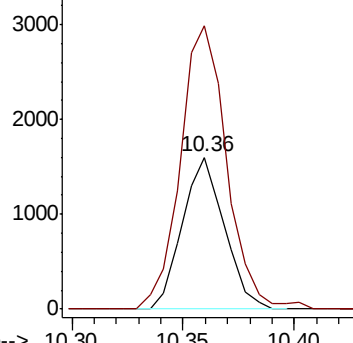



#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1885
Delta R.T. -0.00 min
Lab File: VX004250.D
Acq: 24 Aug 2018 16:42

Tgt Ion:152 Resp: 261292
Ion Ratio Lower Upper
152 100
115 54.6 39.0 117.0
150 158.4 0.0 351.0

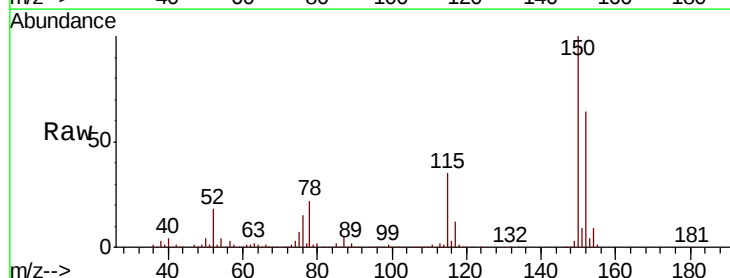

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

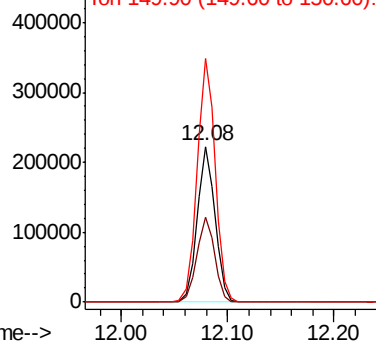



#76

1,2,3-Trichloropropane

Concen: 21.66 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42

Instrument :

MSVOA_X

ClientSampleId :


BU-03-082318

Tot Ion: 75 Resp: 115091

Ion Ratio Lower Upper




75 100

77 1.4 20.2 60.6#

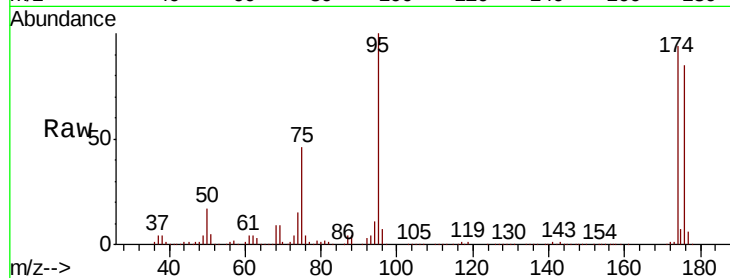

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

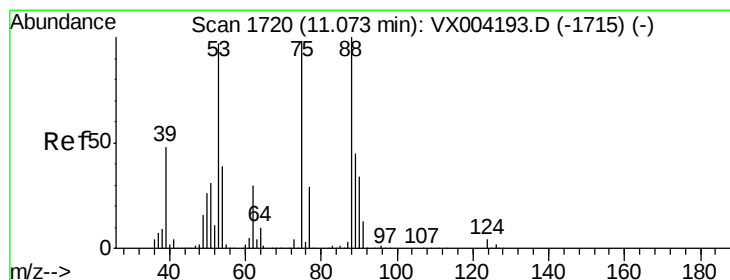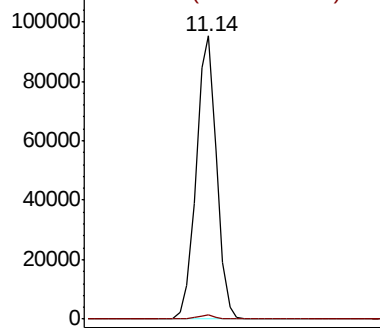

#81

trans-1,4-Dichloro-2-butene

Concen: 70.27 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.07 min

Lab File: VX004250.D

Acq: 24 Aug 2018 16:42


Tgt Ion: 75 Resp: 115091

Ion Ratio Lower Upper

75 100

53 0.1 80.1 120.1#



89 0.0 37.2 55.8#

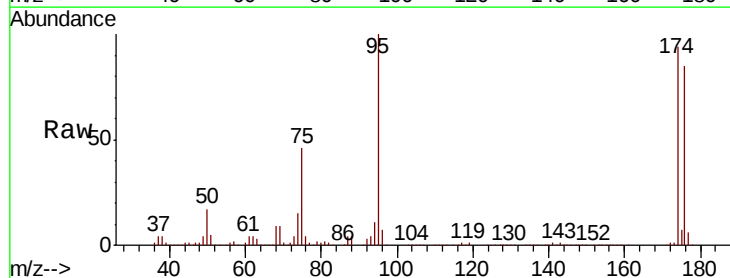


Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0




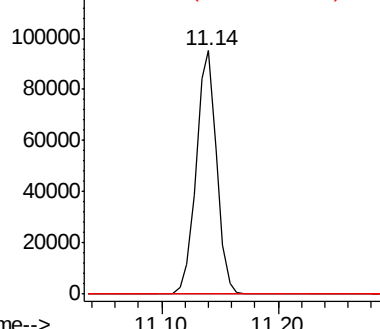




#84
 1,2,4-Trimethylbenzene
 Concen: 0.30 ug/l
 RT: 11.81 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: VX004250.D
 Acq: 24 Aug 2018 16:42

Instrument :
 MSVOA_X
 ClientSampleId :
 BU-03-082318

Tot Ion:105 Resp: 4359
 Ion Ratio Lower Upper
 105 100
 120 41.5 23.2 69.6

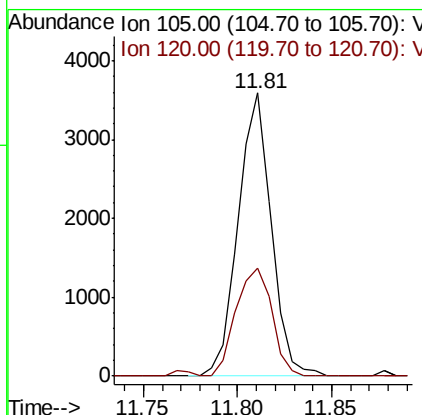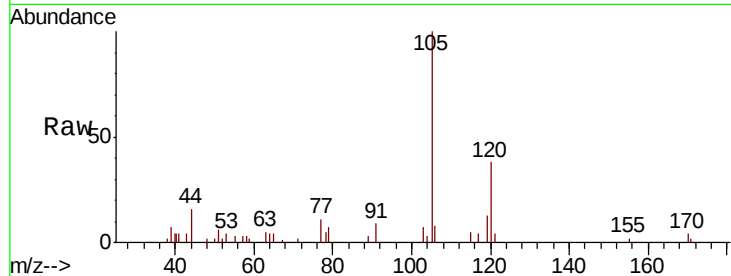

#95
 Naphthalene
 Concen: 1.46 ug/l
 RT: 13.83 min Scan# 2173
 Delta R.T. -0.00 min
 Lab File: VX004250.D
 Acq: 24 Aug 2018 16:42

Tgt Ion:128 Resp: 24969
 Ion Ratio Lower Upper
 128 100
 127 13.4 10.2 15.2
 129 11.0 8.6 12.8

