


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082418\
Data File : VX004238.D
Acq On : 24 Aug 2018 10:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260
Last Update : Thu Aug 23 05:39:44 2018

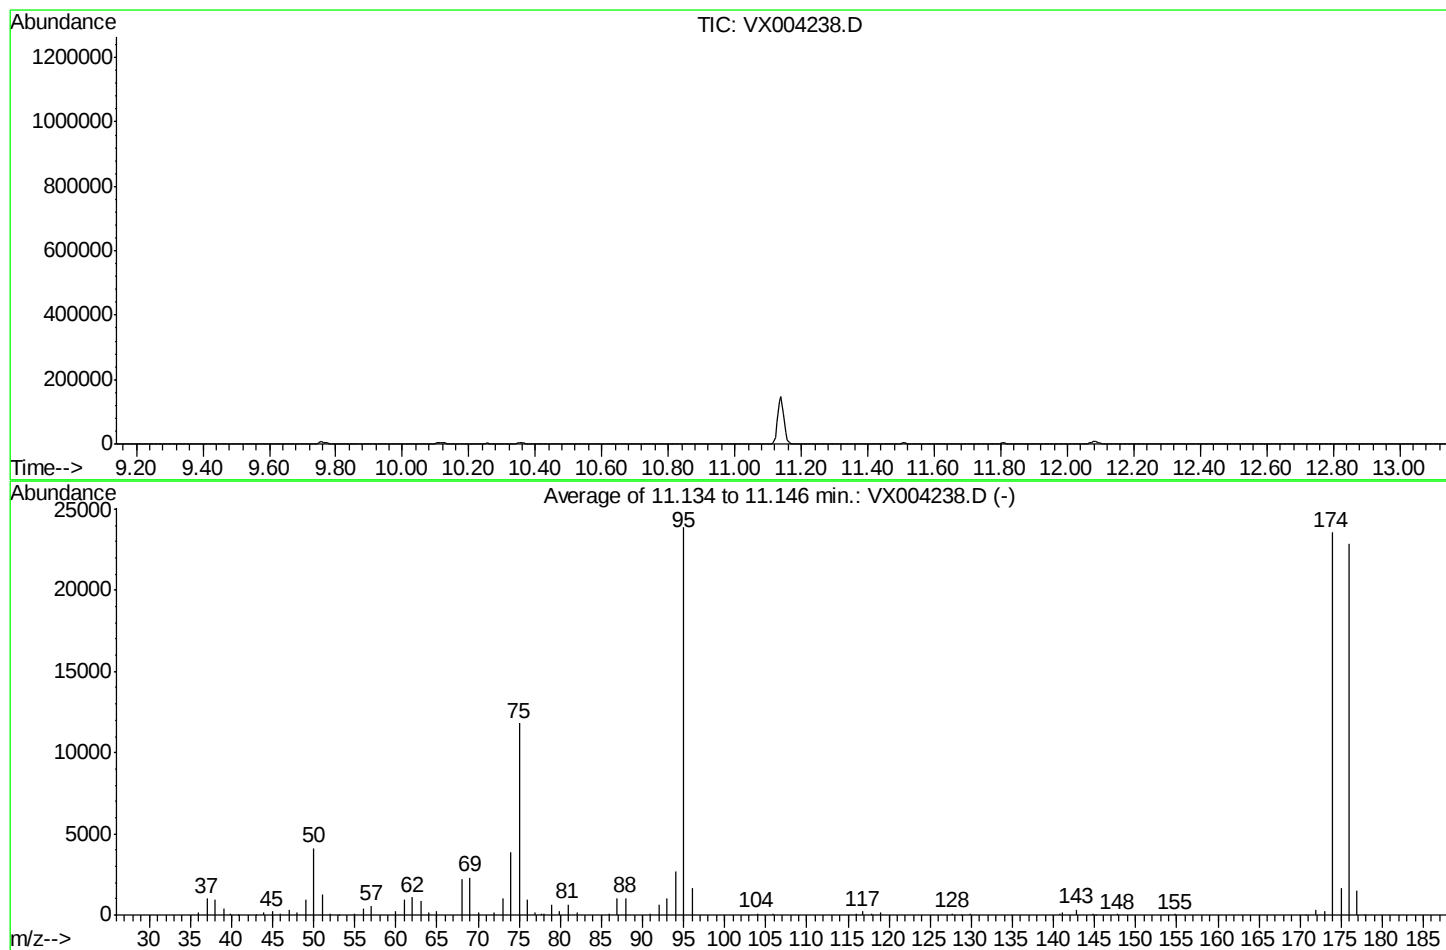

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	4125	PASS
75	95	30	60	49.4	11795	PASS
95	95	100	100	100.0	23877	PASS
96	95	5	9	7.0	1682	PASS
173	174	0.00	2	1.1	251	PASS
174	95	50	100	98.6	23546	PASS
175	174	5	9	7.2	1685	PASS
176	174	95	101	97.2	22896	PASS
177	176	5	9	6.6	1510	PASS