


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082419\  
 Data File : VX011813.D  
 Acq On : 24 Aug 2019 12:40  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X082219W.M  
 Title : SW846 8260  
 Last Update : Fri Aug 23 01:48:12 2019

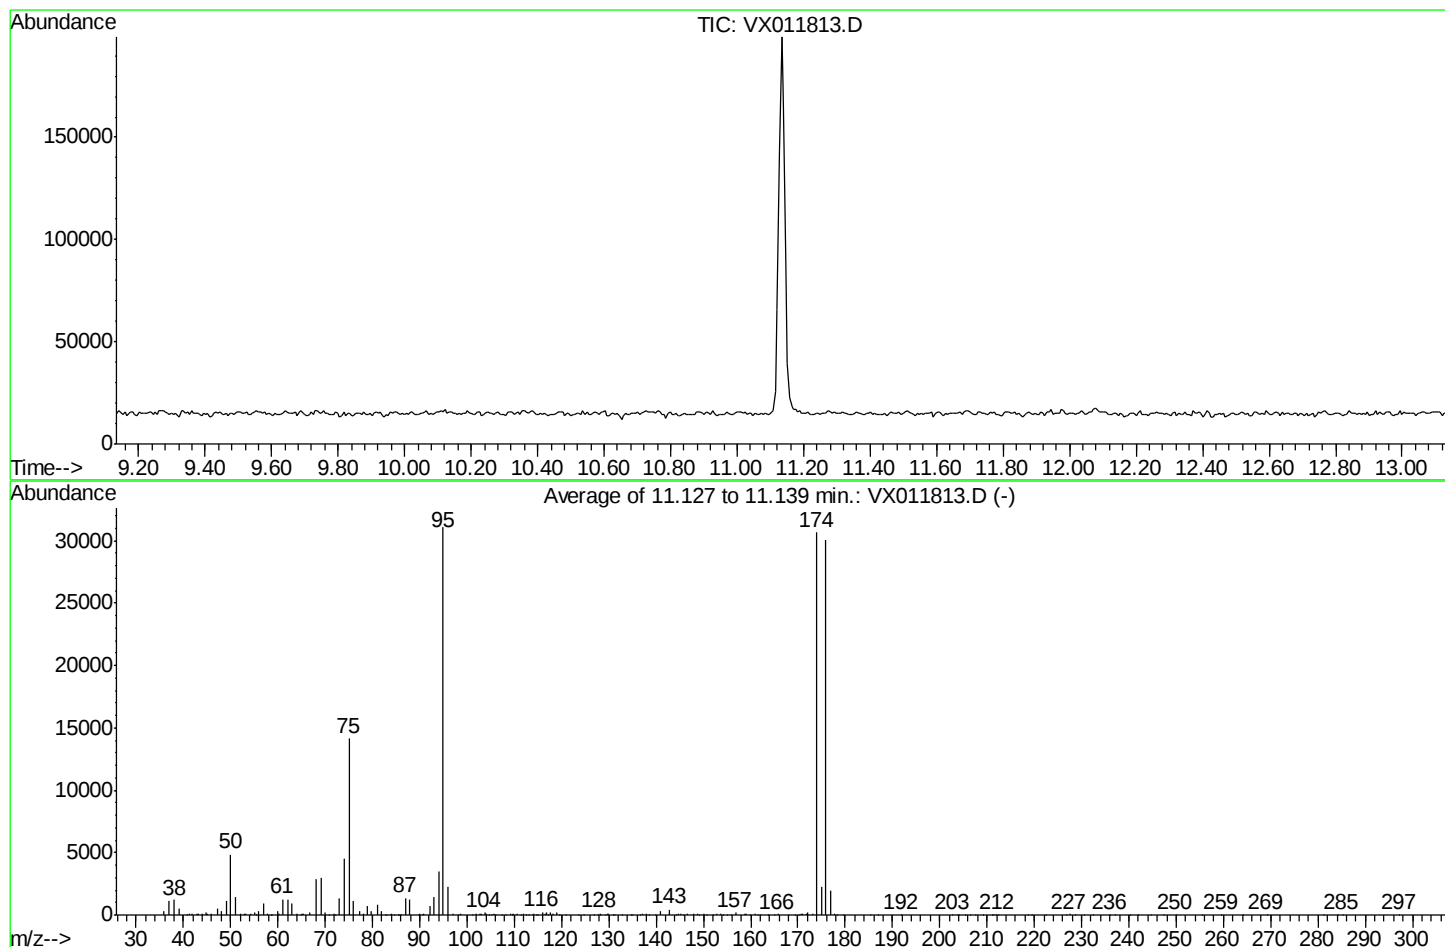

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1625

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.6      | 4842    | PASS             |
| 75          | 95           | 30           | 60           | 45.5      | 14136   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 31066   | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 2237    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.4       | 134     | PASS             |
| 174         | 95           | 50           | 100          | 98.8      | 30682   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 2261    | PASS             |
| 176         | 174          | 95           | 101          | 98.0      | 30074   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 1970    | PASS             |