

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082421\
 Data File : VX023921.D
 Acq On : 24 Aug 2021 11:01
 Operator : JC/MD
 Sample : VX0824WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0824WBL01

Quant Time: Aug 25 03:54:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	201401	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	332200	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	297690	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	128143	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	151628	53.942	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 107.880%	
35) Dibromofluoromethane	5.397	113	112066	50.968	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.940%	
50) Toluene-d8	8.653	98	406370	48.559	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 97.120%	
62) 4-Bromofluorobenzene	11.085	95	141006	45.771	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 91.540%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082421\
Data File : VX023921.D
Acq On : 24 Aug 2021 11:01
Operator : JC/MD
Sample : VX0824WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL01

Quant Time: Aug 25 03:54:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration




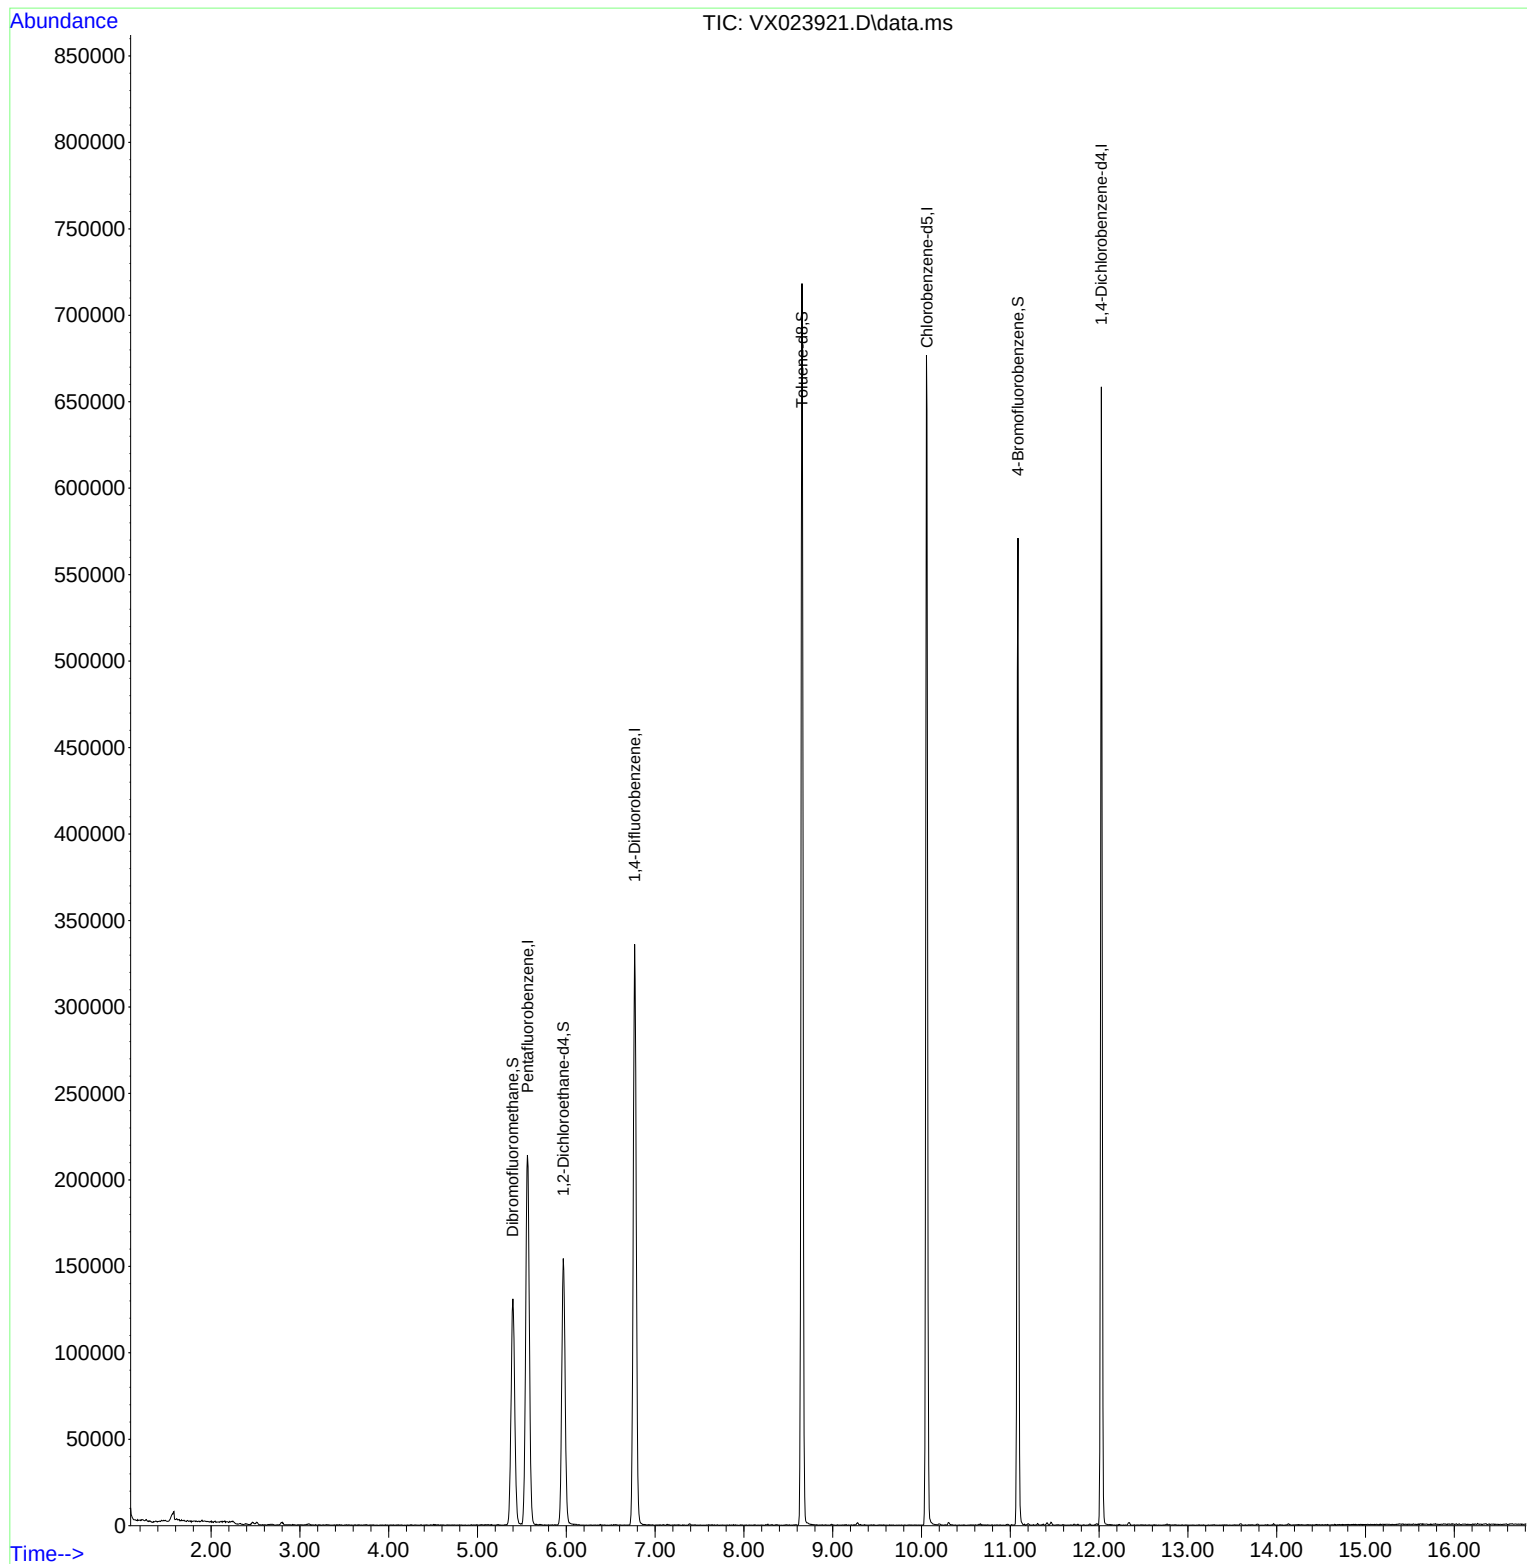


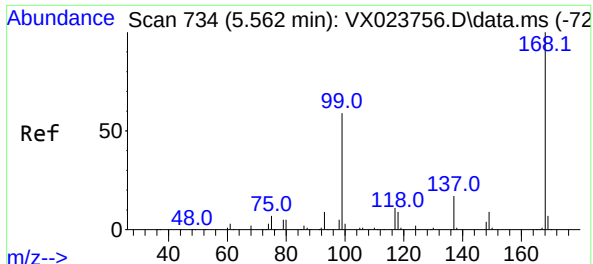

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01




Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL01


Tgt Ion:168 Resp: 201401
Ion Ratio Lower Upper
168 100
99 60.2 45.8 68.6

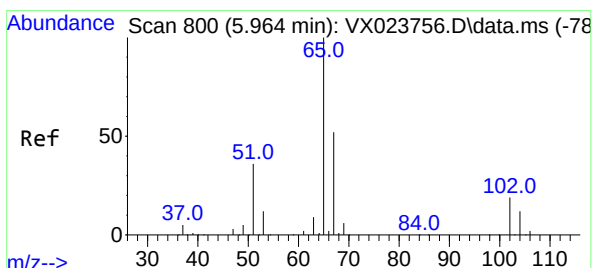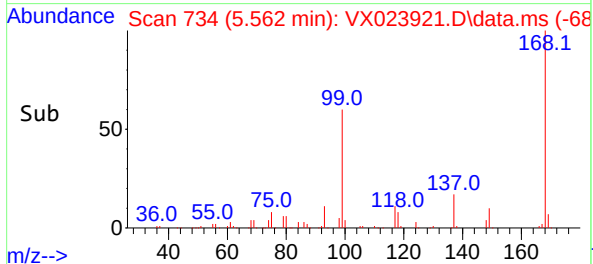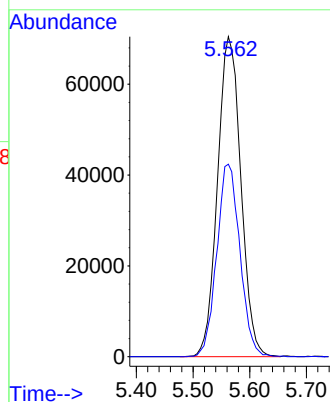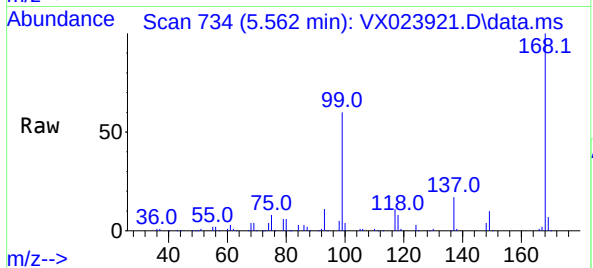

#33
1,2-Dichloroethane-d4
Concen: 53.942 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01

Tgt Ion: 65 Resp: 151628
Ion Ratio Lower Upper
65 100
67 50.4 0.0 105.4


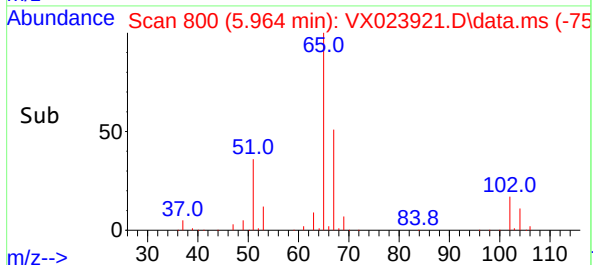
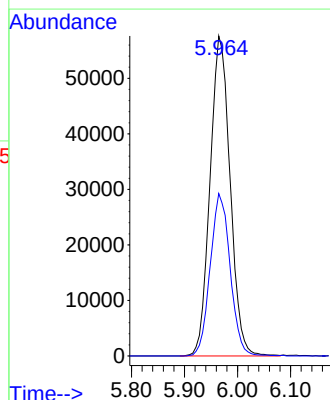
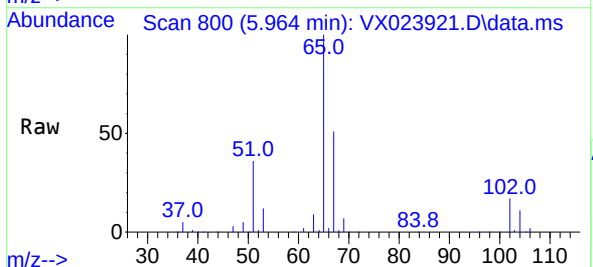


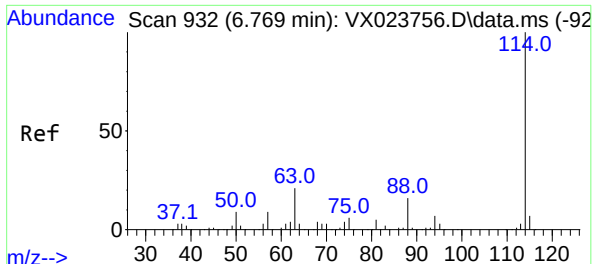

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01




Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL01


Tgt Ion:114 Resp: 332200
Ion Ratio Lower Upper
114 100
63 19.7 0.0 40.8
88 16.7 0.0 32.8

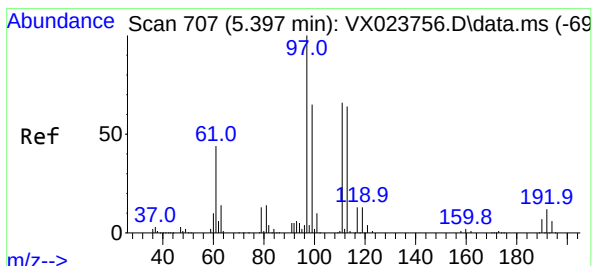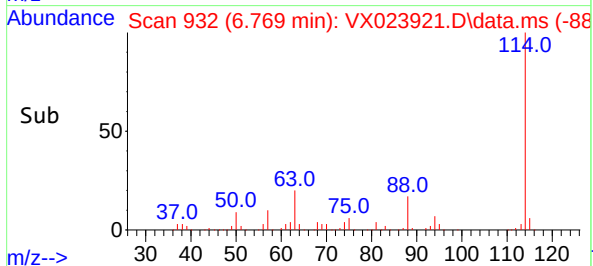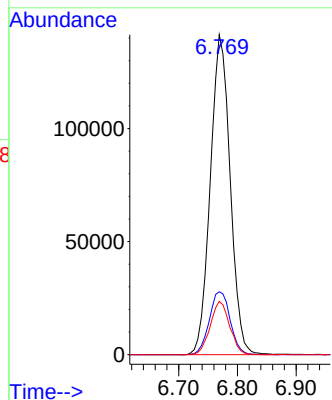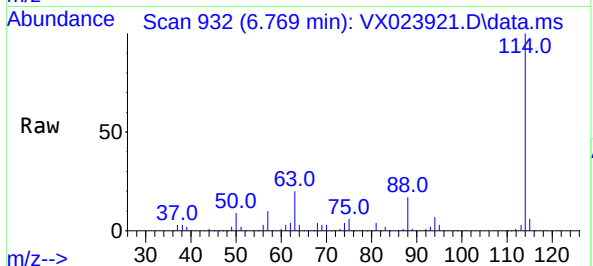

#35
Dibromofluoromethane
Concen: 50.968 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01

Tgt Ion:113 Resp: 112066
Ion Ratio Lower Upper
113 100
111 101.0 81.9 122.9
192 19.7 16.7 25.1


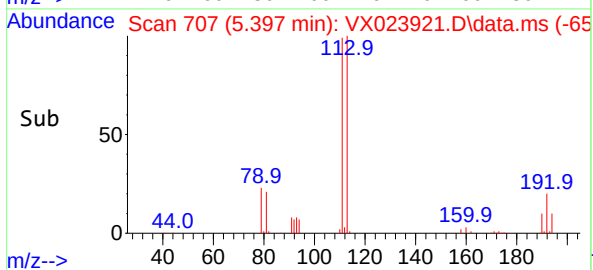
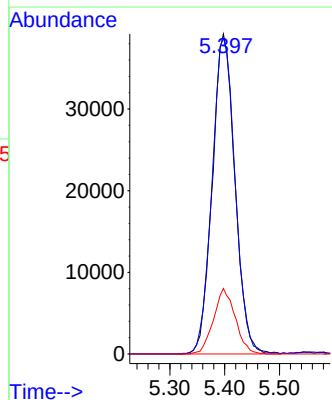
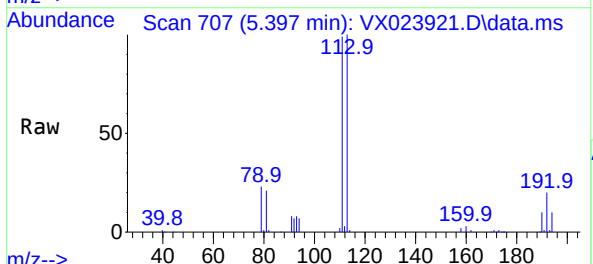


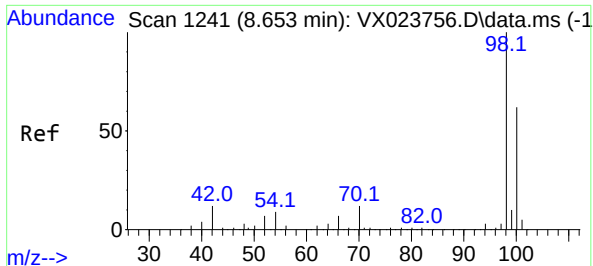

#50
Toluene-d8
Concen: 48.559 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01




Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL01


Tgt Ion: 98 Resp: 406370
Ion Ratio Lower Upper
98 100
100 63.7 51.9 77.9

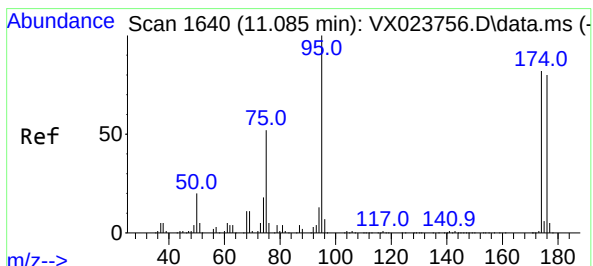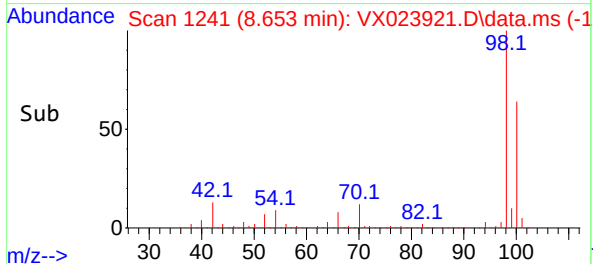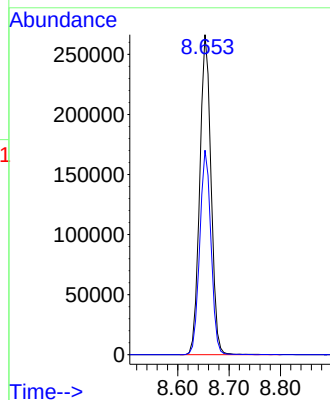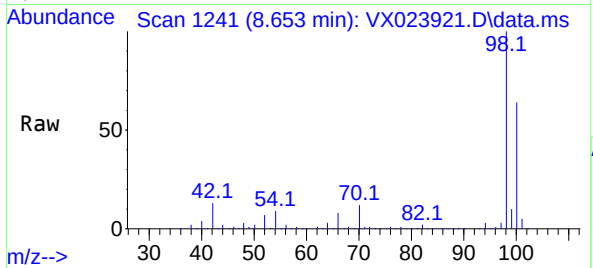

#62
4-Bromofluorobenzene
Concen: 45.771 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01

Tgt Ion: 95 Resp: 141006
Ion Ratio Lower Upper
95 100
174 80.5 0.0 154.6
176 76.7 0.0 155.8


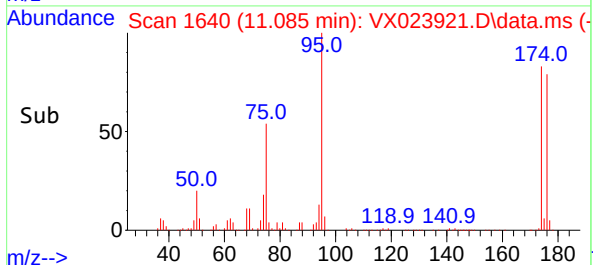
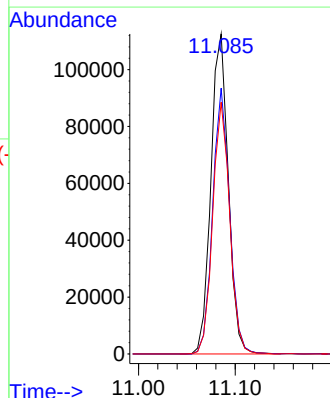
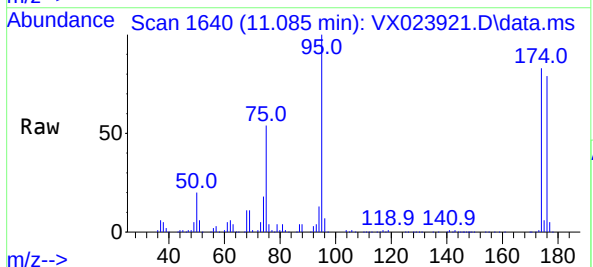


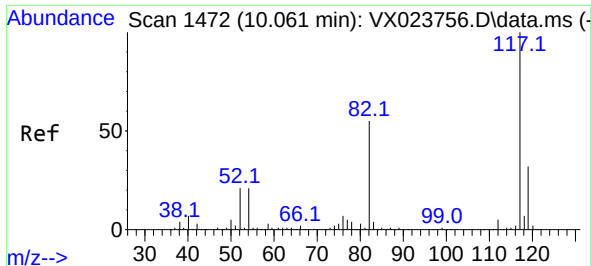

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01

Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL01

Tgt Ion:117 Resp: 297690
Ion Ratio Lower Upper
117 100
82 55.1 47.4 71.2
119 32.0 26.6 39.8

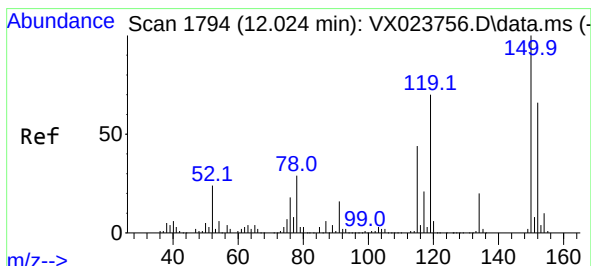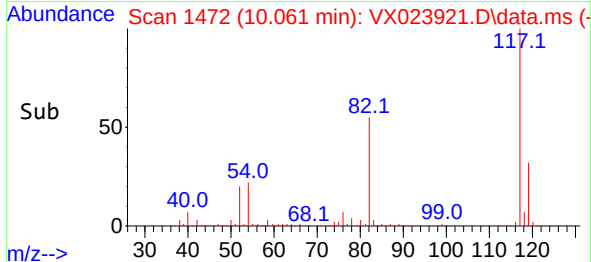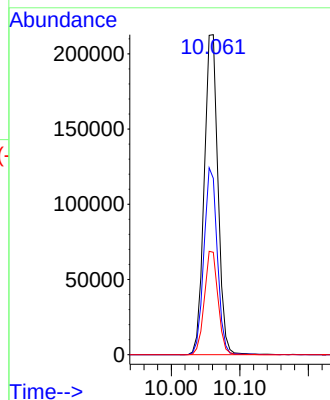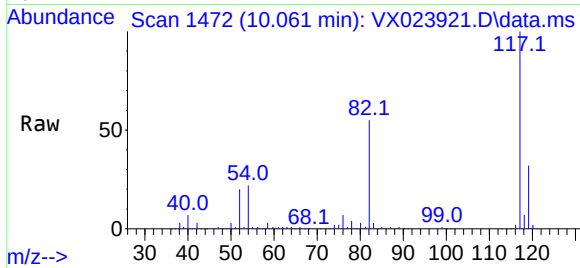

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023921.D
Acq: 24 Aug 2021 11:01

Tgt Ion:152 Resp: 128143
Ion Ratio Lower Upper
152 100
115 60.2 41.1 123.3
150 154.4 0.0 349.0

