
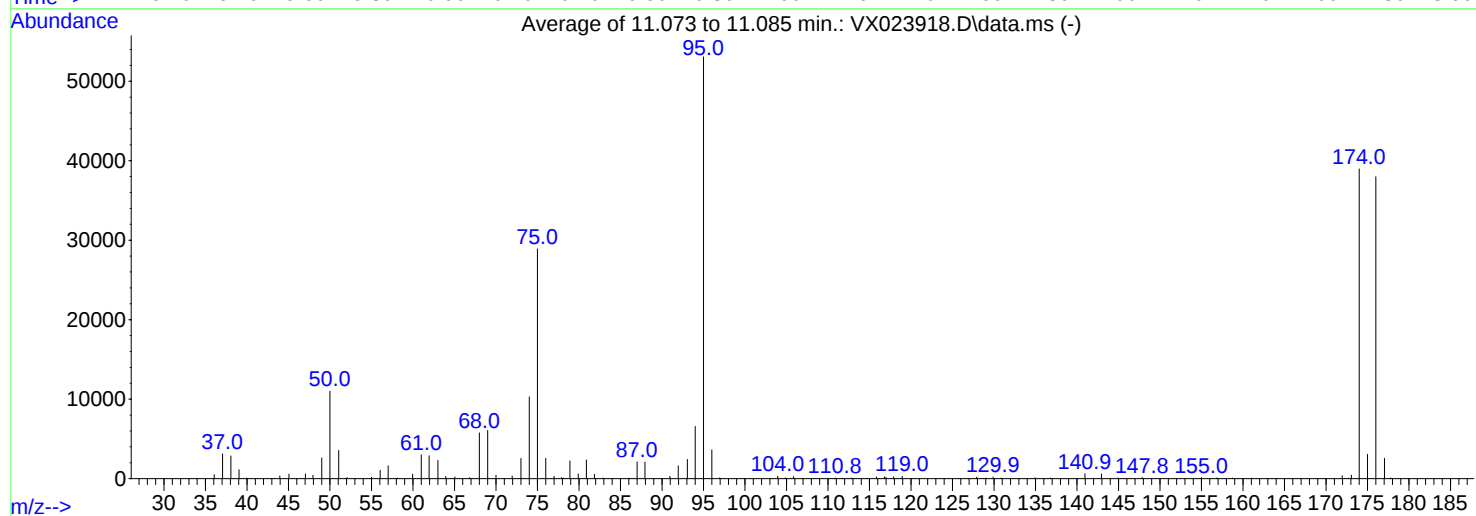


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082421\
 Data File : VX023918.D
 Acq On : 24 Aug 2021 07:25
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260
 Last Update : Tue Aug 17 11:57:51 2021

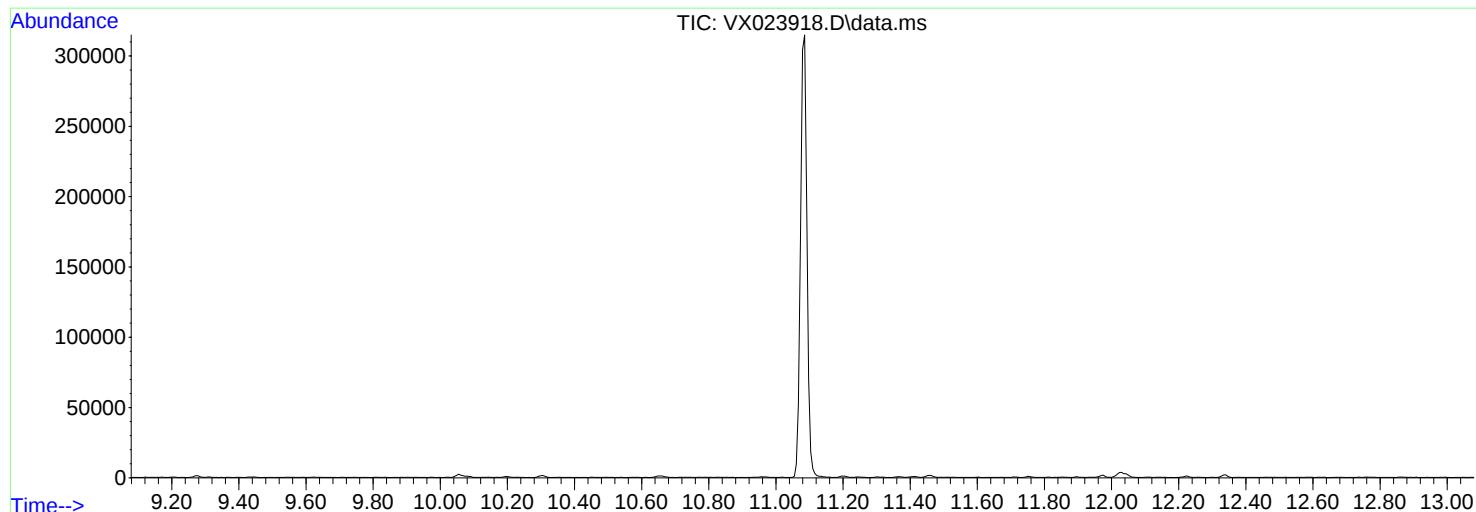

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	11011	PASS
75	95	30	60	54.5	28909	PASS
95	95	100	100	100.0	53069	PASS
96	95	5	9	6.8	3621	PASS
173	174	0.00	2	1.1	439	PASS
174	95	50	100	73.4	38976	PASS
175	174	5	9	7.9	3067	PASS
176	174	95	101	97.5	37997	PASS
177	176	5	9	6.7	2561	PASS