

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
 Data File : VX037231.D
 Acq On : 24 Aug 2023 22:22
 Operator : JC/MD
 Sample : VX0824WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0824WBL02

Quant Time: Aug 24 23:22:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	152122	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	249953	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	224579	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	104108	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	95838	43.700	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	87.400%
35) Dibromofluoromethane	5.385	113	77036	46.537	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.080%
50) Toluene-d8	8.647	98	291733	48.584	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.160%
62) 4-Bromofluorobenzene	11.079	95	111631	47.306	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.620%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037231.D
Acq On : 24 Aug 2023 22:22
Operator : JC/MD
Sample : VX0824WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL02

Quant Time: Aug 24 23:22:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




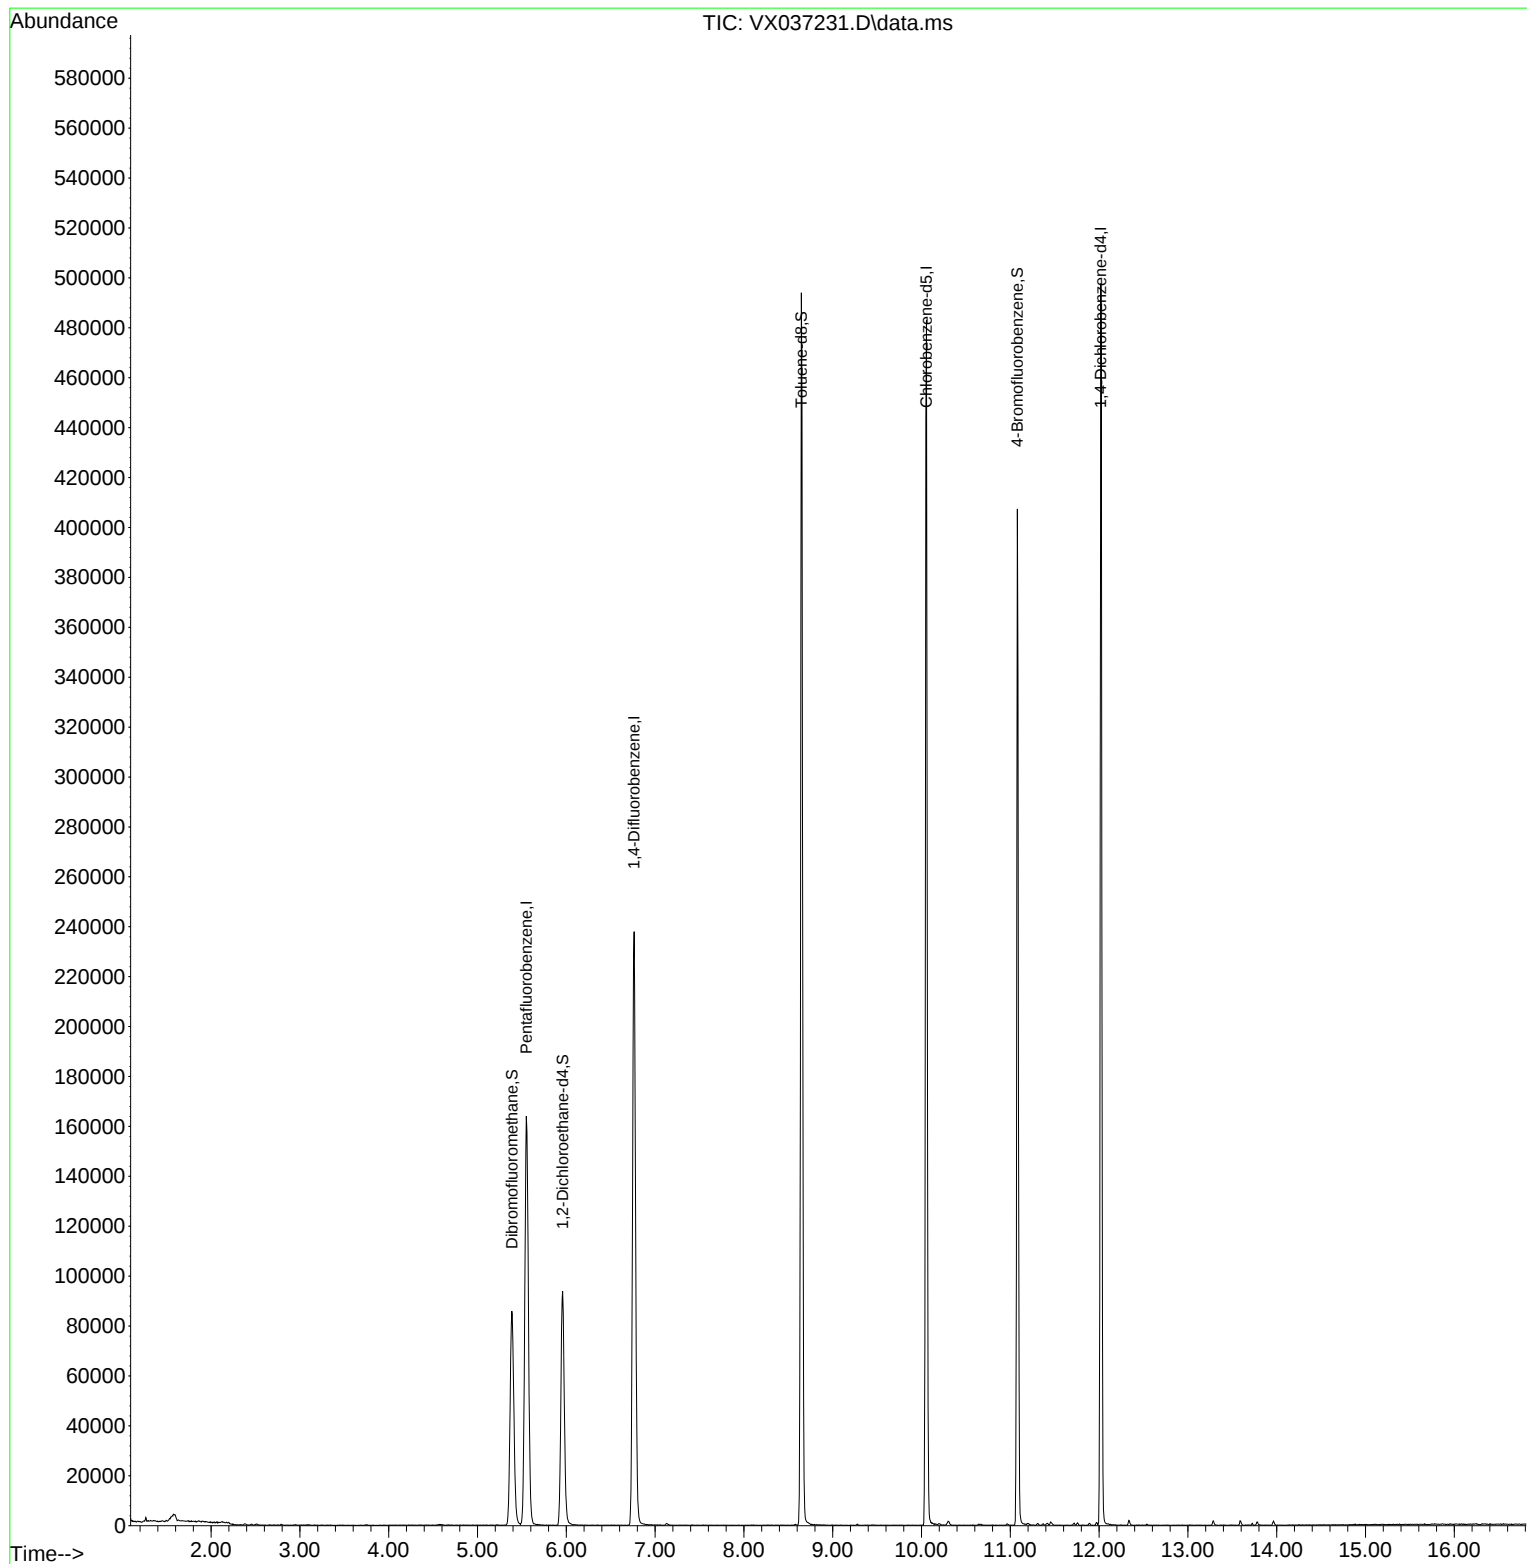




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22




Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL02

Tgt Ion:168 Resp: 152122
Ion Ratio Lower Upper
168 100
99 64.0 56.6 85.0

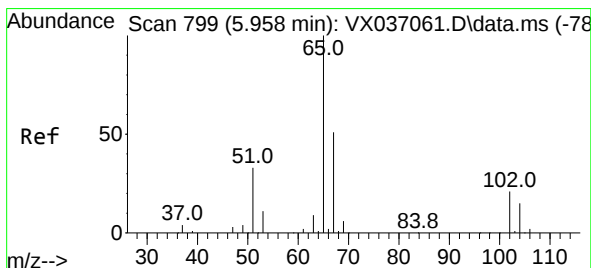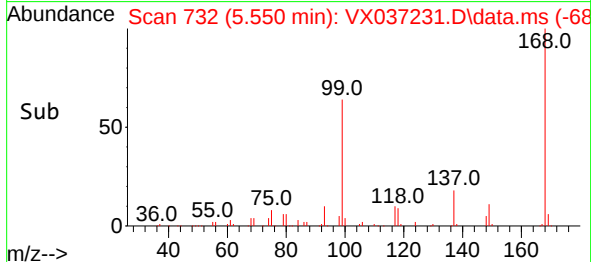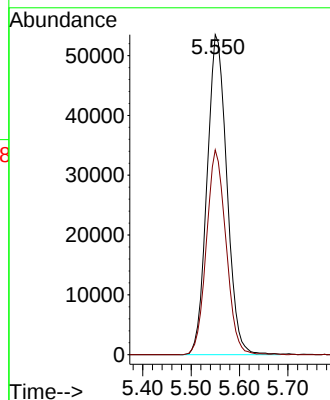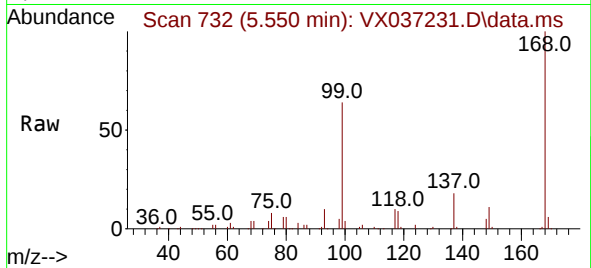

#33
1,2-Dichloroethane-d4
Concen: 43.700 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22

Tgt Ion: 65 Resp: 95838
Ion Ratio Lower Upper
65 100
67 50.8 0.0 100.2

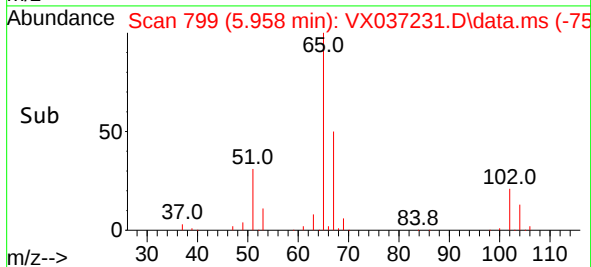
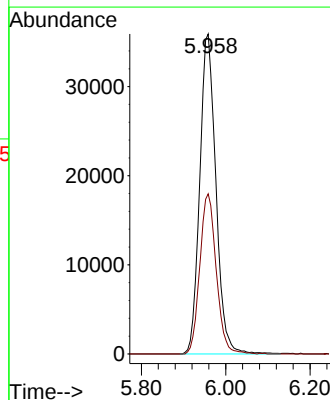
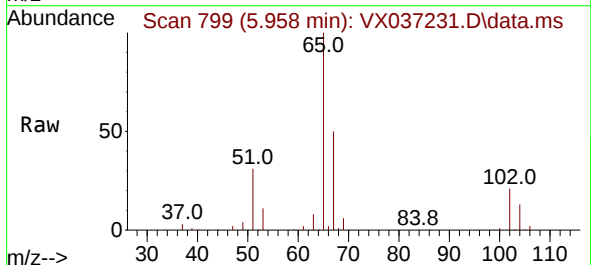




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22




Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL02


Tgt Ion:114 Resp: 249953
Ion Ratio Lower Upper
114 100
63 19.4 0.0 45.0
88 17.0 0.0 36.6

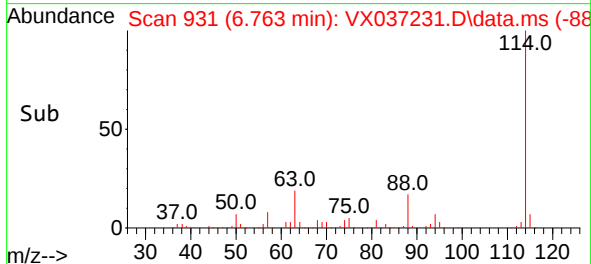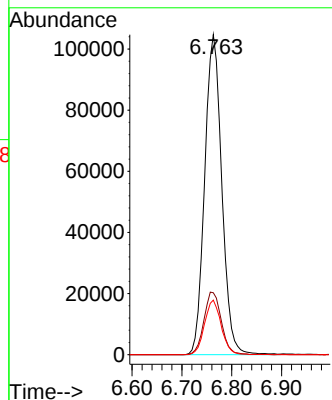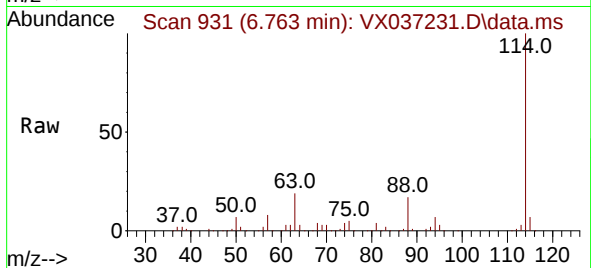

#35
Dibromofluoromethane
Concen: 46.537 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22

Tgt Ion:113 Resp: 77036
Ion Ratio Lower Upper
113 100
111 102.7 82.9 124.3
192 17.8 13.3 19.9


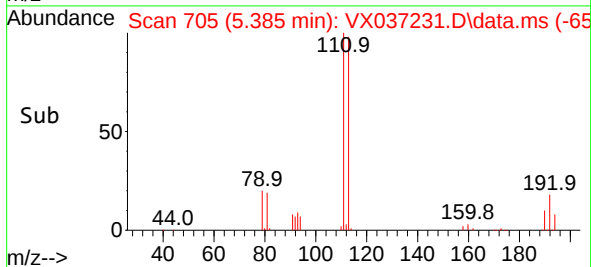
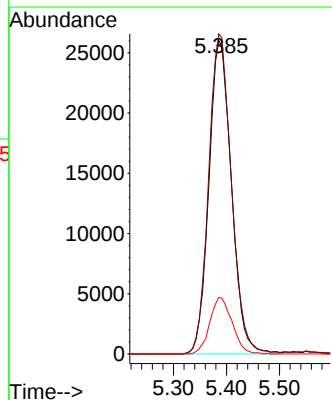
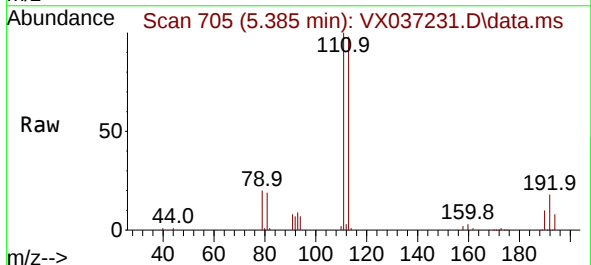


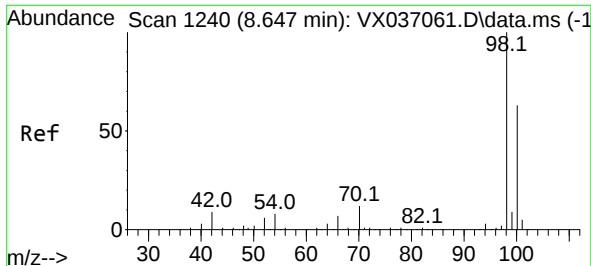

#50
Toluene-d8
Concen: 48.584 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22




Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL02


Tgt Ion: 98 Resp: 291733
Ion Ratio Lower Upper
98 100
100 66.7 53.1 79.7

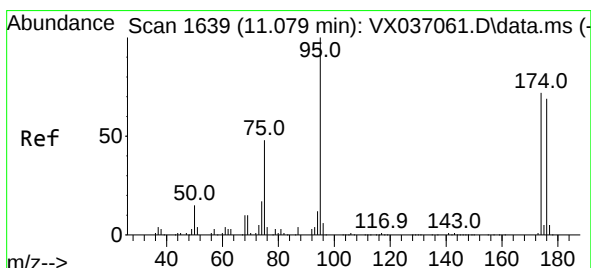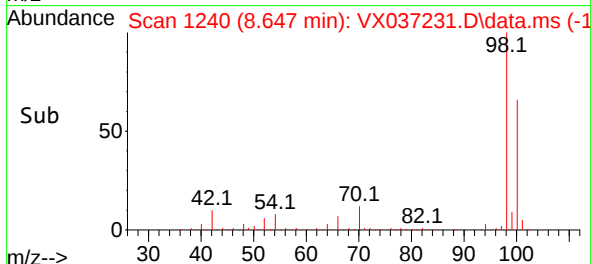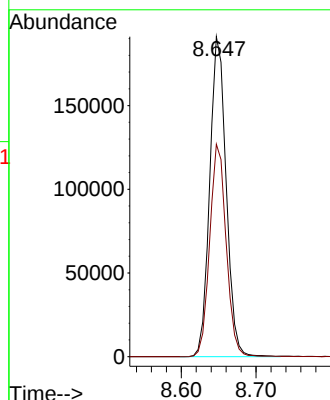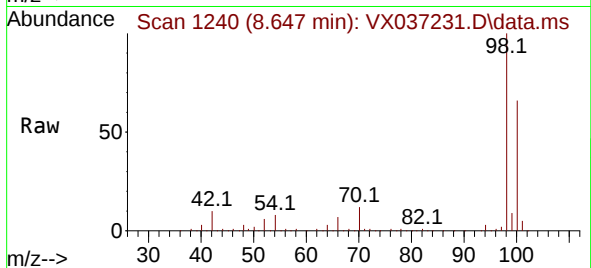

#62
4-Bromofluorobenzene
Concen: 47.306 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22

Tgt Ion: 95 Resp: 111631
Ion Ratio Lower Upper
95 100
174 73.4 0.0 135.6
176 71.0 0.0 131.0


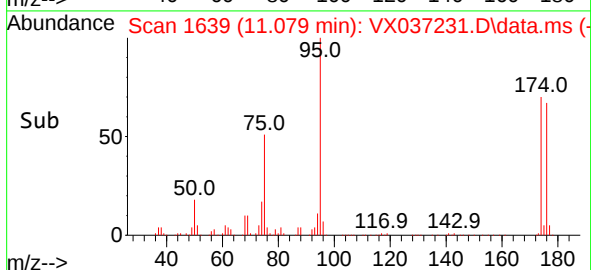
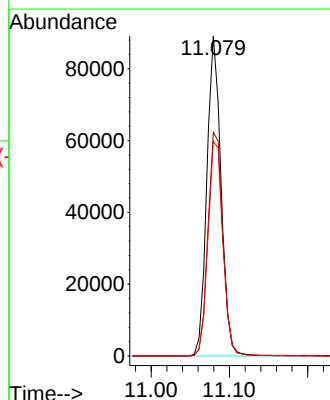
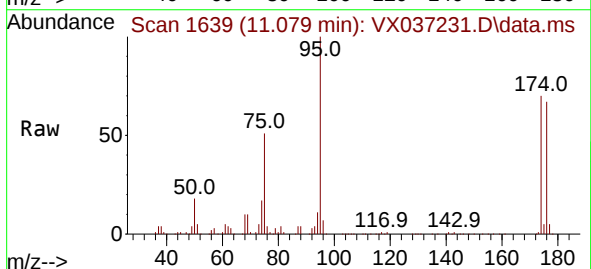


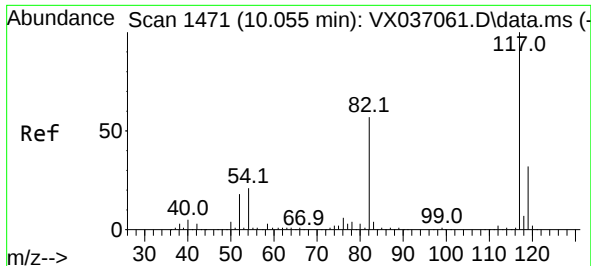

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22

Instrument :
MSVOA_X
ClientSampleId :
VX0824WBL02

Tgt Ion:117 Resp: 224579
Ion Ratio Lower Upper
117 100
82 53.9 46.2 69.4
119 32.0 25.5 38.3

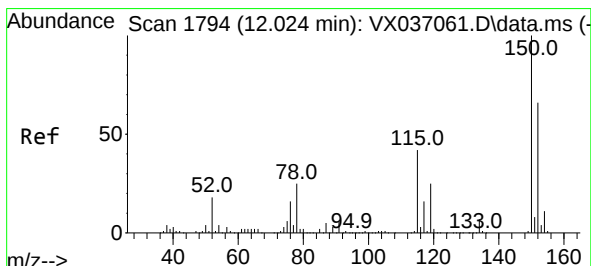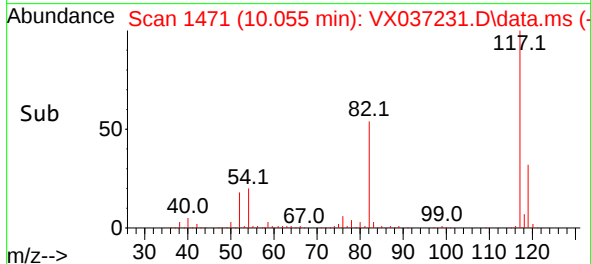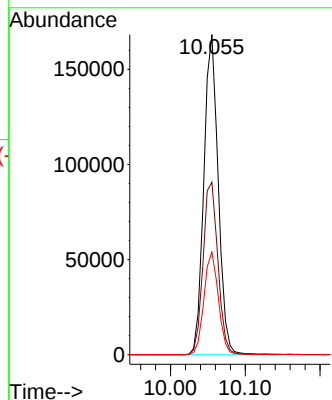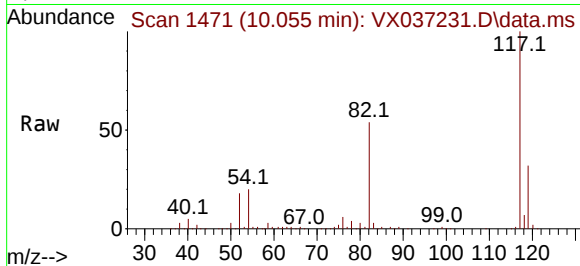

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX037231.D
Acq: 24 Aug 2023 22:22

Tgt Ion:152 Resp: 104108
Ion Ratio Lower Upper
152 100
115 63.4 43.3 129.9
150 157.3 0.0 345.0

