

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
 Data File : VX037248.D
 Acq On : 25 Aug 2023 05:11
 Operator : JC/MD
 Sample : 04095-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB04-20230818

Quant Time: Aug 25 07:46:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 18 09:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	147091	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	243494	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	218833	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	98653	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	92665	43.698	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	87.400%
35) Dibromofluoromethane	5.385	113	74600	46.261	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.520%
50) Toluene-d8	8.647	98	282735	48.335	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	96.660%
62) 4-Bromofluorobenzene	11.079	95	106389	46.281	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.560%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037248.D
Acq On : 25 Aug 2023 05:11
Operator : JC/MD
Sample : 04095-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB04-20230818

Quant Time: Aug 25 07:46:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 18 09:30:38 2023
Response via : Initial Calibration




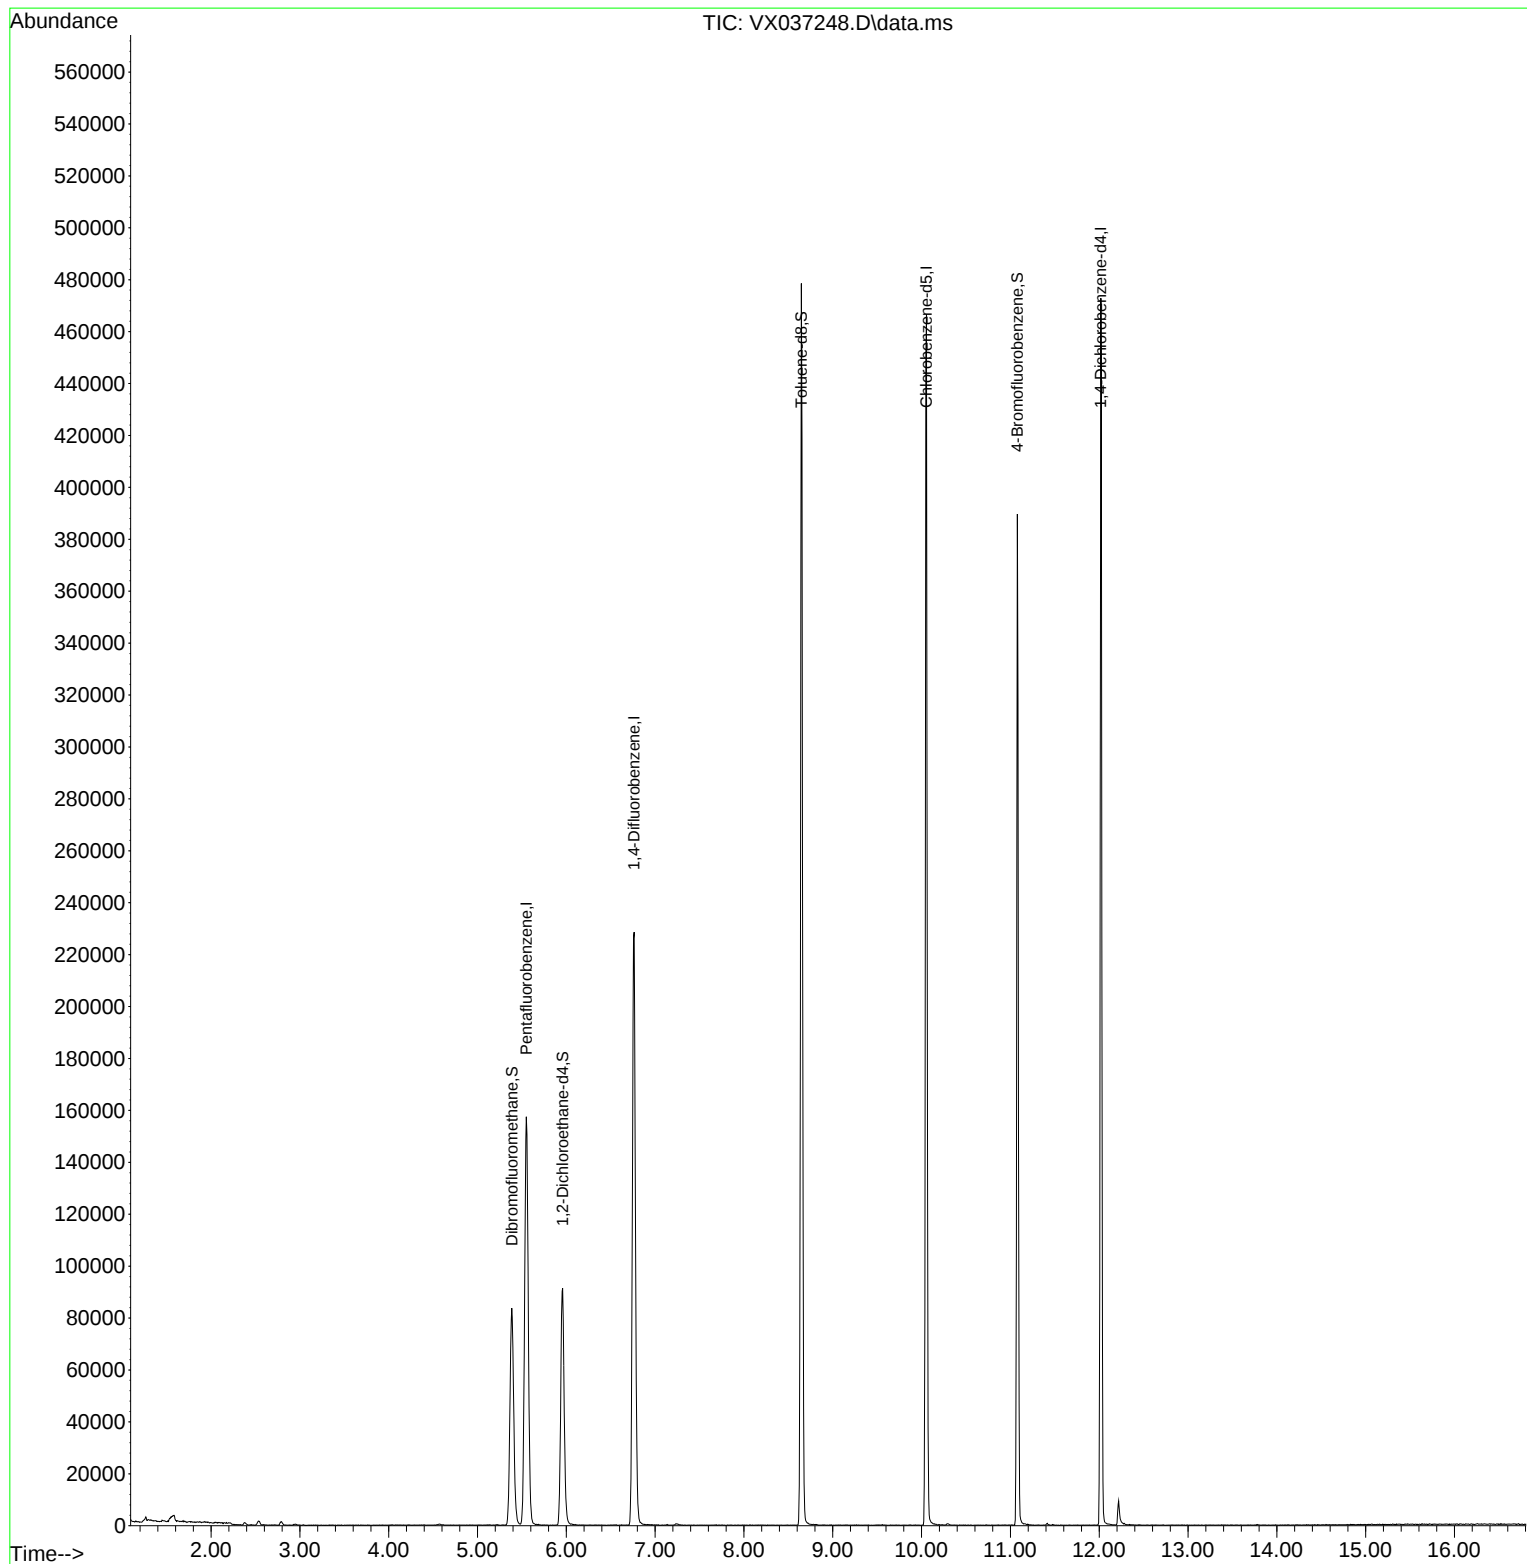




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11




Instrument :
MSVOA_X
ClientSampleId :
TB04-20230818


Tgt Ion:168 Resp: 147091
Ion Ratio Lower Upper
168 100
99 64.5 56.6 85.0

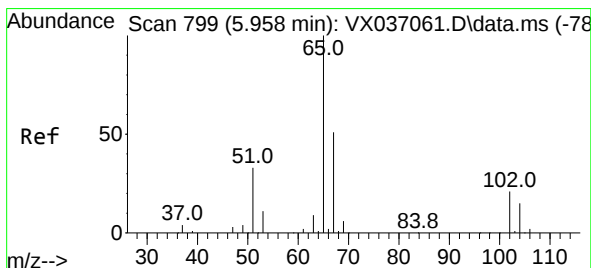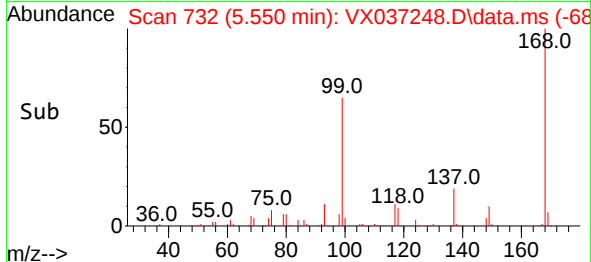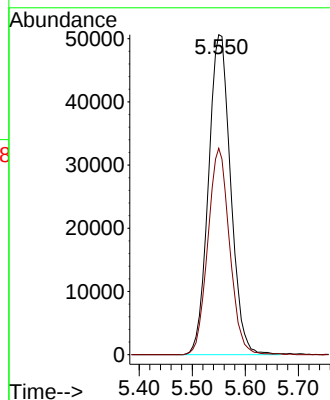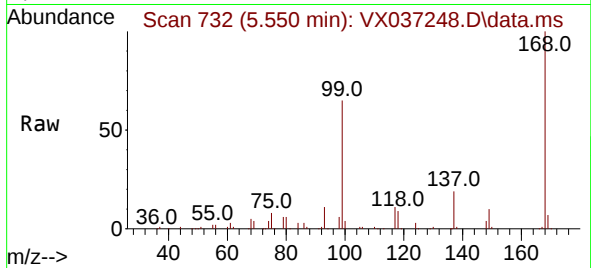

#33
1,2-Dichloroethane-d4
Concen: 43.698 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11

Tgt Ion: 65 Resp: 92665
Ion Ratio Lower Upper
65 100
67 51.1 0.0 100.2

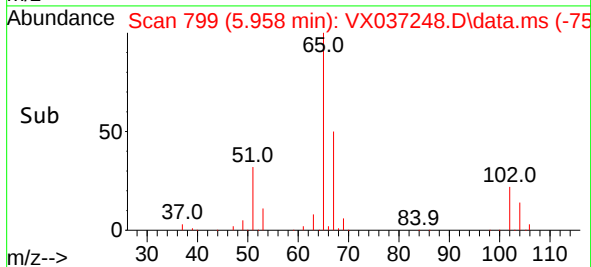
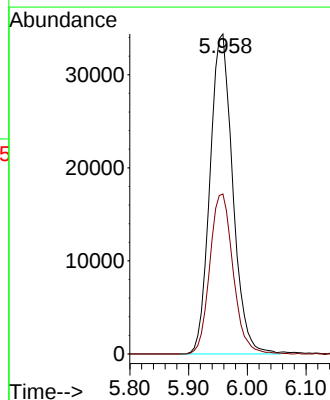
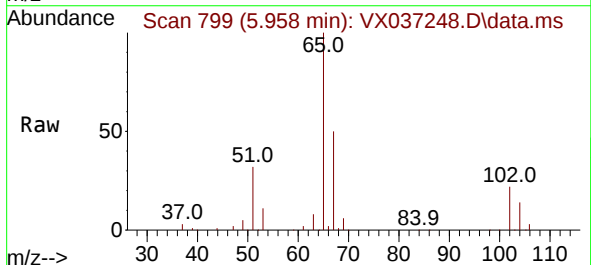


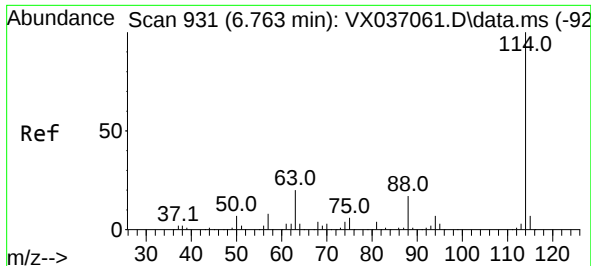

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11




Instrument :
MSVOA_X
ClientSampleId :
TB04-20230818


Tgt Ion:114 Resp: 243494
Ion Ratio Lower Upper
114 100
63 20.5 0.0 45.0
88 17.3 0.0 36.6

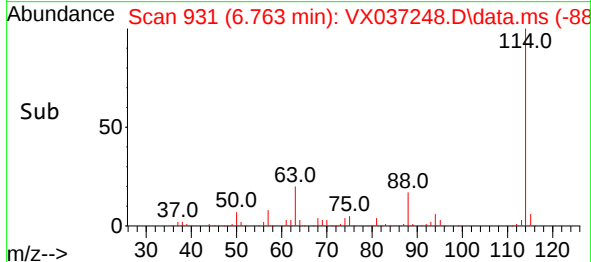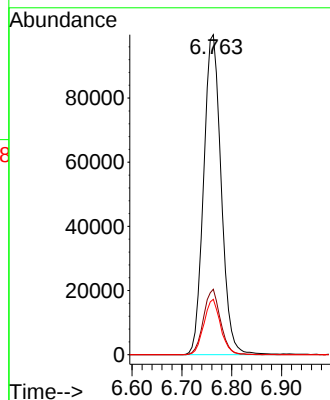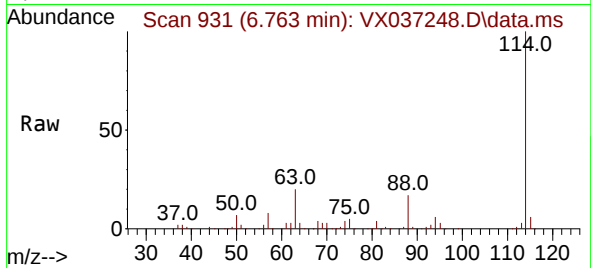

#35
Dibromofluoromethane
Concen: 46.261 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11

Tgt Ion:113 Resp: 74600
Ion Ratio Lower Upper
113 100
111 102.8 82.9 124.3
192 18.7 13.3 19.9


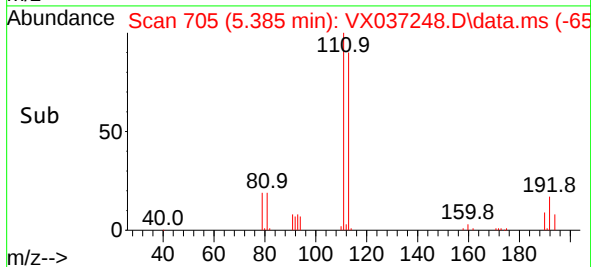
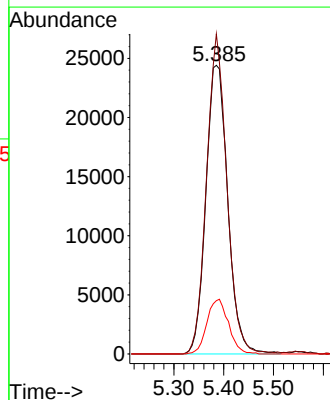
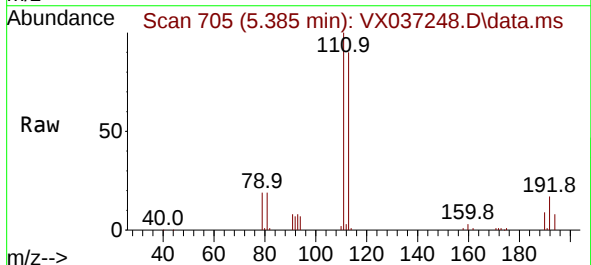


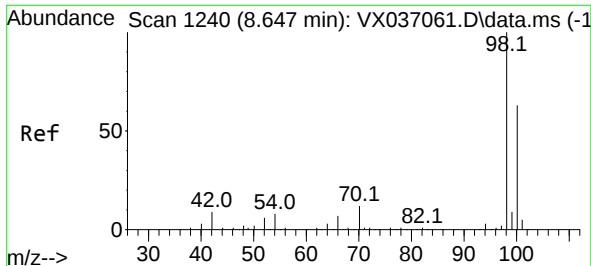

#50
Toluene-d8
Concen: 48.335 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11




Instrument :
MSVOA_X
ClientSampleId :
TB04-20230818


Tgt Ion: 98 Resp: 282735
Ion Ratio Lower Upper
98 100
100 67.2 53.1 79.7

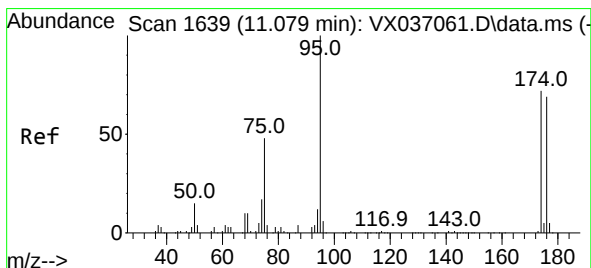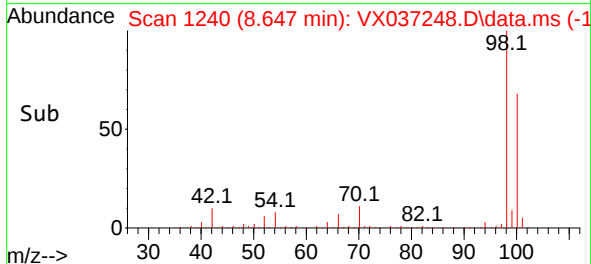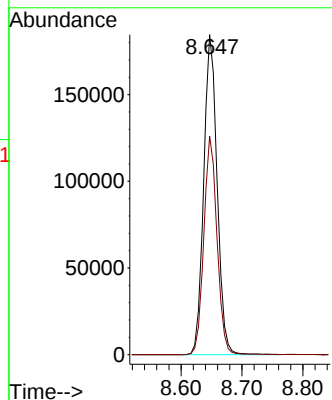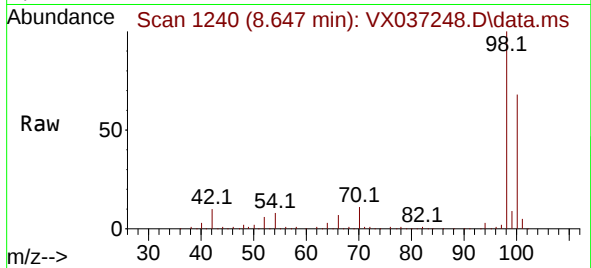

#62
4-Bromofluorobenzene
Concen: 46.281 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11

Tgt Ion: 95 Resp: 106389
Ion Ratio Lower Upper
95 100
174 73.4 0.0 135.6
176 70.8 0.0 131.0


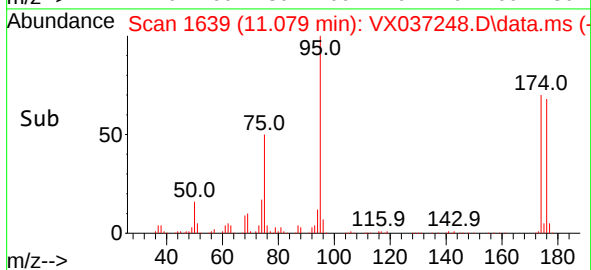
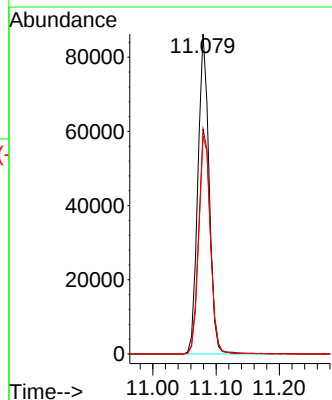
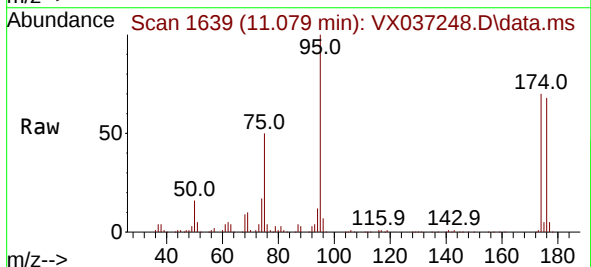


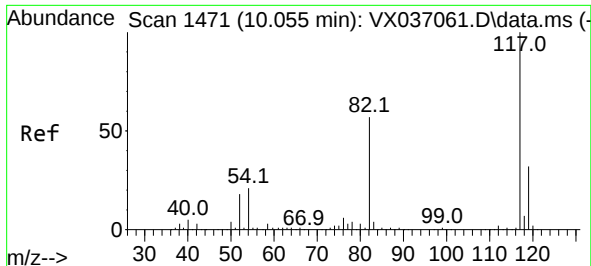

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11

Instrument :
MSVOA_X
ClientSampleId :
TB04-20230818

Tgt Ion:117 Resp: 218833
Ion Ratio Lower Upper
117 100
82 55.2 46.2 69.4
119 31.9 25.5 38.3

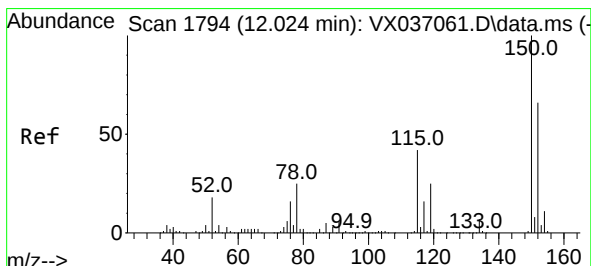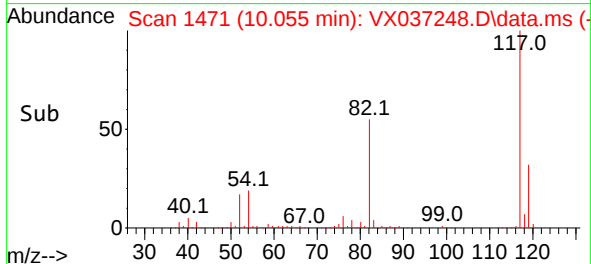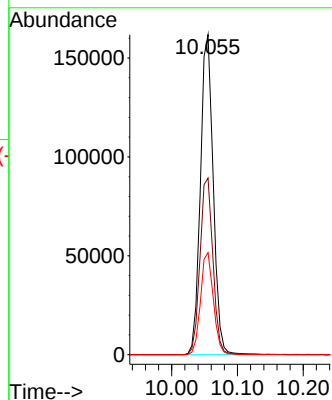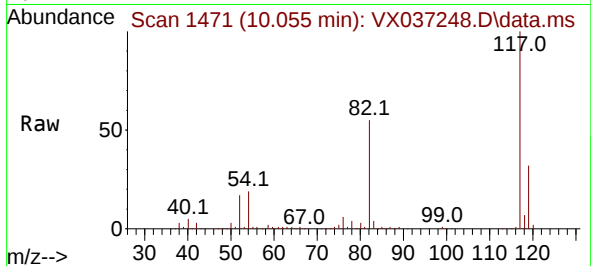

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX037248.D
Acq: 25 Aug 2023 05:11

Tgt Ion:152 Resp: 98653
Ion Ratio Lower Upper
152 100
115 63.6 43.3 129.9
150 158.0 0.0 345.0

