

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082423\  
Data File : VX037209.D  
Acq On : 24 Aug 2023 12:17  
Operator : JC/MD  
Sample : 04093-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-20230818

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037209.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.947       | 296           | 305         | 315          | rVB      | 6460           | 14960         | 1.98%           | 0.363%        |
| 2         | 4.568       | 563           | 571         | 582          | rBV2     | 4083           | 13259         | 1.76%           | 0.322%        |
| 3         | 5.385       | 692           | 705         | 721          | rBV      | 85871          | 251357        | 33.32%          | 6.095%        |
| 4         | 5.550       | 721           | 732         | 749          | rVV      | 163443         | 457700        | 60.68%          | 11.098%       |
| 5         | 5.952       | 788           | 798         | 820          | rBV2     | 92782          | 250295        | 33.18%          | 6.069%        |
| 6         | 6.763       | 921           | 931         | 952          | rBV      | 235569         | 564184        | 74.80%          | 13.681%       |
| 7         | 8.647       | 1233          | 1240        | 1252         | rBV      | 485965         | 754286        | 100.00%         | 18.290%       |
| 8         | 10.055      | 1465          | 1471        | 1484         | rBV      | 486406         | 662745        | 87.86%          | 16.070%       |
| 9         | 11.079      | 1634          | 1639        | 1651         | rBV      | 407759         | 516987        | 68.54%          | 12.536%       |
| 10        | 12.018      | 1788          | 1793        | 1805         | rBV      | 498849         | 638220        | 84.61%          | 15.476%       |




Sum of corrected areas: 4123993

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082423\  
Data File : VX037209.D  
Acq On : 24 Aug 2023 12:17  
Operator : JC/MD  
Sample : 04093-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-20230818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

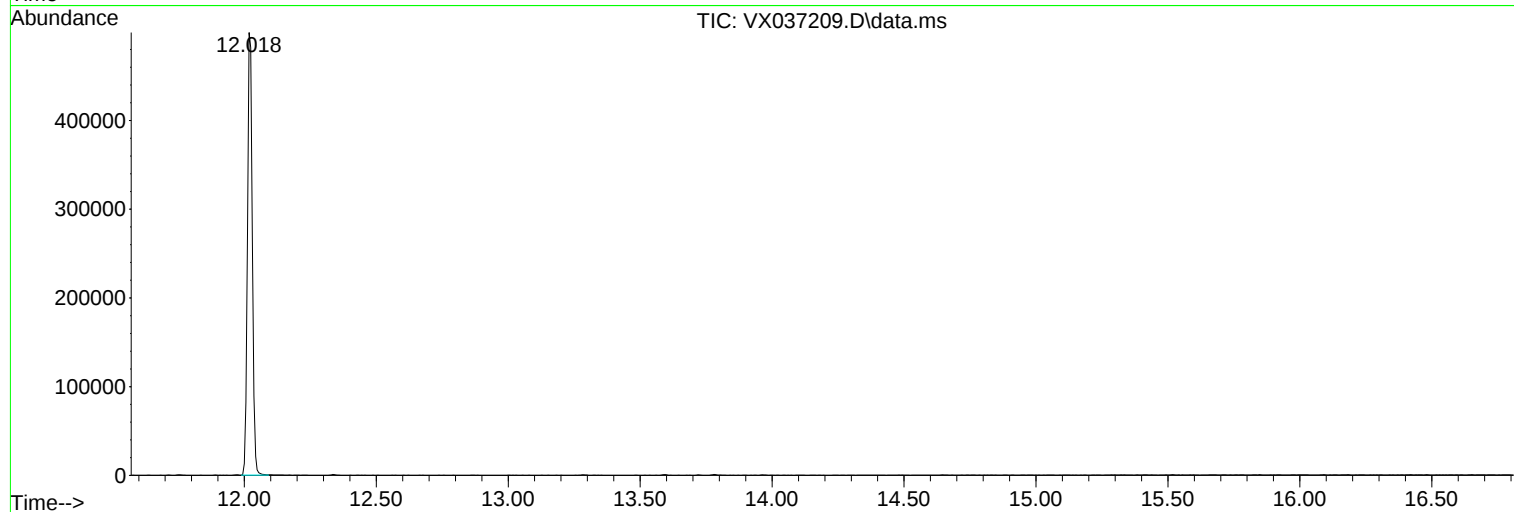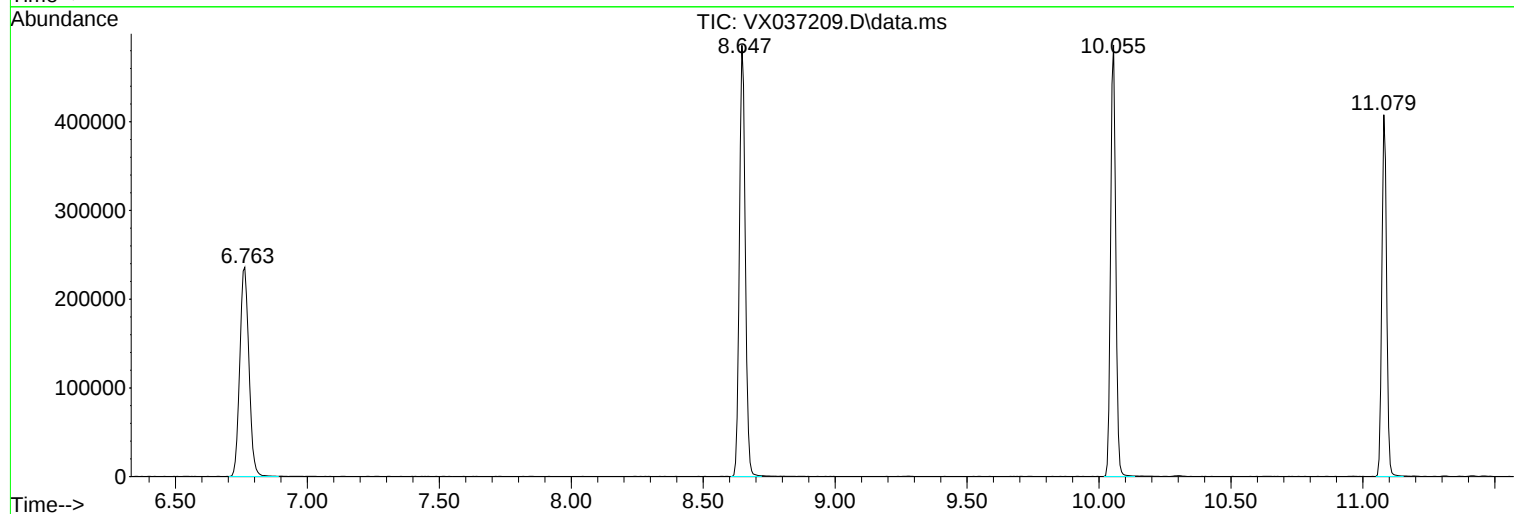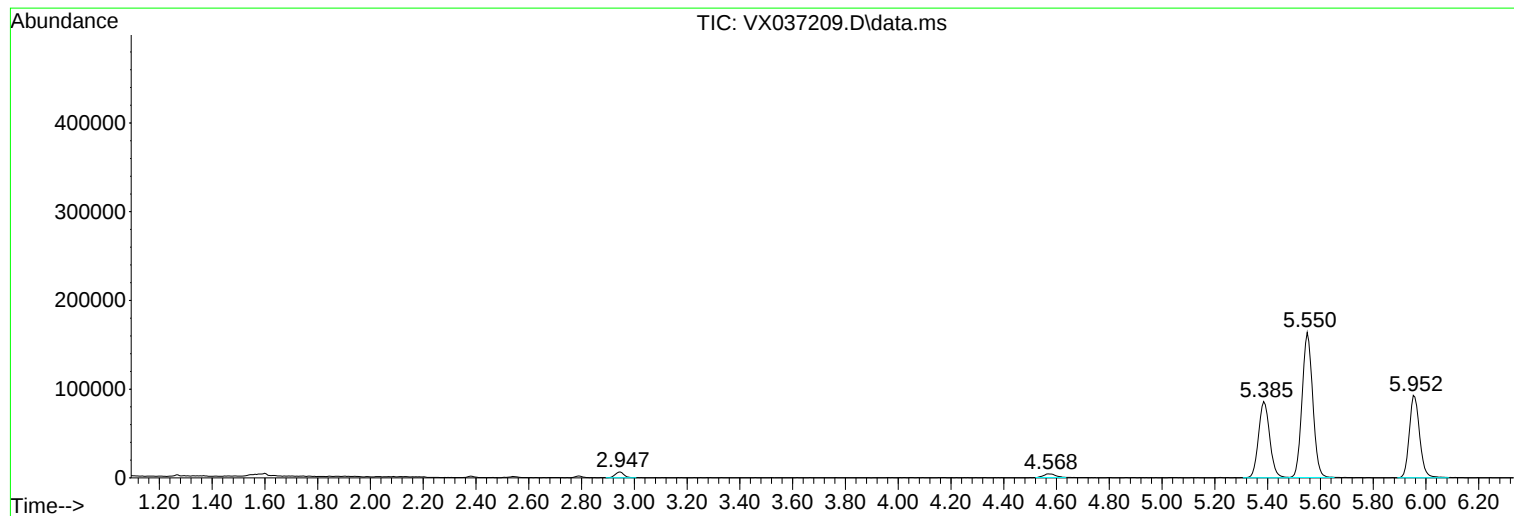

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082423\  
Data File : VX037209.D  
Acq On : 24 Aug 2023 12:17  
Operator : JC/MD  
Sample : 04093-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-20230818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082423\  
Data File : VX037209.D  
Acq On : 24 Aug 2023 12:17  
Operator : JC/MD  
Sample : 04093-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-20230818

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|