

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037244.D
Acq On : 25 Aug 2023 03:35
Operator : JC/MD
Sample : 04110-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RINSATE-BLANK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	31	35	41	rVB	11427	17648	2.40%	0.434%
2	2.380	205	212	219	rBV	4602	7971	1.08%	0.196%
3	3.440	377	386	399	rVB2	39492	88538	12.03%	2.175%
4	5.385	694	705	721	rBV	84057	246047	33.42%	6.045%
5	5.550	721	732	758	rVB2	154977	448590	60.94%	11.021%
6	5.952	789	798	818	rBV	91913	245978	33.41%	6.043%
7	6.763	920	931	949	rBV	227909	553049	75.12%	13.588%
8	8.647	1231	1240	1251	rBV	472599	736175	100.00%	18.087%
9	10.055	1465	1471	1488	rBV	470015	641481	87.14%	15.760%
10	11.079	1634	1639	1654	rBV	400874	488639	66.38%	12.005%
11	12.018	1788	1793	1804	rBV	472736	596103	80.97%	14.645%




Sum of corrected areas: 4070219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037244.D
Acq On : 25 Aug 2023 03:35
Operator : JC/MD
Sample : 04110-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RINSATE-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

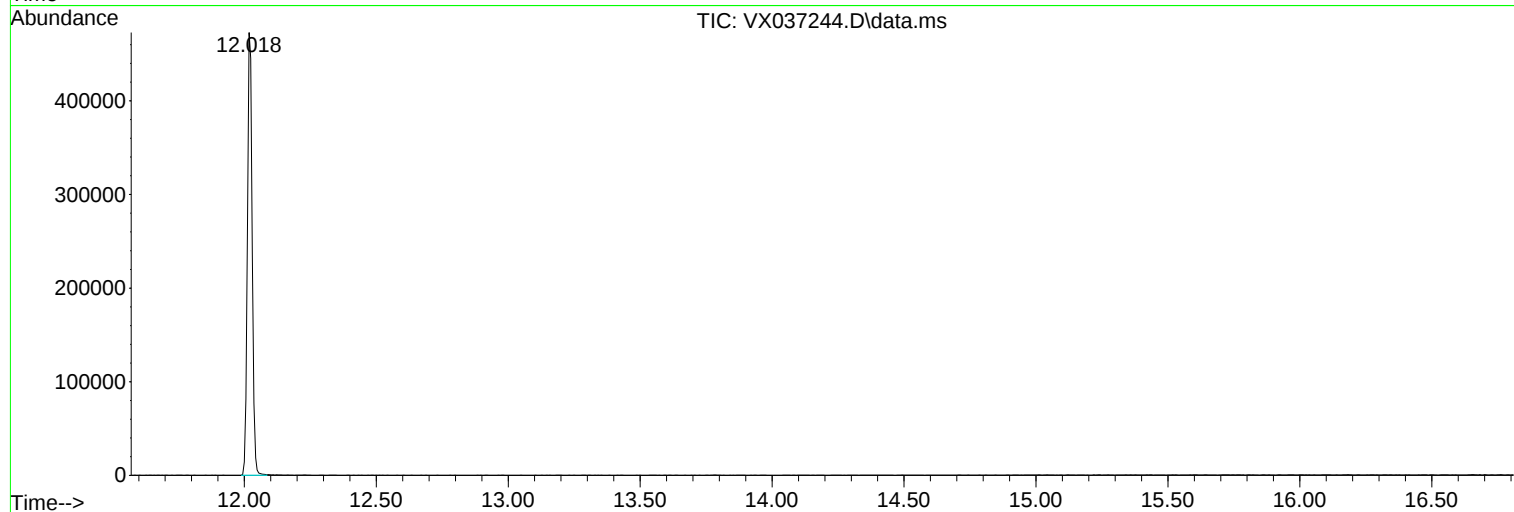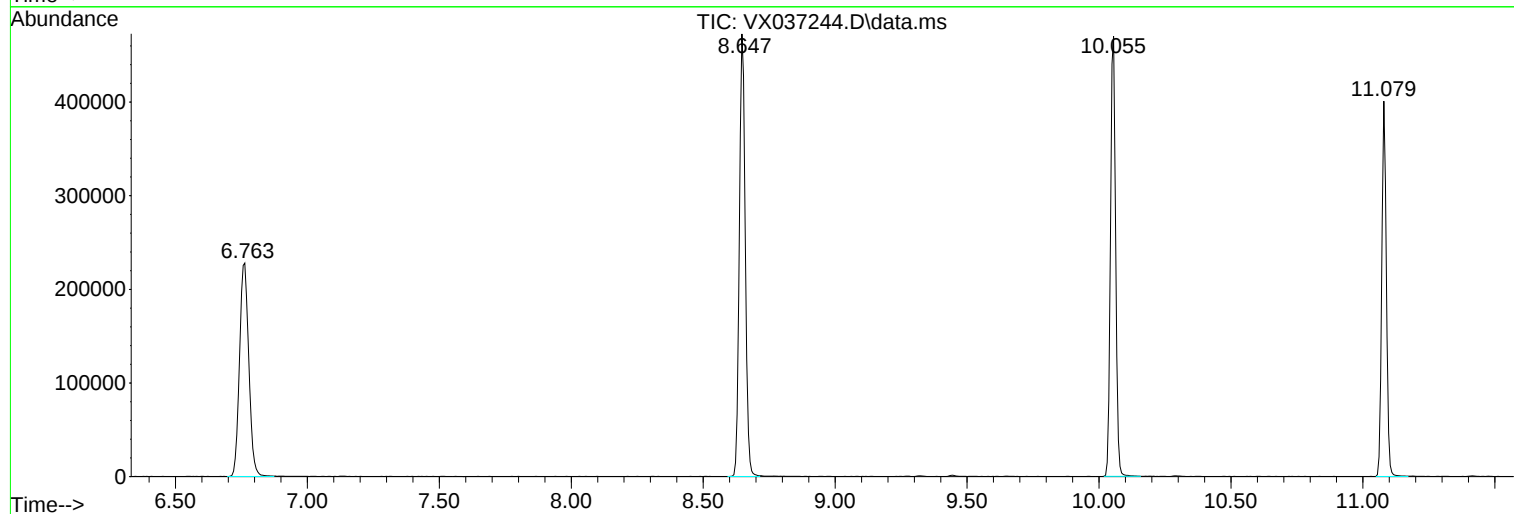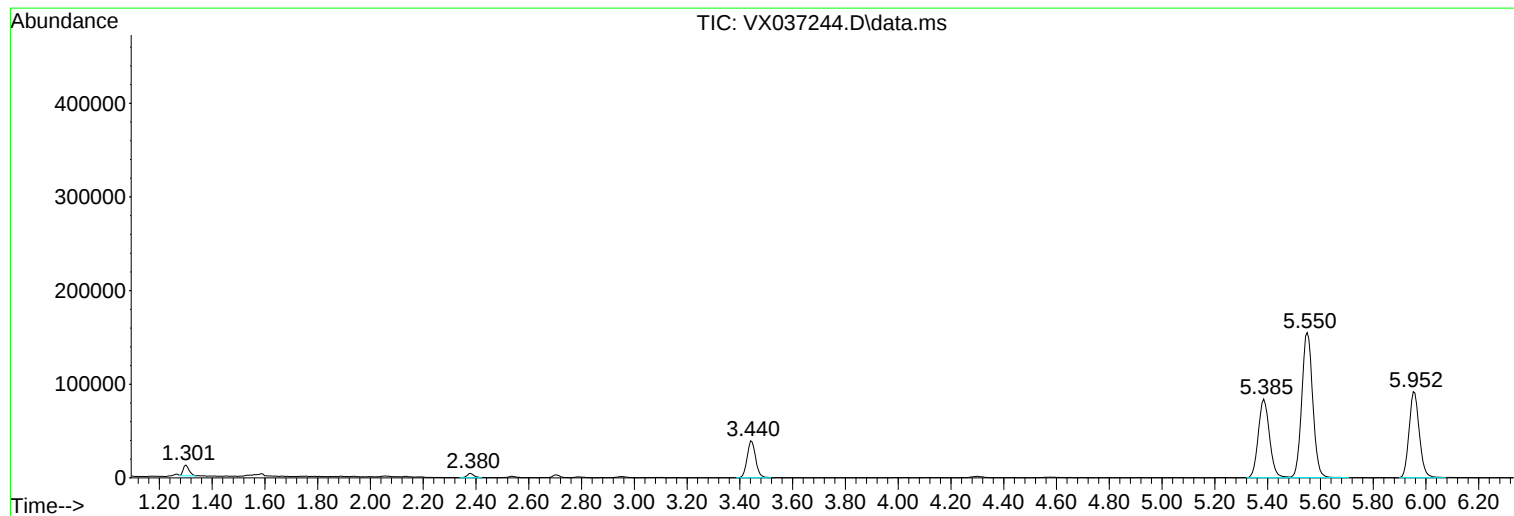

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037244.D
Acq On : 25 Aug 2023 03:35
Operator : JC/MD
Sample : 04110-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RINSATE-BLANK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Ethyl-oxetane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.440	9.87 ug/l	88538	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Ethyl-oxetane	86	C5H10O	1010386-40-2	86
2			n-Hexane	86	C6H14	000110-54-3	80
3			Pentane, 3-methyl-	86	C6H14	000096-14-0	40
4			Furan, tetrahydro-3-methyl-	86	C5H10O	013423-15-9	38
5			1-Pentene, 4-methyl-	84	C6H12	000691-37-2	37

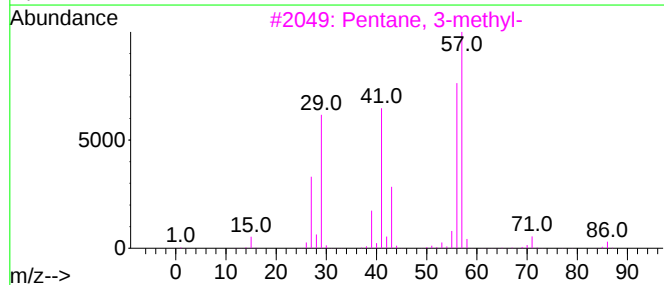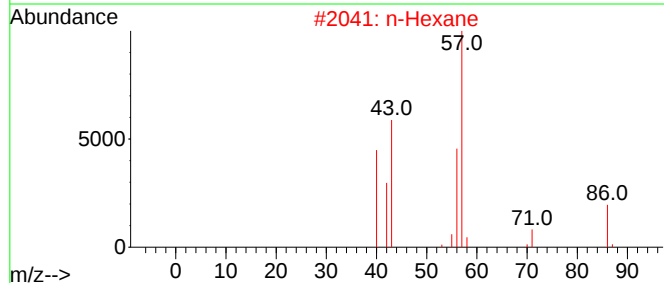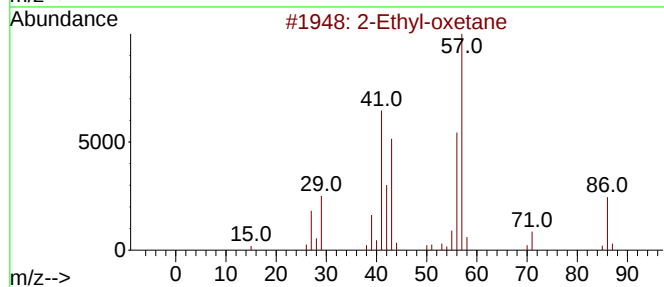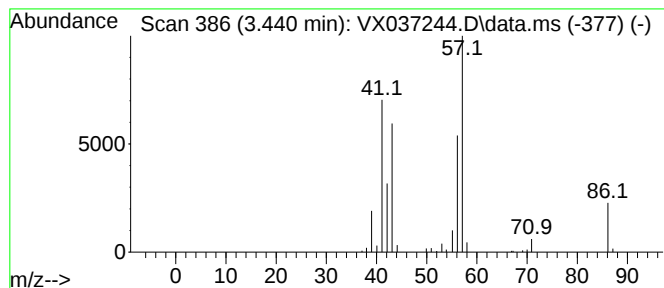

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037244.D
Acq On : 25 Aug 2023 03:35
Operator : JC/MD
Sample : 04110-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RINSATE-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Ethyl-oxetane	3.440	9.9	ug/l	88538	1	5.550	448590	50.0