

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
 Data File : VX037247.D
 Acq On : 25 Aug 2023 04:47
 Operator : JC/MD
 Sample : 04096-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-RW11-MW011-GW-20230817

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M

Title : SW846 8260

Signal : TIC: VX037247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.532	231	237	246	rBV	7389	15092	1.92%	0.352%
2	2.941	297	304	315	rVB	6661	15214	1.94%	0.355%
3	4.568	558	571	582	rBV	6146	21015	2.68%	0.490%
4	5.385	694	705	719	rBV	90531	261062	33.23%	6.089%
5	5.550	721	732	750	rVB	170629	477310	60.76%	11.133%
6	5.952	788	798	813	rBV	97590	261614	33.30%	6.102%
7	6.757	920	930	948	rBV	246008	588683	74.94%	13.731%
8	8.647	1234	1240	1261	rBV	503698	785557	100.00%	18.323%
9	10.055	1465	1471	1488	rBV	500072	688152	87.60%	16.051%
10	11.079	1634	1639	1650	rBV	422408	526441	67.01%	12.279%
11	12.018	1788	1793	1804	rBV	500008	647183	82.39%	15.095%




Sum of corrected areas: 4287323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037247.D
Acq On : 25 Aug 2023 04:47
Operator : JC/MD
Sample : 04096-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW11-MW01I-GW-20230817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

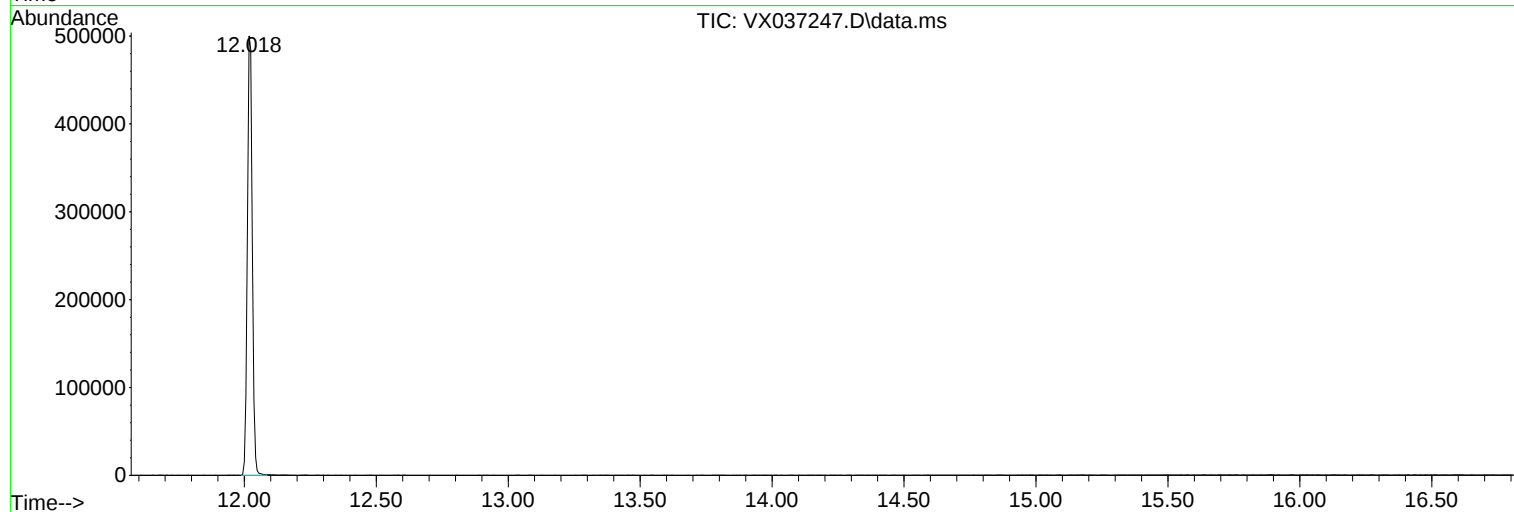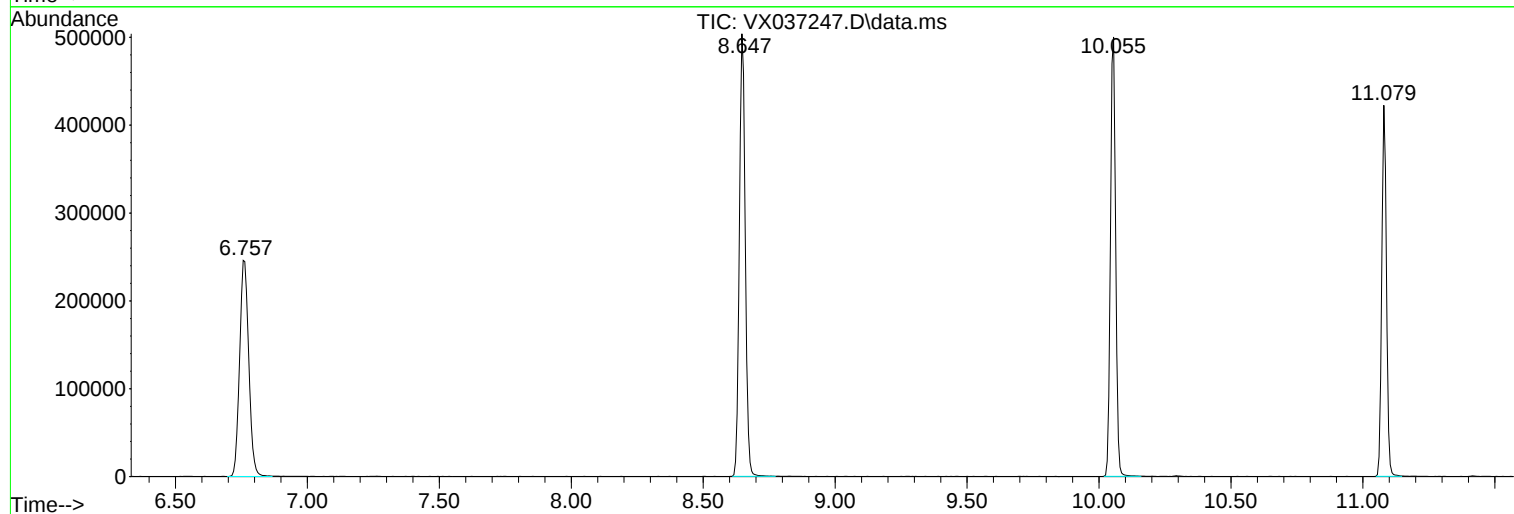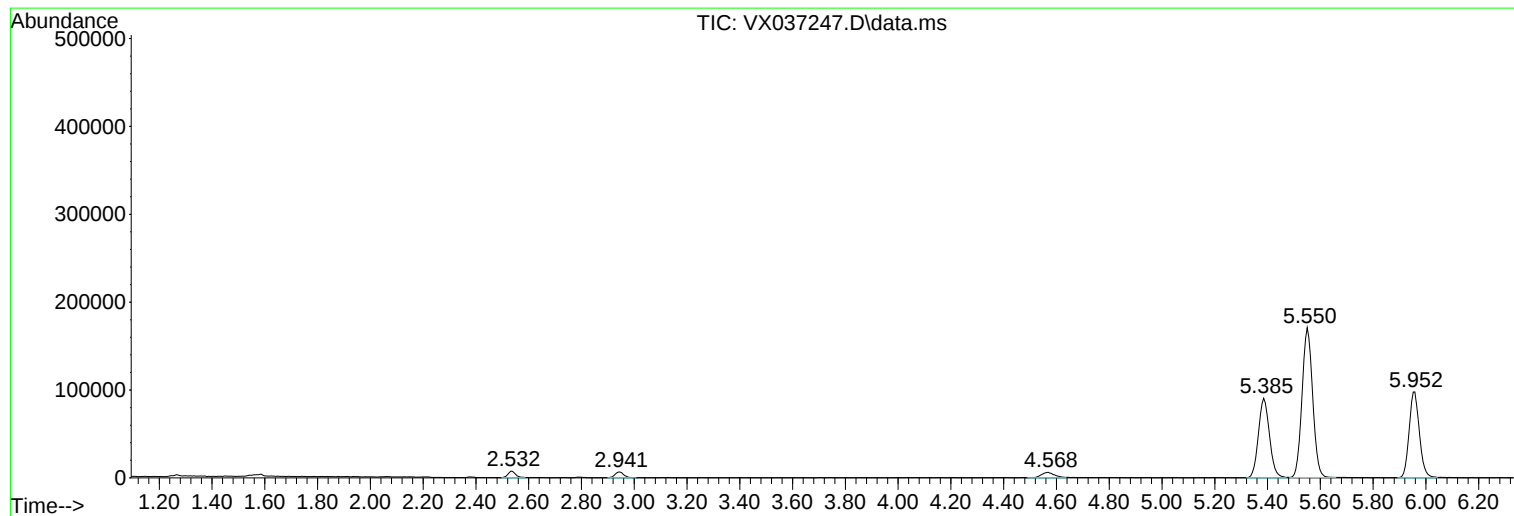

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037247.D
Acq On : 25 Aug 2023 04:47
Operator : JC/MD
Sample : 04096-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW11-MW01I-GW-20230817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037247.D
Acq On : 25 Aug 2023 04:47
Operator : JC/MD
Sample : 04096-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW11-MW01I-GW-20230817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------