

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
 Data File : VX037253.D
 Acq On : 25 Aug 2023 07:12
 Operator : JC/MD
 Sample : 04077-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D2-20230817

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260

Signal : TIC: VX037253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	196	204	219	rVB	91180	178385	4.19%	2.028%
2	5.385	690	705	721	rBV	91570	264613	6.21%	3.008%
3	5.550	721	732	746	rBV	171229	481221	11.29%	5.471%
4	5.952	788	798	816	rBV	98486	264534	6.21%	3.007%
5	6.763	921	931	943	rBV	248614	597460	14.02%	6.792%
6	7.122	980	990	1006	rBV	1965547	4262397	100.00%	48.456%
7	8.646	1233	1240	1248	rBV	516546	793287	18.61%	9.018%
8	9.274	1337	1343	1351	rBV	43332	65964	1.55%	0.750%
9	10.055	1465	1471	1483	rBV	518505	692772	16.25%	7.876%
10	11.079	1634	1639	1654	rBV	434834	534793	12.55%	6.080%
11	12.018	1788	1793	1806	rBV	521763	660921	15.51%	7.514%




Sum of corrected areas: 8796347

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037253.D
Acq On : 25 Aug 2023 07:12
Operator : JC/MD
Sample : 04077-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20230817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

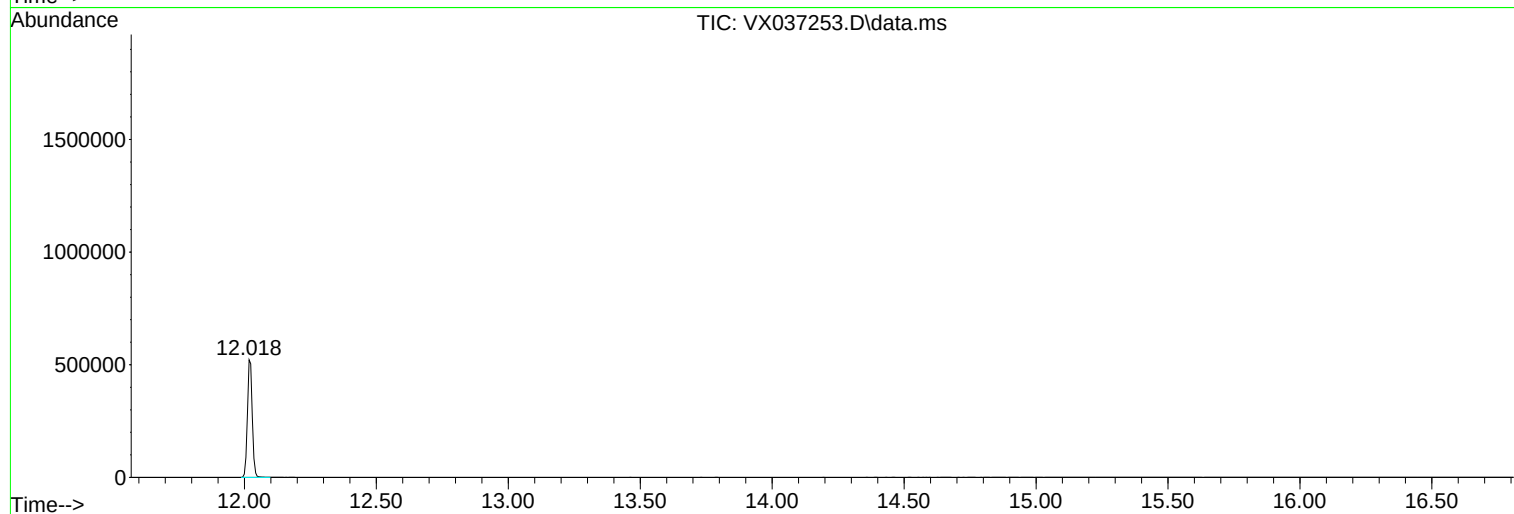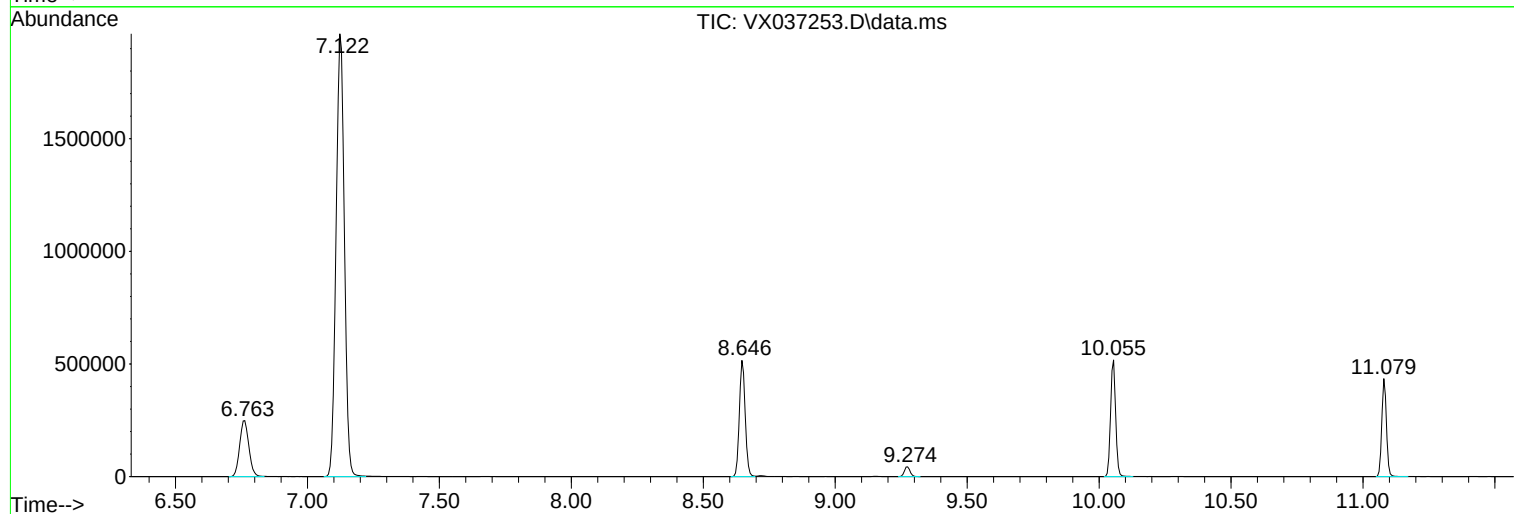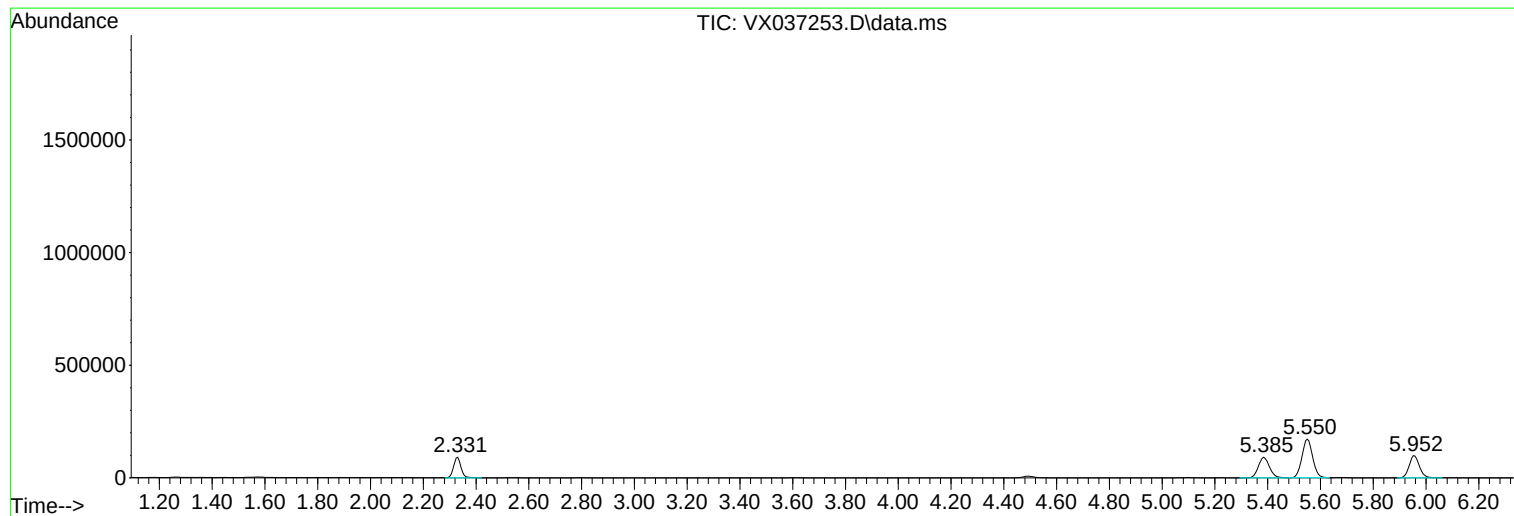

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037253.D
Acq On : 25 Aug 2023 07:12
Operator : JC/MD
Sample : 04077-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20230817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037253.D
Acq On : 25 Aug 2023 07:12
Operator : JC/MD
Sample : 04077-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 57 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20230817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------