


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082423\
Data File : VX037200.D
Acq On : 24 Aug 2023 08:24
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
Title : SW846 8260
Last Update : Fri Aug 18 09:30:38 2023

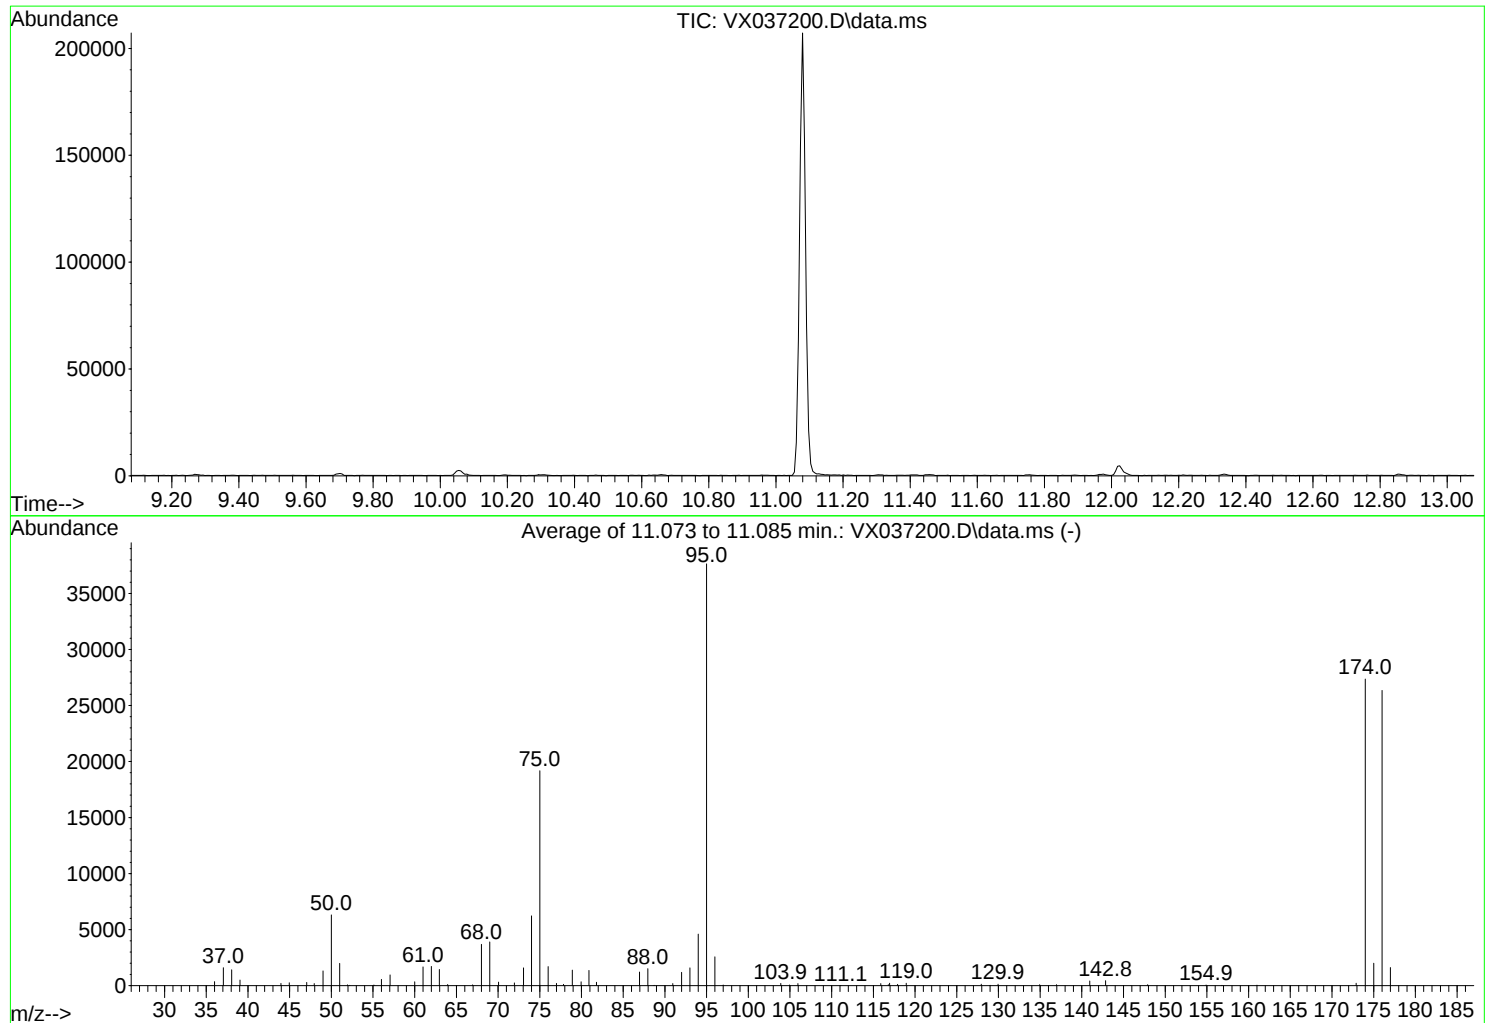

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6317	PASS
75	95	30	60	50.9	19172	PASS
95	95	100	100	100.0	37643	PASS
96	95	5	9	6.8	2573	PASS
173	174	0.00	2	0.8	215	PASS
174	95	50	100	72.7	27360	PASS
175	174	5	9	7.3	2005	PASS
176	174	95	101	96.3	26347	PASS
177	176	5	9	6.1	1620	PASS