

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
 Data File : VX023937.D
 Acq On : 25 Aug 2021 14:43
 Operator : JC/MD
 Sample : M3525-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WVLY-SW-02-GW-081921

Quant Time: Aug 26 07:36:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	134980	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	227702	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	214242	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	91199	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	95580	50.735	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 101.480%	
35) Dibromofluoromethane	5.397	113	75846	50.326	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.660%	
50) Toluene-d8	8.653	98	275397	48.011	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 96.020%	
62) 4-Bromofluorobenzene	11.085	95	95668	45.306	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 90.620%	
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.173	85	519	0.364	ug/l	95
5) Bromomethane	1.618	94	340	0.355	ug/l	100
6) Chloroethane	1.654	64	19	2.232	ug/l #	43
7) Trichlorofluoromethane	1.892	101	207421	86.145	ug/l	97
8) Diethyl Ether	1.892	74	232	0.276	ug/l #	37
9) 1,1,2-Trichlorotrifluo...	2.331	101	1155	0.852	ug/l	90
10) Methyl Iodide	2.471	142	523	0.277	ug/l #	80
12) 1,1-Dichloroethene	2.319	96	4139	3.195	ug/l	95
13) Acrolein	2.239	56	50	0.221	ug/l #	82
16) Acetone	2.386	43	3052	3.623	ug/l	98
20) Methylene Chloride	2.794	84	514	0.319	ug/l #	81
27) cis-1,2-Dichloroethene	4.495	96	1716	1.042	ug/l	89
28) Bromochloromethane	5.105	49	7830	6.508	ug/l #	9
29) Tetrahydrofuran	5.044	42	200	0.242	ug/l #	34
30) Chloroform	5.111	83	91874	32.790	ug/l	98
31) Cyclohexane	5.556	56	3240	1.339	ug/l #	26
32) 1,1,1-Trichloroethane	5.391	97	711	0.296	ug/l #	41
36) 1,1-Dichloropropene	5.562	75	11016	5.224	ug/l #	46
38) Carbon Tetrachloride	5.684	117	677	0.308	ug/l #	84
39) Methylcyclohexane	7.129	83	820	0.319	ug/l #	1
42) 1,2-Dichloroethane	6.105	62	1068	0.436	ug/l #	73
44) Trichloroethene	7.135	130	71198	41.335	ug/l	100
47) Bromodichloromethane	7.830	83	1163	0.558	ug/l #	78
51) 4-Methyl-2-Pentanone	8.659	43	1418	0.541	ug/l #	1
60) Dibromochloromethane	9.275	129	3796	3.684	ug/l #	11
64) Tetrachloroethene	9.281	164	3741	2.186	ug/l	90
76) 1,2,3-Trichloropropane	11.085	75	53451	25.125	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	53451	73.905	ug/l #	12
95) Naphthalene	13.786	128	48	1.289	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
Data File : VX023937.D
Acq On : 25 Aug 2021 14:43
Operator : JC/MD
Sample : M3525-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921

Quant Time: Aug 26 07:36:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration




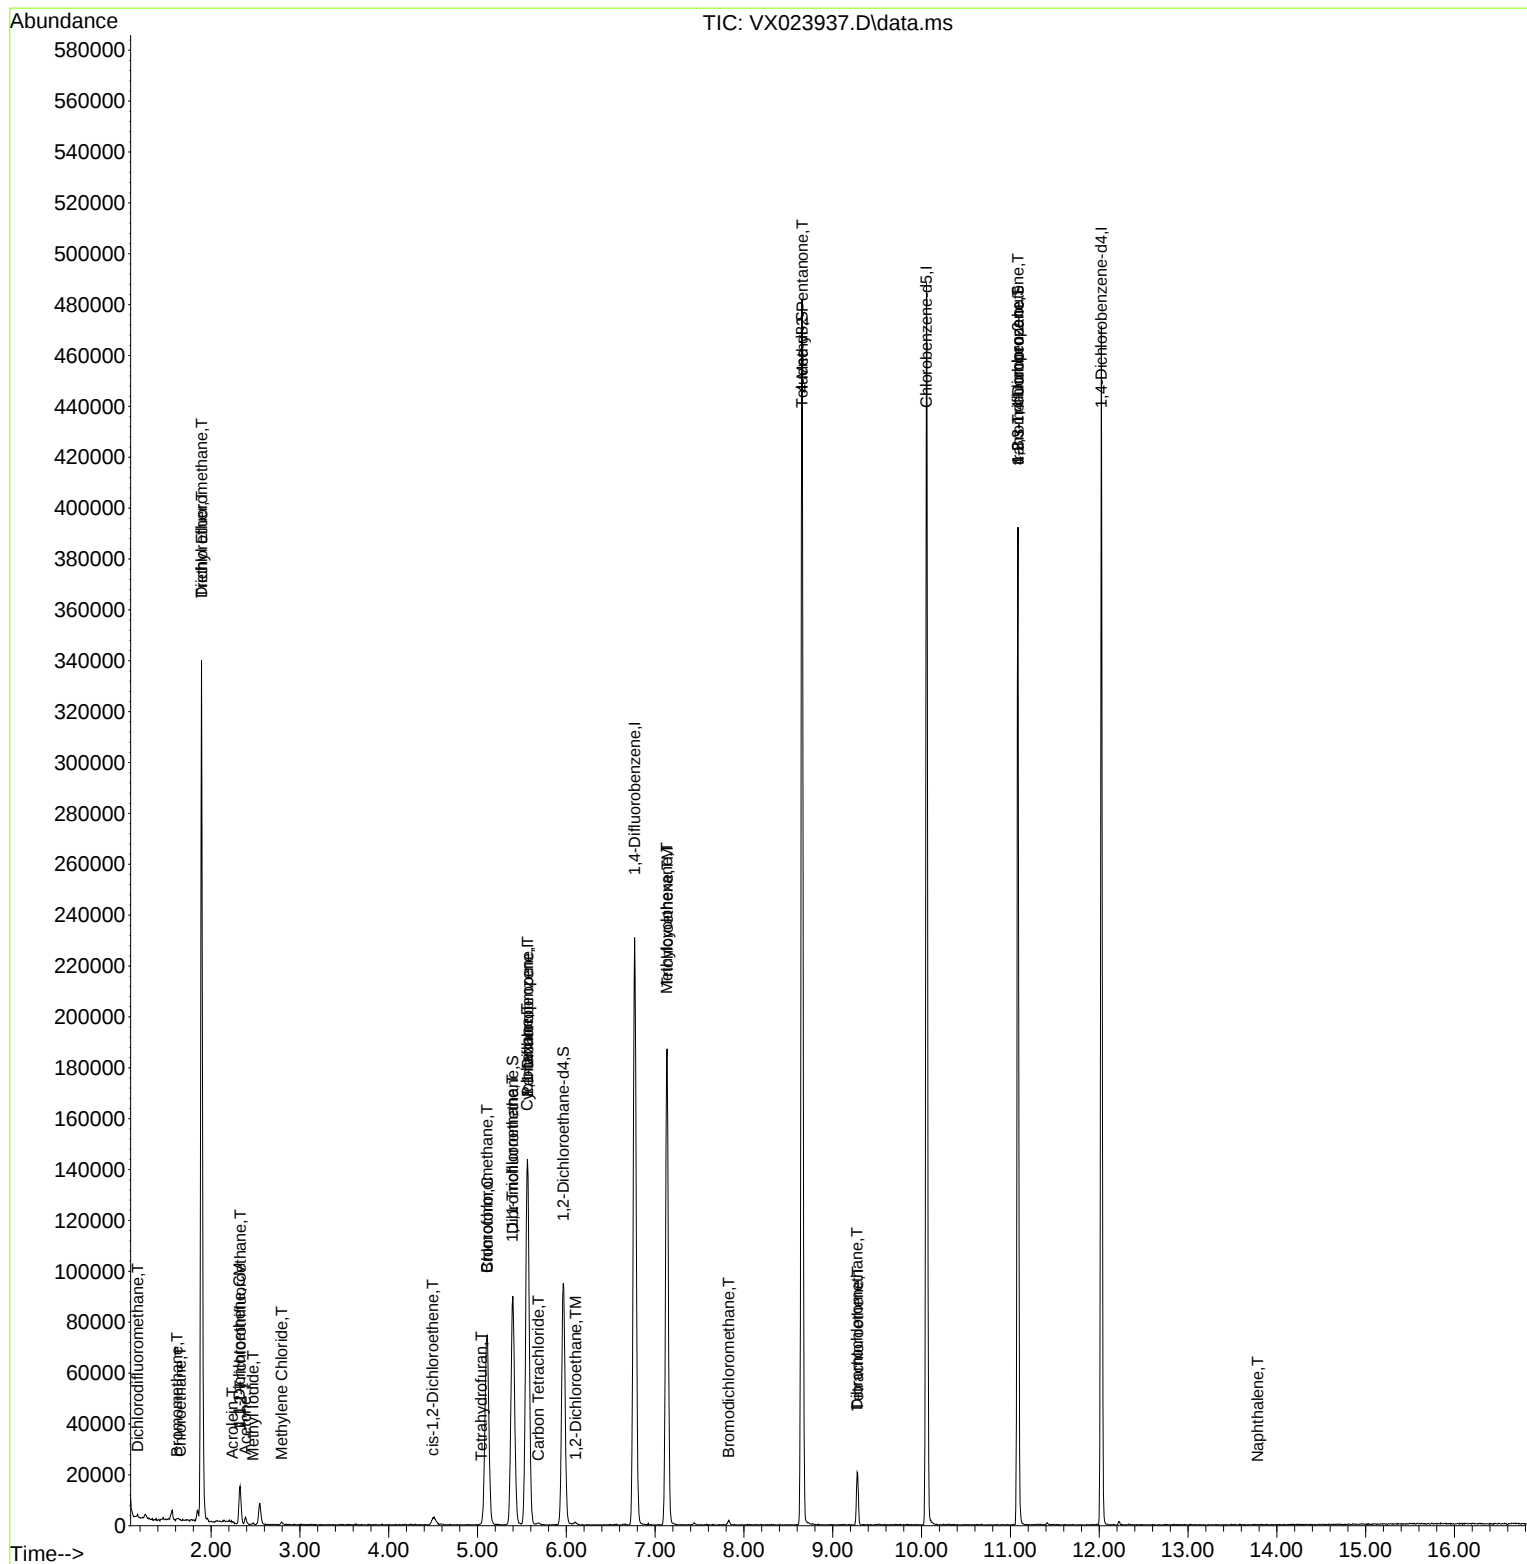




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion:168 Resp: 134980
Ion Ratio Lower Upper
168 100
99 60.1 45.8 68.6

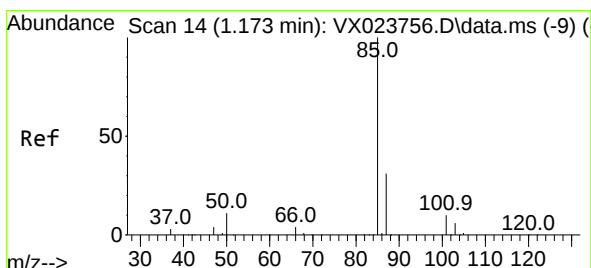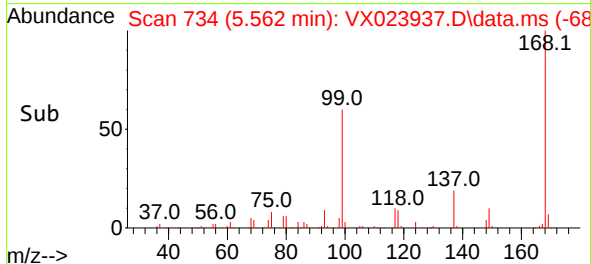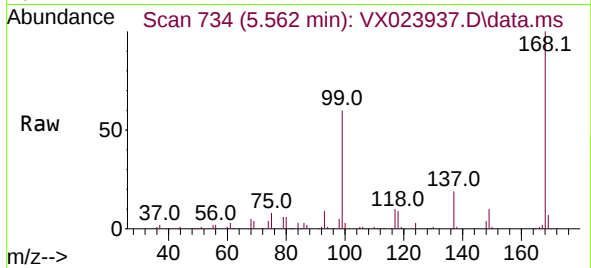

#2
Dichlorodifluoromethane
Concen: 0.364 ug/l
RT: 1.173 min Scan# 14
Delta R.T. -0.000 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Tgt Ion: 85 Resp: 519
Ion Ratio Lower Upper
85 100
87 35.4 16.4 49.2


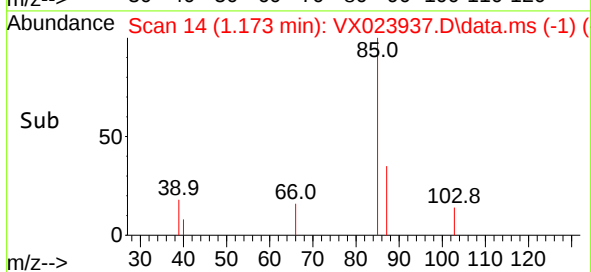




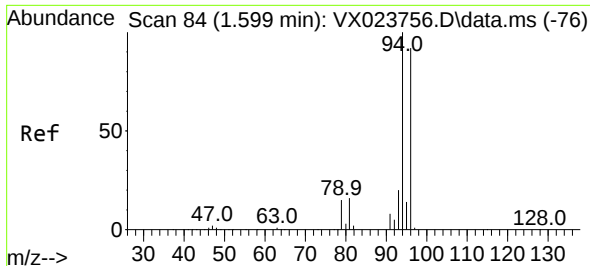

#5
Bromomethane
Concen: 0.355 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.019 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion: 94 Resp: 340
Ion Ratio Lower Upper
94 100
96 95.4 76.4 114.6

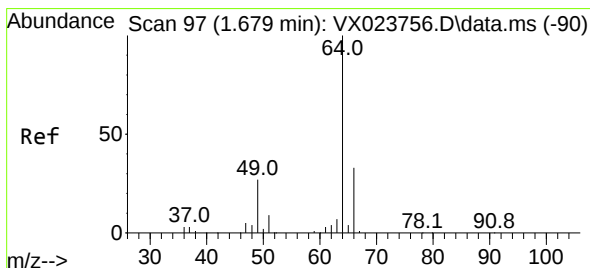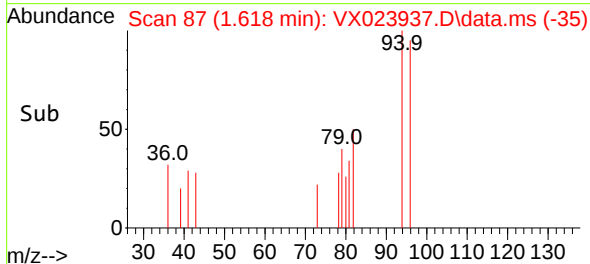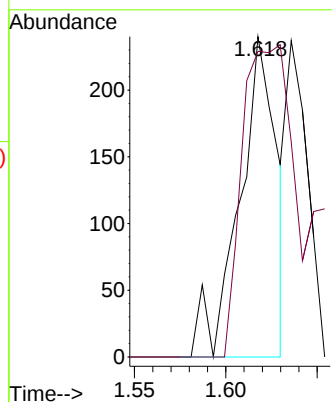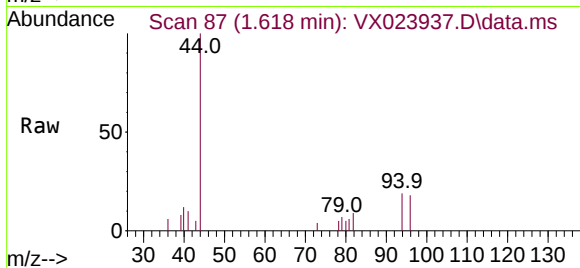

#6
Chloroethane
Concen: 2.232 ug/l
RT: 1.654 min Scan# 93
Delta R.T. -0.025 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Tgt Ion: 64 Resp: 19
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#


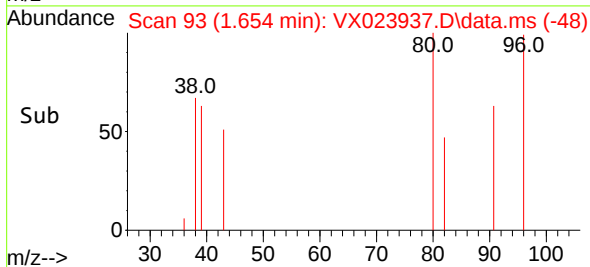
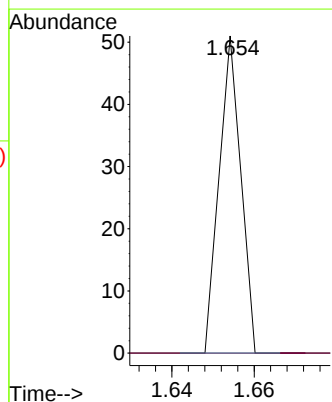
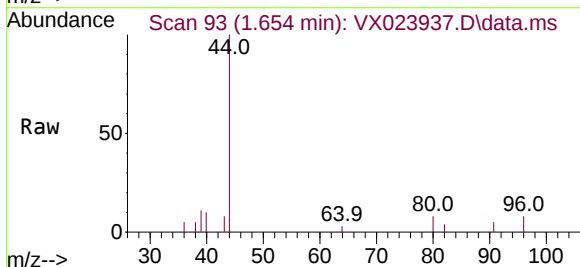




#7
 Trichlorofluoromethane
 Concen: 86.145 ug/l
 RT: 1.892 min Scan# 132
 Delta R.T. 0.006 min
 Lab File: VX023937.D
 Acq: 25 Aug 2021 14:43




Instrument :
 MSVOA_X
 ClientSampleId :
 WVLY-SW-02-GW-081921


Tgt Ion:101 Resp: 207421
 Ion Ratio Lower Upper
 101 100
 103 64.3 53.2 79.8

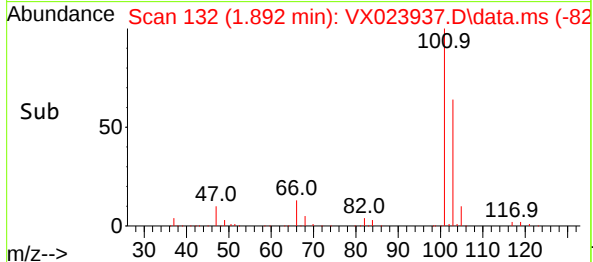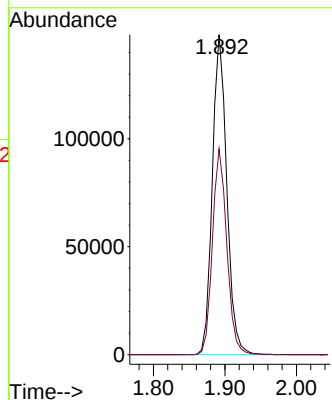

#8
 Diethyl Ether
 Concen: 0.276 ug/l
 RT: 1.892 min Scan# 132
 Delta R.T. -0.250 min
 Lab File: VX023937.D
 Acq: 25 Aug 2021 14:43

Tgt Ion: 74 Resp: 232
 Ion Ratio Lower Upper
 74 100
 45 30.2 44.5 133.5#


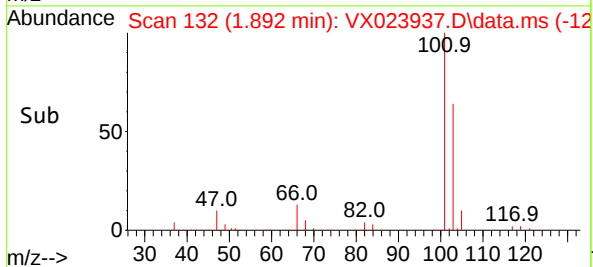
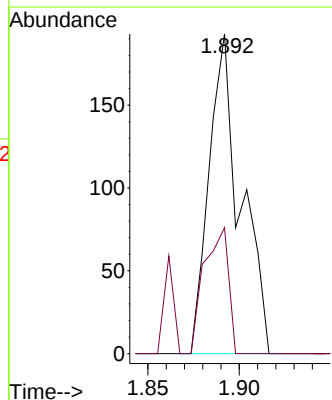
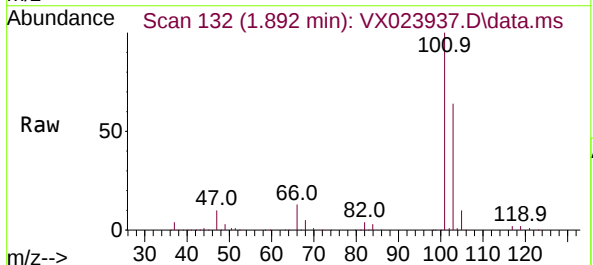




#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.852 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion:101	Resp:	1155
Ion	Ratio	Lower Upper
101	100	
85	37.7	34.9 52.3
151	67.4	61.4 92.2

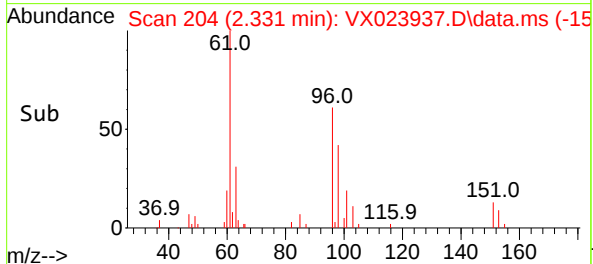

#10
Methyl Iodide
Concen: 0.277 ug/l
RT: 2.471 min Scan# 227
Delta R.T. 0.018 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Tgt Ion:142	Resp:	523
Ion	Ratio	Lower Upper
142	100	
127	31.9	33.3 49.9#
141	0.0	11.4 17.0#

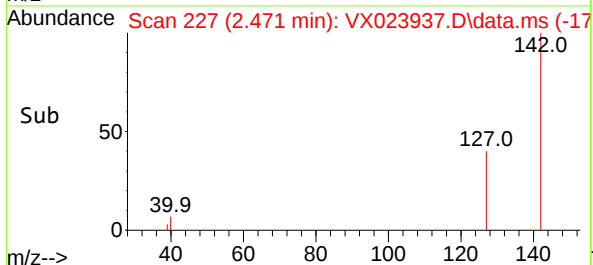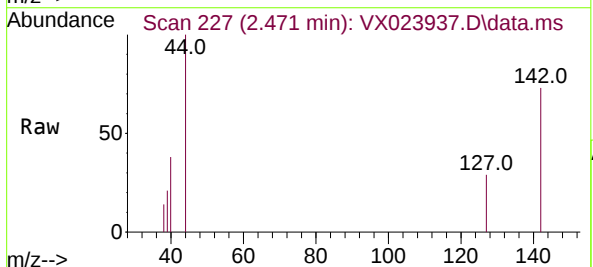



#12

1,1-Dichloroethene

Concen: 3.195 ug/l

RT: 2.319 min Scan# 202

Delta R.T. -0.000 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43





Tgt Ion: 96 Resp: 4139

Ion Ratio Lower Upper

96 100

61 151.4 124.6 187.0

98 57.3 50.6 76.0

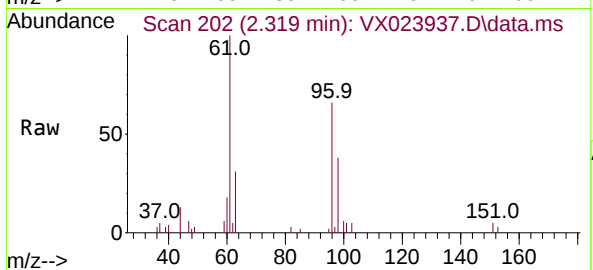

#13

Acrolein

Concen: 0.221 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.006 min

Lab File: VX023937.D




Acq: 25 Aug 2021 14:43


Tgt Ion: 56 Resp: 50

Ion Ratio Lower Upper

56 100

55 56.0 56.4 84.6#


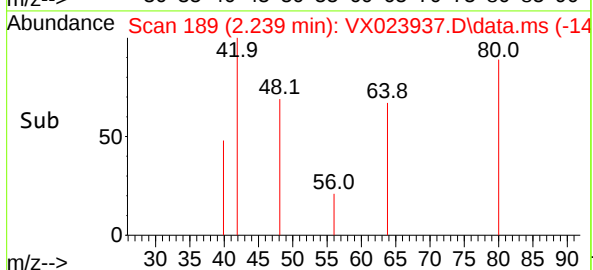

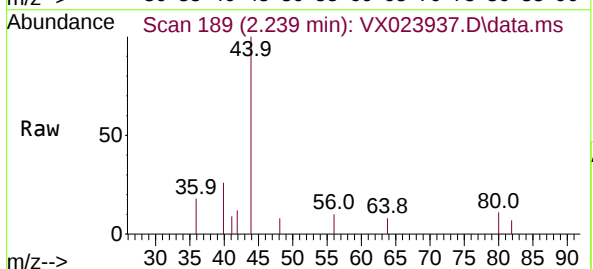




#16
Acetone
Concen: 3.623 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion: 43 Resp: 3052
Ion Ratio Lower Upper
43 100
58 35.8 27.8 41.8

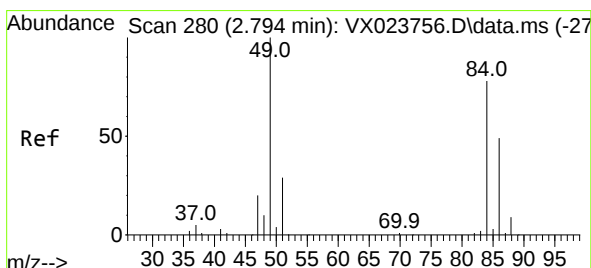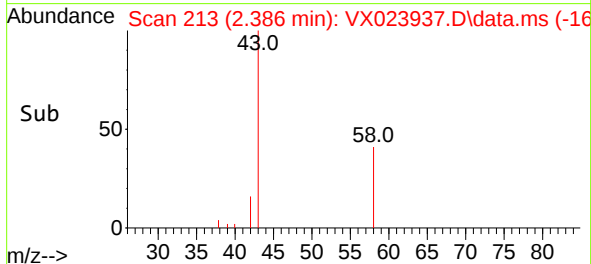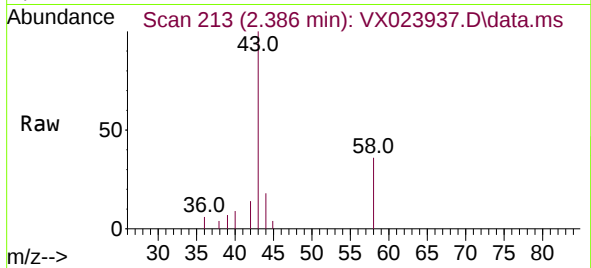

#20
Methylene Chloride
Concen: 0.319 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Tgt Ion: 84 Resp: 514
Ion Ratio Lower Upper
84 100
49 121.5 88.6 132.8
51 27.4 27.0 40.6
86 93.4 50.3 75.5#

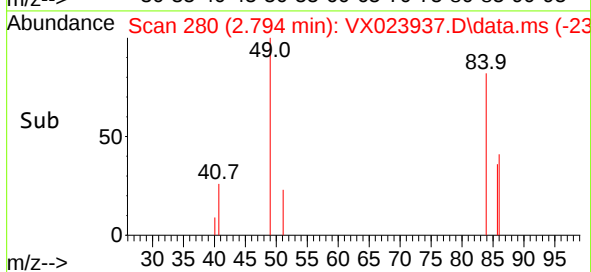



#27

cis-1,2-Dichloroethene

Concen: 1.042 ug/l

RT: 4.495 min Scan# 559





Delta R.T. -0.006 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43

Tgt Ion:	96	Resp:	1716
Ion	Ratio	Lower	Upper
96	100		
61	129.4	0.0	285.6
98	72.9	0.0	129.6

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921



#28

Bromochloromethane

Concen: 6.508 ug/l




RT: 5.105 min Scan# 659


Delta R.T. 0.195 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43

Tgt Ion:	49	Resp:	7830
Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	4.0
130	0.0	68.2	102.2#

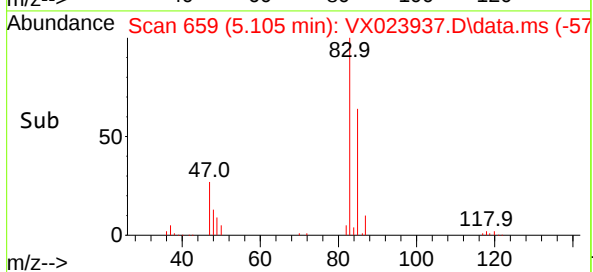



#29

Tetrahydrofuran

Concen: 0.242 ug/l

RT: 5.044 min Scan# 649





Delta R.T. 0.025 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43

Tgt Ion: 42	Resp: 200
Ion Ratio	Lower Upper
42 100	
72 0.0	41.7 62.5#
71 10.0	38.4 57.6#

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921



#30

Chloroform

Concen: 32.790 ug/l




RT: 5.111 min Scan# 660


Delta R.T. 0.006 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43

Tgt Ion: 83	Resp: 91874
Ion Ratio	Lower Upper
83 100	
85 63.7	52.0 78.0


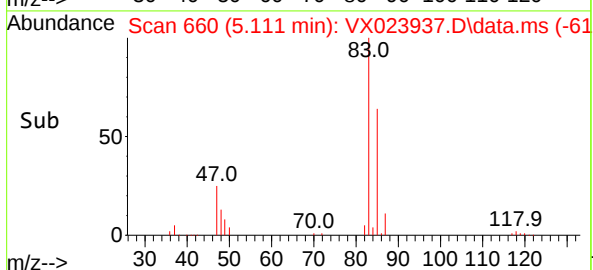






#31
Cyclohexane
Concen: 1.339 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.079 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion: 56 Resp: 3240
Ion Ratio Lower Upper
56 100
69 152.5 25.3 37.9#
84 110.2 71.4 107.0#

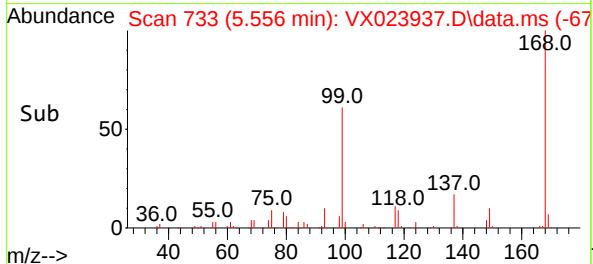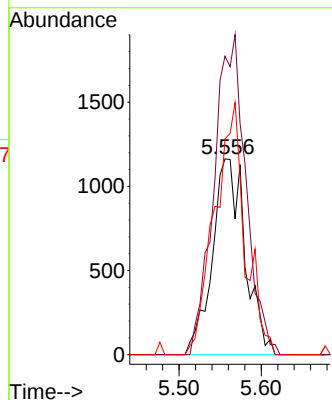

#32
1,1,1-Trichloroethane
Concen: 0.296 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Tgt Ion: 97 Resp: 711
Ion Ratio Lower Upper
97 100
99 0.0 51.5 77.3#
61 57.7 34.2 51.4#

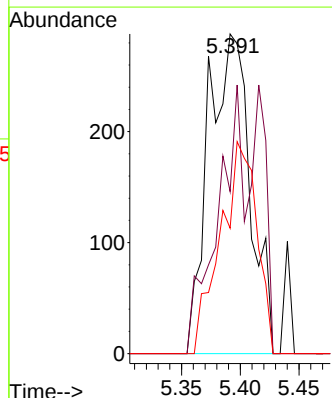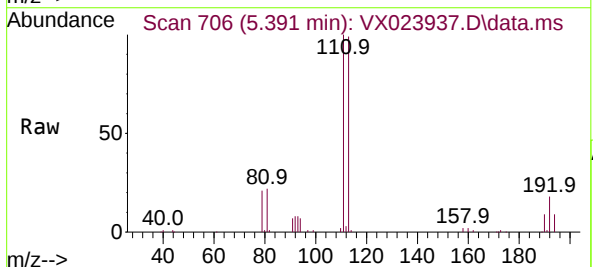



#33

1,2-Dichloroethane-d4

Concen: 50.735 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX023937.D





Acq: 25 Aug 2021 14:43

Tgt Ion: 65 Resp: 95580

Ion Ratio Lower Upper

65 100

67 51.0 0.0 105.4

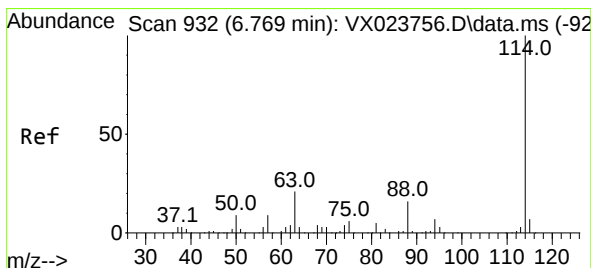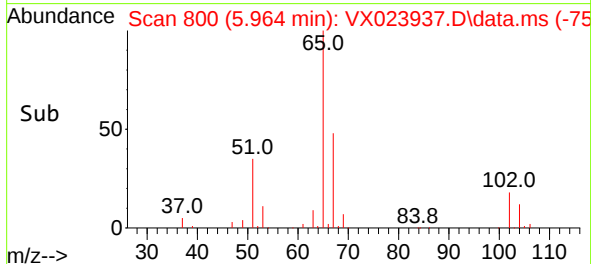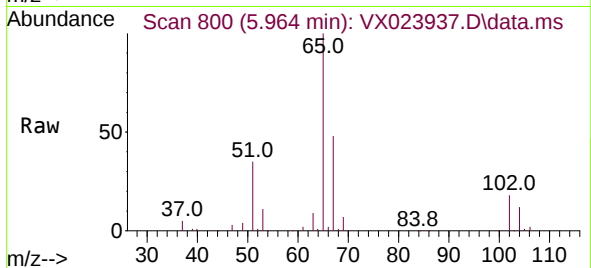

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43




Tgt Ion: 114 Resp: 227702


Ion Ratio Lower Upper

114 100

63 21.8 0.0 40.8

88 15.6 0.0 32.8

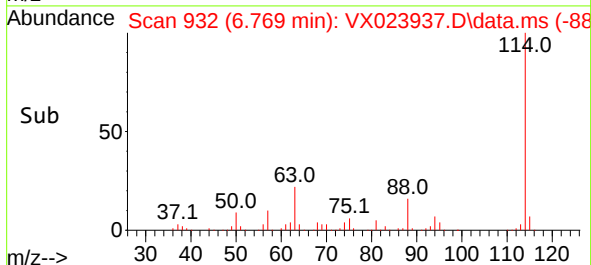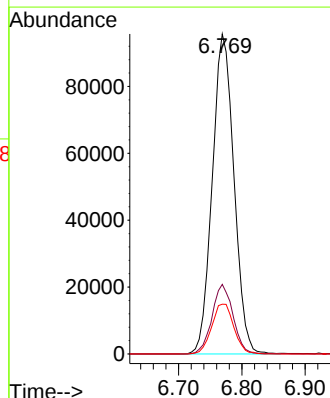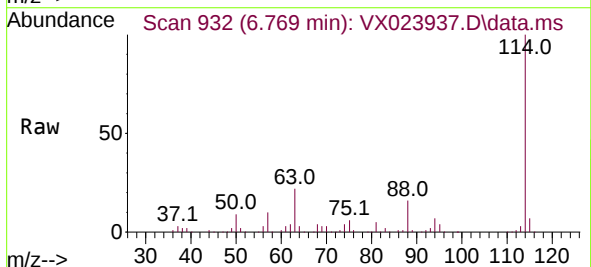



#35

Dibromofluoromethane

Concen: 50.326 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.000 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43





Tgt Ion:113 Resp: 75846

Ion Ratio Lower Upper

113 100

111 103.2 81.9 122.9

192 19.7 16.7 25.1

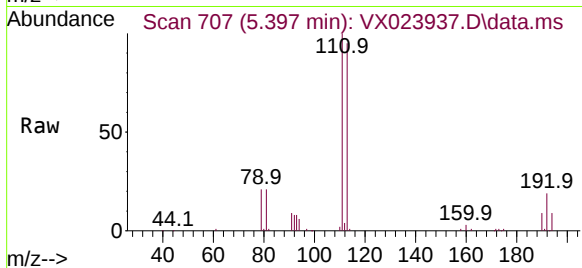

#36

1,1-Dichloropropene

Concen: 5.224 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.140 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43




Tgt Ion: 75 Resp: 11016


Ion Ratio Lower Upper

75 100

110 5.5 18.1 54.4#

77 0.0 25.3 37.9#


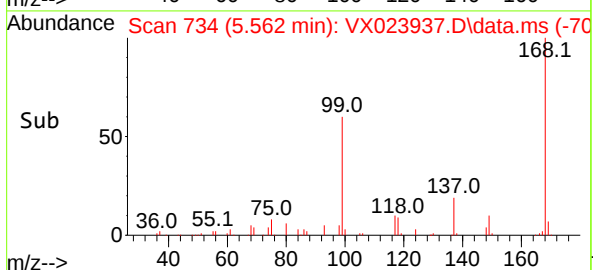

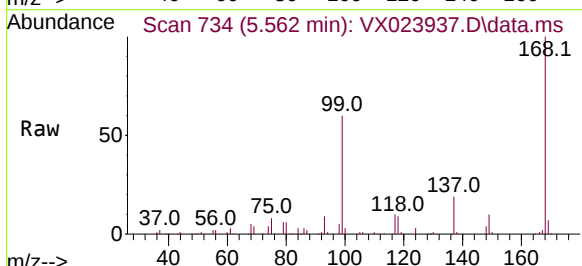




#38
Carbon Tetrachloride
Concen: 0.308 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.006 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion:117 Resp: 677
Ion Ratio Lower Upper
117 100
119 88.0 76.2 114.2
121 55.0 24.8 37.2#



#39
Methylcyclohexane
Concen: 0.319 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.256 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Tgt Ion: 83 Resp: 820
Ion Ratio Lower Upper
83 100
55 0.0 58.9 88.3#
98 171.0 38.1 57.1#

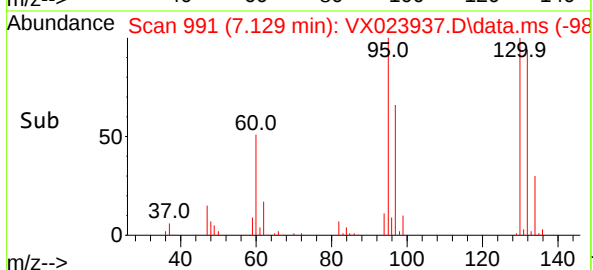



#42

1,2-Dichloroethane

Concen: 0.436 ug/l

RT: 6.105 min Scan# 823

Delta R.T. 0.007 min

Lab File: VX023937.D





Acq: 25 Aug 2021 14:43

Tgt Ion: 62 Resp: 1068

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2

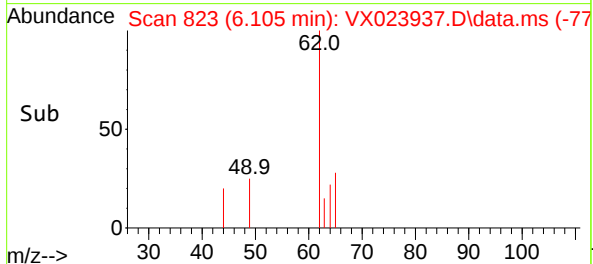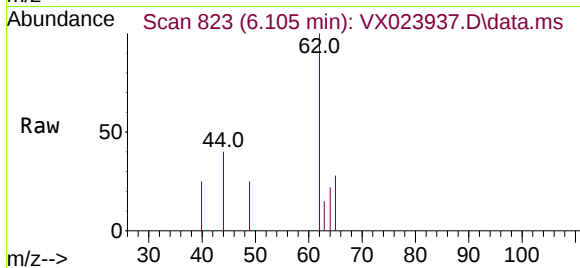

#44

Trichloroethene

Concen: 41.335 ug/l

RT: 7.135 min Scan# 992

Delta R.T. 0.006 min

Lab File: VX023937.D




Acq: 25 Aug 2021 14:43


Tgt Ion: 130 Resp: 71198

Ion Ratio Lower Upper

130 100

95 99.1 0.0 198.0

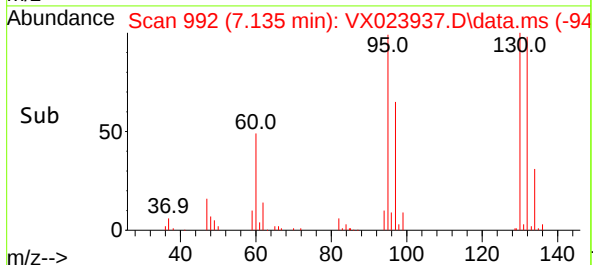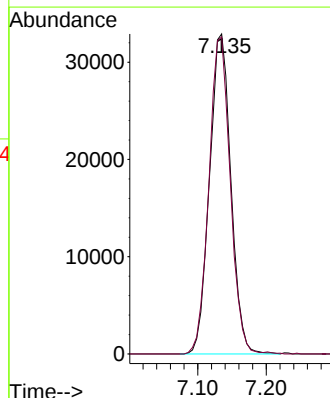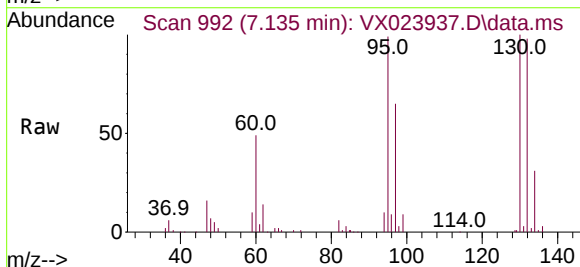



#47

Bromodichloromethane

Concen: 0.558 ug/l

RT: 7.830 min Scan# 1106

Delta R.T. -0.000 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43





Instrument :

MSVOA_X

ClientSampleId :

WVLY-SW-02-GW-081921

Tgt Ion:	83	Resp:	1163
Ion	Ratio	Lower	Upper
83	100		
85	81.4	51.4	77.0#
127	14.8	6.8	10.2#

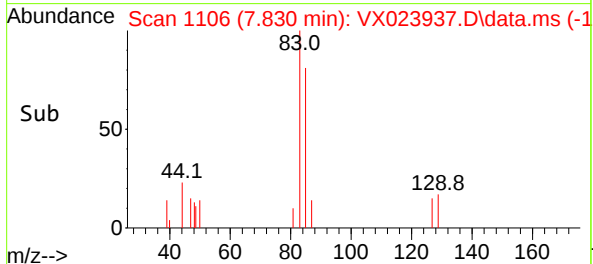

#50

Toluene-d8

Concen: 48.011 ug/l




RT: 8.653 min Scan# 1241


Delta R.T. -0.000 min

Lab File: VX023937.D

Acq: 25 Aug 2021 14:43

Tgt Ion:	98	Resp:	275397
Ion	Ratio	Lower	Upper
98	100		
100	64.0	51.9	77.9


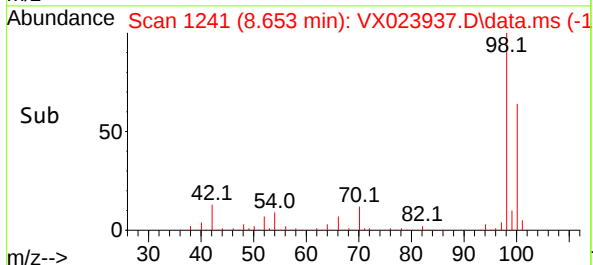

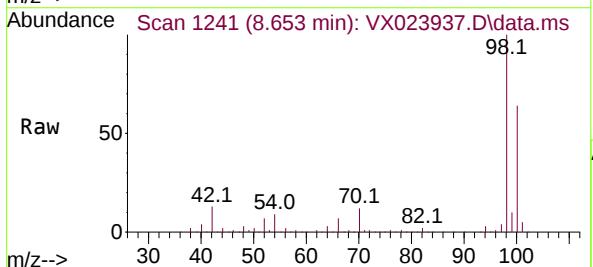




#51
4-Methyl-2-Pentanone
Concen: 0.541 ug/l
RT: 8.659 min Scan# 1242
Delta R.T. 0.079 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion: 43 Resp: 1418
Ion Ratio Lower Upper
43 100
58 179.3 35.4 53.0#

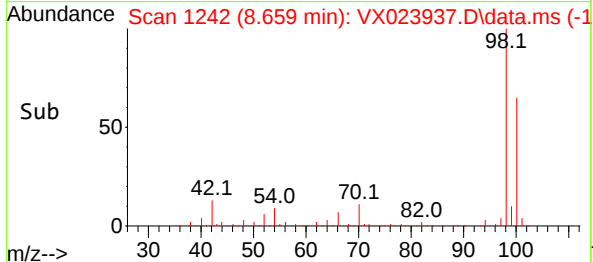

#60
Dibromochloromethane
Concen: 3.684 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Tgt Ion: 129 Resp: 3796
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#


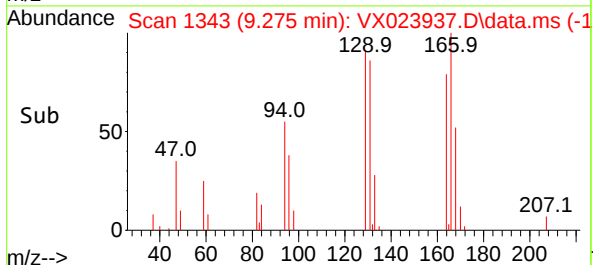
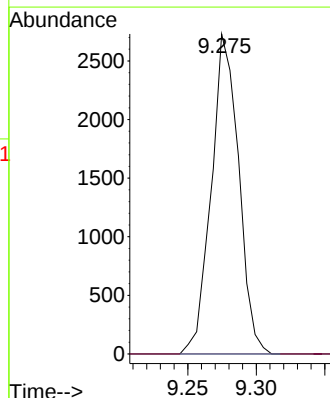
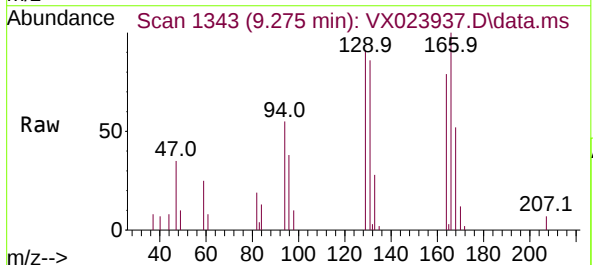




#62
4-Bromofluorobenzene
Concen: 45.306 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion: 95 Resp: 95668
Ion Ratio Lower Upper
95 100
174 80.6 0.0 154.6
176 76.8 0.0 155.8

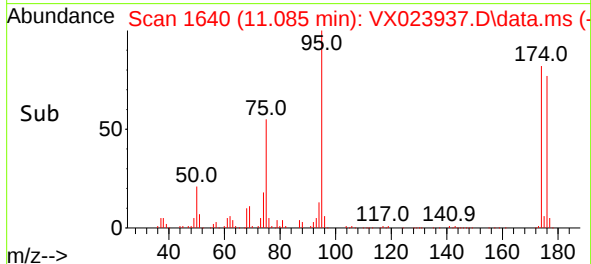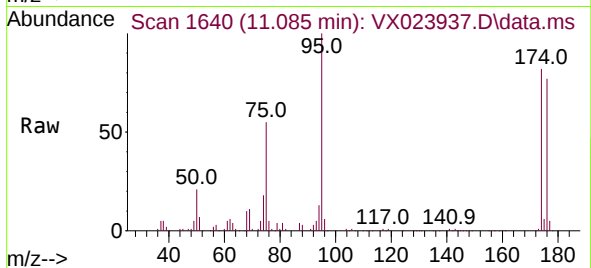

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43


Tgt Ion: 117 Resp: 214242
Ion Ratio Lower Upper
117 100
82 59.1 47.4 71.2
119 31.8 26.6 39.8

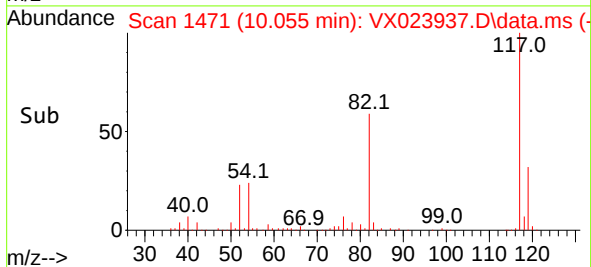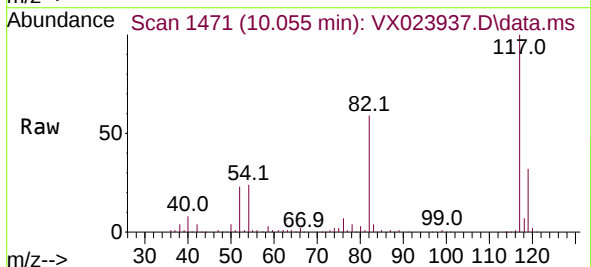






#64
Tetrachloroethene
Concen: 2.186 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.006 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43


Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921

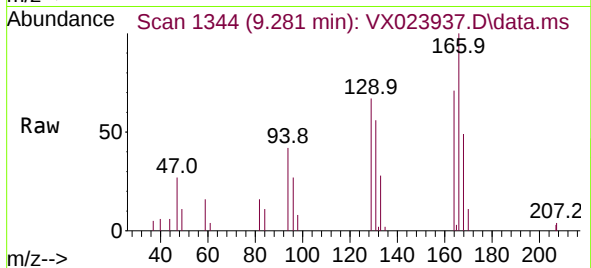



Tgt Ion:164	Resp:	3741
Ion	Ratio	Lower Upper
164	100	
166	141.0	103.4 155.2
129	95.1	70.8 106.2
131	78.6	72.5 108.7

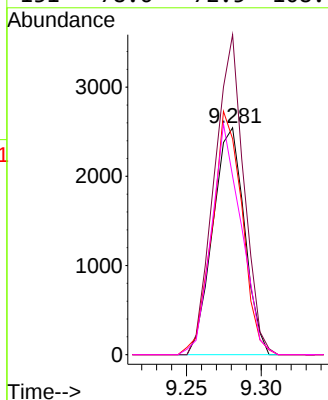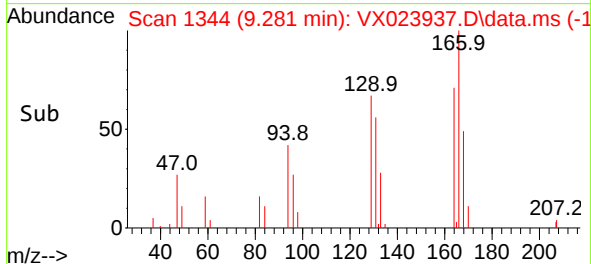


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

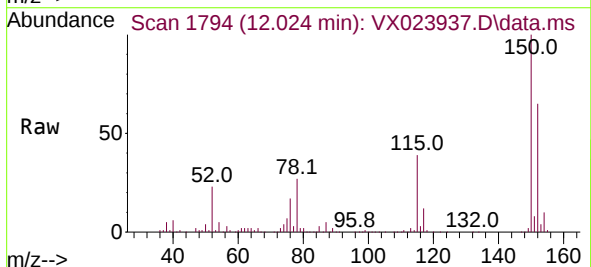

Tgt Ion:152	Resp:	91199
Ion	Ratio	Lower Upper
152	100	
115	59.0	41.1 123.3
150	155.2	0.0 349.0



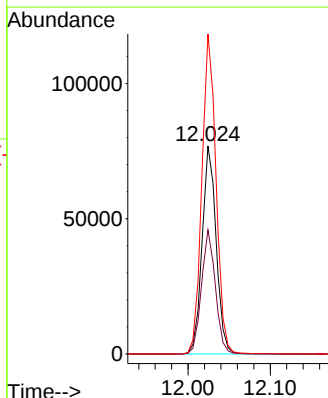
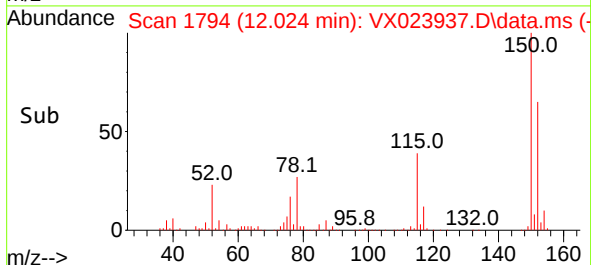




#76
1,2,3-Trichloropropane
Concen: 25.125 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921


Tgt Ion: 75 Resp: 53451
Ion Ratio Lower Upper
75 100
77 0.9 19.1 57.5#

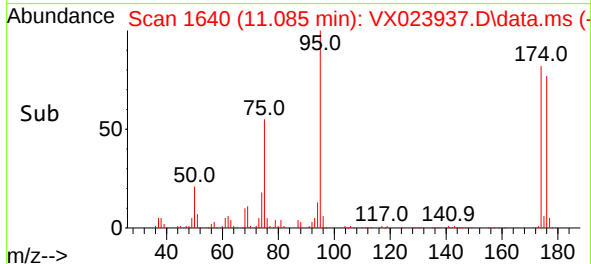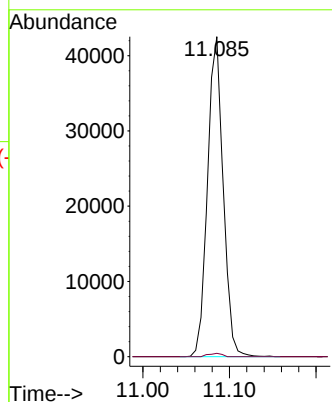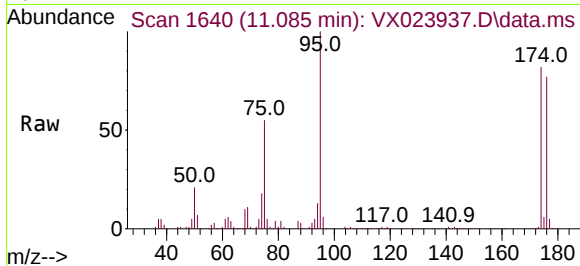

#81
trans-1,4-Dichloro-2-butene
Concen: 73.905 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43


Tgt Ion: 75 Resp: 53451
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

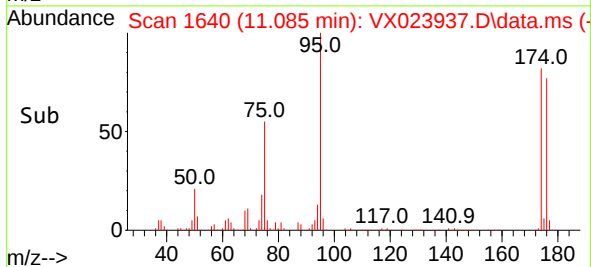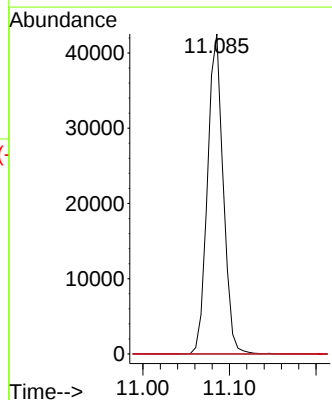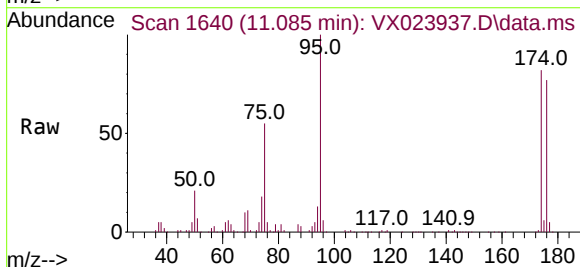

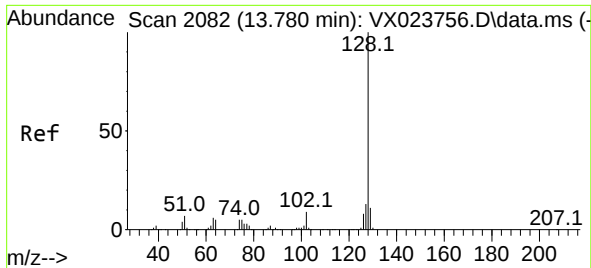

#95
Naphthalene
Concen: 1.289 ug/l
RT: 13.786 min Scan# 2083
Delta R.T. 0.006 min
Lab File: VX023937.D
Acq: 25 Aug 2021 14:43

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-02-GW-081921

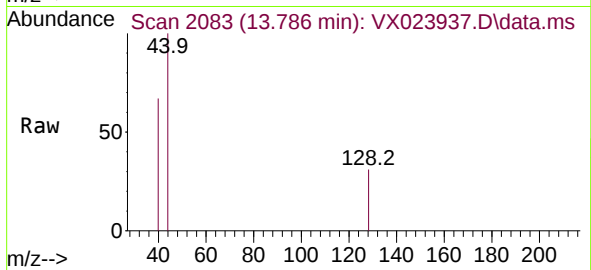

Tgt Ion:128 Resp: 48
Ion Ratio Lower Upper
128 100
127 0.0 10.3 15.5#
129 0.0 8.8 13.2#

