

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
 Data File : VX023942.D
 Acq On : 25 Aug 2021 16:41
 Operator : JC/MD
 Sample : M3525-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WVLY-SW-17-GW-082021

Quant Time: Aug 26 07:37:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	137498	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	235282	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	220028	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	88294	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	98351	51.250	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.500%			
35) Dibromofluoromethane	5.397	113	75823	48.690	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 97.380%			
50) Toluene-d8	8.653	98	283347	47.806	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 95.620%			
62) 4-Bromofluorobenzene	11.085	95	97330	44.608	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 89.220%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.172	85	764	0.527	ug/l	78
3) Chloromethane	1.300	50	438	0.275	ug/l	96
5) Bromomethane	1.617	94	454	0.465	ug/l #	76
6) Chloroethane	1.684	64	68	2.268	ug/l #	43
7) Trichlorofluoromethane	1.892	101	278815	113.675	ug/l	98
9) 1,1,2-Trichlorotrifluo...	2.337	101	1266	0.917	ug/l	98
11) Tert butyl alcohol	2.953	59	122	0.314	ug/l #	73
12) 1,1-Dichloroethene	2.325	96	10526	7.977	ug/l	89
14) Allyl chloride	2.544	41	1065	0.438	ug/l #	32
16) Acetone	2.392	43	3050	3.555	ug/l	89
20) Methylene Chloride	2.800	84	592	0.361	ug/l #	84
27) cis-1,2-Dichloroethene	4.501	96	3408	2.032	ug/l	94
28) Bromochloromethane	5.105	49	11853	9.671	ug/l #	9
29) Tetrahydrofuran	5.025	42	1627	1.933	ug/l #	42
30) Chloroform	5.105	83	136007	47.652	ug/l	99
31) Cyclohexane	5.556	56	3439	1.395	ug/l #	31
32) 1,1,1-Trichloroethane	5.391	97	894	0.366	ug/l #	47
36) 1,1-Dichloropropene	5.556	75	11457	5.258	ug/l #	50
38) Carbon Tetrachloride	5.684	117	874	0.385	ug/l #	87
39) Methylcyclohexane	7.135	83	2285	0.861	ug/l #	1
41) Methacrylonitrile	5.019	41	1086	0.748	ug/l #	35
42) 1,2-Dichloroethane	6.098	62	2477	0.978	ug/l	90
44) Trichloroethene	7.135	130	178919	100.528	ug/l	98
47) Bromodichloromethane	7.830	83	1284	0.596	ug/l	96
49) 1,4-Dioxane	7.677	88	268	6.205	ug/l #	84
51) 4-Methyl-2-Pentanone	8.653	43	1583	0.585	ug/l #	1
60) Dibromochloromethane	9.525	129	247	1.814	ug/l	95
64) Tetrachloroethene	9.281	164	6035	3.434	ug/l	96
76) 1,2,3-Trichloropropane	11.085	75	53249	25.853	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	53249	76.048	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
Data File : VX023942.D
Acq On : 25 Aug 2021 16:41
Operator : JC/MD
Sample : M3525-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021

Quant Time: Aug 26 07:37:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration




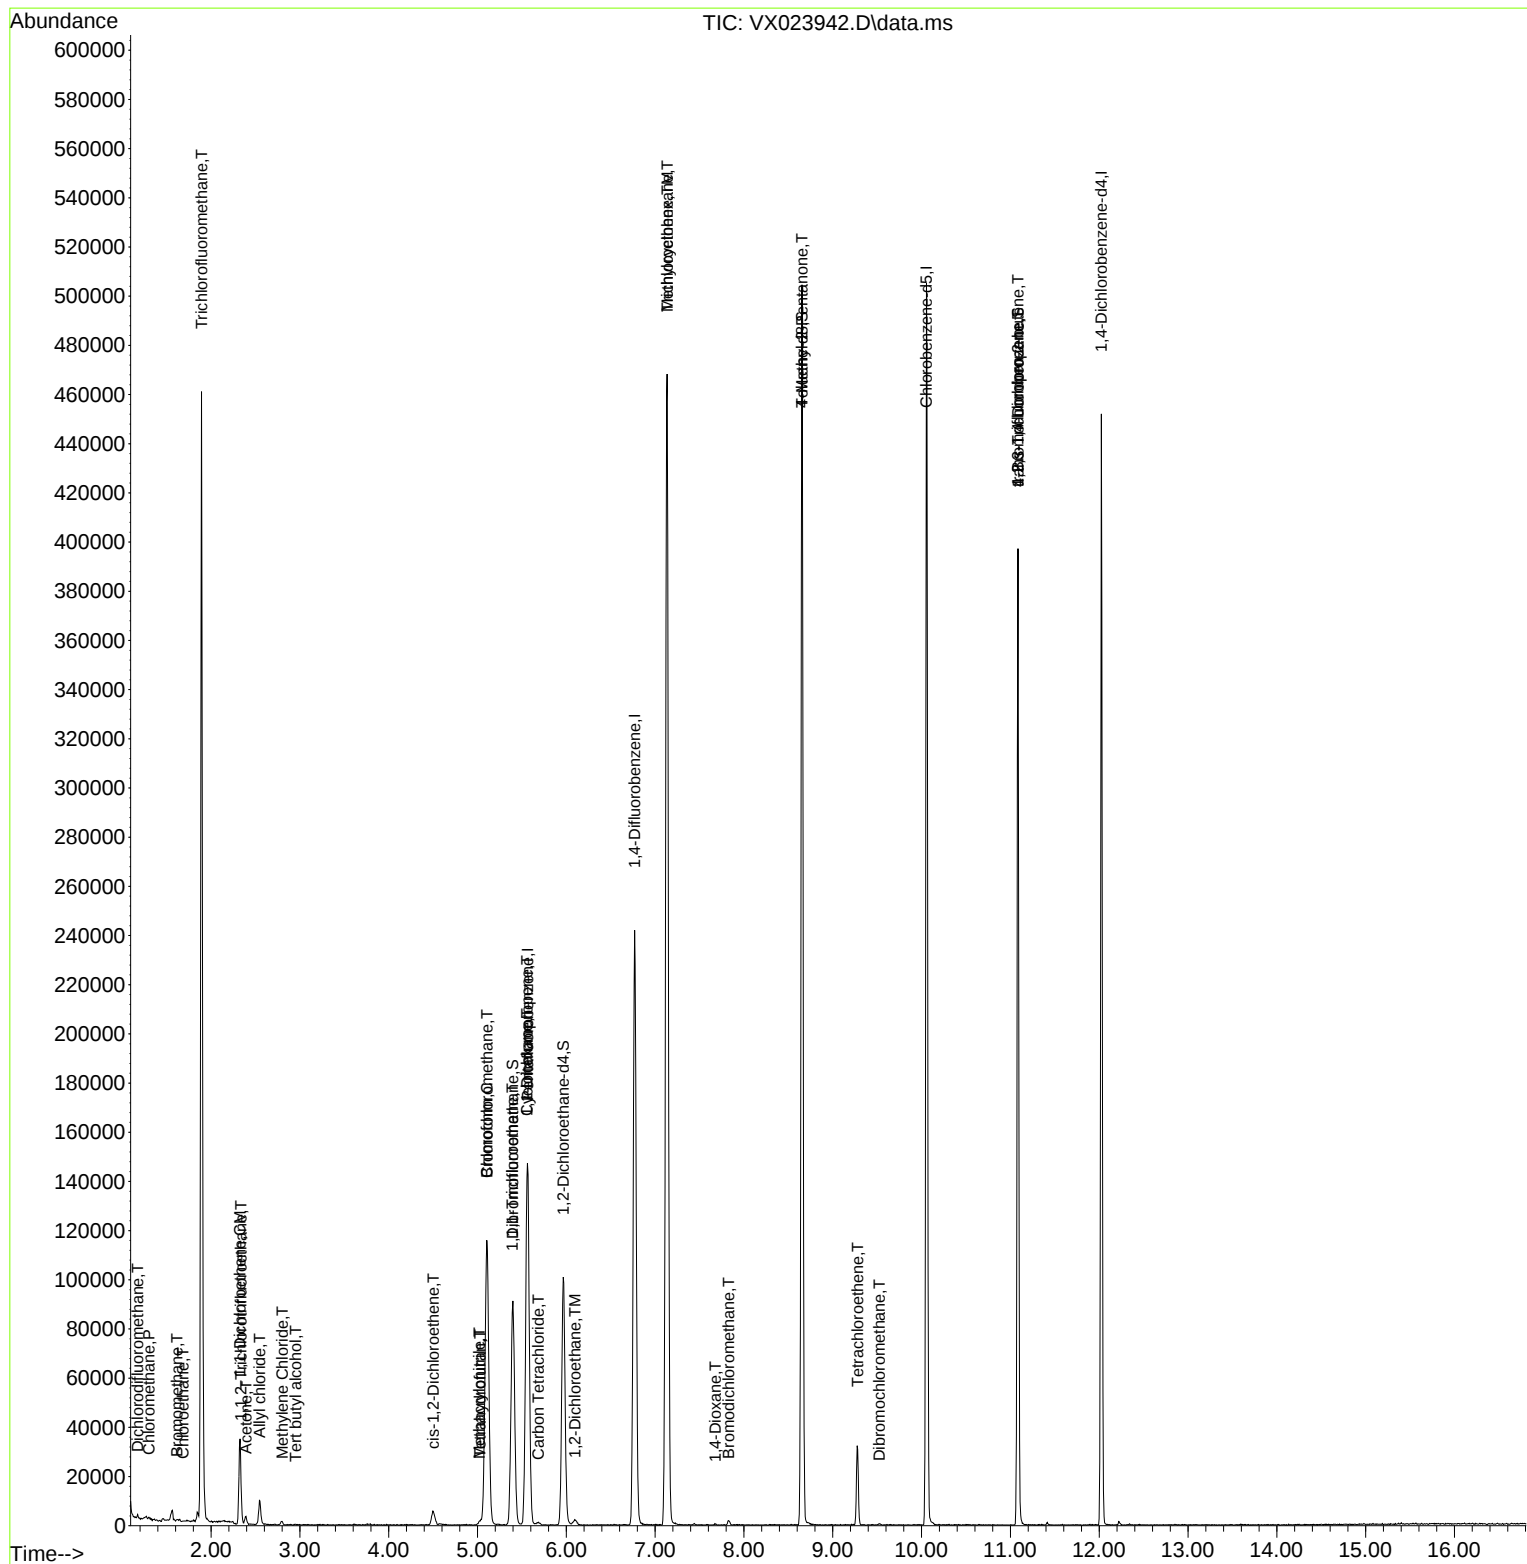


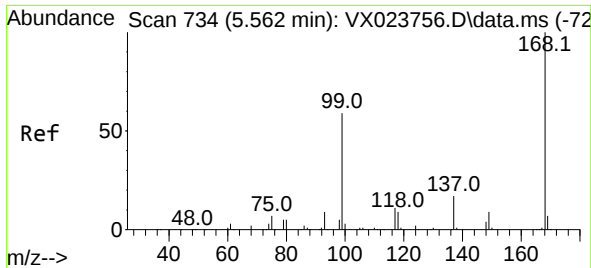

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion:168 Resp: 137498
Ion Ratio Lower Upper
168 100
99 61.3 45.8 68.6

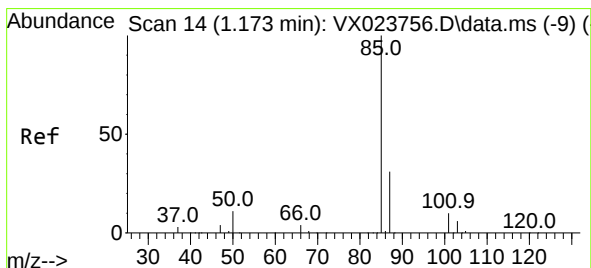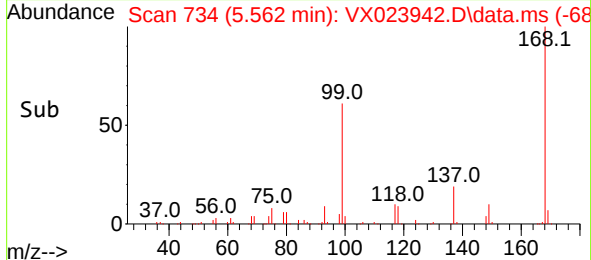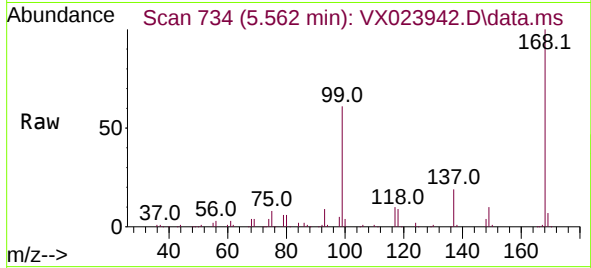

#2
Dichlorodifluoromethane
Concen: 0.527 ug/l
RT: 1.172 min Scan# 14
Delta R.T. -0.001 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 85 Resp: 764
Ion Ratio Lower Upper
85 100
87 20.2 16.4 49.2


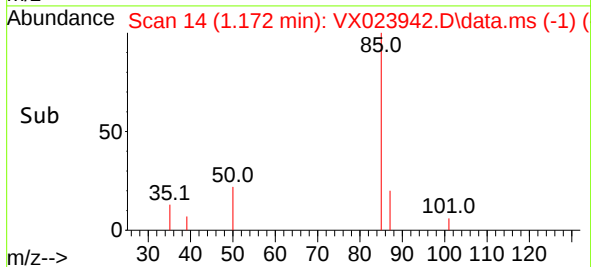

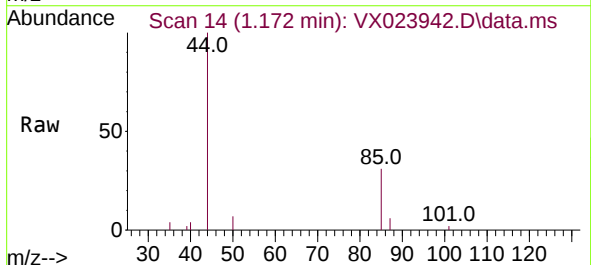


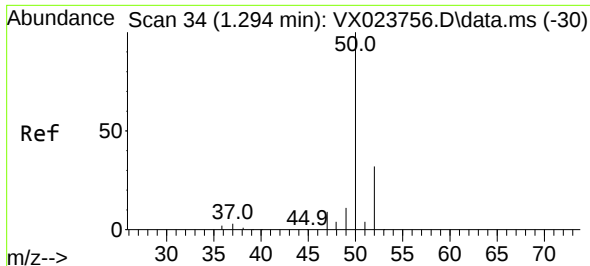

#3
Chloromethane
Concen: 0.275 ug/l
RT: 1.300 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion: 50 Resp: 438
Ion Ratio Lower Upper
50 100
52 35.4 26.4 39.6

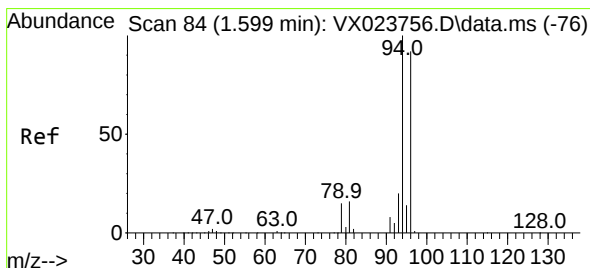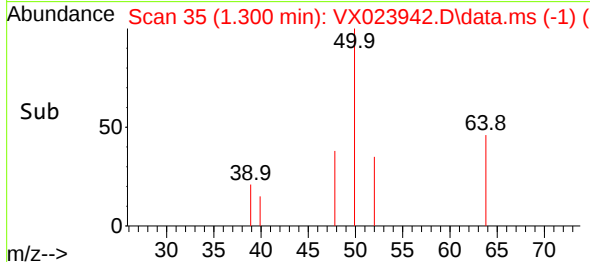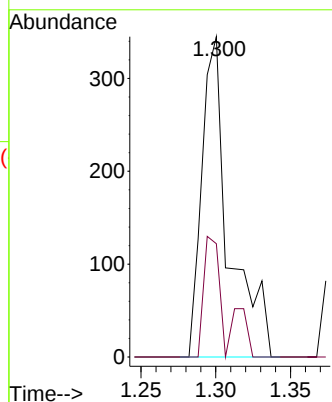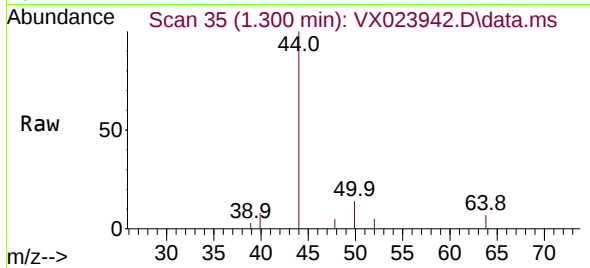

#5
Bromomethane
Concen: 0.465 ug/l
RT: 1.617 min Scan# 87
Delta R.T. 0.018 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 94 Resp: 454
Ion Ratio Lower Upper
94 100
96 119.2 76.4 114.6#


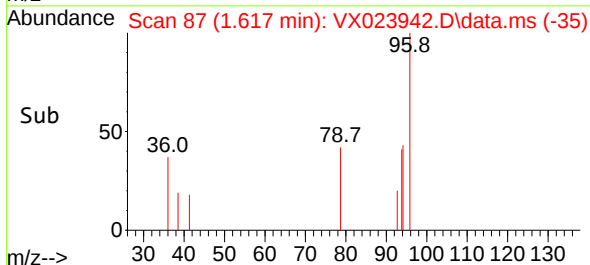

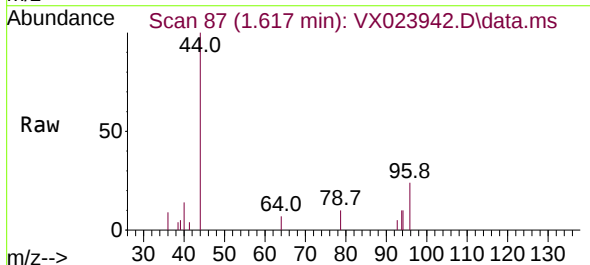


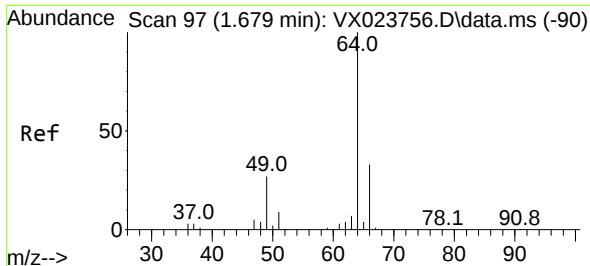

#6
Chloroethane
Concen: 2.268 ug/l
RT: 1.684 min Scan# 98
Delta R.T. 0.005 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion: 64 Resp: 68
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

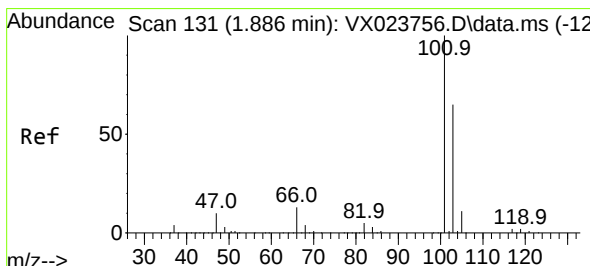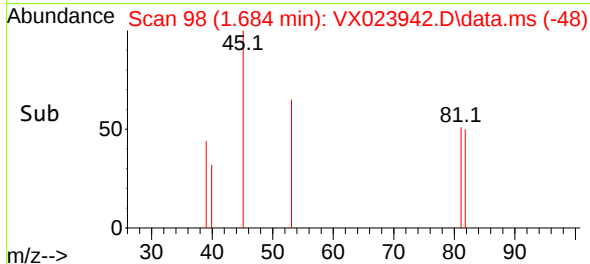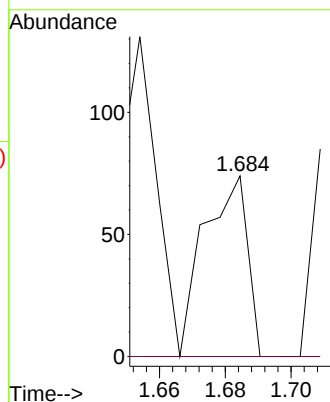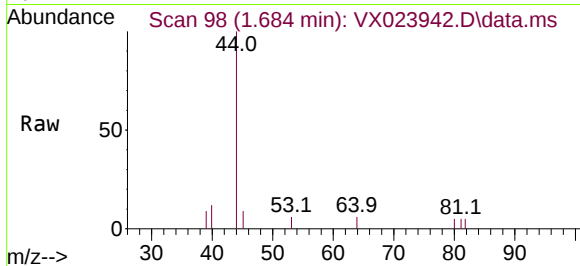

#7
Trichlorofluoromethane
Concen: 113.675 ug/l
RT: 1.892 min Scan# 132
Delta R.T. 0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 101 Resp: 278815
Ion Ratio Lower Upper
101 100
103 64.9 53.2 79.8


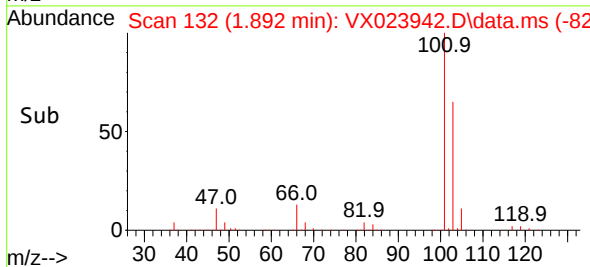
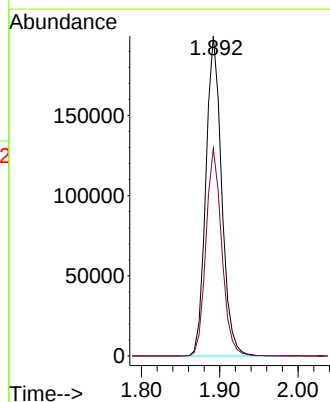
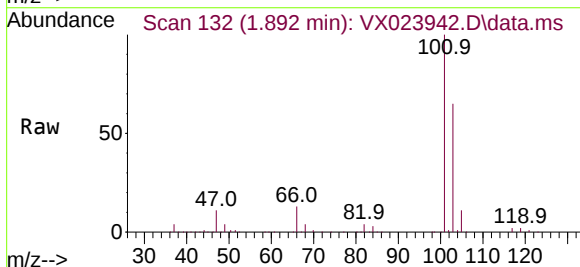




#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.917 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion:101 Resp: 1266
Ion Ratio Lower Upper
101 100
85 45.7 34.9 52.3
151 75.2 61.4 92.2

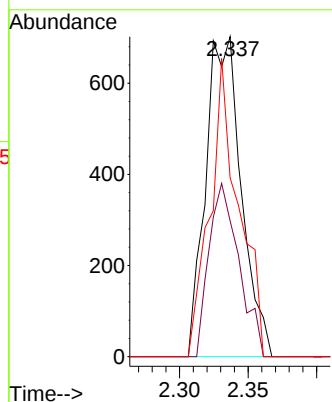

#11
Tert butyl alcohol
Concen: 0.314 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.030 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 59 Resp: 122
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

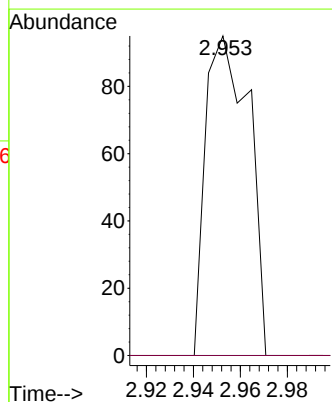



#12

1,1-Dichloroethene

Concen: 7.977 ug/l

RT: 2.325 min Scan# 203





Delta R.T. 0.006 min

Lab File: VX023942.D

Acq: 25 Aug 2021 16:41

Tgt Ion: 96 Resp: 10526

Ion	Ratio	Lower	Upper
96	100		
61	173.4	124.6	187.0
98	67.9	50.6	76.0

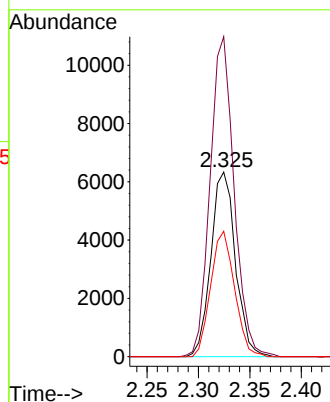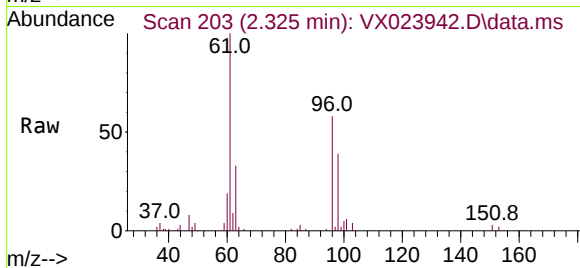

#14

Allyl chloride

Concen: 0.438 ug/l

RT: 2.544 min Scan# 239




Delta R.T. -0.122 min


Lab File: VX023942.D

Acq: 25 Aug 2021 16:41

Tgt Ion: 41 Resp: 1065


Ion	Ratio	Lower	Upper
41	100		
39	119.7	51.6	77.4#
76	0.0	30.5	45.7#

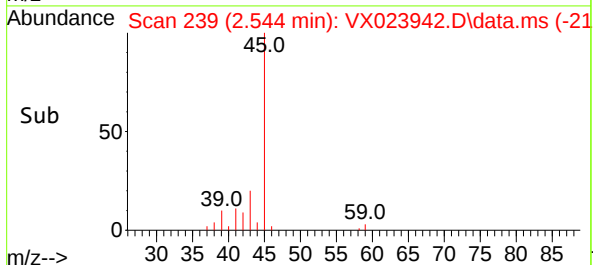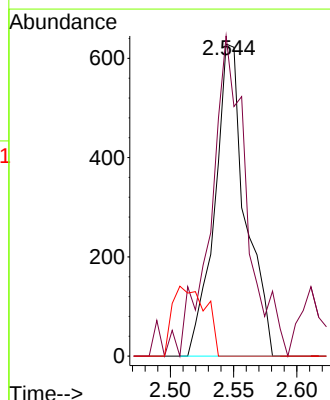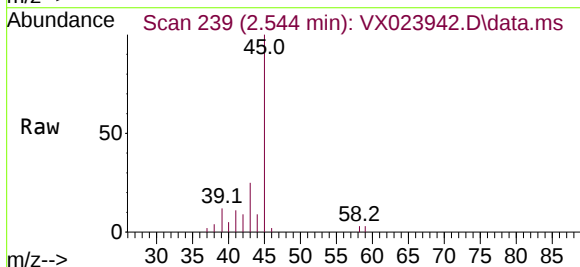



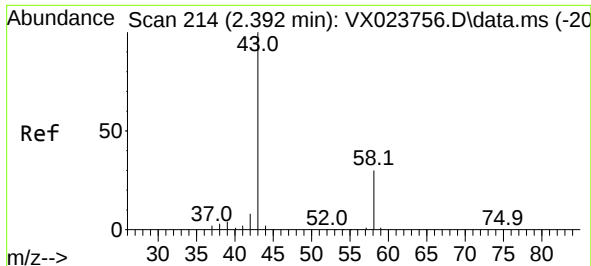


#16
Acetone
Concen: 3.555 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41


Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021

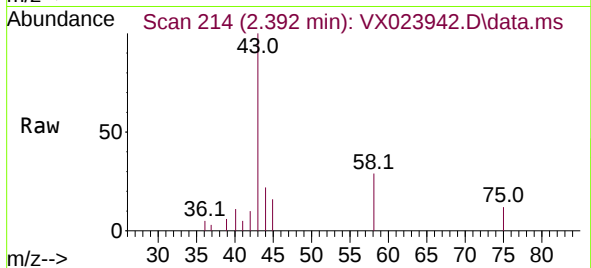



Tgt Ion: 43 Resp: 3050
Ion Ratio Lower Upper
43 100
58 28.6 27.8 41.8

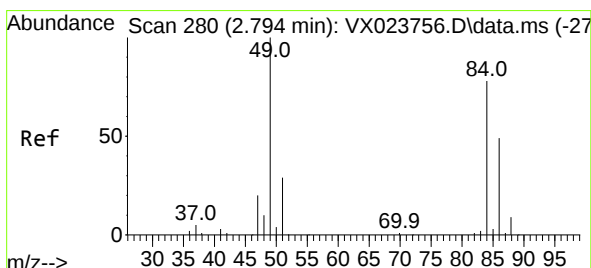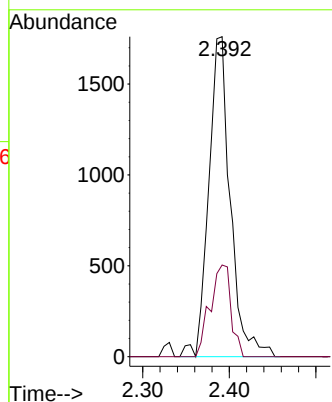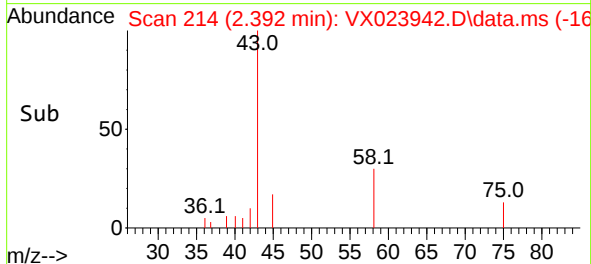


#20
Methylene Chloride
Concen: 0.361 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

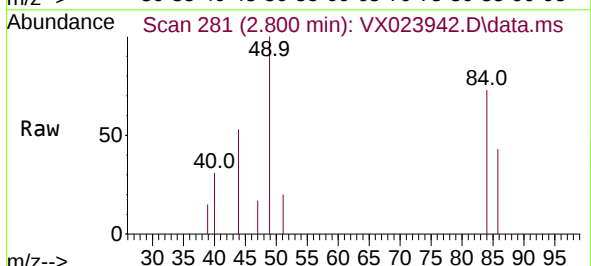

Tgt Ion: 84 Resp: 592
Ion Ratio Lower Upper
84 100
49 136.8 88.6 132.8#
51 27.7 27.0 40.6
86 59.1 50.3 75.5

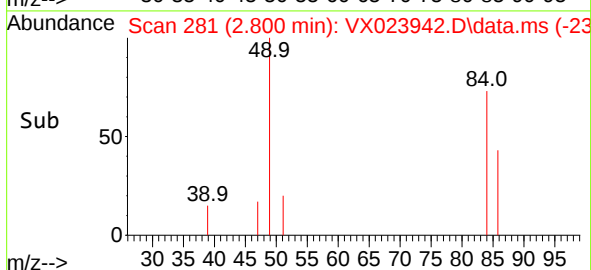



#27

cis-1,2-Dichloroethene

Concen: 2.032 ug/l

RT: 4.501 min Scan# 560





Delta R.T. 0.000 min

Lab File: VX023942.D

Acq: 25 Aug 2021 16:41

Tgt Ion:	96	Resp:	3408
Ion	Ratio	Lower	Upper
96	100		
61	132.7	0.0	285.6
98	63.3	0.0	129.6

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021

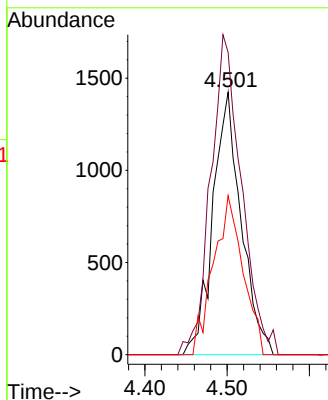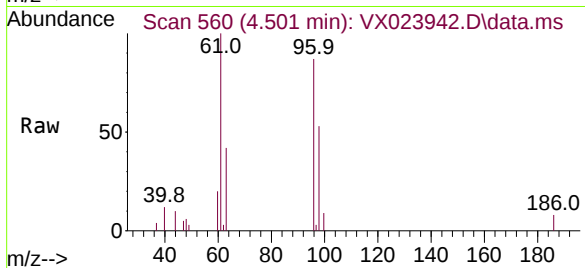

#28

Bromochloromethane

Concen: 9.671 ug/l




RT: 5.105 min Scan# 659


Delta R.T. 0.195 min

Lab File: VX023942.D

Acq: 25 Aug 2021 16:41

Tgt Ion:	49	Resp:	11853
Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	4.0
130	0.0	68.2	102.2#

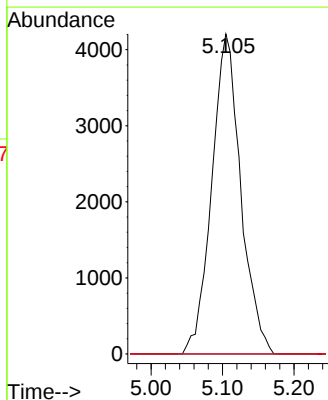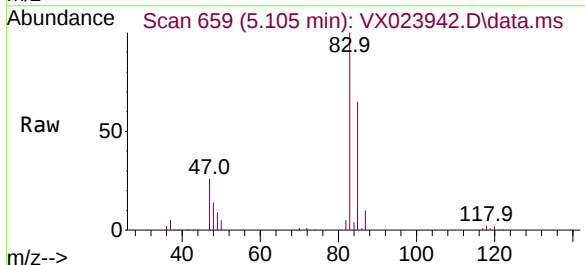

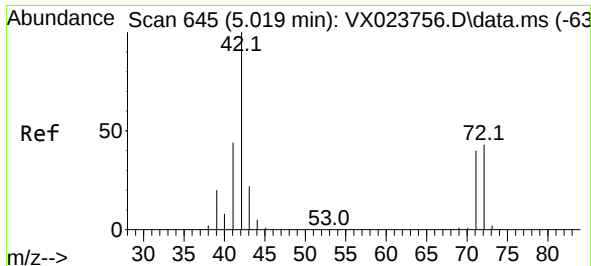

#29

Tetrahydrofuran

Concen: 1.933 ug/l

RT: 5.025 min Scan# 646





Delta R.T. 0.006 min

Lab File: VX023942.D

Acq: 25 Aug 2021 16:41

Tgt Ion:	42	Resp:	1627
Ion Ratio	Lower	Upper	
42	100		
72	0.0	41.7	62.5#
71	20.0	38.4	57.6#

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021

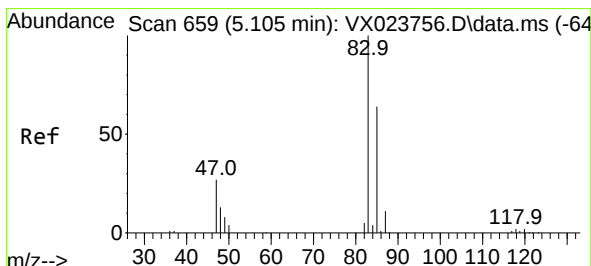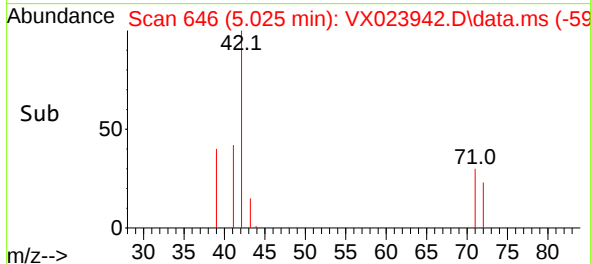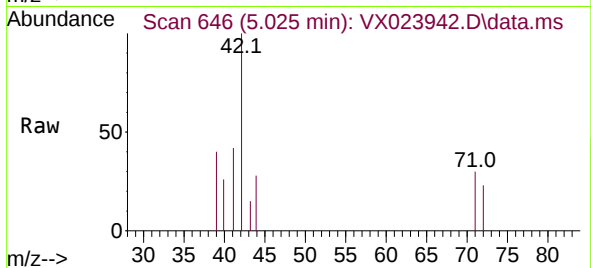

#30

Chloroform

Concen: 47.652 ug/l




RT: 5.105 min Scan# 659


Delta R.T. -0.000 min

Lab File: VX023942.D

Acq: 25 Aug 2021 16:41


Tgt Ion:	83	Resp:	136007
Ion Ratio	Lower	Upper	
83	100		
85	64.6	52.0	78.0

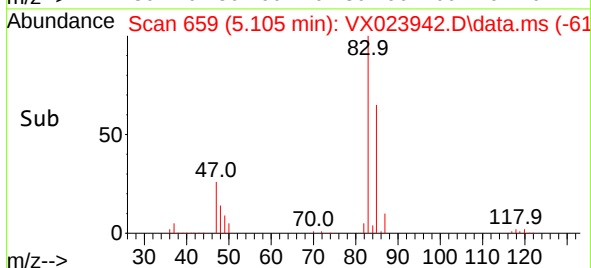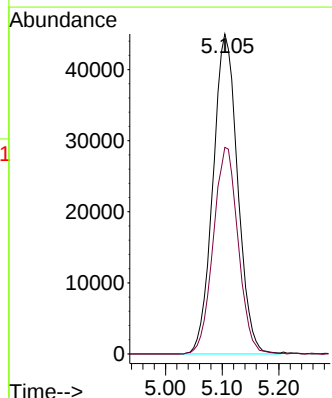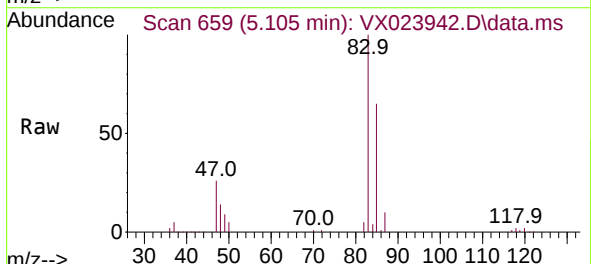






#31
Cyclohexane
Concen: 1.395 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.079 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021







Tgt Ion: 56 Resp: 3439
Ion Ratio Lower Upper
56 100
69 141.9 25.3 37.9#
84 110.5 71.4 107.0#

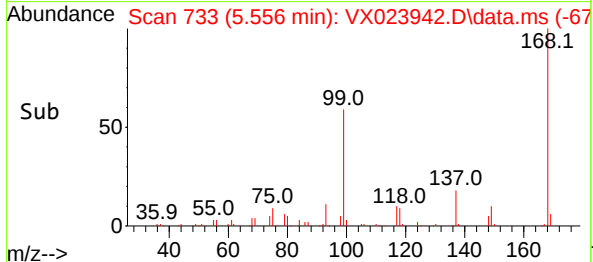

#32
1,1,1-Trichloroethane
Concen: 0.366 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 97 Resp: 894
Ion Ratio Lower Upper
97 100
99 0.0 51.5 77.3#
61 37.6 34.2 51.4

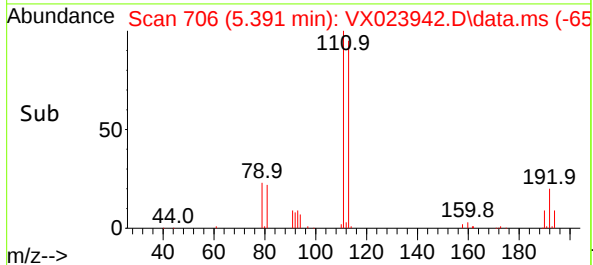







#33

1,2-Dichloroethane-d4
Concen: 51.250 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021




Tgt Ion: 65 Resp: 98351
Ion Ratio Lower Upper
65 100
67 51.1 0.0 105.4

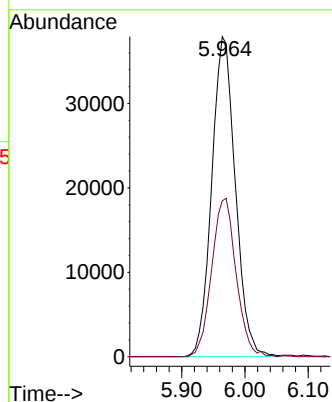


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 114 Resp: 235282
Ion Ratio Lower Upper
114 100
63 21.3 0.0 40.8
88 15.9 0.0 32.8

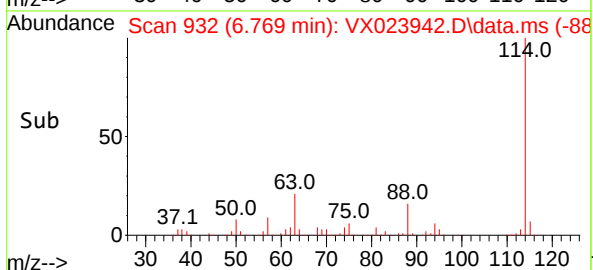



#35

Dibromofluoromethane

Concen: 48.690 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.000 min

Lab File: VX023942.D

Acq: 25 Aug 2021 16:41





Tgt Ion:113 Resp: 75823

Ion Ratio Lower Upper

113 100

111 104.4 81.9 122.9

192 19.7 16.7 25.1

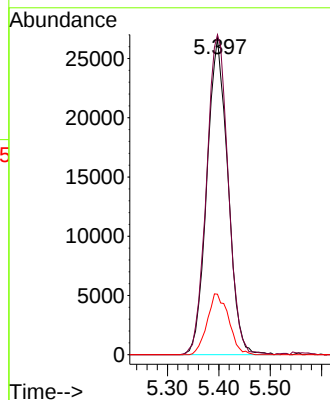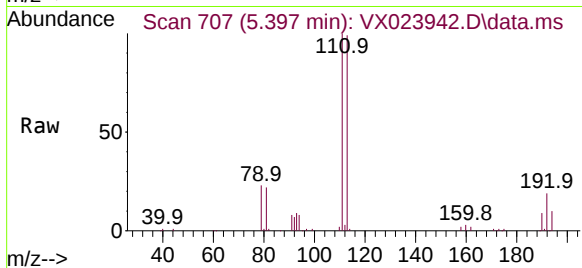

#36

1,1-Dichloropropene

Concen: 5.258 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.146 min

Lab File: VX023942.D

Acq: 25 Aug 2021 16:41




Tgt Ion: 75 Resp: 11457


Ion Ratio Lower Upper

75 100

110 9.9 18.1 54.4#

77 0.0 25.3 37.9#



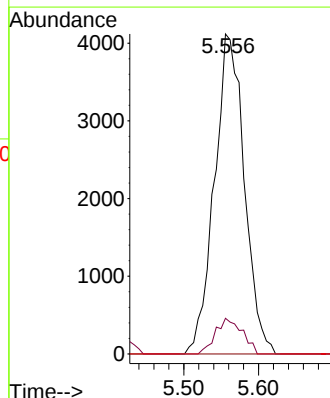
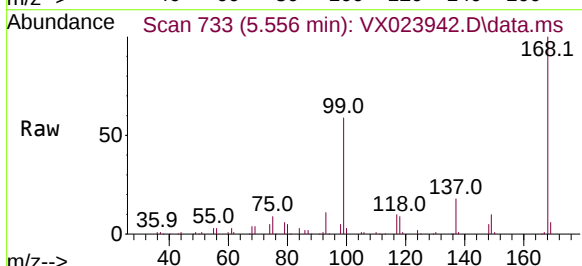




#38
Carbon Tetrachloride
Concen: 0.385 ug/l
RT: 5.684 min Scan# 754
Delta R.T. -0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion:117 Resp: 874
Ion Ratio Lower Upper
117 100
119 106.5 76.2 114.2
121 20.9 24.8 37.2#

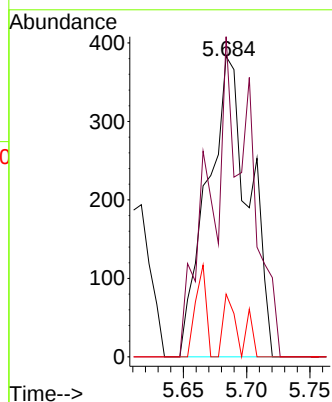

#39
Methylcyclohexane
Concen: 0.861 ug/l
RT: 7.135 min Scan# 992
Delta R.T. -0.250 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 83 Resp: 2285
Ion Ratio Lower Upper
83 100
55 0.0 58.9 88.3#
98 208.2 38.1 57.1#


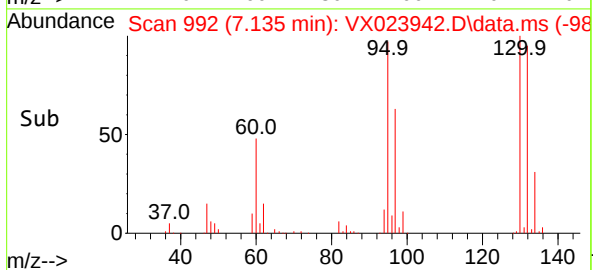

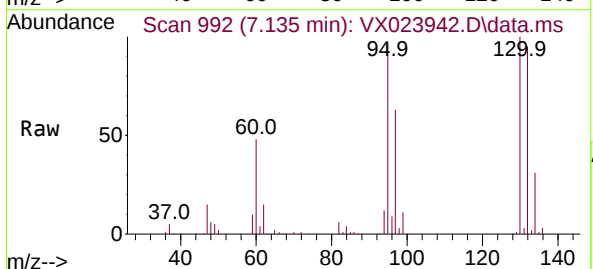




#41
Methacrylonitrile
Concen: 0.748 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.085 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion:	41	Resp:	1086
Ion	Ratio	Lower	Upper
41	100		
39	74.0	42.5	63.7#
67	0.0	65.0	97.6#
52	0.0	25.3	37.9#

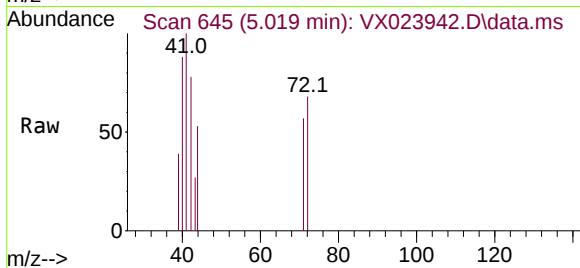

#42
1,2-Dichloroethane
Concen: 0.978 ug/l
RT: 6.098 min Scan# 822
Delta R.T. 0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion:	62	Resp:	2477
Ion	Ratio	Lower	Upper
62	100		
98	6.2	0.0	20.2




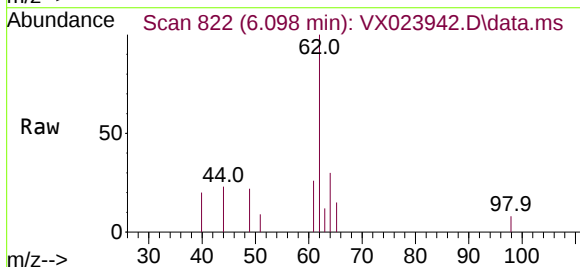




#44
Trichloroethene
Concen: 100.528 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion:130 Resp: 178919
Ion Ratio Lower Upper
130 100
95 96.7 0.0 198.0

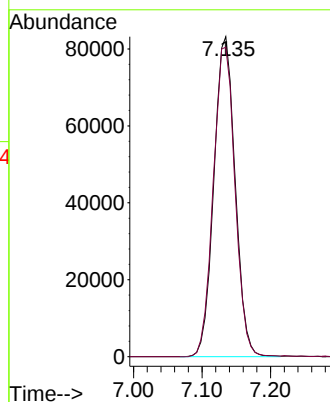

#47
Bromodichloromethane
Concen: 0.596 ug/l
RT: 7.830 min Scan# 1106
Delta R.T. -0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 83 Resp: 1284
Ion Ratio Lower Upper
83 100
85 61.1 51.4 77.0
127 8.4 6.8 10.2


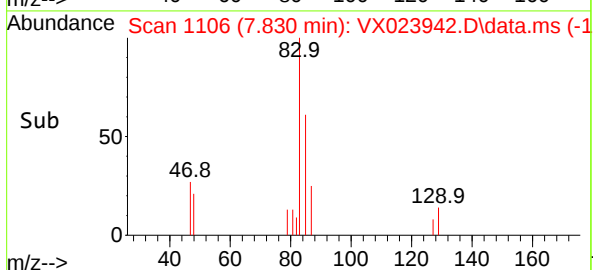
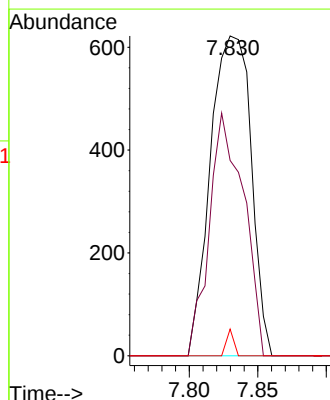





#49
1,4-Dioxane
Concen: 6.205 ug/l
RT: 7.677 min Scan# 1081
Delta R.T. 0.012 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion: 88 Resp: 268
Ion Ratio Lower Upper
88 100
43 6.7 23.2 34.8#
58 64.6 55.0 82.4

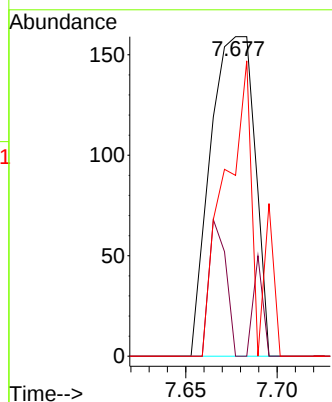

#50
Toluene-d8
Concen: 47.806 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 98 Resp: 283347
Ion Ratio Lower Upper
98 100
100 63.1 51.9 77.9



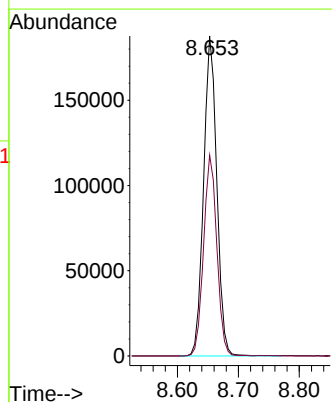





#51
4-Methyl-2-Pentanone
Concen: 0.585 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion: 43 Resp: 1583
Ion Ratio Lower Upper
43 100
58 164.6 35.4 53.0#

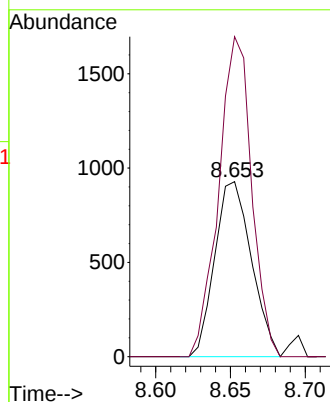

#60
Dibromochloromethane
Concen: 1.814 ug/l
RT: 9.525 min Scan# 1384
Delta R.T. -0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 129 Resp: 247
Ion Ratio Lower Upper
129 100
127 72.9 38.4 115.2



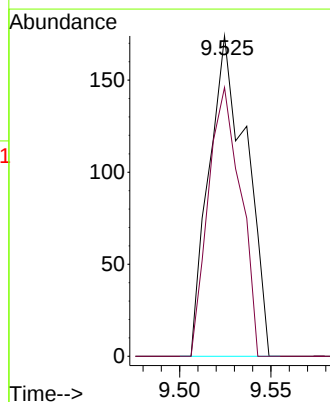



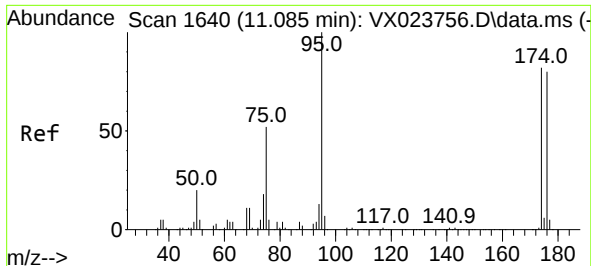

#62
4-Bromofluorobenzene
Concen: 44.608 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41




Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021


Tgt Ion: 95 Resp: 97330
Ion Ratio Lower Upper
95 100
174 81.5 0.0 154.6
176 77.5 0.0 155.8

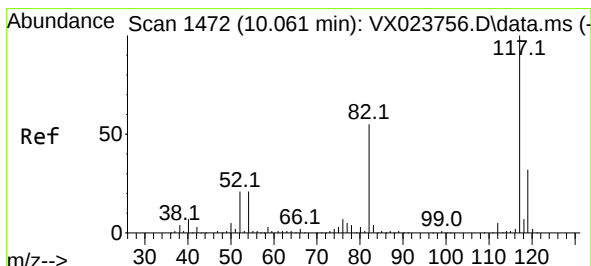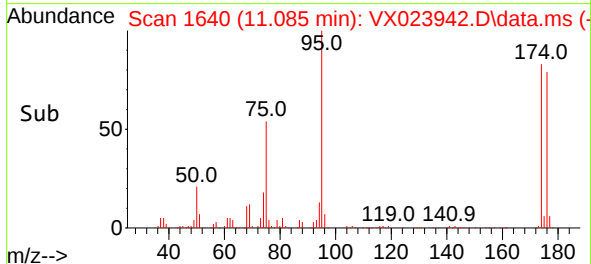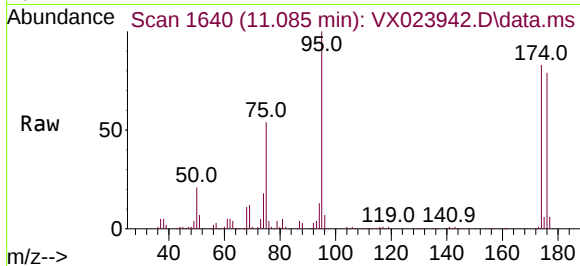

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41


Tgt Ion: 117 Resp: 220028
Ion Ratio Lower Upper
117 100
82 59.8 47.4 71.2
119 31.9 26.6 39.8

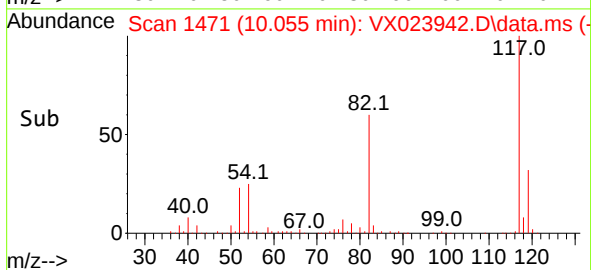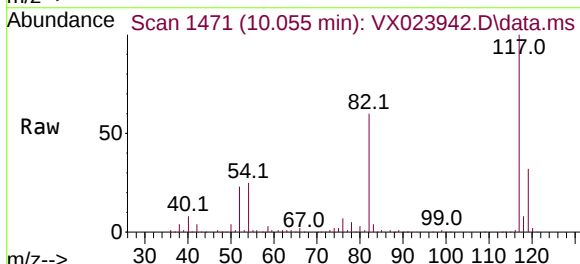






#64
Tetrachloroethene
Concen: 3.434 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. 0.006 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021







Tgt Ion:164 Resp: 6035
Ion Ratio Lower Upper
164 100
166 117.8 103.4 155.2
129 88.9 70.8 106.2
131 90.1 72.5 108.7



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion:152 Resp: 88294
Ion Ratio Lower Upper
152 100
115 59.8 41.1 123.3
150 158.1 0.0 349.0







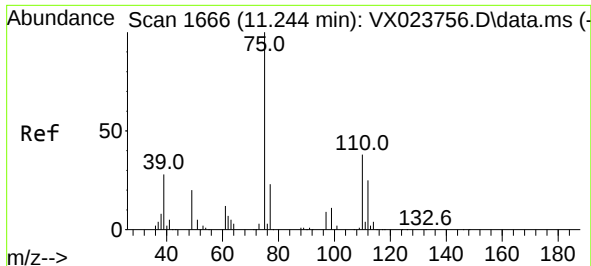

#76
1,2,3-Trichloropropane
Concen: 25.853 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Instrument :
MSVOA_X
ClientSampleId :
WVLY-SW-17-GW-082021

Tgt Ion: 75 Resp: 53249
Ion Ratio Lower Upper
75 100
77 1.0 19.1 57.5#

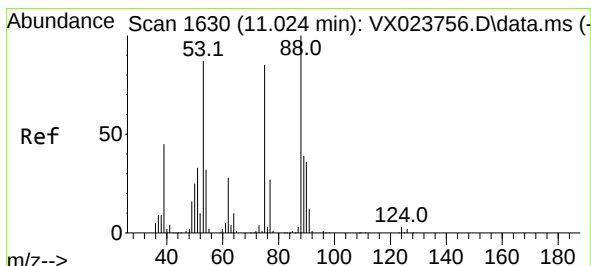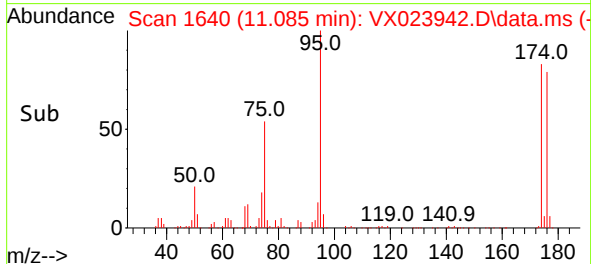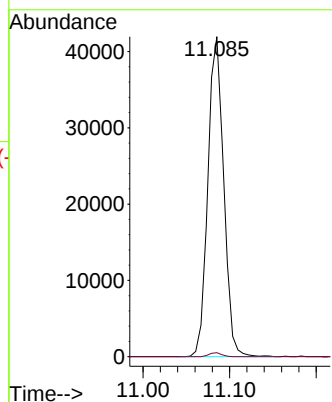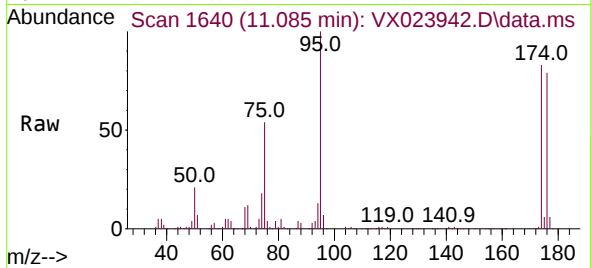

#81
trans-1,4-Dichloro-2-butene
Concen: 76.048 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023942.D
Acq: 25 Aug 2021 16:41

Tgt Ion: 75 Resp: 53249
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#

