

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
 Data File : VX023929.D
 Acq On : 25 Aug 2021 10:50
 Operator : JC/MD
 Sample : VX0825WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0825WBL01

Quant Time: Aug 25 11:22:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	191166	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	307101	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	276494	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	124340	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	142911	53.563	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 107.120%	
35) Dibromofluoromethane	5.397	113	105406	51.857	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.720%	
50) Toluene-d8	8.653	98	377108	48.745	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 97.500%	
62) 4-Bromofluorobenzene	11.085	95	133713	46.951	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 93.900%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
Data File : VX023929.D
Acq On : 25 Aug 2021 10:50
Operator : JC/MD
Sample : VX0825WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL01

Quant Time: Aug 25 11:22:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration




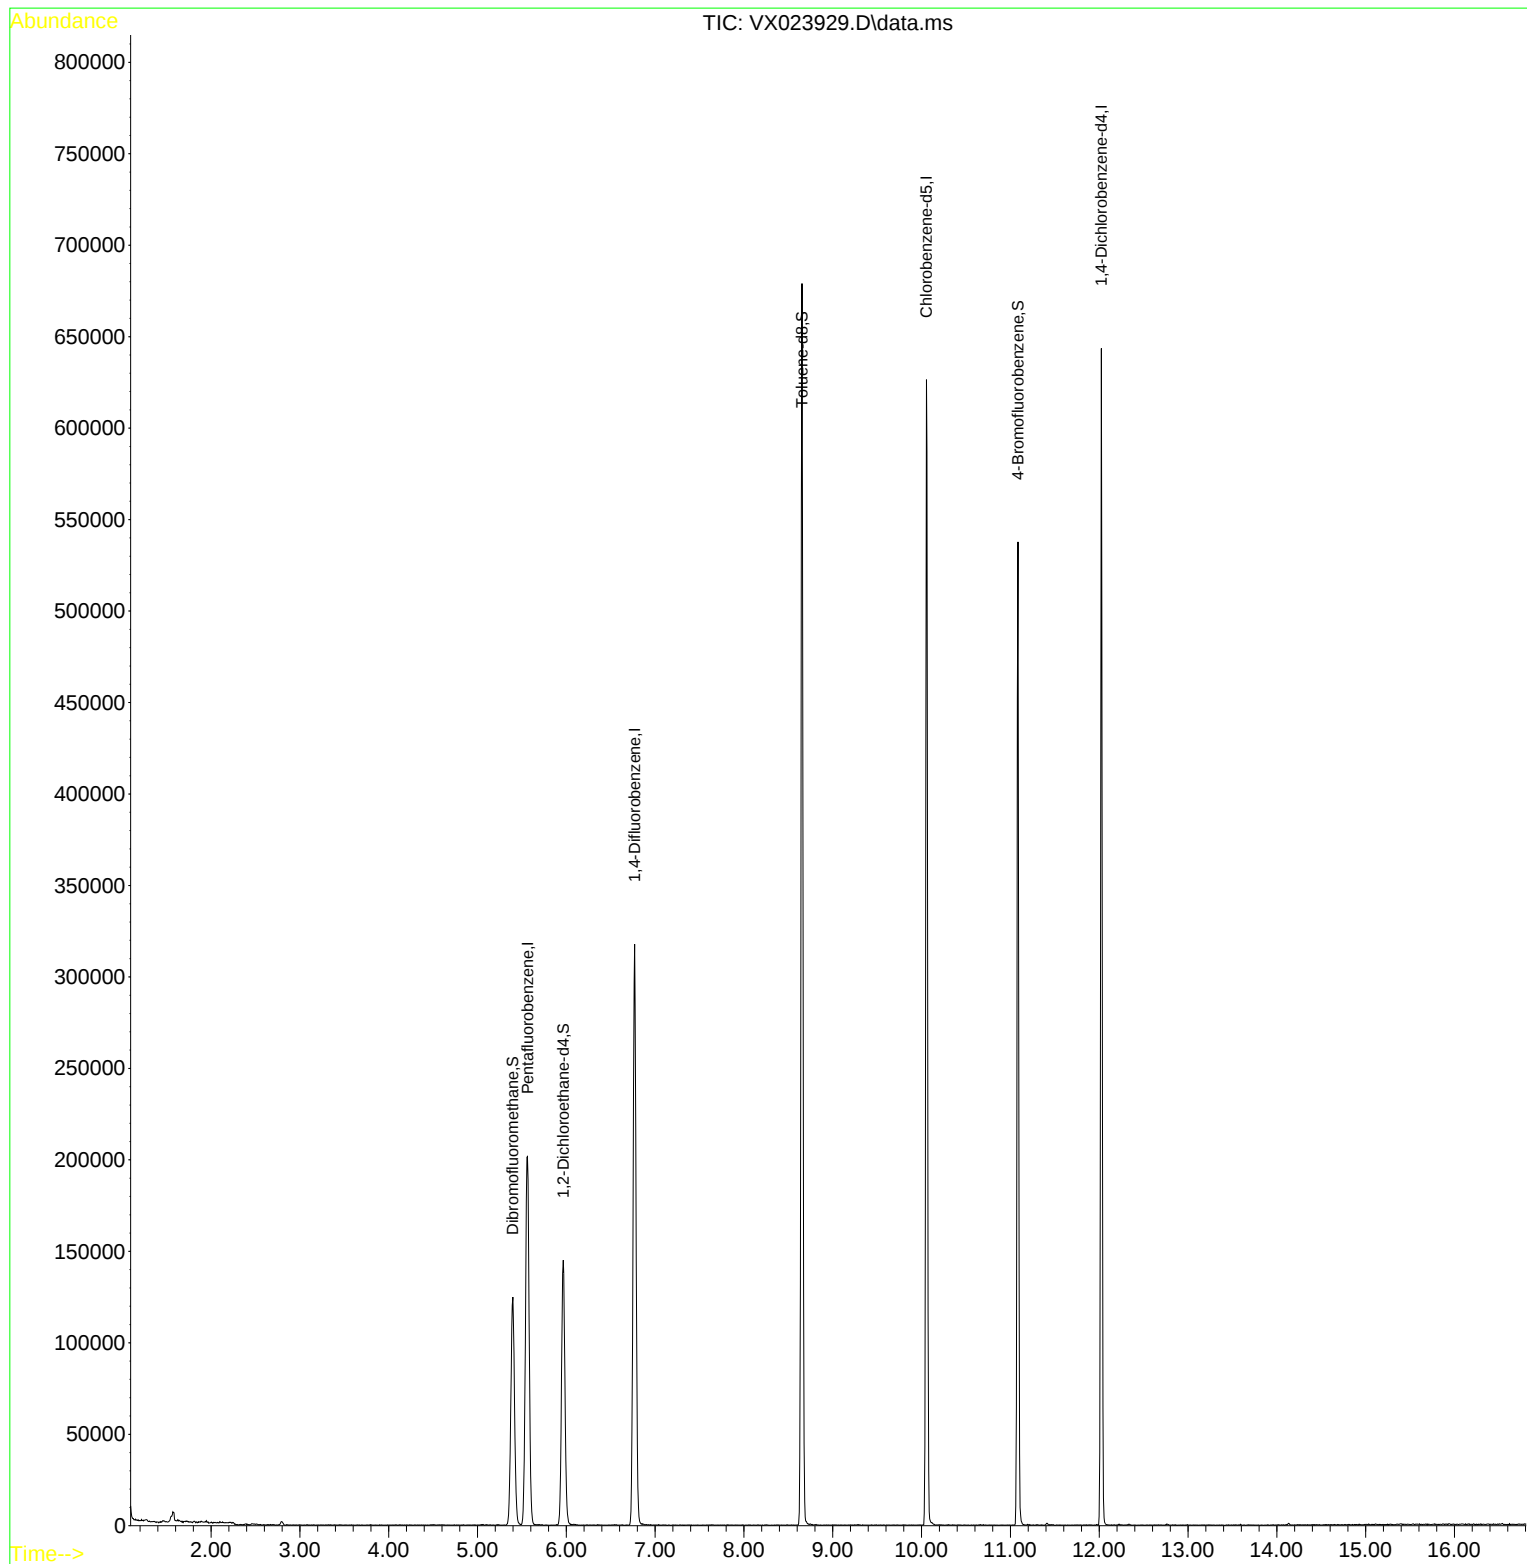


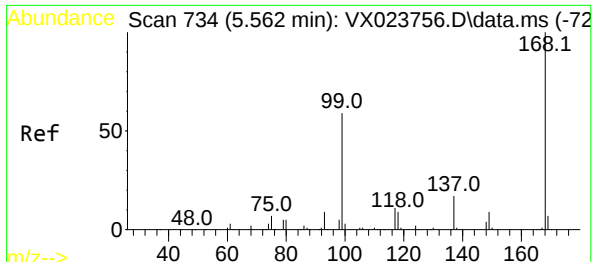

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL01


Tgt Ion:168 Resp: 191166
Ion Ratio Lower Upper
168 100
99 56.7 45.8 68.6

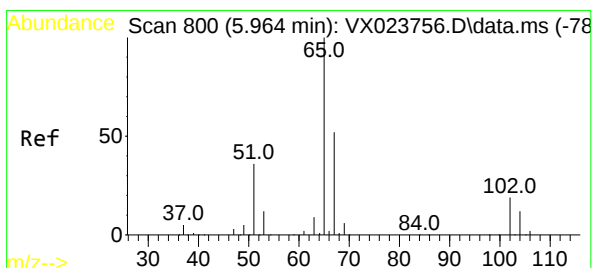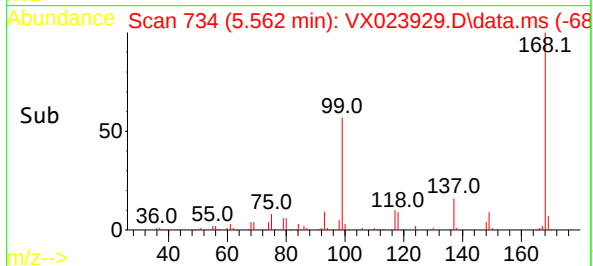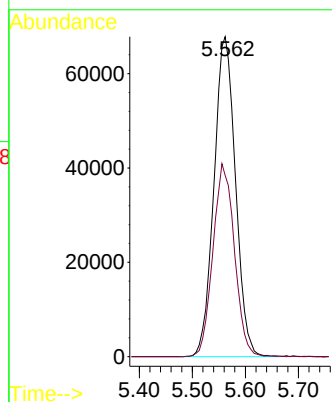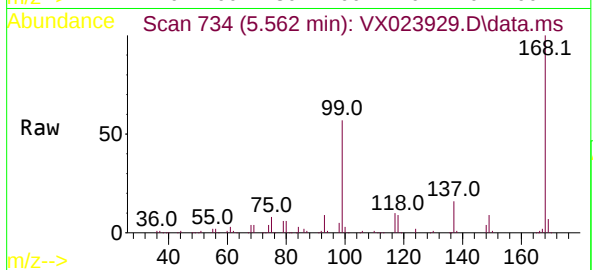

#33
1,2-Dichloroethane-d4
Concen: 53.563 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50

Tgt Ion: 65 Resp: 142911
Ion Ratio Lower Upper
65 100
67 51.2 0.0 105.4


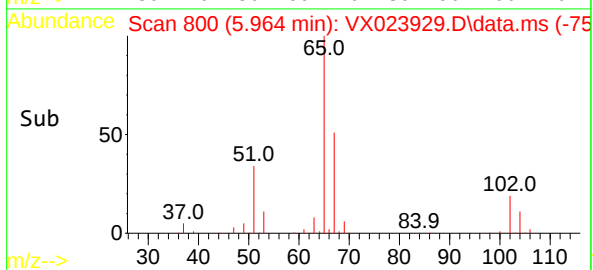
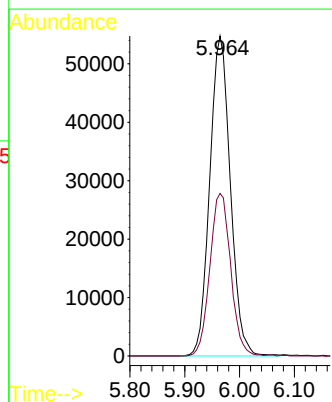
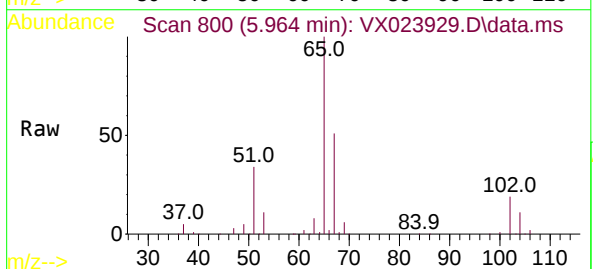


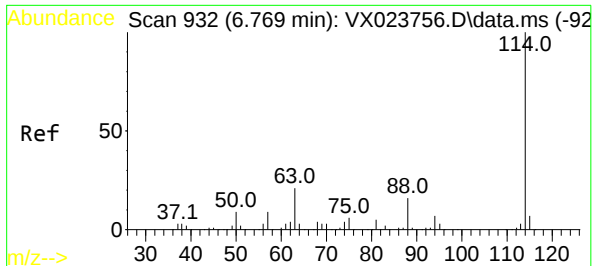

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL01


Tgt Ion:114 Resp: 307101
Ion Ratio Lower Upper
114 100
63 21.9 0.0 40.8
88 15.6 0.0 32.8

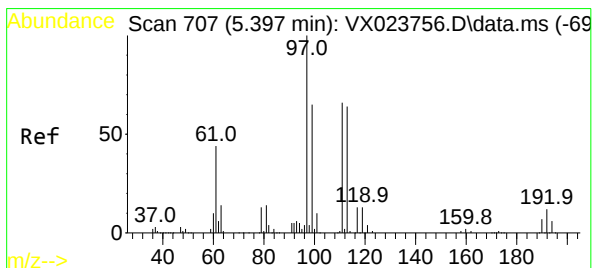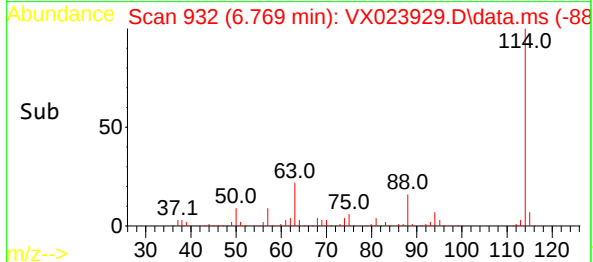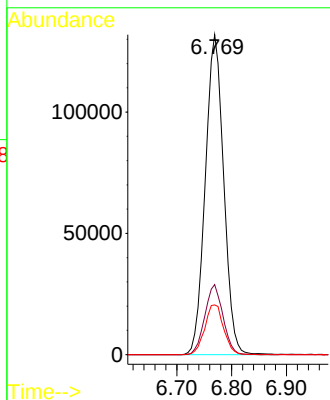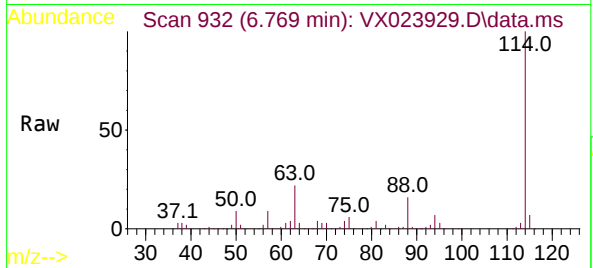

#35
Dibromofluoromethane
Concen: 51.857 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50

Tgt Ion:113 Resp: 105406
Ion Ratio Lower Upper
113 100
111 102.5 81.9 122.9
192 19.6 16.7 25.1


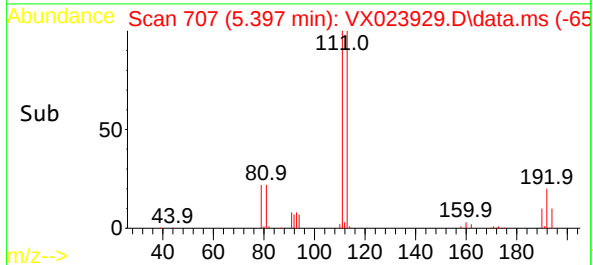
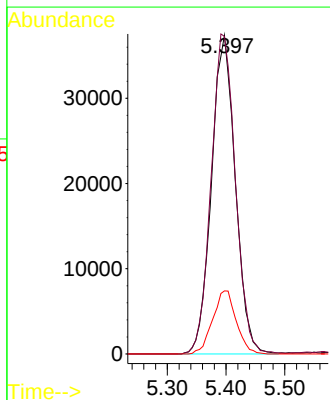
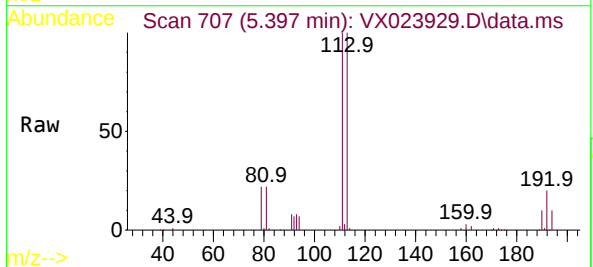


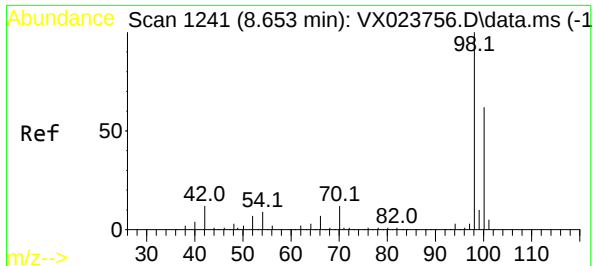

#50
Toluene-d8
Concen: 48.745 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL01


Tgt Ion: 98 Resp: 377108
Ion Ratio Lower Upper
98 100
100 64.2 51.9 77.9

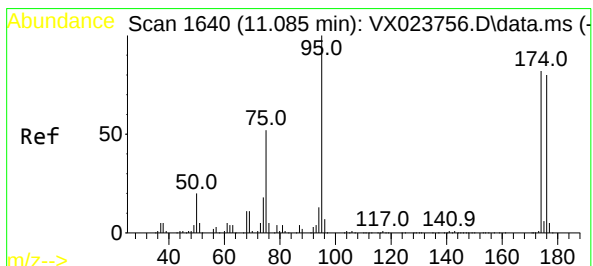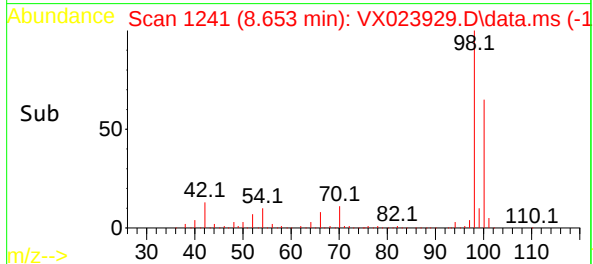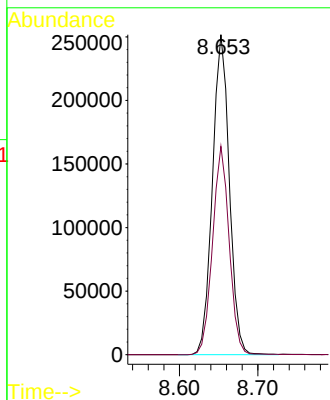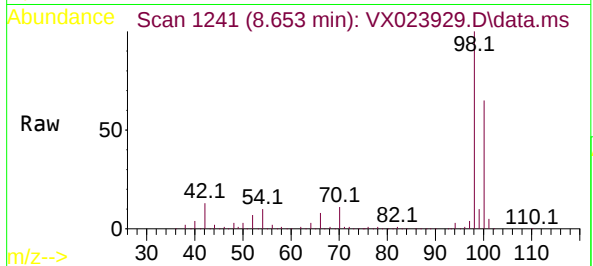

#62
4-Bromofluorobenzene
Concen: 46.951 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50

Tgt Ion: 95 Resp: 133713
Ion Ratio Lower Upper
95 100
174 80.3 0.0 154.6
176 77.9 0.0 155.8


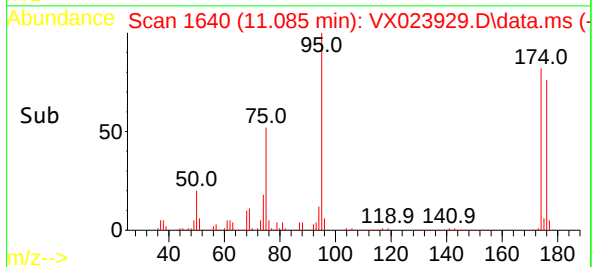
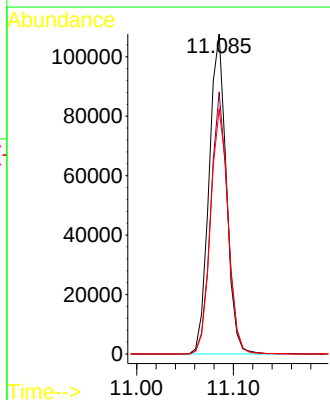
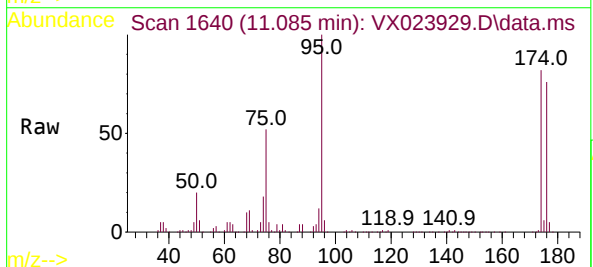


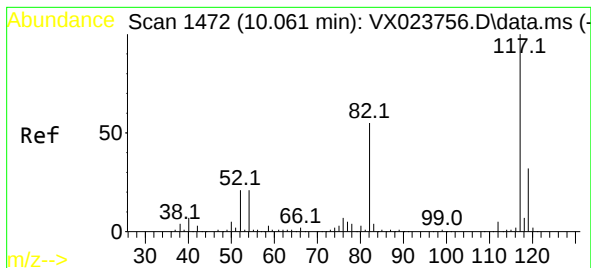

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50

Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL01

Tgt Ion:117 Resp: 276494
Ion Ratio Lower Upper
117 100
82 57.5 47.4 71.2
119 31.8 26.6 39.8

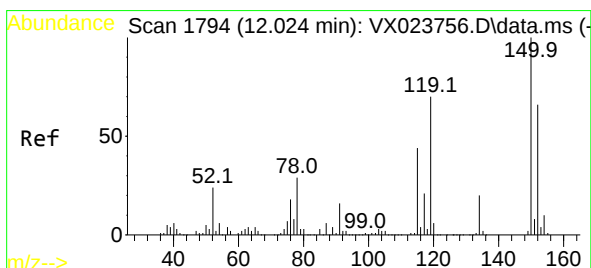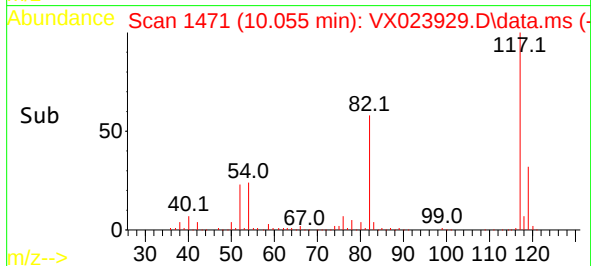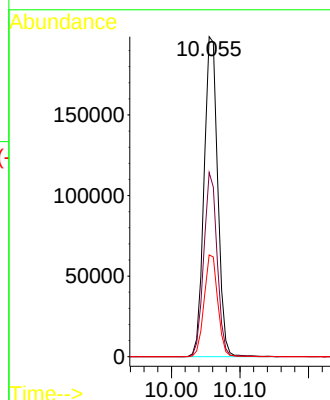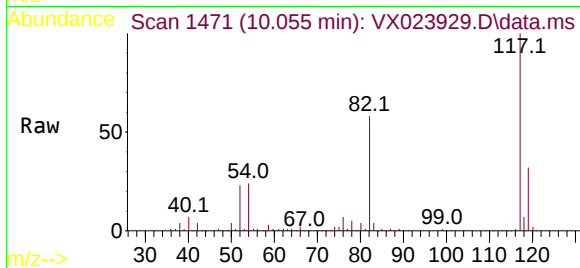

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023929.D
Acq: 25 Aug 2021 10:50

Tgt Ion:152 Resp: 124340
Ion Ratio Lower Upper
152 100
115 59.8 41.1 123.3
150 157.6 0.0 349.0

