

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
 Data File : VX023933.D
 Acq On : 25 Aug 2021 13:09
 Operator : JC/MD
 Sample : M3483-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-VPB-RW7-EB-20210817

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX023933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.556	69	77	81	rBV3	4841	9033	1.14%	0.203%
2	2.386	208	213	222	rBV	23343	37684	4.76%	0.845%
3	2.544	234	239	250	rVB2	6611	12620	1.59%	0.283%
4	2.971	302	309	318	rBV	17632	38661	4.88%	0.867%
5	4.227	503	515	529	rBV3	12109	37467	4.73%	0.840%
6	5.397	696	707	722	rBV	90916	263955	33.33%	5.921%
7	5.562	722	734	750	rVB	155209	437268	55.22%	9.809%
8	5.964	787	800	816	rBV	101253	269766	34.07%	6.051%
9	6.769	919	932	947	rBV	247314	587528	74.19%	13.179%
10	7.860	1104	1111	1115	rBV	14463	30723	3.88%	0.689%
11	7.909	1115	1119	1127	rVB	13396	26068	3.29%	0.585%
12	8.653	1234	1241	1251	rBV	520668	791914	100.00%	17.764%
13	10.055	1465	1471	1481	rBV	521966	725772	91.65%	16.280%
14	11.085	1634	1640	1652	rBV	423131	535639	67.64%	12.015%
15	12.024	1789	1794	1802	rBV	522740	643357	81.24%	14.432%
16	12.219	1822	1826	1831	rBV2	7548	10506	1.33%	0.236%




Sum of corrected areas: 4457961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
Data File : VX023933.D
Acq On : 25 Aug 2021 13:09
Operator : JC/MD
Sample : M3483-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-EB-20210817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

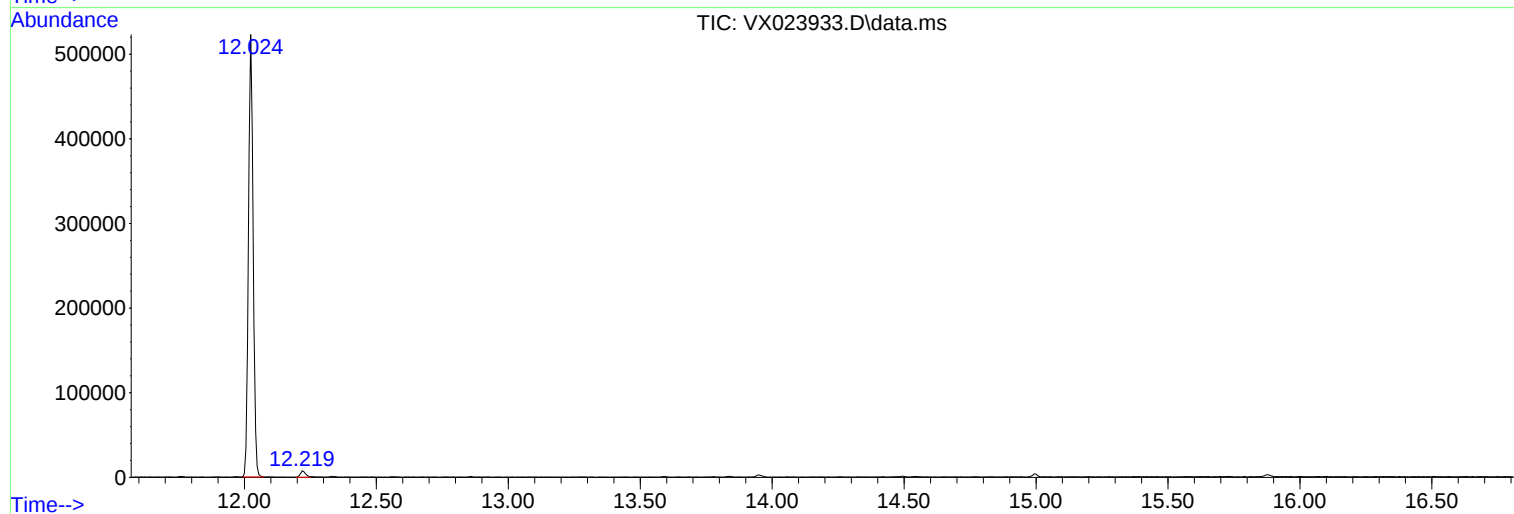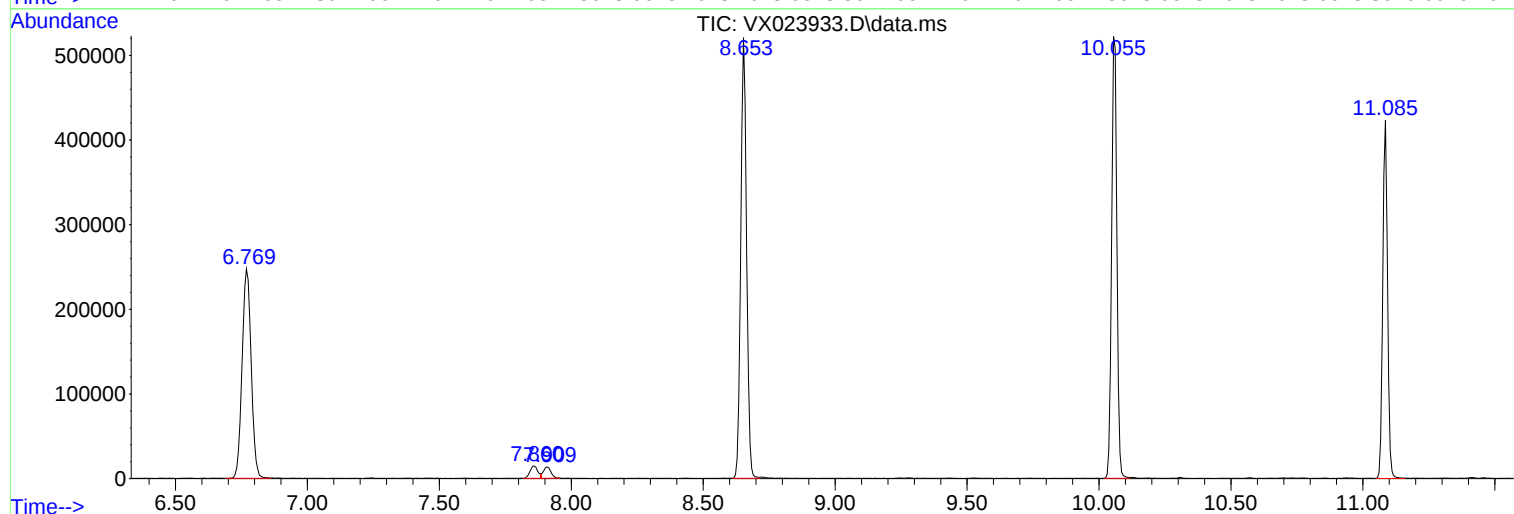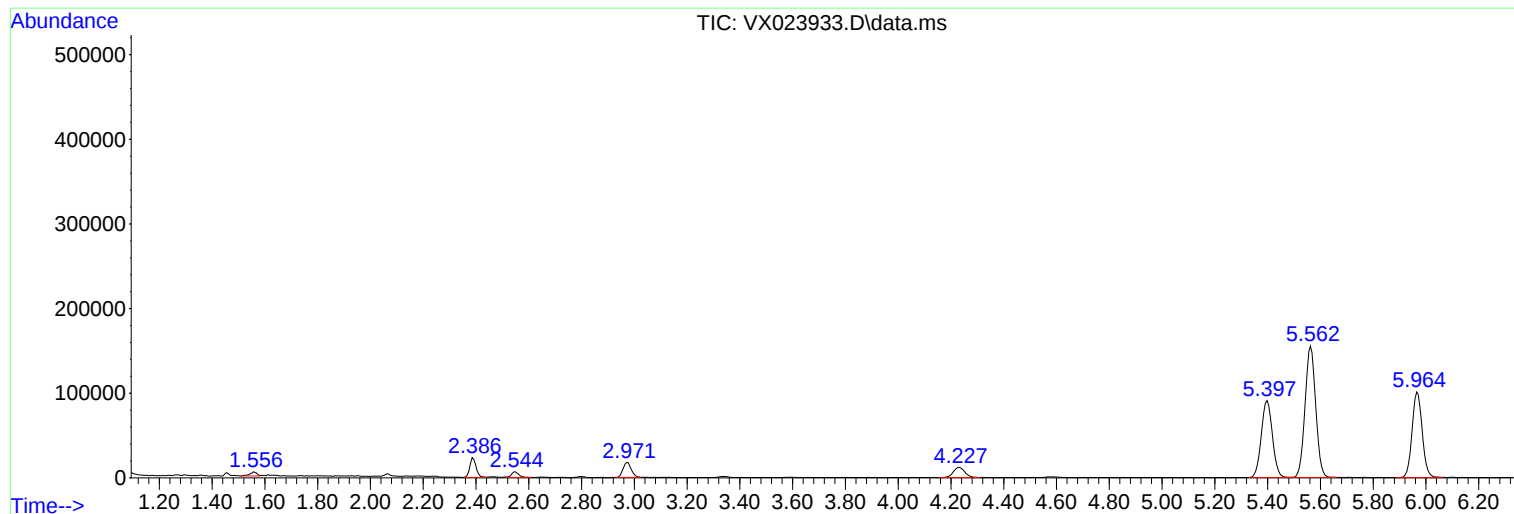

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
Data File : VX023933.D
Acq On : 25 Aug 2021 13:09
Operator : JC/MD
Sample : M3483-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-EB-20210817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082521\
Data File : VX023933.D
Acq On : 25 Aug 2021 13:09
Operator : JC/MD
Sample : M3483-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-VPB-RW7-EB-20210817

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
