

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082521\  
 Data File : VX023936.D  
 Acq On : 25 Aug 2021 14:20  
 Operator : JC/MD  
 Sample : M3525-08  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 WVLY-FB-082021

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M

Title : SW846 8260

Signal : TIC: VX023936.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.252       | 24            | 27          | 32           | rBV      | 72828          | 66433         | 8.37%           | 1.513%        |
| 2         | 1.569       | 71            | 79          | 81           | rBV4     | 4830           | 9066          | 1.14%           | 0.206%        |
| 3         | 2.544       | 231           | 239         | 248          | rVB      | 9182           | 17415         | 2.19%           | 0.397%        |
| 4         | 2.947       | 299           | 305         | 316          | rVB3     | 5574           | 13789         | 1.74%           | 0.314%        |
| 5         | 4.593       | 566           | 575         | 582          | rBV2     | 4966           | 15641         | 1.97%           | 0.356%        |
| 6         | 5.397       | 695           | 707         | 722          | rBV      | 91993          | 267311        | 33.68%          | 6.086%        |
| 7         | 5.562       | 722           | 734         | 747          | rBV      | 157456         | 446422        | 56.24%          | 10.164%       |
| 8         | 5.964       | 787           | 800         | 818          | rBV      | 101999         | 271213        | 34.17%          | 6.175%        |
| 9         | 6.769       | 922           | 932         | 952          | rVB      | 256600         | 604085        | 76.10%          | 13.754%       |
| 10        | 8.653       | 1234          | 1241        | 1251         | rBV      | 520391         | 793783        | 100.00%         | 18.073%       |
| 11        | 10.055      | 1465          | 1471        | 1486         | rBV      | 546543         | 736461        | 92.78%          | 16.768%       |
| 12        | 11.085      | 1634          | 1640        | 1651         | rBV      | 417619         | 521286        | 65.67%          | 11.869%       |
| 13        | 12.024      | 1789          | 1794        | 1806         | rVB      | 522069         | 629101        | 79.25%          | 14.324%       |




Sum of corrected areas: 4392006

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082521\  
Data File : VX023936.D  
Acq On : 25 Aug 2021 14:20  
Operator : JC/MD  
Sample : M3525-08  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
WVLY-FB-082021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

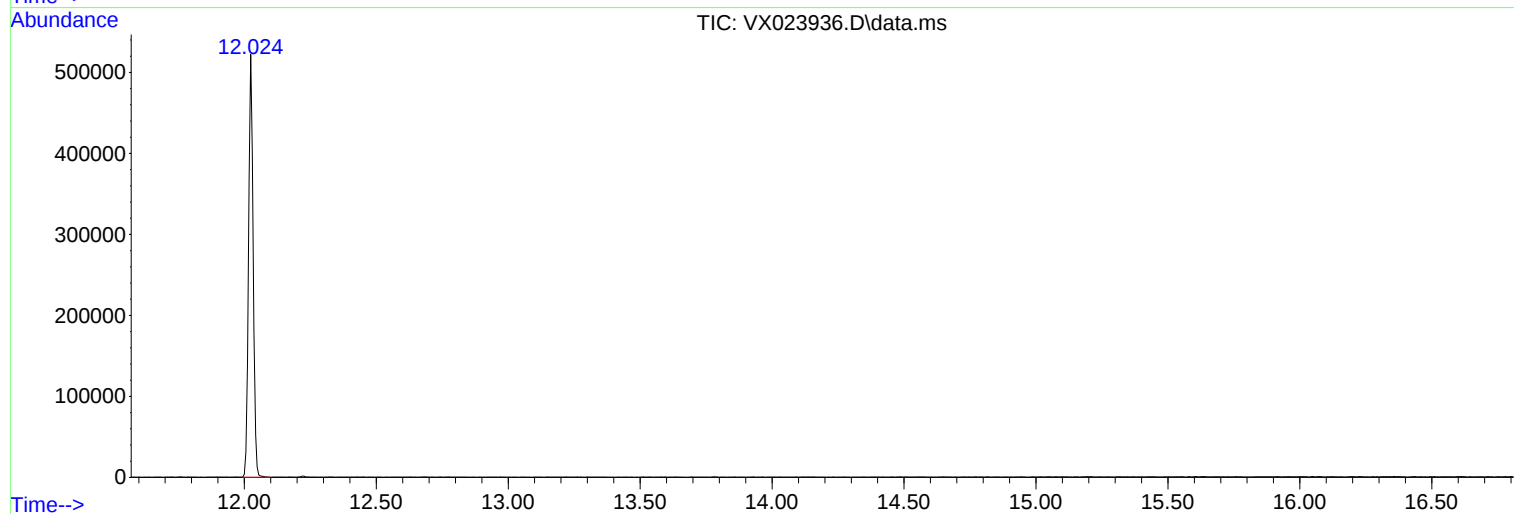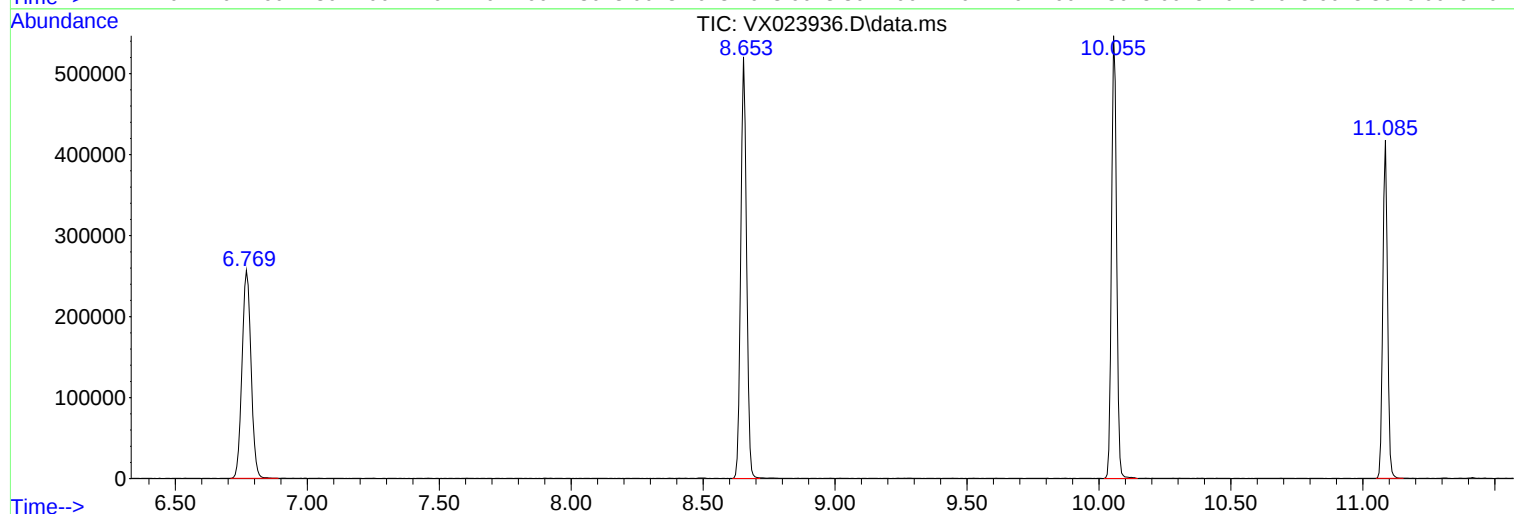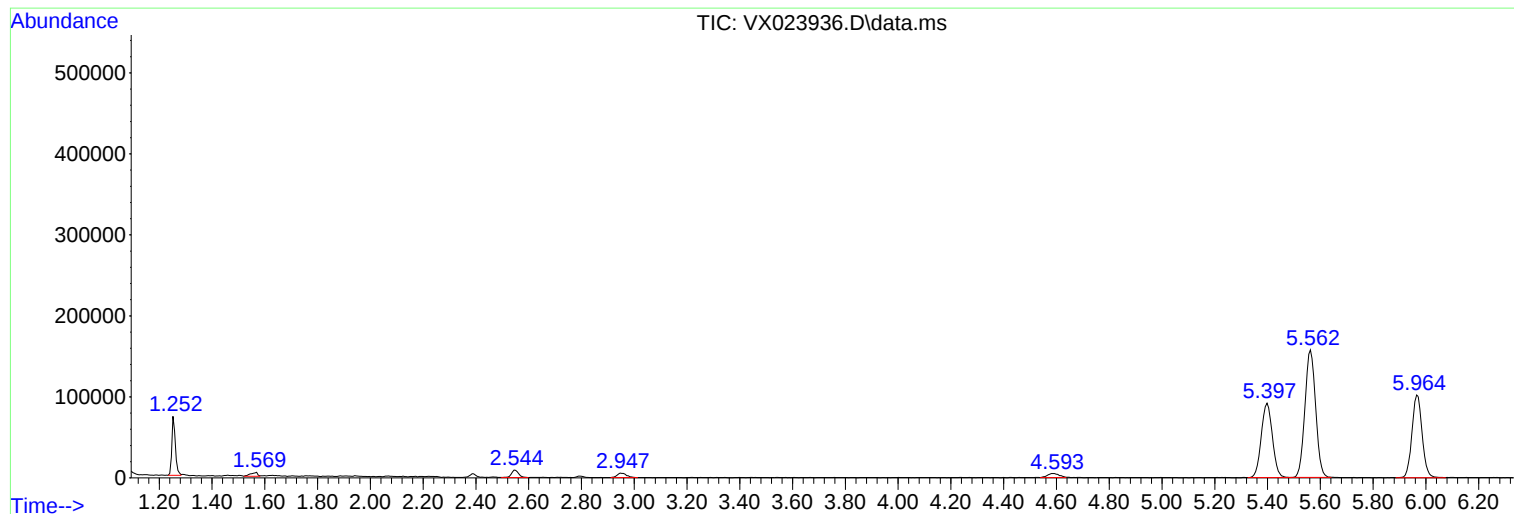

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082521\  
Data File : VX023936.D  
Acq On : 25 Aug 2021 14:20  
Operator : JC/MD  
Sample : M3525-08  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
WVLY-FB-082021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX082521\  
Data File : VX023936.D  
Acq On : 25 Aug 2021 14:20  
Operator : JC/MD  
Sample : M3525-08  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
WVLY-FB-082021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081721W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----