

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
 Data File : VX030772.D
 Acq On : 25 Aug 2022 15:10
 Operator : JC/MD
 Sample : N4245-01DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW17811-20220816DL

Quant Time: Aug 26 02:40:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	243746	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	404686	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	354420	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	162255	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	143103	49.912	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	99.820%		
35) Dibromofluoromethane	5.391	113	125127	50.310	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	100.620%		
50) Toluene-d8	8.653	98	466110	53.781	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	107.560%		
62) 4-Bromofluorobenzene	11.085	95	155819	48.291	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	96.580%		
Target Compounds						Qvalue
3) Chloromethane	1.288	50	586	Below Cal	#	84
4) Vinyl Chloride	1.368	62	132	Below Cal	#	78
5) Bromomethane	1.611	94	561	0.494	ug/l #	80
6) Chloroethane	1.685	64	210	Below Cal	#	41
10) Methyl Iodide	2.459	142	579	4.298	ug/l #	88
11) Tert butyl alcohol	2.947	59	6394	10.273	ug/l #	75
12) 1,1-Dichloroethene	2.319	96	1085	0.491	ug/l #	73
13) Acrolein	2.239	56	131	10.281	ug/l	91
15) Acrylonitrile	3.081	53	313	0.205	ug/l #	79
16) Acetone	2.392	43	1325	1.000	ug/l #	53
17) Carbon Disulfide	2.508	76	1774	Below Cal	#	90
20) Methylene Chloride	2.794	84	4925	1.242	ug/l	91
21) trans-1,2-Dichloroethene	3.099	96	485	0.204	ug/l #	59
25) 2-Butanone	4.587	43	981	0.460	ug/l #	48
27) cis-1,2-Dichloroethene	4.495	96	16153	5.509	ug/l	89
36) 1,1-Dichloropropene	5.550	75	18809	5.554	ug/l #	49
38) Carbon Tetrachloride	5.556	117	24576	6.879	ug/l #	18
44) Trichloroethene	7.129	130	166502	56.877	ug/l	97
45) 1,2-Dichloropropane	7.440	63	10018	3.574	ug/l	98
48) Methyl methacrylate	7.440	41	5355	1.778	ug/l #	37
49) 1,4-Dioxane	7.580	88	20	0.269	ug/l #	25
60) Dibromochloromethane	9.281	129	8261	2.819	ug/l #	11
64) Tetrachloroethene	9.275	164	7645	2.738	ug/l #	80
76) 1,2,3-Trichloropropane	11.085	75	75258	21.171	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	75258	68.306	ug/l #	13
87) 1,3-Dichlorobenzene	11.969	146	1018	0.201	ug/l	92
93) 1,2,4-Trichlorobenzene	13.591	180	1063	0.320	ug/l	93
94) Hexachlorobutadiene	13.725	225	392	0.283	ug/l	95
95) Naphthalene	13.780	128	2886	0.249	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	893	0.254	ug/l	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030772.D
Acq On : 25 Aug 2022 15:10
Operator : JC/MD
Sample : N4245-01DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL

Quant Time: Aug 26 02:40:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 26 02:03:28 2022
Response via : Initial Calibration




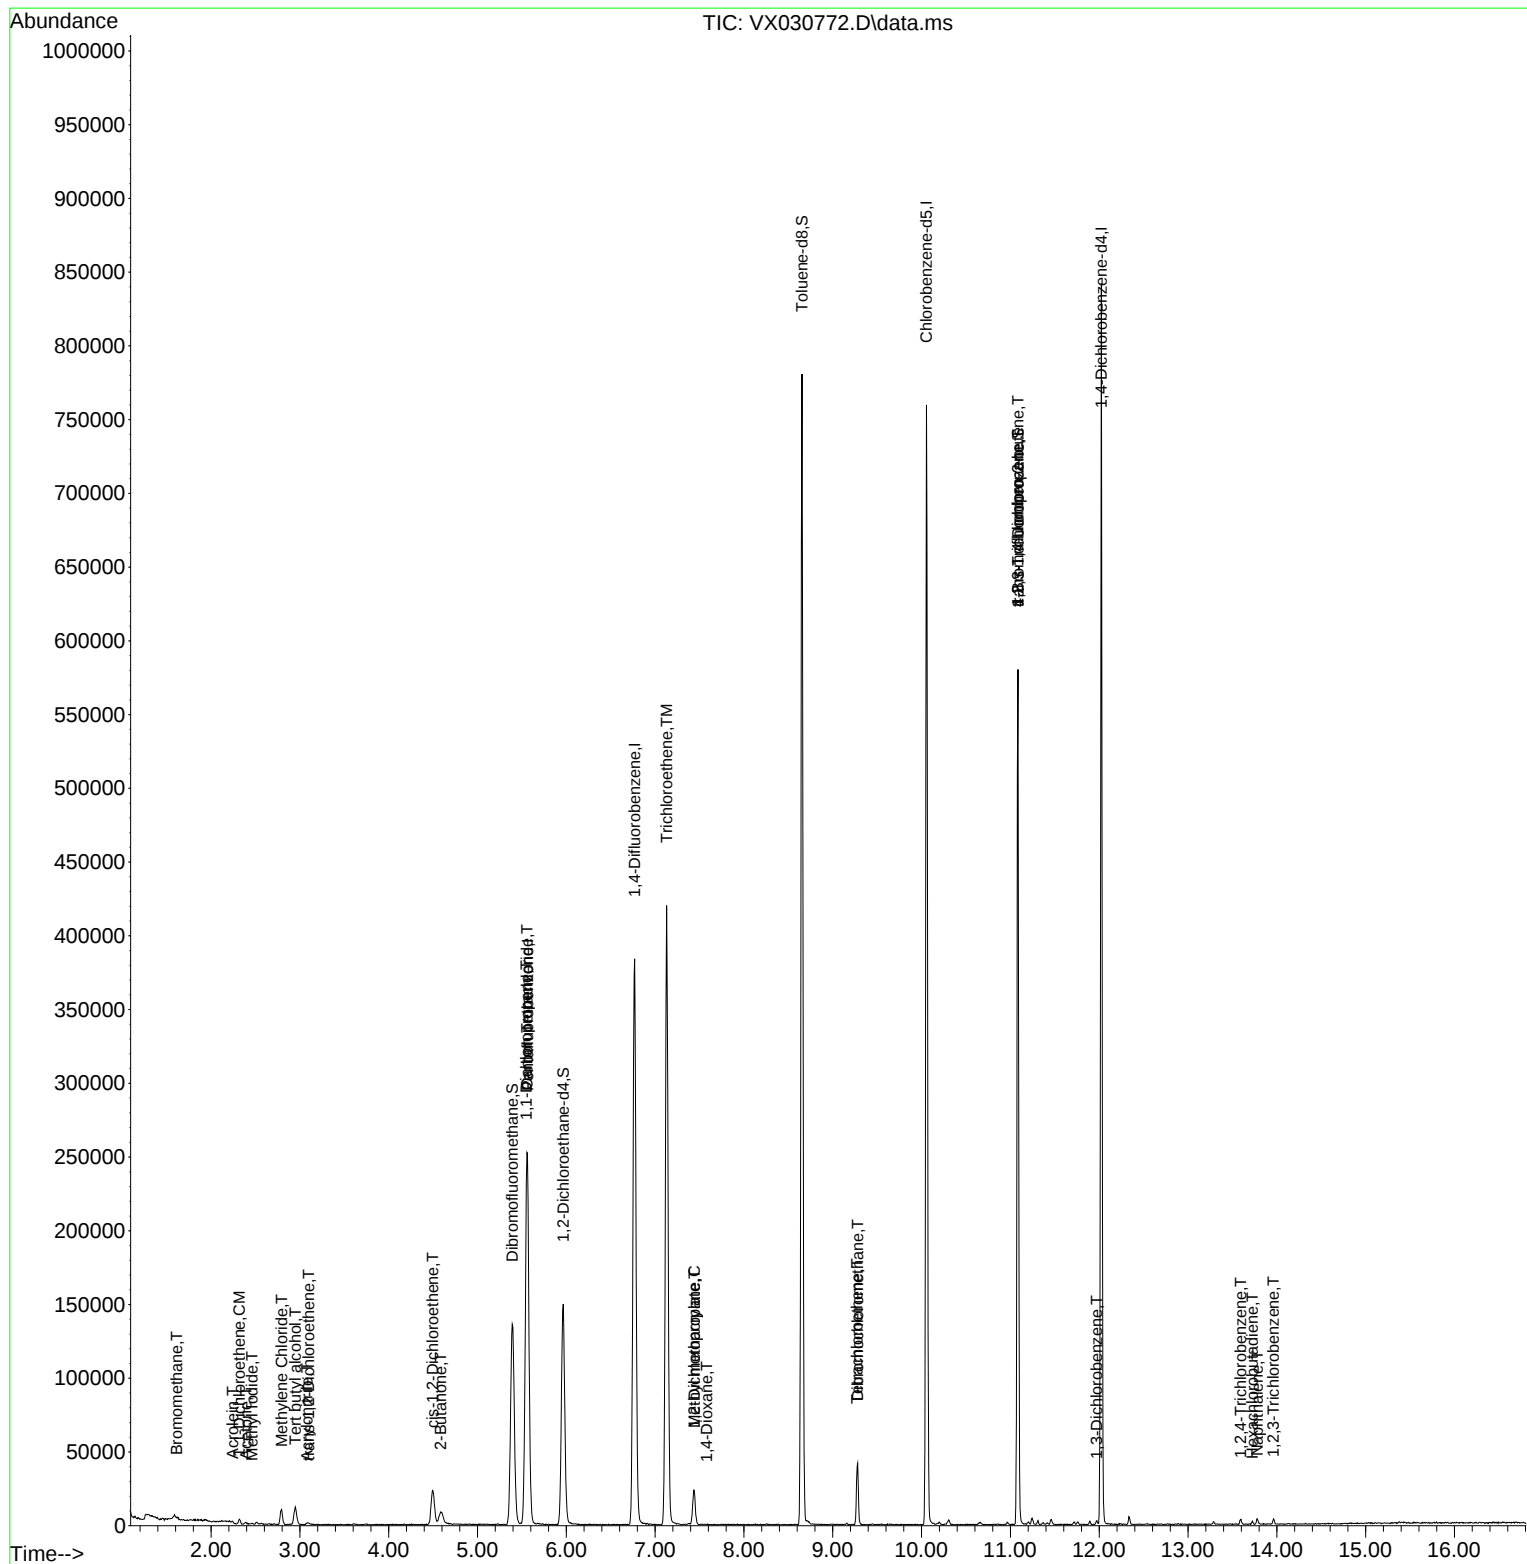




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL


Tgt Ion:168 Resp: 243746
Ion Ratio Lower Upper
168 100
99 56.1 44.0 66.0

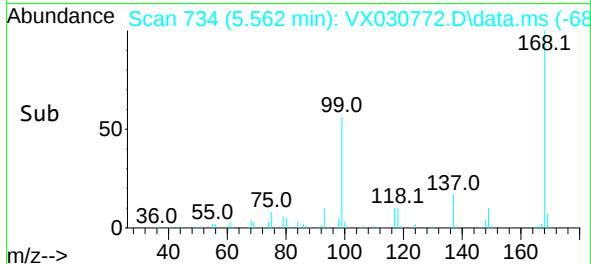

#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. 0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion: 50 Resp: 586
Ion Ratio Lower Upper
50 100
52 23.8 26.3 39.5#


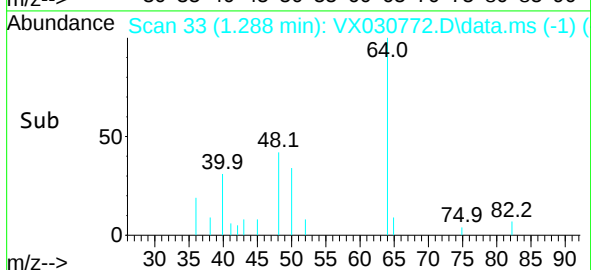

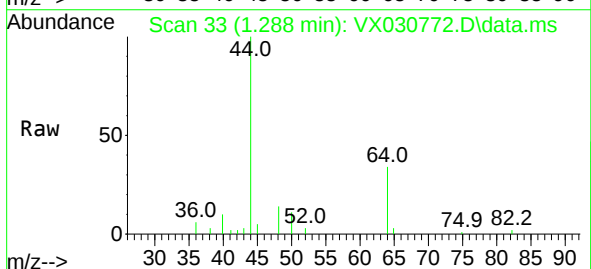


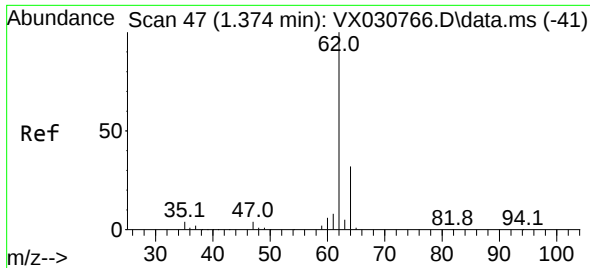

#4
 Vinyl Chloride
 Concen: Below Cal
 RT: 1.368 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VX030772.D
 Acq: 25 Aug 2022 15:10




Instrument :
 MSVOA_X
 ClientSampleId :
 MW17811-20220816DL


Tgt Ion: 62 Resp: 132
 Ion Ratio Lower Upper
 62 100
 64 19.5 25.2 37.8#

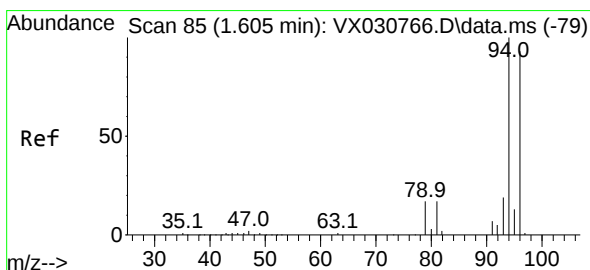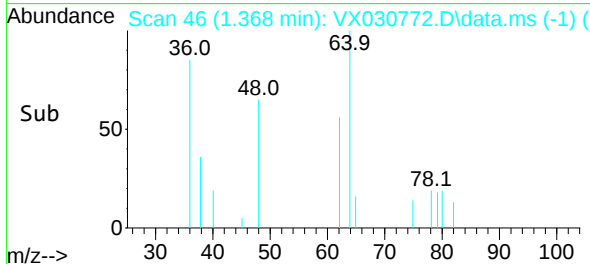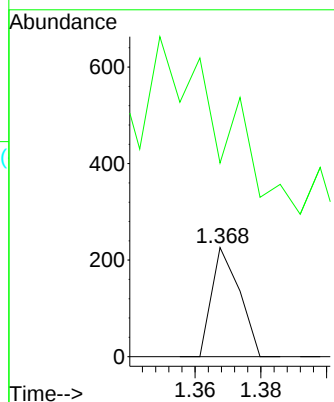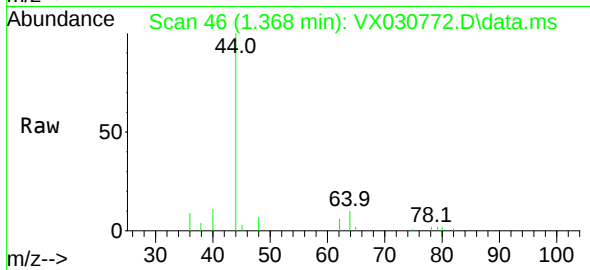

#5
 Bromomethane
 Concen: 0.494 ug/l
 RT: 1.611 min Scan# 86
 Delta R.T. 0.006 min
 Lab File: VX030772.D
 Acq: 25 Aug 2022 15:10

Tgt Ion: 94 Resp: 561
 Ion Ratio Lower Upper
 94 100
 96 76.2 76.9 115.3#


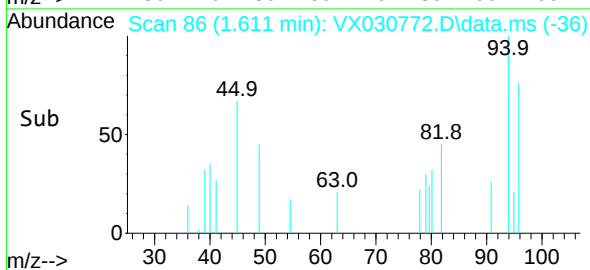
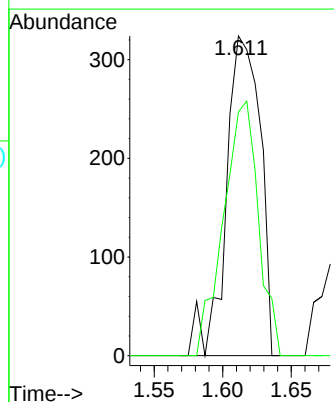
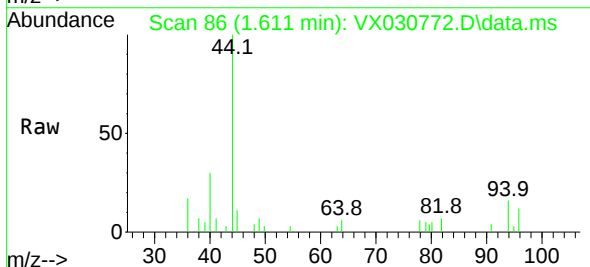


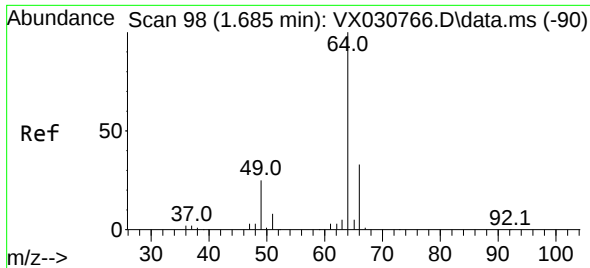

#6
Chloroethane
Concen: Below Cal
RT: 1.685 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL


Tgt Ion: 64 Resp: 210
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

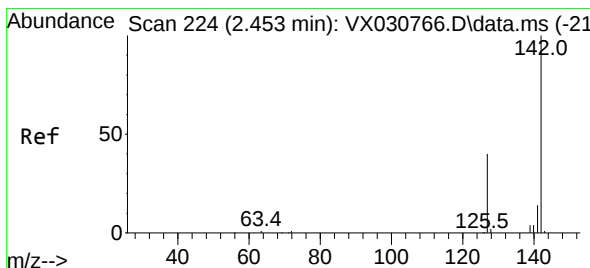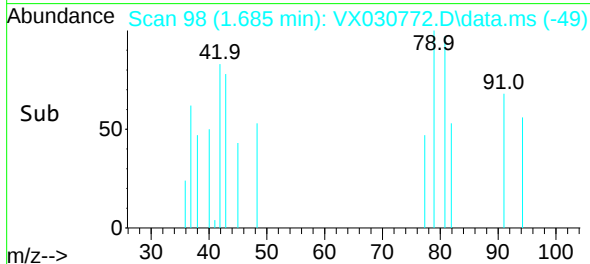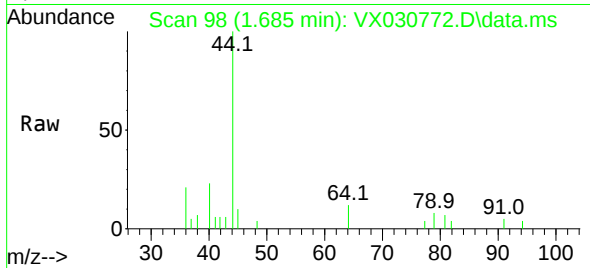

#10
Methyl Iodide
Concen: 4.298 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion: 142 Resp: 579
Ion Ratio Lower Upper
142 100
127 44.4 30.2 45.2
141 7.6 11.3 16.9#


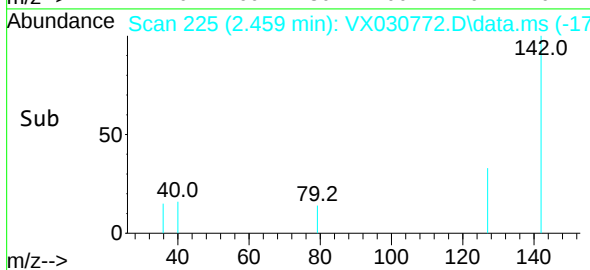

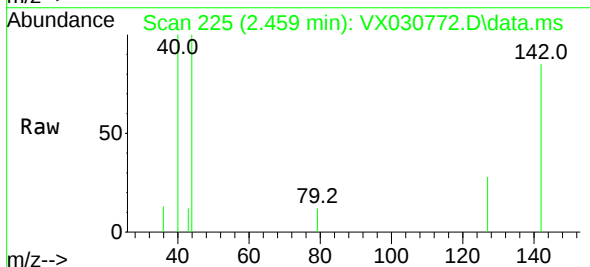


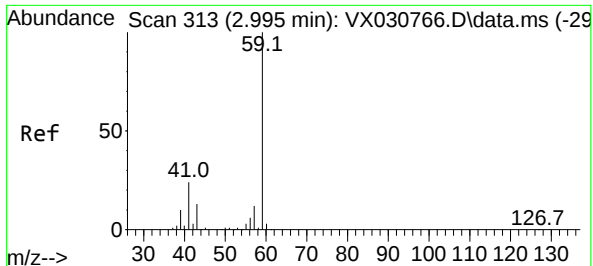

#11
Tert butyl alcohol
Concen: 10.273 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.049 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW178I1-20220816DL


Tgt Ion: 59 Resp: 6394
Ion Ratio Lower Upper
59 100
57 0.3 7.4 11.2#

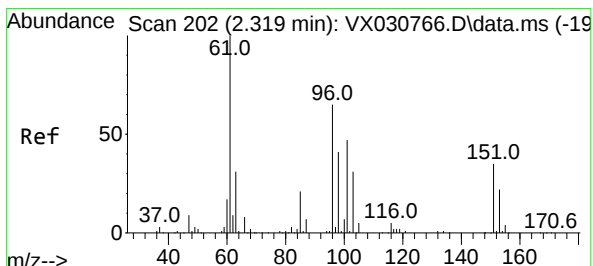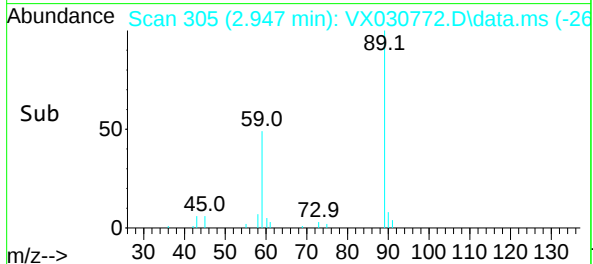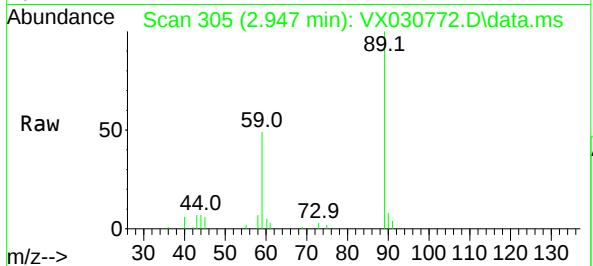

#12
1,1-Dichloroethene
Concen: 0.491 ug/l
RT: 2.319 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion: 96 Resp: 1085
Ion Ratio Lower Upper
96 100
61 168.1 117.4 176.0
98 103.6 52.2 78.4#


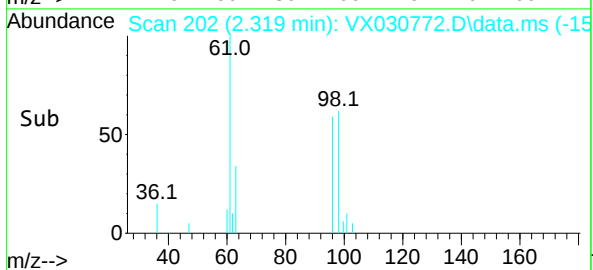

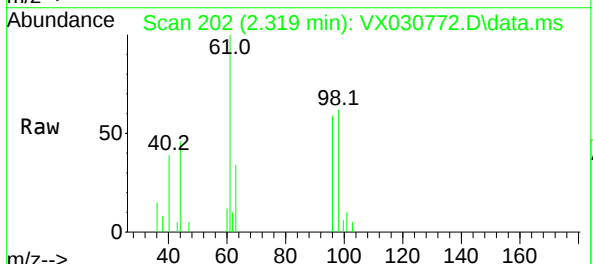




#13
Acrolein
Concen: 10.281 ug/l
RT: 2.239 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL


Tgt Ion: 56 Resp: 131
Ion Ratio Lower Upper
56 100
55 77.9 56.6 84.8

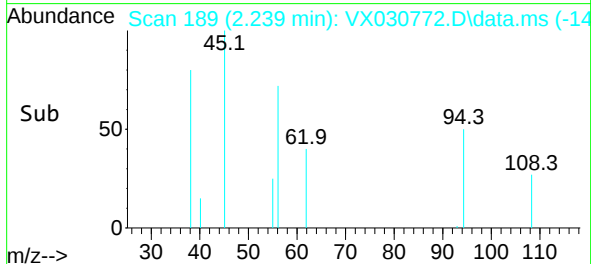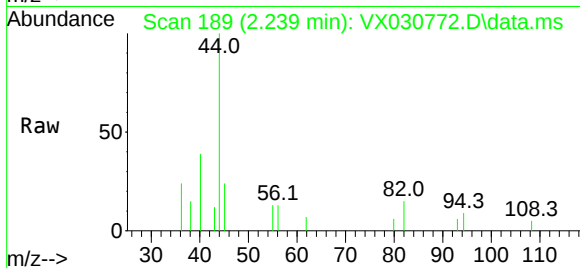

#15
Acrylonitrile
Concen: 0.205 ug/l
RT: 3.081 min Scan# 327
Delta R.T. 0.012 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion: 53 Resp: 313
Ion Ratio Lower Upper
53 100
52 86.3 65.4 98.0
51 0.0 27.7 41.5#

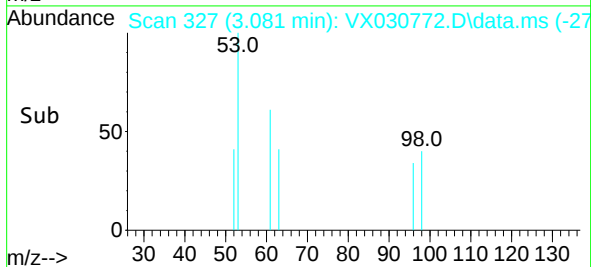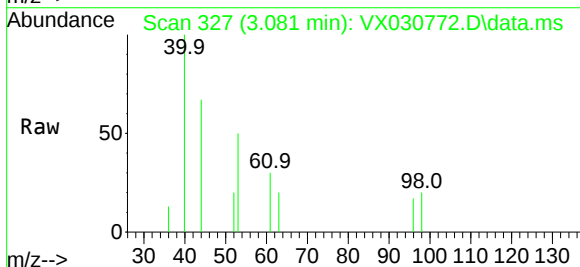

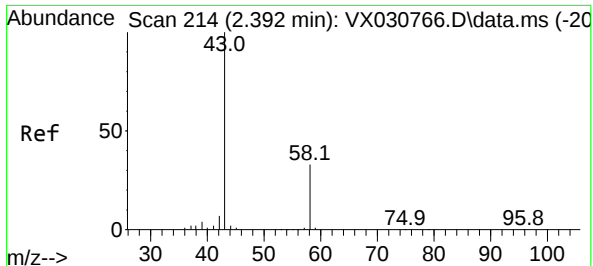

#16

Acetone

Concen: 1.000 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10

Instrument :

MSVOA_X

ClientSampleId :





MW178I1-20220816DL

Tgt Ion: 43 Resp: 1325

Ion Ratio Lower Upper

43 100

58 61.5 27.7 41.5#

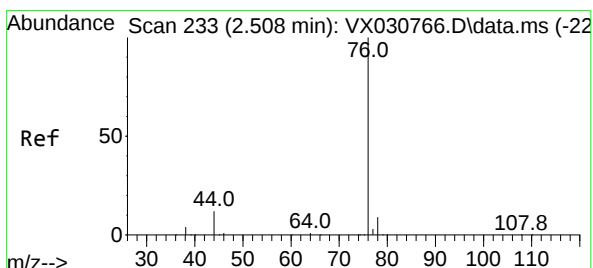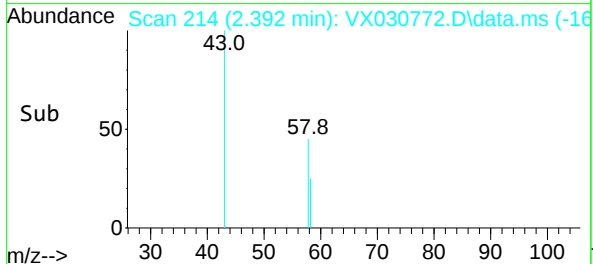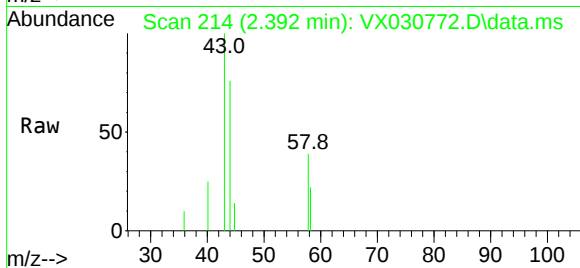

#17

Carbon Disulfide

Concen: Below Cal

RT: 2.508 min Scan# 233

Delta R.T. -0.000 min

Lab File: VX030772.D




Acq: 25 Aug 2022 15:10


Tgt Ion: 76 Resp: 1774

Ion Ratio Lower Upper

76 100

78 6.1 7.8 11.6#


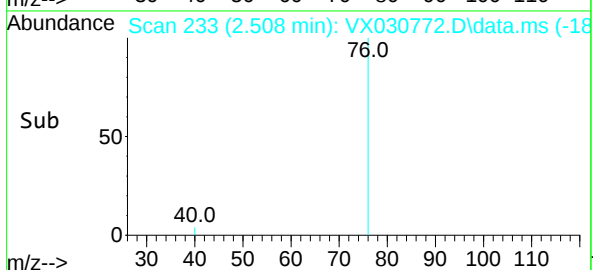

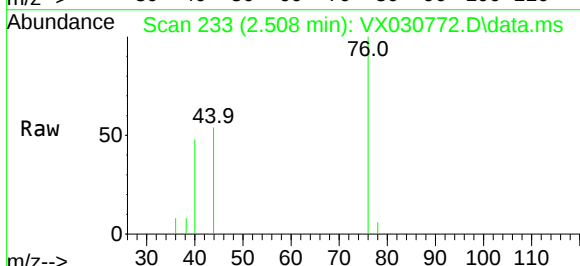




#20
Methylene Chloride
Concen: 1.242 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL


Tgt Ion: 84	Resp: 4925
Ion Ratio	Lower Upper
84 100	
49 109.0	93.8 140.6
51 40.5	29.4 44.0
86 74.8	51.0 76.4

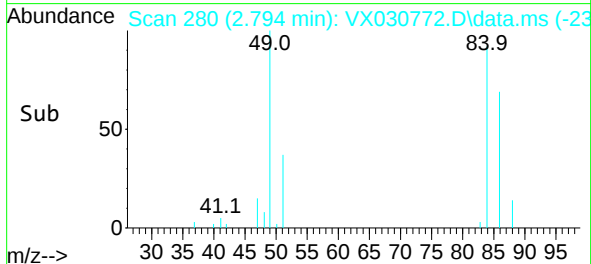

#21
trans-1,2-Dichloroethene
Concen: 0.204 ug/l
RT: 3.099 min Scan# 330
Delta R.T. 0.006 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion: 96	Resp: 485		
Ion Ratio	Lower	Upper	
96 100			
61 68.8	105.6	158.4#	
98 51.3	50.1	75.1	


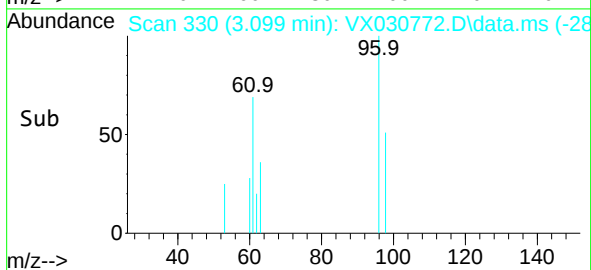

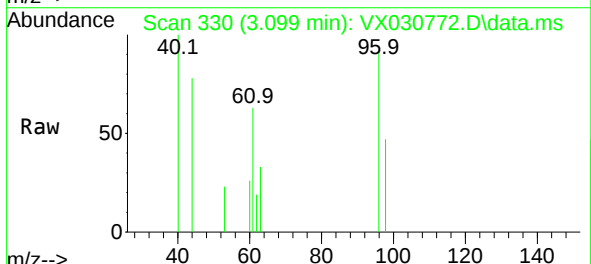




#25
2-Butanone
Concen: 0.460 ug/l
RT: 4.587 min Scan# 51
Delta R.T. 0.019 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL


Tgt Ion: 43 Resp: 981
Ion Ratio Lower Upper
43 100
72 0.0 21.7 32.5#

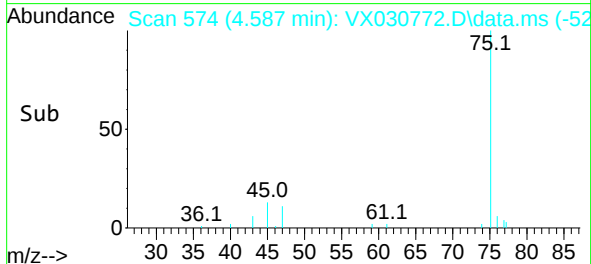

#27
cis-1,2-Dichloroethene
Concen: 5.509 ug/l
RT: 4.495 min Scan# 559
Delta R.T. 0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion: 96 Resp: 16153
Ion Ratio Lower Upper
96 100
61 118.2 0.0 270.0
98 60.3 0.0 127.8

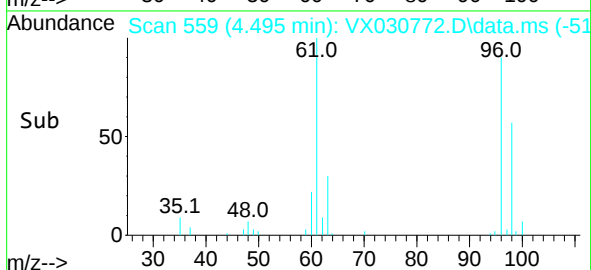

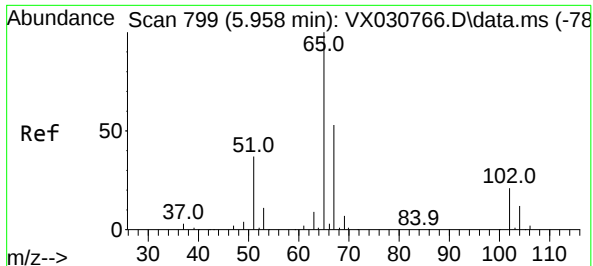

#33

1,2-Dichloroethane-d4

Concen: 49.912 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10

Instrument :

MSVOA_X

ClientSampleId :





MW17811-20220816DL

Tgt Ion: 65 Resp: 143103

Ion Ratio Lower Upper

65 100

67 54.6 0.0 109.6

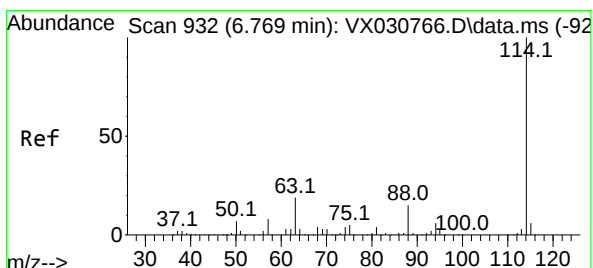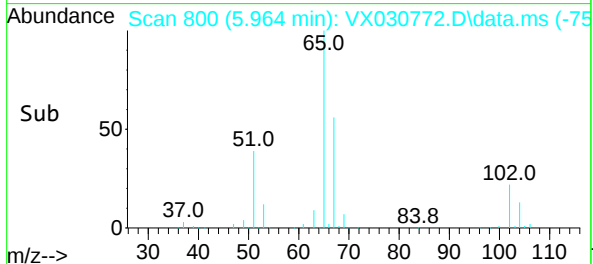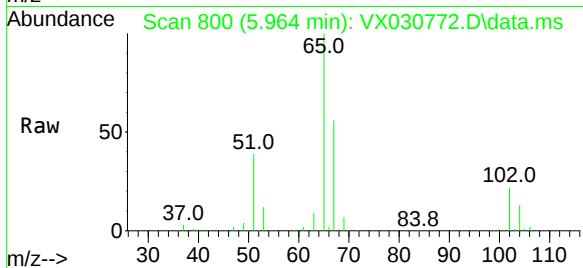

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10




Tgt Ion: 114 Resp: 404686


Ion Ratio Lower Upper

114 100

63 22.2 0.0 38.4

88 17.2 0.0 31.8


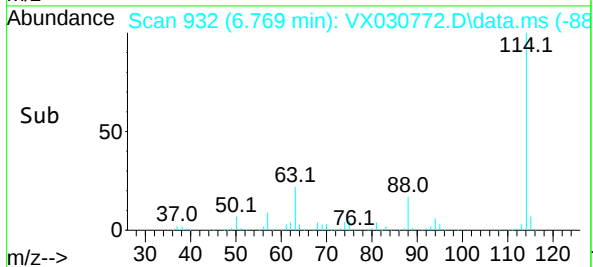

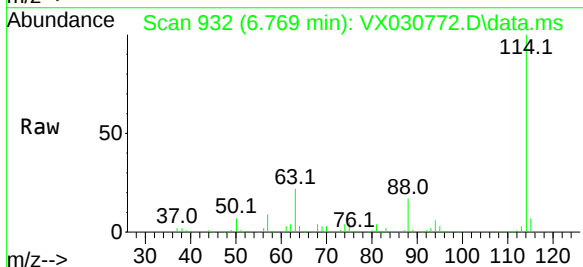


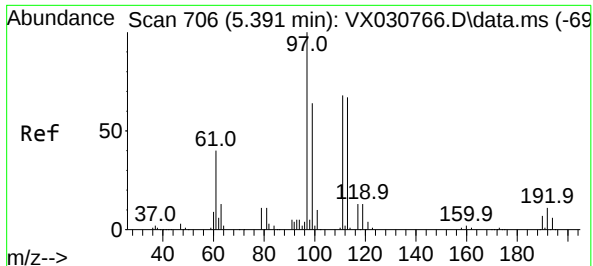

#35
Dibromofluoromethane
Concen: 50.310 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW178I1-20220816DL


Tgt Ion:113 Resp: 125127
Ion Ratio Lower Upper
113 100
111 102.5 83.2 124.8
192 18.7 14.8 22.2

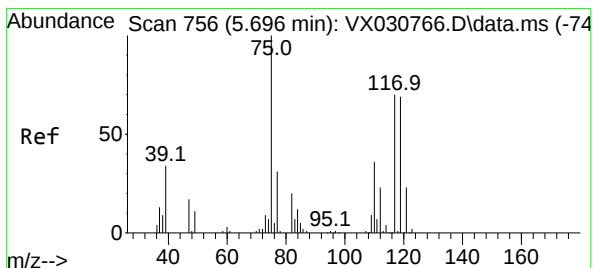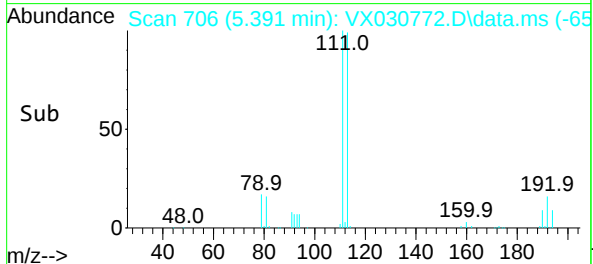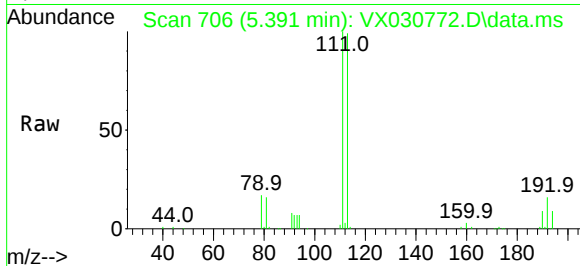

#36
1,1-Dichloropropene
Concen: 5.554 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.146 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10


Tgt Ion: 75 Resp: 18809
Ion Ratio Lower Upper
75 100
110 9.8 19.3 57.9#
77 0.0 24.4 36.6#

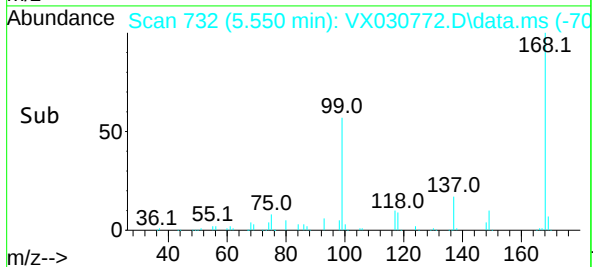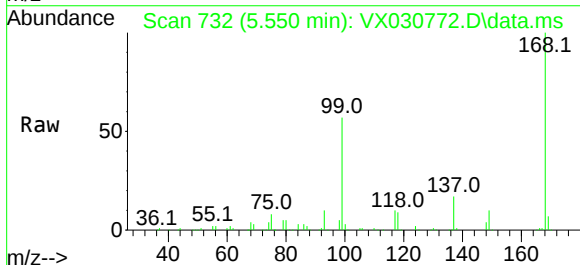






#38
Carbon Tetrachloride
Concen: 6.879 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.122 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL







Tgt Ion:117 Resp: 24576
Ion Ratio Lower Upper
117 100
119 6.6 74.1 111.1#
121 0.0 25.8 38.8#

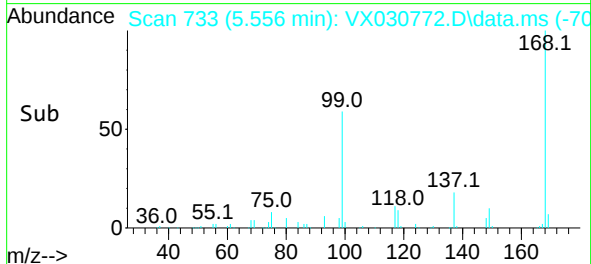

#44
Trichloroethene
Concen: 56.877 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion:130 Resp: 166502
Ion Ratio Lower Upper
130 100
95 94.5 0.0 194.8

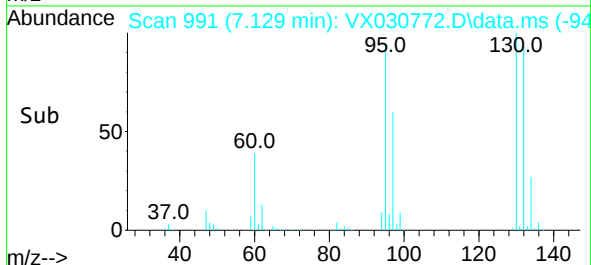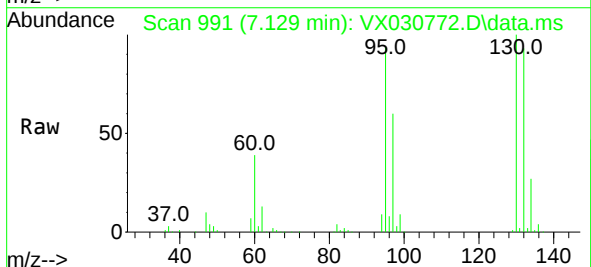

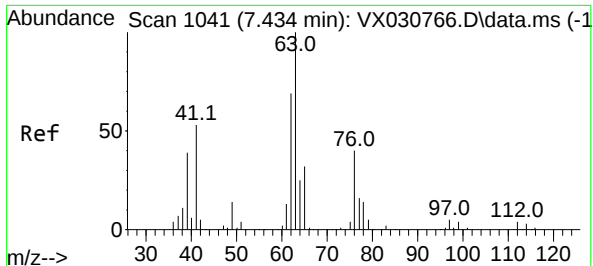

#45

1,2-Dichloropropane

Concen: 3.574 ug/l

RT: 7.440 min Scan# 1042

Delta R.T. 0.006 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10

Instrument :

MSVOA_X

ClientSampleId :





MW17811-20220816DL

Tgt Ion: 63 Resp: 10018

Ion Ratio Lower Upper

63 100

65 30.2 25.2 37.8

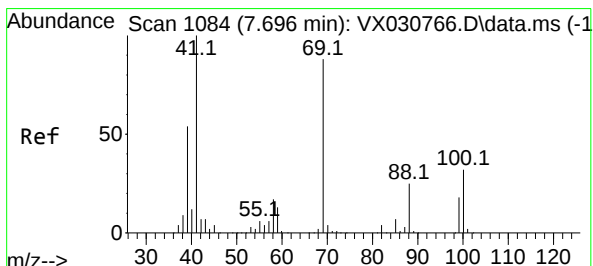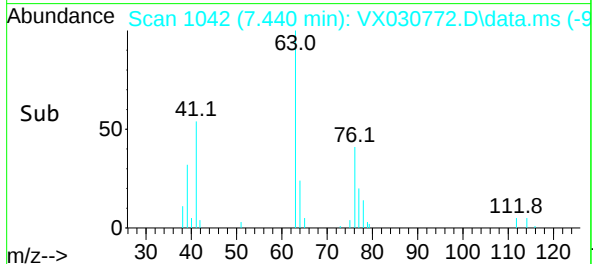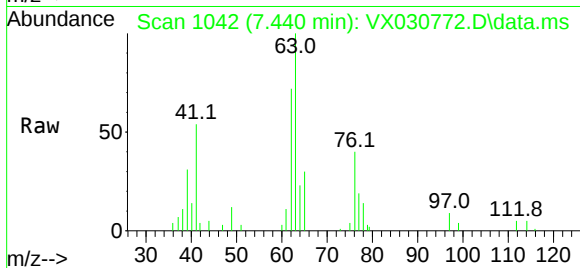

#48

Methyl methacrylate

Concen: 1.778 ug/l

RT: 7.440 min Scan# 1042

Delta R.T. -0.256 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10




Tgt Ion: 41 Resp: 5355


Ion Ratio Lower Upper

41 100

69 0.0 68.8 103.2#

39 67.1 44.6 66.8#

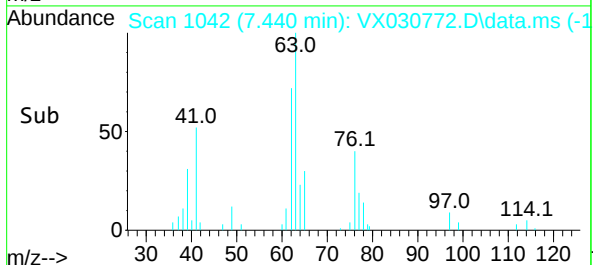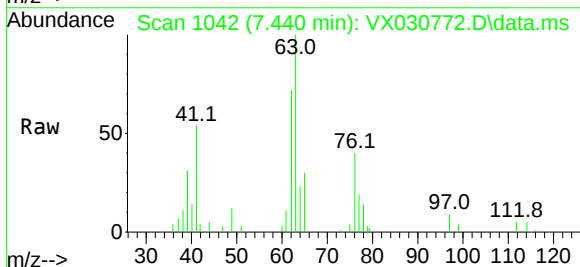



#49

1,4-Dioxane

Concen: 0.269 ug/l

RT: 7.580 min Scan# 1065

Delta R.T. -0.098 min

Lab File: VX030772.D


Acq: 25 Aug 2022 15:10

Instrument :




MSVOA_X

ClientSampleId :

MW178I1-20220816DL



Tgt Ion:	88	Resp:	20
Ion	Ratio	Lower	Upper
88	100		
43	0.0	23.8	35.8#
58	0.0	53.8	80.6#



#50

Toluene-d8

Concen: 53.781 ug/l




RT: 8.653 min Scan# 1241


Delta R.T. -0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10

Tgt Ion:	98	Resp:	466110
Ion	Ratio	Lower	Upper
98	100		
100	64.5	52.3	78.5


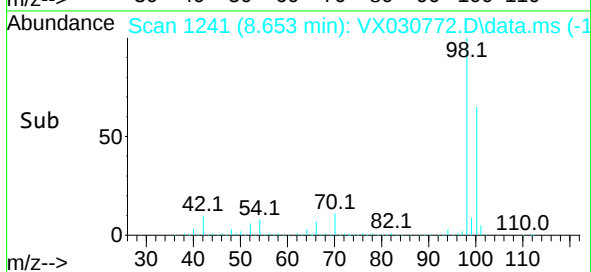






#60
 Dibromochloromethane
 Concen: 2.819 ug/l
 RT: 9.281 min Scan# 11
 Delta R.T. -0.244 min
 Lab File: VX030772.D
 Acq: 25 Aug 2022 15:10




Instrument :
 MSVOA_X
 ClientSampleId :
 MW178I1-20220816DL


Tgt Ion:129 Resp: 8261
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.5 115.5#

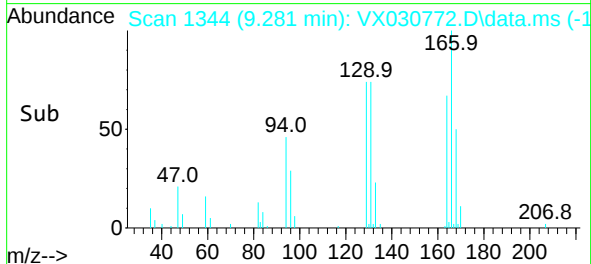

#62
 4-Bromofluorobenzene
 Concen: 48.291 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. 0.000 min
 Lab File: VX030772.D
 Acq: 25 Aug 2022 15:10

Tgt Ion: 95 Resp: 155819
 Ion Ratio Lower Upper
 95 100
 174 79.0 0.0 149.0
 176 76.6 0.0 146.0




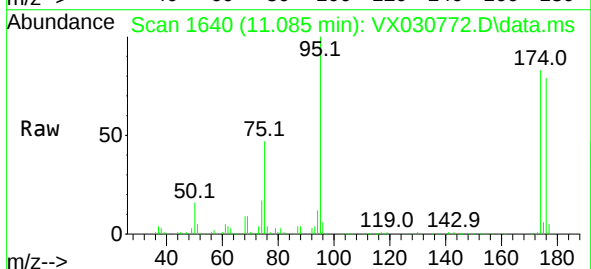




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL


Tgt Ion:117 Resp: 354420
Ion Ratio Lower Upper
117 100
82 57.0 42.7 64.1
119 31.7 25.4 38.2

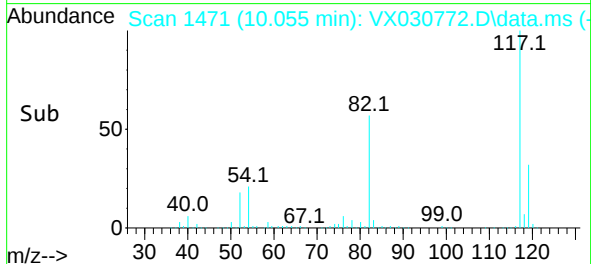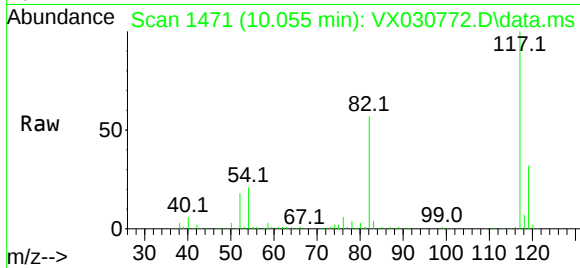

#64
Tetrachloroethene
Concen: 2.738 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion:164 Resp: 7645
Ion Ratio Lower Upper
164 100
166 149.3 98.2 147.4#
129 105.2 80.8 121.2
131 126.1 75.5 113.3#

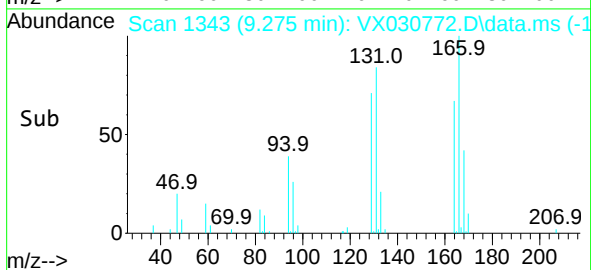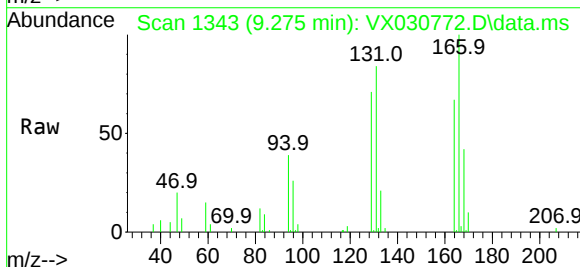



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10

Instrument :

MSVOA_X

ClientSampleId :

MW17811-20220816DL





Tgt Ion:152 Resp: 162255

Ion Ratio Lower Upper

152 100

115 58.9 40.5 121.5

150 157.9 0.0 347.0

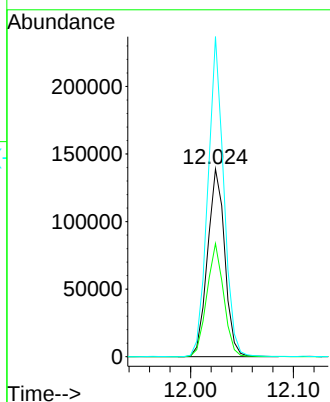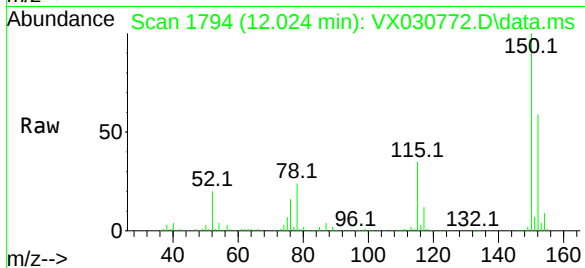

#76

1,2,3-Trichloropropane

Concen: 21.171 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.159 min

Lab File: VX030772.D




Acq: 25 Aug 2022 15:10


Tgt Ion: 75 Resp: 75258

Ion Ratio Lower Upper

75 100

77 1.5 19.8 59.3#


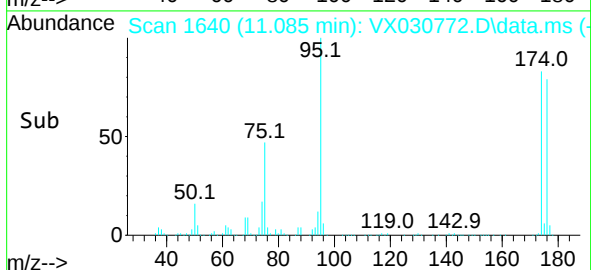
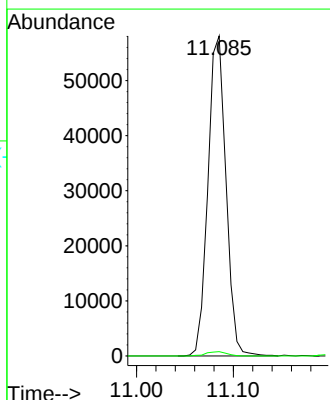
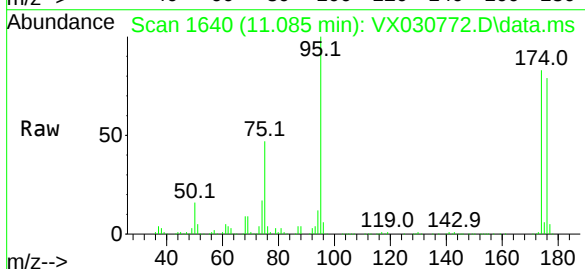




#81
trans-1,4-Dichloro-2-butene
Concen: 68.306 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.067 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10




Instrument :
MSVOA_X
ClientSampleId :
MW17811-20220816DL


Tgt Ion: 75 Resp: 75258
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.8 52.2#

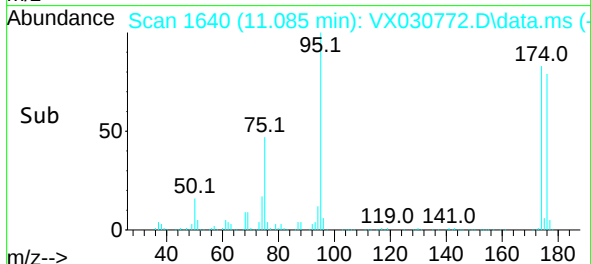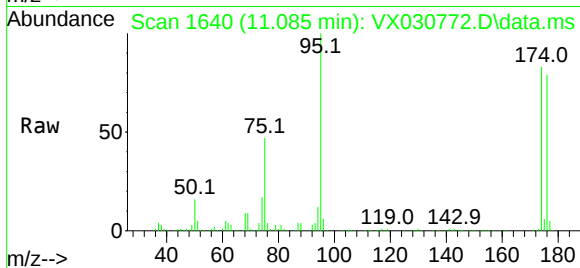

#87
1,3-Dichlorobenzene
Concen: 0.201 ug/l
RT: 11.969 min Scan# 1785
Delta R.T. 0.000 min
Lab File: VX030772.D
Acq: 25 Aug 2022 15:10

Tgt Ion:146 Resp: 1018
Ion Ratio Lower Upper
146 100
111 41.5 20.3 60.8
148 73.5 31.8 95.3

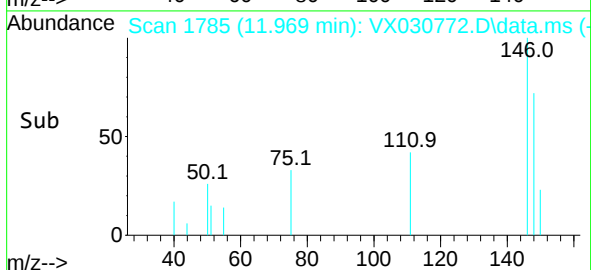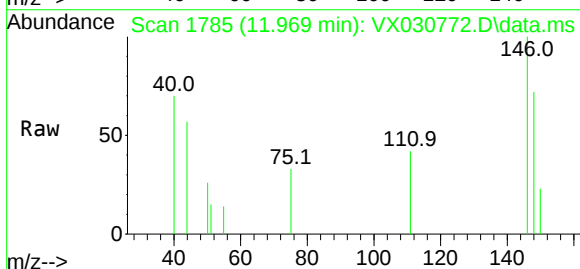

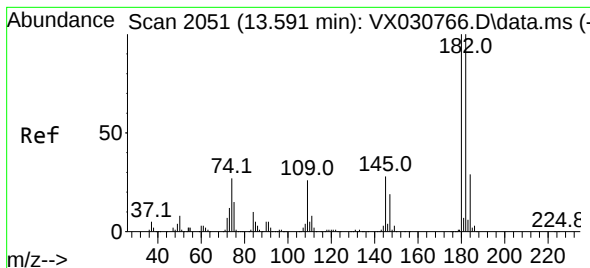

#93

1,2,4-Trichlorobenzene

Concen: 0.320 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. -0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10





Instrument :

MSVOA_X

ClientSampleId :

MW17811-20220816DL

Tgt Ion:180	Resp:	1063
Ion Ratio	Lower	Upper
180	100	
182	99.2	48.2 144.6
145	43.0	15.9 47.6

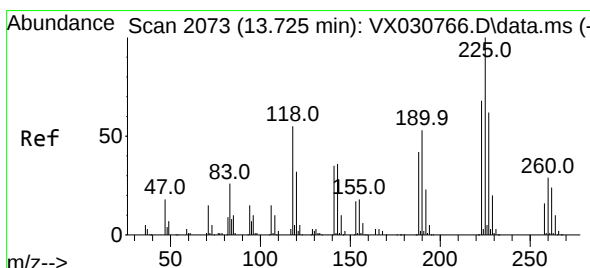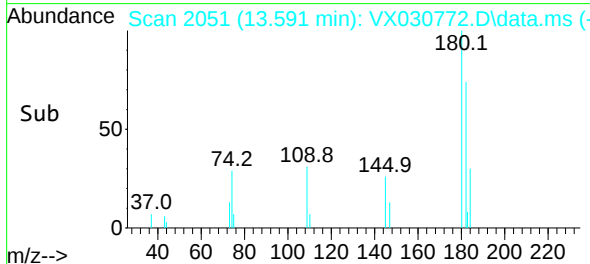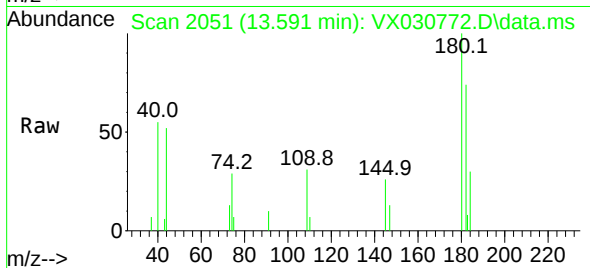

#94

Hexachlorobutadiene

Concen: 0.283 ug/l




RT: 13.725 min Scan# 2073


Delta R.T. 0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10

Tgt Ion:225	Resp:	392
Ion Ratio	Lower	Upper
225	100	
223	64.0	30.6 91.6
227	58.9	31.9 95.9

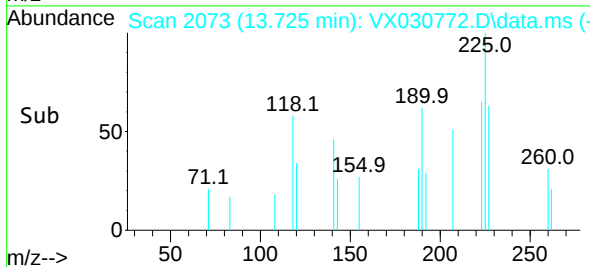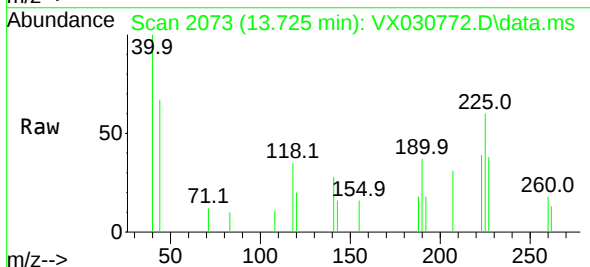

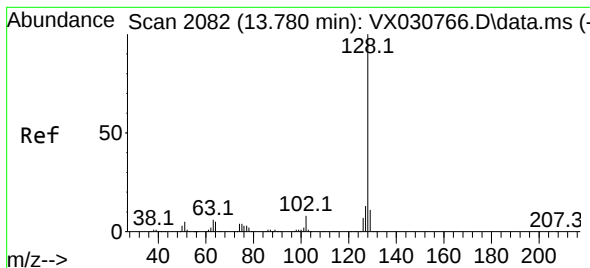

#95

Naphthalene

Concen: 0.249 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. -0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10





Instrument :

MSVOA_X

ClientSampleId :

MW17811-20220816DL

Tgt Ion:	128	Resp:	2886
Ion	Ratio	Lower	Upper
128	100		
127	12.9	10.2	15.2
129	9.9	8.6	13.0

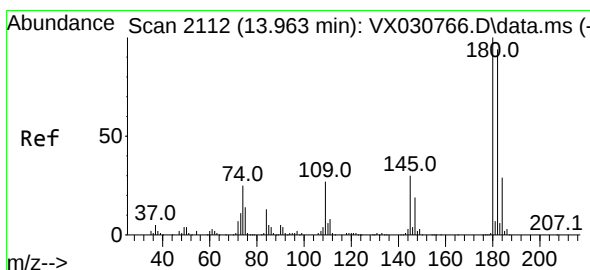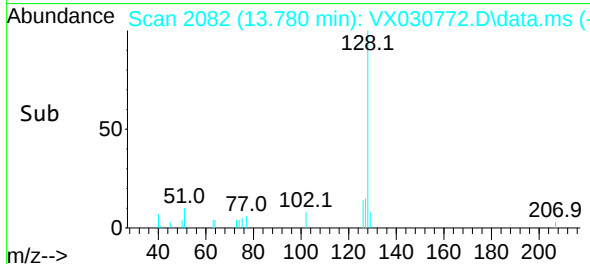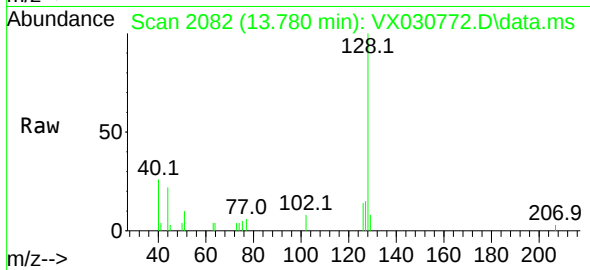

#96

1,2,3-Trichlorobenzene

Concen: 0.254 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX030772.D

Acq: 25 Aug 2022 15:10

Tgt Ion:	180	Resp:	893
Ion	Ratio	Lower	Upper
180	100		
182	126.4	47.0	141.0
145	49.8	17.0	50.9

