

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
 Data File : VX030787.D
 Acq On : 25 Aug 2022 21:54
 Operator : JC/MD
 Sample : VX0825WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0825WBL02

Quant Time: Aug 26 02:42:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	233655	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	385357	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	343269	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	147307	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	138125	50.256	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	= 100.520%		
35) Dibromofluoromethane	5.391	113	118886	50.198	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	= 100.400%		
50) Toluene-d8	8.653	98	444988	53.919	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	= 107.840%		
62) 4-Bromofluorobenzene	11.085	95	149336	48.603	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery	= 97.200%		
Target Compounds						Qvalue
3) Chloromethane	1.288	50	471	Below Cal		98
4) Vinyl Chloride	1.374	62	290	Below Cal	#	74
5) Bromomethane	1.611	94	657	0.603	ug/l	92
6) Chloroethane	1.685	64	114	Below Cal	#	41
10) Methyl Iodide	2.459	142	782	4.408	ug/l	# 75
11) Tert butyl alcohol	2.947	59	1586	2.658	ug/l	# 74
13) Acrolein	2.245	56	323	10.639	ug/l	95
15) Acrylonitrile	3.087	53	682	0.466	ug/l	# 83
16) Acetone	2.386	43	726	0.572	ug/l	# 73
17) Carbon Disulfide	2.514	76	2692	Below Cal	#	88
21) trans-1,2-Dichloroethene	3.099	96	546	0.240	ug/l	# 88
23) Vinyl Acetate	3.751	43	1288	0.204	ug/l	# 72
25) 2-Butanone	4.586	43	550	0.269	ug/l	# 48
29) Tetrahydrofuran	5.044	42	386	0.289	ug/l	# 43
38) Carbon Tetrachloride	5.562	117	24047	7.069	ug/l	# 18
44) Trichloroethene	7.129	130	805	0.289	ug/l	72
60) Dibromochloromethane	9.275	129	664	0.238	ug/l	# 11
68) m/p-Xylenes	10.311	106	1178	0.268	ug/l	99
76) 1,2,3-Trichloropropane	11.085	75	71250	22.077	ug/l	# 38
81) trans-1,4-Dichloro-2-b...	11.085	75	71250	71.231	ug/l	# 13
82) 4-Chlorotoluene	11.457	91	1940	0.249	ug/l	83
85) sec-Butylbenzene	11.896	105	2158	0.208	ug/l	92
86) p-Isopropyltoluene	12.012	119	1828	0.215	ug/l	# 72
87) 1,3-Dichlorobenzene	11.975	146	1599	0.348	ug/l	86
88) 1,4-Dichlorobenzene	11.975	146	1599	0.340	ug/l	85
89) n-Butylbenzene	12.335	91	2072	0.263	ug/l	95
91) 1,2-Dichlorobenzene	12.341	146	1282	0.265	ug/l	94
93) 1,2,4-Trichlorobenzene	13.591	180	1639	0.543	ug/l	95
94) Hexachlorobutadiene	13.725	225	749	0.595	ug/l	88
95) Naphthalene	13.780	128	4543	0.432	ug/l	96
96) 1,2,3-Trichlorobenzene	13.963	180	1526	0.478	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030787.D
Acq On : 25 Aug 2022 21:54
Operator : JC/MD
Sample : VX0825WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02

Quant Time: Aug 26 02:42:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 26 02:03:28 2022
Response via : Initial Calibration




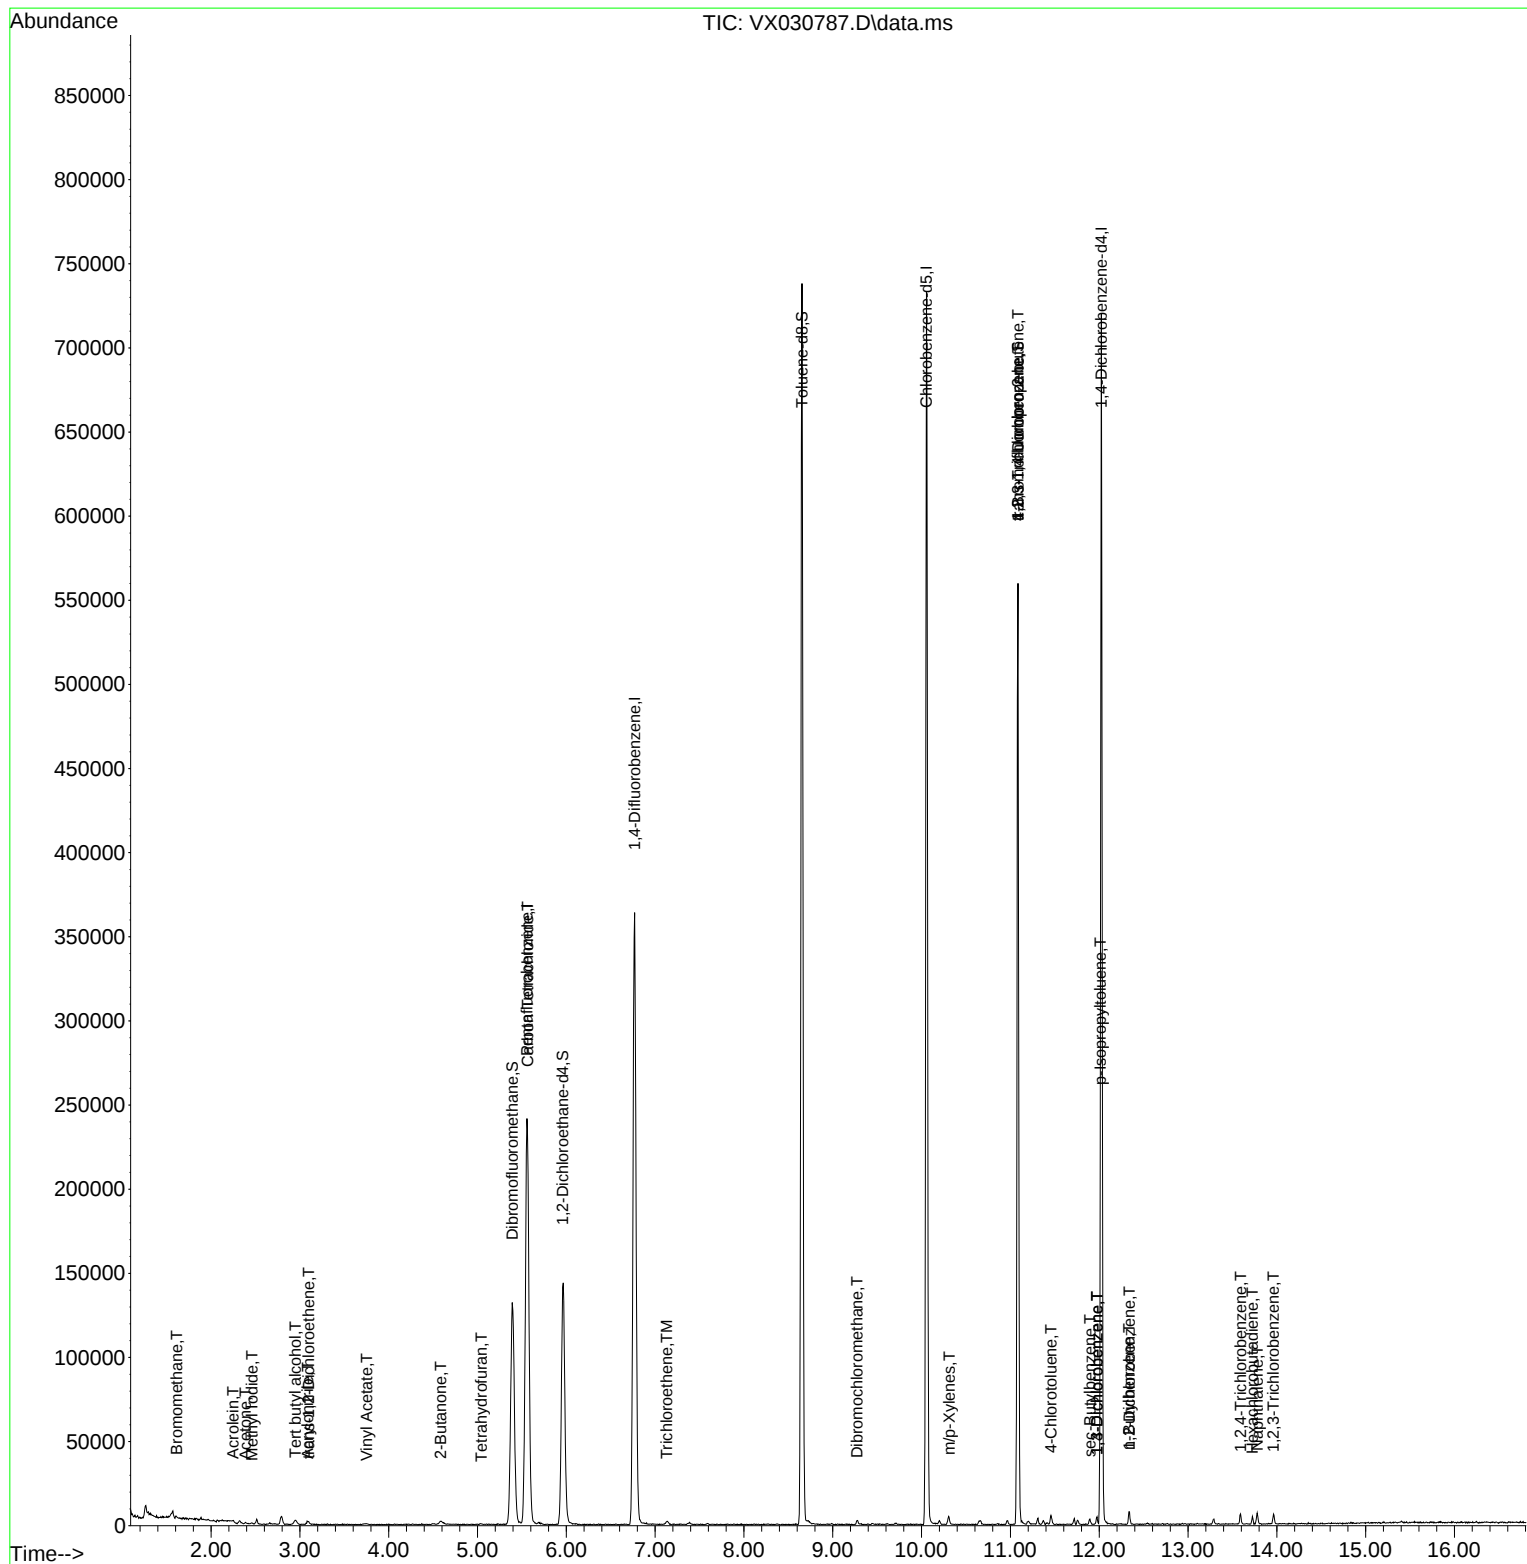




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion:168 Resp: 233655
Ion Ratio Lower Upper
168 100
99 55.6 44.0 66.0

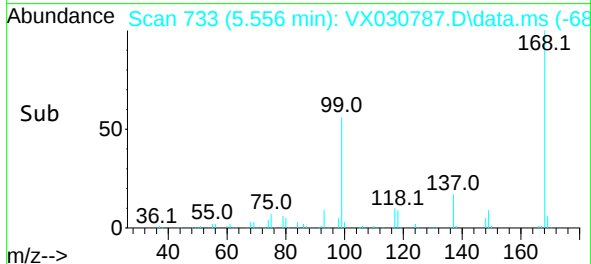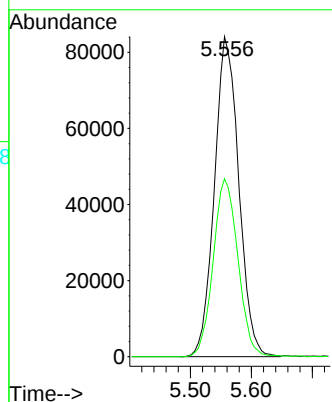

#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. 0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 50 Resp: 471
Ion Ratio Lower Upper
50 100
52 34.3 26.3 39.5


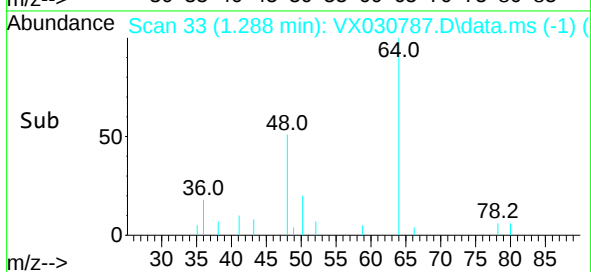
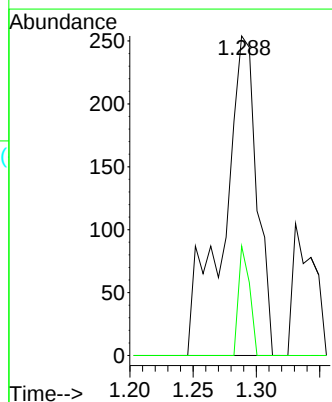



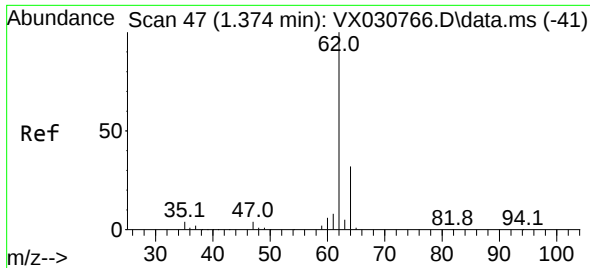

#4
 Vinyl Chloride
 Concen: Below Cal
 RT: 1.374 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VX030787.D
 Acq: 25 Aug 2022 21:54




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0825WBL02


Tgt Ion: 62 Resp: 290
 Ion Ratio Lower Upper
 62 100
 64 45.7 25.2 37.8#

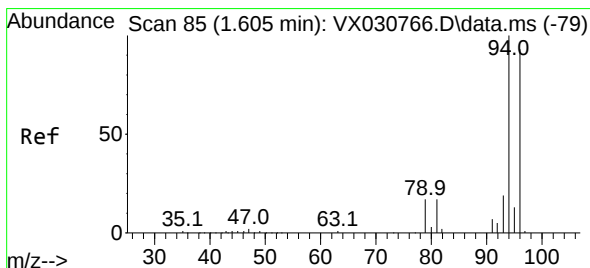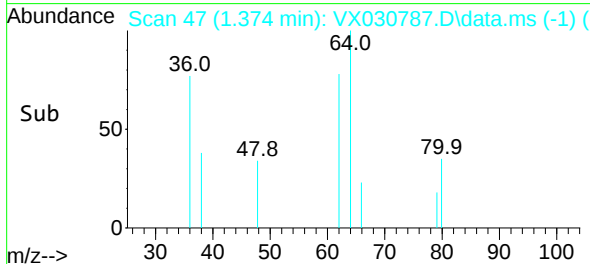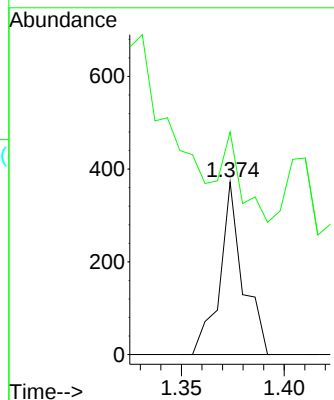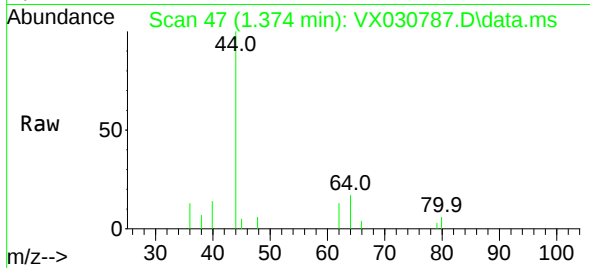

#5
 Bromomethane
 Concen: 0.603 ug/l
 RT: 1.611 min Scan# 86
 Delta R.T. 0.006 min
 Lab File: VX030787.D
 Acq: 25 Aug 2022 21:54

Tgt Ion: 94 Resp: 657
 Ion Ratio Lower Upper
 94 100
 96 103.9 76.9 115.3


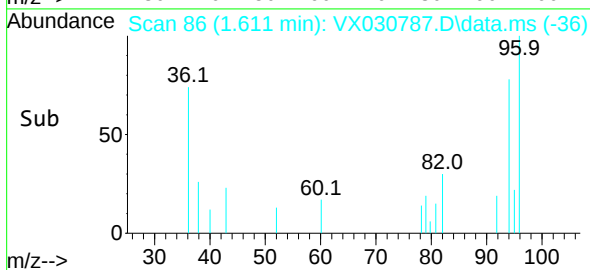
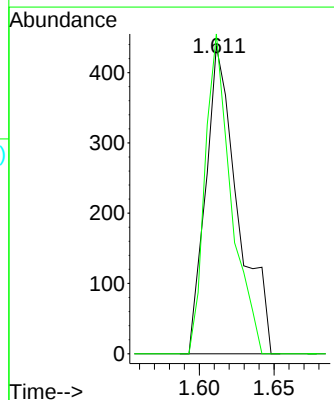
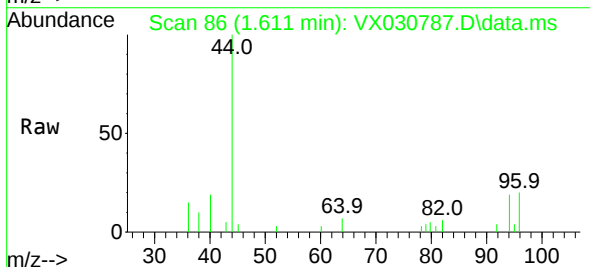


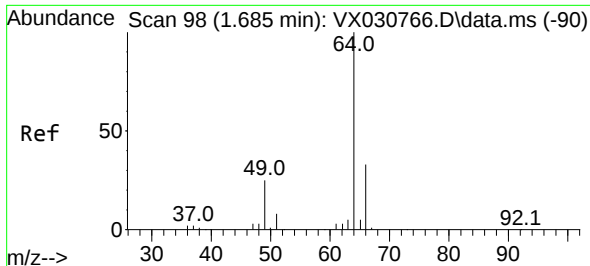

#6
Chloroethane
Concen: Below Cal
RT: 1.685 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion: 64 Resp: 114
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

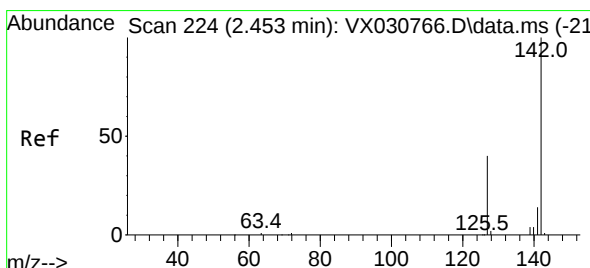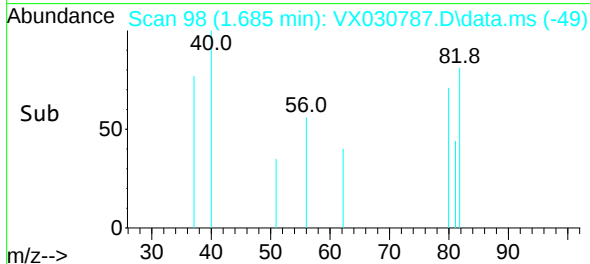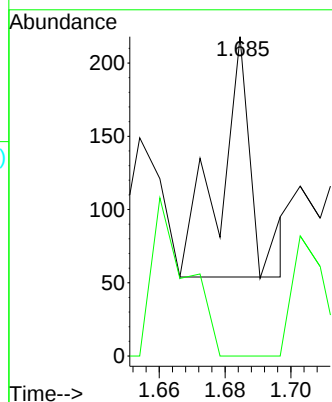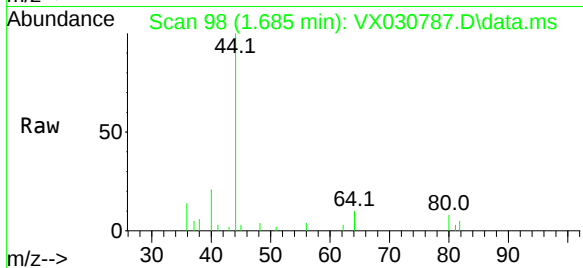

#10
Methyl Iodide
Concen: 4.408 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 142 Resp: 782
Ion Ratio Lower Upper
142 100
127 25.1 30.2 45.2#
141 0.0 11.3 16.9#

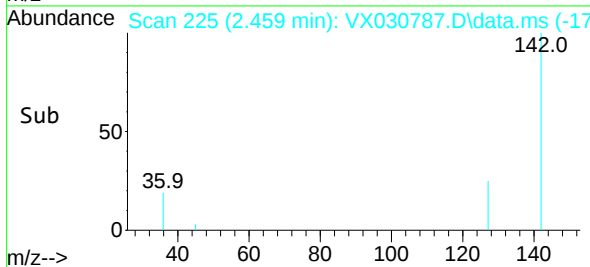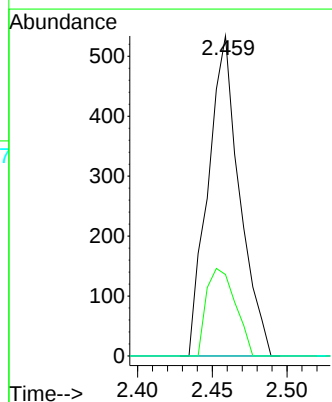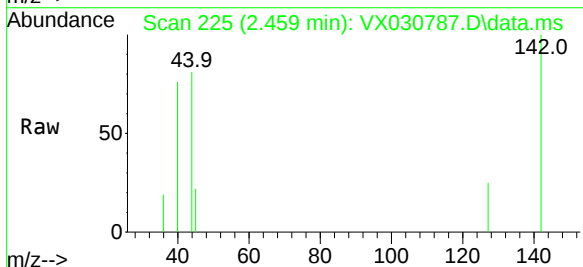

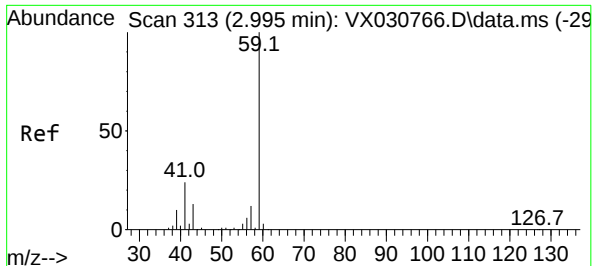

#11

Tert butyl alcohol

Concen: 2.658 ug/l

RT: 2.947 min Scan# 305

Delta R.T. -0.049 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54

Instrument :

MSVOA_X

ClientSampleId :





VX0825WBL02

Tgt Ion: 59 Resp: 1586

Ion Ratio Lower Upper

59 100

57 0.0 7.4 11.2#

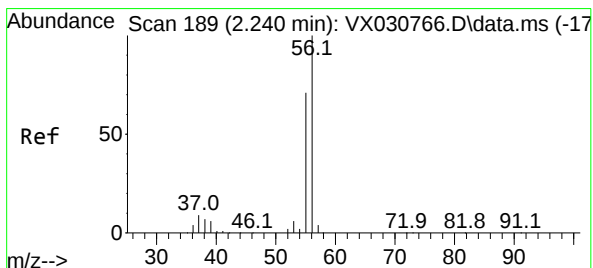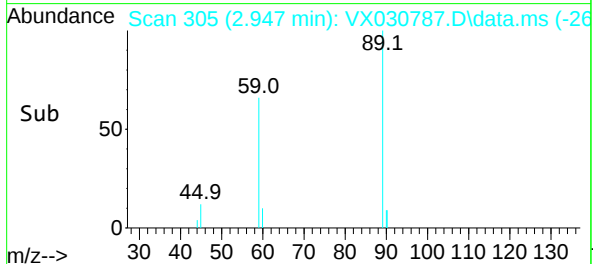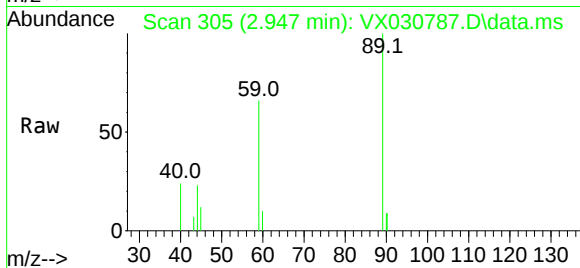

#13

Acrolein

Concen: 10.639 ug/l

RT: 2.245 min Scan# 190

Delta R.T. 0.005 min

Lab File: VX030787.D




Acq: 25 Aug 2022 21:54


Tgt Ion: 56 Resp: 323

Ion Ratio Lower Upper

56 100

55 66.3 56.6 84.8


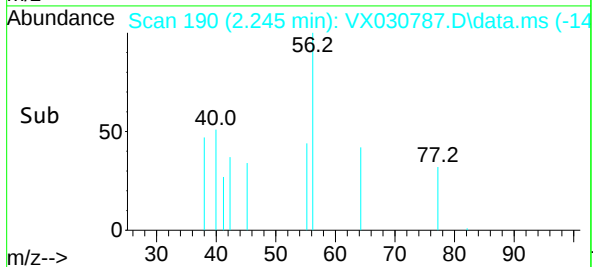

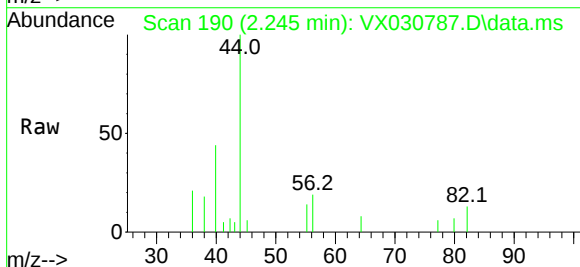




#15
Acrylonitrile
Concen: 0.466 ug/l
RT: 3.087 min Scan# 31
Delta R.T. 0.018 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion: 53 Resp: 682
Ion Ratio Lower Upper
53 100
52 64.8 65.4 98.0#
51 42.1 27.7 41.5#

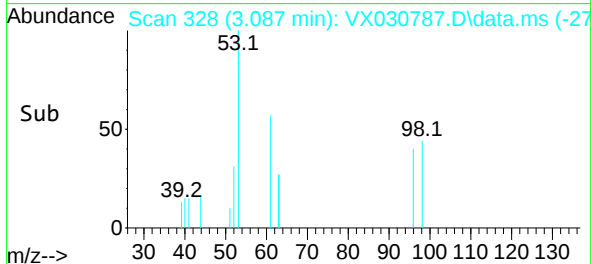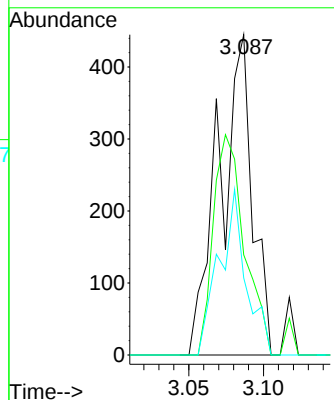

#16
Acetone
Concen: 0.572 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 43 Resp: 726
Ion Ratio Lower Upper
43 100
58 19.1 27.7 41.5#


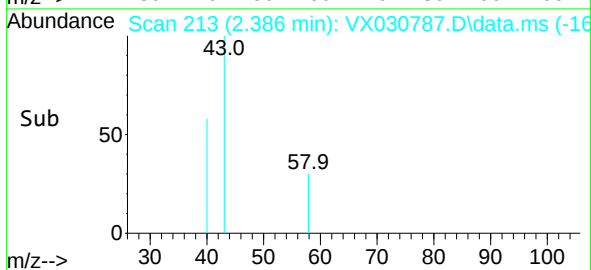
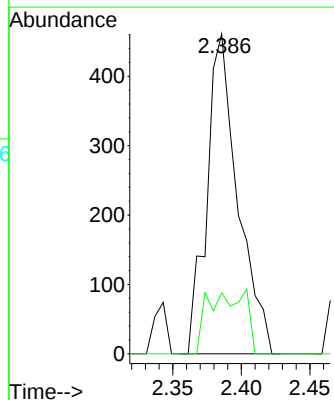
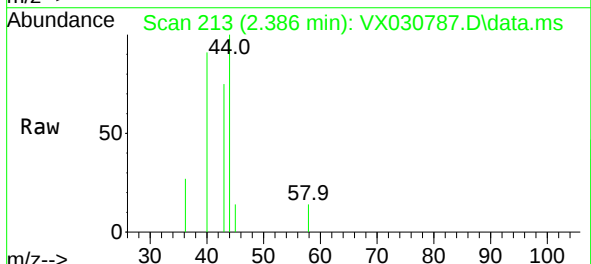




#21
trans-1,2-Dichloroethene
Concen: 0.240 ug/l
RT: 3.099 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion: 96 Resp: 546
Ion Ratio Lower Upper
96 100
61 119.9 105.6 158.4
98 49.3 50.1 75.1#

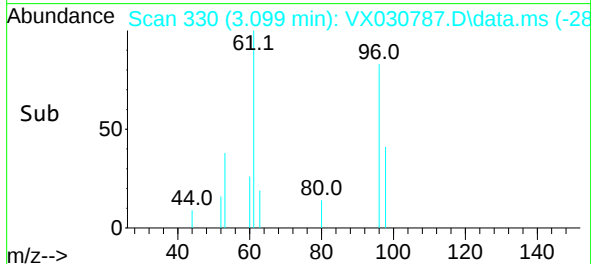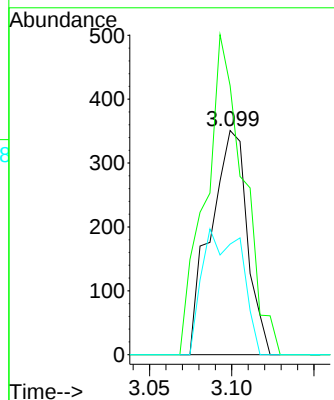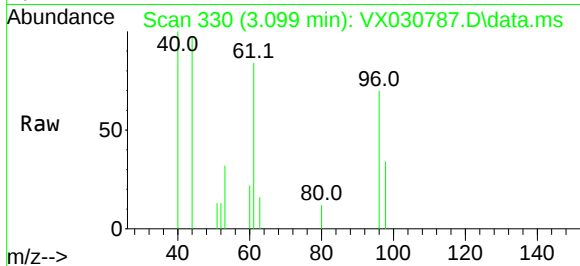

#23
Vinyl Acetate
Concen: 0.204 ug/l
RT: 3.751 min Scan# 437
Delta R.T. 0.024 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 43 Resp: 1288
Ion Ratio Lower Upper
43 100
86 0.0 8.5 12.7#


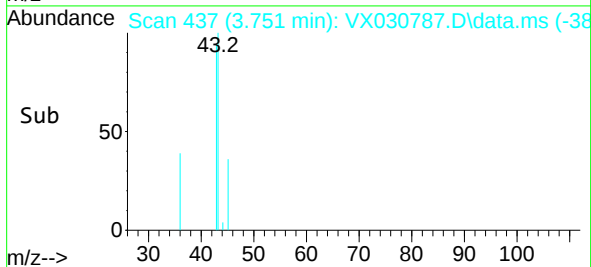
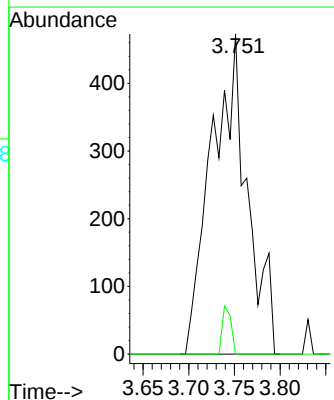
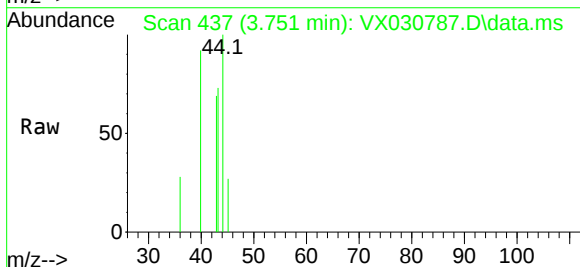


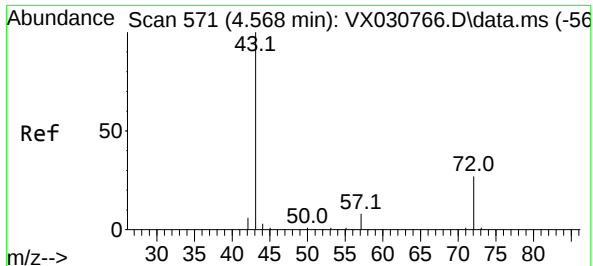

#25
2-Butanone
Concen: 0.269 ug/l
RT: 4.586 min Scan# 51
Delta R.T. 0.018 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion: 43 Resp: 550
Ion Ratio Lower Upper
43 100
72 0.0 21.7 32.5#

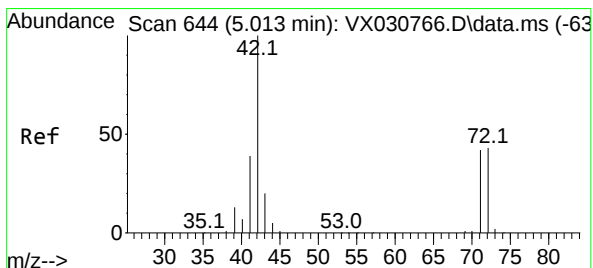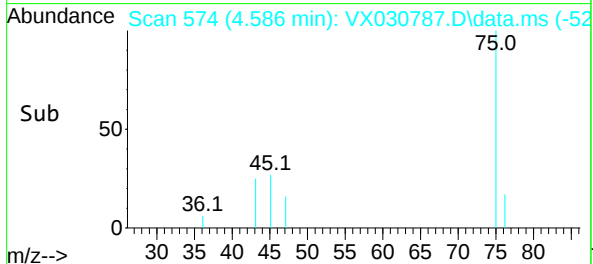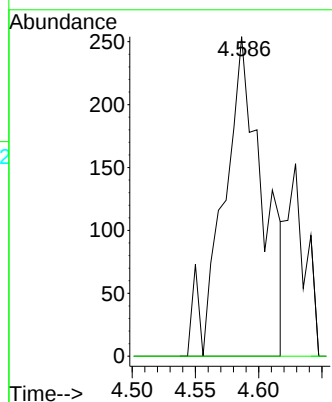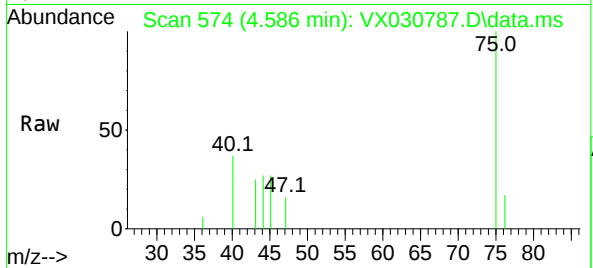

#29
Tetrahydrofuran
Concen: 0.289 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.031 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 42 Resp: 386
Ion Ratio Lower Upper
42 100
72 0.0 36.5 54.7#
71 14.0 33.9 50.9#

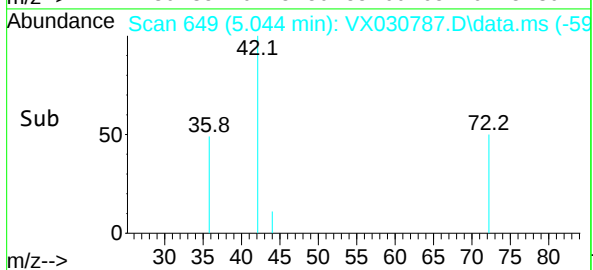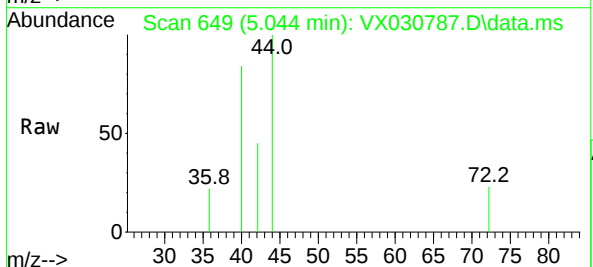



#33

1,2-Dichloroethane-d4

Concen: 50.256 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54

Instrument :

MSVOA_X

ClientSampleId :





VX0825WBL02

Tgt Ion: 65 Resp: 138125

Ion Ratio Lower Upper

65 100

67 53.7 0.0 109.6

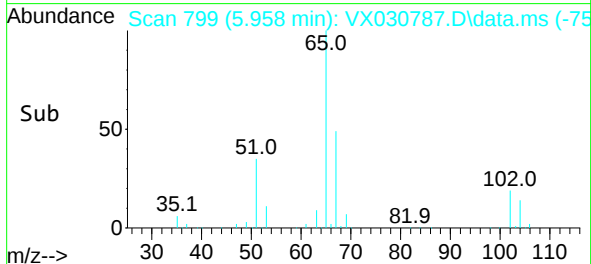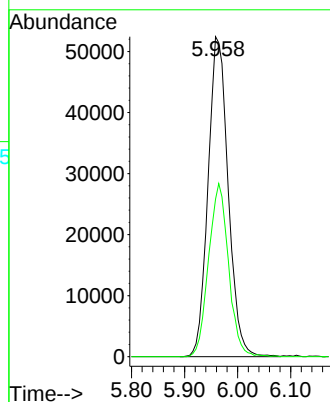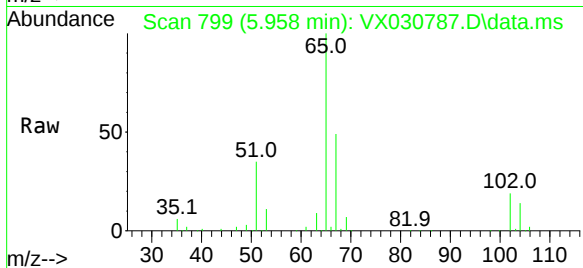

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54




Tgt Ion: 114 Resp: 385357


Ion Ratio Lower Upper

114 100

63 19.1 0.0 38.4

88 14.9 0.0 31.8

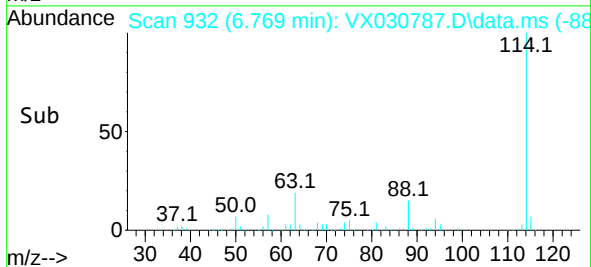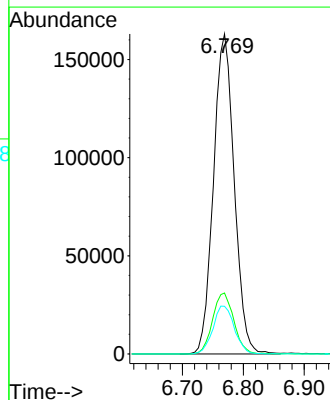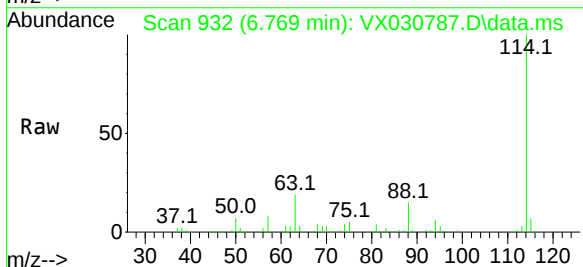

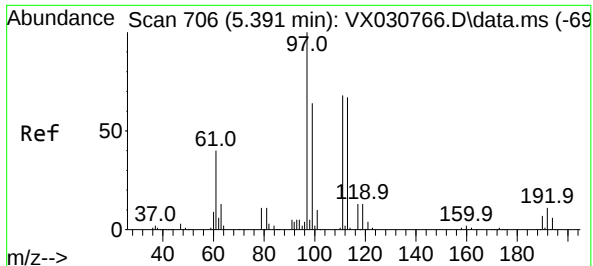

#35

Dibromofluoromethane

Concen: 50.198 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54

Instrument :

MSVOA_X

ClientSampleId :

VX0825WBL02





Tgt Ion:113 Resp: 118886

Ion Ratio Lower Upper

113 100

111 103.1 83.2 124.8

192 18.6 14.8 22.2

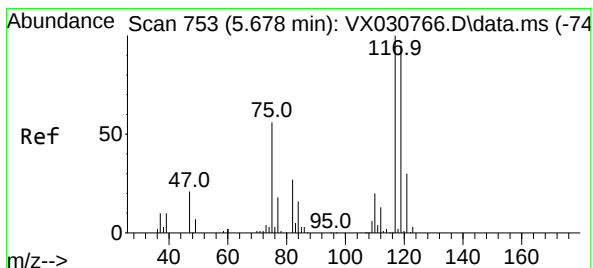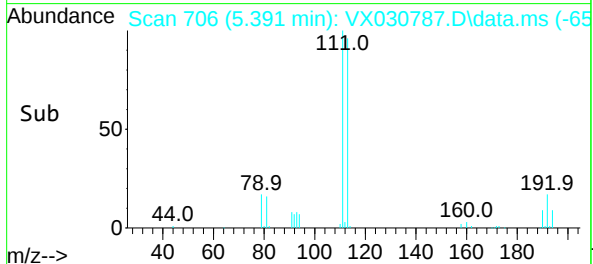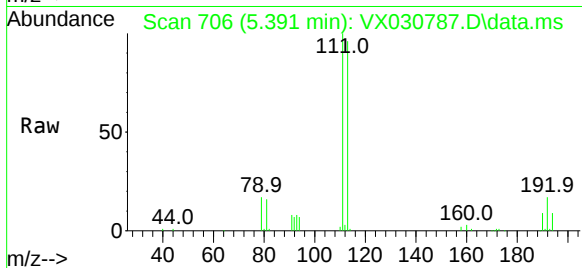

#38

Carbon Tetrachloride

Concen: 7.069 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.116 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54




Tgt Ion:117 Resp: 24047


Ion Ratio Lower Upper

117 100

119 5.5 74.1 111.1#

121 0.0 25.8 38.8#


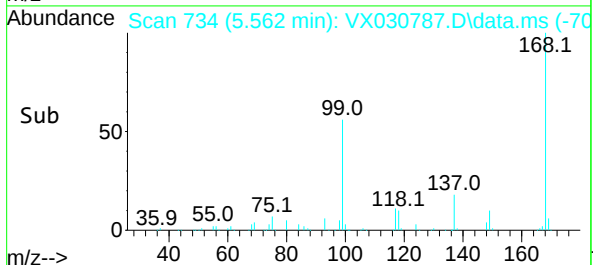
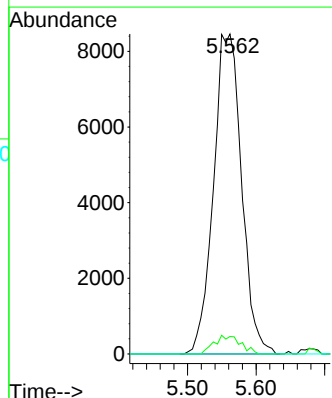
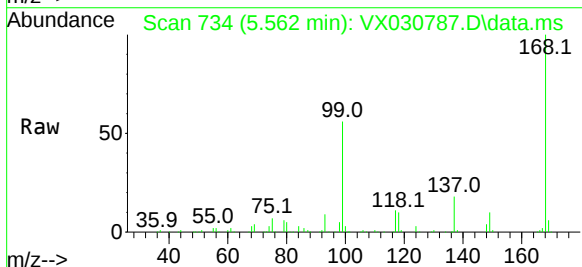


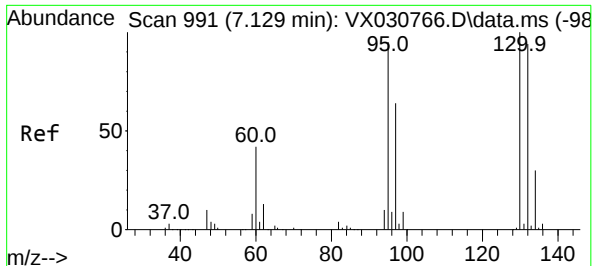

#44
Trichloroethene
Concen: 0.289 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion:130 Resp: 805
Ion Ratio Lower Upper
130 100
95 124.6 0.0 194.8

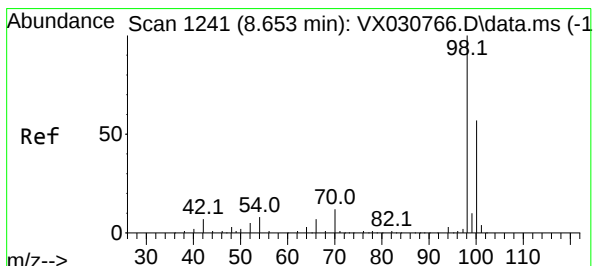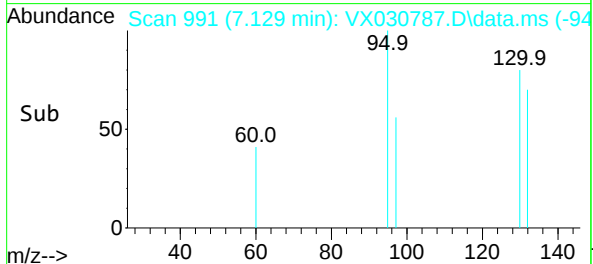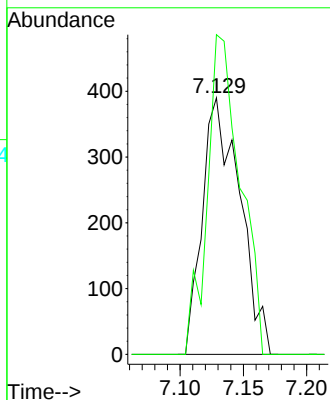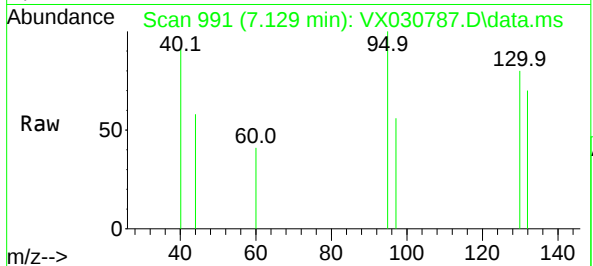

#50
Toluene-d8
Concen: 53.919 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 98 Resp: 444988
Ion Ratio Lower Upper
98 100
100 64.0 52.3 78.5


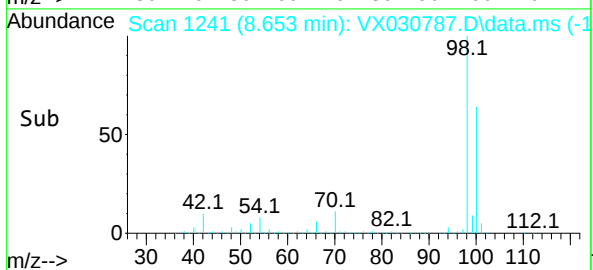
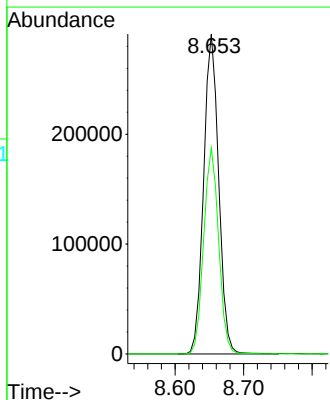
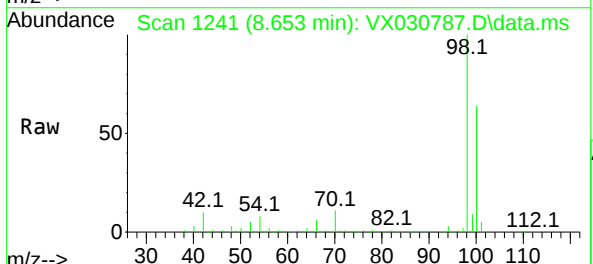


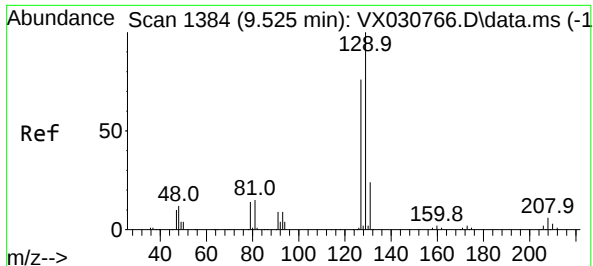

#60
Dibromochloromethane
Concen: 0.238 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion:129 Resp: 664
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.5#

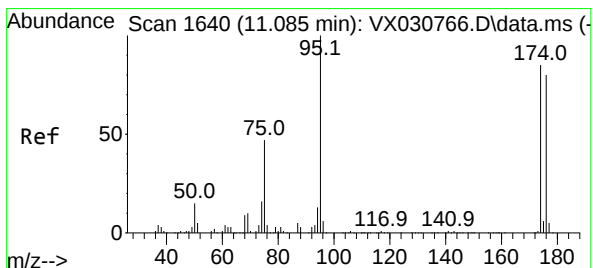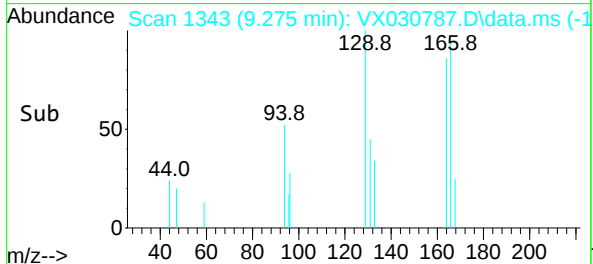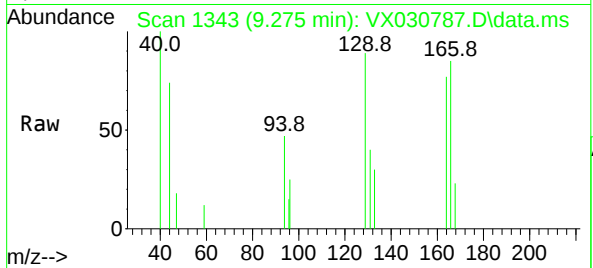

#62
4-Bromofluorobenzene
Concen: 48.603 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 95 Resp: 149336
Ion Ratio Lower Upper
95 100
174 80.2 0.0 149.0
176 76.7 0.0 146.0


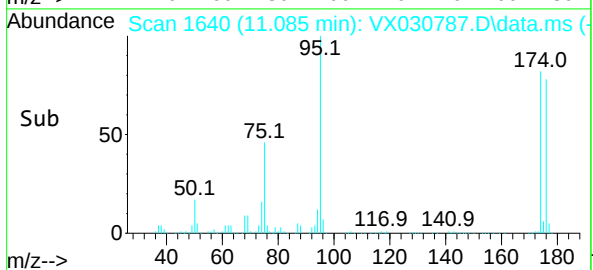

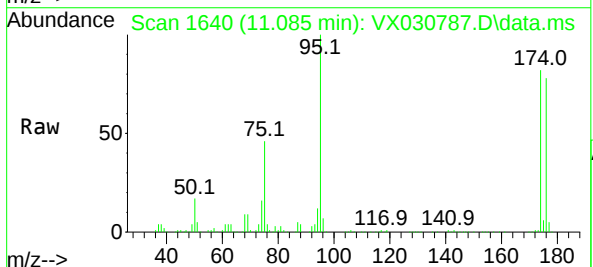




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion:117 Resp: 343269
Ion Ratio Lower Upper
117 100
82 57.3 42.7 64.1
119 33.0 25.4 38.2

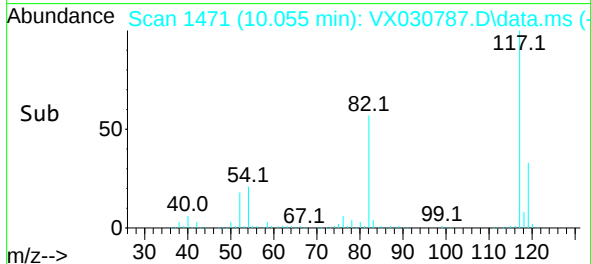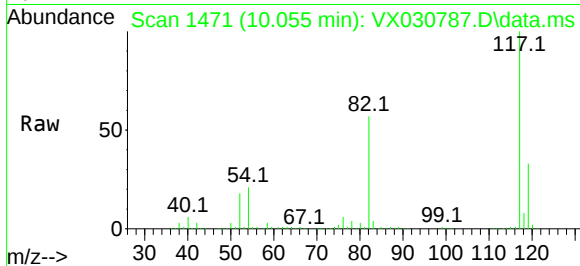

#68
m/p-Xylenes
Concen: 0.268 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.006 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion:106 Resp: 1178
Ion Ratio Lower Upper
106 100
91 199.0 158.2 237.4


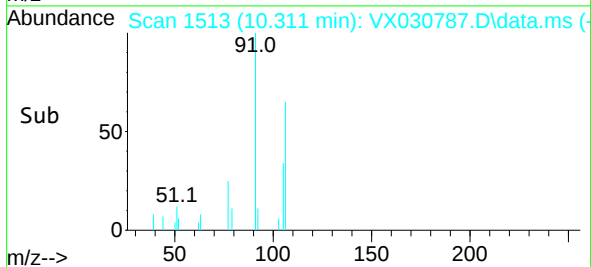

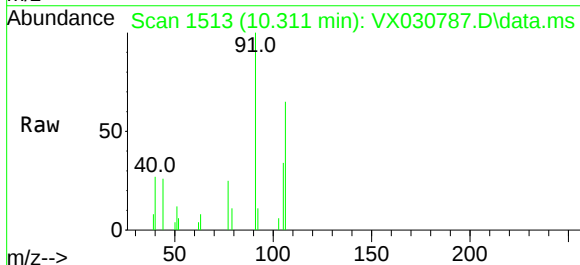




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX030787.D
 Acq: 25 Aug 2022 21:54




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0825WBL02


Tgt Ion:152 Resp: 147307
 Ion Ratio Lower Upper
 152 100
 115 61.2 40.5 121.5
 150 158.6 0.0 347.0

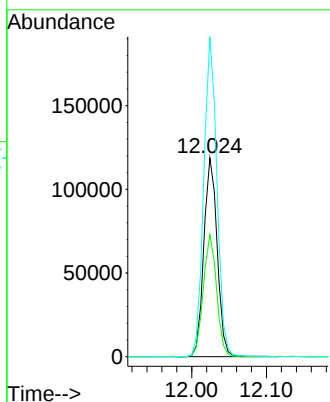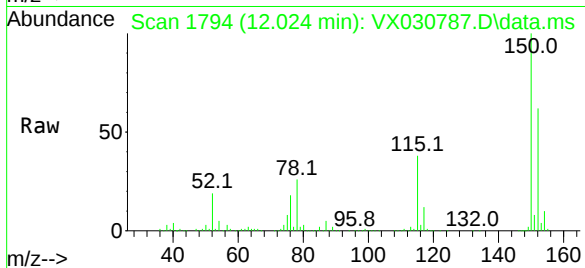

#76
 1,2,3-Trichloropropane
 Concen: 22.077 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX030787.D
 Acq: 25 Aug 2022 21:54

Tgt Ion: 75 Resp: 71250
 Ion Ratio Lower Upper
 75 100
 77 1.3 19.8 59.3#


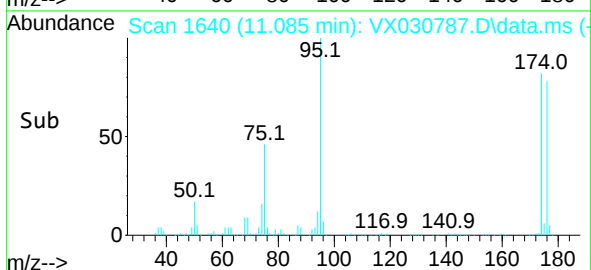
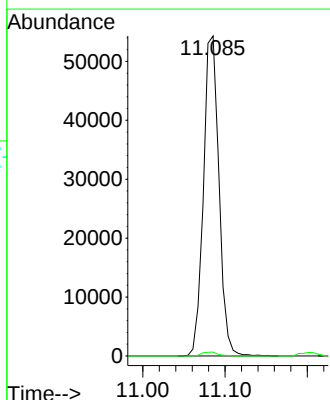
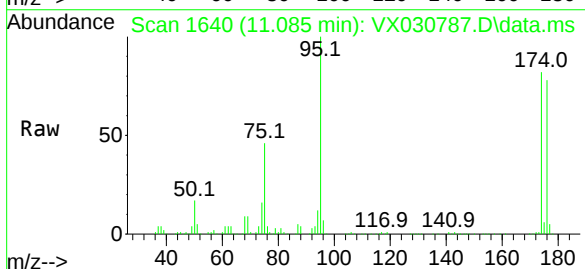




#81
trans-1,4-Dichloro-2-butene
Concen: 71.231 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.067 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54




Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02


Tgt Ion: 75 Resp: 71250
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.1 34.8 52.2#

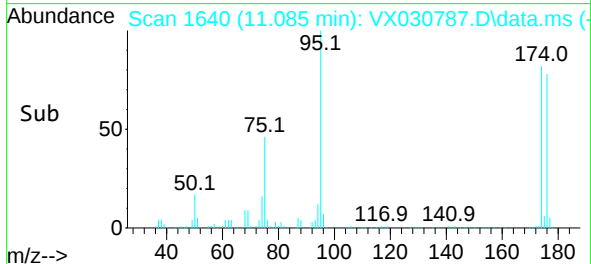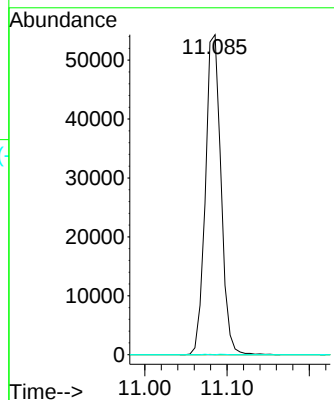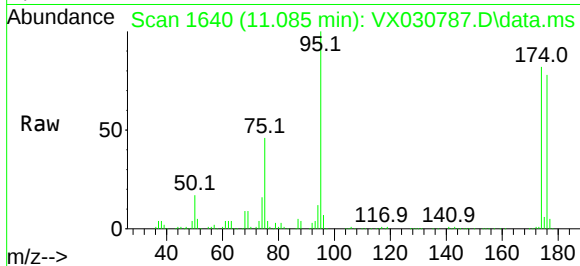

#82
4-Chlorotoluene
Concen: 0.249 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion: 91 Resp: 1940
Ion Ratio Lower Upper
91 100
126 40.1 15.3 45.9


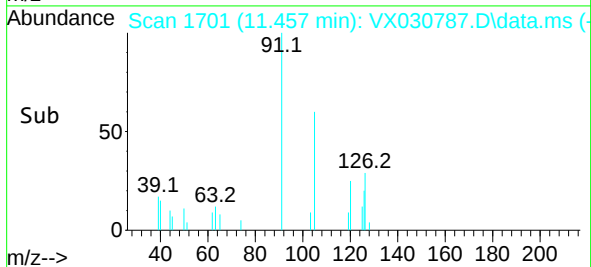
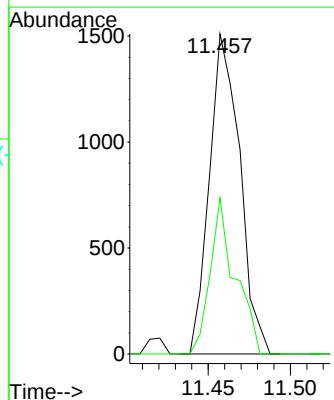
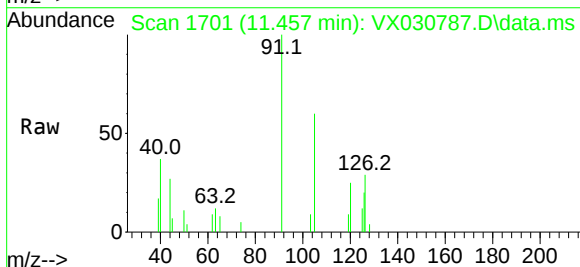




#85
 sec-Butylbenzene
 Concen: 0.208 ug/l
 RT: 11.896 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX030787.D
 Acq: 25 Aug 2022 21:54




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0825WBL02


Tgt Ion:105 Resp: 2158
 Ion Ratio Lower Upper
 105 100
 134 16.4 10.0 30.0

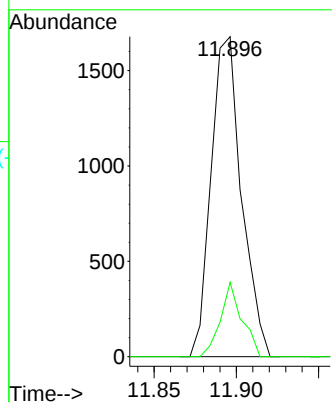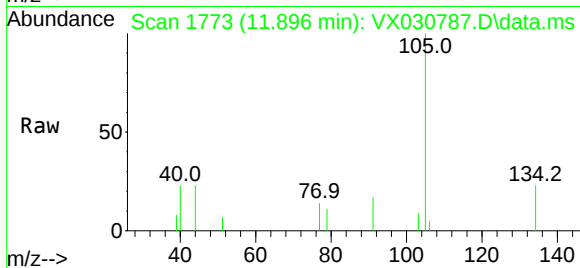

#86
 p-Isopropyltoluene
 Concen: 0.215 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. -0.000 min
 Lab File: VX030787.D
 Acq: 25 Aug 2022 21:54

Tgt Ion:119 Resp: 1828
 Ion Ratio Lower Upper
 119 100
 134 35.8 13.9 41.6
 91 44.6 11.8 35.3#

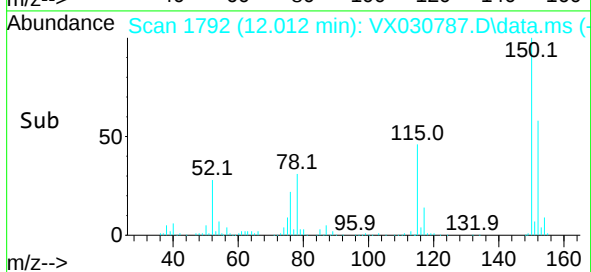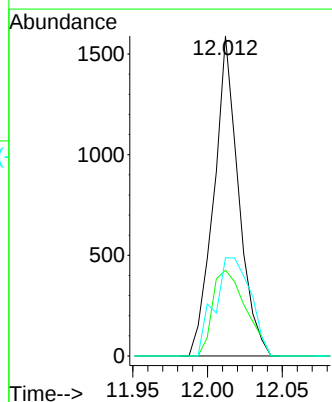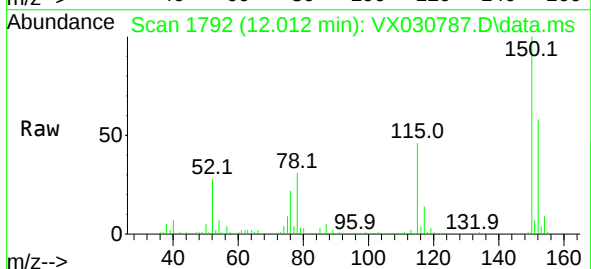



#87

1,3-Dichlorobenzene

Concen: 0.348 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. 0.006 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54

Instrument :

MSVOA_X

ClientSampleId :

VX0825WBL02





Tgt Ion:146 Resp: 1599

Ion Ratio Lower Upper

146 100

111 49.0 20.3 60.8

148 52.1 31.8 95.3

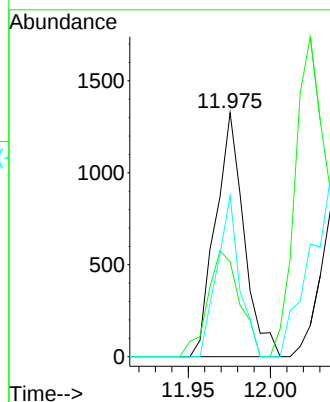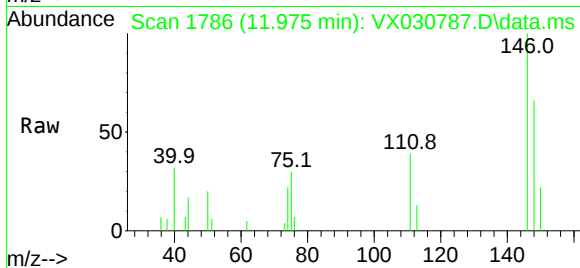

#88

1,4-Dichlorobenzene

Concen: 0.340 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. -0.068 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54




Tgt Ion:146 Resp: 1599


Ion Ratio Lower Upper

146 100

111 49.0 20.3 60.9

148 52.1 32.3 96.8

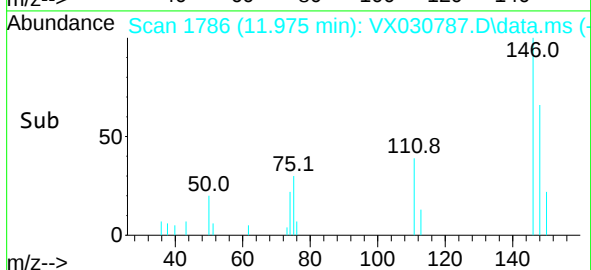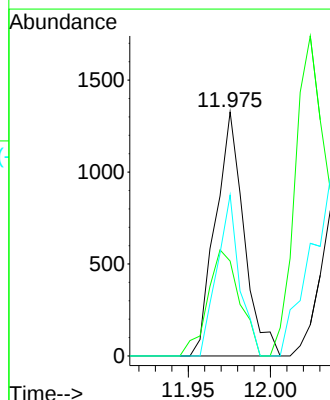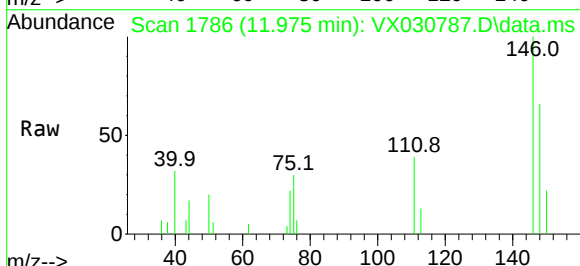



#89

n-Butylbenzene

Concen: 0.263 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.000 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54

Instrument :

MSVOA_X

ClientSampleId :

VX0825WBL02





Tgt Ion: 91 Resp: 2072

Ion Ratio Lower Upper

91 100

92 54.0 26.2 78.5

134 30.0 12.6 37.8

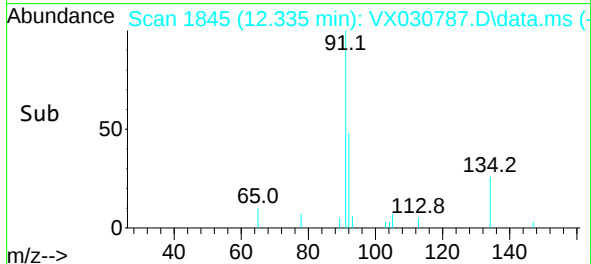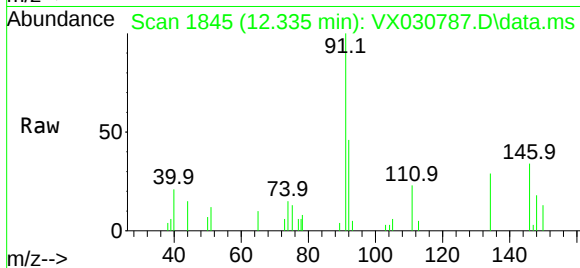

#91

1,2-Dichlorobenzene

Concen: 0.265 ug/l

RT: 12.341 min Scan# 1846

Delta R.T. 0.006 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54




Tgt Ion: 146 Resp: 1282


Ion Ratio Lower Upper

146 100

111 48.4 20.7 62.1

148 61.5 32.0 96.2

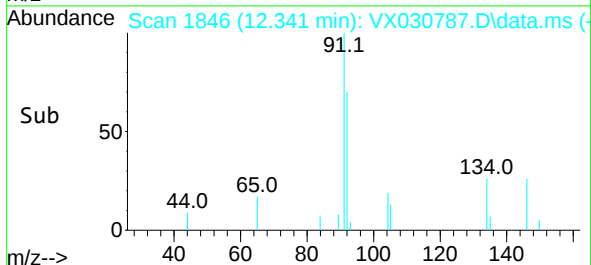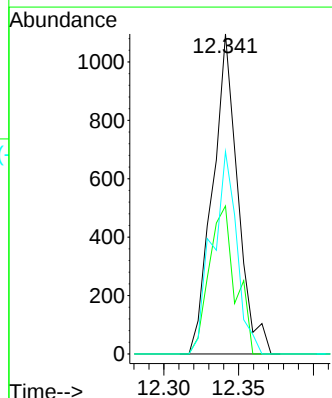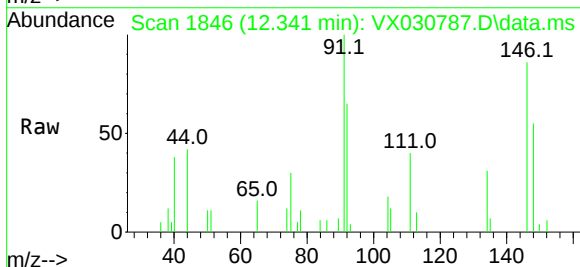

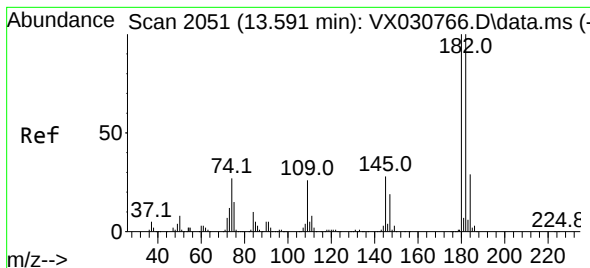

#93

1,2,4-Trichlorobenzene

Concen: 0.543 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. -0.000 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54

Instrument :

MSVOA_X

ClientSampleId :

VX0825WBL02





Tgt Ion:180 Resp: 1639

Ion Ratio Lower Upper

180 100

182 94.1 48.2 144.6

145 24.6 15.9 47.6

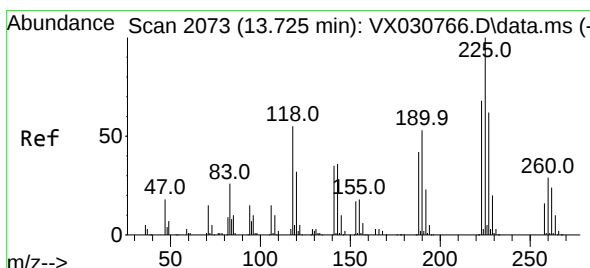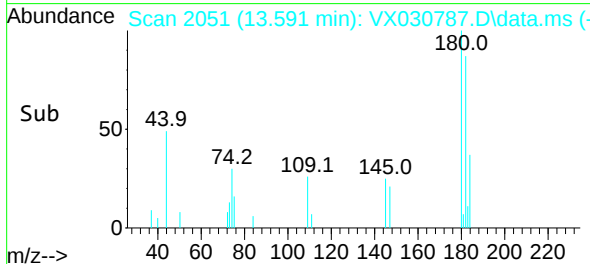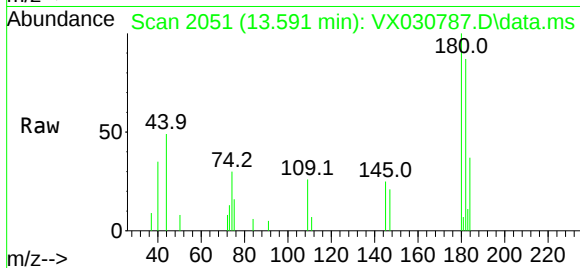

#94

Hexachlorobutadiene

Concen: 0.595 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.000 min

Lab File: VX030787.D

Acq: 25 Aug 2022 21:54




Tgt Ion:225 Resp: 749


Ion Ratio Lower Upper

225 100

223 52.1 30.6 91.6

227 54.2 31.9 95.9


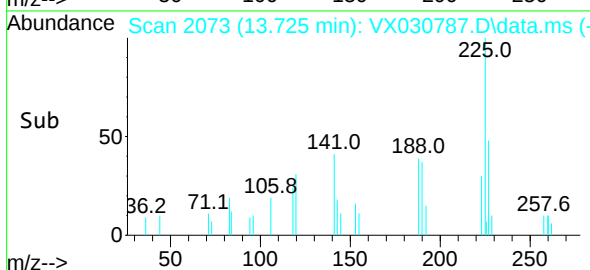

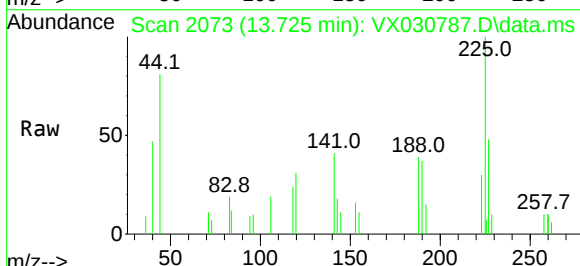




#95
Naphthalene
Concen: 0.432 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Instrument :
MSVOA_X
ClientSampleId :
VX0825WBL02

Tgt Ion:128 Resp: 4543
Ion Ratio Lower Upper
128 100
127 11.2 10.2 15.2
129 8.8 8.6 13.0

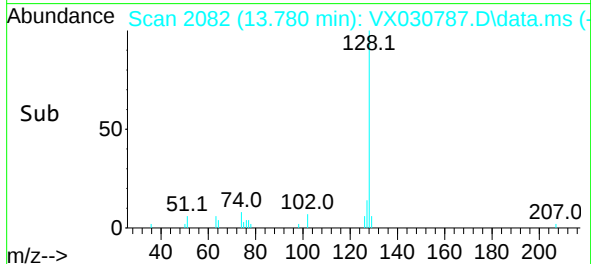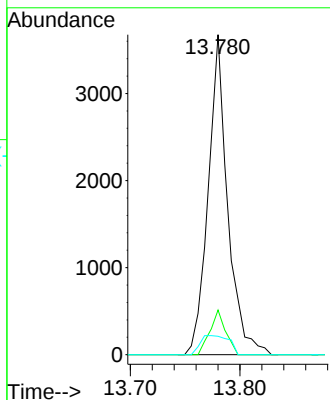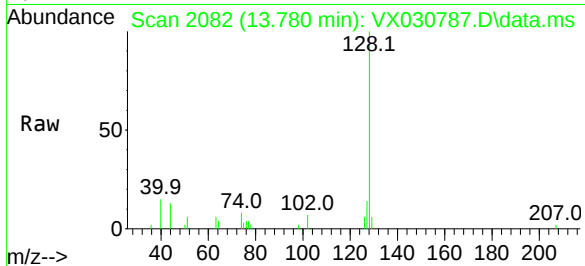

#96
1,2,3-Trichlorobenzene
Concen: 0.478 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX030787.D
Acq: 25 Aug 2022 21:54

Tgt Ion:180 Resp: 1526
Ion Ratio Lower Upper
180 100
182 102.9 47.0 141.0
145 33.6 17.0 50.9

