

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
 Data File : VX030790.D
 Acq On : 25 Aug 2022 23:28
 Operator : JC/MD
 Sample : N4245-03DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW179D2-20220816DL

Quant Time: Aug 26 02:43:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	235556	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	389102	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	347571	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	151823	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	139858	50.476	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 100.960%			
35) Dibromofluoromethane	5.391	113	122206	51.103	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 102.200%			
50) Toluene-d8	8.653	98	452920	54.352	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 108.700%			
62) 4-Bromofluorobenzene	11.085	95	154210	49.707	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 99.420%			
Target Compounds						
					Qvalue	
3) Chloromethane	1.288	50	501	Below Cal	#	82
4) Vinyl Chloride	1.374	62	124	Below Cal	#	31
5) Bromomethane	1.611	94	526	0.479	ug/l	90
6) Chloroethane	1.684	64	282	Below Cal	#	41
10) Methyl Iodide	2.447	142	597	4.316	ug/l	# 85
11) Tert butyl alcohol	2.946	59	6316	10.501	ug/l	# 74
12) 1,1-Dichloroethene	2.319	96	1554	0.728	ug/l	# 80
13) Acrolein	2.239	56	165	10.350	ug/l	# 30
15) Acrylonitrile	3.062	53	450	0.305	ug/l	# 53
16) Acetone	2.386	43	1319	1.030	ug/l	# 83
17) Carbon Disulfide	2.508	76	1637	Below Cal	#	94
20) Methylene Chloride	2.788	84	3328	0.623	ug/l	# 82
21) trans-1,2-Dichloroethene	3.087	96	470	0.205	ug/l	# 79
24) 1,1-Dichloroethane	3.623	63	1053	0.234	ug/l	# 82
25) 2-Butanone	4.580	43	1019	0.494	ug/l	# 48
27) cis-1,2-Dichloroethene	4.501	96	16904	5.965	ug/l	95
31) Cyclohexane	5.556	56	4859	1.371	ug/l	# 1
36) 1,1-Dichloropropene	5.556	75	18295	5.618	ug/l	# 48
38) Carbon Tetrachloride	5.556	117	23899	6.958	ug/l	# 17
44) Trichloroethene	7.129	130	139865	49.691	ug/l	98
60) Dibromochloromethane	9.275	129	10621	3.769	ug/l	# 11
64) Tetrachloroethene	9.275	164	11001	4.018	ug/l	94
76) 1,2,3-Trichloropropane	11.085	75	74463	22.386	ug/l	# 37
81) trans-1,4-Dichloro-2-b...	11.085	75	74463	72.229	ug/l	# 12
87) 1,3-Dichlorobenzene	11.969	146	985	0.208	ug/l	88
88) 1,4-Dichlorobenzene	11.969	146	985	0.203	ug/l	88
93) 1,2,4-Trichlorobenzene	13.591	180	1102	0.354	ug/l	97
95) Naphthalene	13.780	128	2426	0.224	ug/l	97
96) 1,2,3-Trichlorobenzene	13.963	180	816	0.248	ug/l	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030790.D
Acq On : 25 Aug 2022 23:28
Operator : JC/MD
Sample : N4245-03DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL

Quant Time: Aug 26 02:43:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 26 02:03:28 2022
Response via : Initial Calibration




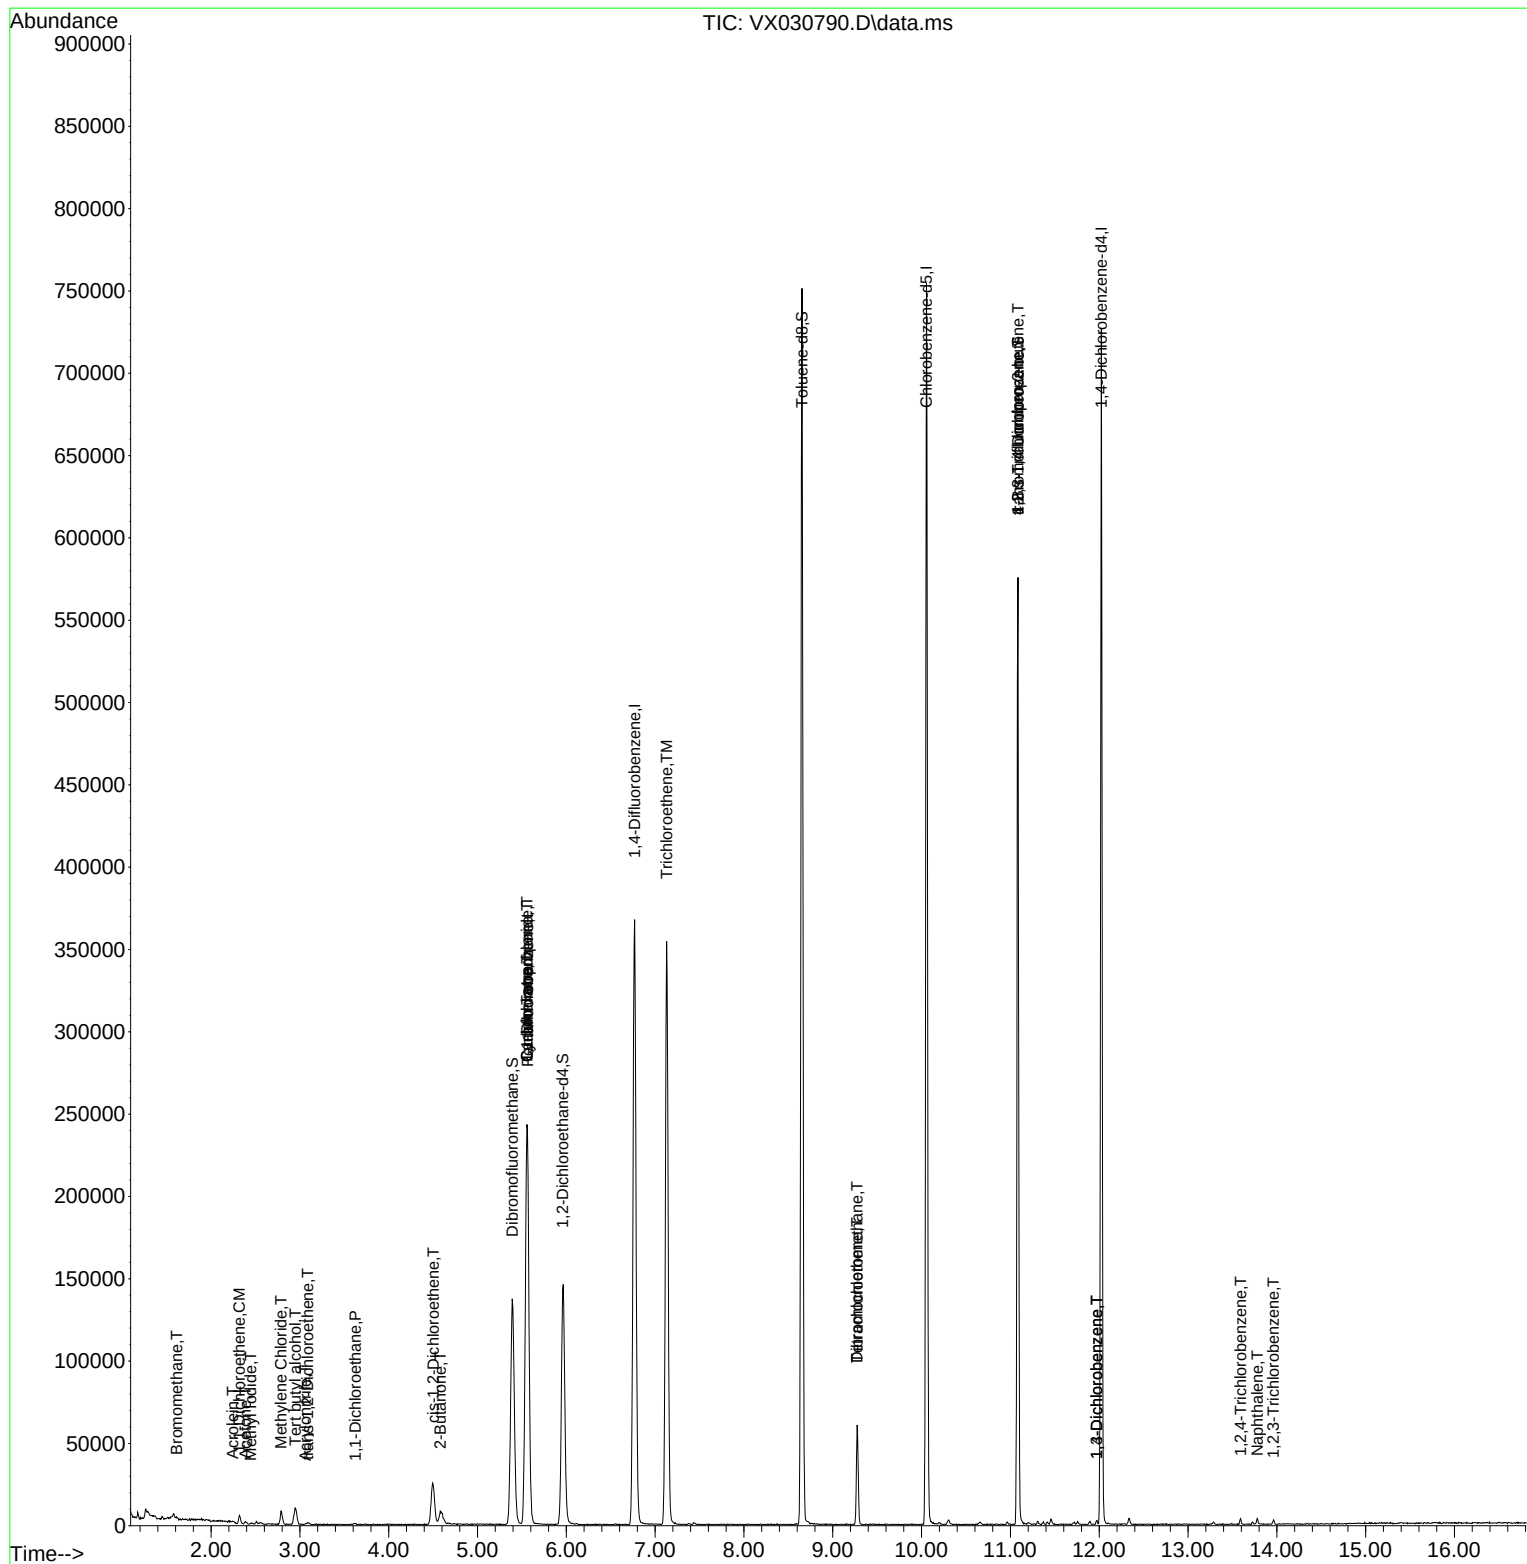




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion:168 Resp: 235556
Ion Ratio Lower Upper
168 100
99 56.7 44.0 66.0

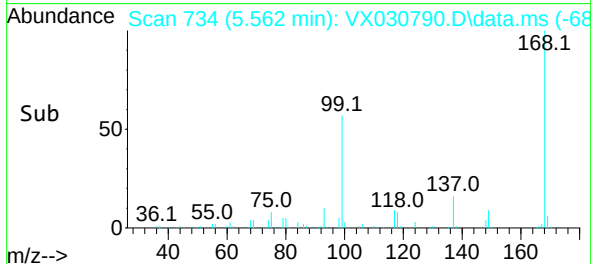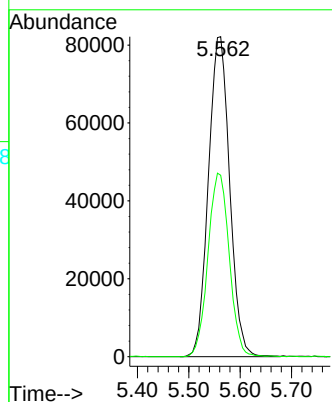

#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. 0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion: 50 Resp: 501
Ion Ratio Lower Upper
50 100
52 22.9 26.3 39.5#


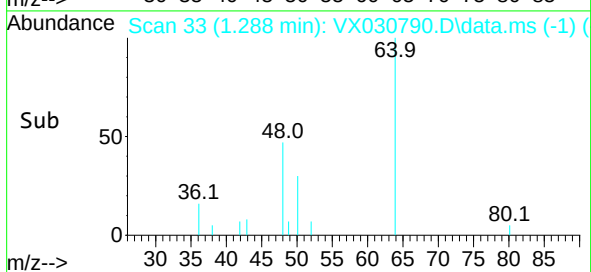
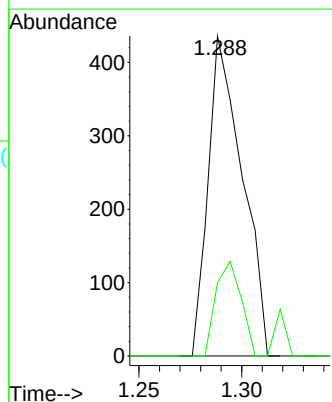



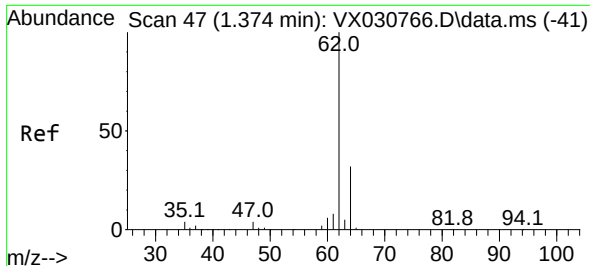

#4
 Vinyl Chloride
 Concen: Below Cal
 RT: 1.374 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VX030790.D
 Acq: 25 Aug 2022 23:28




Instrument :
 MSVOA_X
 ClientSampleId :
 MW179D2-20220816DL


Tgt Ion: 62 Resp: 124
 Ion Ratio Lower Upper
 62 100
 64 69.6 25.2 37.8#

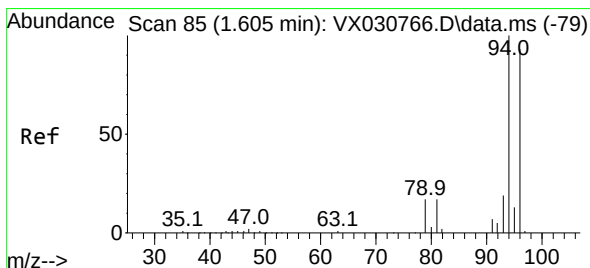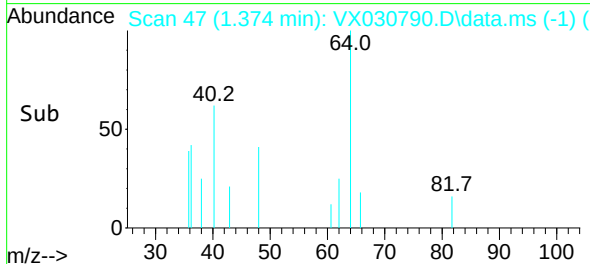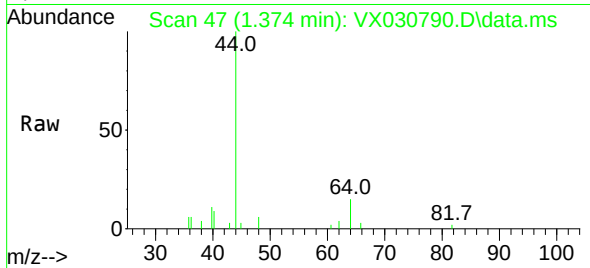

#5
 Bromomethane
 Concen: 0.479 ug/l
 RT: 1.611 min Scan# 86
 Delta R.T. 0.006 min
 Lab File: VX030790.D
 Acq: 25 Aug 2022 23:28

Tgt Ion: 94 Resp: 526
 Ion Ratio Lower Upper
 94 100
 96 86.6 76.9 115.3


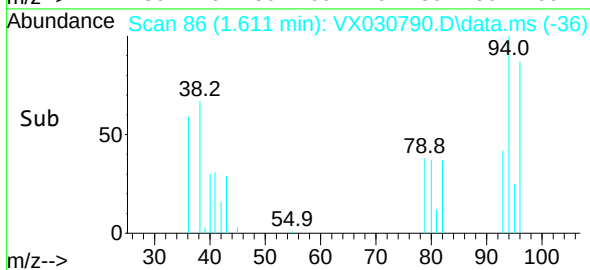

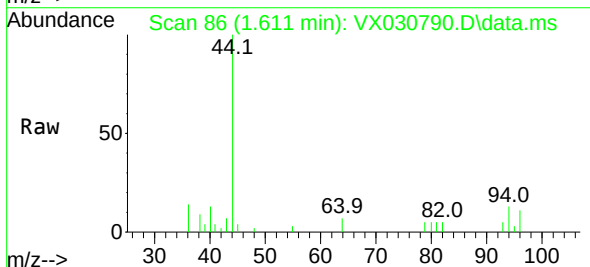


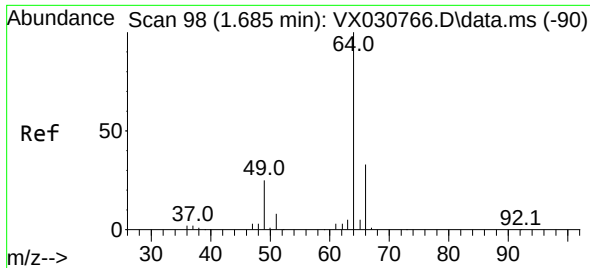

#6
Chloroethane
Concen: Below Cal
RT: 1.684 min Scan# 91
Delta R.T. -0.001 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion: 64 Resp: 282
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

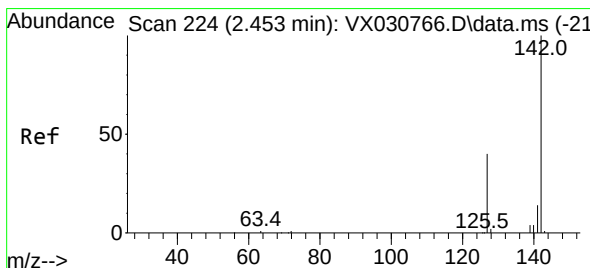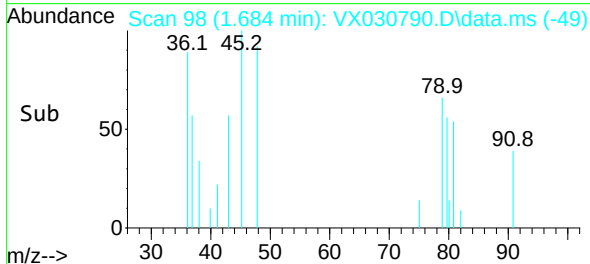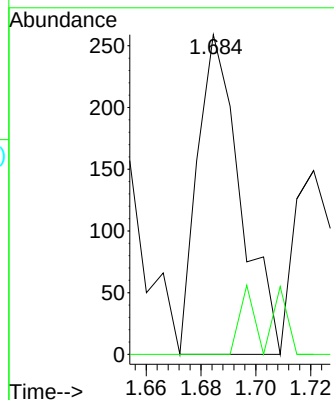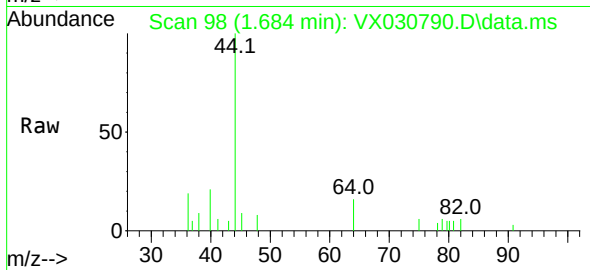

#10
Methyl Iodide
Concen: 4.316 ug/l
RT: 2.447 min Scan# 223
Delta R.T. -0.006 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion:142 Resp: 597
Ion Ratio Lower Upper
142 100
127 42.0 30.2 45.2
141 0.0 11.3 16.9#


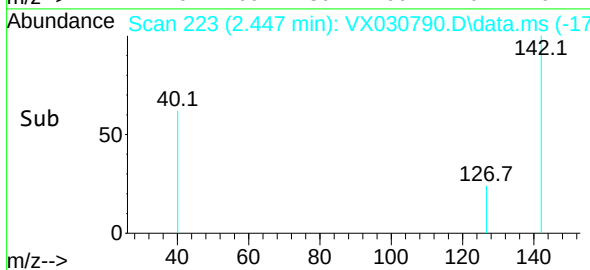
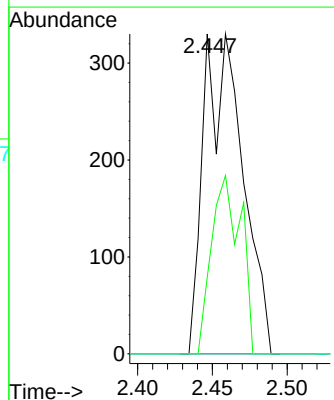
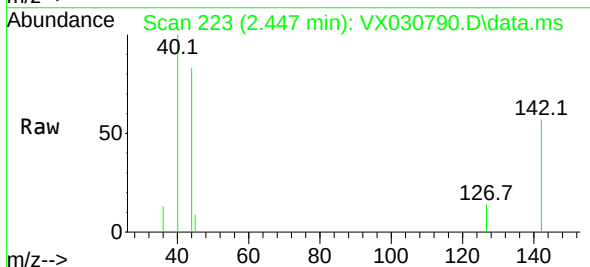




#11
Tert butyl alcohol
Concen: 10.501 ug/l
RT: 2.946 min Scan# 305
Delta R.T. -0.049 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion: 59 Resp: 6316
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#

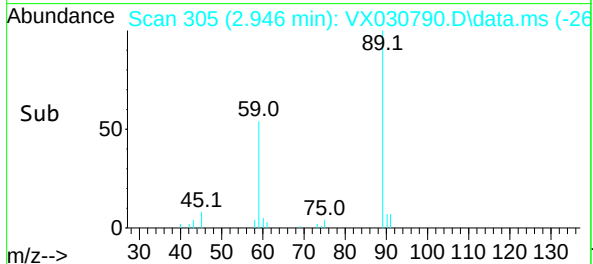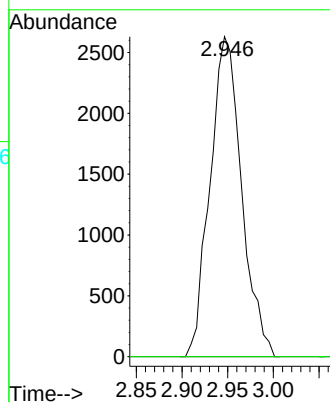

#12
1,1-Dichloroethene
Concen: 0.728 ug/l
RT: 2.319 min Scan# 202
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion: 96 Resp: 1554
Ion Ratio Lower Upper
96 100
61 169.3 117.4 176.0
98 83.9 52.2 78.4#


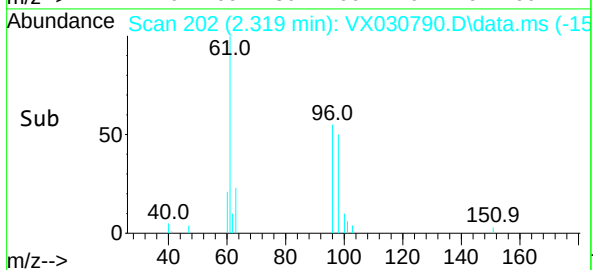
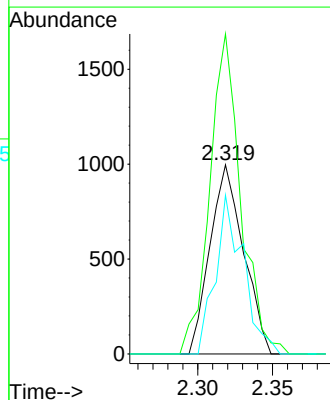
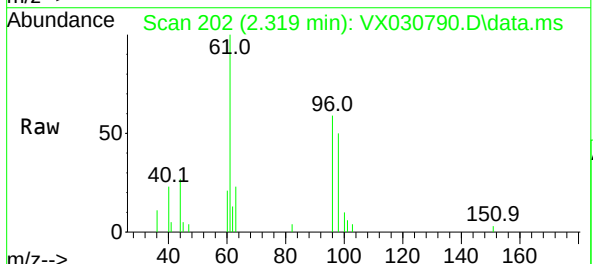




#13
Acrolein
Concen: 10.350 ug/l
RT: 2.239 min Scan# 11
Delta R.T. -0.001 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion: 56 Resp: 165
Ion Ratio Lower Upper
56 100
55 13.3 56.6 84.8#

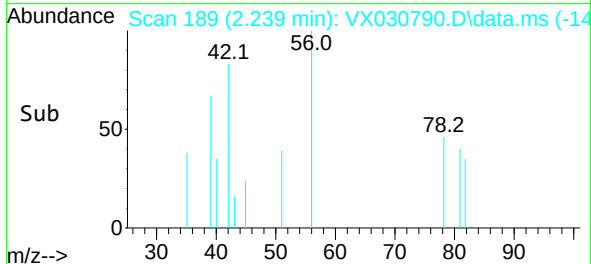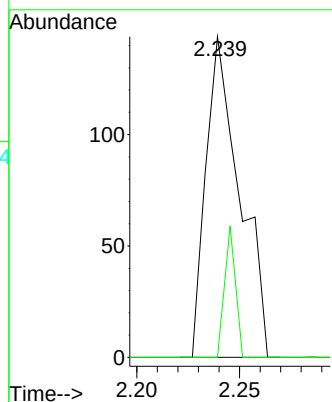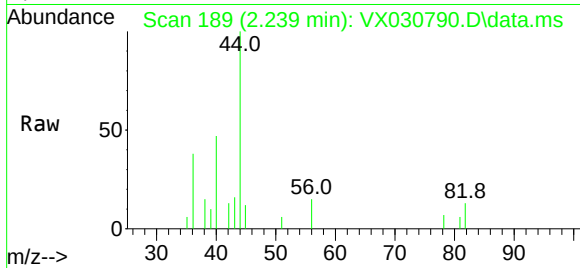

#15
Acrylonitrile
Concen: 0.305 ug/l
RT: 3.062 min Scan# 324
Delta R.T. -0.006 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion: 53 Resp: 450
Ion Ratio Lower Upper
53 100
52 32.2 65.4 98.0#
51 18.2 27.7 41.5#

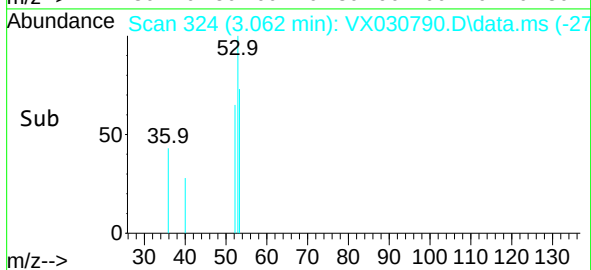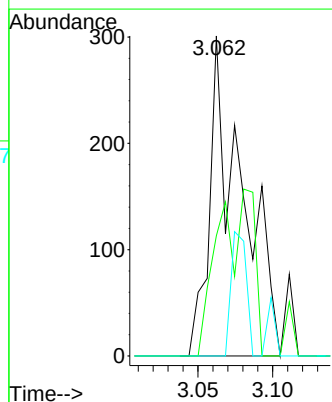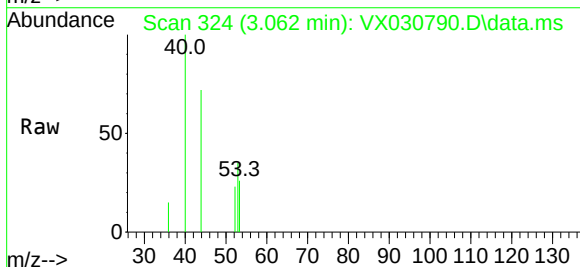



#16

Acetone

Concen: 1.030 ug/l

RT: 2.386 min Scan# 214

Delta R.T. -0.006 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28

Instrument :

MSVOA_X

ClientSampleId :





MW179D2-20220816DL

Tgt Ion: 43 Resp: 1319

Ion Ratio Lower Upper

43 100

58 44.7 27.7 41.5#

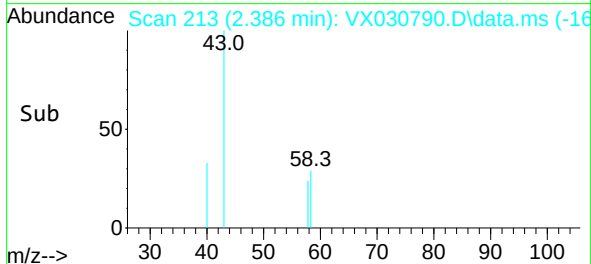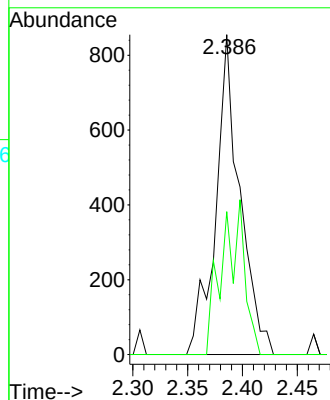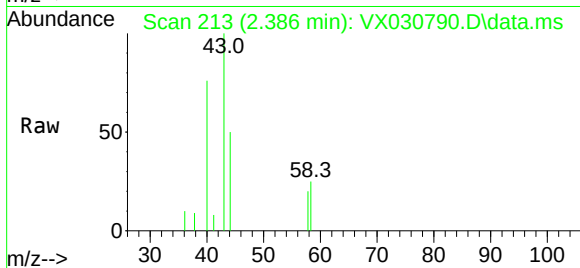

#17

Carbon Disulfide

Concen: Below Cal

RT: 2.508 min Scan# 233

Delta R.T. -0.000 min

Lab File: VX030790.D




Acq: 25 Aug 2022 23:28


Tgt Ion: 76 Resp: 1637

Ion Ratio Lower Upper

76 100


78 7.4 7.8 11.6#

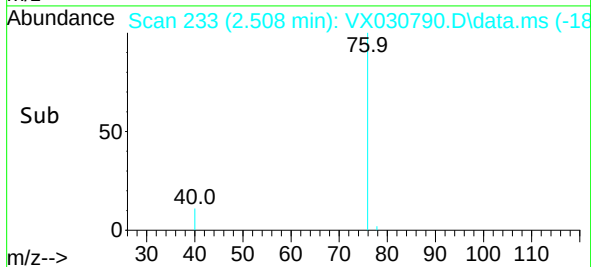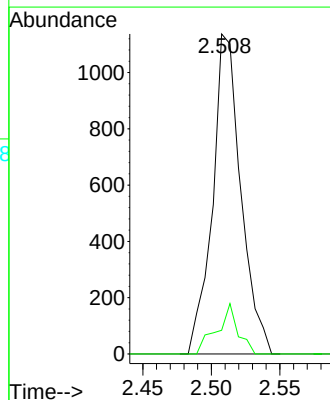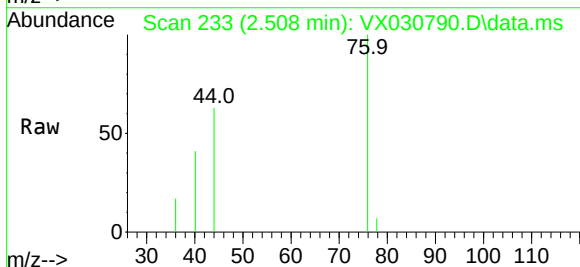






#20
Methylene Chloride
Concen: 0.623 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL



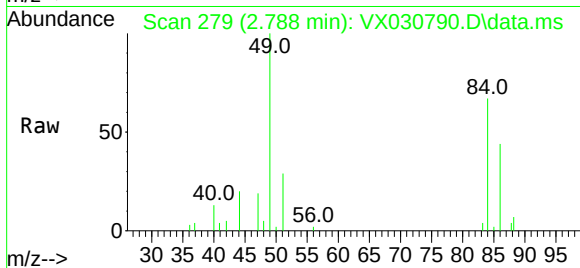



Tgt Ion:	84	Resp:	3328
Ion	Ratio	Lower	Upper
84	100		
49	148.8	93.8	140.6#
51	42.9	29.4	44.0
86	65.4	51.0	76.4

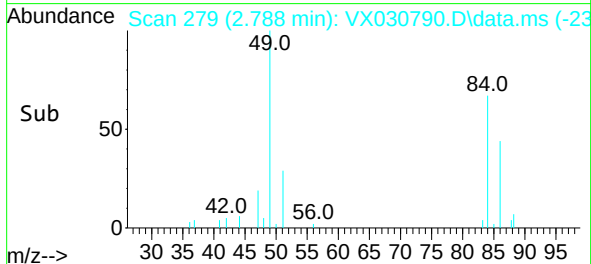

#21
trans-1,2-Dichloroethene
Concen: 0.205 ug/l
RT: 3.087 min Scan# 328
Delta R.T. -0.006 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion:	96	Resp:	470
Ion	Ratio	Lower	Upper
96	100		
61	96.9	105.6	158.4#
98	65.1	50.1	75.1

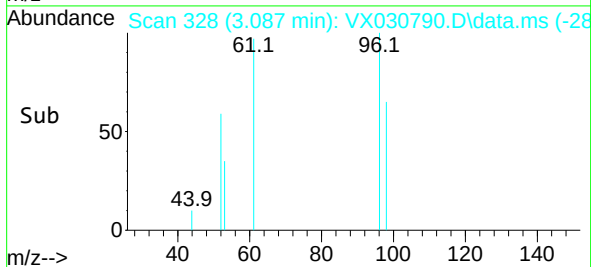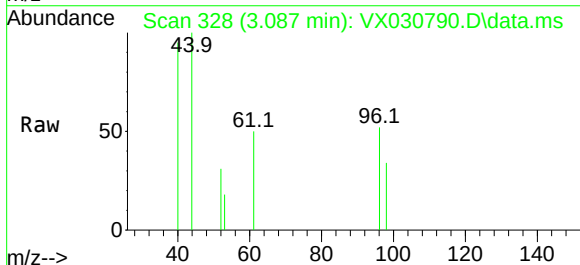



#24

1,1-Dichloroethane

Concen: 0.234 ug/l

RT: 3.623 min Scan# 41

Delta R.T. 0.012 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28

Instrument :

MSVOA_X

ClientSampleId :

MW179D2-20220816DL





Tgt Ion: 63 Resp: 1053

Ion Ratio Lower Upper

63 100

98 0.0 3.5 10.5#

100 0.0 2.3 6.9#

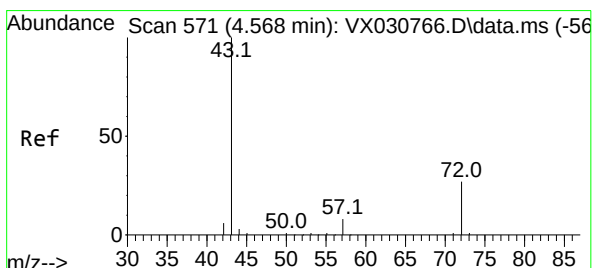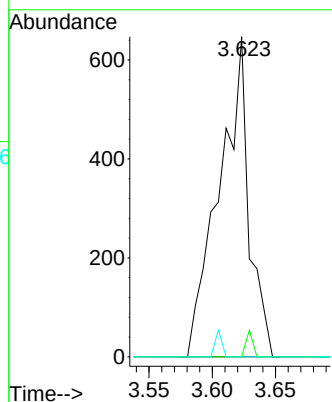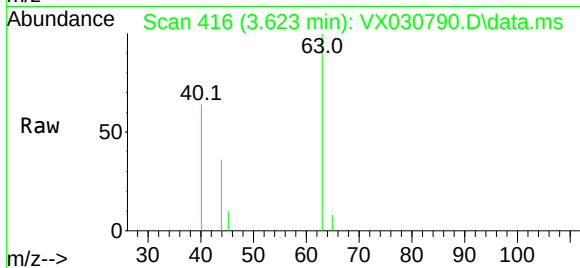

#25

2-Butanone

Concen: 0.494 ug/l

RT: 4.580 min Scan# 573

Delta R.T. 0.012 min

Lab File: VX030790.D




Acq: 25 Aug 2022 23:28


Tgt Ion: 43 Resp: 1019

Ion Ratio Lower Upper

43 100

72 0.0 21.7 32.5#

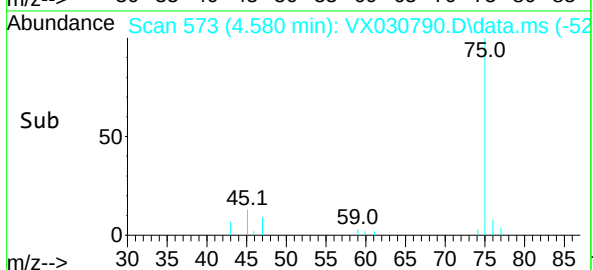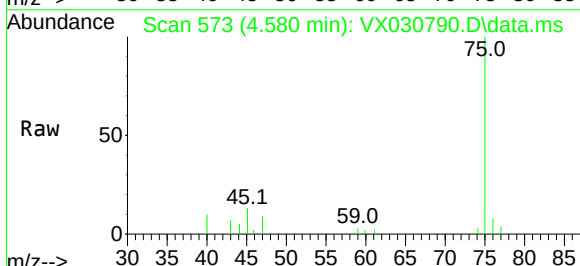



#27

cis-1,2-Dichloroethene

Concen: 5.965 ug/l

RT: 4.501 min Scan# 51

Delta R.T. 0.006 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28

Instrument :

MSVOA_X

ClientSampleId :

MW179D2-20220816DL





Tgt Ion: 96 Resp: 16904

Ion Ratio Lower Upper

96 100

61 126.4 0.0 270.0

98 63.2 0.0 127.8

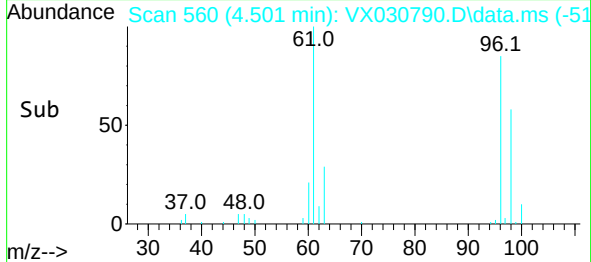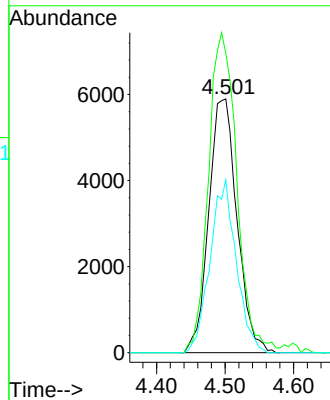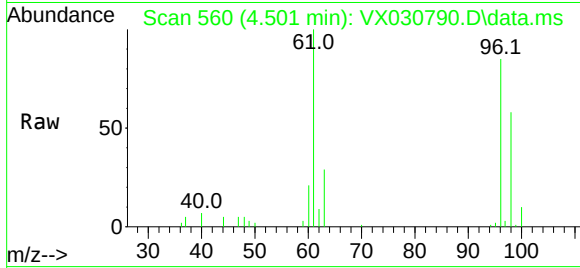

#31

Cyclohexane

Concen: 1.371 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.085 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28




Tgt Ion: 56 Resp: 4859


Ion Ratio Lower Upper

56 100

69 170.5 25.4 38.0#

84 149.2 68.9 103.3#

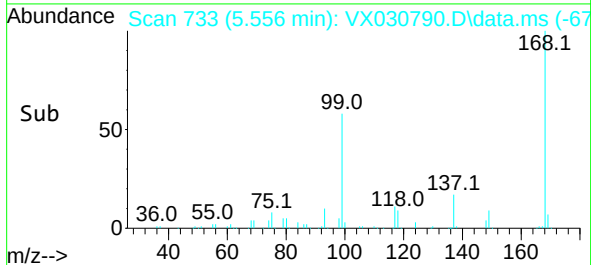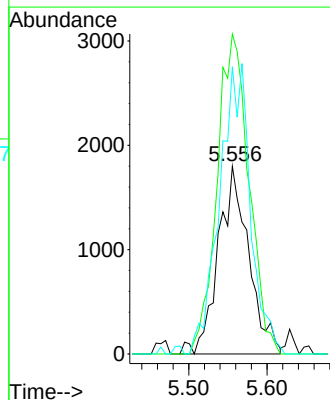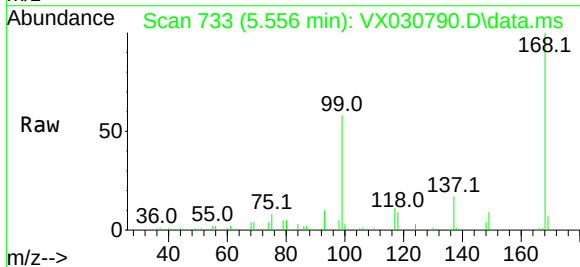



#33

1,2-Dichloroethane-d4

Concen: 50.476 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28

Instrument :

MSVOA_X

ClientSampleId :





MW179D2-20220816DL

Tgt Ion: 65 Resp: 139858

Ion Ratio Lower Upper

65 100

67 54.5 0.0 109.6

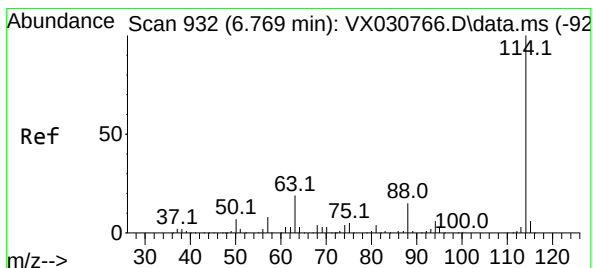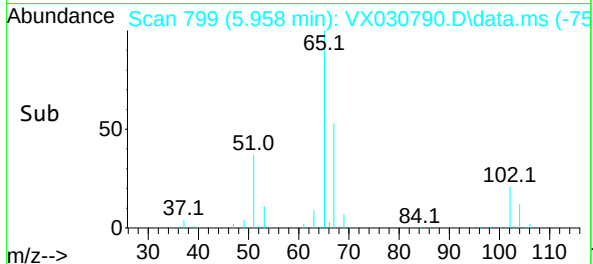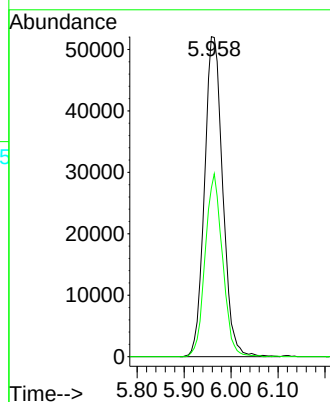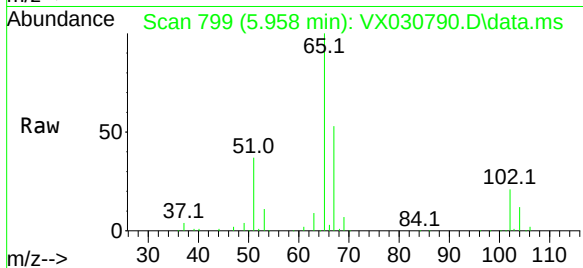

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.000 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28




Tgt Ion: 114 Resp: 389102


Ion Ratio Lower Upper

114 100

63 19.1 0.0 38.4

88 15.8 0.0 31.8

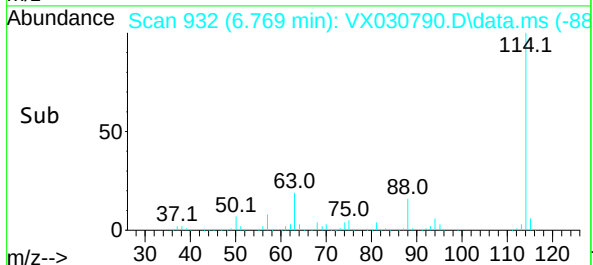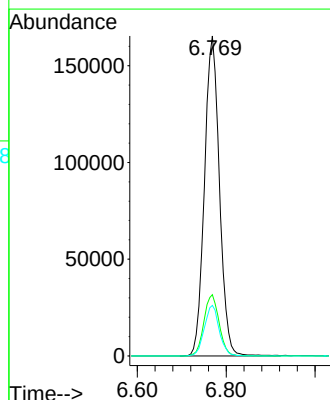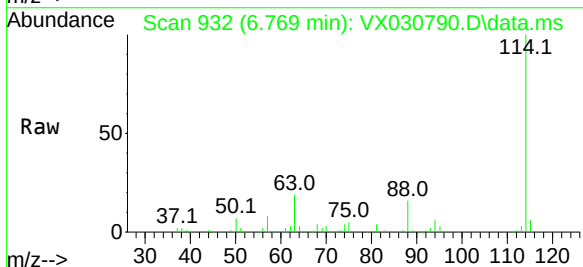



#35

Dibromofluoromethane

Concen: 51.103 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28

Instrument :

MSVOA_X

ClientSampleId :

MW179D2-20220816DL





Tgt Ion:113 Resp: 122206

Ion Ratio Lower Upper

113 100

111 101.9 83.2 124.8

192 18.7 14.8 22.2

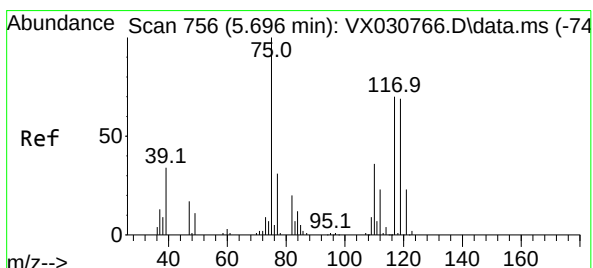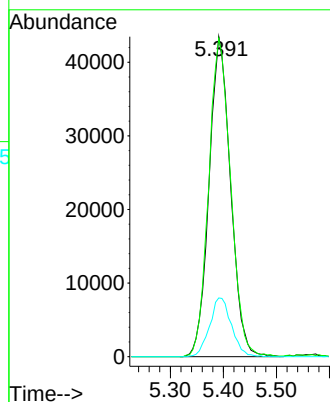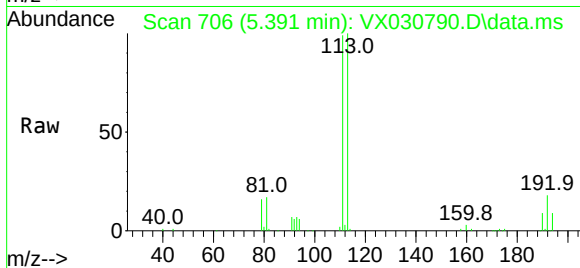

#36

1,1-Dichloropropene

Concen: 5.618 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28




Tgt Ion: 75 Resp: 18295


Ion Ratio Lower Upper

75 100

110 8.5 19.3 57.9#


77 0.0 24.4 36.6#

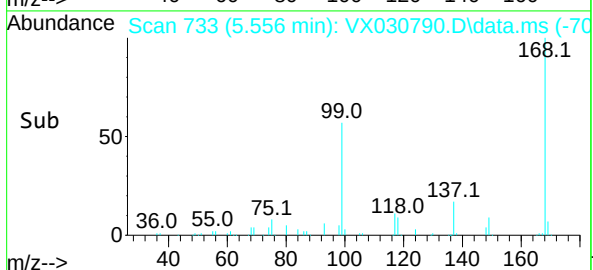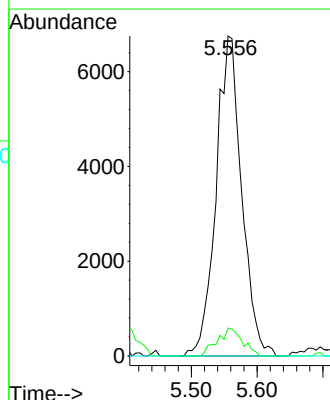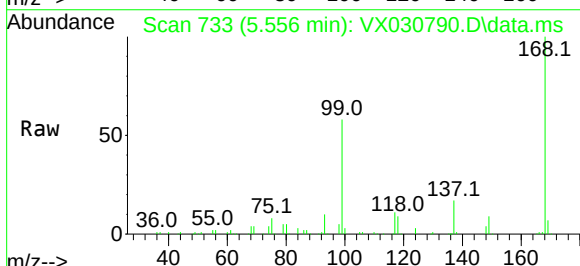






#38
Carbon Tetrachloride
Concen: 6.958 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.122 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL



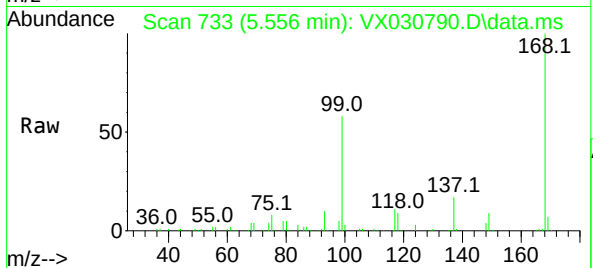



Tgt Ion:117 Resp: 23899
Ion Ratio Lower Upper
117 100
119 4.4 74.1 111.1#
121 0.0 25.8 38.8#

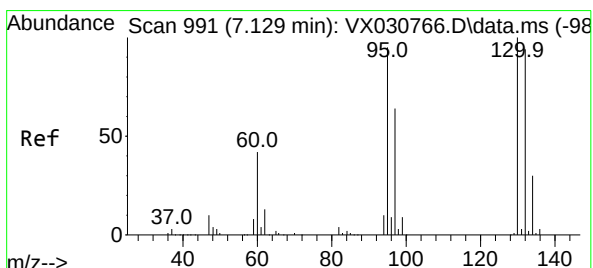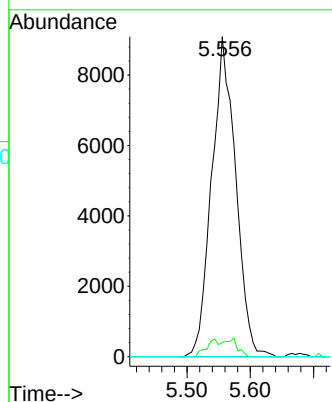

#44
Trichloroethene
Concen: 49.691 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion:130 Resp: 139865
Ion Ratio Lower Upper
130 100
95 98.9 0.0 194.8


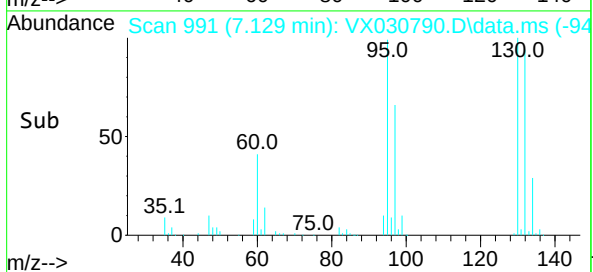
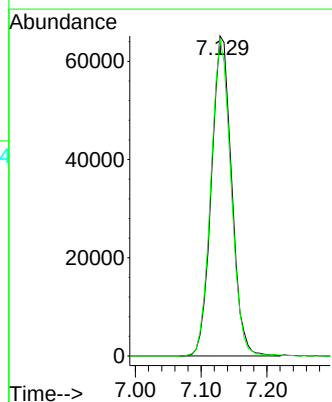
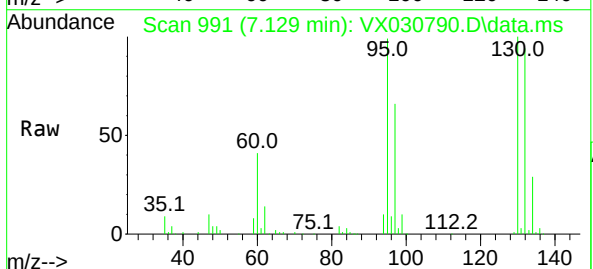




#50
Toluene-d8
Concen: 54.352 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion: 98 Resp: 452920
Ion Ratio Lower Upper
98 100
100 63.6 52.3 78.5

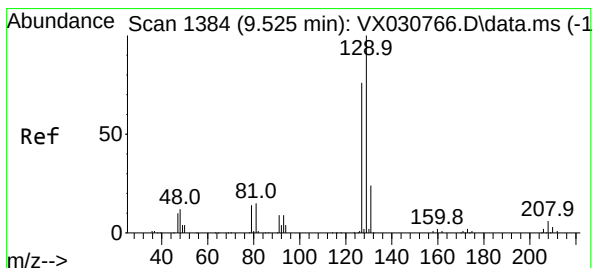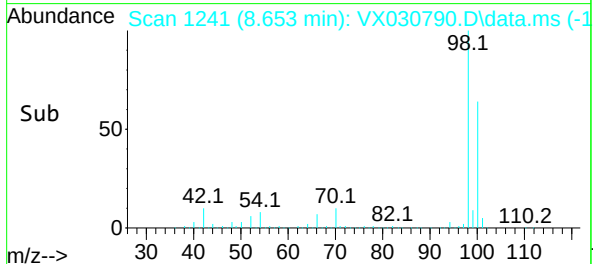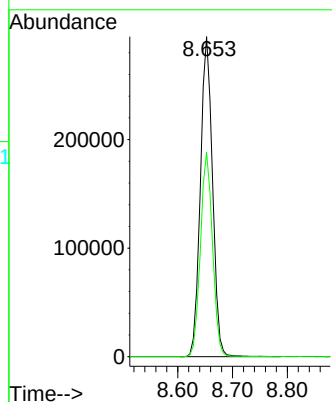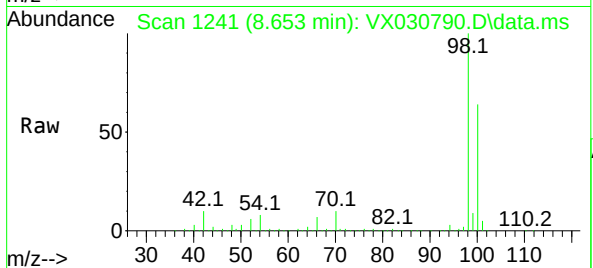

#60
Dibromochloromethane
Concen: 3.769 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.250 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion: 129 Resp: 10621
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.5#


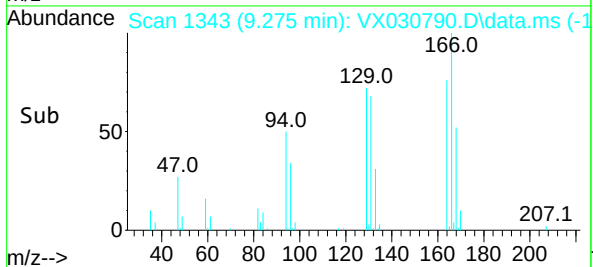
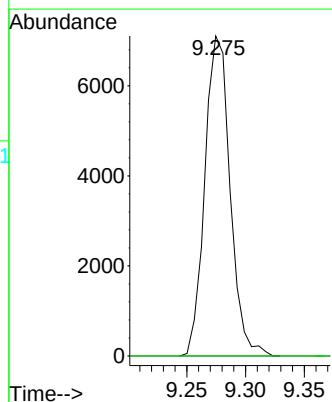
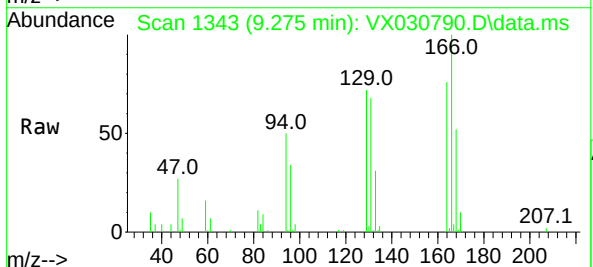




#62
4-Bromofluorobenzene
Concen: 49.707 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion: 95 Resp: 154210
Ion Ratio Lower Upper
95 100
174 78.7 0.0 149.0
176 76.1 0.0 146.0

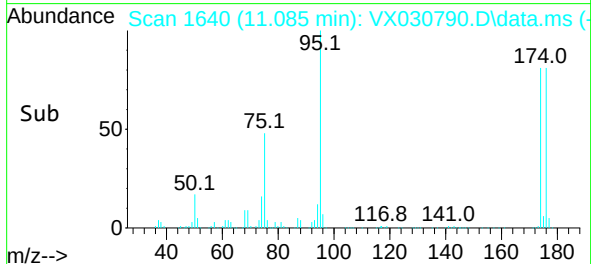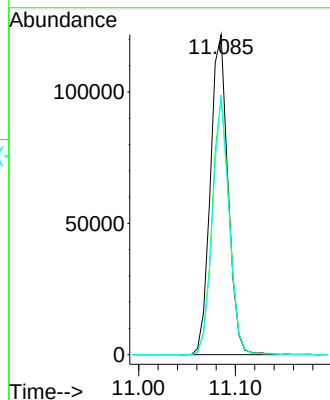

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion: 117 Resp: 347571
Ion Ratio Lower Upper
117 100
82 58.0 42.7 64.1
119 33.5 25.4 38.2


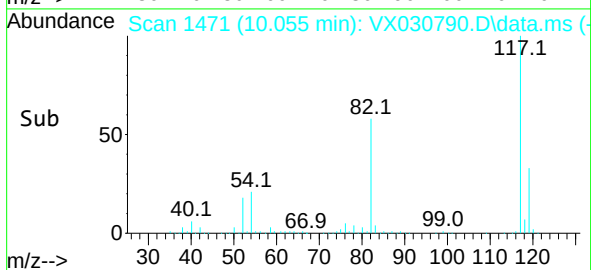
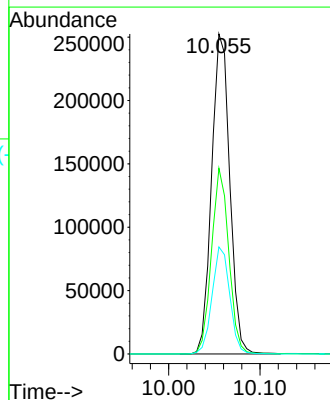
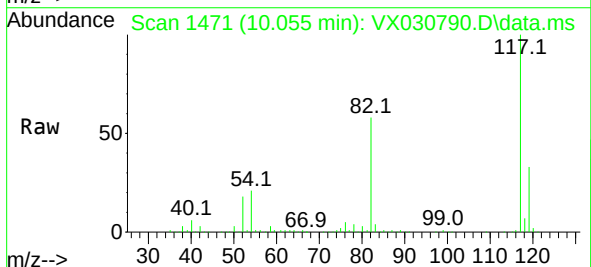




#64
Tetrachloroethene
Concen: 4.018 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion:164	Resp:	11001
Ion	Ratio	Lower Upper
164	100	
166	132.2	98.2 147.4
129	95.7	80.8 121.2
131	89.8	75.5 113.3

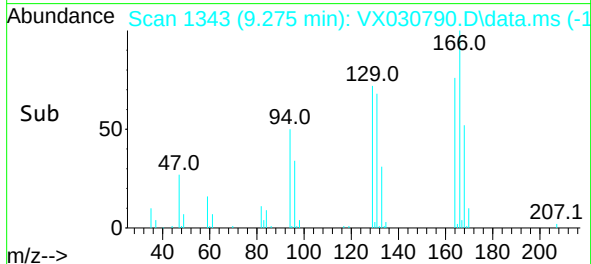

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion:152	Resp:	151823
Ion	Ratio	Lower Upper
152	100	
115	59.4	40.5 121.5
150	154.8	0.0 347.0



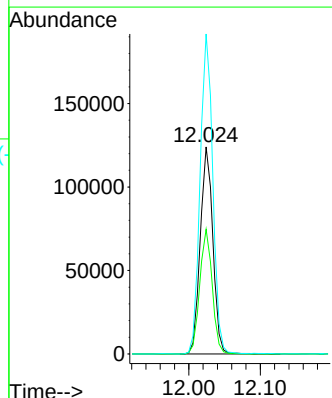
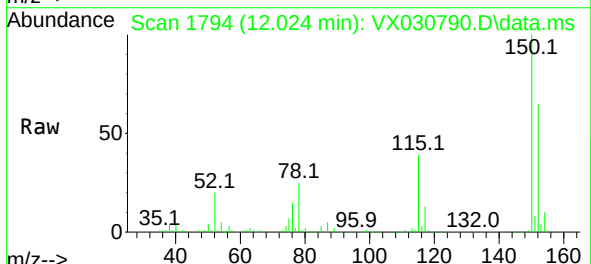




#76
1,2,3-Trichloropropane
Concen: 22.386 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion: 75 Resp: 74463
Ion Ratio Lower Upper
75 100
77 1.1 19.8 59.3#

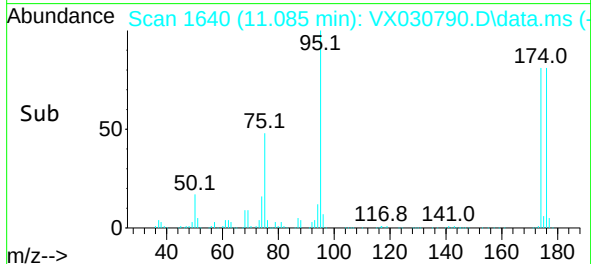

#81
trans-1,4-Dichloro-2-butene
Concen: 72.229 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28

Tgt Ion: 75 Resp: 74463
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.8 52.2#

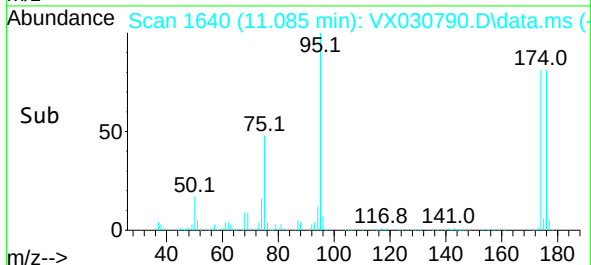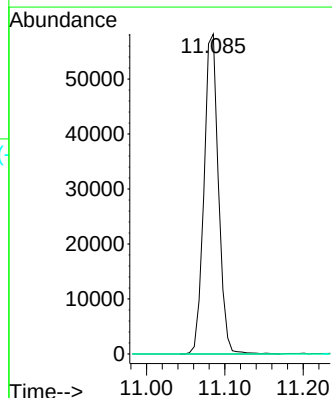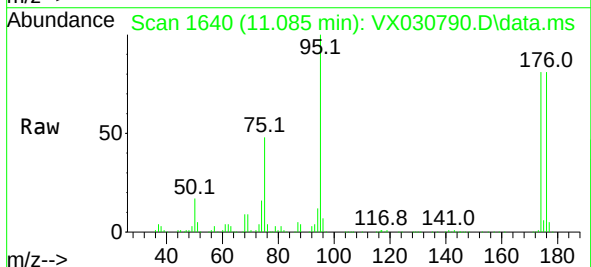



#87

1,3-Dichlorobenzene

Concen: 0.208 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.000 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28

Instrument :

MSVOA_X

ClientSampleId :

MW179D2-20220816DL





Tgt Ion:146 Resp: 985

Ion Ratio Lower Upper

146 100

111 49.4 20.3 60.8

148 55.5 31.8 95.3

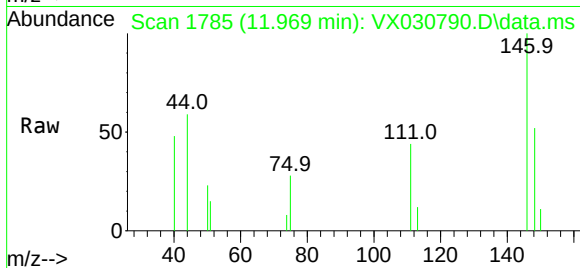

#88

1,4-Dichlorobenzene

Concen: 0.203 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.074 min

Lab File: VX030790.D

Acq: 25 Aug 2022 23:28




Tgt Ion:146 Resp: 985


Ion Ratio Lower Upper

146 100

111 49.4 20.3 60.9

148 55.5 32.3 96.8


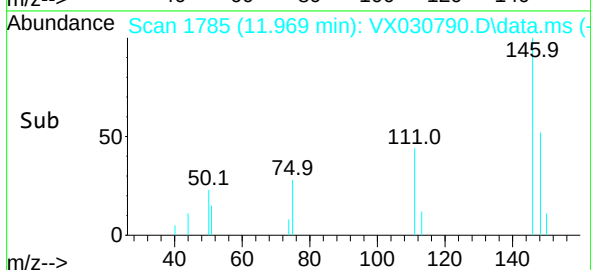

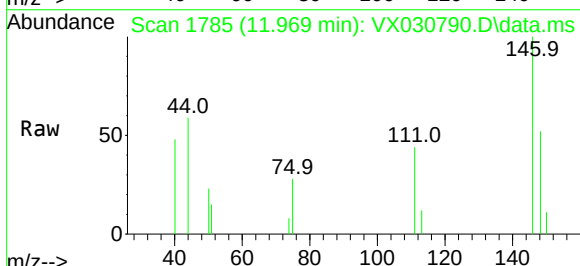


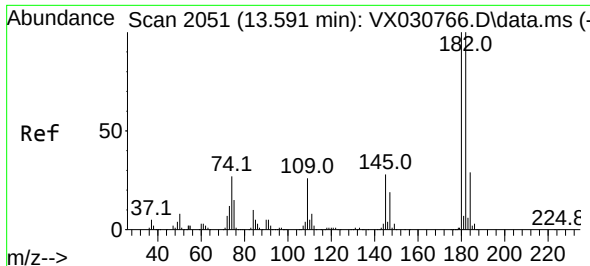

#93
1,2,4-Trichlorobenzene
Concen: 0.354 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28




Instrument :
MSVOA_X
ClientSampleId :
MW179D2-20220816DL


Tgt Ion:180	Resp:	1102
Ion	Ratio	Lower Upper
180	100	
182	94.9	48.2 144.6
145	26.8	15.9 47.6

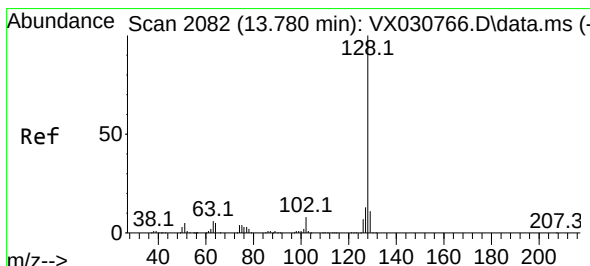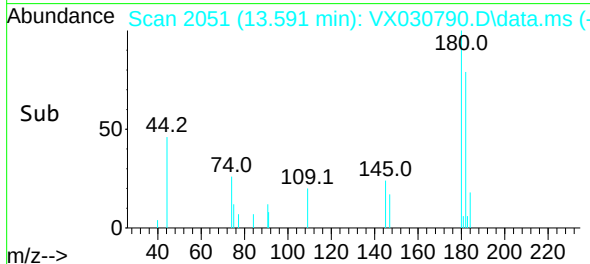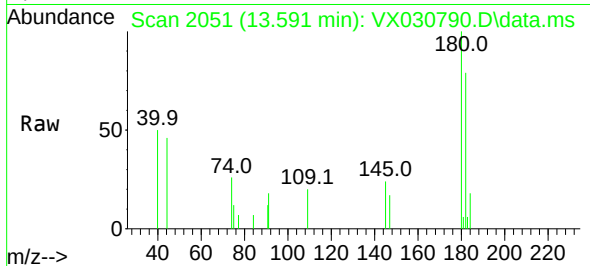

#95
Naphthalene
Concen: 0.224 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX030790.D
Acq: 25 Aug 2022 23:28


Tgt Ion:128	Resp:	2426
Ion	Ratio	Lower Upper
128	100	
127	13.3	10.2 15.2
129	9.1	8.6 13.0

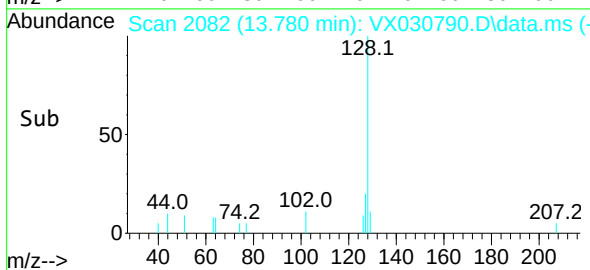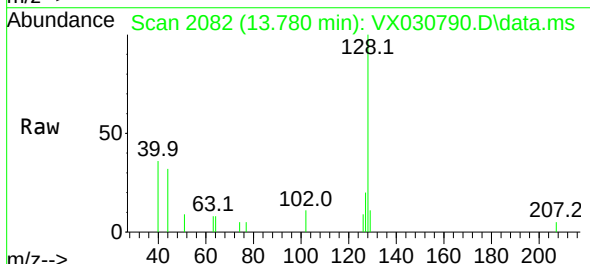



#96
 1,2,3-Trichlorobenzene
 Concen: 0.248 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. -0.000 min
 Lab File: VX030790.D
 Acq: 25 Aug 2022 23:28

Instrument :
 MSVOA_X
 ClientSampleId :
 MW179D2-20220816DL

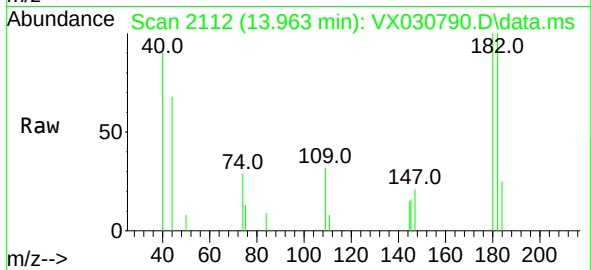

Tgt Ion:	180	Resp:	816
Ion	Ratio	Lower	Upper
180	100		
182	106.0	47.0	141.0
145	26.6	17.0	50.9

