



Chloromethane

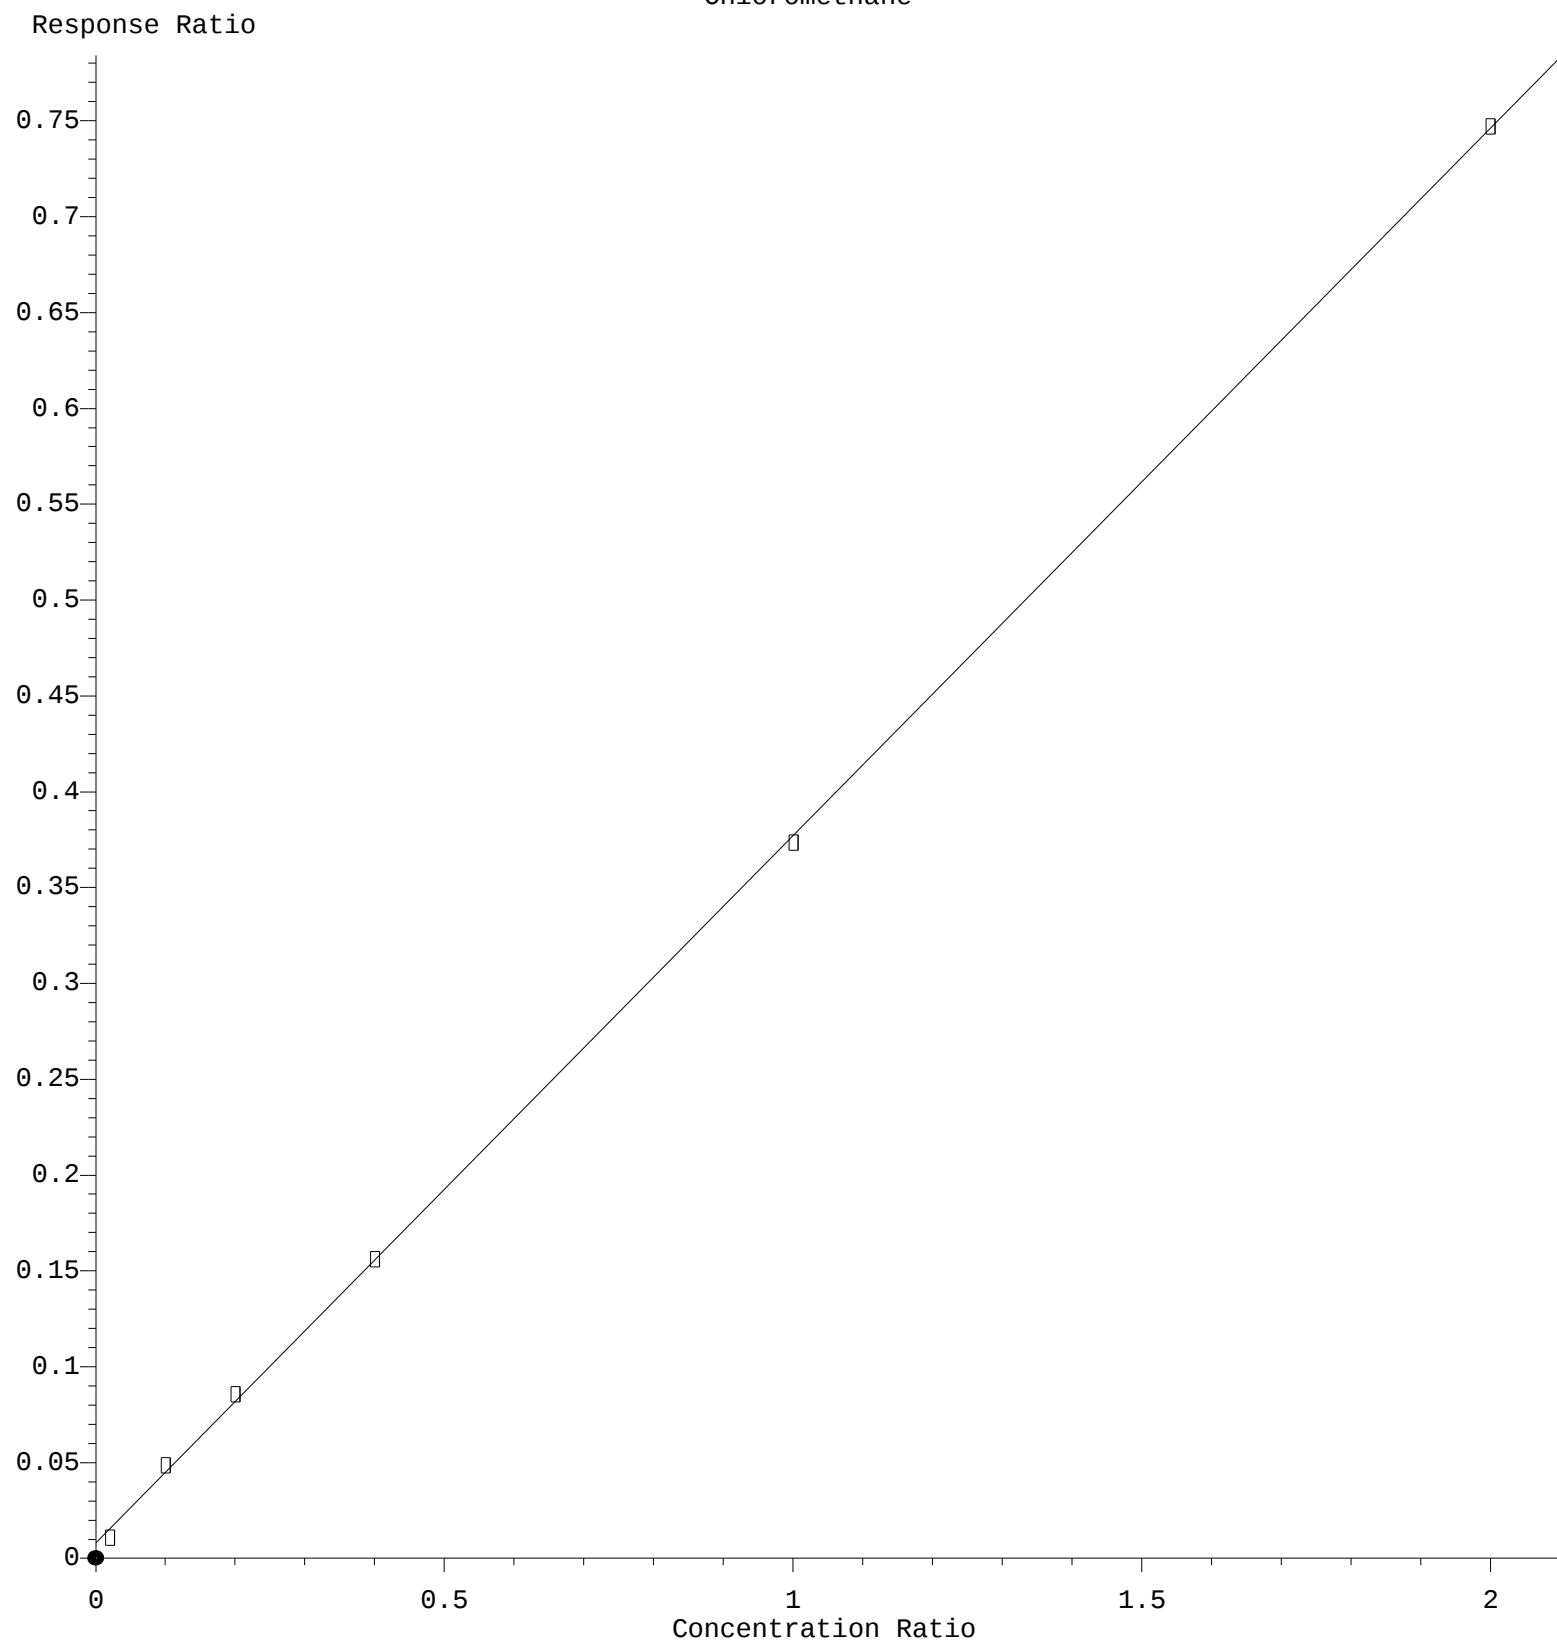

Response = $3.688 \times 10^{-1} \times \text{Amt} + 8.212 \times 10^{-3}$
Coef of Det (r^2) = 0.999846 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Calibration Table Last Updated: Fri Aug 26 02:03:28 2022

Vinyl Chloride

Response Ratio

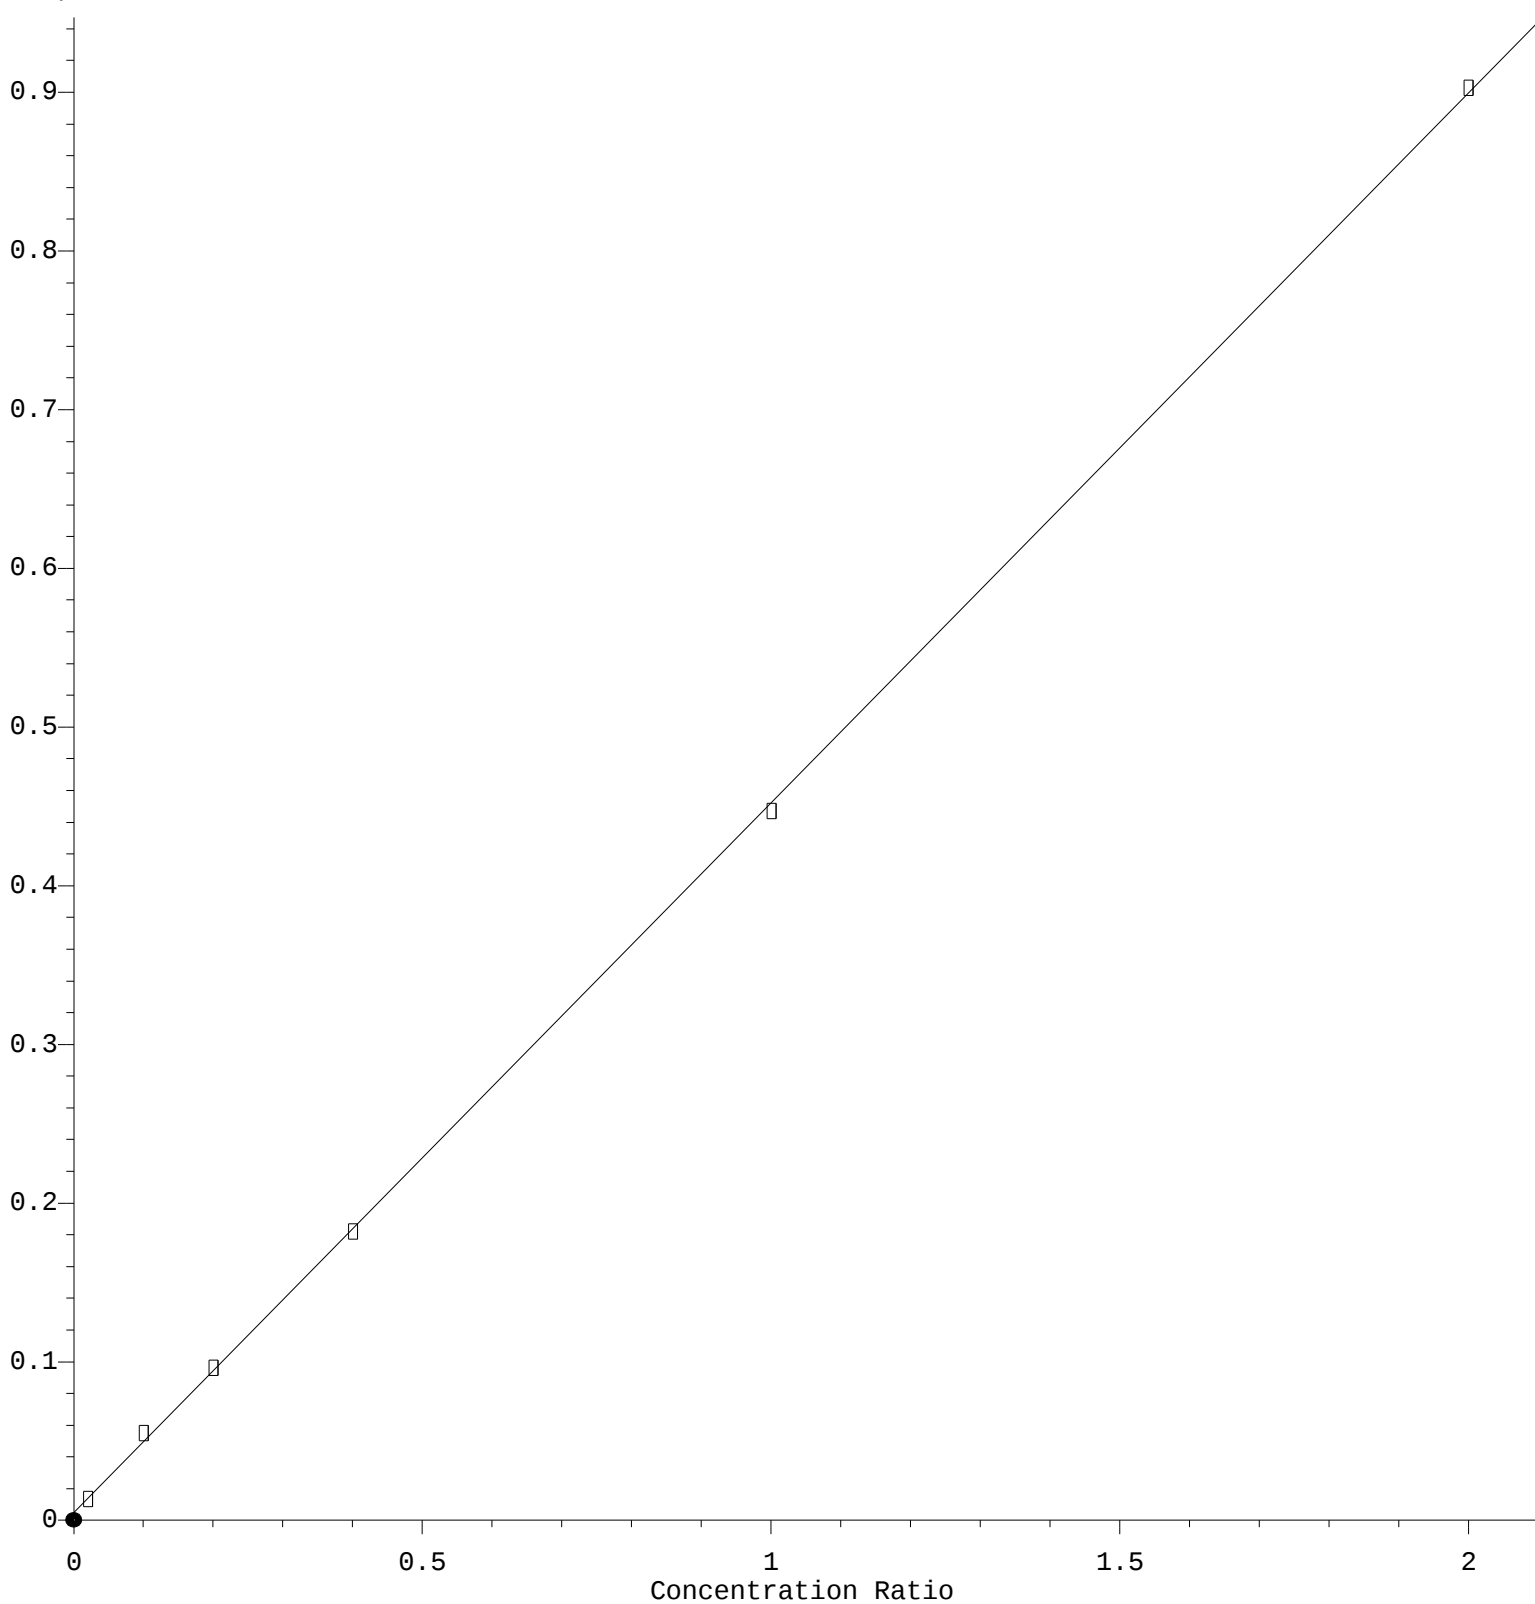


$$\text{Response} = 4.472\text{e-}001 * \text{Amt} + 5.265\text{e-}003$$

Coef of Det (r^2) = 0.999881 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Calibration Table Last Updated: Fri Aug 26 02:03:28 2022


Chloroethane

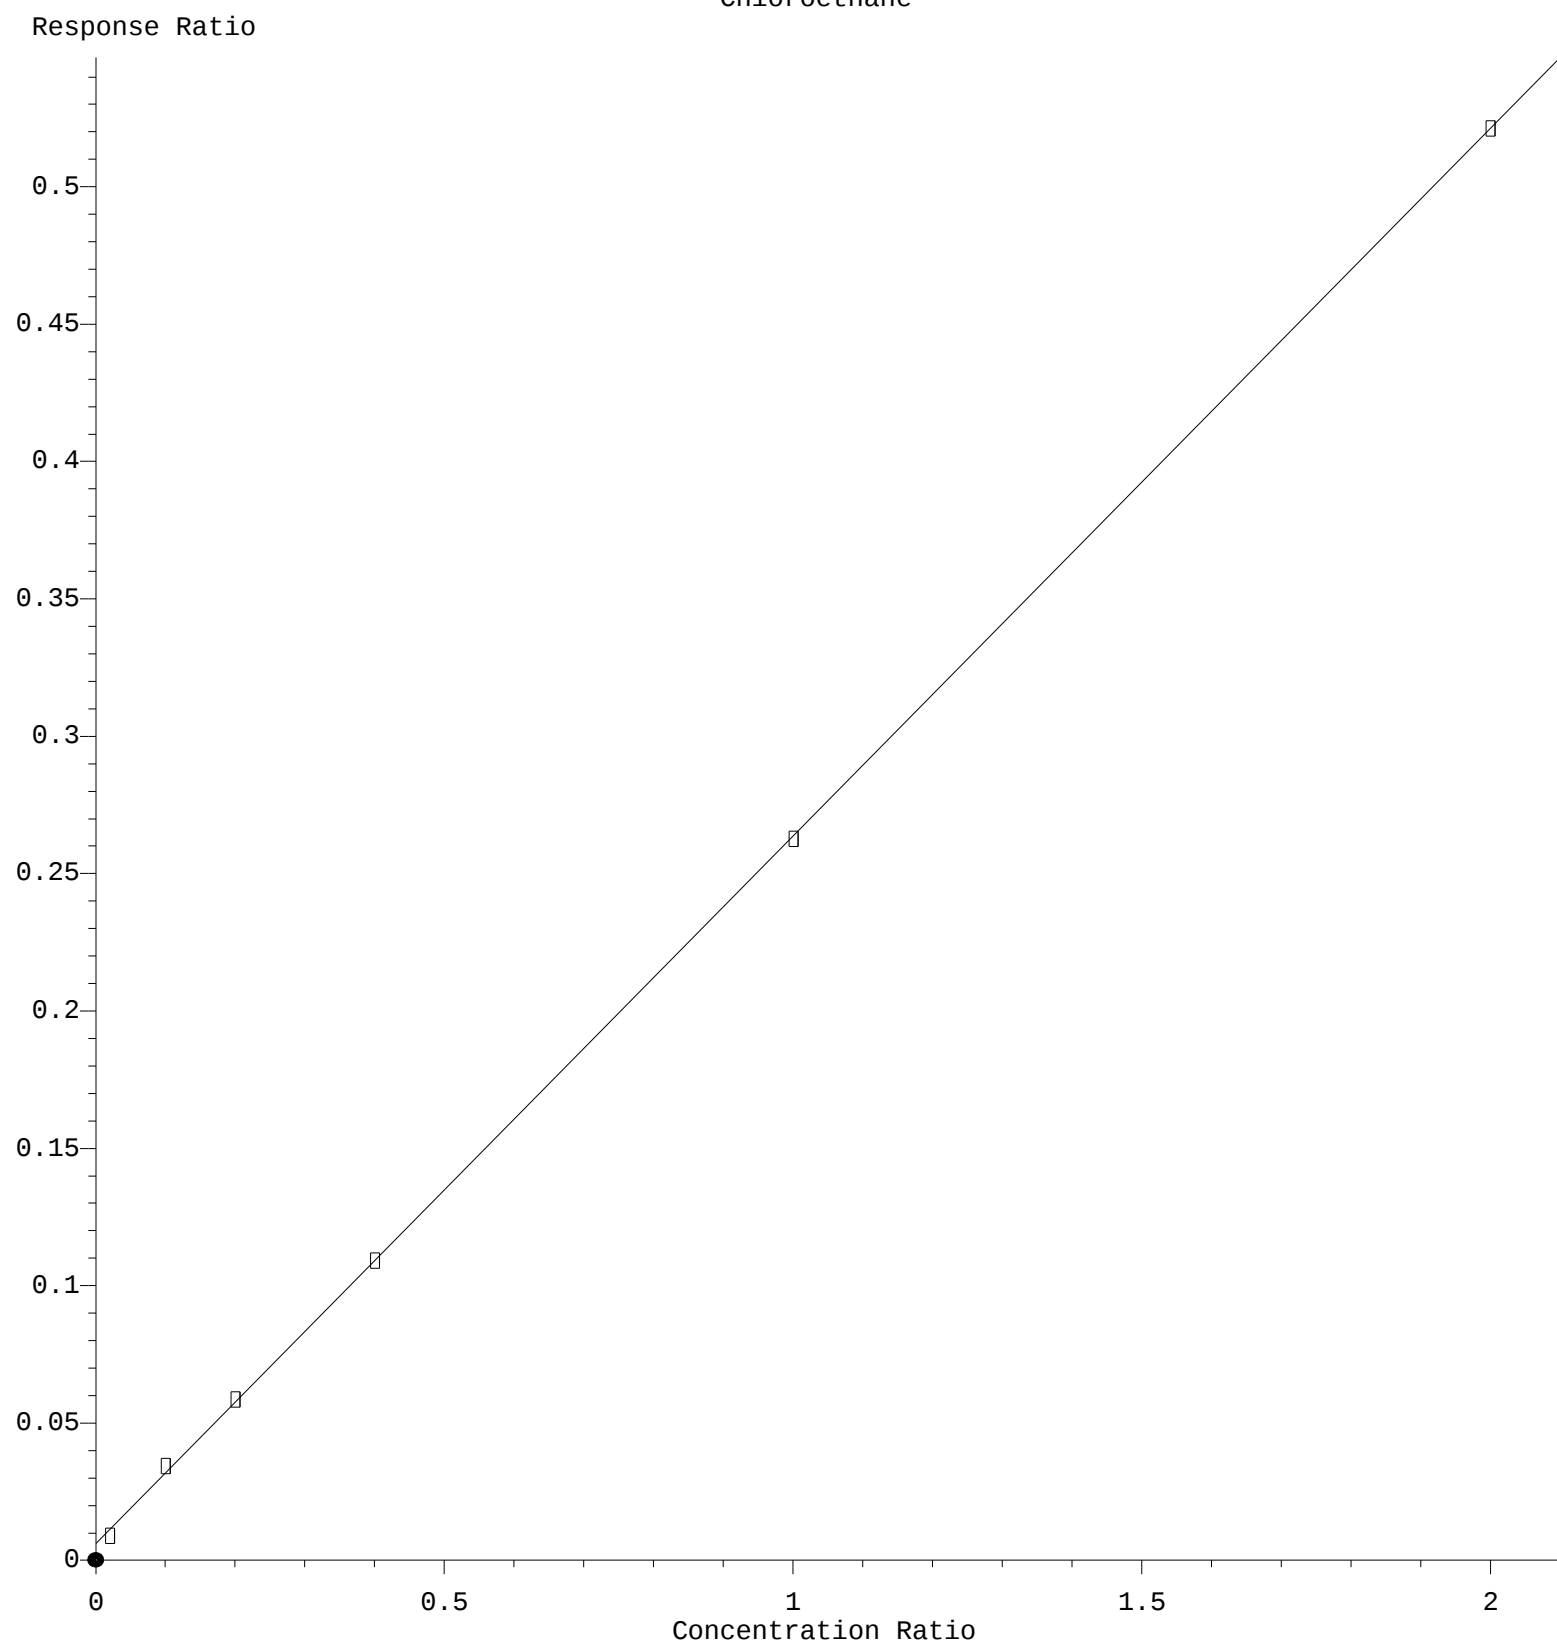

Response = $2.573 \times 10^{-1} \times \text{Amt} + 6.177 \times 10^{-3}$
Coef of Det (r^2) = 0.999931 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Calibration Table Last Updated: Fri Aug 26 02:03:28 2022

Methyl Iodide

Response Ratio

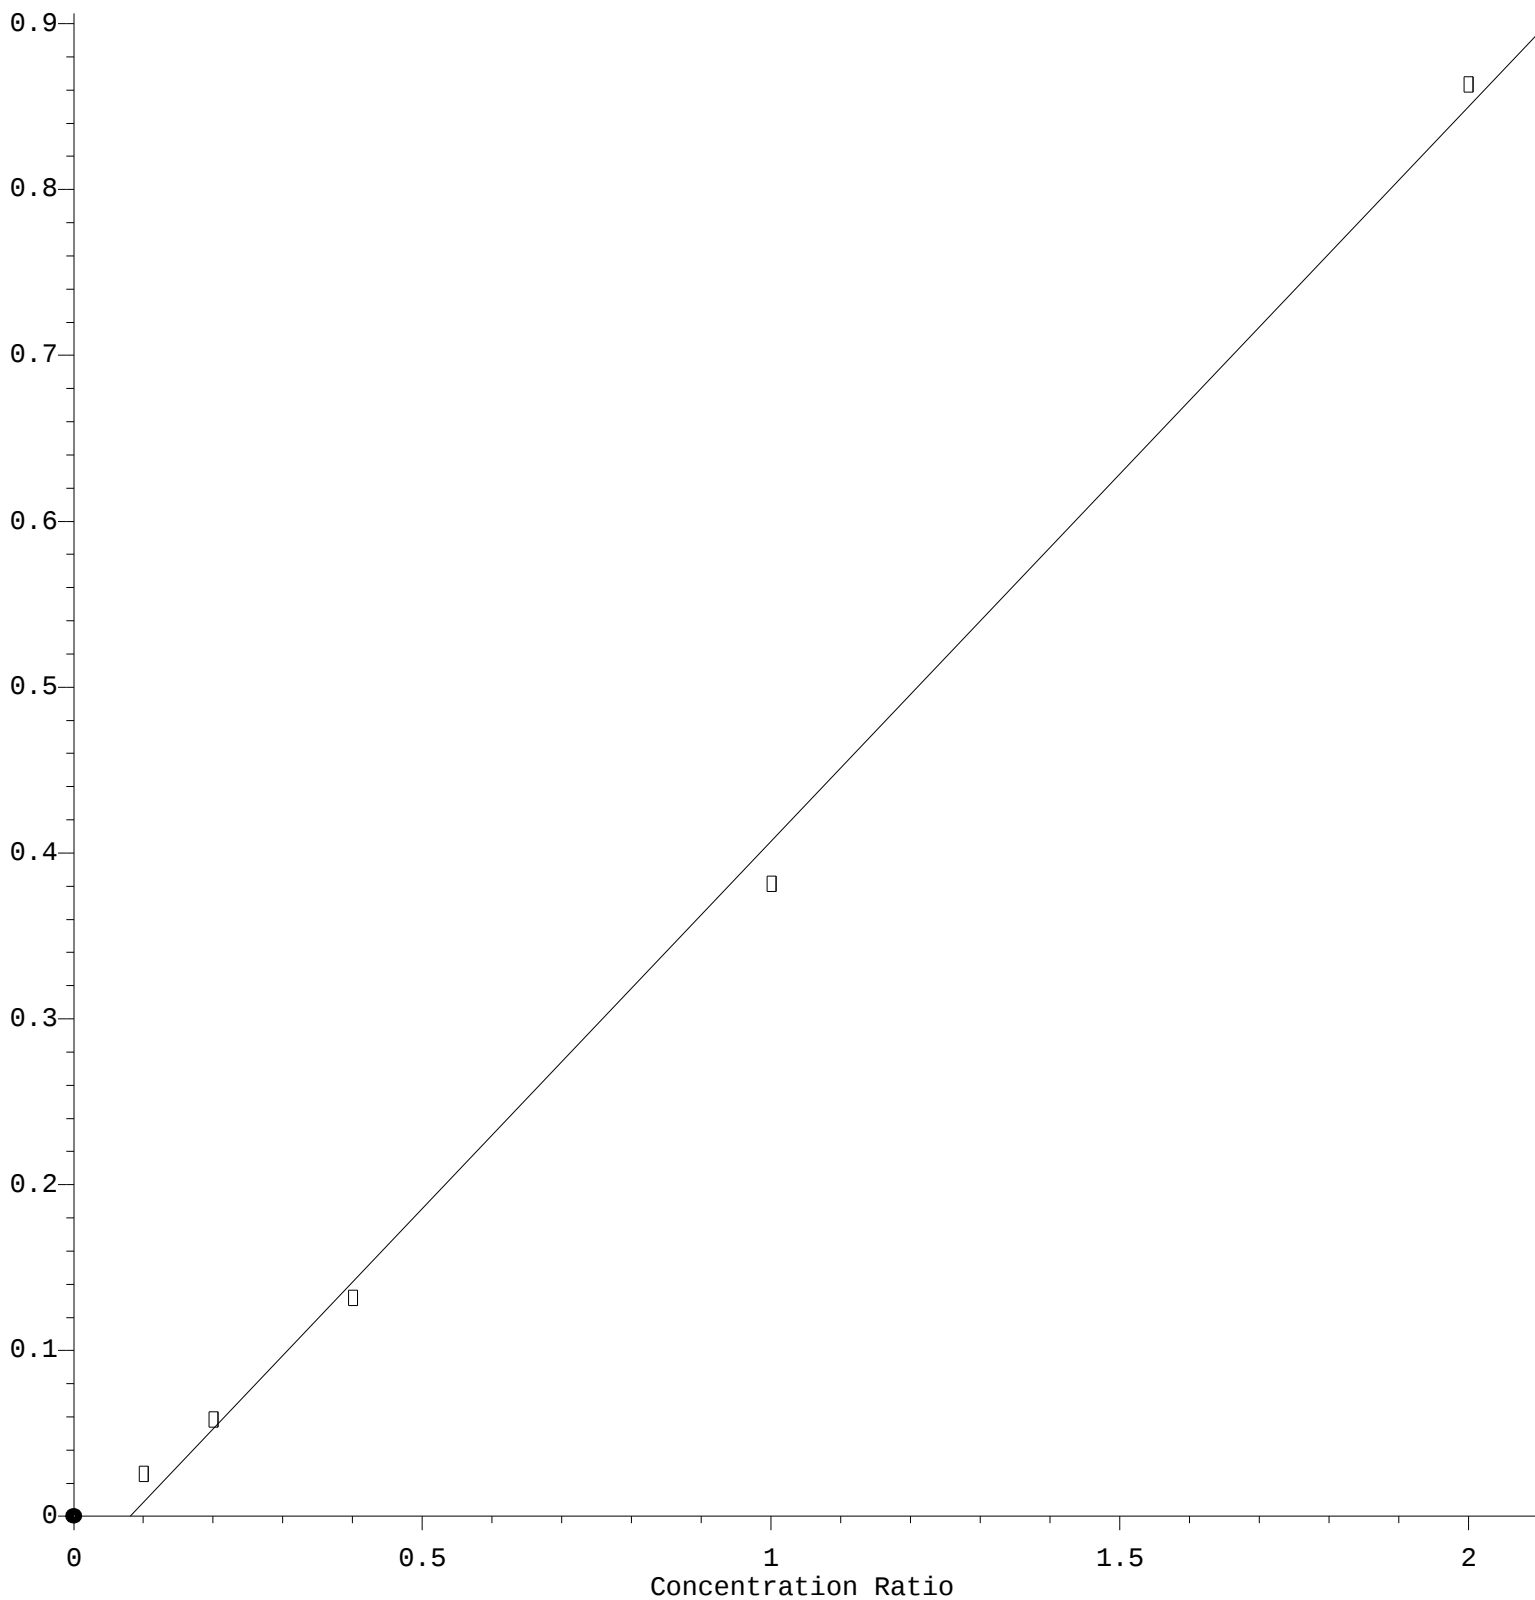

$$\text{Response} = 4.426\text{e-}001 * \text{Amt} - 3.567\text{e-}002$$


Coef of Det (r^2) = 0.997407 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Calibration Table Last Updated: Fri Aug 26 02:03:28 2022

Acrolein

Response Ratio

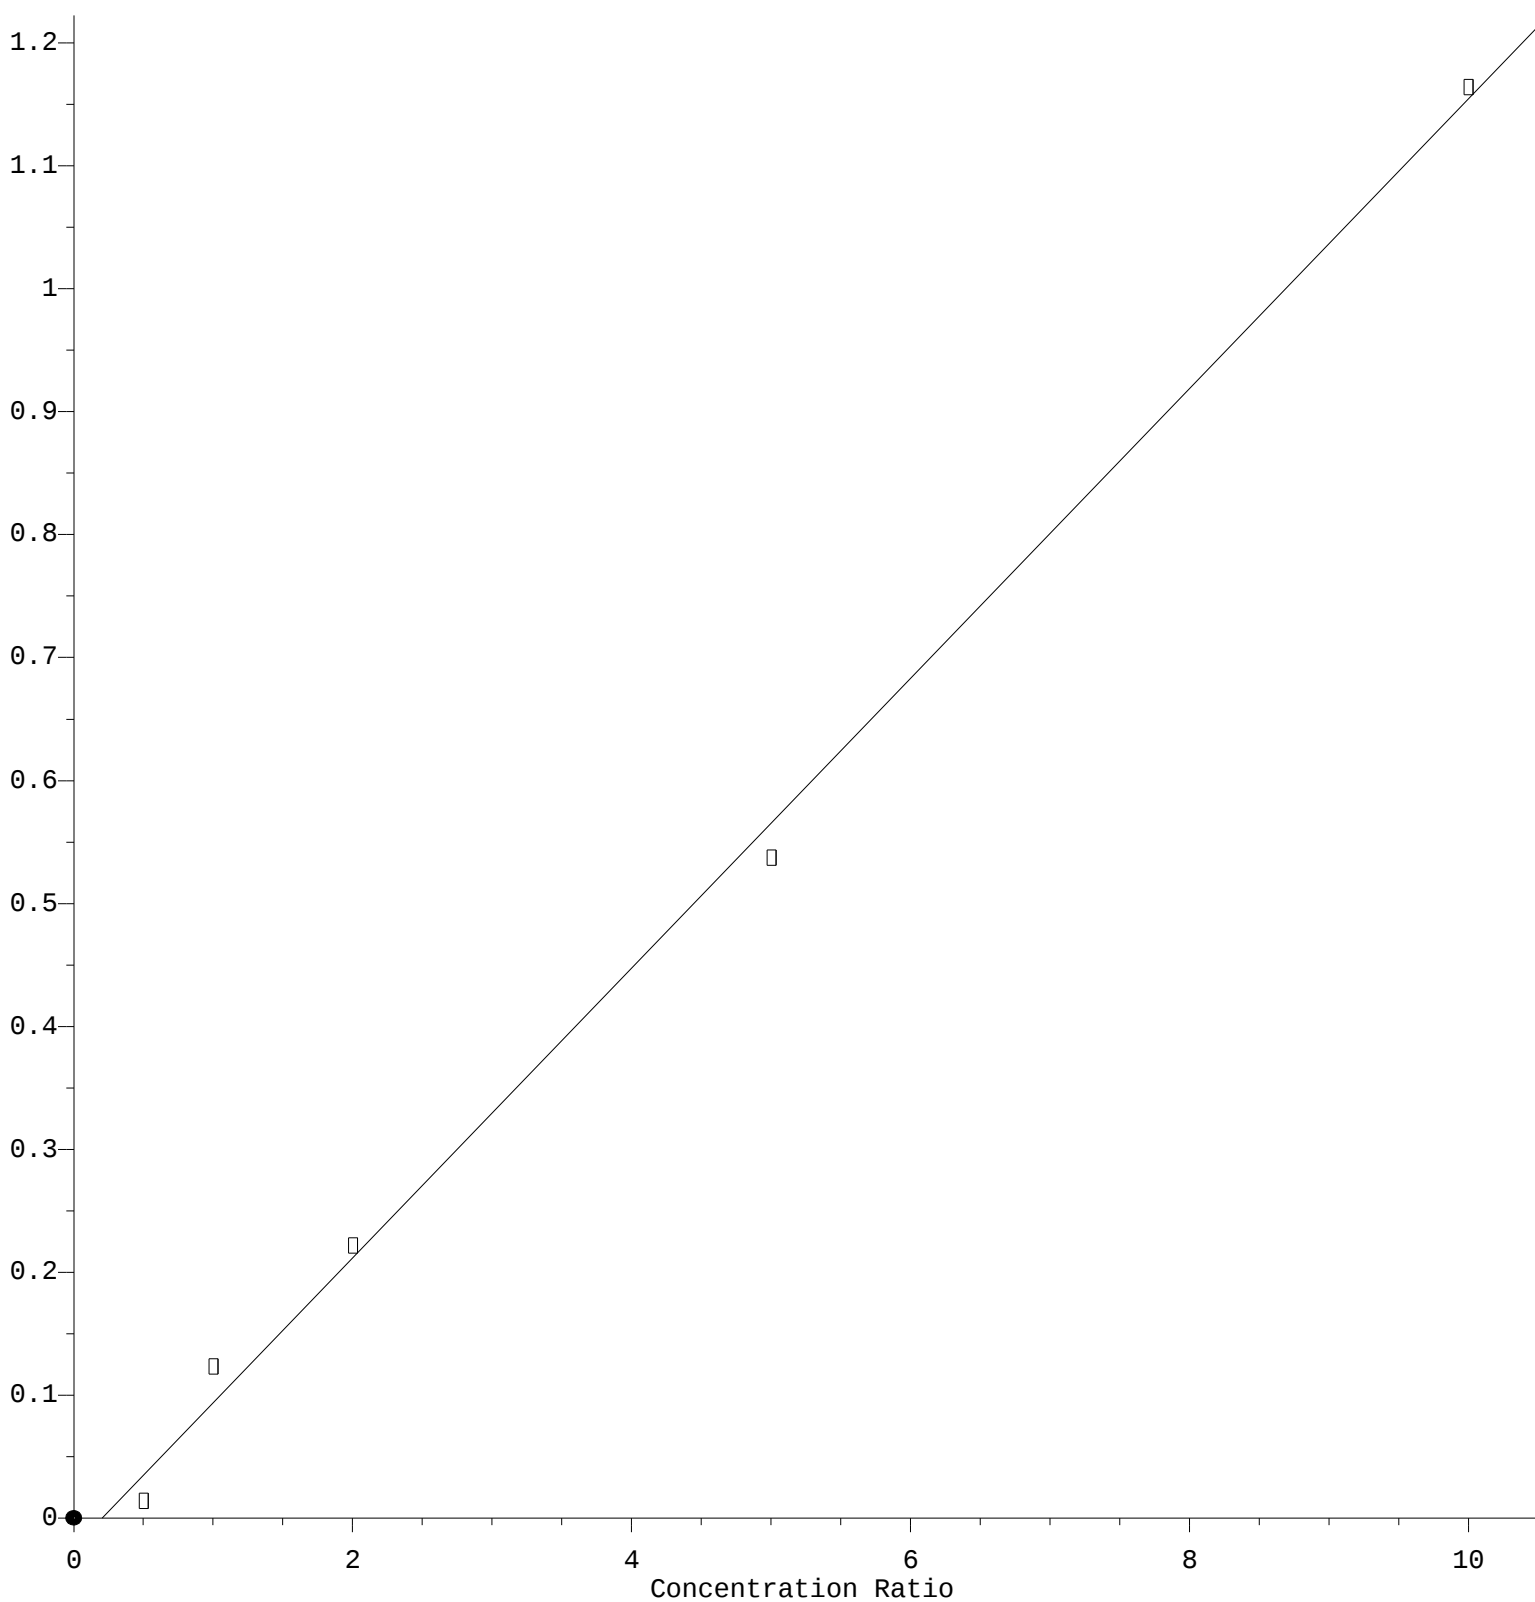

$$\text{Response} = 1.177\text{e-}001 * \text{Amt} - 2.367\text{e-}002$$


Coef of Det (r^2) = 0.997349 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Calibration Table Last Updated: Fri Aug 26 02:03:28 2022

Acetone

Response Ratio

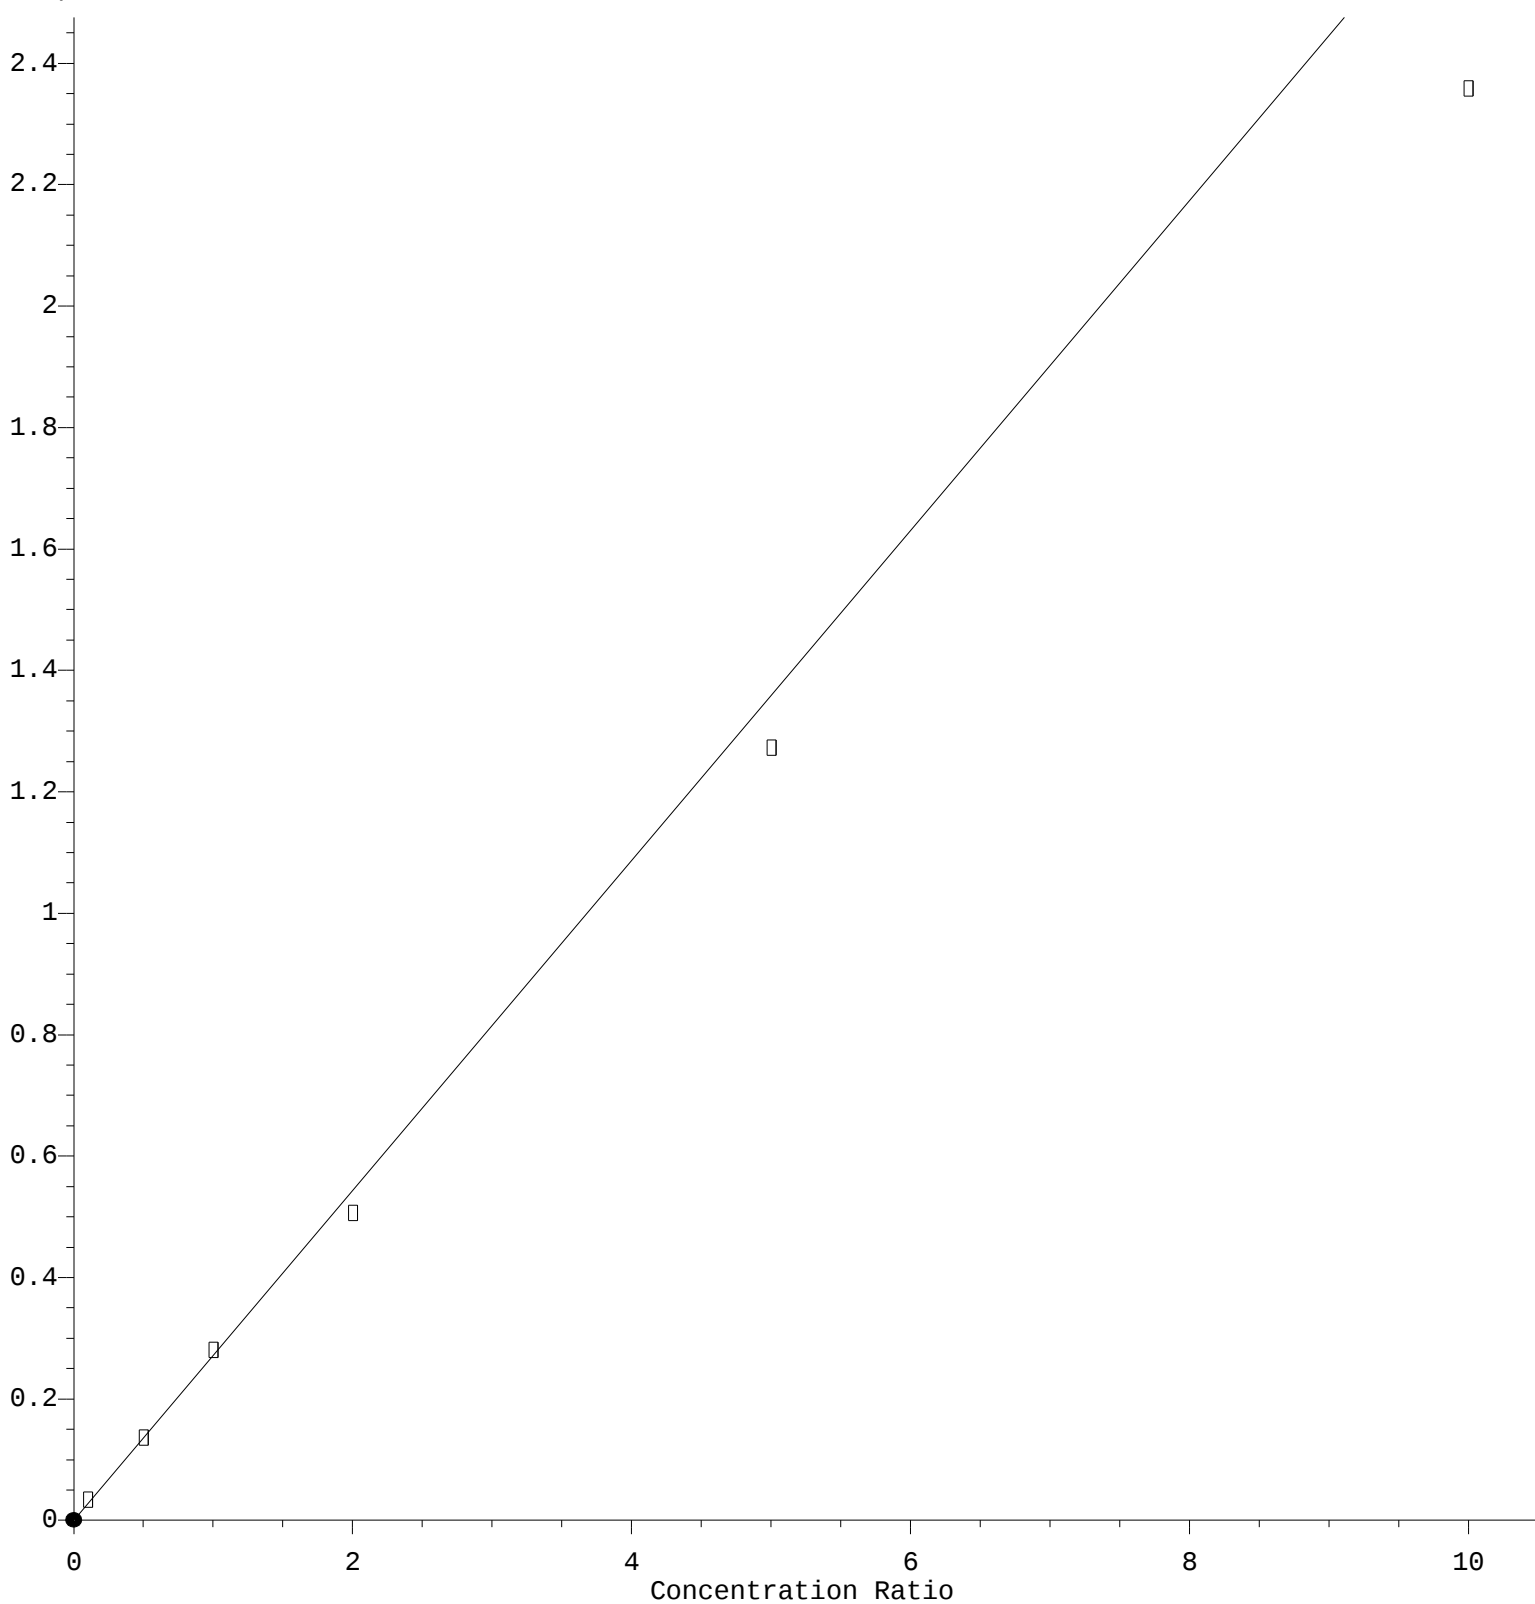

$$\text{Response} = 2.718\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 12.831% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Calibration Table Last Updated: Fri Aug 26 02:03:28 2022

Carbon Disulfide

Response Ratio

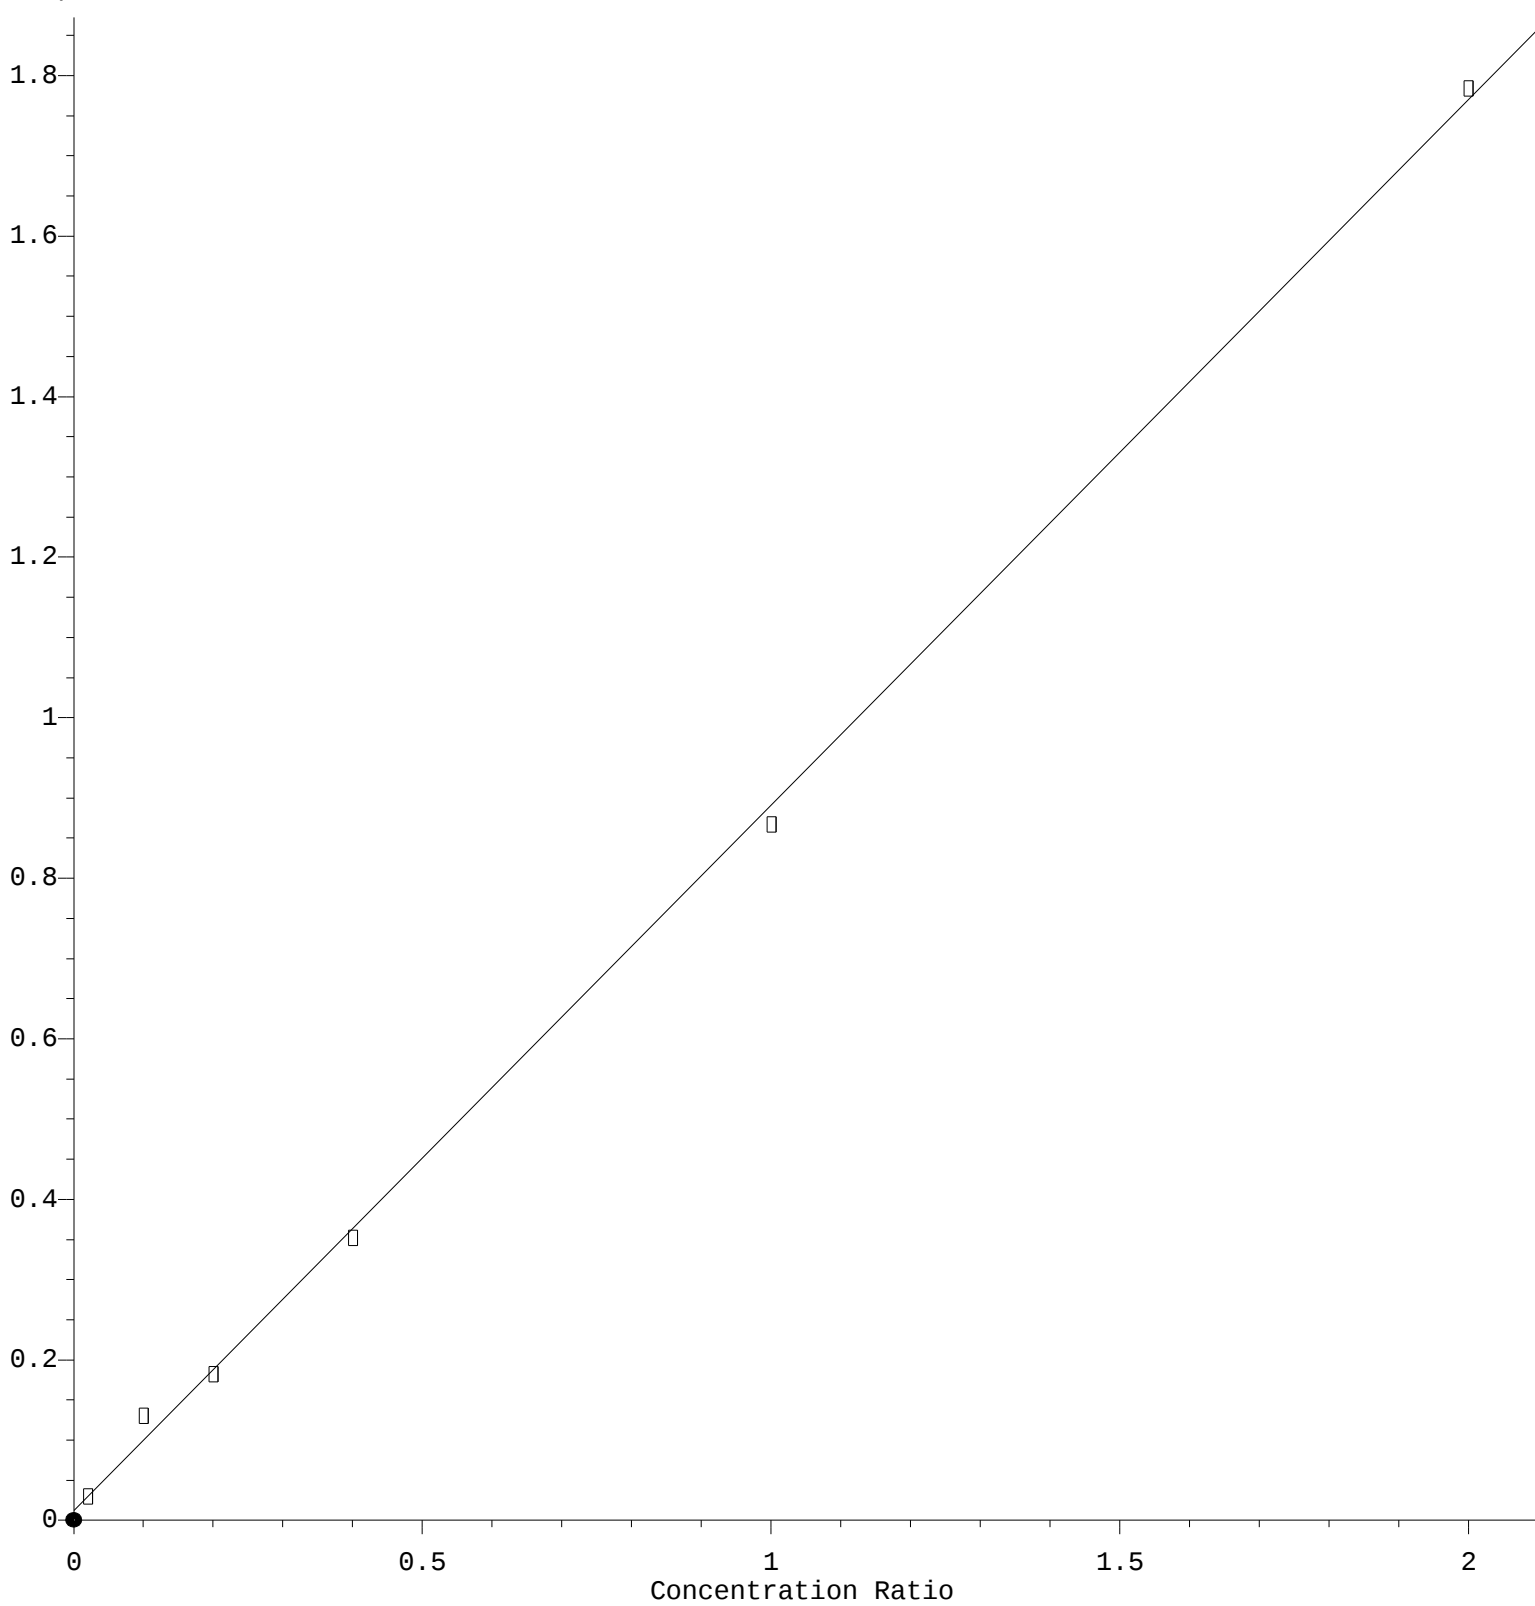

$$\text{Response} = 8.786\text{e-}001 * \text{Amt} + 1.242\text{e-}002$$


Coef of Det (r^2) = 0.999160 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Calibration Table Last Updated: Fri Aug 26 02:03:28 2022

Methylene Chloride

Response Ratio

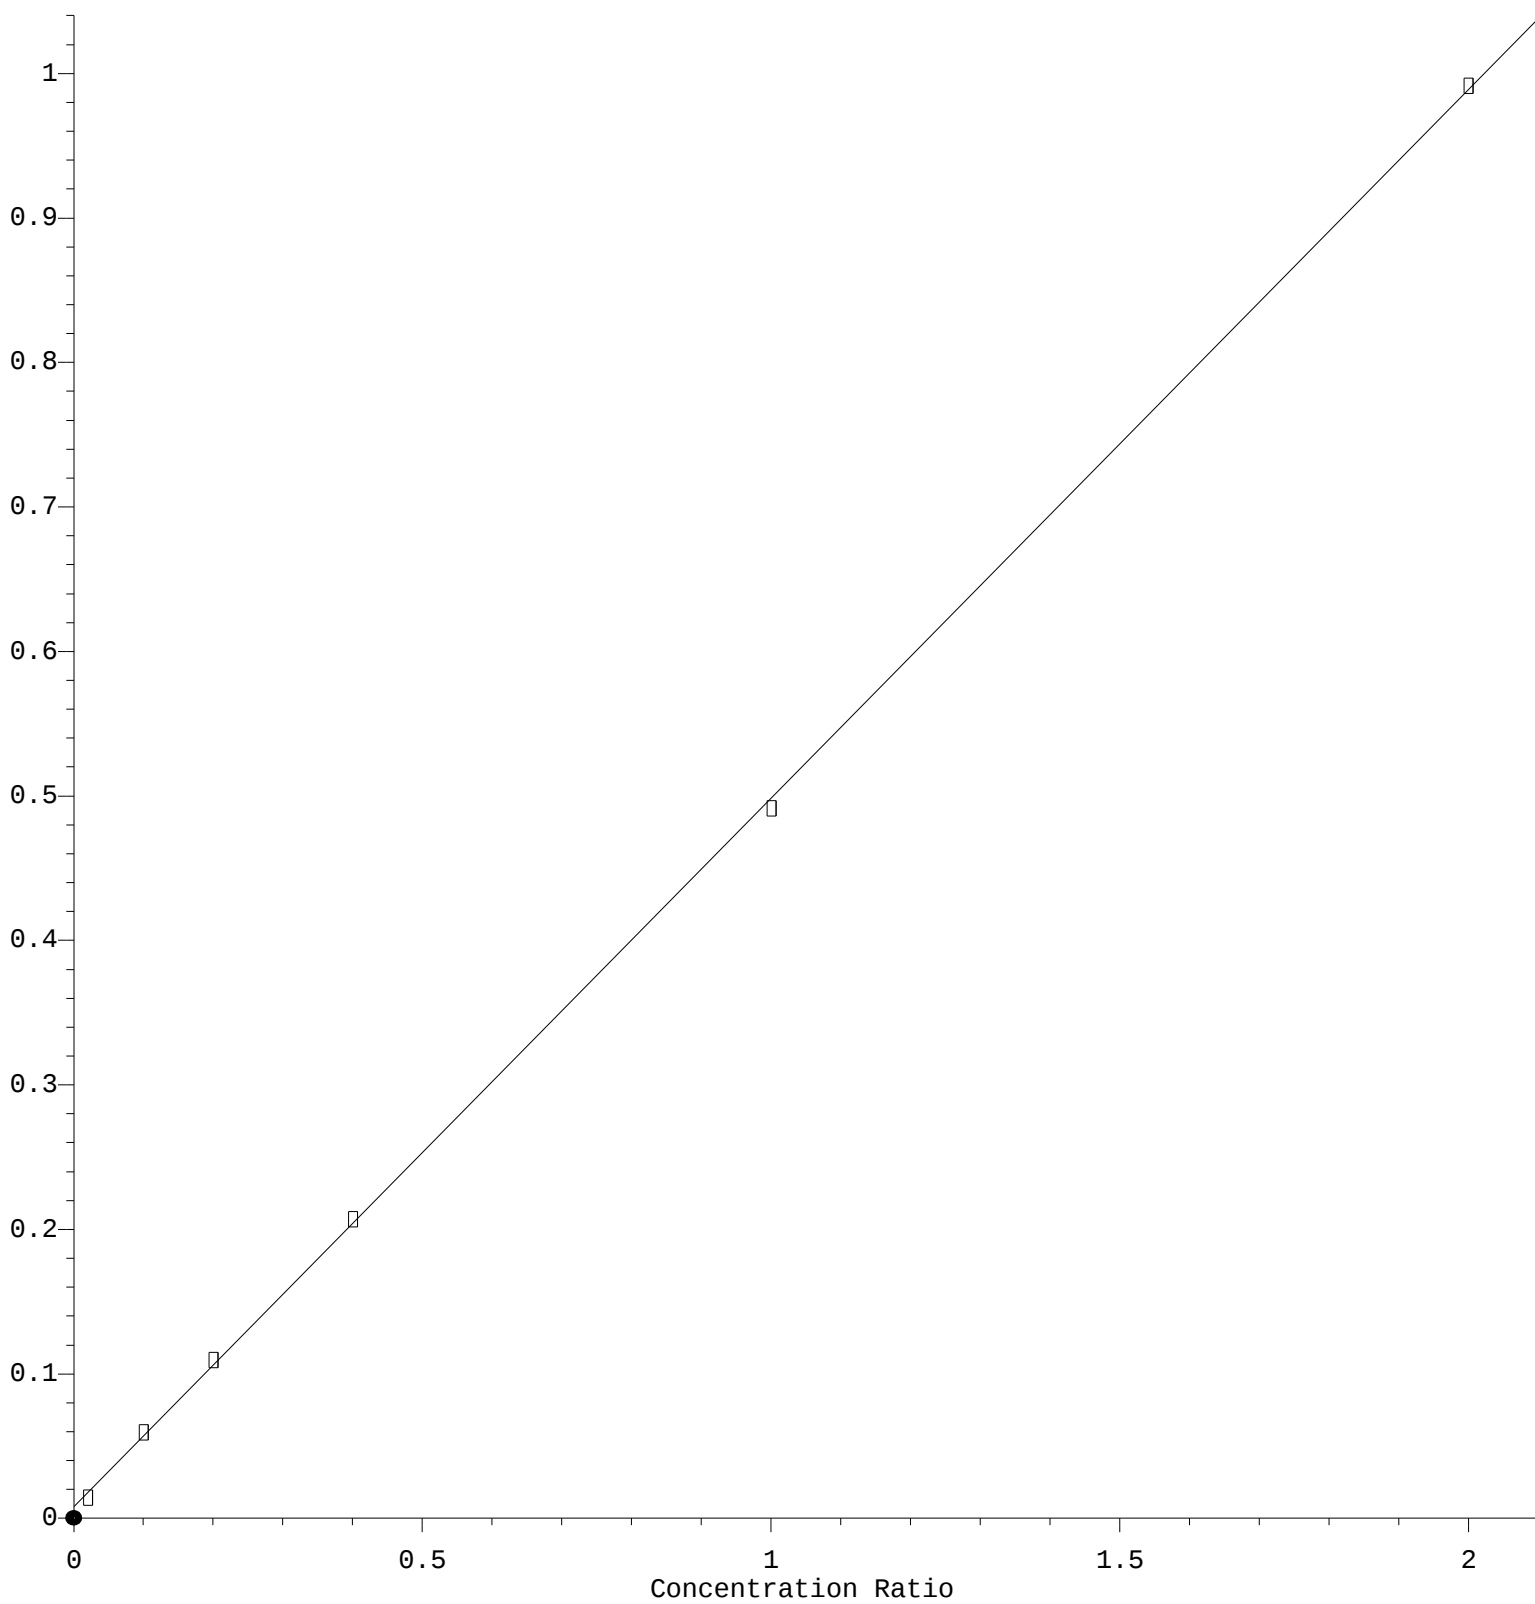

$$\text{Response} = 4.903\text{e-}001 * \text{Amt} + 8.024\text{e-}003$$

Coef of Det (r^2) = 0.999863 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Calibration Table Last Updated: Fri Aug 26 02:03:28 2022