

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
 Data File : VX030774.D
 Acq On : 25 Aug 2022 16:24
 Operator : JC/MD
 Sample : N4266-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Aug 26 02:40:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	235114	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	391409	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	348949	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	150719	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	137642	49.770	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.540%
35) Dibromofluoromethane	5.385	113	118275	49.168	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.340%
50) Toluene-d8	8.647	98	450452	53.737	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	107.480%
62) 4-Bromofluorobenzene	11.085	95	152685	48.925	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030774.D
Acq On : 25 Aug 2022 16:24
Operator : JC/MD
Sample : N4266-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Aug 26 02:40:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 26 02:03:28 2022
Response via : Initial Calibration




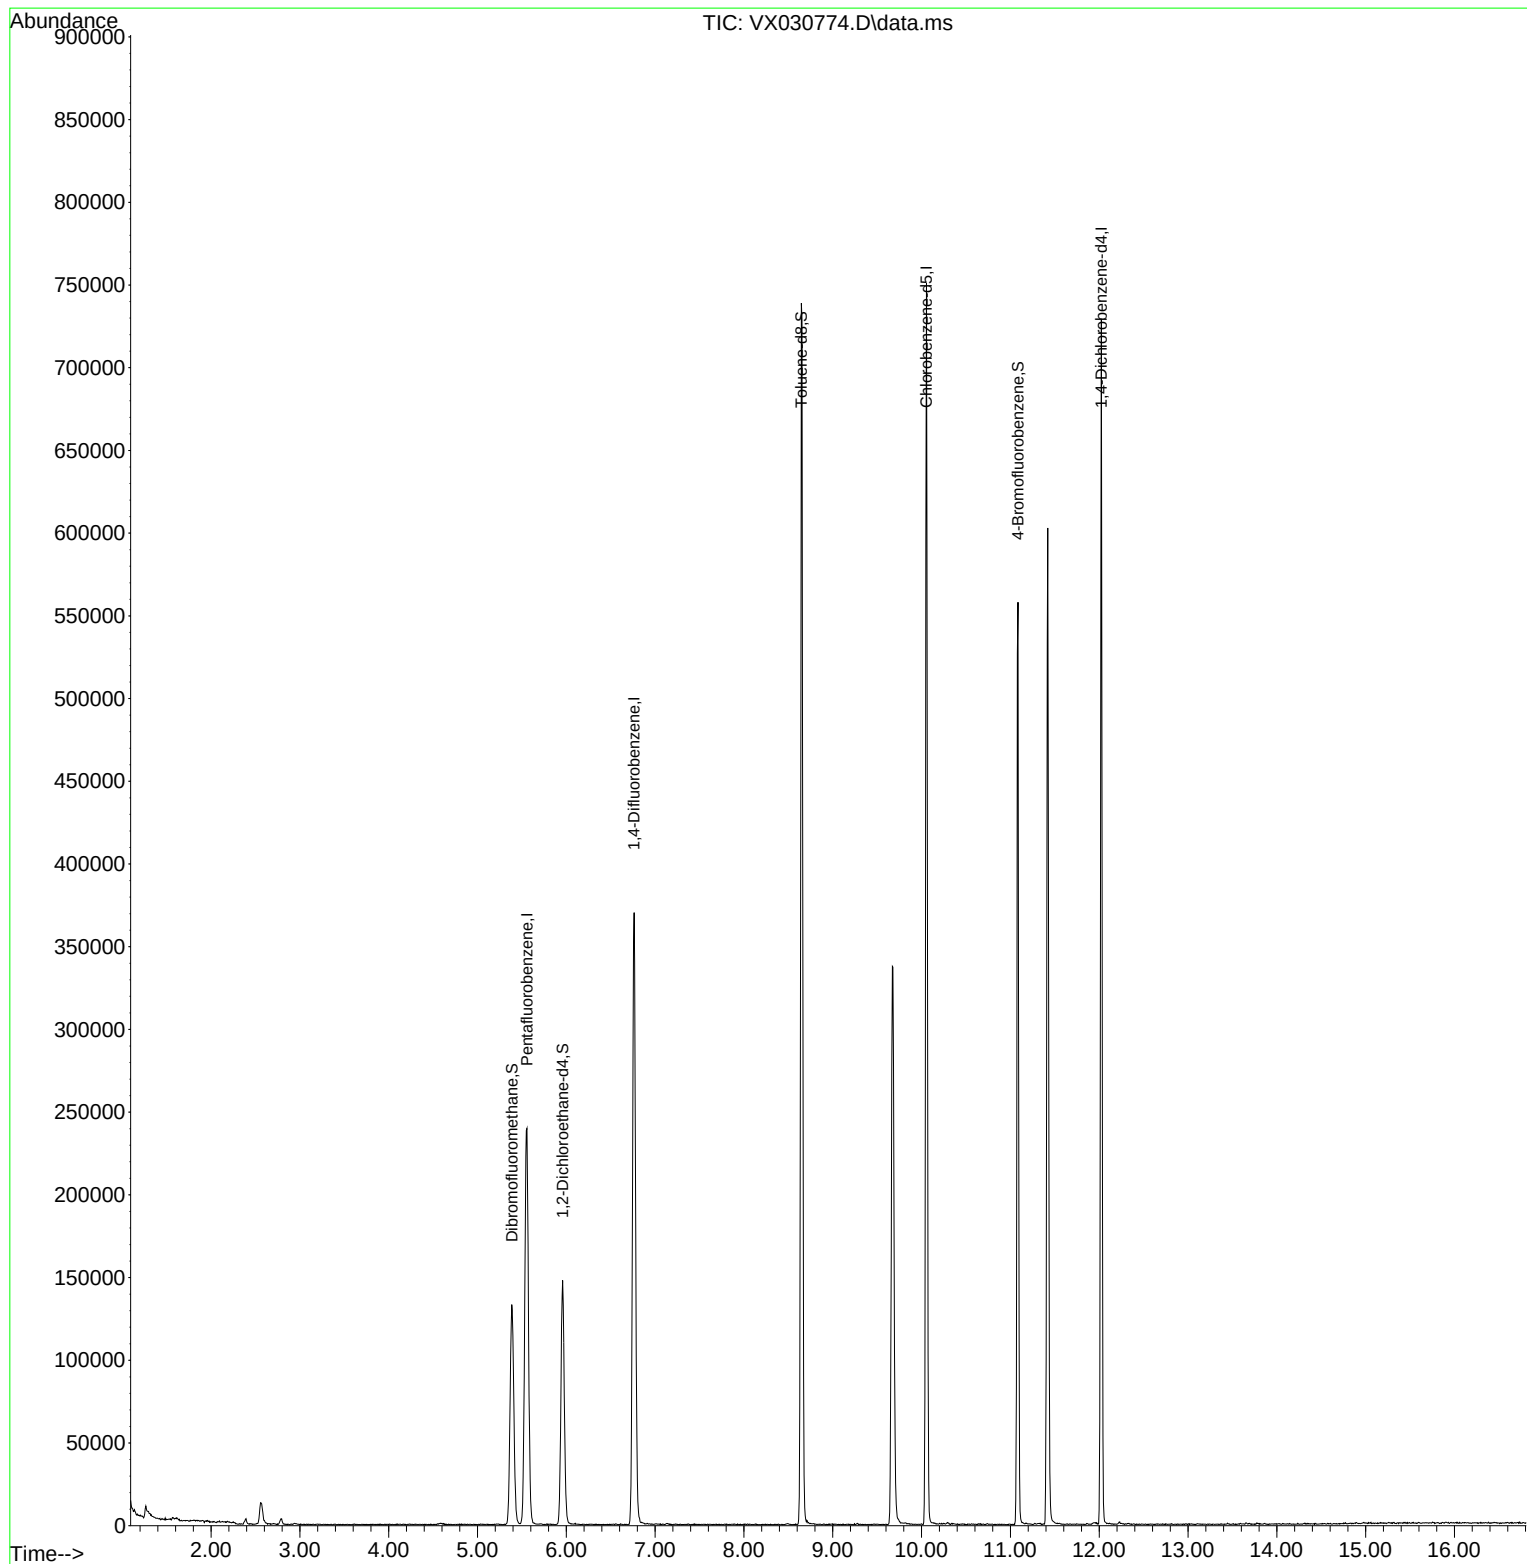


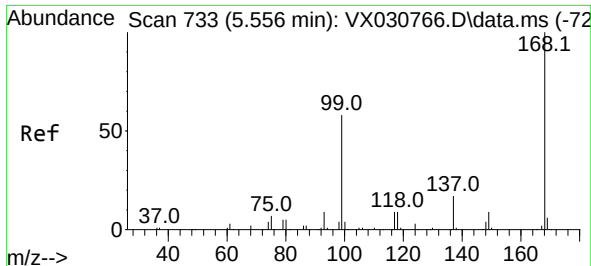

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 235114
Ion Ratio Lower Upper
168 100
99 56.1 44.0 66.0

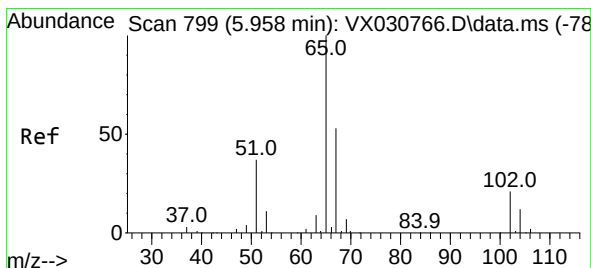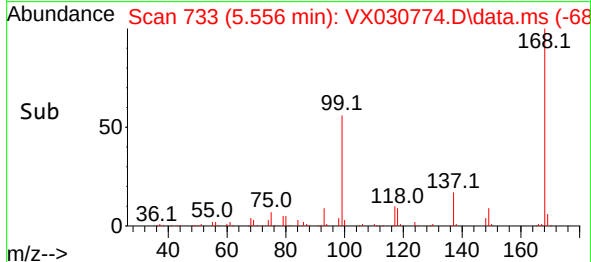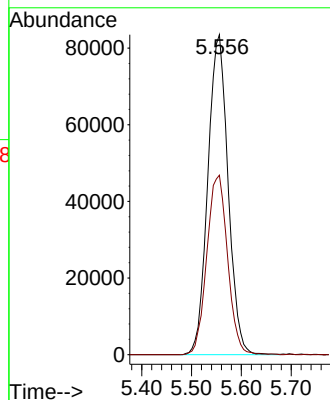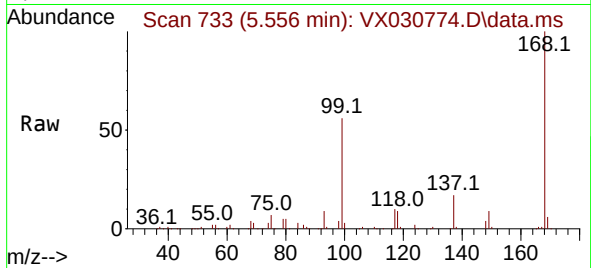

#33
1,2-Dichloroethane-d4
Concen: 49.770 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24

Tgt Ion: 65 Resp: 137642
Ion Ratio Lower Upper
65 100
67 54.2 0.0 109.6


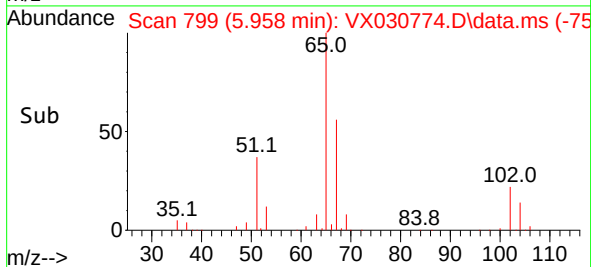
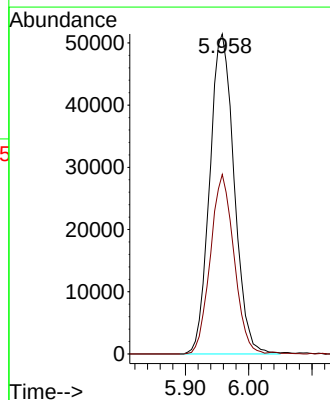
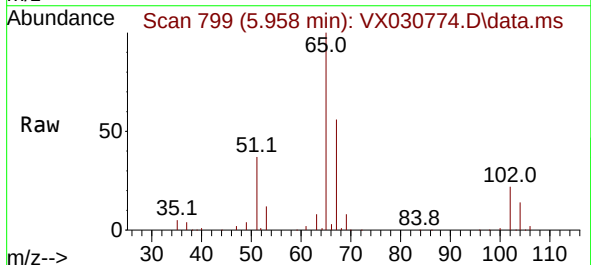


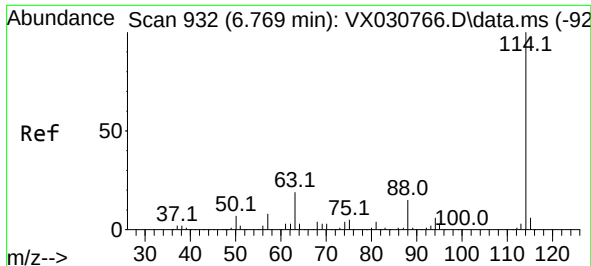

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:114 Resp: 391409
Ion Ratio Lower Upper
114 100
63 19.8 0.0 38.4
88 14.6 0.0 31.8

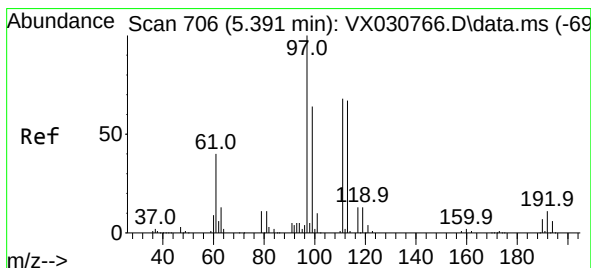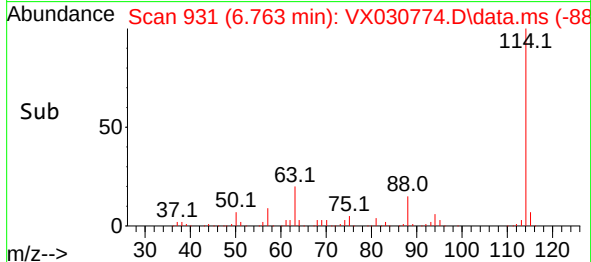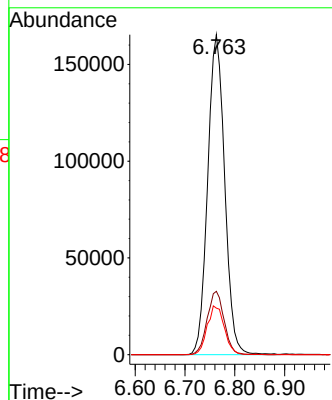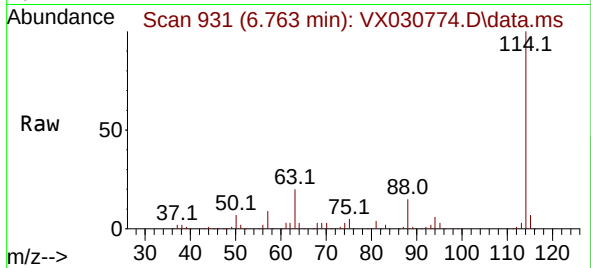

#35
Dibromofluoromethane
Concen: 49.168 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24

Tgt Ion:113 Resp: 118275
Ion Ratio Lower Upper
113 100
111 104.2 83.2 124.8
192 19.7 14.8 22.2


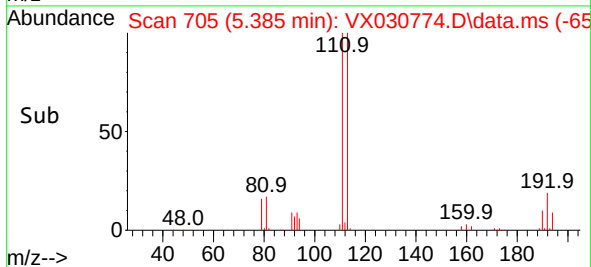
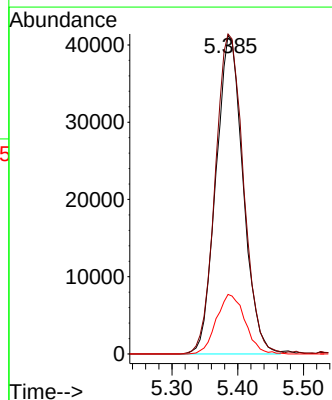
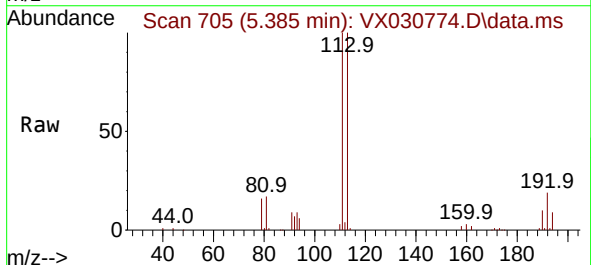


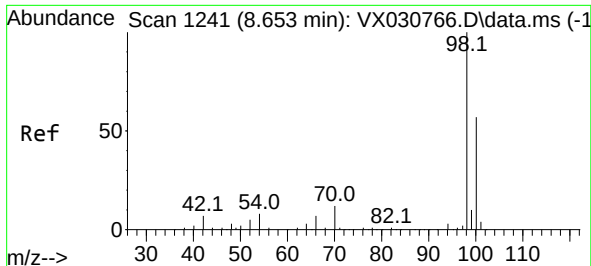

#50
Toluene-d8
Concen: 53.737 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 450452
Ion Ratio Lower Upper
98 100
100 64.2 52.3 78.5

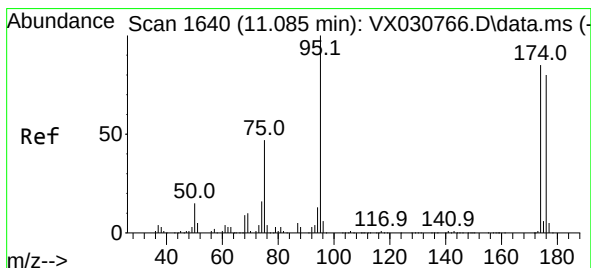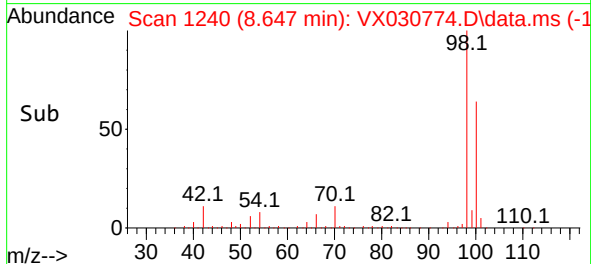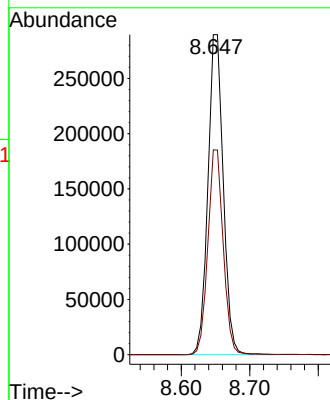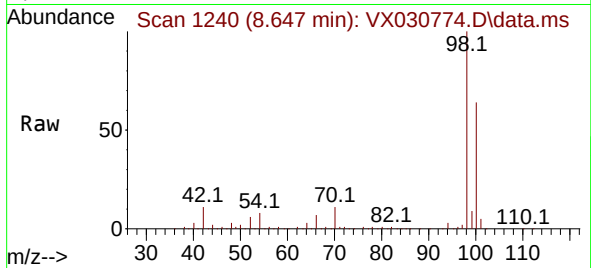

#62
4-Bromofluorobenzene
Concen: 48.925 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24

Tgt Ion: 95 Resp: 152685
Ion Ratio Lower Upper
95 100
174 79.6 0.0 149.0
176 75.8 0.0 146.0


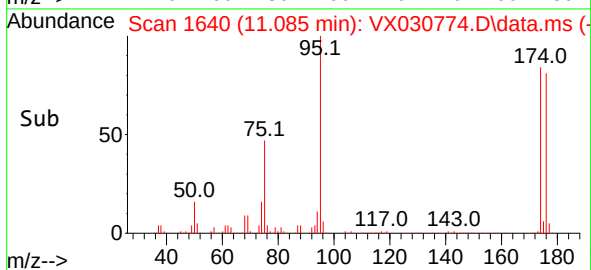
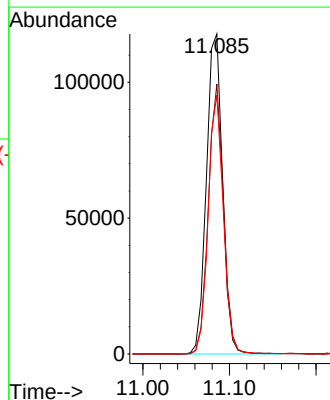
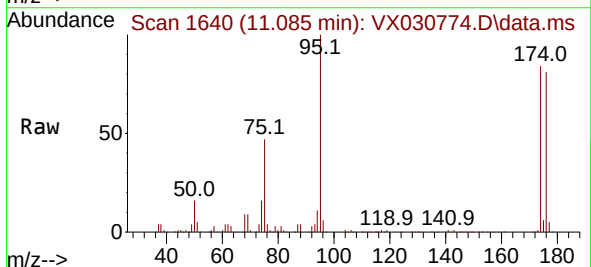


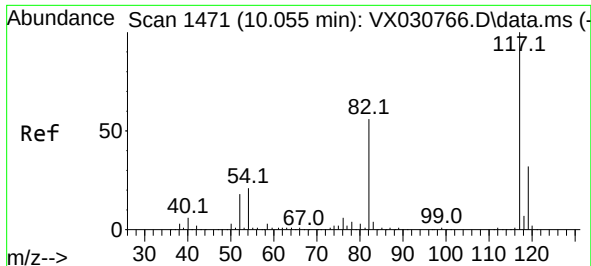

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 348949
Ion Ratio Lower Upper
117 100
82 55.0 42.7 64.1
119 33.1 25.4 38.2

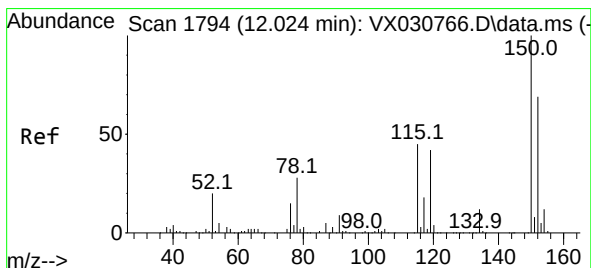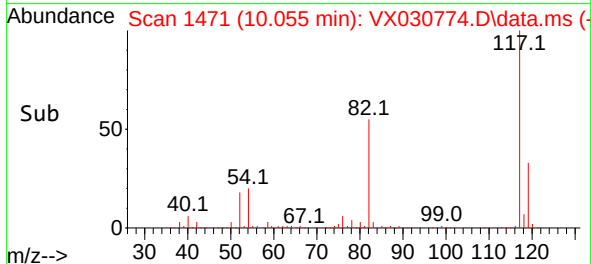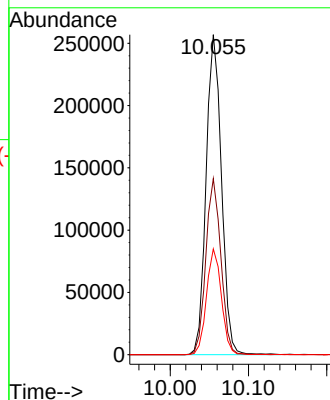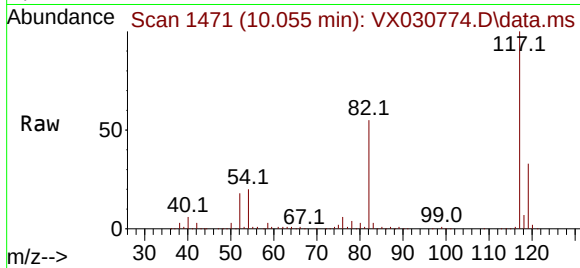

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030774.D
Acq: 25 Aug 2022 16:24

Tgt Ion:152 Resp: 150719
Ion Ratio Lower Upper
152 100
115 59.2 40.5 121.5
150 156.1 0.0 347.0

