

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
 Data File : VX030796.D
 Acq On : 26 Aug 2022 01:50
 Operator : JC/MD
 Sample : N4245-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE117D1-20220816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Title : SW846 8260

Signal : TIC: VX030796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.319	198	202	209	rBV3	12670	23879	1.57%	0.316%
2	5.391	693	706	721	rBV	133136	391277	25.73%	5.184%
3	5.556	721	733	746	rVV2	239822	677328	44.54%	8.973%
4	5.684	746	754	762	rVB4	5114	15939	1.05%	0.211%
5	5.964	788	800	814	rBV	145729	384607	25.29%	5.095%
6	6.763	921	931	951	rBV	366054	894403	58.81%	11.849%
7	7.129	981	991	1008	rBV	705153	1520867	100.00%	20.149%
8	8.653	1234	1241	1251	rBV	746997	1139073	74.90%	15.091%
9	10.055	1465	1471	1484	rBV	751607	977662	64.28%	12.952%
10	11.085	1634	1640	1651	rBV	543595	687083	45.18%	9.103%
11	12.024	1789	1794	1803	rBV	691153	835998	54.97%	11.076%




Sum of corrected areas: 7548116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030796.D
Acq On : 26 Aug 2022 01:50
Operator : JC/MD
Sample : N4245-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

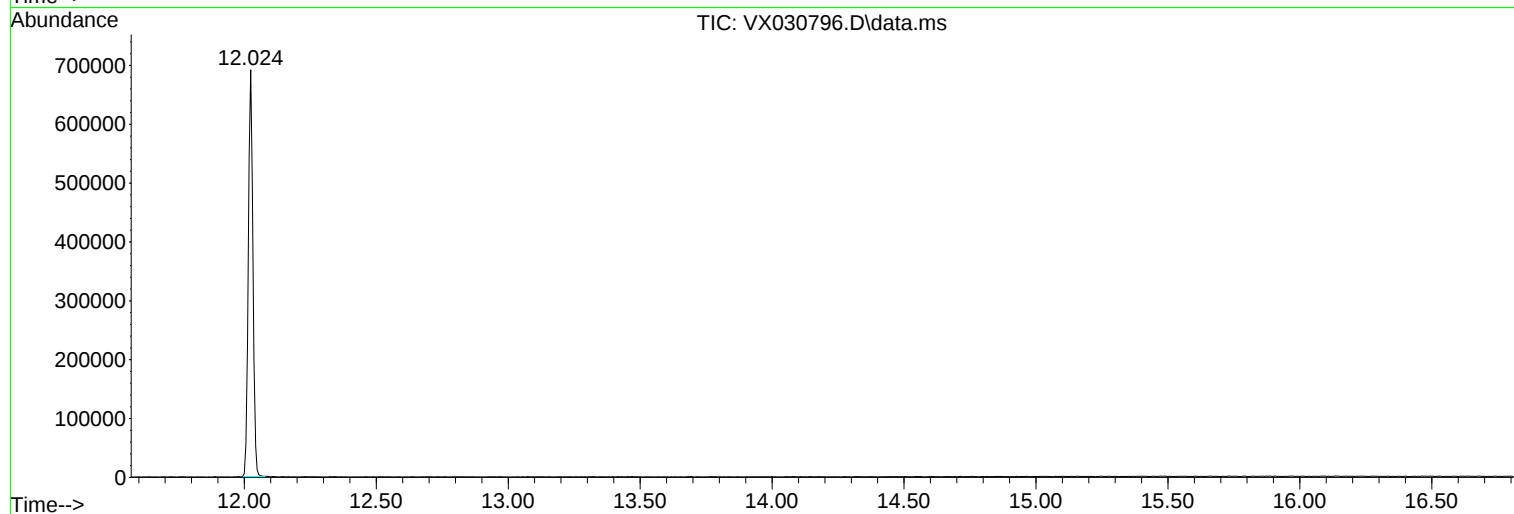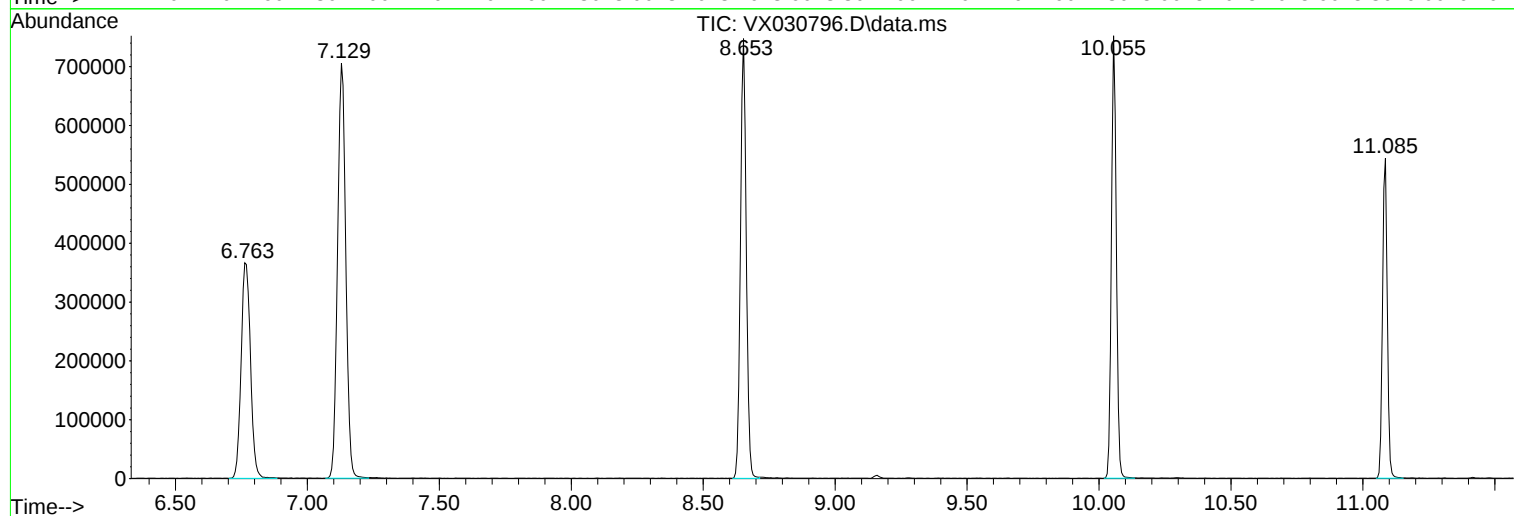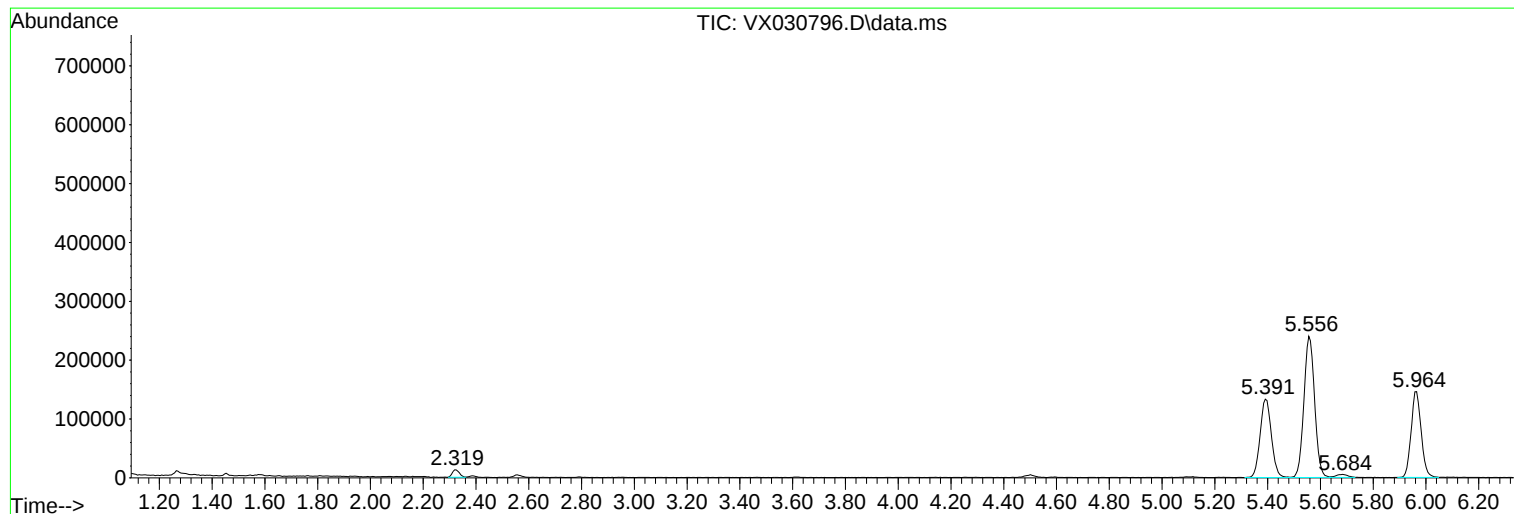

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030796.D
Acq On : 26 Aug 2022 01:50
Operator : JC/MD
Sample : N4245-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030796.D
Acq On : 26 Aug 2022 01:50
Operator : JC/MD
Sample : N4245-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE117D1-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc