

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030797.D
Acq On : 26 Aug 2022 02:13
Operator : JC/MD
Sample : N4245-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20220816

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M

Title : SW846 8260

Signal : TIC: VX030797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.325	196	203	209	rBV3	12180	24151	1.59%	0.317%
2	5.391	693	706	718	rBV2	136861	389724	25.60%	5.115%
3	5.556	721	733	747	rVV	240232	675802	44.38%	8.870%
4	5.678	747	753	764	rVB6	5602	16431	1.08%	0.216%
5	5.964	788	800	814	rBV	144728	383977	25.22%	5.040%
6	6.763	922	931	948	rBV	355854	870903	57.20%	11.430%
7	7.129	980	991	1004	rBV	703057	1522634	100.00%	19.984%
8	8.653	1234	1241	1251	rBV	746353	1151885	75.65%	15.118%
9	10.055	1465	1471	1479	rBV	748899	991562	65.12%	13.014%
10	11.085	1634	1640	1651	rBV	557540	707856	46.49%	9.290%
11	12.024	1789	1794	1802	rBV	729830	884232	58.07%	11.605%




Sum of corrected areas: 7619157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030797.D
Acq On : 26 Aug 2022 02:13
Operator : JC/MD
Sample : N4245-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

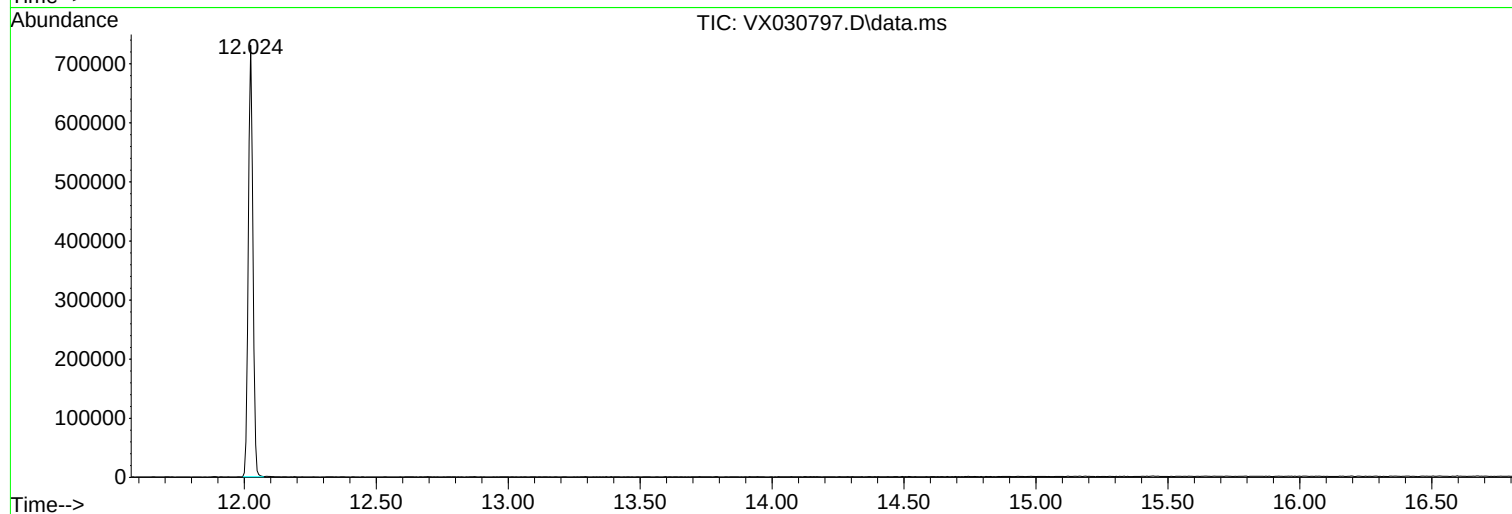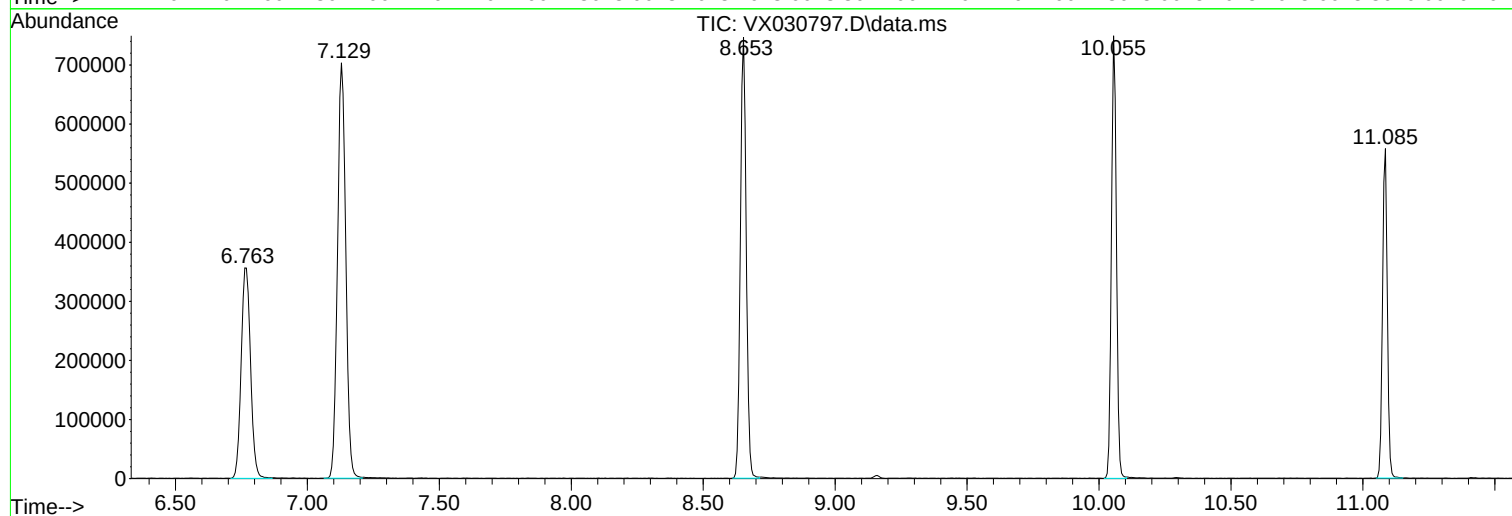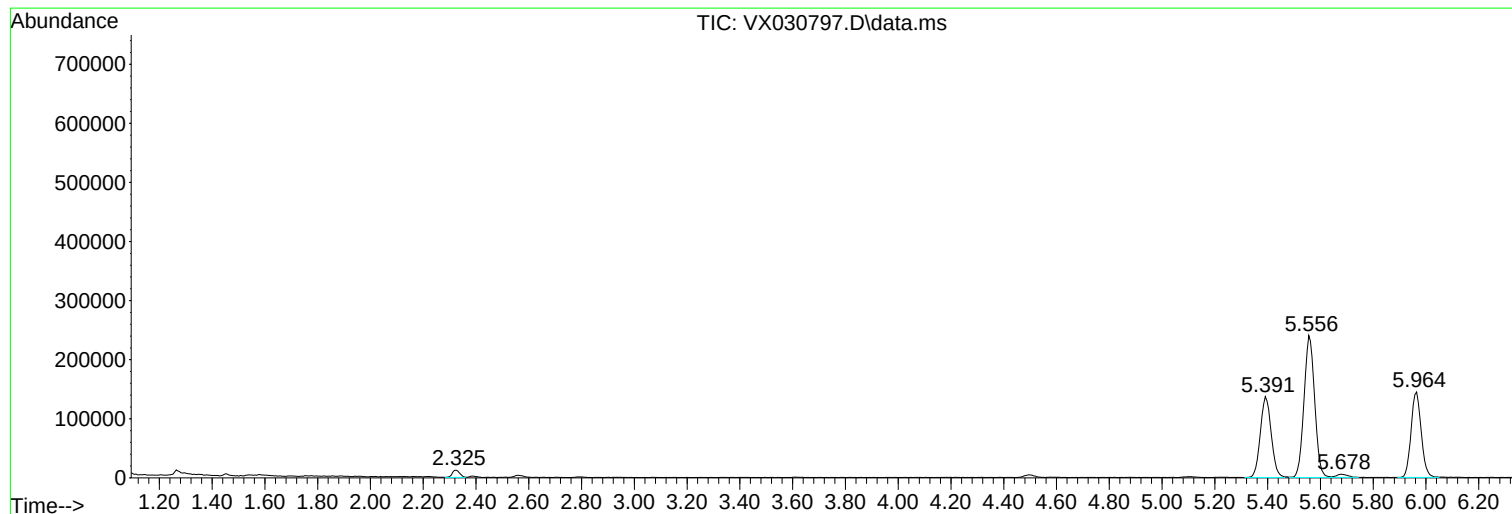

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030797.D
Acq On : 26 Aug 2022 02:13
Operator : JC/MD
Sample : N4245-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082522\
Data File : VX030797.D
Acq On : 26 Aug 2022 02:13
Operator : JC/MD
Sample : N4245-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP04-20220816

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc