

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082625\
 Data File : VX047523.D
 Acq On : 26 Aug 2025 10:22
 Operator : JC/MD
 Sample : VX0826MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0826MBL01

Quant Time: Aug 27 01:31:20 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	176054	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.763	114	346044	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	350142	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	170182	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	141927	57.602	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	115.200%
35) Dibromofluoromethane	5.391	113	121126	53.933	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	107.860%
50) Toluene-d8	8.647	98	426357	53.113	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	106.220%
62) 4-Bromofluorobenzene	11.079	95	173876	58.698	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	117.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082625\
Data File : VX047523.D
Acq On : 26 Aug 2025 10:22
Operator : JC/MD
Sample : VX0826MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0826MBL01


Quant Time: Aug 27 01:31:20 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration

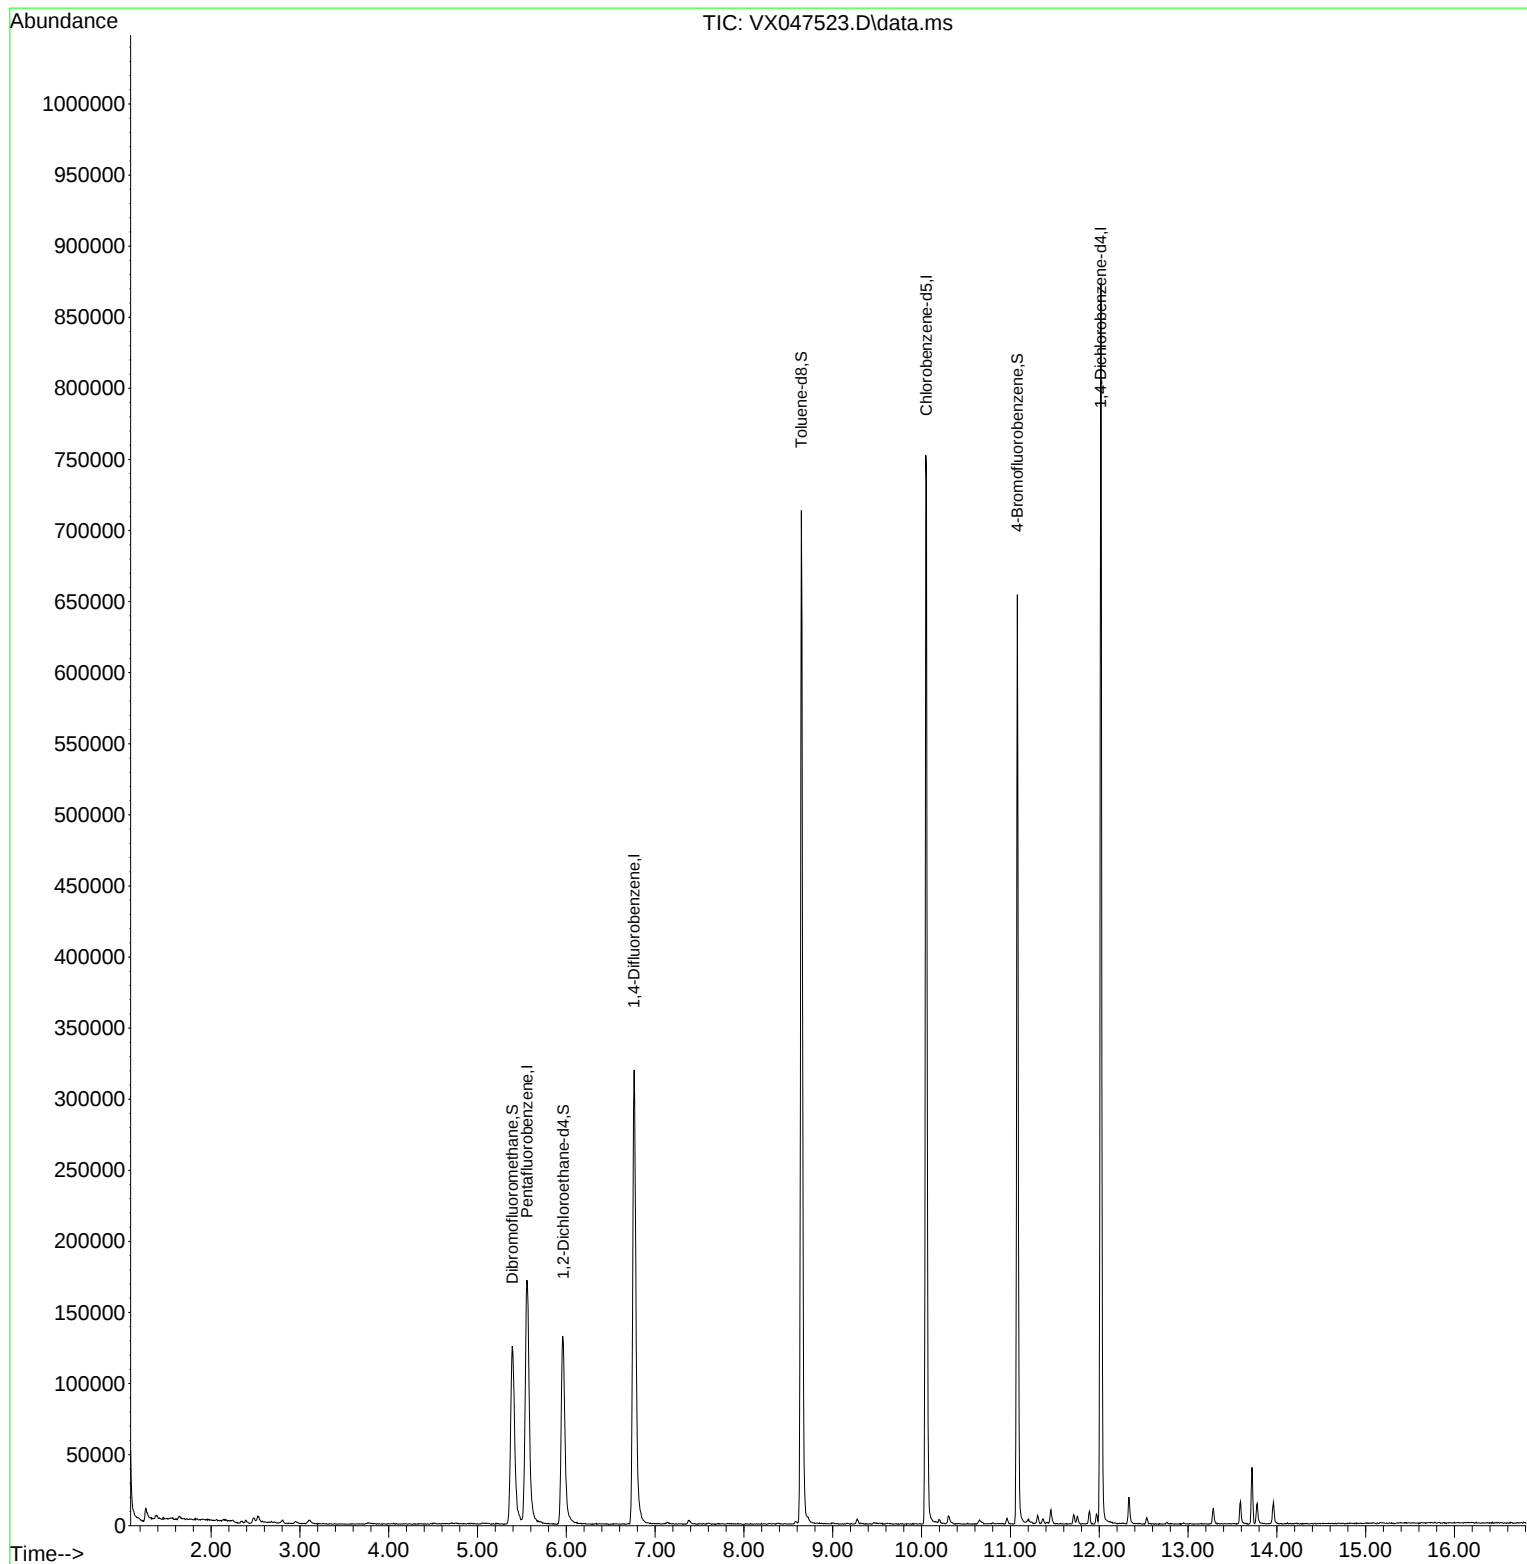



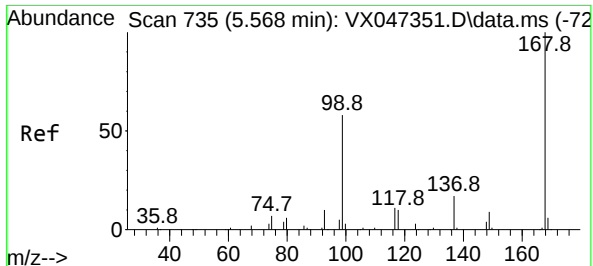


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.012 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22


Instrument :
MSVOA_X
ClientSampleId :
VX0826MBL01

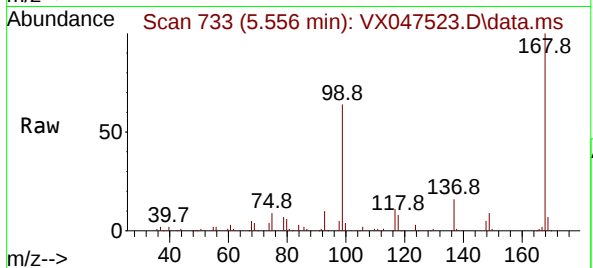



Tgt Ion:168 Resp: 176054
Ion Ratio Lower Upper
168 100
99 63.8 47.9 71.9

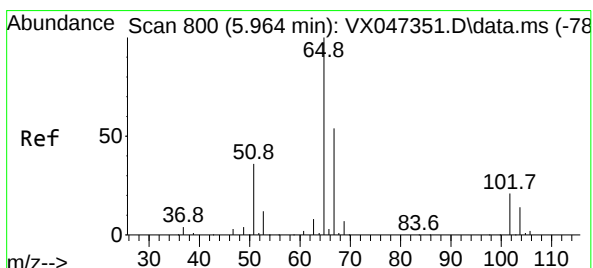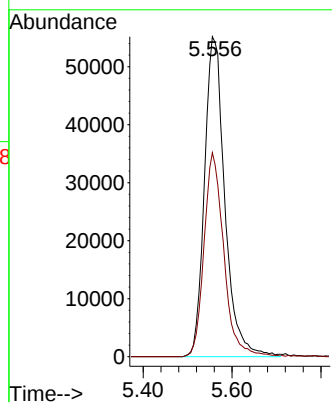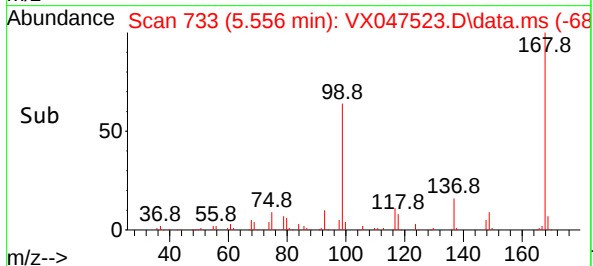


#33
1,2-Dichloroethane-d4
Concen: 57.602 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22

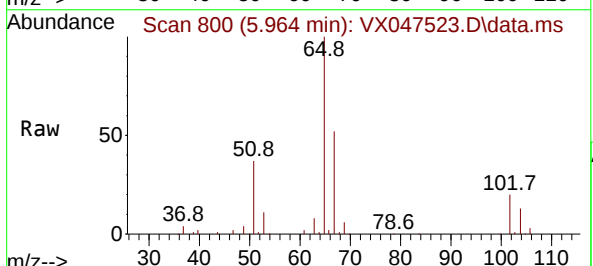

Tgt Ion: 65 Resp: 141927
Ion Ratio Lower Upper
65 100
67 52.5 0.0 106.0



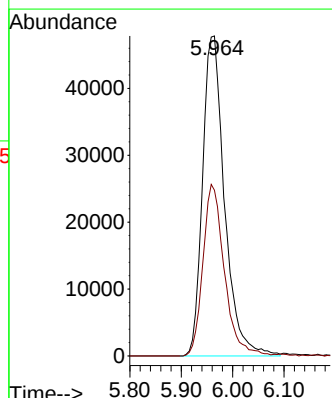
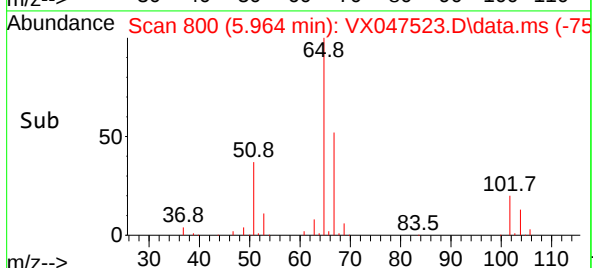


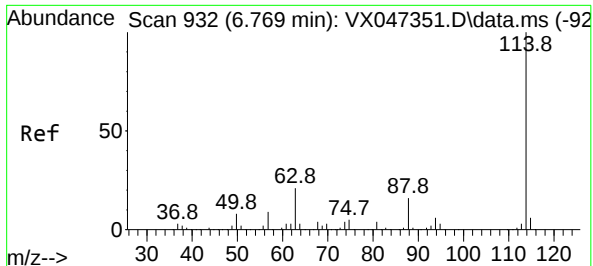

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.006 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22




Instrument :
MSVOA_X
ClientSampleId :
VX0826MBL01


Tgt Ion:114 Resp: 346044
Ion Ratio Lower Upper
114 100
63 22.0 0.0 42.4
88 15.8 0.0 33.0

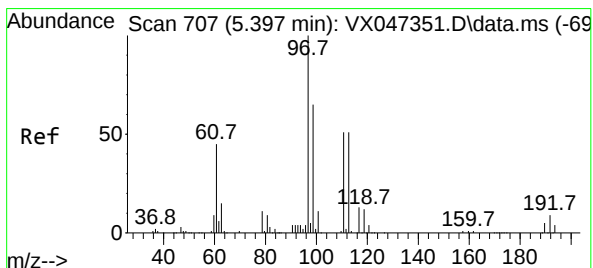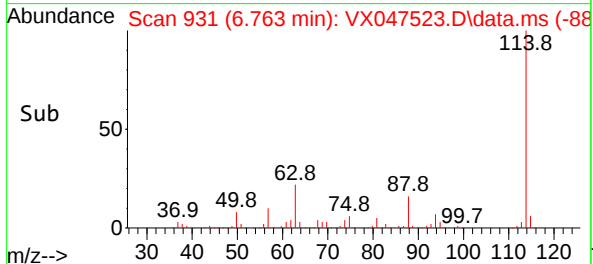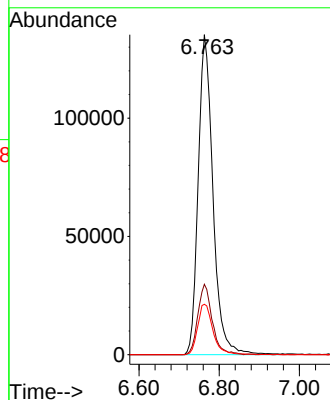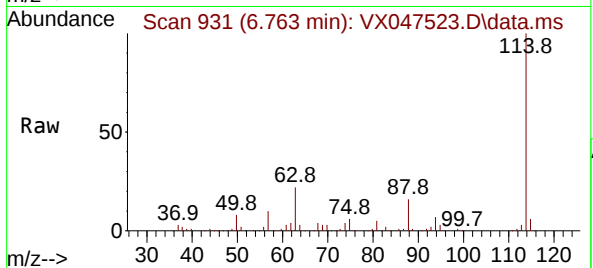

#35
Dibromofluoromethane
Concen: 53.933 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22

Tgt Ion:113 Resp: 121126
Ion Ratio Lower Upper
113 100
111 102.6 81.4 122.2
192 17.8 14.1 21.1


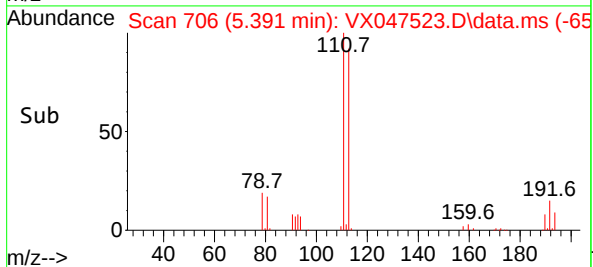
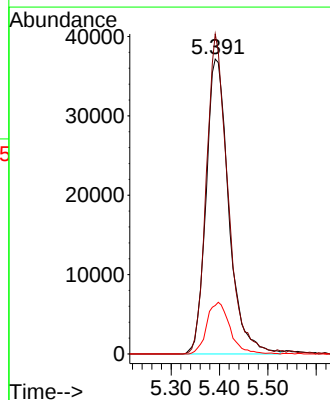
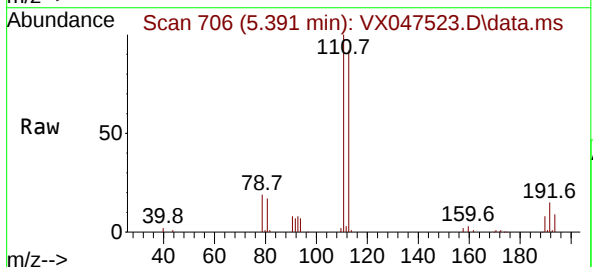


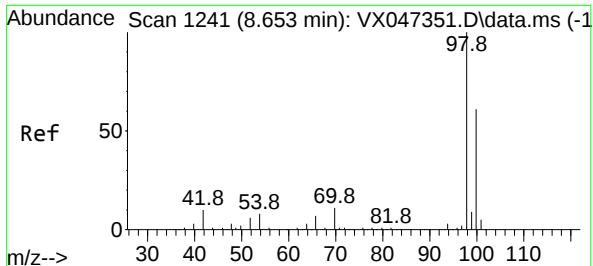

#50
Toluene-d8
Concen: 53.113 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22




Instrument :
MSVOA_X
ClientSampleId :
VX0826MBL01


Tgt Ion: 98 Resp: 426357
Ion Ratio Lower Upper
98 100
100 66.5 53.9 80.9

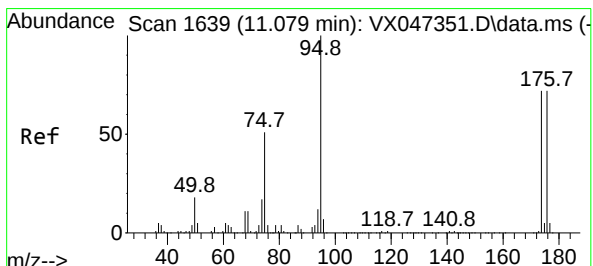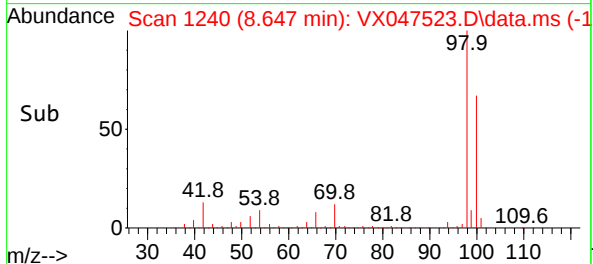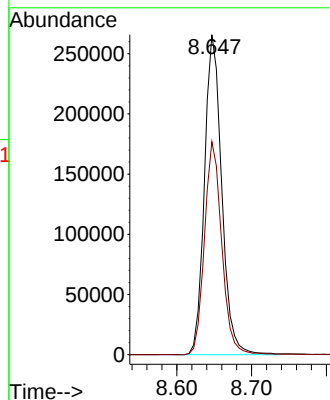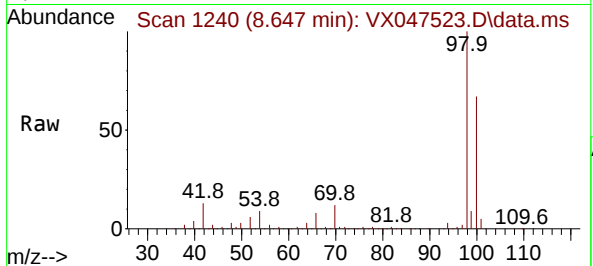

#62
4-Bromofluorobenzene
Concen: 58.698 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22

Tgt Ion: 95 Resp: 173876
Ion Ratio Lower Upper
95 100
174 75.5 0.0 148.0
176 72.2 0.0 145.4


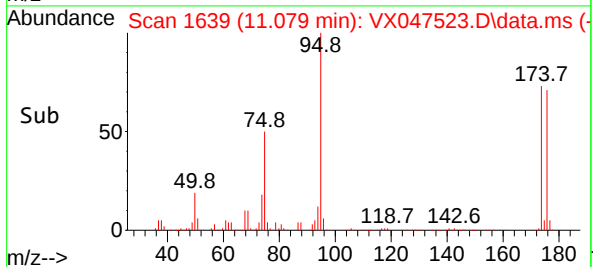
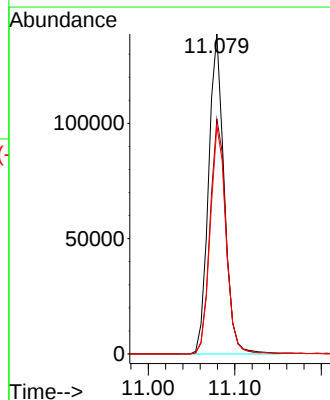
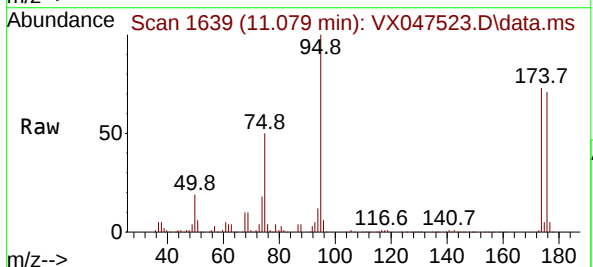


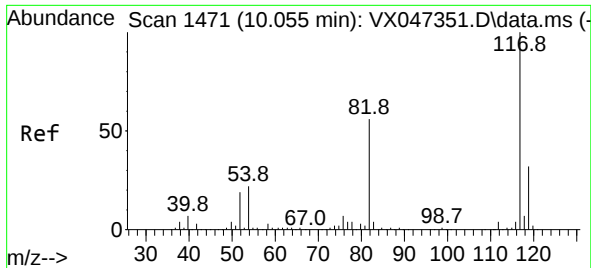

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22

Instrument :
MSVOA_X
ClientSampleId :
VX0826MBL01

Tgt Ion:117 Resp: 350142
Ion Ratio Lower Upper
117 100
82 53.7 45.0 67.4
119 31.7 25.8 38.8

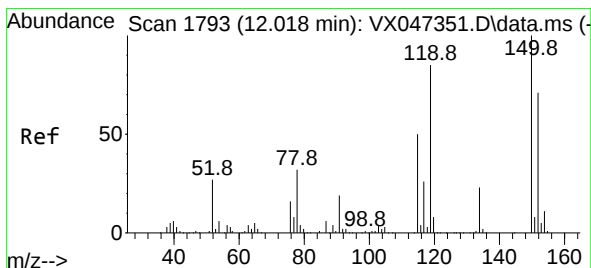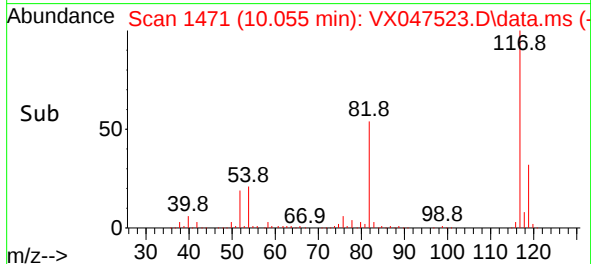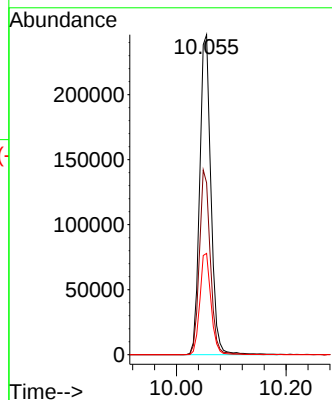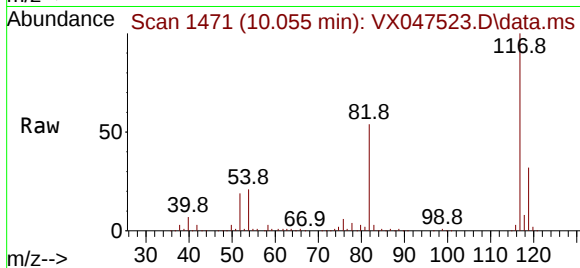

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX047523.D
Acq: 26 Aug 2025 10:22

Tgt Ion:152 Resp: 170182
Ion Ratio Lower Upper
152 100
115 62.7 44.6 133.8
150 158.4 0.0 349.8

