



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082625\
Data File : VX047521.D
Acq On : 26 Aug 2025 07:45
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Title : SW846 8260
Last Update : Mon Aug 18 04:18:28 2025

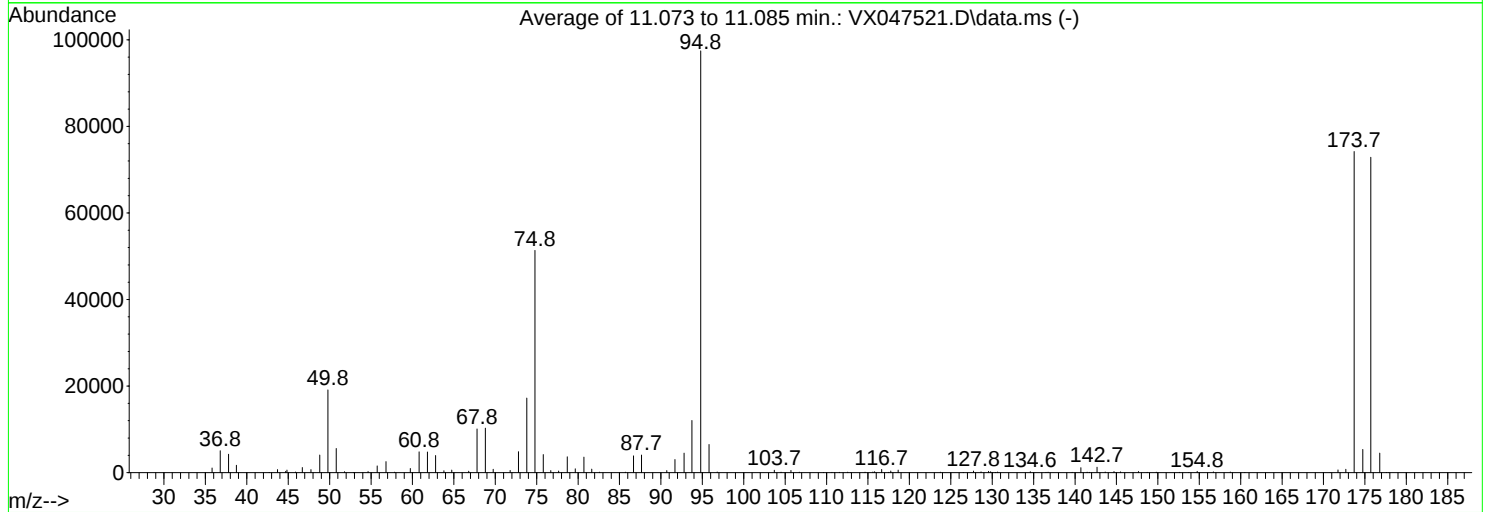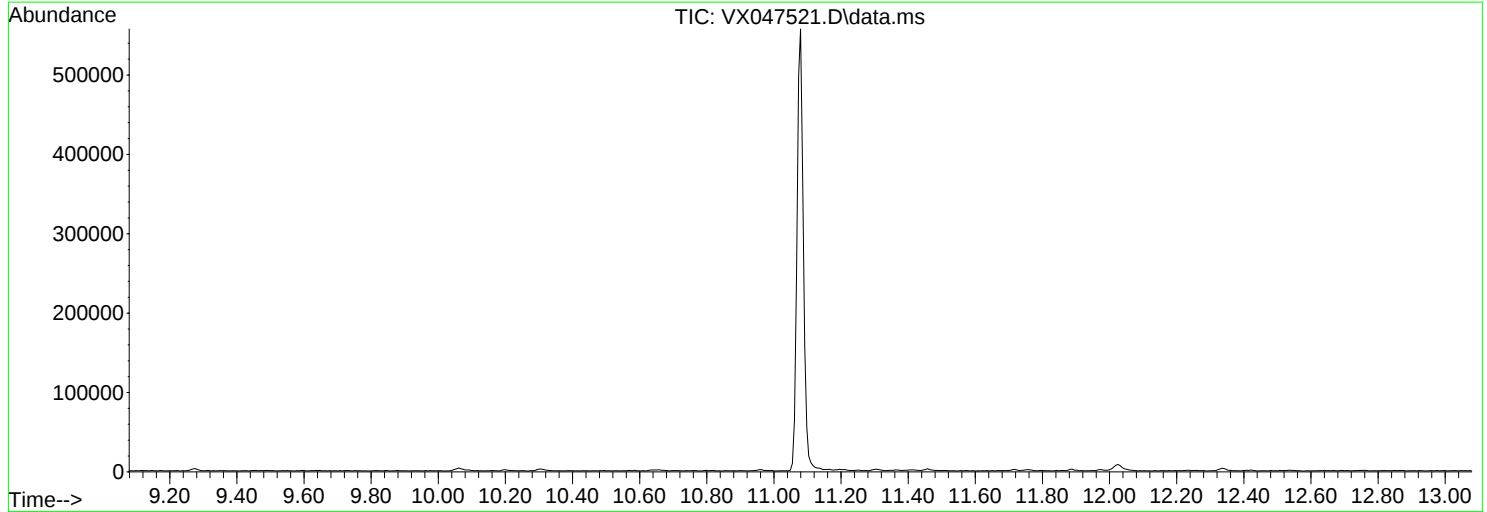

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	19115	PASS
75	95	30	60	52.7	51344	PASS
95	95	100	100	100.0	97453	PASS
96	95	5	9	6.7	6505	PASS
173	174	0.00	2	1.0	771	PASS
174	95	50	100	76.1	74187	PASS
175	174	5	9	7.2	5348	PASS
176	174	95	101	98.2	72877	PASS
177	176	5	9	6.2	4516	PASS