


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082718\
 Data File : VX004258.D
 Acq On : 27 Aug 2018 09:28
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
 Title : SW846 8260
 Last Update : Thu Aug 23 05:39:44 2018

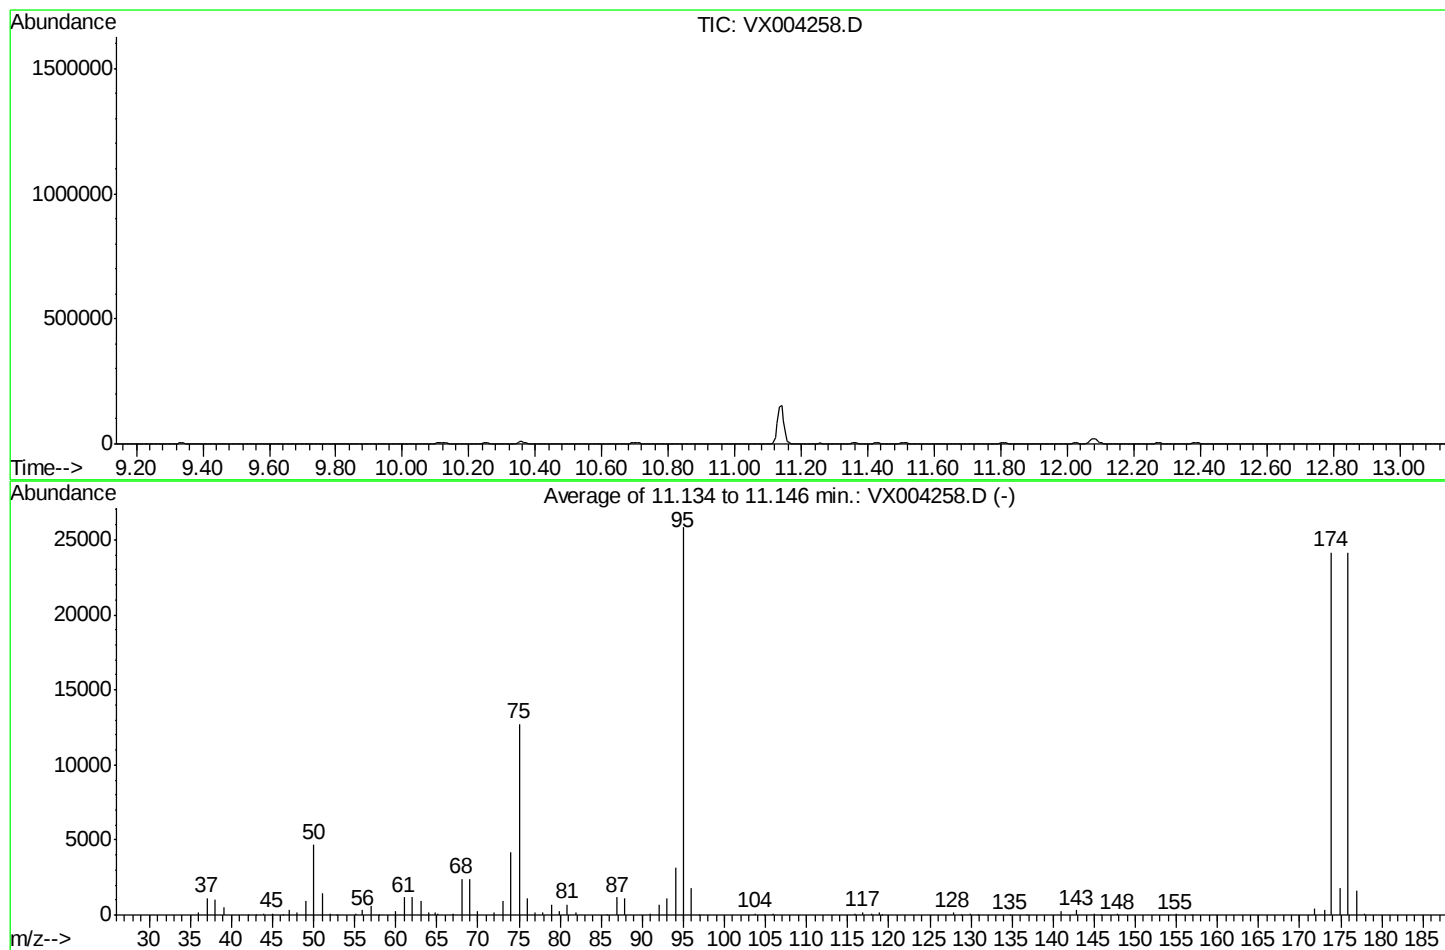

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1722

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4667	PASS
75	95	30	60	49.3	12728	PASS
95	95	100	100	100.0	25829	PASS
96	95	5	9	7.0	1818	PASS
173	174	0.00	2	1.3	322	PASS
174	95	50	100	93.5	24162	PASS
175	174	5	9	7.3	1756	PASS
176	174	95	101	99.8	24122	PASS
177	176	5	9	6.8	1644	PASS