

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082719\  
 Data File : VX011844.D  
 Acq On : 27 Aug 2019 12:56  
 Operator : JC/SP  
 Sample : K4553-01  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BP-TB-20190826

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X082219W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.373       | 24            | 36          | 38           | rBV10    | 14390          | 51433         | 3.05%           | 0.553%        |
| 2         | 1.599       | 67            | 73          | 83           | rBV10    | 21308          | 45122         | 2.67%           | 0.485%        |
| 3         | 2.434       | 206           | 210         | 216          | rVB      | 13269          | 22870         | 1.36%           | 0.246%        |
| 4         | 5.488       | 698           | 711         | 724          | rBV      | 207897         | 597222        | 35.39%          | 6.423%        |
| 5         | 5.653       | 727           | 738         | 754          | rVV      | 384004         | 1065249       | 63.12%          | 11.456%       |
| 6         | 6.055       | 794           | 804         | 817          | rBV      | 212977         | 557311        | 33.02%          | 5.994%        |
| 7         | 6.854       | 924           | 935         | 948          | rBV      | 538458         | 1268928       | 75.19%          | 13.647%       |
| 8         | 8.713       | 1233          | 1240        | 1249         | rBV      | 1048900        | 1687604       | 100.00%         | 18.149%       |
| 9         | 10.110      | 1463          | 1469        | 1485         | rBV      | 1099801        | 1459950       | 86.51%          | 15.701%       |
| 10        | 11.134      | 1631          | 1637        | 1647         | rBV      | 953264         | 1175040       | 69.63%          | 12.637%       |
| 11        | 12.073      | 1786          | 1791        | 1803         | rBV      | 1097338        | 1367709       | 81.04%          | 14.709%       |


Sum of corrected areas: 9298438

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX082719\  
Data File : VX011844.D  
Acq On : 27 Aug 2019 12:56  
Operator : JC/SP  
Sample : K4553-01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BP-TB-20190826

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X082219W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

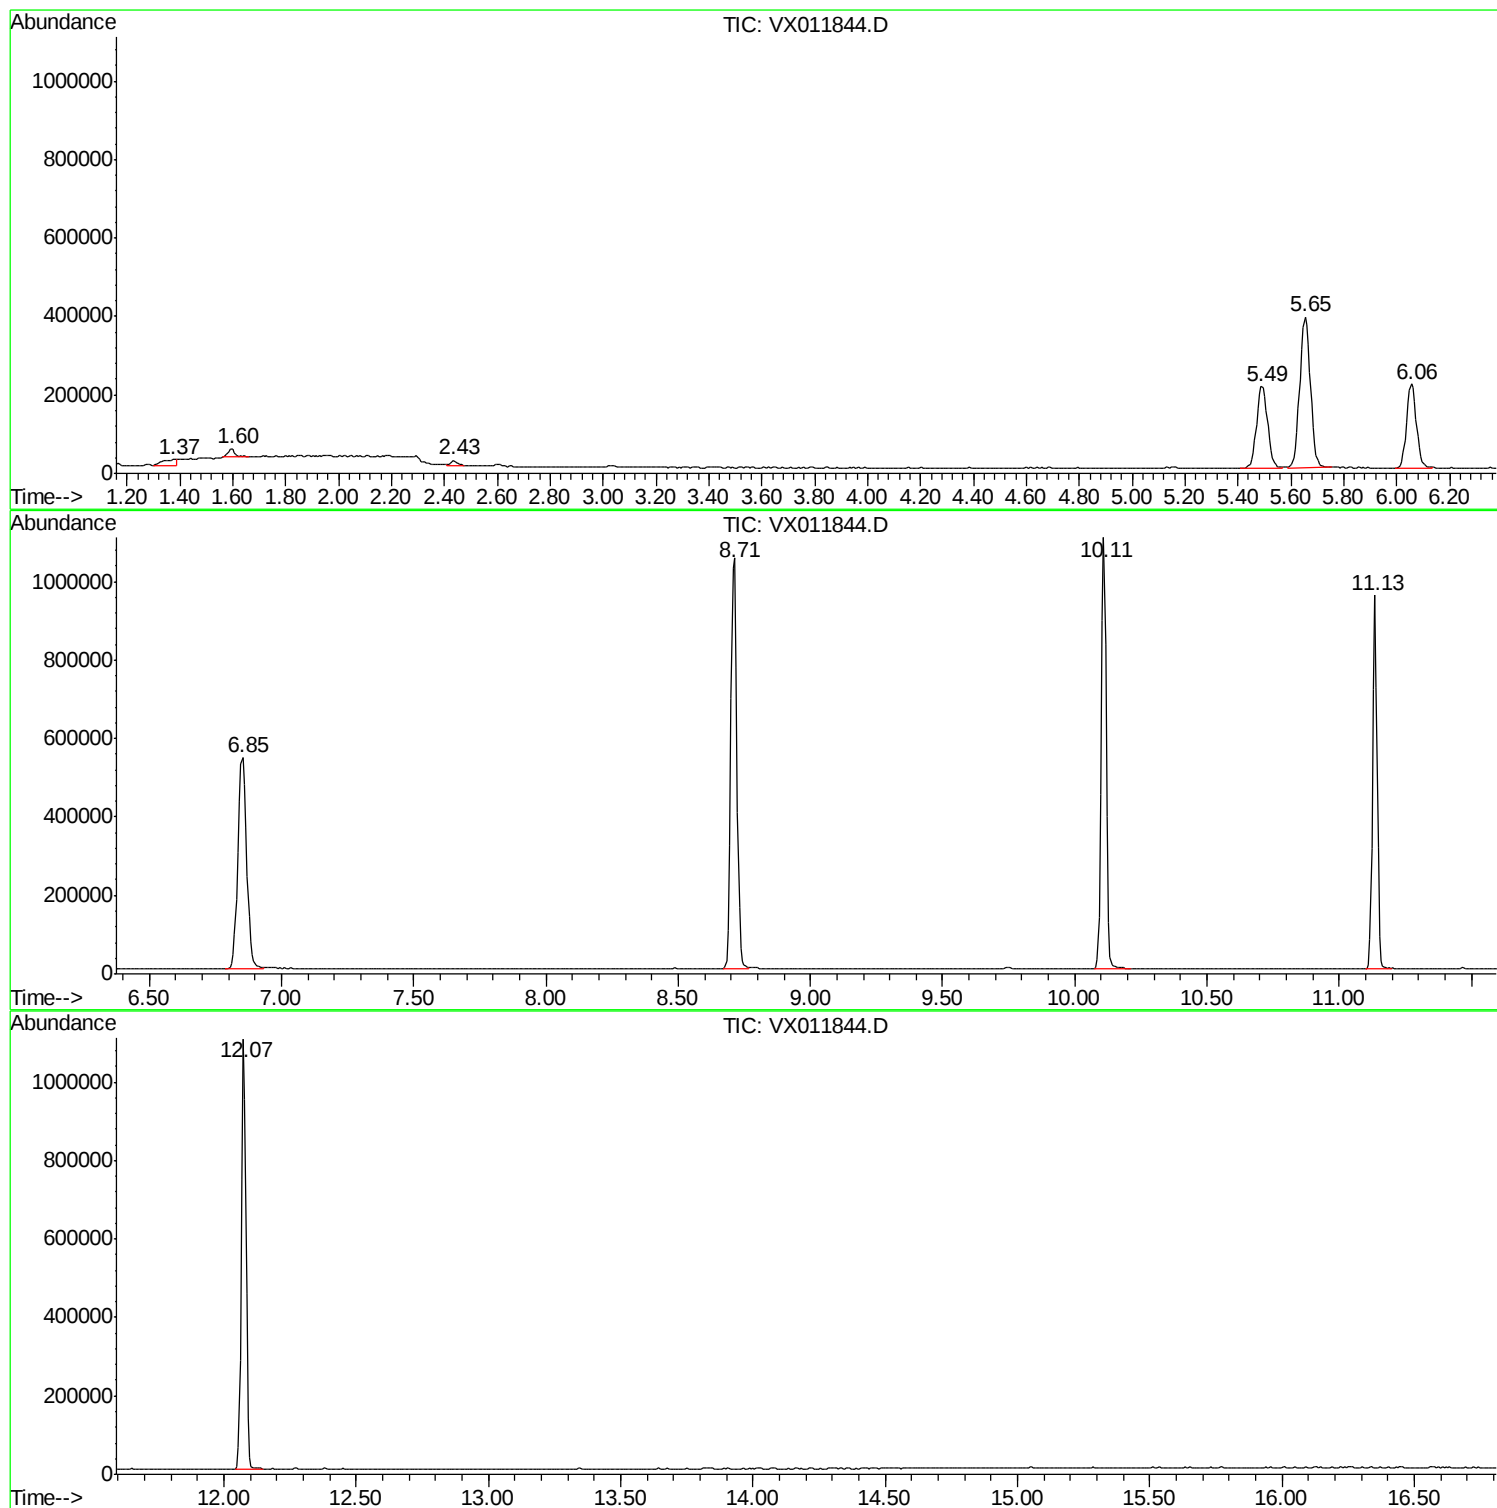

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A\_X\DATA\VX082719\  
Data File : VX011844.D  
Acq On : 27 Aug 2019 12:56  
Operator : JC/SP  
Sample : K4553-01  
Misc : 5.0mL/MSV0A\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSV0A\_X  
ClientSampleId :  
BP-TB-20190826

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A\_X\METHOD\82X082219W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX082719\  
Data File : VX011844.D  
Acq On : 27 Aug 2019 12:56  
Operator : JC/SP  
Sample : K4553-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BP-TB-20190826

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X082219W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |