

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX082720\
 Data File : VX018097.D
 Acq On : 27 Aug 2020 17:27
 Operator : JC/SP
 Sample : L3805-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FM782

Quant Time: Aug 28 03:04:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 21 03:03:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	584867	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	946297	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	914663	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	421656	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.03	65	389614	47.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.98%	
35) Dibromofluoromethane	5.47	113	319192	49.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.06%	
50) Toluene-d8	8.70	98	1181477	49.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.44%	
62) 4-Bromofluorobenzene	11.12	95	438219	46.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.80%	

Target Compounds


					Qvalue	
3) Chloromethane	1.31	50	5545	0.739	ug/l	96
5) Bromomethane	1.64	94	1226	0.340	ug/l	84
6) Chloroethane	1.73	64	890	0.222	ug/l #	36
10) Methyl Iodide	2.49	142	1332	5.489	ug/l #	75
11) Tert butyl alcohol	3.02	59	1370	0.868	ug/l #	71
13) Acrolein	2.28	56	595	0.909	ug/l #	36
15) Acrylonitrile	3.13	53	1456	0.407	ug/l #	79
16) Acetone	2.42	43	28942	9.148	ug/l	91
17) Carbon Disulfide	2.55	76	6379	0.369	ug/l #	77
20) Methylene Chloride	2.84	84	3599	Below Cal		87
21) trans-1,2-Dichloroethene	3.14	96	1795	0.283	ug/l #	48
25) 2-Butanone	4.65	43	3062	0.589	ug/l #	84
29) Tetrahydrofuran	5.10	42	927	0.280	ug/l #	80
38) Carbon Tetrachloride	5.63	117	61841	6.287	ug/l #	16
39) Methylcyclohexane	7.44	83	2021	0.212	ug/l	91
49) 1,4-Dioxane	7.74	88	668	4.524	ug/l #	19
76) 1,2,3-Trichloropropane	11.12	75	222919	23.766	ug/l #	36
81) trans-1,4-Dichloro-2-buten	11.12	75	222919	64.187	ug/l #	12
85) sec-Butylbenzene	11.93	105	6026	0.235	ug/l	79
86) p-Isopropyltoluene	12.05	119	6238	0.265	ug/l #	73
87) 1,3-Dichlorobenzene	12.01	146	2764	0.205	ug/l	89
88) 1,4-Dichlorobenzene	12.01	146	2764	0.205	ug/l	89
89) n-Butylbenzene	12.37	91	7610	0.354	ug/l	99
90) Hexachloroethane	12.58	117	1335	0.288	ug/l	90
93) 1,2,4-Trichlorobenzene	13.63	180	4044	0.477	ug/l	83
94) Hexachlorobutadiene	13.77	225	2257	0.675	ug/l #	68
95) Naphthalene	13.82	128	6239	0.224	ug/l #	71
96) 1,2,3-Trichlorobenzene	14.01	180	3316	0.396	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX082720\
Data File : VX018097.D
Acq On : 27 Aug 2020 17:27
Operator : JC/SP
Sample : L3805-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FM782

Quant Time: Aug 28 03:04:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 21 03:03:56 2020
Response via : Initial Calibration

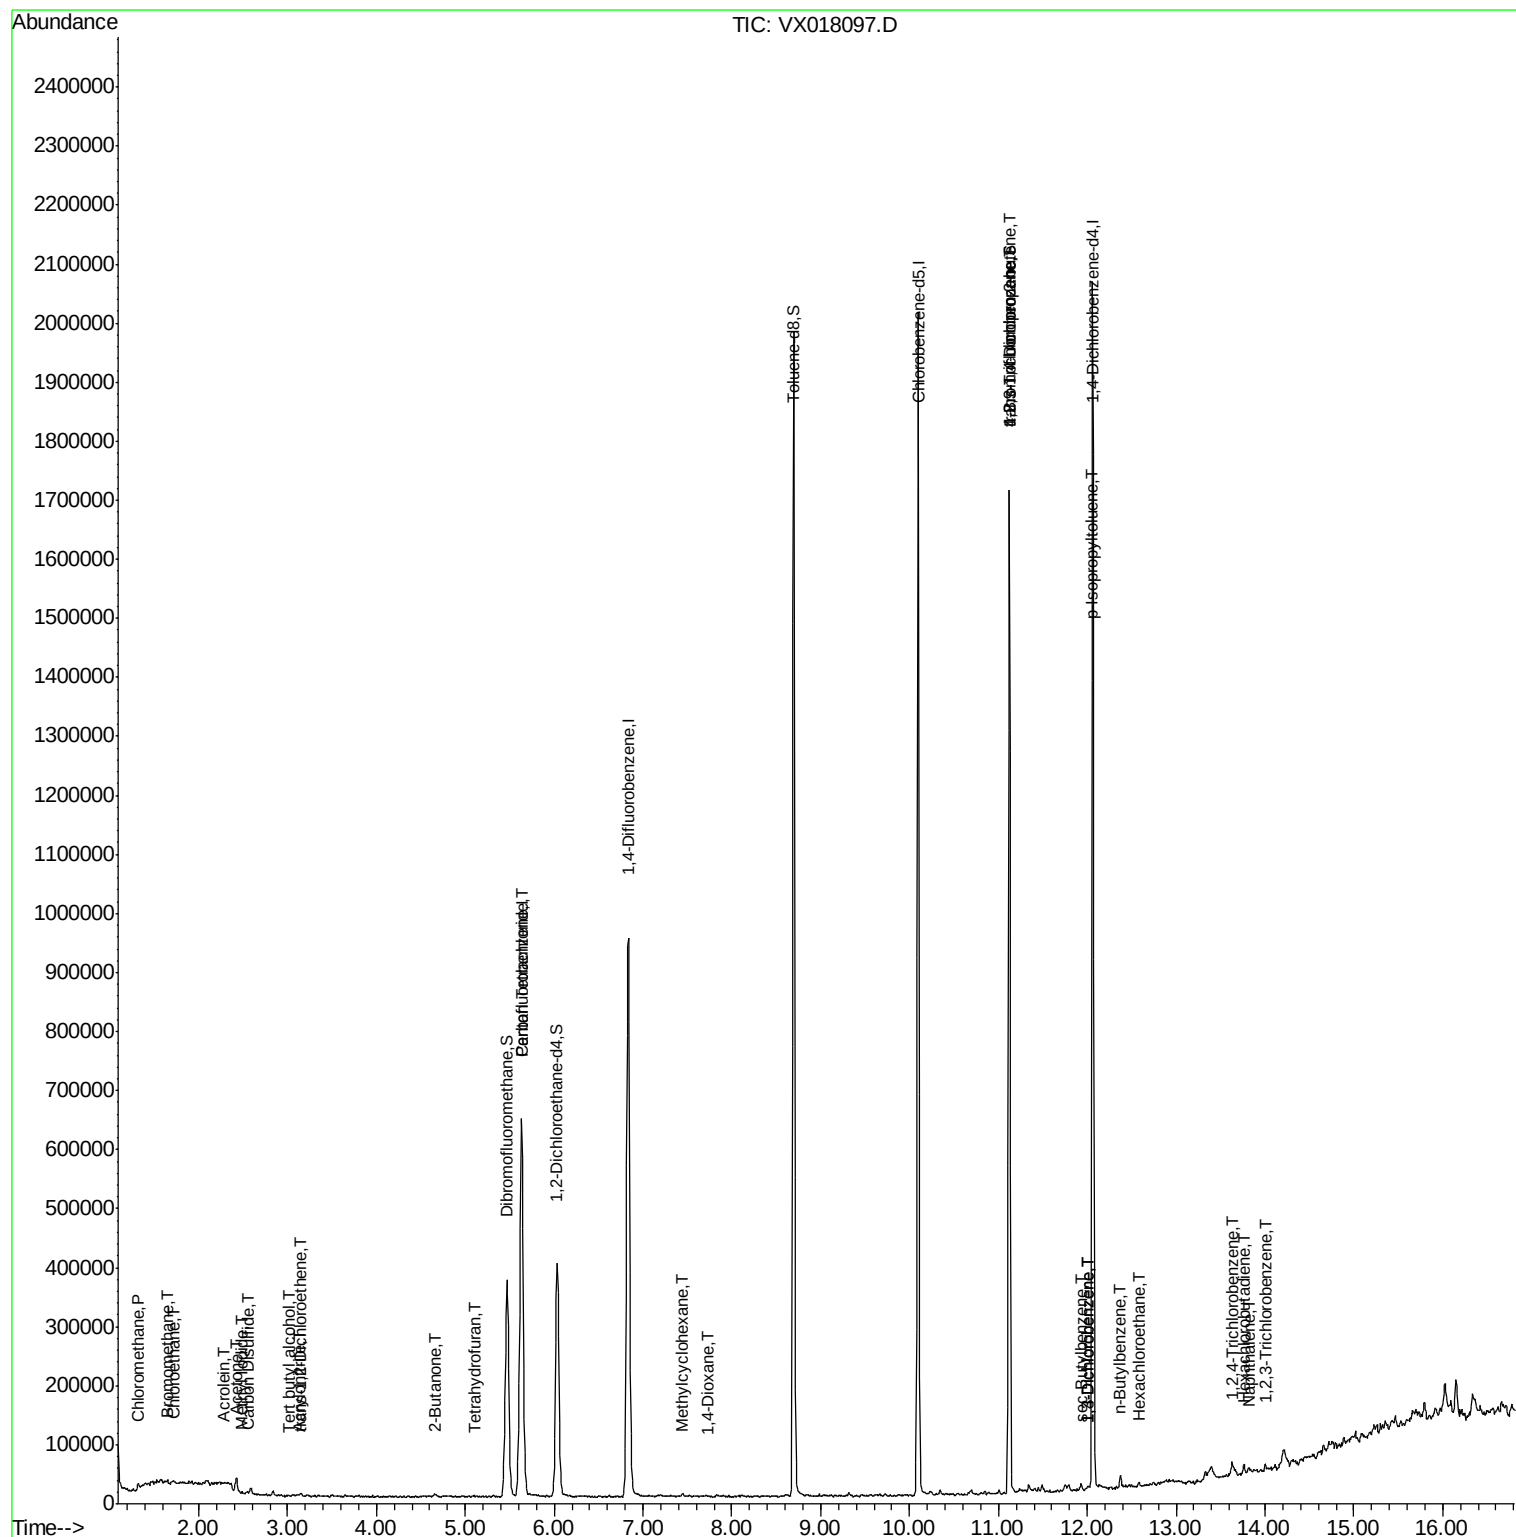

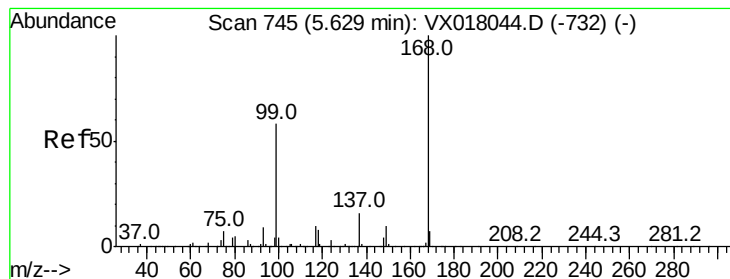

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 746

Delta R.T. 0.01 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampled :


FM782

Tot Ion:168 Resp: 584867

Ion Ratio Lower Upper




168 100

99 53.7 46.3 69.5

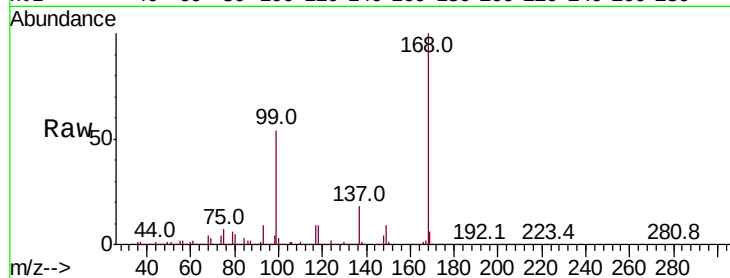

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

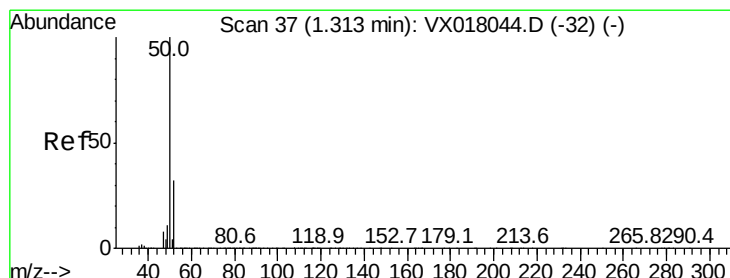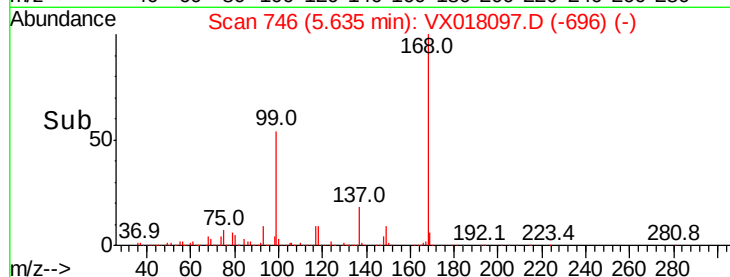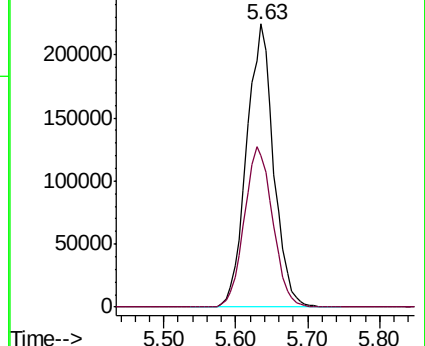

#3

Chloromethane

Concen: 0.739 ug/l

RT: 1.31 min Scan# 37

Delta R.T. -0.00 min

Lab File: VX018097.D


Acq: 27 Aug 2020 17:27

Tgt Ion: 50 Resp: 5545

Ion Ratio Lower Upper



50 100


52 29.4 25.4 38.2

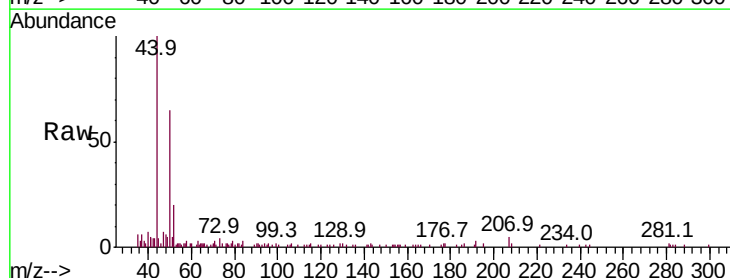

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

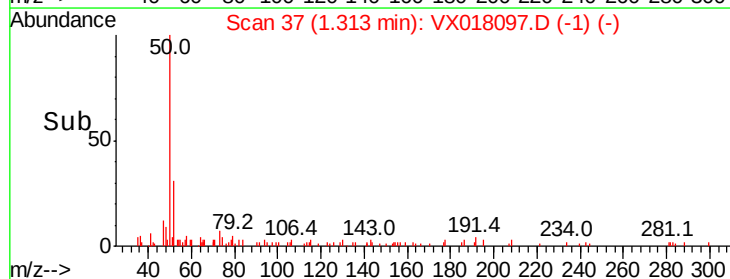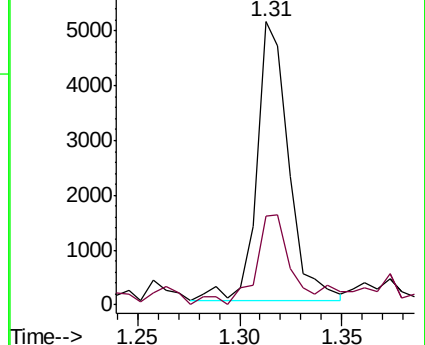

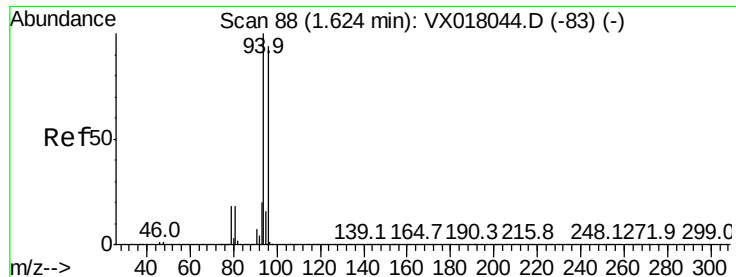

#5

Bromomethane

Concen: 0.340 ug/l

RT: 1.64 min Scan# 91

Delta R.T. 0.02 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampled :





FM782

Tot Ion: 94 Resp: 1226

Ion Ratio Lower Upper

94 100

96 78.4 74.8 112.2

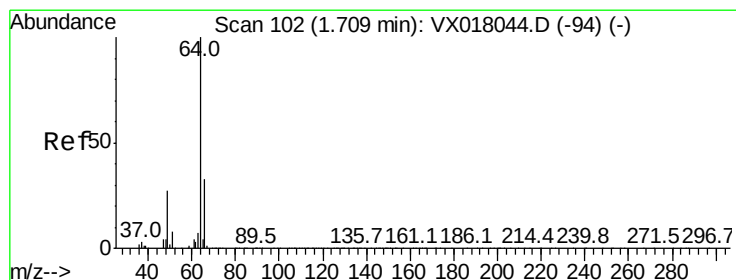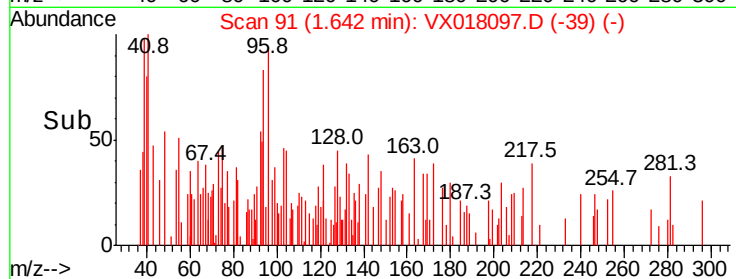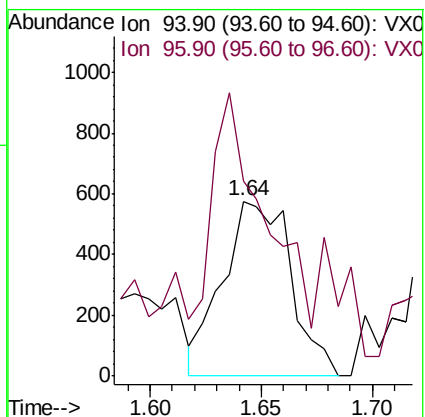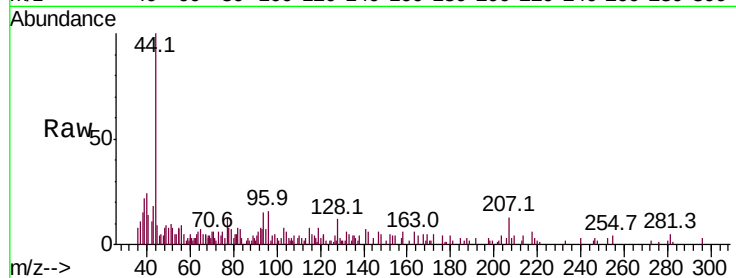

#6

Chloroethane

Concen: 0.222 ug/l

RT: 1.73 min Scan# 105

Delta R.T. 0.02 min

Lab File: VX018097.D




Acq: 27 Aug 2020 17:27


Tgt Ion: 64 Resp: 890

Ion Ratio Lower Upper

64 100

66 69.3 26.6 39.8#


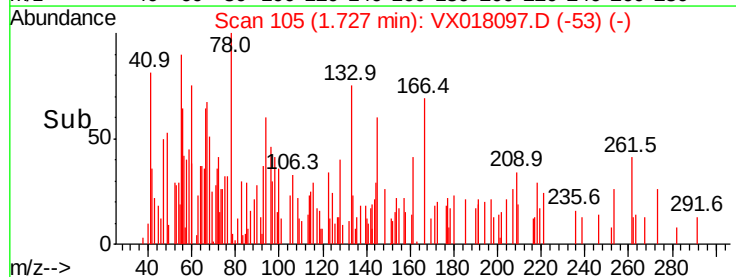
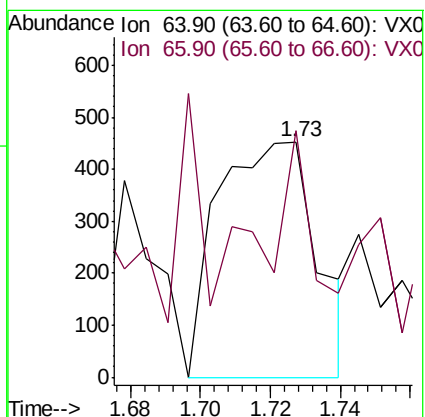
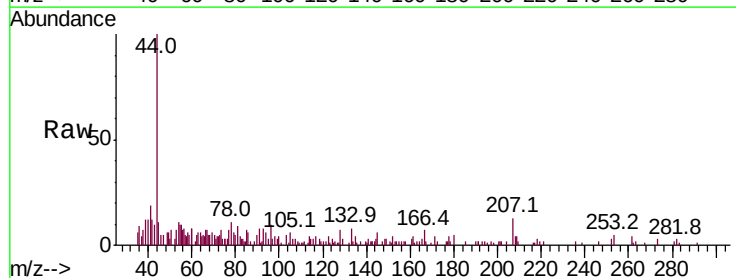


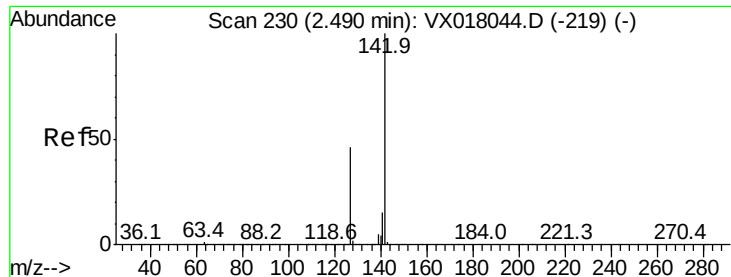

#10
Methyl Iodide
Concen: 5.489 ug/l
RT: 2.49 min Scan# 230
Delta R.T. 0.00 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27




Instrument :
MSVOA_X
ClientSampled :
FM782


Tot Ion	Ratio	Lower	Upper
142	100		
127	29.4	37.0	55.6#
141	23.9	11.5	17.3#

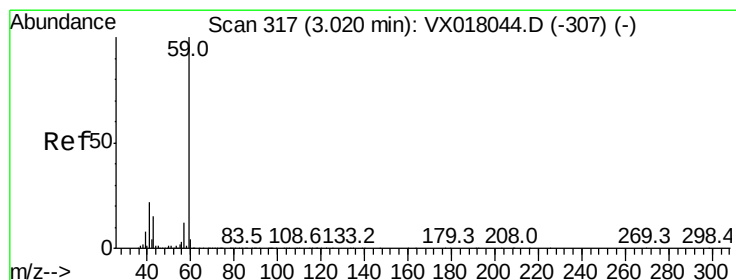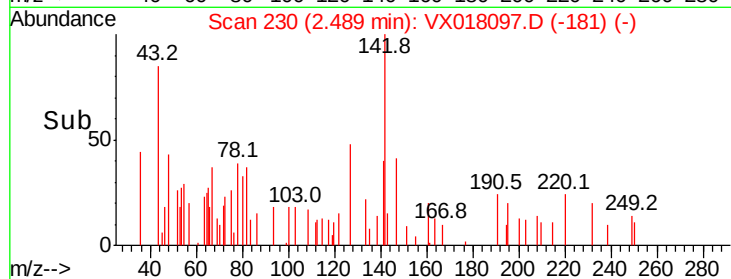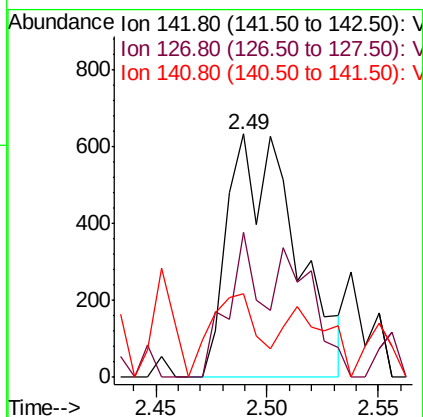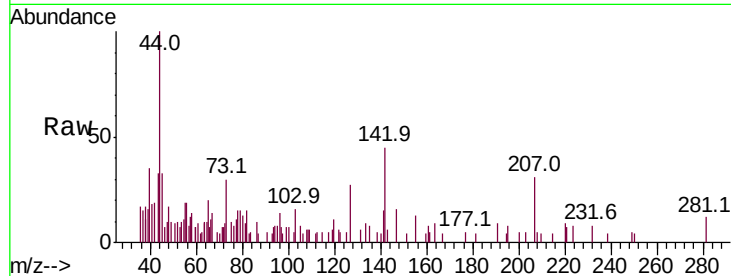

#11
Tert butyl alcohol
Concen: 0.868 ug/l
RT: 3.02 min Scan# 317
Delta R.T. -0.00 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27

Tgt Ion	Ratio	Lower	Upper
59	100		
57	0.0	8.9	13.3#

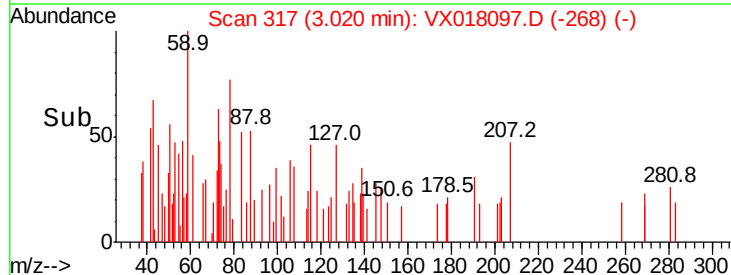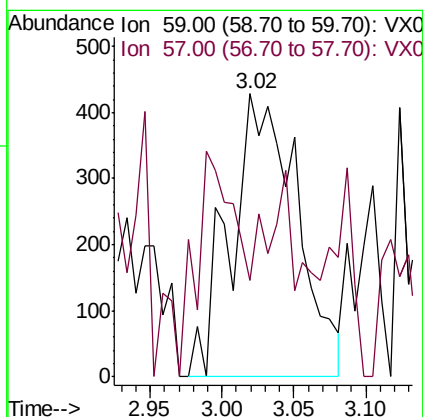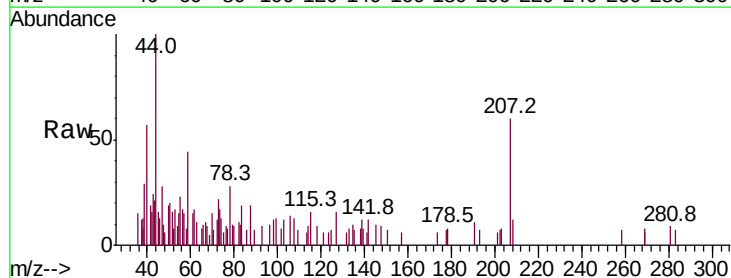

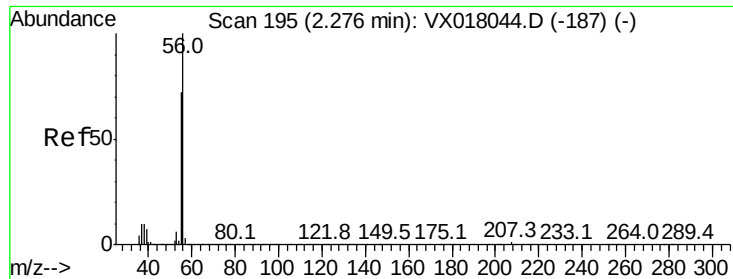

#13

Acrolein

Concen: 0.909 ug/l

RT: 2.28 min Scan# 195

Delta R.T. -0.00 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampled :





FM782

Tot Ion: 56 Resp: 595

Ion Ratio Lower Upper

56 100

55 18.0 57.0 85.6#

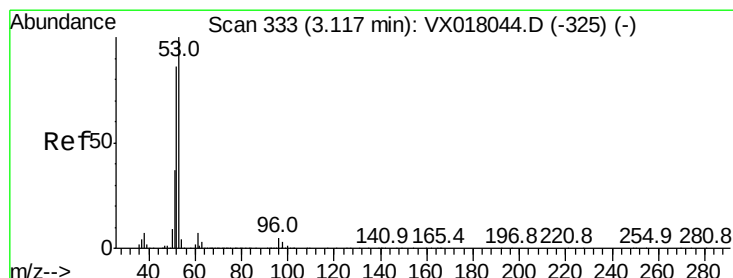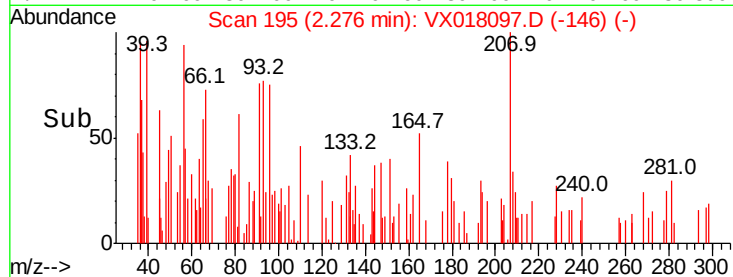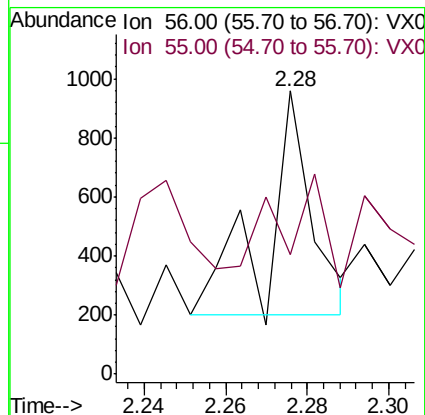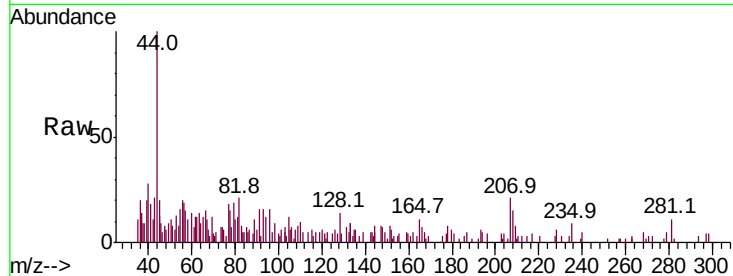

#15

Acrylonitrile

Concen: 0.407 ug/l

RT: 3.13 min Scan# 335

Delta R.T. 0.01 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27




Tgt Ion: 53 Resp: 1456


Ion Ratio Lower Upper

53 100

52 102.3 66.9 100.3#

51 24.0 28.7 43.1#

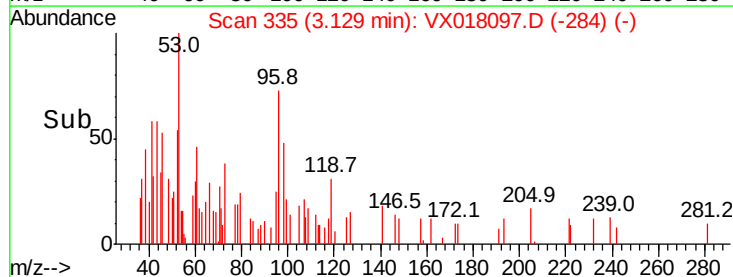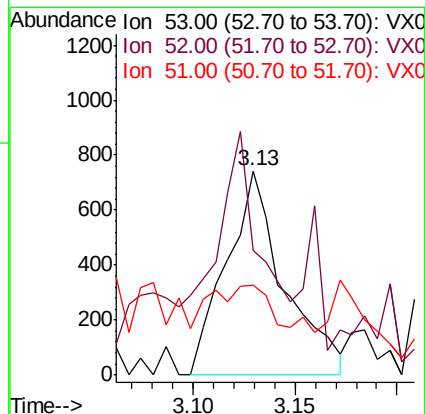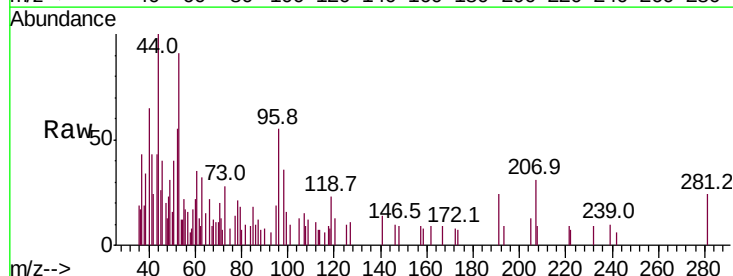

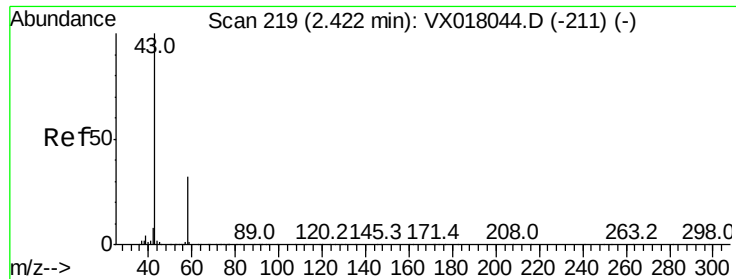

#16

Acetone

Concen: 9.148 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampleId :





FM782

Tot Ion: 43 Resp: 28942

Ion Ratio Lower Upper

43 100

58 27.1 25.5 38.3

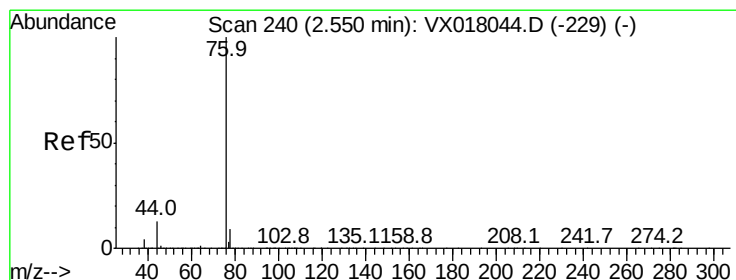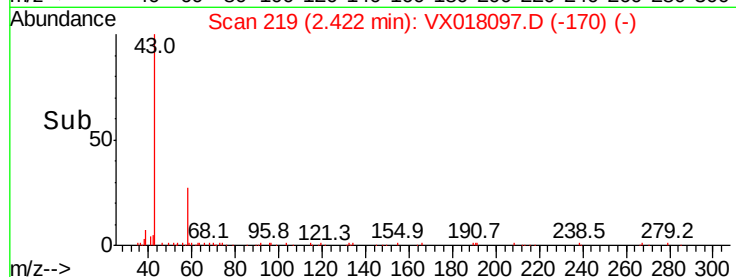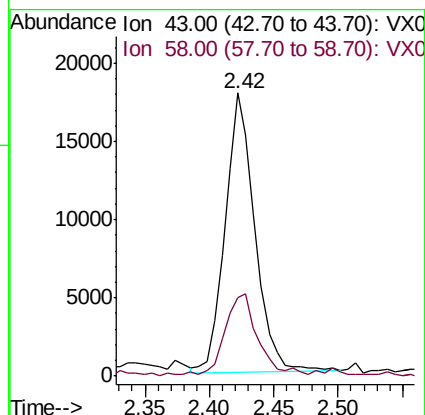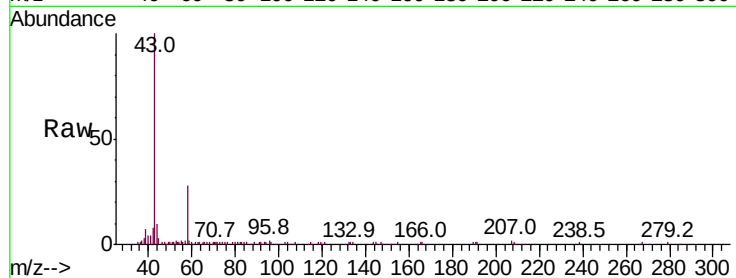

#17

Carbon Disulfide

Concen: 0.369 ug/l

RT: 2.55 min Scan# 240

Delta R.T. -0.00 min

Lab File: VX018097.D




Acq: 27 Aug 2020 17:27


Tgt Ion: 76 Resp: 6379

Ion Ratio Lower Upper

76 100

78 17.7 7.4 11.0#


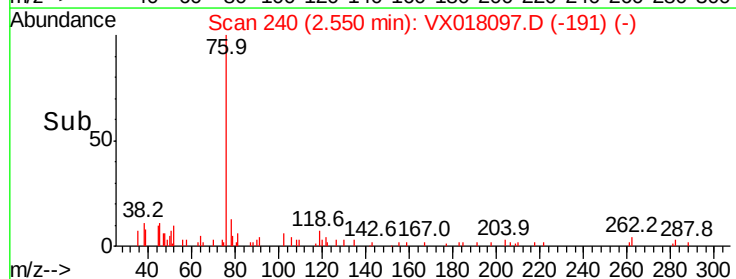
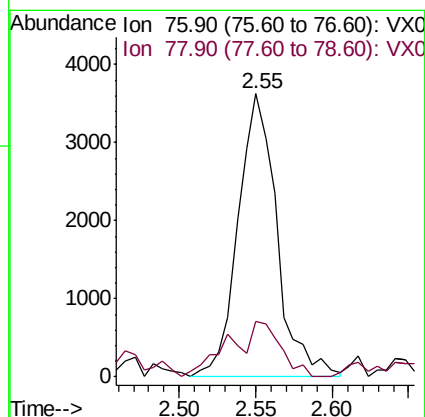
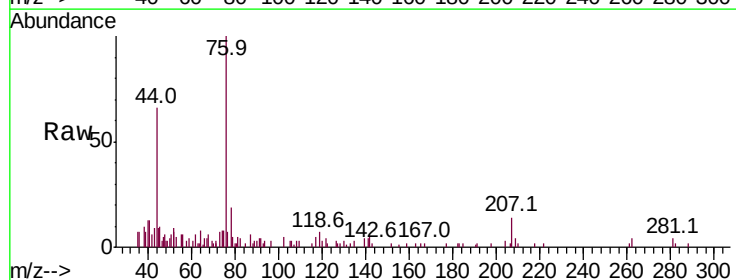


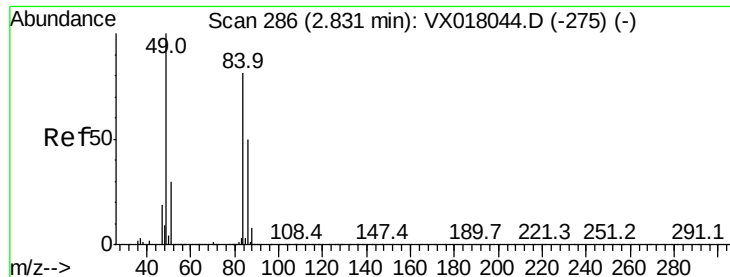

#20
Methylene Chloride
Concen: Below Cal
RT: 2.84 min Scan# 288
Delta R.T. 0.01 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27




Instrument :
MSVOA_X
ClientSampleId :
FM782


Tot Ion:	84	Resp:	3599
Ion	Ratio	Lower	Upper
84	100		
49	109.1	98.6	148.0
51	30.3	29.6	44.4
86	50.8	49.8	74.6

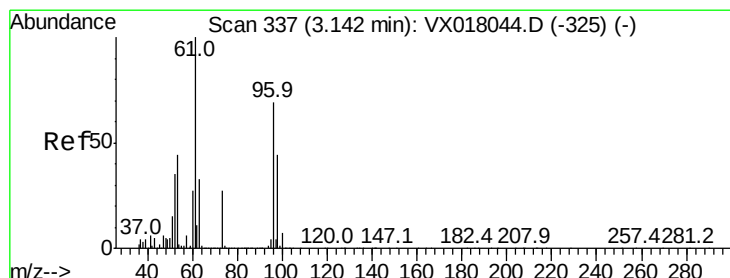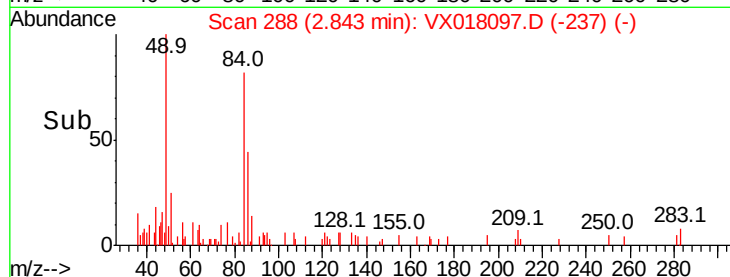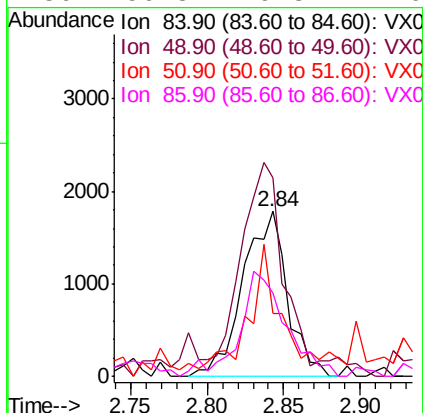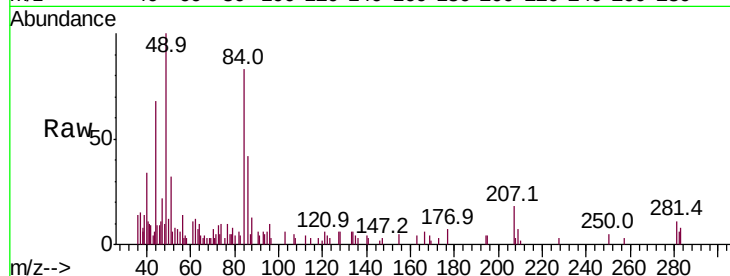

#21
trans-1,2-Dichloroethene
Concen: 0.283 ug/l
RT: 3.14 min Scan# 336
Delta R.T. -0.01 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27

Tgt Ion:	96	Resp:	1795
Ion	Ratio	Lower	Upper
96	100		
61	66.7	115.4	173.0#
98	40.8	51.1	76.7#

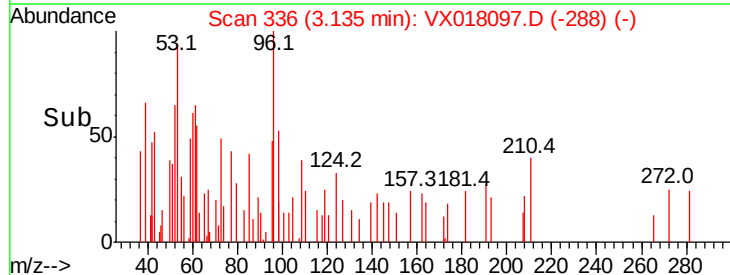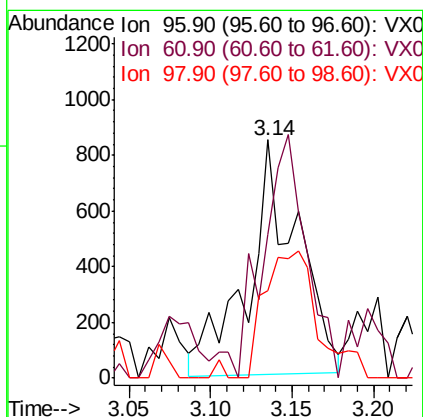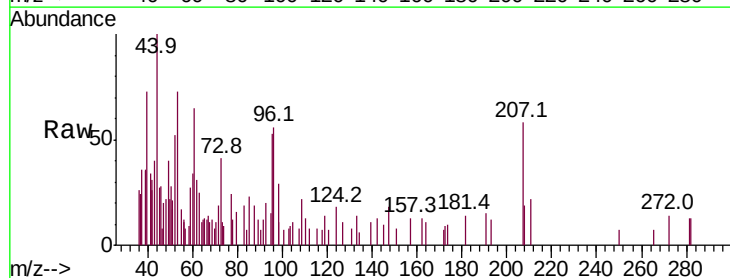

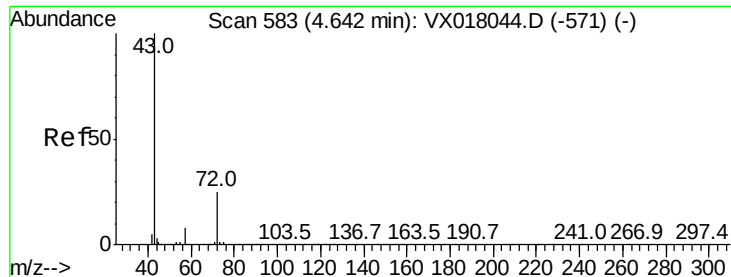

#25

2-Butanone

Concen: 0.589 ug/l

RT: 4.65 min Scan# 585

Delta R.T. 0.01 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampled :





FM782

Tot Ion: 43 Resp: 3062

Ion Ratio Lower Upper

43 100

72 32.5 19.8 29.6#

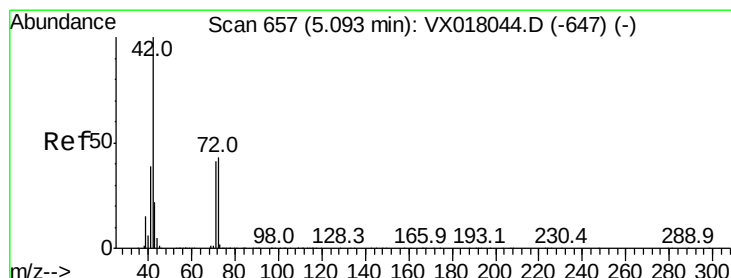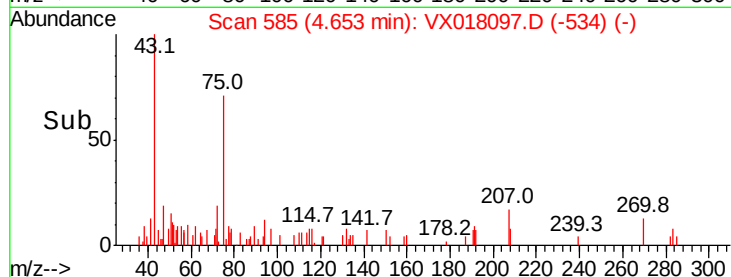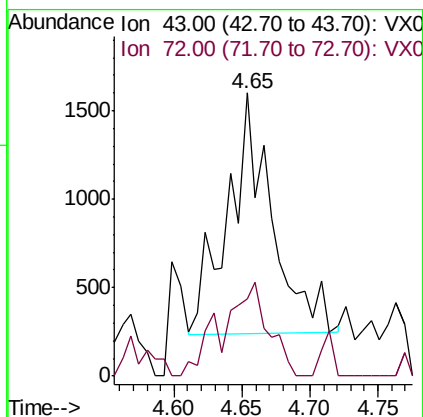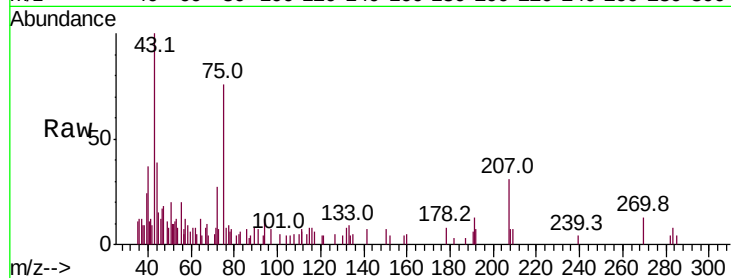

#29

Tetrahydrofuran

Concen: 0.280 ug/l

RT: 5.10 min Scan# 659

Delta R.T. 0.01 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27




Tgt Ion: 42 Resp: 927


Ion Ratio Lower Upper

42 100

72 62.0 34.2 51.4#

71 34.7 32.1 48.1


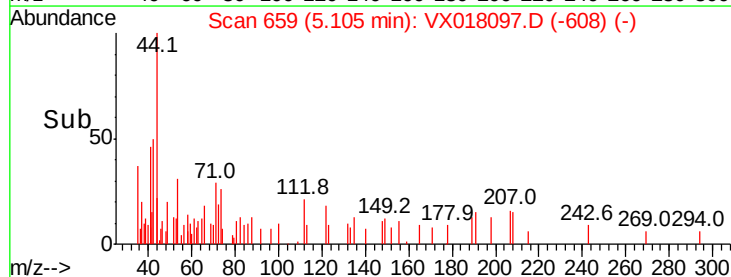
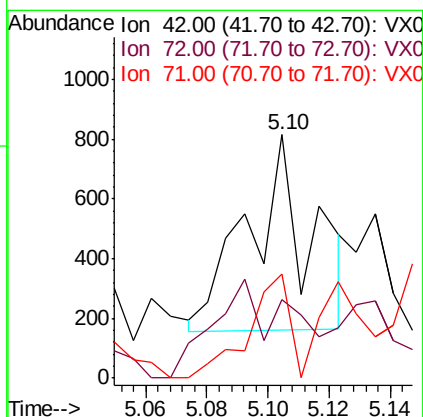
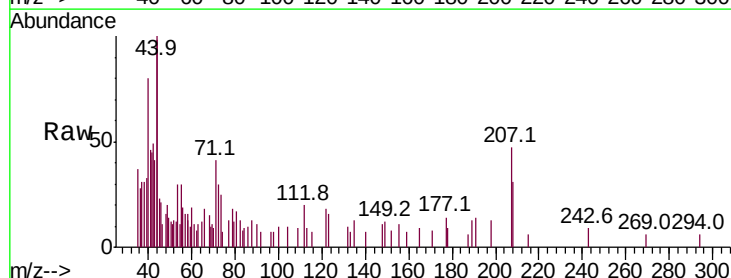


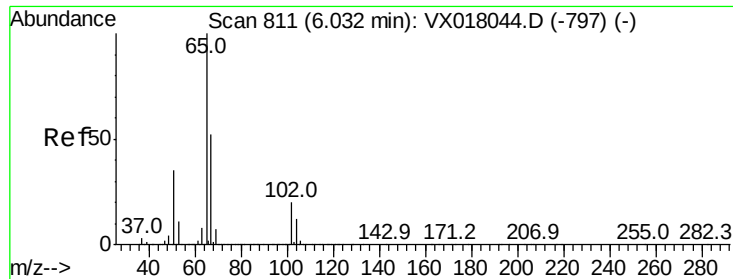

#33
 1,2-Dichloroethane-d4
 Concen: 47.985 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27




Instrument :
 MSVOA_X
 ClientSampleId :
 FM782


Tot Ion: 65 Resp: 389614
 Ion Ratio Lower Upper
 65 100
 67 52.3 0.0 105.8

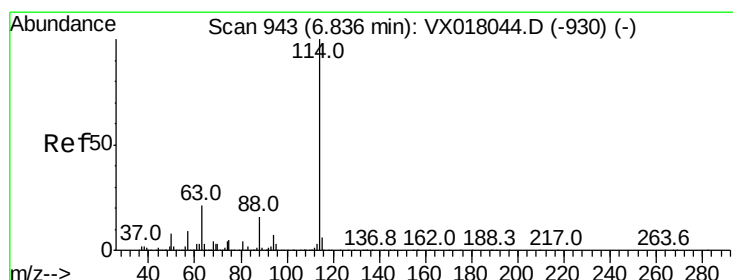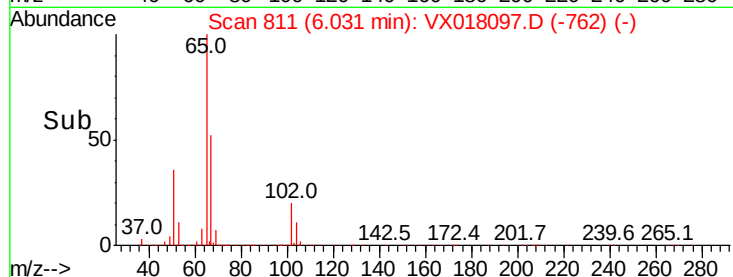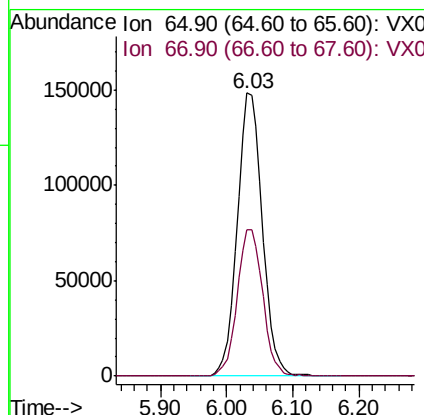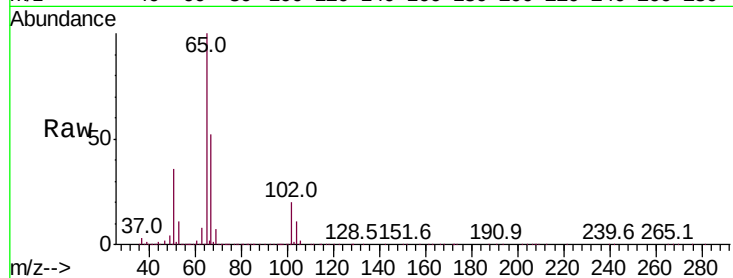

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.84 min Scan# 943
 Delta R.T. -0.00 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27

Tgt Ion: 114 Resp: 946297
 Ion Ratio Lower Upper
 114 100
 63 20.5 0.0 42.6
 88 17.1 0.0 31.8


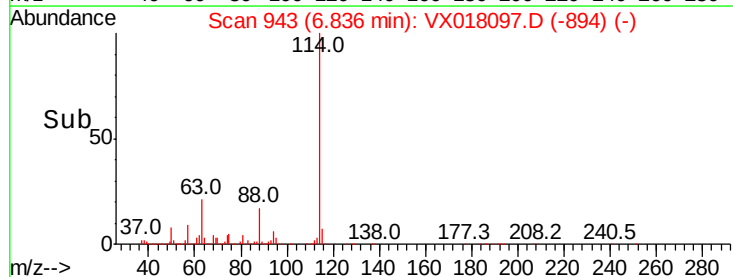
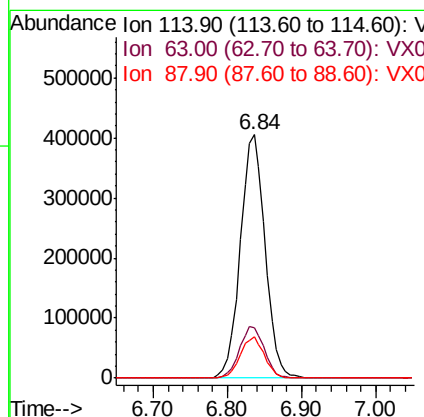
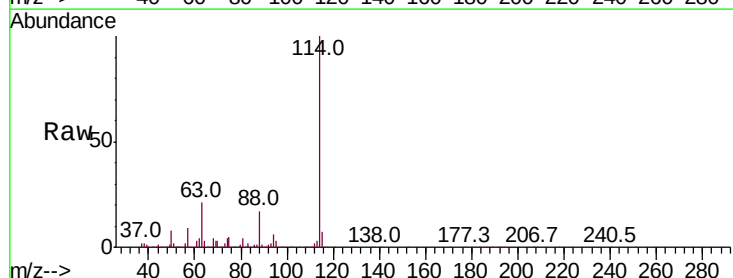


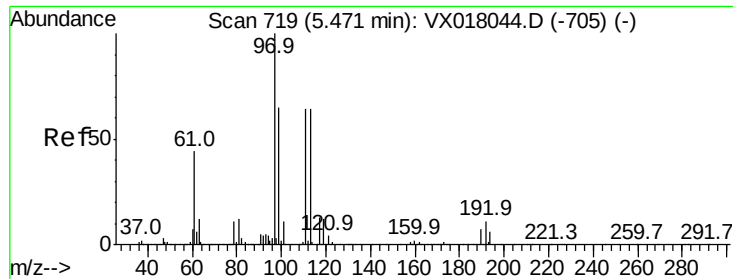

#35
 Dibromofluoromethane
 Concen: 49.528 ug/l
 RT: 5.47 min Scan# 719
 Delta R.T. -0.00 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27




Instrument :
 MSVOA_X
 ClientSampled :
 FM782


Tot Ion	Ratio	Lower	Upper
113	100		
111	101.8	81.6	122.4
192	20.0	15.8	23.8

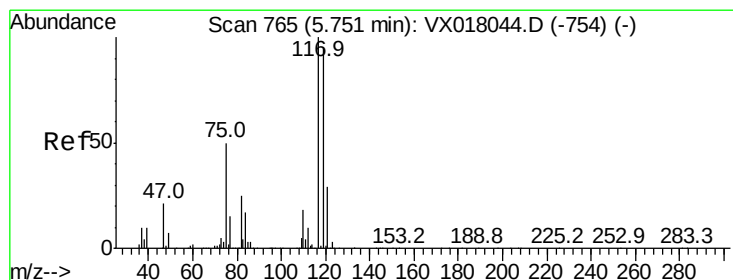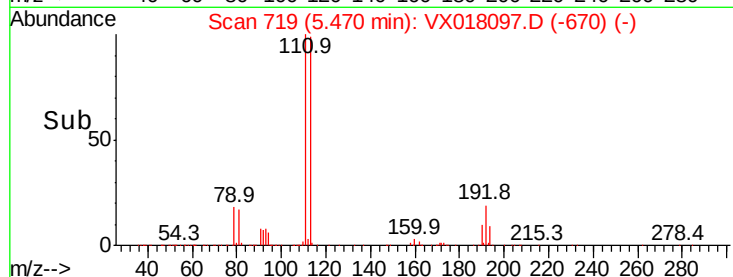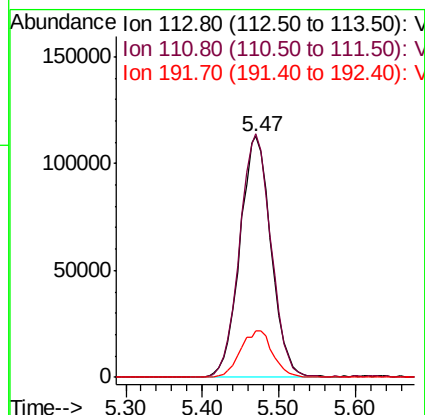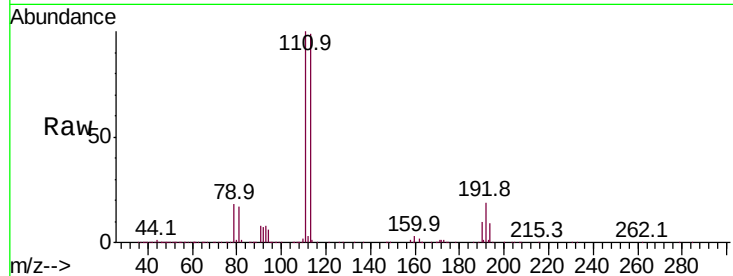

#38
 Carbon Tetrachloride
 Concen: 6.287 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.12 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27

Tgt Ion	Ratio	Lower	Upper
117	100		
119	4.5	75.8	113.6#
121	0.0	23.4	35.0#


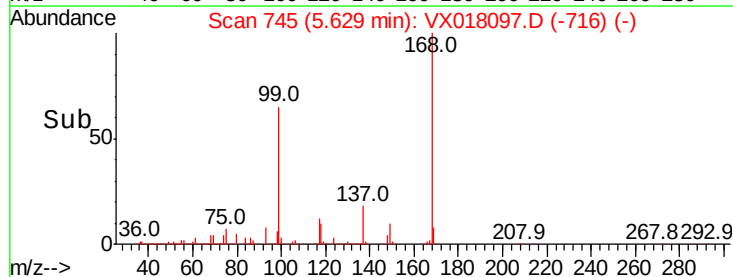
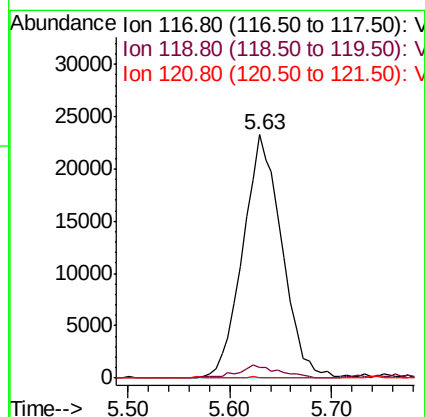
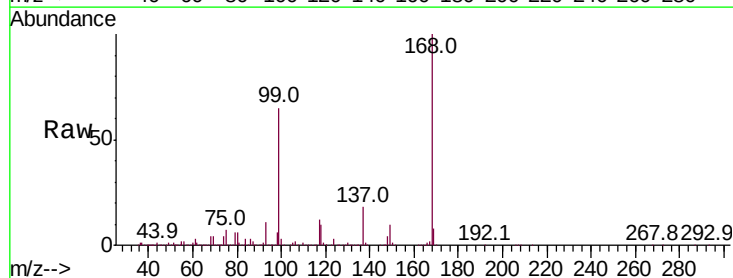


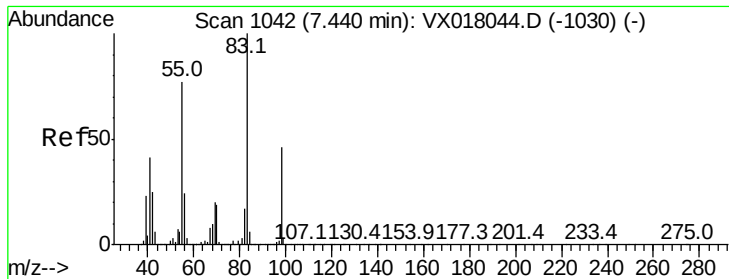

#39
Methylvlcyclohexane
Concen: 0.212 ug/l
RT: 7.44 min Scan# 1042
Delta R.T. -0.00 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27




Instrument :
MSVOA_X
ClientSampled :
FM782


Tot Ion: 83 Resp: 2021
Ion Ratio Lower Upper
83 100
55 66.0 61.8 92.6
98 44.0 36.6 55.0

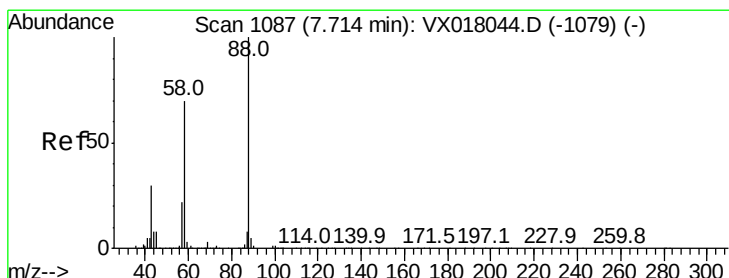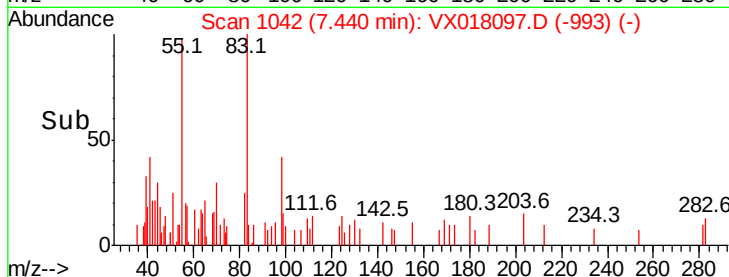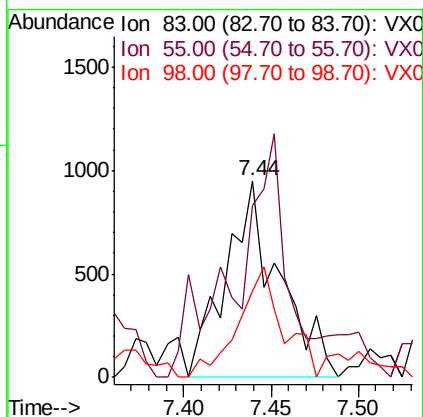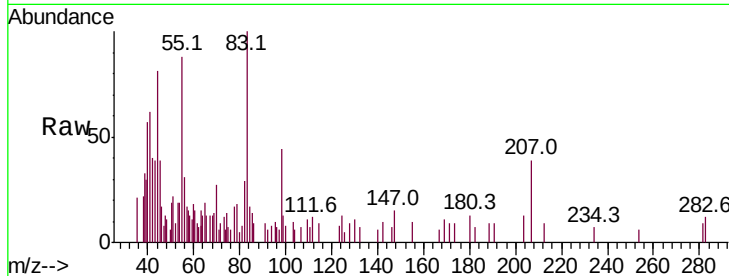

#49
1,4-Dioxane
Concen: 4.524 ug/l
RT: 7.74 min Scan# 1091
Delta R.T. 0.02 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27

Tgt Ion: 88 Resp: 668
Ion Ratio Lower Upper
88 100
43 0.0 27.4 41.0#
58 145.2 56.4 84.6#


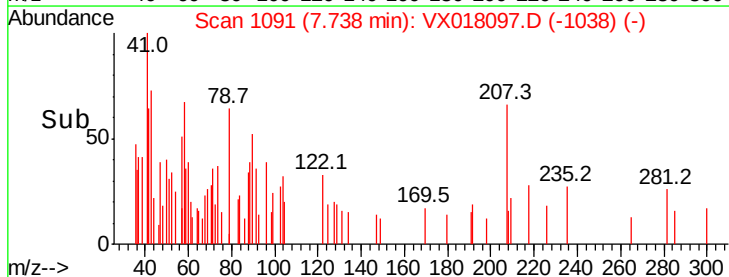
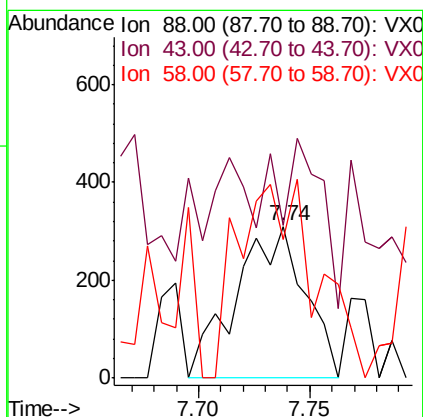
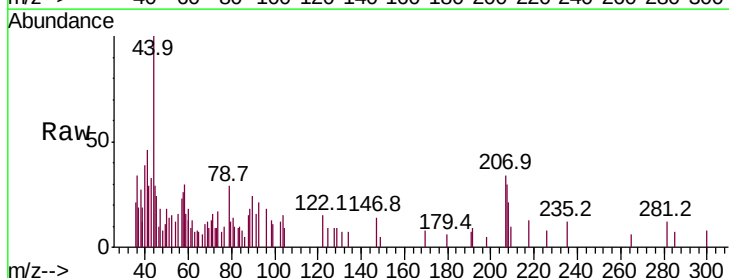


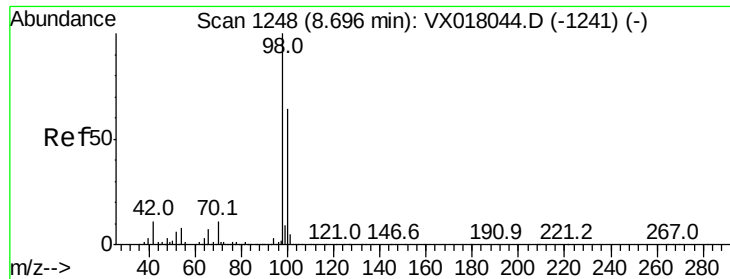

#50
Toluene-d8
Concen: 49.220 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27




Instrument :
MSVOA_X
ClientSampleId :
FM782


Tot Ion: 98 Resp: 1181477
Ion Ratio Lower Upper
98 100
100 63.6 52.2 78.4

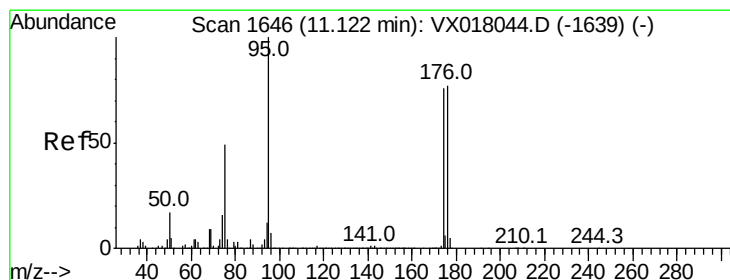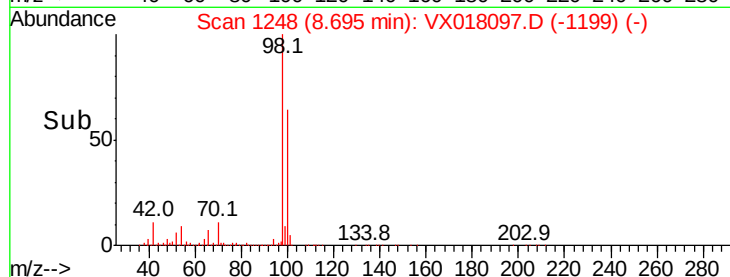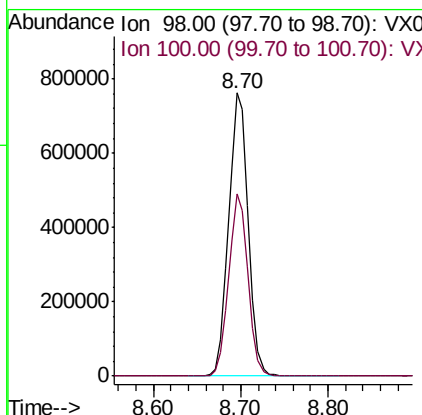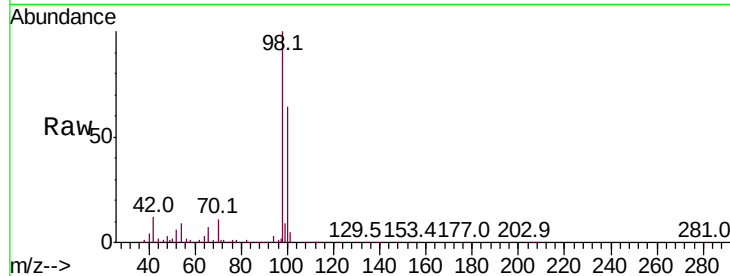

#62
4-Bromofluorobenzene
Concen: 46.402 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27

Tgt Ion: 95 Resp: 438219
Ion Ratio Lower Upper
95 100
174 78.8 0.0 160.2
176 74.4 0.0 155.8

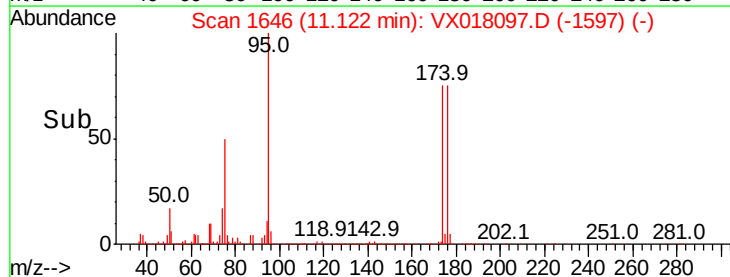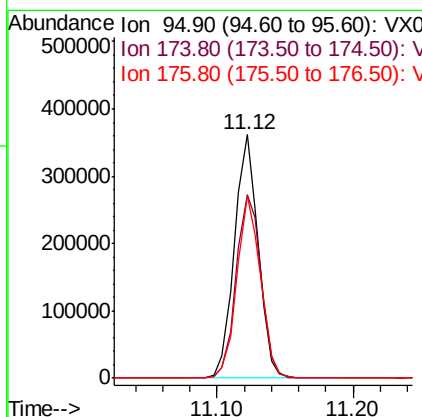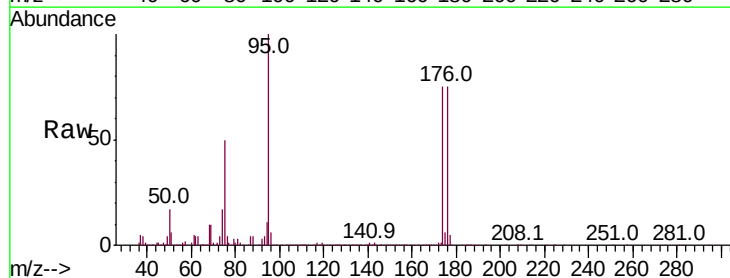

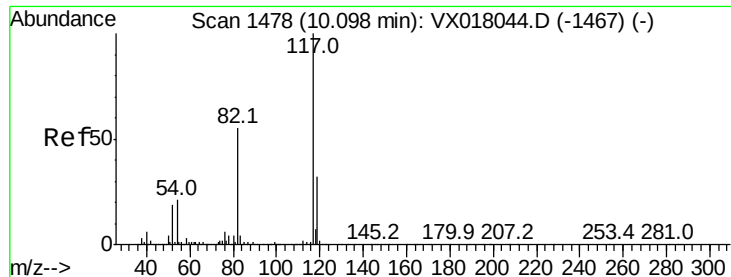

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. -0.00 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampled :

FM782


Tot Ion:117 Resp: 914663

Ion Ratio Lower Upper

117 100

82 55.7 44.2 66.2




119 33.4 25.7 38.5

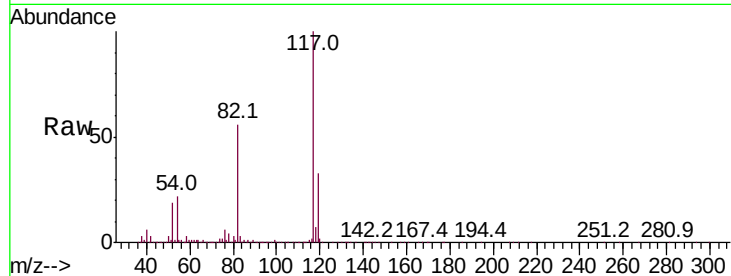

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

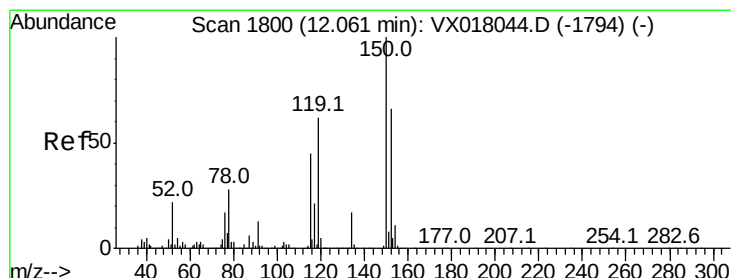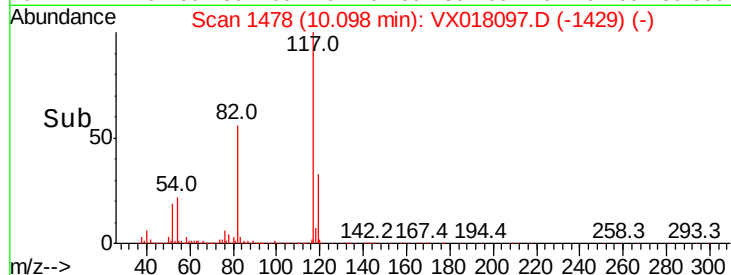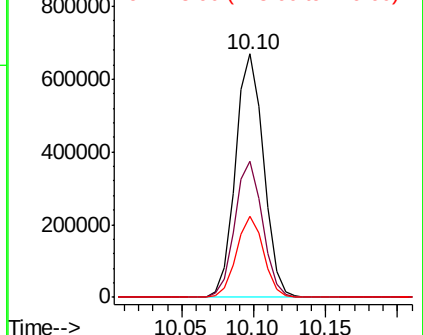

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27


Tgt Ion:152 Resp: 421656

Ion Ratio Lower Upper

152 100

115 60.7 41.5 124.5



150 160.1 0.0 343.8

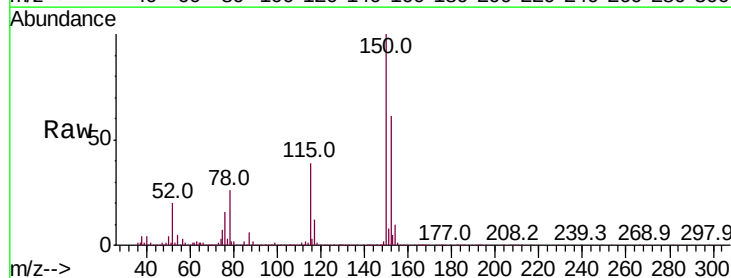


Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

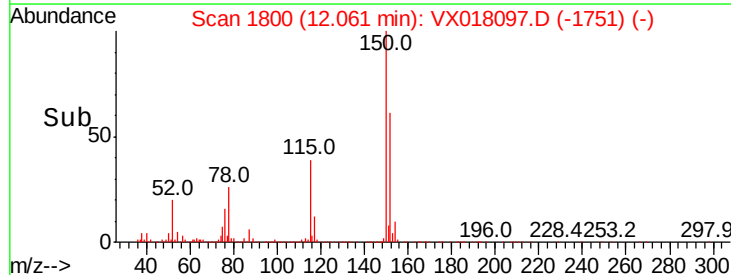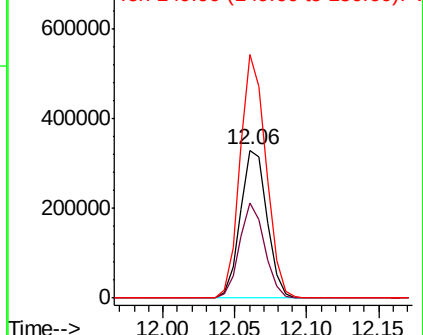

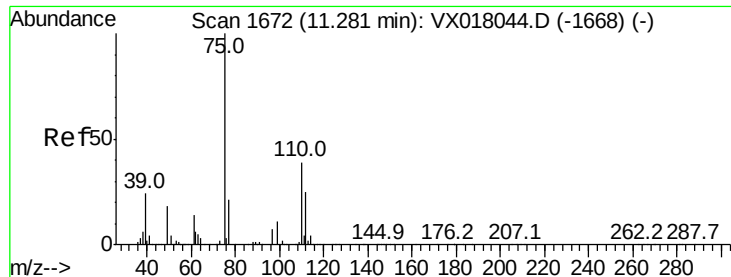

#76

1,2,3-Trichloropropane

Concen: 23.766 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampleId :


FM782

Tot Ion: 75 Resp: 222919

Ion Ratio Lower Upper

75 100

77 1.3 20.8 62.2#

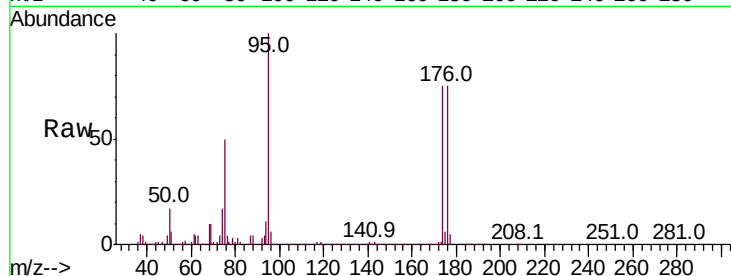

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

11.12

200000



150000

100000

50000

0

Time--> 11.05 11.10 11.15 11.20

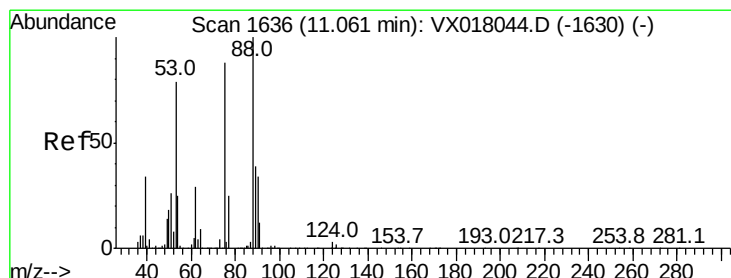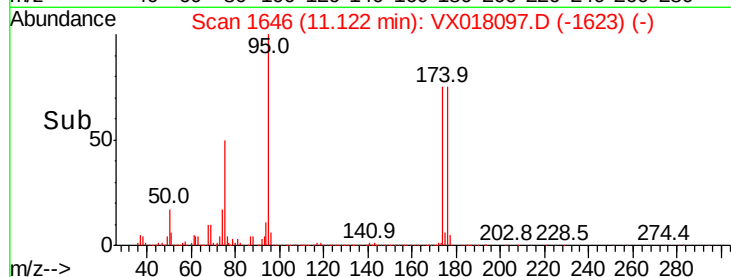

#81

trans-1,4-Dichloro-2-butene

Concen: 64.187 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27


Tgt Ion: 75 Resp: 222919

Ion Ratio Lower Upper

75 100

53 0.3 74.7 112.1#

89 0.1 36.6 54.8#

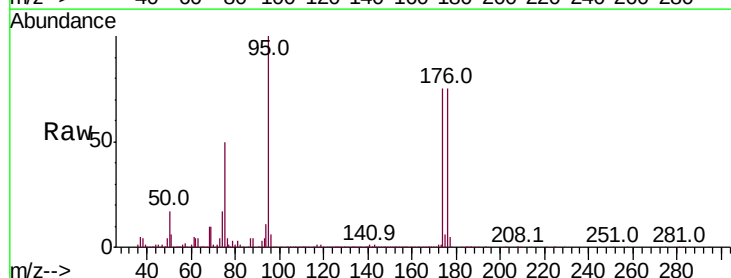

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

250000

200000


150000


100000

50000

0

Time--> 11.05 11.10 11.15 11.20




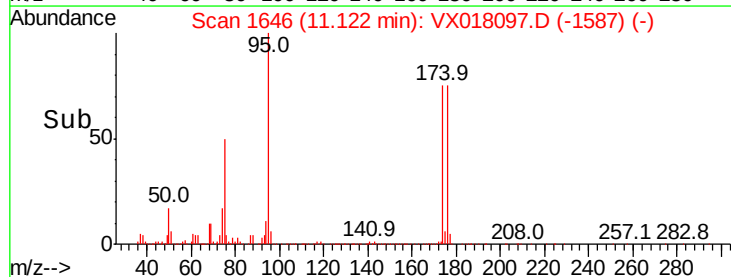


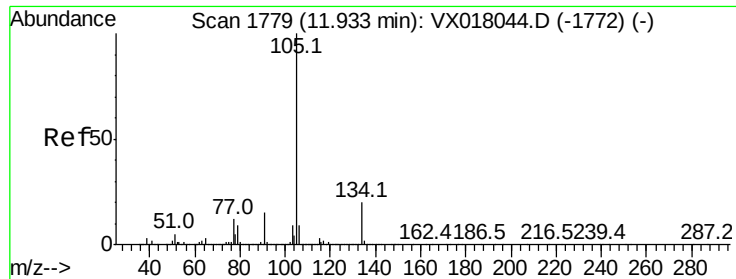

#85
 sec-Butylbenzene
 Concen: 0.235 ug/l
 RT: 11.93 min Scan# 1779
 Delta R.T. -0.00 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27




Instrument :
 MSVOA_X
 ClientSampleId :
 FM782


Tot Ion:105 Resp: 6026
 Ion Ratio Lower Upper
 105 100
 134 30.1 10.1 30.3

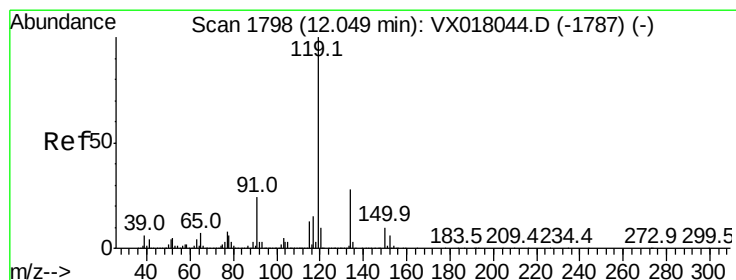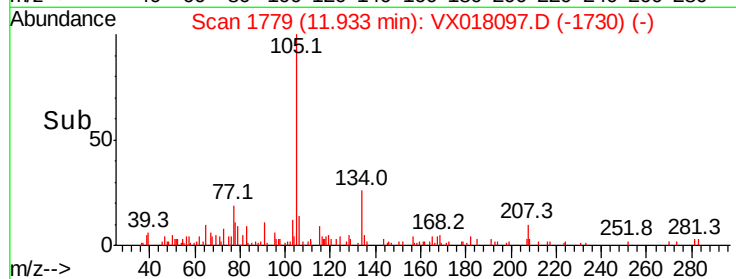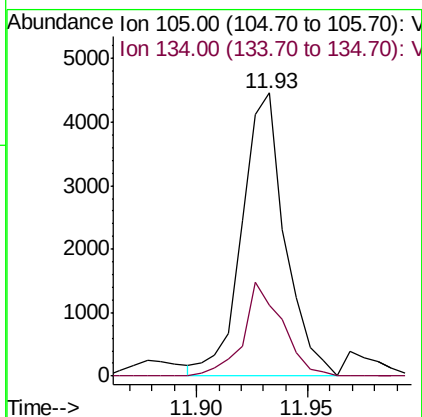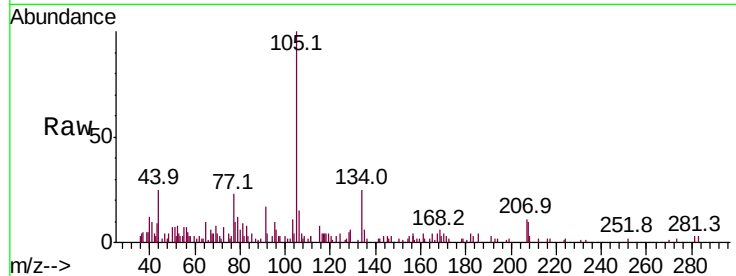

#86
 p-Isopropyltoluene
 Concen: 0.265 ug/l
 RT: 12.05 min Scan# 1798
 Delta R.T. -0.00 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27

Tgt Ion:119 Resp: 6238
 Ion Ratio Lower Upper
 119 100
 134 28.7 13.2 39.5
 91 48.5 11.8 35.4#


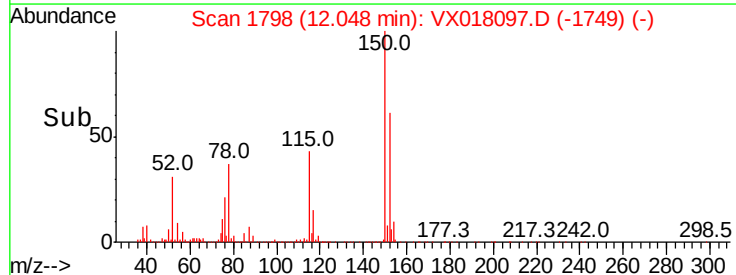
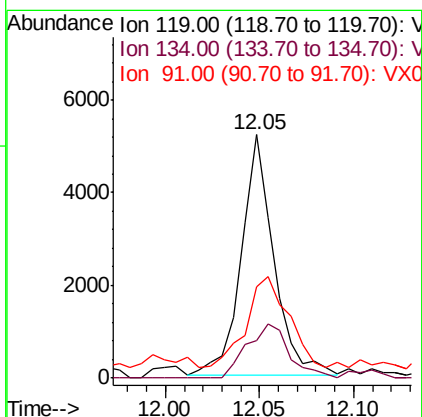
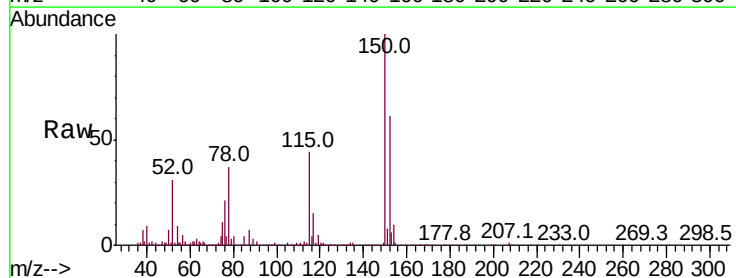


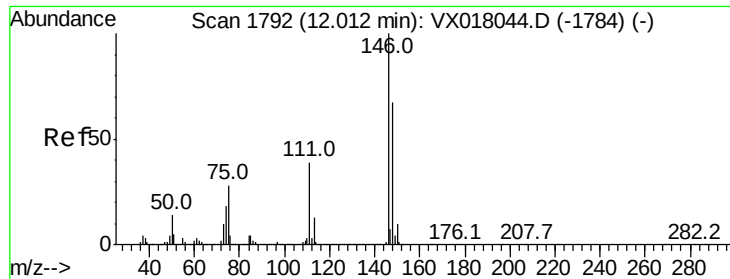

#87
 1,3-Dichlorobenzene
 Concen: 0.205 ug/l
 RT: 12.01 min Scan# 1792
 Delta R.T. -0.00 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27




Instrument :
 MSVOA_X
 ClientSampleId :
 FM782


Tot Ion	Ratio	Lower	Upper
146	100		
111	37.2	20.6	61.8
148	54.6	33.1	99.2

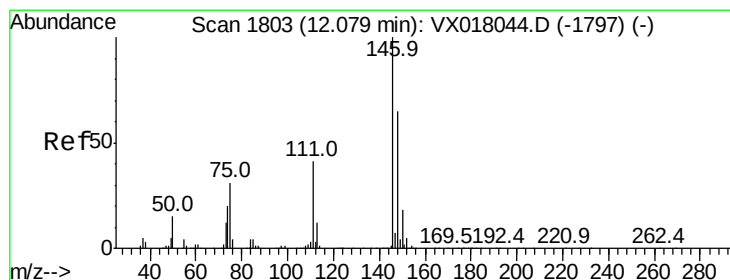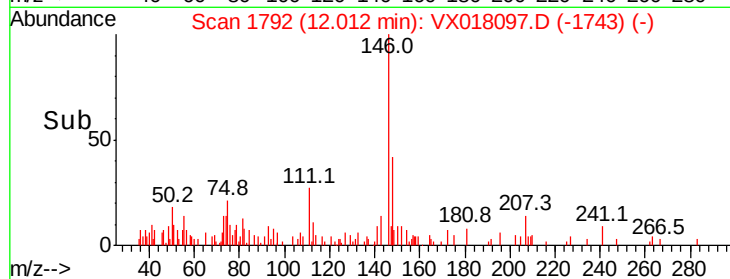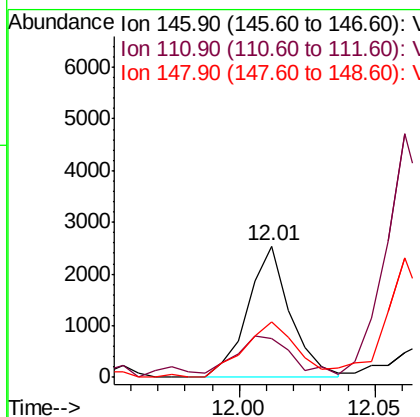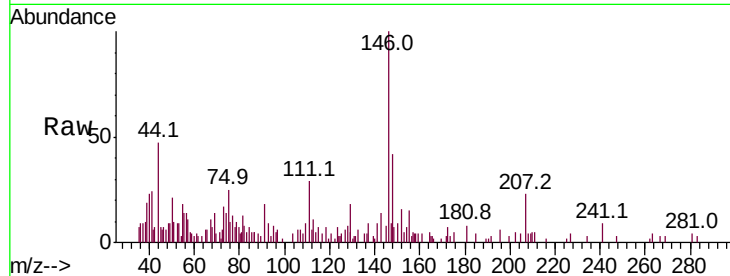

#88
 1,4-Dichlorobenzene
 Concen: 0.205 ug/l
 RT: 12.01 min Scan# 1792
 Delta R.T. -0.07 min
 Lab File: VX018097.D
 Acq: 27 Aug 2020 17:27

Tgt Ion	Ratio	Lower	Upper
146	100		
111	37.2	20.3	60.8
148	54.6	33.1	99.2


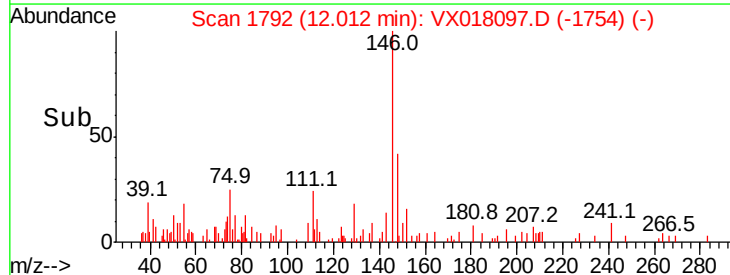
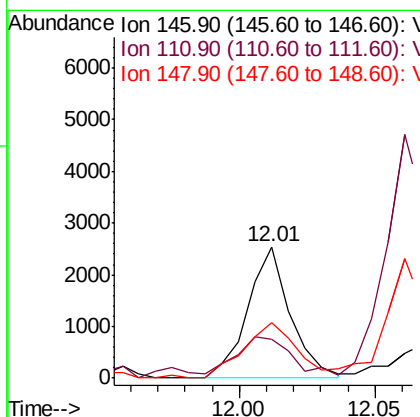
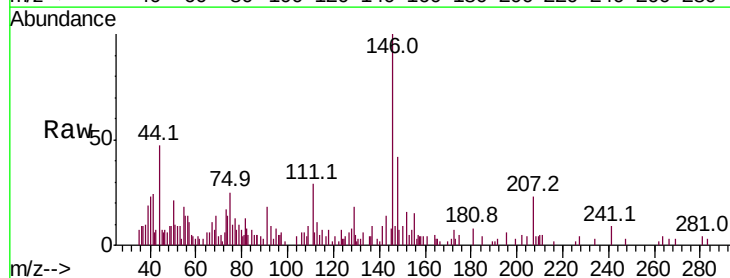


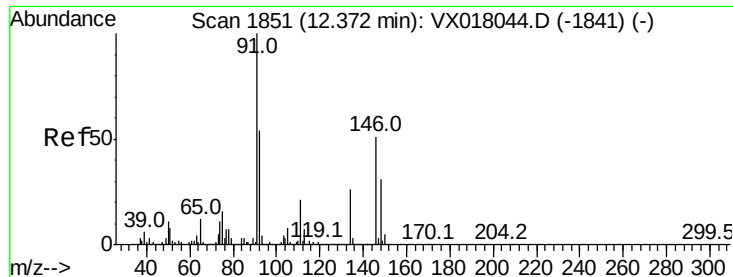

#89
n-Butylbenzene
Concen: 0.354 ug/l
RT: 12.37 min Scan# 1851
Delta R.T. -0.00 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27




Instrument :
MSVOA_X
ClientSampled :
FM782


Tot Ion	Ratio	Lower	Upper
91	100		
92	53.4	26.4	79.2
134	26.2	12.9	38.7

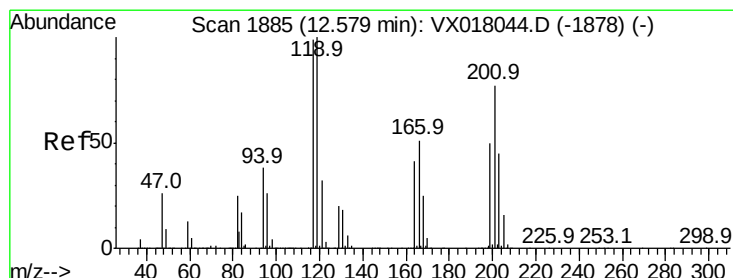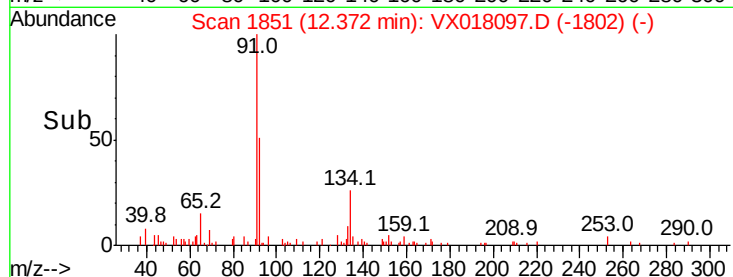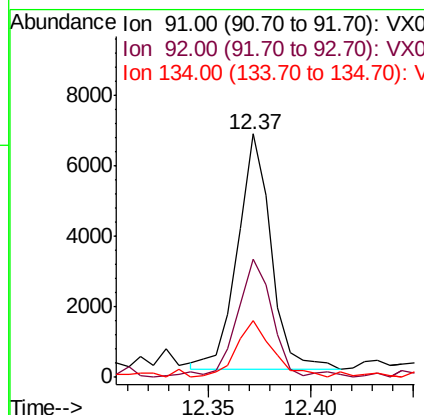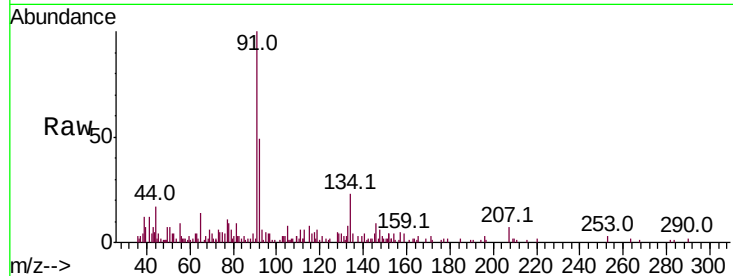

#90
Hexachloroethane
Concen: 0.288 ug/l
RT: 12.58 min Scan# 1885
Delta R.T. -0.00 min
Lab File: VX018097.D
Acq: 27 Aug 2020 17:27

Tgt Ion	Ratio	Lower	Upper
117	100		
201	67.9	38.5	115.3

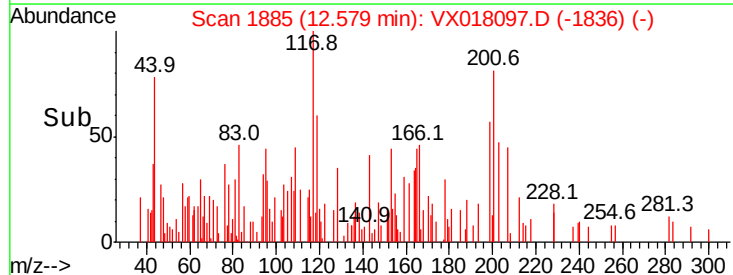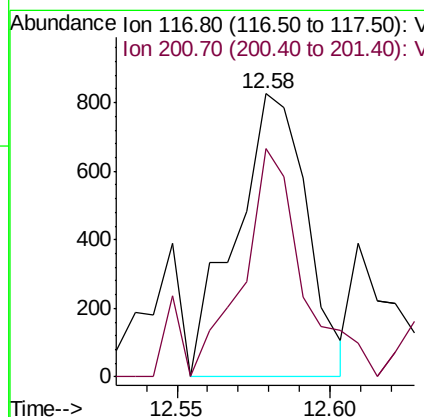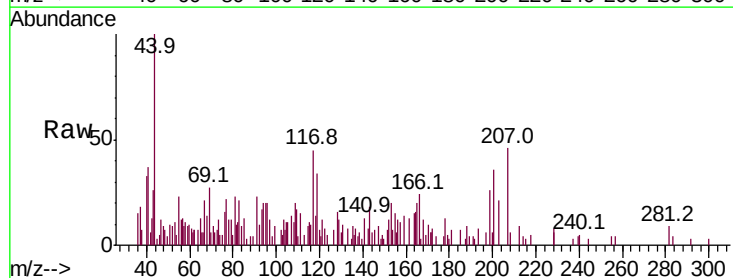

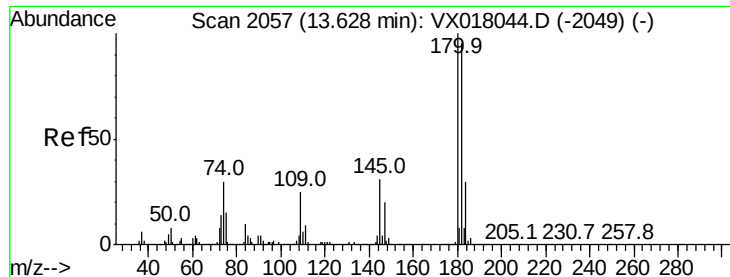

#93

1,2,4-Trichlorobenzene

Concen: 0.477 ug/l

RT: 13.63 min Scan# 2057

Delta R.T. -0.00 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampled :

FM782


Tot Ion:180 Resp: 4044

Ion Ratio Lower Upper

180 100

182 80.2 47.5 142.6




145 43.2 15.7 47.1

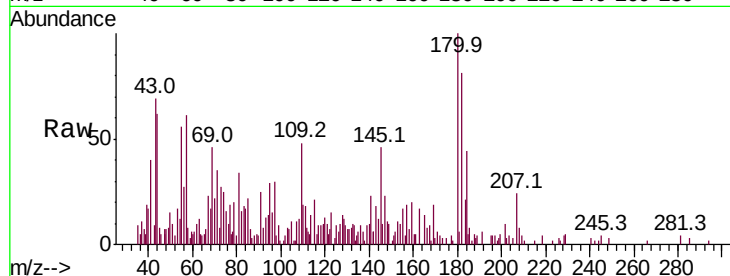

Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.80 (144.50 to 145.50): V

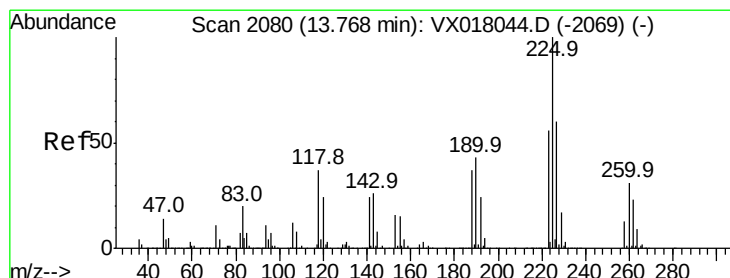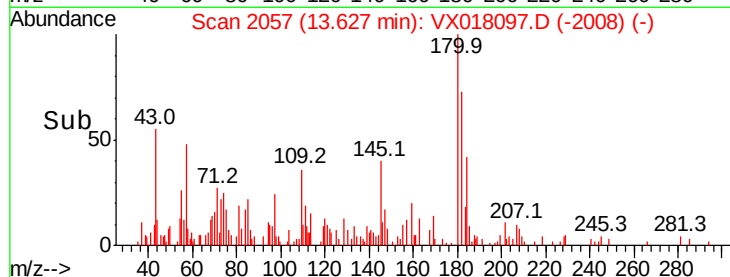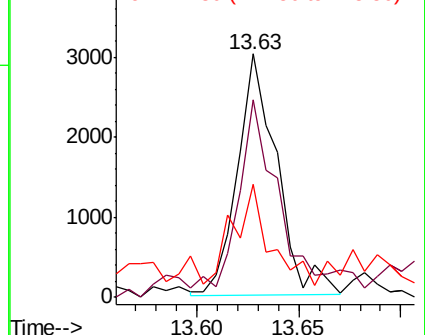

#94

Hexachlorobutadiene

Concen: 0.675 ug/l

RT: 13.77 min Scan# 2080

Delta R.T. -0.00 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27


Tgt Ion:225 Resp: 2257

Ion Ratio Lower Upper

225 100

223 94.4 30.7 92.1#



227 82.4 32.6 97.8

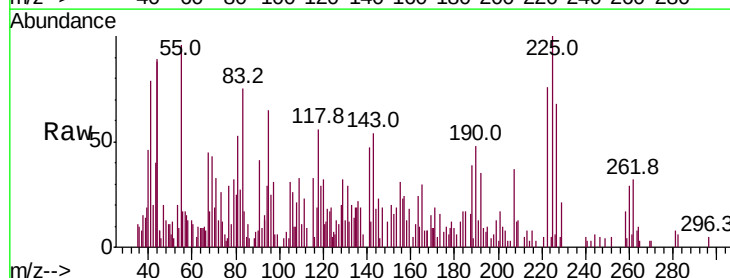


Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

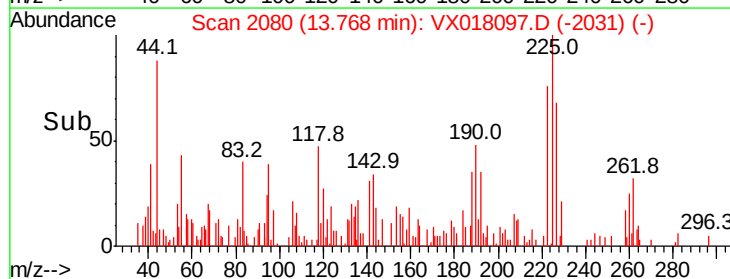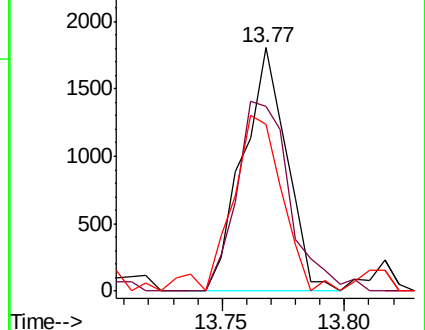

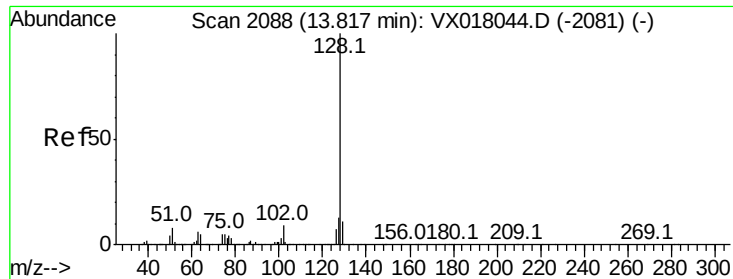

#95

Naphthalene

Concen: 0.224 ug/l

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Instrument :

MSVOA_X

ClientSampled :

FM782





Tot Ion:128 Resp: 6239

Ion Ratio Lower Upper

128 100

127 30.4 10.2 15.2#

129 14.6 8.7 13.1#

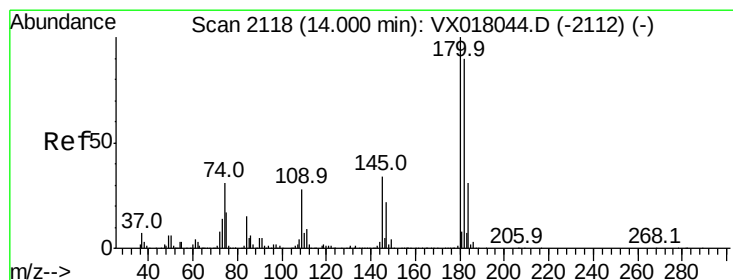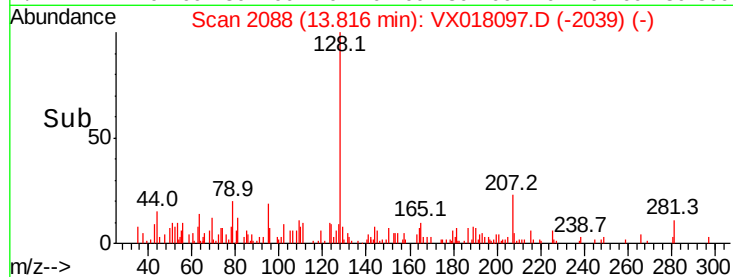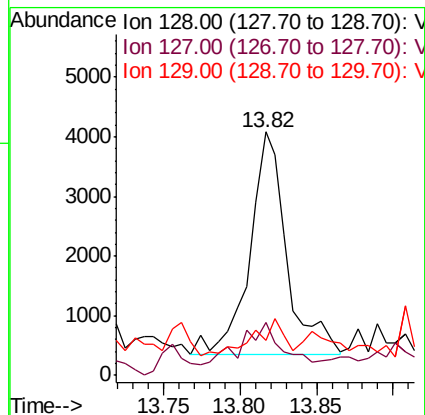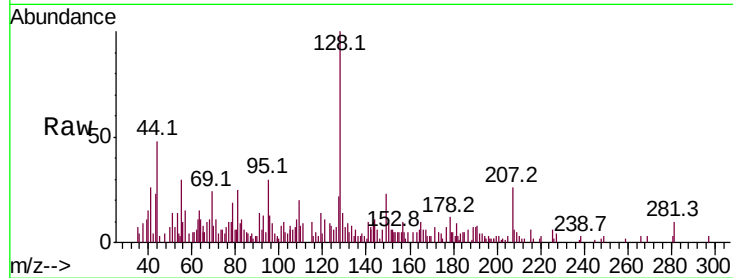

#96

1,2,3-Trichlorobenzene

Concen: 0.396 ug/l

RT: 14.01 min Scan# 2119

Delta R.T. 0.01 min

Lab File: VX018097.D

Acq: 27 Aug 2020 17:27

Tgt Ion:180 Resp: 3316

Ion Ratio Lower Upper

180 100

182 96.9 47.3 142.0

145 49.1 17.5 52.6

