
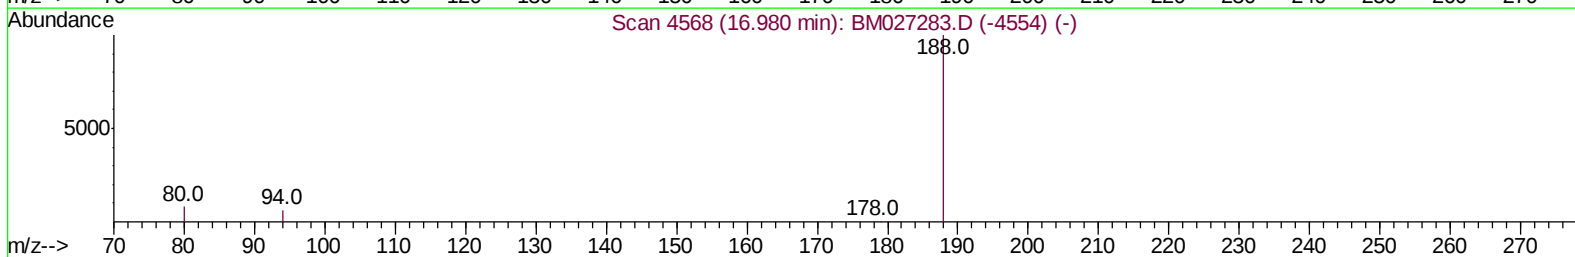
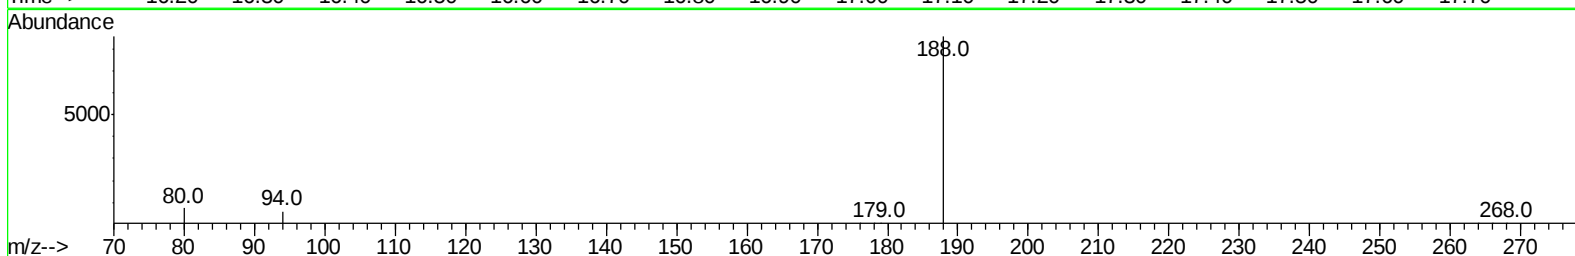


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082820\
Data File : BM027284.D
Acq On : 28 Aug 2020 10:51
Operator : JU/CG
Sample : PB131070BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
SSTD02006

Quant Time: Aug 28 11:28:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 10:39:41 2020
Response via : Initial Calibration

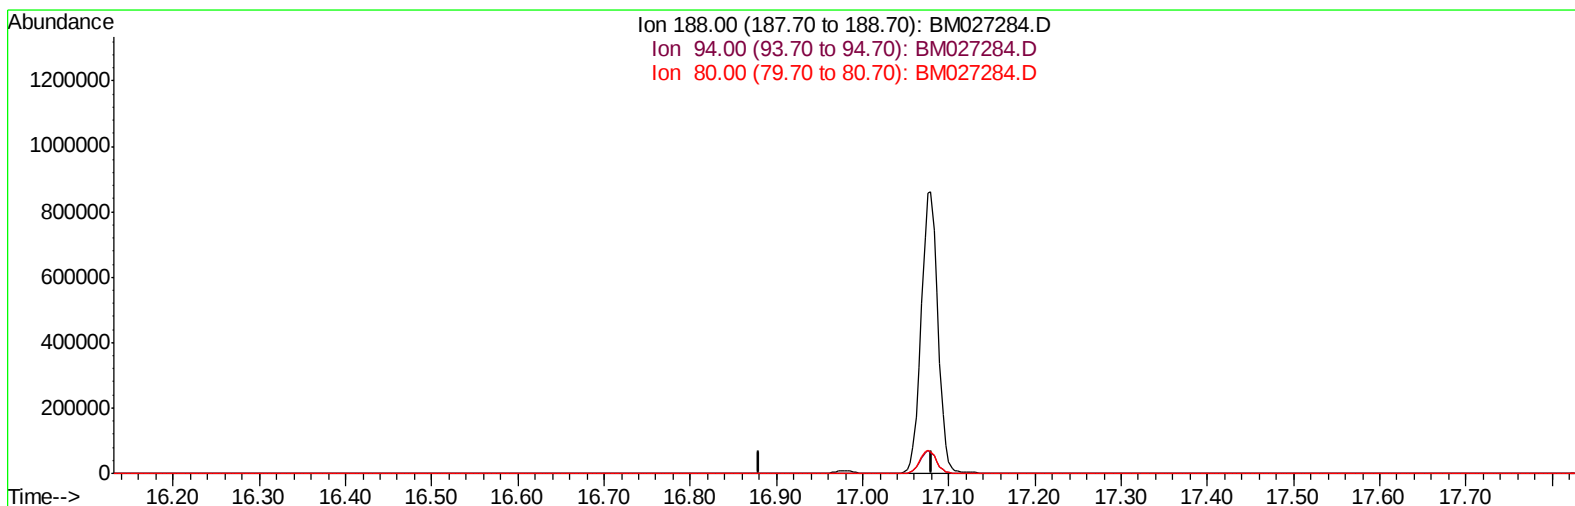

TIC: BM027284.D

(10) Phenanthrene-d10 (I)

16.980min (-16.980) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.80	0.00#
80.00	9.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082820\
 Data File : BM027284.D
 Acq On : 28 Aug 2020 10:51
 Operator : JU/CG
 Sample : PB131070BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 SST02006

Quant Time: Aug 28 11:28:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 28 10:39:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2457	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	8607	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	5963	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.98
16) Chrysene-d12	21.18	240	9275	0.40	ng/ul	0.00
20) Perylene-d12	23.36	264	9160	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	5045	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.02	212	11358	0.00	ng/ul	0.00
Target Compounds				Ovalue		
9) Fluorene	15.23	166	2047	0.076	ng/ul#	14
17) Pyrene	19.38	202	2115	0.053	ng/ul#	1
23) Benzo(a)pyrene	23.22	252	3522	0.099	ng/ul#	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM082820\
Data File : BM027284.D
Acq On : 28 Aug 2020 10:51
Operator : JU/CG
Sample : PB131070BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
SSTD02006

Quant Time: Aug 28 11:28:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM081720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 28 10:39:41 2020
Response via : Initial Calibration

