


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082720\
 Data File : VX018087.D
 Acq On : 27 Aug 2020 13:22
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082120W.M
 Title : SW846 8260
 Last Update : Fri Aug 21 03:03:56 2020

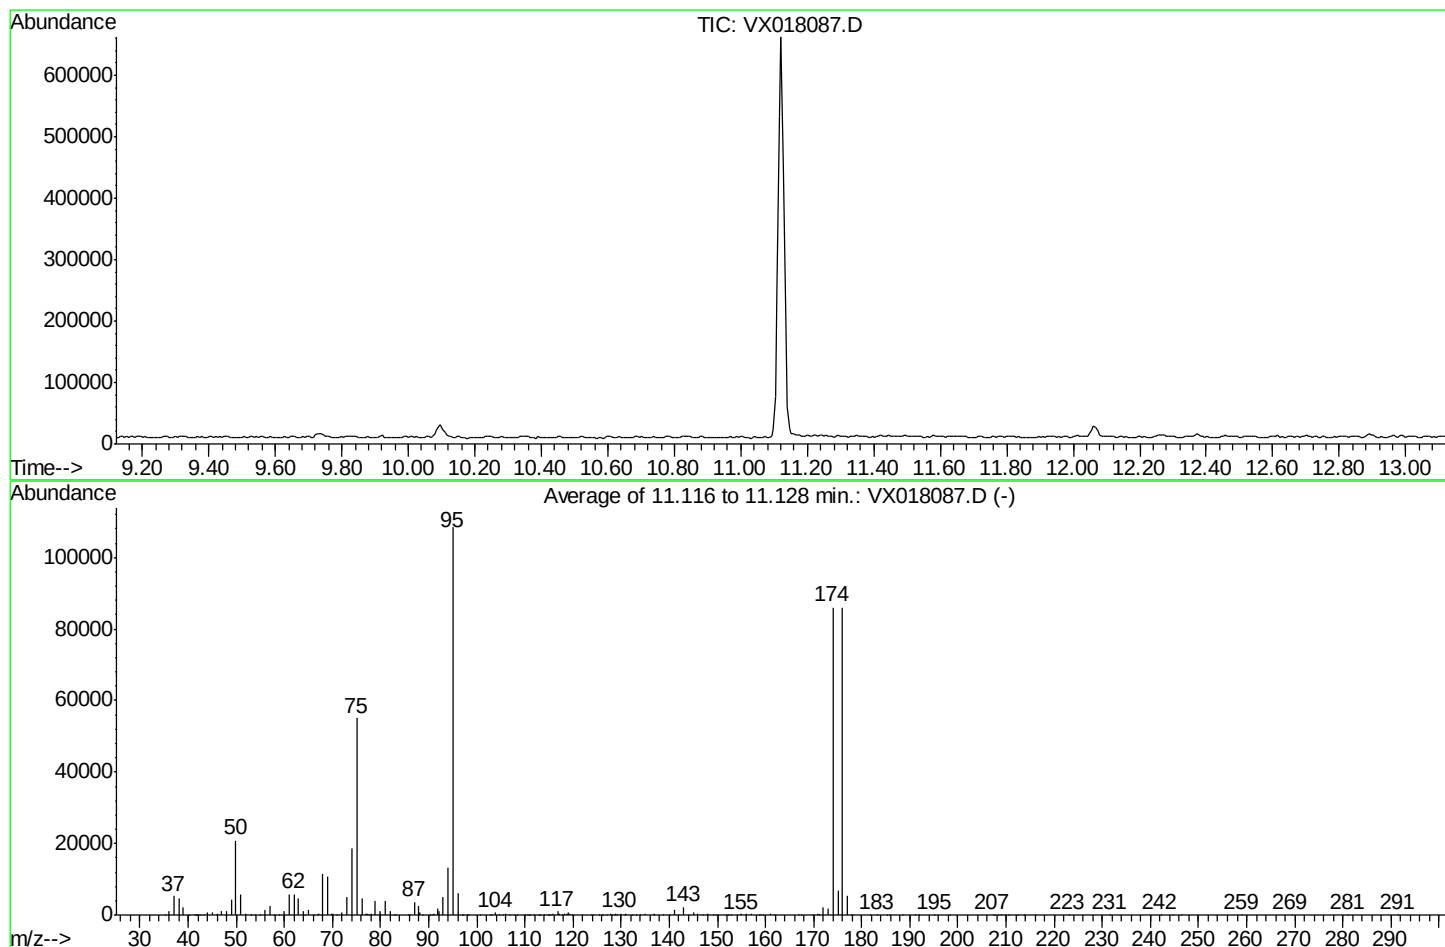

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	20839	PASS
75	95	30	60	50.7	55045	PASS
95	95	100	100	100.0	108464	PASS
96	95	5	9	5.7	6224	PASS
173	174	0.00	2	1.9	1654	PASS
174	95	50	100	79.2	85957	PASS
175	174	5	9	8.0	6848	PASS
176	174	95	101	99.9	85845	PASS
177	176	5	9	6.4	5458	PASS