
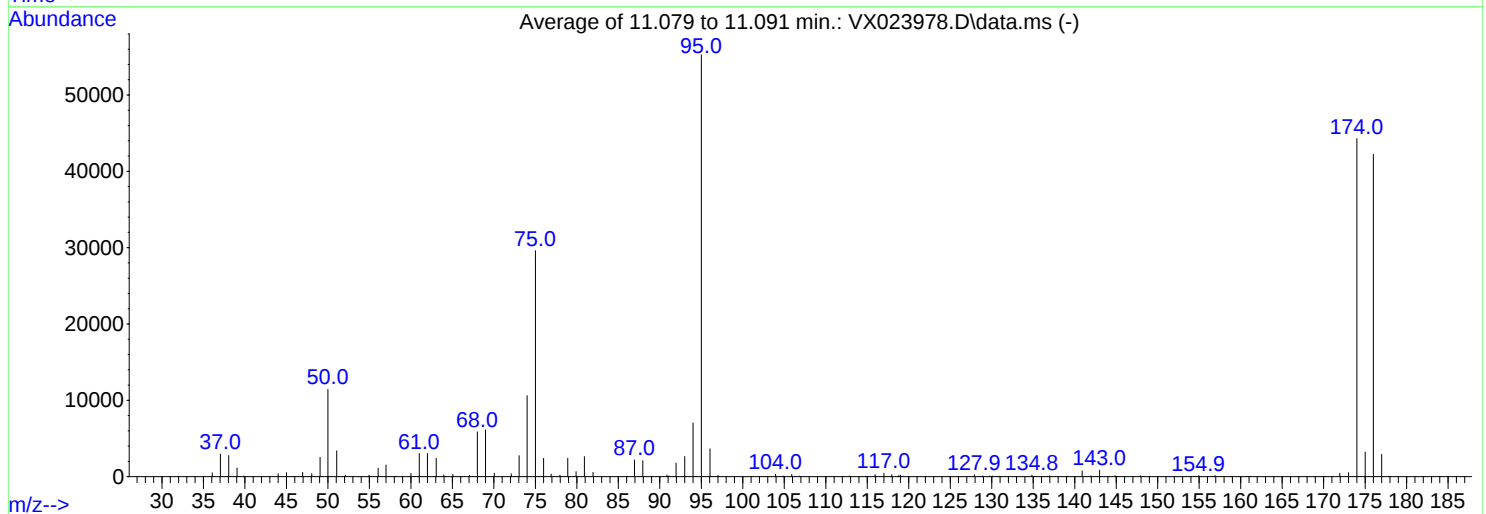


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082721\
Data File : VX023978.D
Acq On : 27 Aug 2021 08:28
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Title : SW846 8260
Last Update : Tue Aug 17 11:57:51 2021

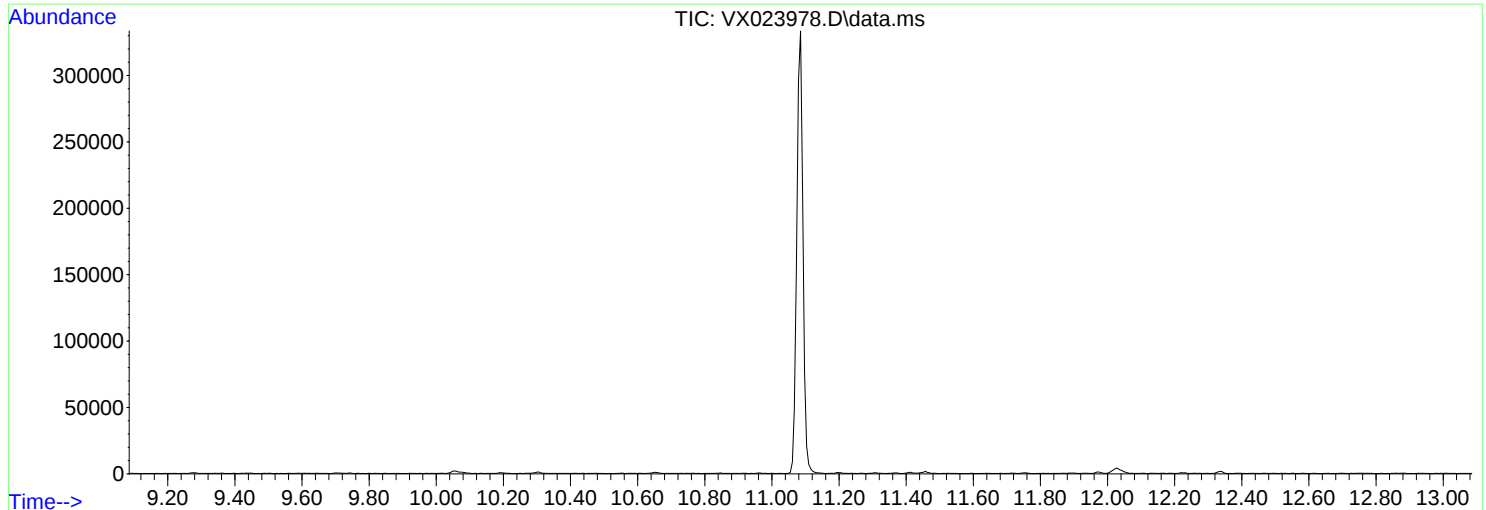

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	11426	PASS
75	95	30	60	53.6	29605	PASS
95	95	100	100	100.0	55261	PASS
96	95	5	9	6.6	3647	PASS
173	174	0.00	2	1.2	533	PASS
174	95	50	100	80.2	44299	PASS
175	174	5	9	7.3	3224	PASS
176	174	95	101	95.3	42219	PASS
177	176	5	9	6.9	2922	PASS