

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
 Data File : VX030891.D
 Acq On : 27 Aug 2022 23:43
 Operator : JC/MD
 Sample : VX0827WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0827WBL02

Quant Time: Aug 29 01:13:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	194112	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	327563	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	288366	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	113467	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	134465	58.891	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	117.780%
35) Dibromofluoromethane	5.391	113	105462	52.387	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.780%
50) Toluene-d8	8.653	98	394609	56.251	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	112.500%
62) 4-Bromofluorobenzene	11.085	95	124111	47.520	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.040%
Target Compounds						
					Qvalue	
3) Chloromethane	1.288	50	391	Below Cal	#	61
4) Vinyl Chloride	1.374	62	310	Below Cal	#	84
5) Bromomethane	1.611	94	665	0.735	ug/l #	78
6) Chloroethane	1.684	64	415	Below Cal	#	41
9) 1,1,2-Trichlorotrifluo...	2.331	101	405	0.214	ug/l #	83
10) Methyl Iodide	2.453	142	575	4.364	ug/l #	55
11) Tert butyl alcohol	2.953	59	1529	3.085	ug/l #	74
12) 1,1-Dichloroethene	2.325	96	382	0.217	ug/l #	80
13) Acrolein	2.239	56	215	10.523	ug/l #	65
15) Acrylonitrile	3.074	53	696	0.573	ug/l #	77
16) Acetone	2.386	43	786	0.745	ug/l #	67
17) Carbon Disulfide	2.514	76	2057	Below Cal		99
20) Methylene Chloride	2.794	84	737	Below Cal	#	66
21) trans-1,2-Dichloroethene	3.087	96	491	0.260	ug/l #	83
25) 2-Butanone	4.611	43	698	0.411	ug/l #	48
29) Tetrahydrofuran	5.056	42	392	0.353	ug/l #	32
36) 1,1-Dichloropropene	5.696	75	568	0.207	ug/l #	57
38) Carbon Tetrachloride	5.556	117	20443	7.070	ug/l #	17
76) 1,2,3-Trichloropropane	11.085	75	65349	26.288	ug/l #	38
77) Bromobenzene	11.207	156	404	0.216	ug/l	82
78) n-propylbenzene	11.305	91	1874	0.214	ug/l	93
79) 2-Chlorotoluene	11.372	91	1151	0.215	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.085	75	65349	84.816	ug/l #	13
82) 4-Chlorotoluene	11.457	91	1599	0.266	ug/l	88
86) p-Isopropyltoluene	12.012	119	1571	0.239	ug/l #	80
87) 1,3-Dichlorobenzene	11.975	146	1205	0.341	ug/l	93
88) 1,4-Dichlorobenzene	11.975	146	1205	0.332	ug/l	92
89) n-Butylbenzene	12.335	91	1708	0.281	ug/l	88
91) 1,2-Dichlorobenzene	12.335	146	939	0.252	ug/l	91
93) 1,2,4-Trichlorobenzene	13.597	180	1274	0.548	ug/l	90
94) Hexachlorobutadiene	13.731	225	393	0.406	ug/l	82
95) Naphthalene	13.774	128	3470	0.428	ug/l	98
96) 1,2,3-Trichlorobenzene	13.963	180	1171	0.476	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
 Data File : VX030891.D
 Acq On : 27 Aug 2022 23:43
 Operator : JC/MD
 Sample : VX0827WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0827WBL02

Quant Time: Aug 29 01:13:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration




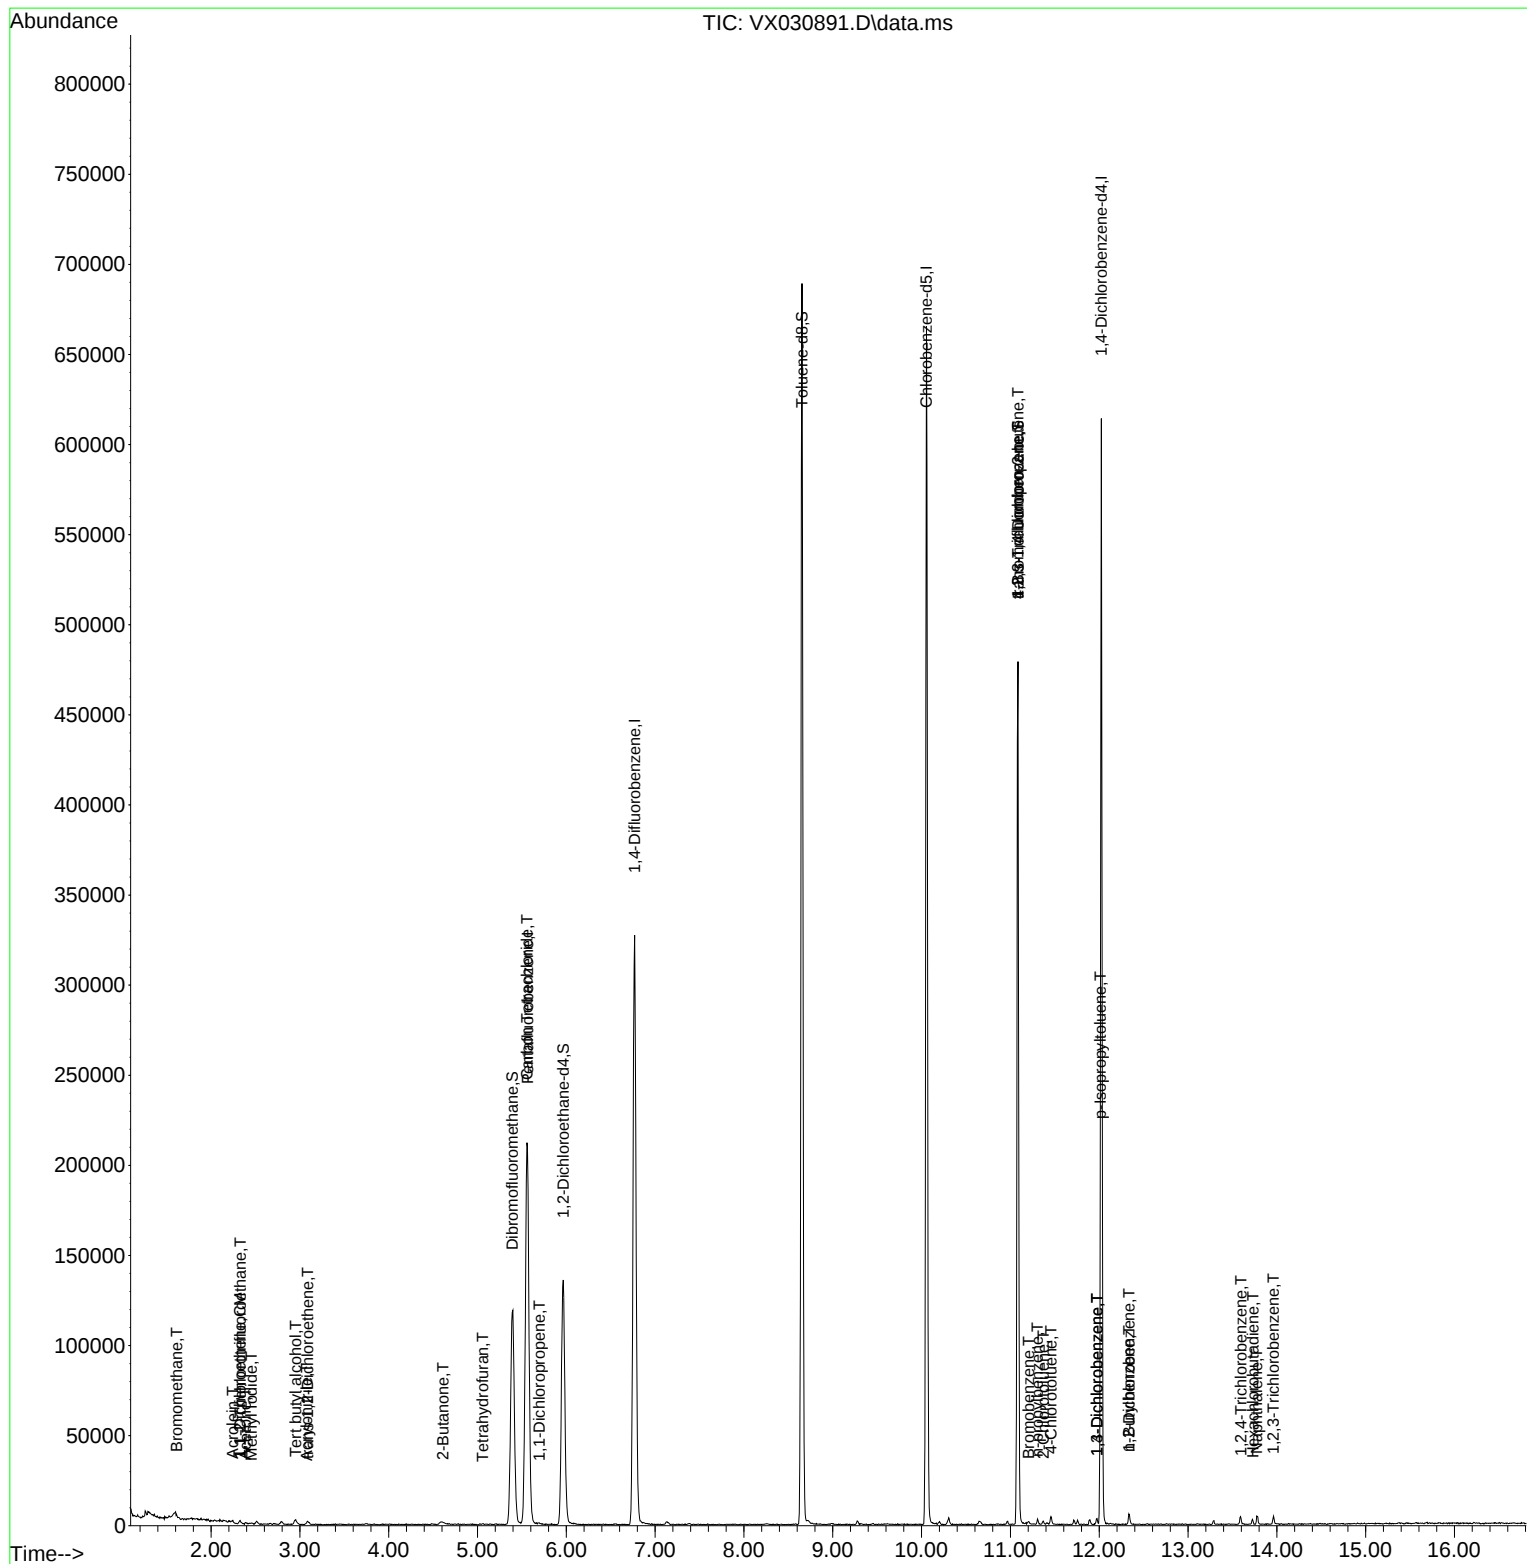




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion:168 Resp: 194112
Ion Ratio Lower Upper
168 100
99 61.2 44.0 66.0



#3
Chloromethane
Concen: Below Cal
RT: 1.288 min Scan# 33
Delta R.T. 0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 50 Resp: 391
Ion Ratio Lower Upper
50 100
52 54.7 26.3 39.5#




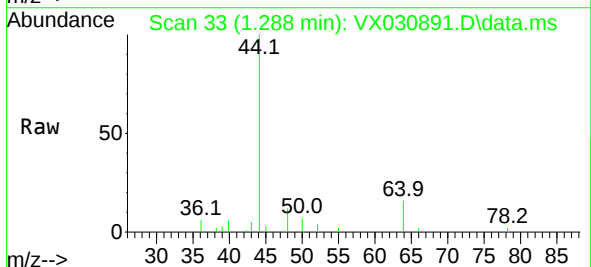


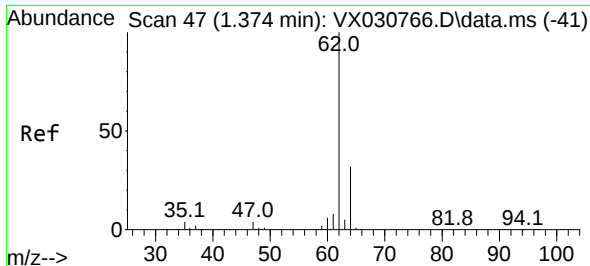

#4
 Vinyl Chloride
 Concen: Below Cal
 RT: 1.374 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VX030891.D
 Acq: 27 Aug 2022 23:43




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0827WBL02


Tgt Ion: 62 Resp: 310
 Ion Ratio Lower Upper
 62 100
 64 40.1 25.2 37.8#

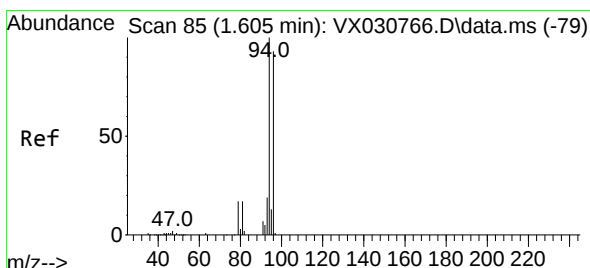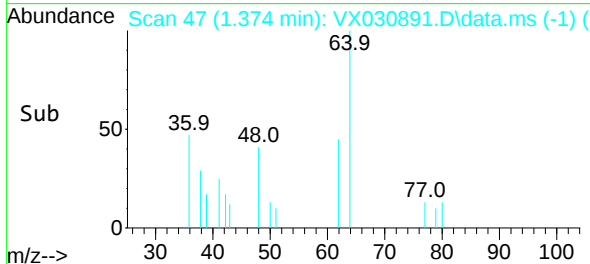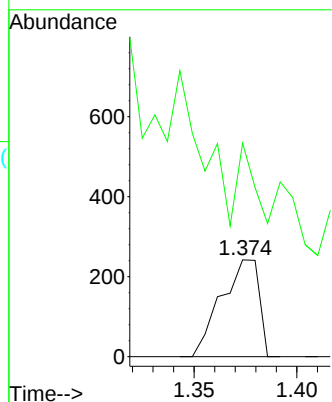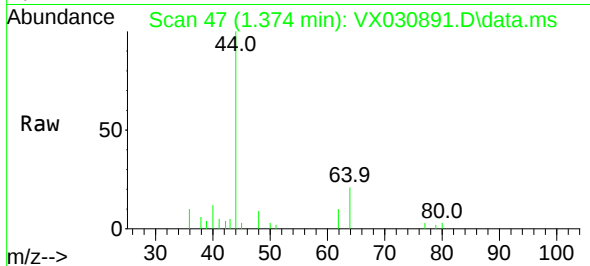

#5
 Bromomethane
 Concen: 0.735 ug/l
 RT: 1.611 min Scan# 86
 Delta R.T. 0.006 min
 Lab File: VX030891.D
 Acq: 27 Aug 2022 23:43

Tgt Ion: 94 Resp: 665
 Ion Ratio Lower Upper
 94 100
 96 74.5 76.9 115.3#


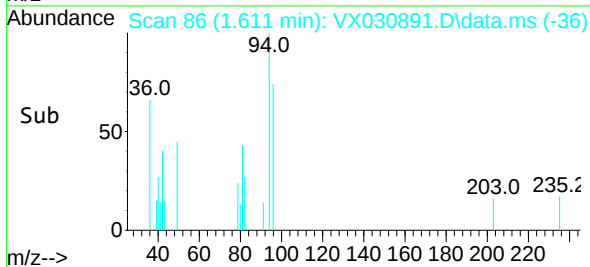
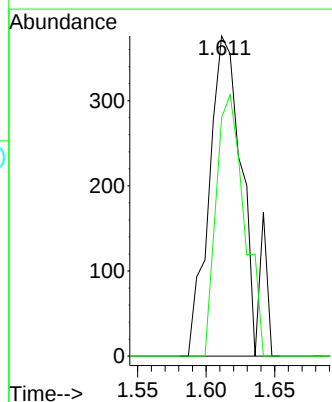
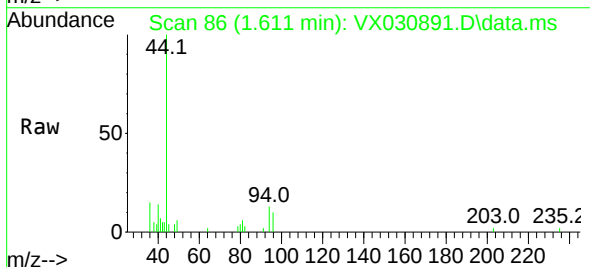


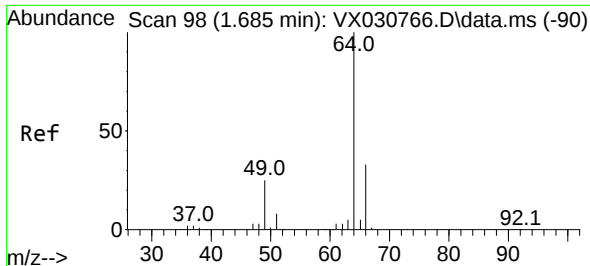

#6
Chloroethane
Concen: Below Cal
RT: 1.684 min Scan# 91
Delta R.T. -0.001 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion: 64 Resp: 415
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#

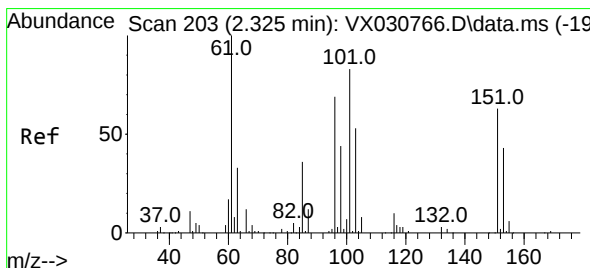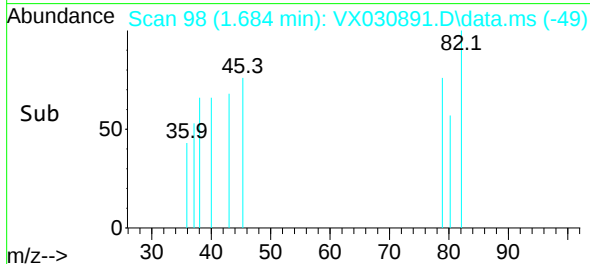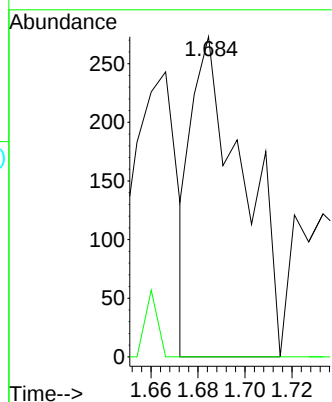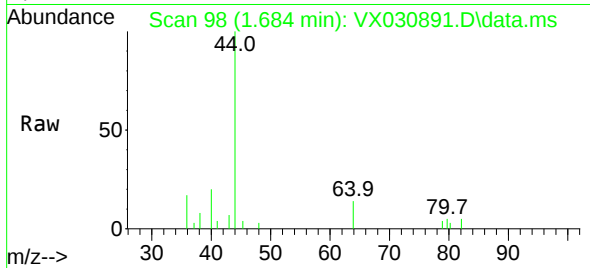

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.214 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43


Tgt Ion: 101 Resp: 405
Ion Ratio Lower Upper
101 100
85 24.9 34.0 51.0#
151 83.0 59.4 89.0

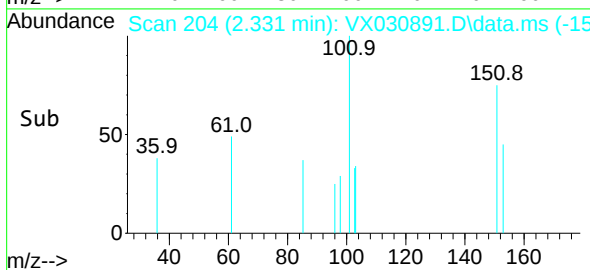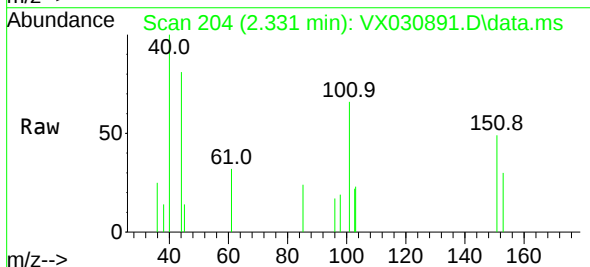



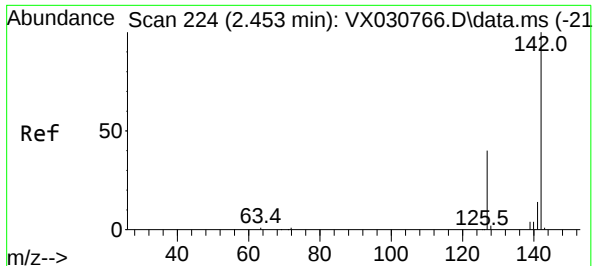


#10
Methyl Iodide
Concen: 4.364 ug/l
RT: 2.453 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02



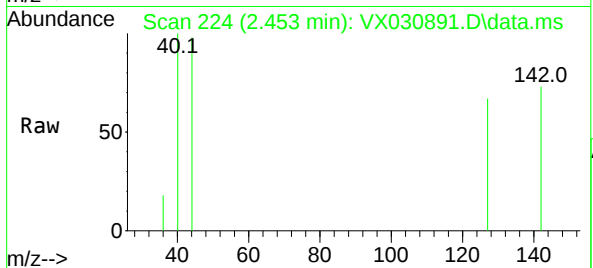



Tgt Ion:142 Resp: 575
Ion Ratio Lower Upper
142 100
127 67.5 30.2 45.2#
141 0.0 11.3 16.9#

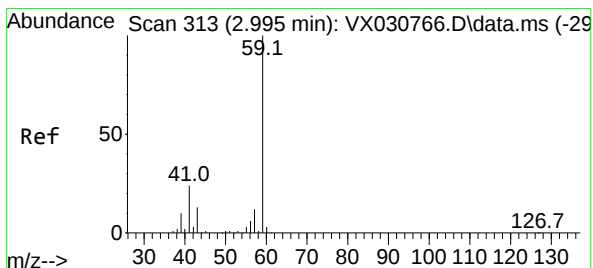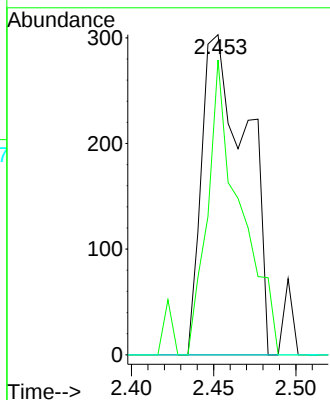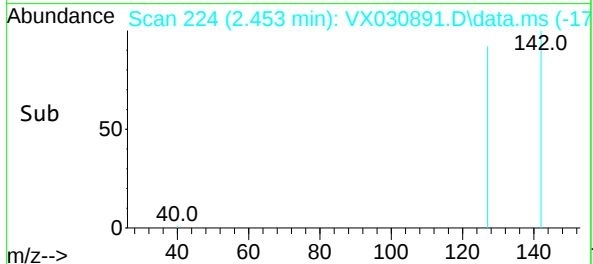

#11
Tert butyl alcohol
Concen: 3.085 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.043 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 59 Resp: 1529
Ion Ratio Lower Upper
59 100
57 0.0 7.4 11.2#

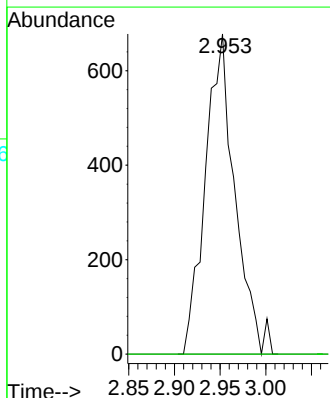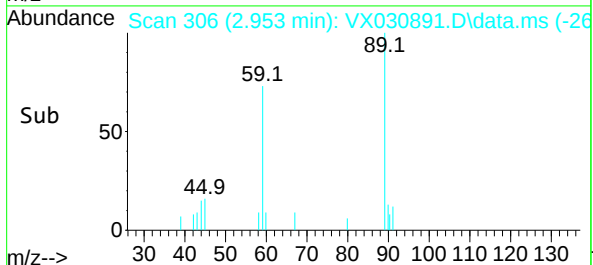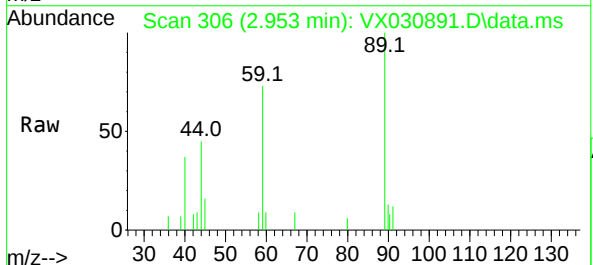

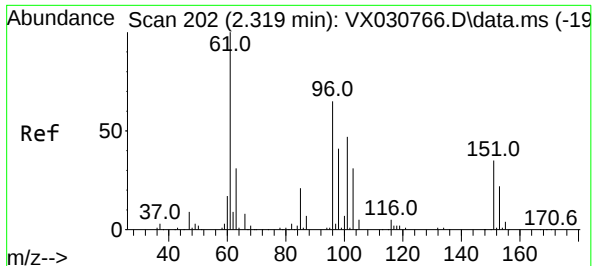

#12

1,1-Dichloroethene

Concen: 0.217 ug/l

RT: 2.325 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX030891.D

Acq: 27 Aug 2022 23:43

Instrument :

MSVOA_X

ClientSampleId :

VX0827WBL02





Tgt Ion: 96 Resp: 382

Ion Ratio Lower Upper

96 100

61 129.5 117.4 176.0

98 39.5 52.2 78.4#

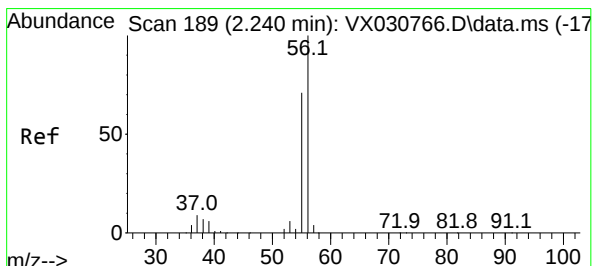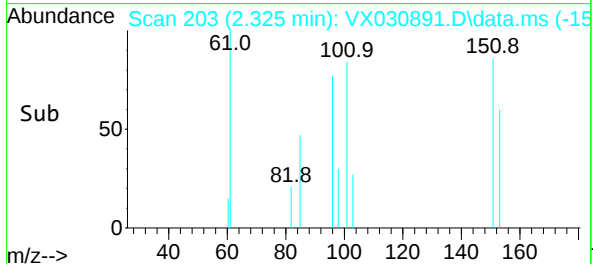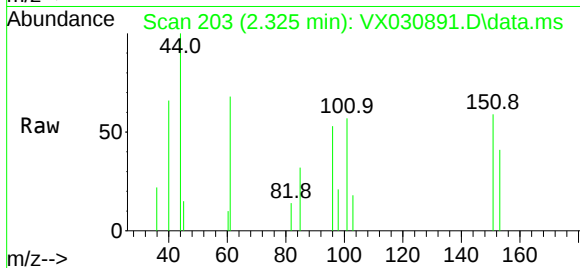

#13

Acrolein

Concen: 10.523 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.001 min

Lab File: VX030891.D




Acq: 27 Aug 2022 23:43


Tgt Ion: 56 Resp: 215

Ion Ratio Lower Upper

56 100

55 99.5 56.6 84.8#


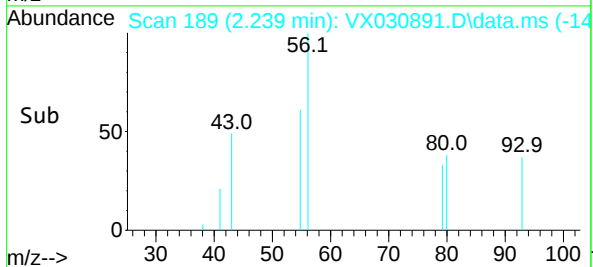

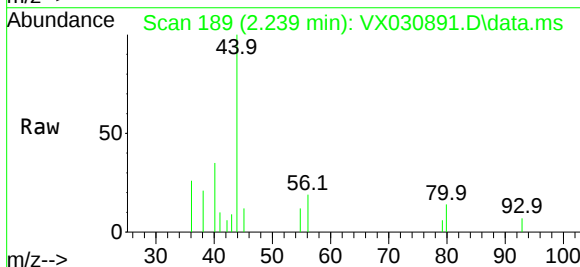




#15
Acrylonitrile
Concen: 0.573 ug/l
RT: 3.074 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion: 53 Resp: 696
Ion Ratio Lower Upper
53 100
52 55.2 65.4 98.0#
51 38.8 27.7 41.5



#16
Acetone
Concen: 0.745 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 43 Resp: 786
Ion Ratio Lower Upper
43 100
58 15.3 27.7 41.5#

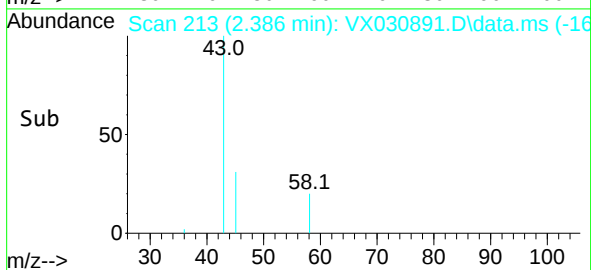







#20
Methylene Chloride
Concen: Below Cal
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02

Tgt Ion: 84 Resp: 737




Ion	Ratio	Lower	Upper
84	100		
49	78.5	93.8	140.6#
51	25.8	29.4	44.0#
86	30.8	51.0	76.4#

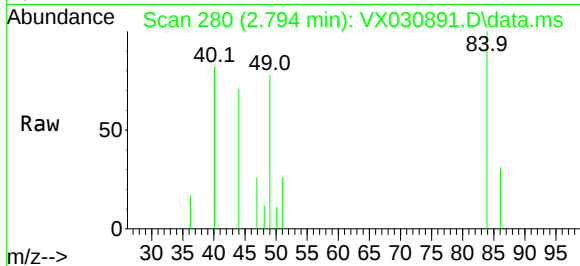


#21
trans-1,2-Dichloroethene
Concen: 0.260 ug/l
RT: 3.087 min Scan# 328
Delta R.T. -0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 96 Resp: 491

Ion	Ratio	Lower	Upper
96	100		
61	152.6	105.6	158.4
98	49.8	50.1	75.1#

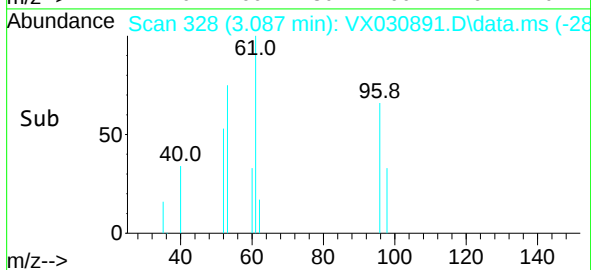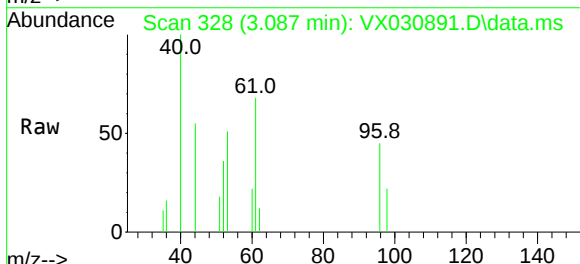

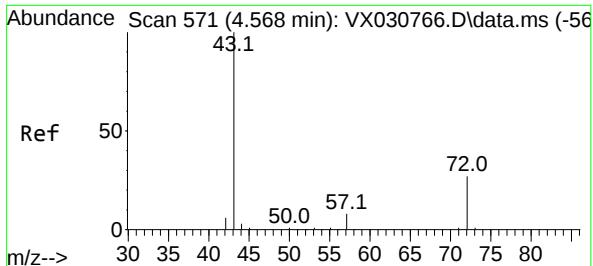

#25

2-Butanone

Concen: 0.411 ug/l

RT: 4.611 min Scan# 51

Delta R.T. 0.043 min

Lab File: VX030891.D

Acq: 27 Aug 2022 23:43

Instrument :

MSVOA_X

ClientSampleId :





VX0827WBL02

Tgt Ion: 43 Resp: 698

Ion Ratio Lower Upper

43 100

72 0.0 21.7 32.5#

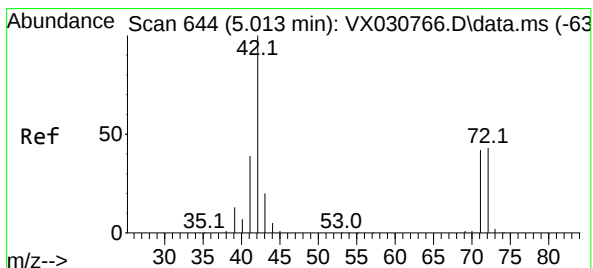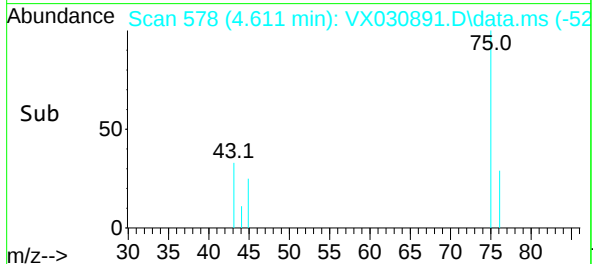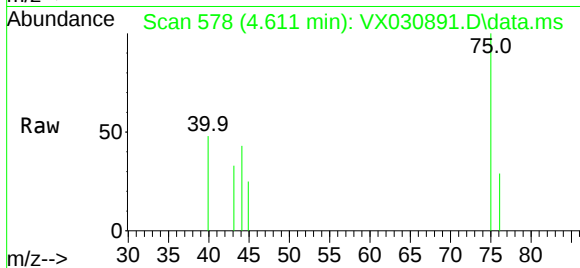

#29

Tetrahydrofuran

Concen: 0.353 ug/l

RT: 5.056 min Scan# 651

Delta R.T. 0.043 min

Lab File: VX030891.D

Acq: 27 Aug 2022 23:43




Tgt Ion: 42 Resp: 392


Ion Ratio Lower Upper

42 100

72 0.0 36.5 54.7#

71 0.0 33.9 50.9#

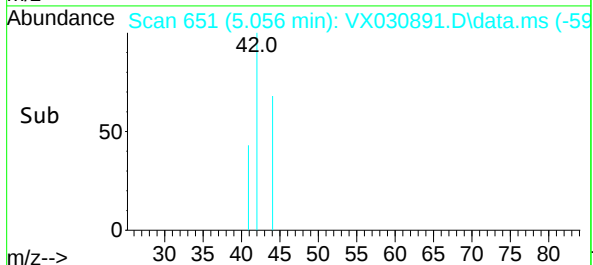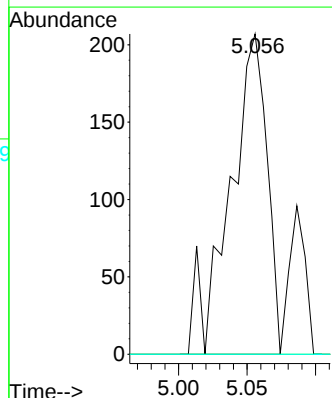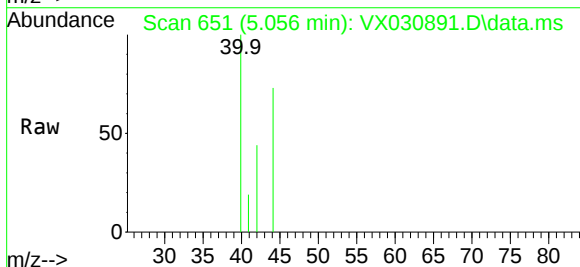



#33

1,2-Dichloroethane-d4

Concen: 58.891 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX030891.D

Acq: 27 Aug 2022 23:43

Instrument :

MSVOA_X

ClientSampleId :





VX0827WBL02

Tgt Ion: 65 Resp: 134465

Ion Ratio Lower Upper

65 100

67 52.3 0.0 109.6

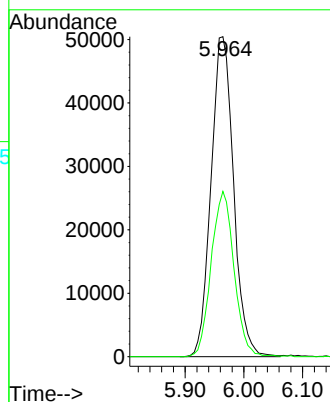

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.000 min

Lab File: VX030891.D

Acq: 27 Aug 2022 23:43




Tgt Ion: 114 Resp: 327563


Ion Ratio Lower Upper

114 100

63 21.5 0.0 38.4

88 15.5 0.0 31.8


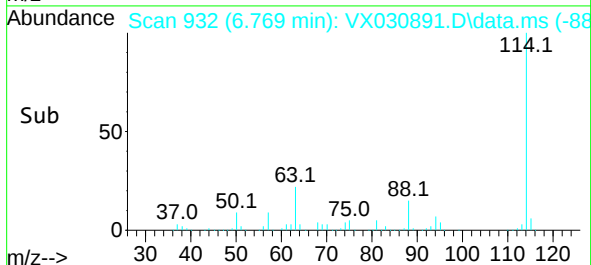
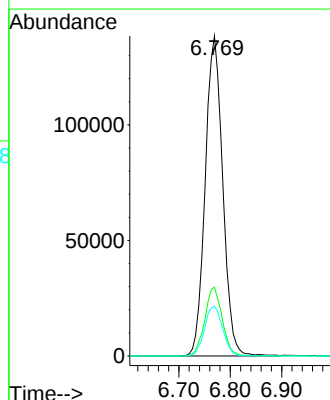
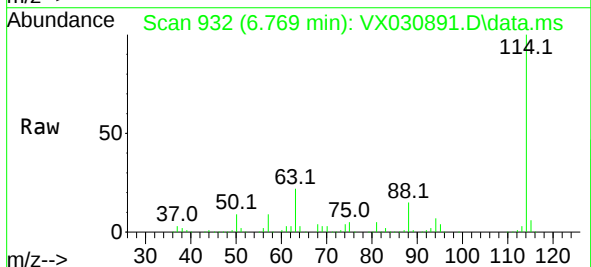


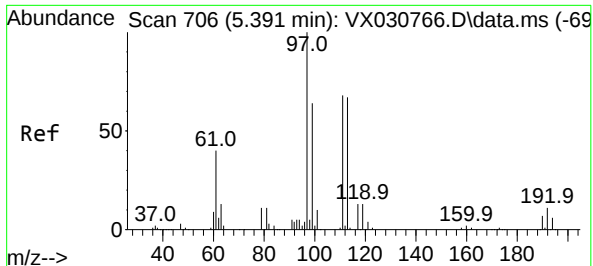

#35
Dibromofluoromethane
Concen: 52.387 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion:113 Resp: 105462
Ion Ratio Lower Upper
113 100
111 103.5 83.2 124.8
192 18.2 14.8 22.2

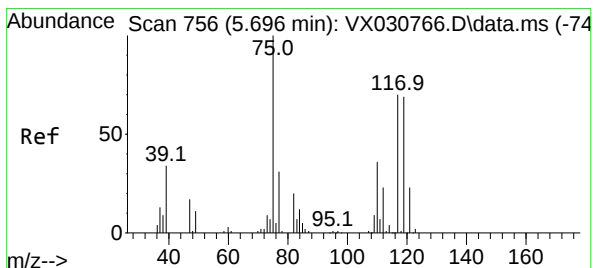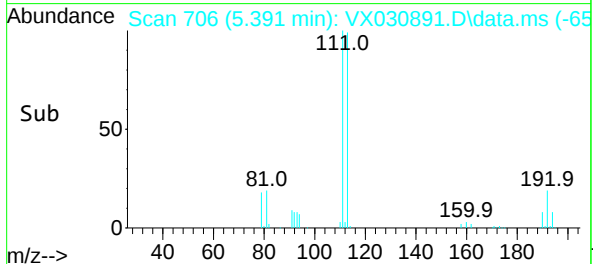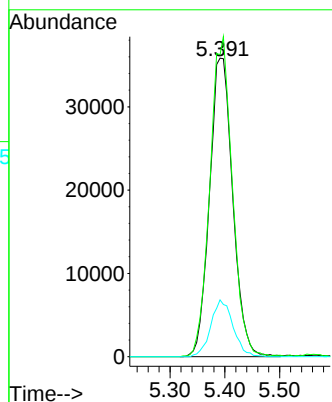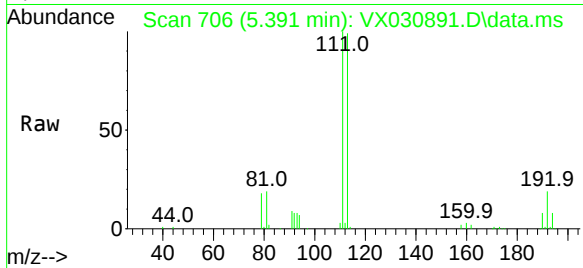

#36
1,1-Dichloropropene
Concen: 0.207 ug/l
RT: 5.696 min Scan# 756
Delta R.T. -0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43


Tgt Ion: 75 Resp: 568
Ion Ratio Lower Upper
75 100
110 19.2 19.3 57.9#
77 0.0 24.4 36.6#

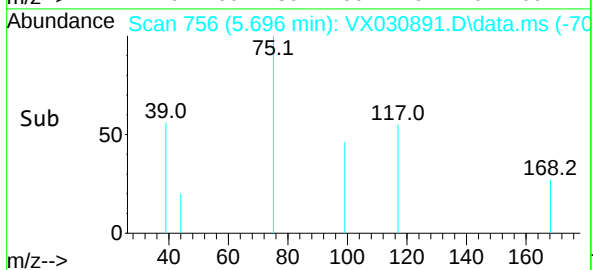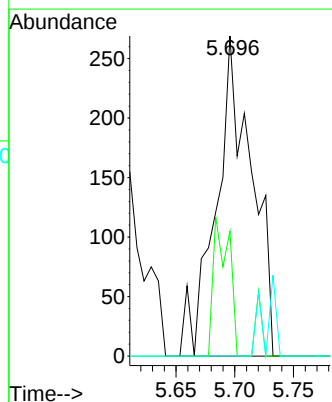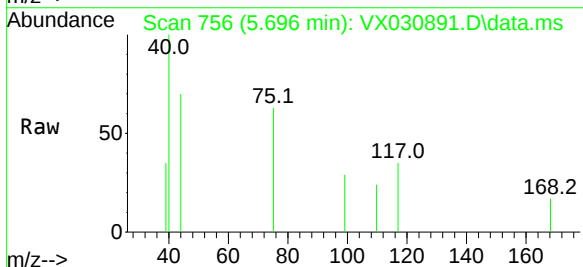



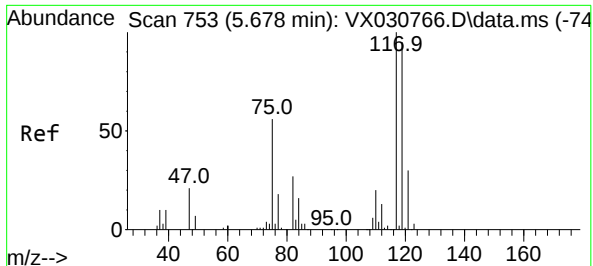


#38
Carbon Tetrachloride
Concen: 7.070 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02



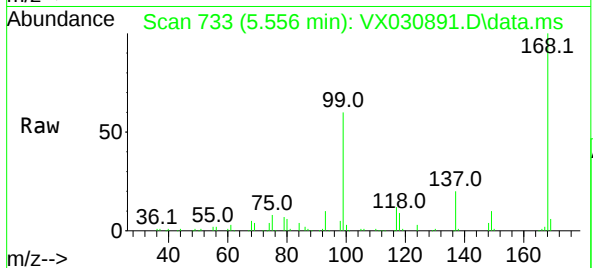



Tgt Ion:117 Resp: 20443
Ion Ratio Lower Upper
117 100
119 5.3 74.1 111.1#
121 0.0 25.8 38.8#

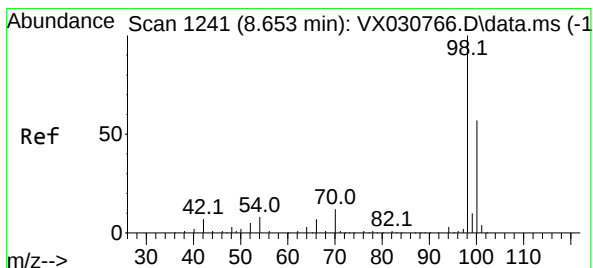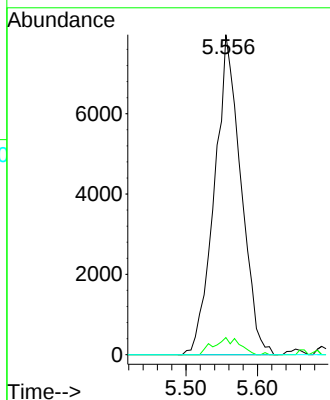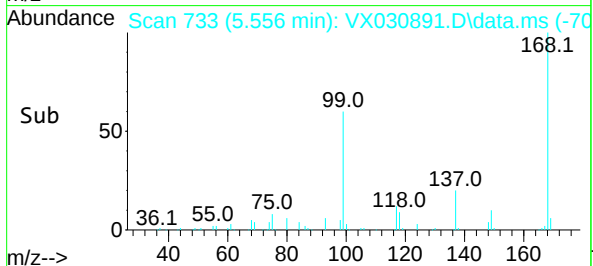

#50
Toluene-d8
Concen: 56.251 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 98 Resp: 394609
Ion Ratio Lower Upper
98 100
100 63.4 52.3 78.5


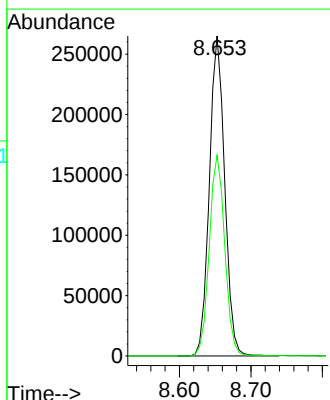
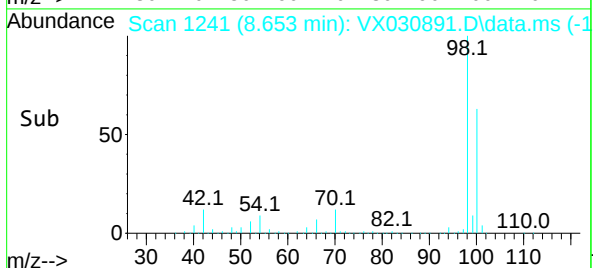
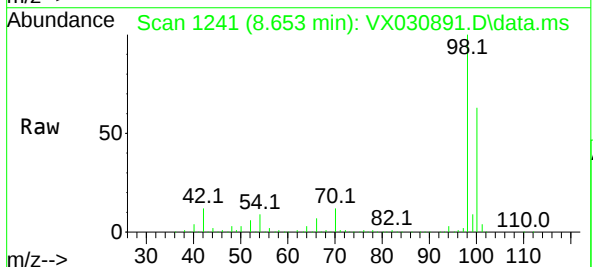




#62
4-Bromofluorobenzene
Concen: 47.520 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion: 95 Resp: 124111
Ion Ratio Lower Upper
95 100
174 76.9 0.0 149.0
176 73.5 0.0 146.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 117 Resp: 288366
Ion Ratio Lower Upper
117 100
82 58.1 42.7 64.1
119 32.2 25.4 38.2


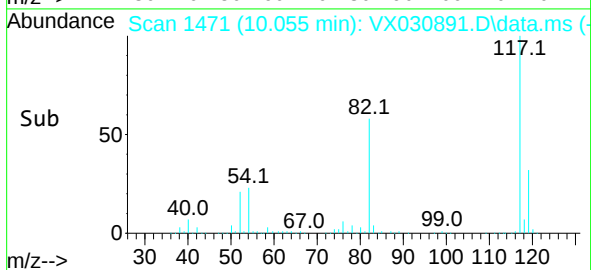






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX030891.D
 Acq: 27 Aug 2022 23:43




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0827WBL02


Tgt Ion:152 Resp: 113467
 Ion Ratio Lower Upper
 152 100
 115 63.0 40.5 121.5
 150 158.7 0.0 347.0

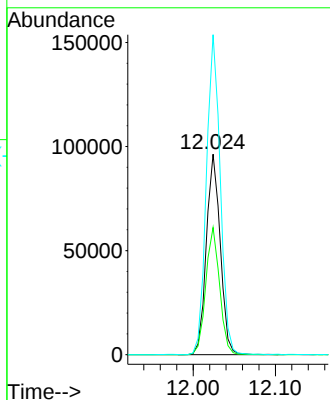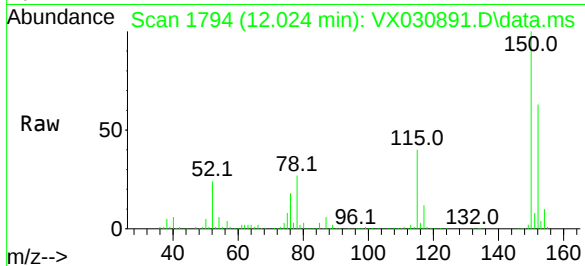

#76
 1,2,3-Trichloropropane
 Concen: 26.288 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX030891.D
 Acq: 27 Aug 2022 23:43

Tgt Ion: 75 Resp: 65349
 Ion Ratio Lower Upper
 75 100
 77 1.2 19.8 59.3#


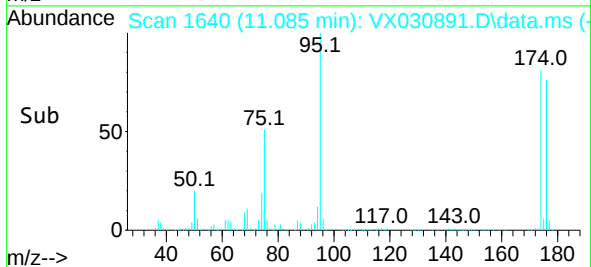
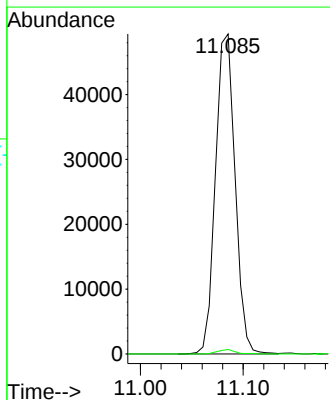
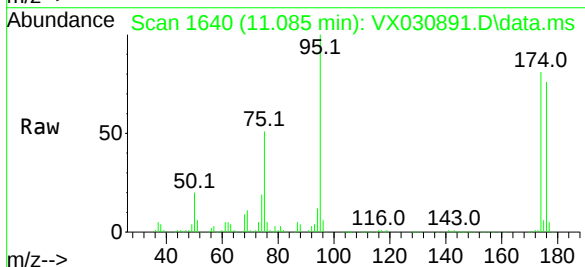




#77
Bromobenzene
Concen: 0.216 ug/l
RT: 11.207 min Scan# 1660
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion:156 Resp: 404
Ion Ratio Lower Upper
156 100
77 129.5 82.7 247.9
158 91.3 47.5 142.5

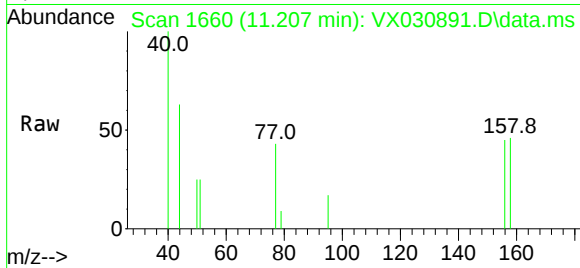

#78
n-propylbenzene
Concen: 0.214 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 91 Resp: 1874
Ion Ratio Lower Upper
91 100
120 19.9 11.6 34.8


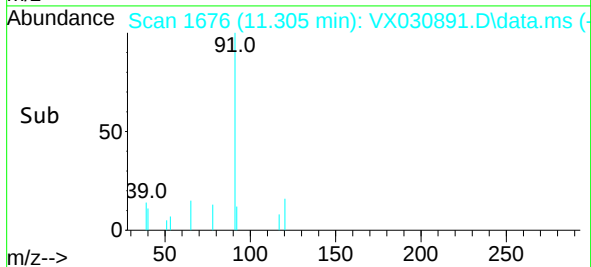

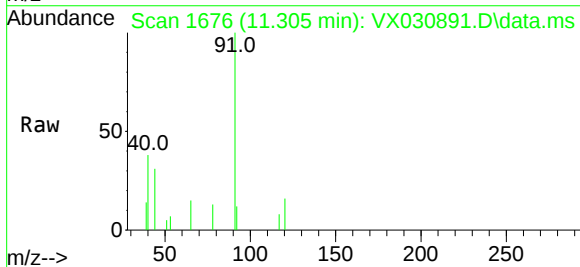




#79
2-Chlorotoluene
Concen: 0.215 ug/l
RT: 11.372 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion: 91 Resp: 1151
Ion Ratio Lower Upper
91 100
126 33.3 17.4 52.3

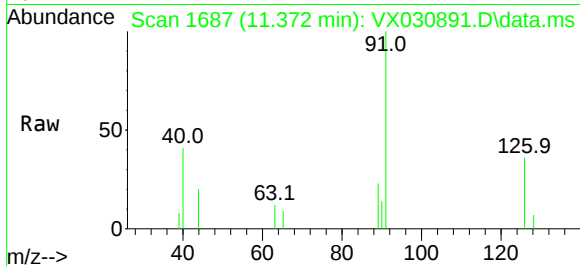

#81
trans-1,4-Dichloro-2-butene
Concen: 84.816 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.067 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 75 Resp: 65349
Ion Ratio Lower Upper
75 100
53 0.1 74.2 111.4#
89 0.0 34.8 52.2#


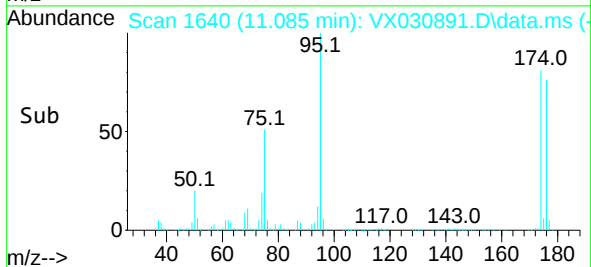

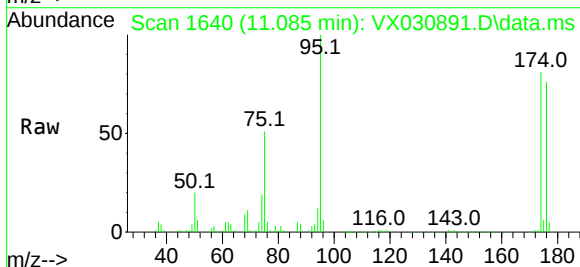




#82
4-Chlorotoluene
Concen: 0.266 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion: 91 Resp: 1599
Ion Ratio Lower Upper
91 100
126 24.0 15.3 45.9

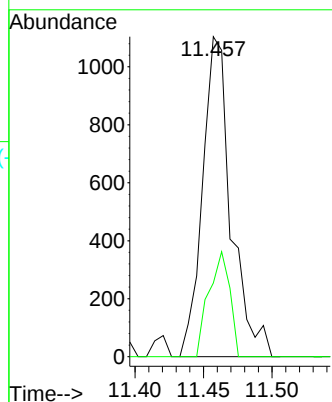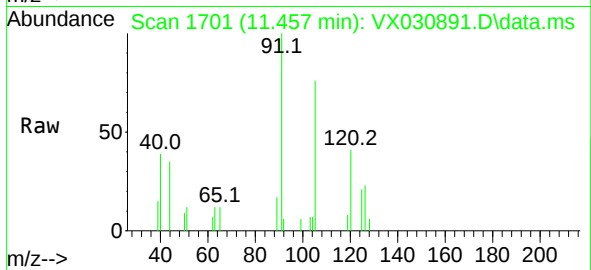

#86
p-Isopropyltoluene
Concen: 0.239 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion: 119 Resp: 1571
Ion Ratio Lower Upper
119 100
134 27.5 13.9 41.6
91 44.4 11.8 35.3#

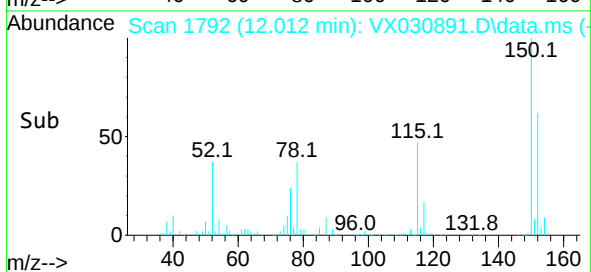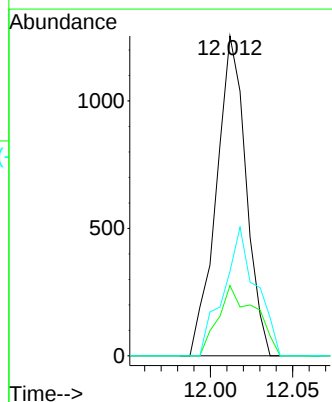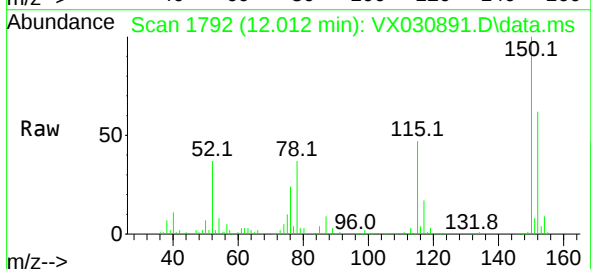



#87

1,3-Dichlorobenzene

Concen: 0.341 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. 0.006 min

Lab File: VX030891.D

Acq: 27 Aug 2022 23:43

Instrument :

MSVOA_X

ClientSampleId :

VX0827WBL02





Tgt Ion:146 Resp: 1205

Ion Ratio Lower Upper

146 100

111 34.9 20.3 60.8

148 58.7 31.8 95.3

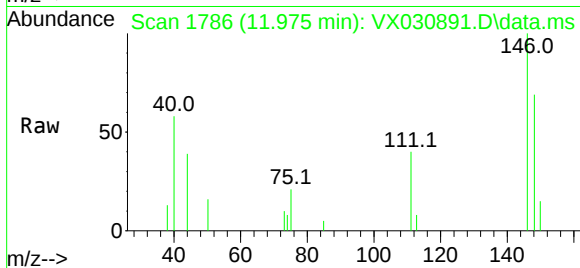

#88

1,4-Dichlorobenzene

Concen: 0.332 ug/l

RT: 11.975 min Scan# 1786

Delta R.T. -0.068 min

Lab File: VX030891.D

Acq: 27 Aug 2022 23:43




Tgt Ion:146 Resp: 1205


Ion Ratio Lower Upper

146 100

111 34.9 20.3 60.9

148 58.7 32.3 96.8


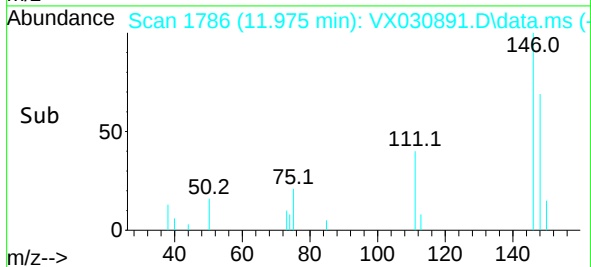

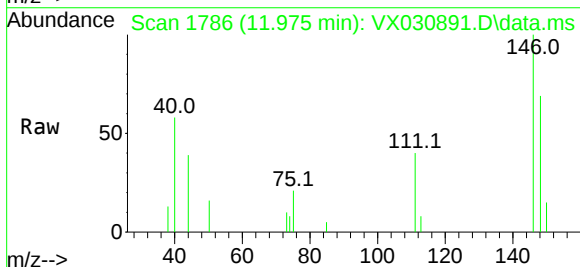


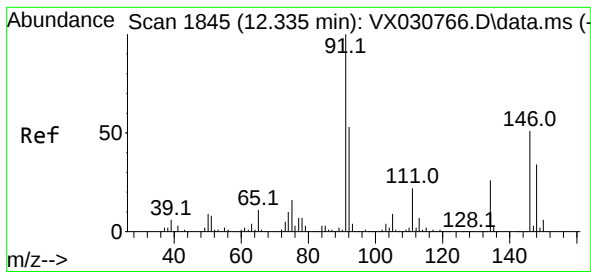

#89
n-Butylbenzene
Concen: 0.281 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion: 91	Resp:	1708	
Ion	Ratio	Lower	Upper
91	100		
92	60.9	26.2	78.5
134	30.3	12.6	37.8

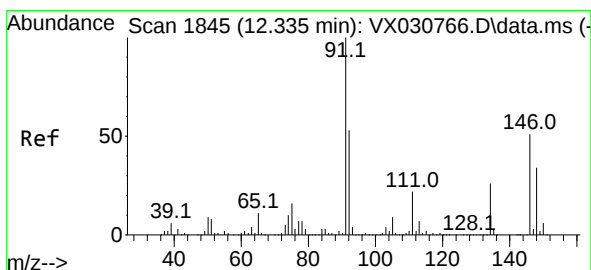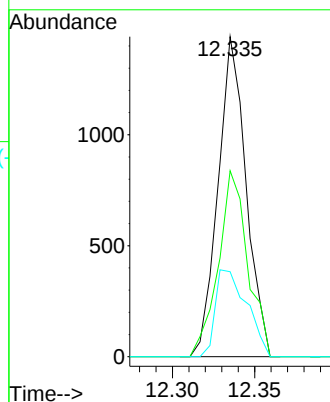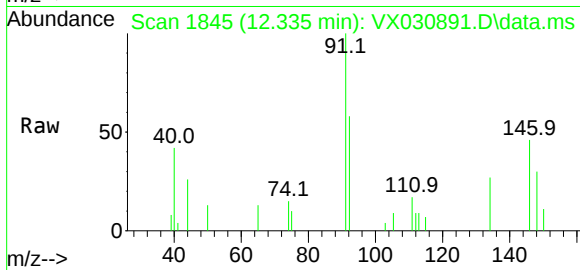

#91
1,2-Dichlorobenzene
Concen: 0.252 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion:146	Resp:	939	
Ion	Ratio	Lower	Upper
146	100		
111	51.1	20.7	62.1
148	60.7	32.0	96.2


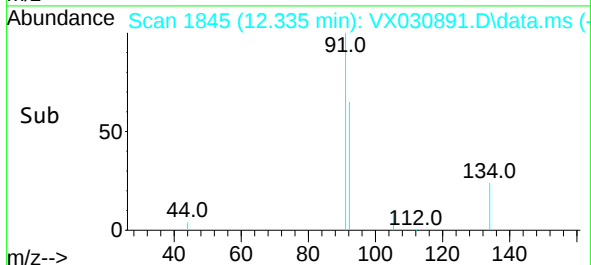
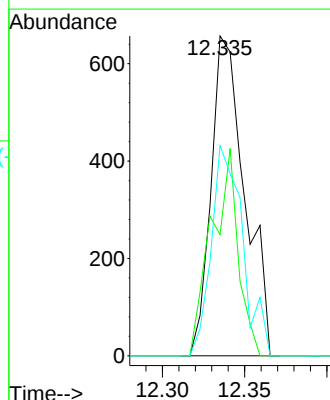
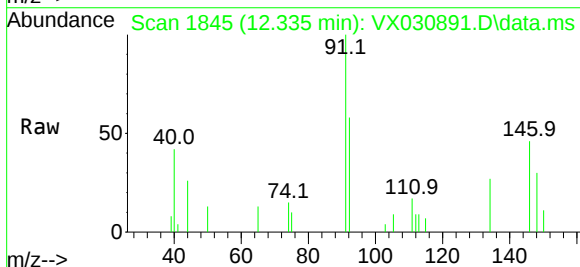




#93
1,2,4-Trichlorobenzene
Concen: 0.548 ug/l
RT: 13.597 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02


Tgt Ion:180 Resp: 1274
Ion Ratio Lower Upper
180 100
182 86.3 48.2 144.6
145 37.2 15.9 47.6

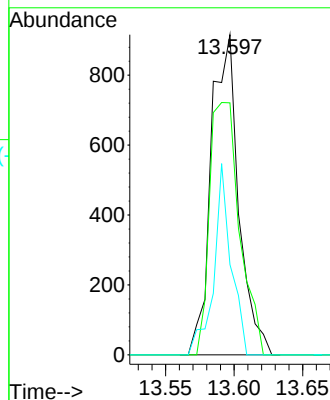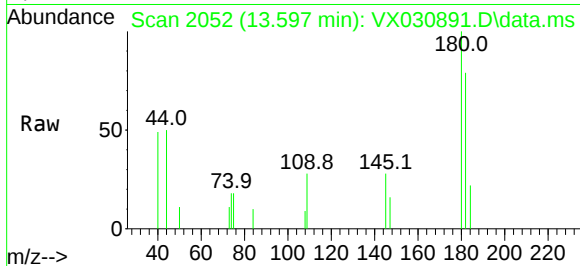

#94
Hexachlorobutadiene
Concen: 0.406 ug/l
RT: 13.731 min Scan# 2074
Delta R.T. 0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion:225 Resp: 393
Ion Ratio Lower Upper
225 100
223 78.6 30.6 91.6
227 74.8 31.9 95.9


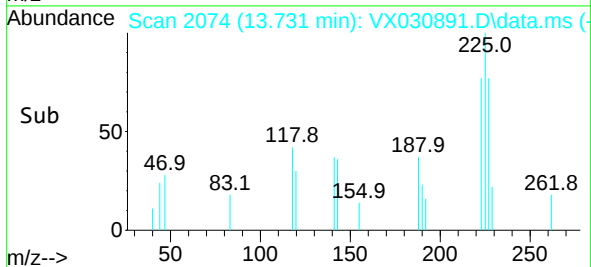
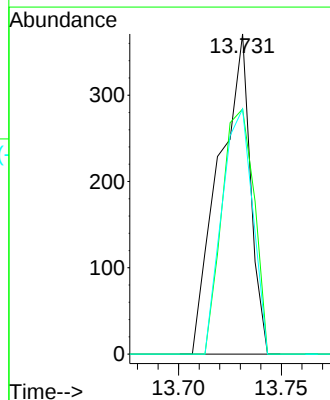
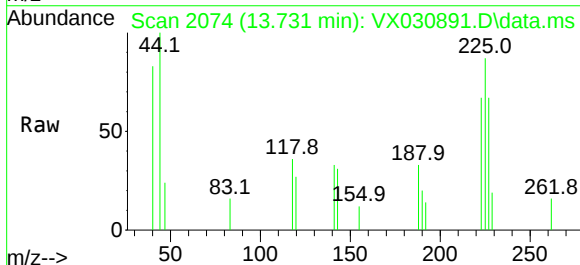




#95
Naphthalene
Concen: 0.428 ug/l
RT: 13.774 min Scan# 2082
Delta R.T. -0.006 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL02

Tgt Ion:128	Resp:	3470
Ion Ratio	Lower	Upper
128	100	
127	11.1	10.2 15.2
129	10.8	8.6 13.0

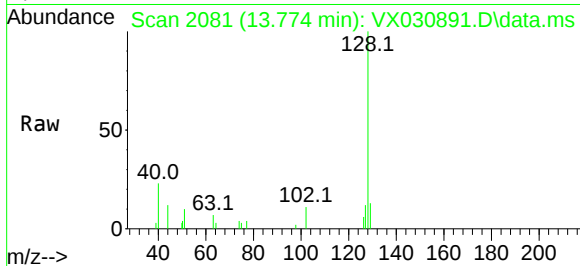

#96
1,2,3-Trichlorobenzene
Concen: 0.476 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX030891.D
Acq: 27 Aug 2022 23:43

Tgt Ion:180	Resp:	1171
Ion Ratio	Lower	Upper
180	100	
182	93.1	47.0 141.0
145	34.8	17.0 50.9

