

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
 Data File : VX030896.D
 Acq On : 28 Aug 2022 02:27
 Operator : JC/MD
 Sample : N4360-1
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT180D2-20220823

Quant Time: Aug 29 01:15:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	190877	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	332709	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	293936	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	125753	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	137523	61.251	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 122.500%	
35) Dibromofluoromethane	5.391	113	105648	51.667	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.340%	
50) Toluene-d8	8.653	98	398144	55.877	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 111.760%	
62) 4-Bromofluorobenzene	11.085	95	133553	50.345	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 100.680%	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.167	85	962	0.544	ug/l	91
3) Chloromethane	1.295	50	413	Below Cal	#	74
4) Vinyl Chloride	1.374	62	175	Below Cal	#	1
5) Bromomethane	1.612	94	215	0.242	ug/l #	62
6) Chloroethane	1.679	64	216	Below Cal	#	41
7) Trichlorofluoromethane	1.886	101	1550	0.530	ug/l	86
9) 1,1,2-Trichlorotrifluo...	2.331	101	69853	37.579	ug/l	97
10) Methyl Iodide	2.453	142	280	4.195	ug/l #	72
12) 1,1-Dichloroethene	2.319	96	39809	23.008	ug/l #	83
16) Acetone	2.386	43	1310	1.263	ug/l #	73
17) Carbon Disulfide	2.520	76	470	Below Cal	#	74
20) Methylene Chloride	2.788	84	314	Below Cal	#	70
24) 1,1-Dichloroethane	3.617	63	8120	2.228	ug/l	98
27) cis-1,2-Dichloroethene	4.501	96	7591	3.306	ug/l	96
30) Chloroform	5.099	83	3498	0.912	ug/l	96
31) Cyclohexane	5.550	56	4627	1.612	ug/l #	1
32) 1,1,1-Trichloroethane	5.391	97	6600	2.128	ug/l	97
36) 1,1-Dichloropropene	5.556	75	16111	5.786	ug/l #	49
38) Carbon Tetrachloride	5.684	117	6579	2.240	ug/l #	94
39) Methylcyclohexane	7.129	83	11501	3.451	ug/l #	1
42) 1,2-Dichloroethane	6.099	62	1572	0.532	ug/l	76
44) Trichloroethene	7.129	130	884106	367.344	ug/l	93
49) 1,4-Dioxane	7.690	88	1306	21.364	ug/l #	76
51) 4-Methyl-2-Pentanone	8.647	43	1790	0.534	ug/l #	1
55) 1,1,2-Trichloroethane	9.159	97	2179	0.943	ug/l	96
60) Dibromochloromethane	9.275	129	697	0.289	ug/l #	11
64) Tetrachloroethene	9.275	164	658	0.284	ug/l #	86
76) 1,2,3-Trichloropropane	11.085	75	69965	25.395	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.085	75	69965	81.935	ug/l #	13

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
Data File : VX030896.D
Acq On : 28 Aug 2022 02:27
Operator : JC/MD
Sample : N4360-1
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823

Quant Time: Aug 29 01:15:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 26 02:03:28 2022
Response via : Initial Calibration




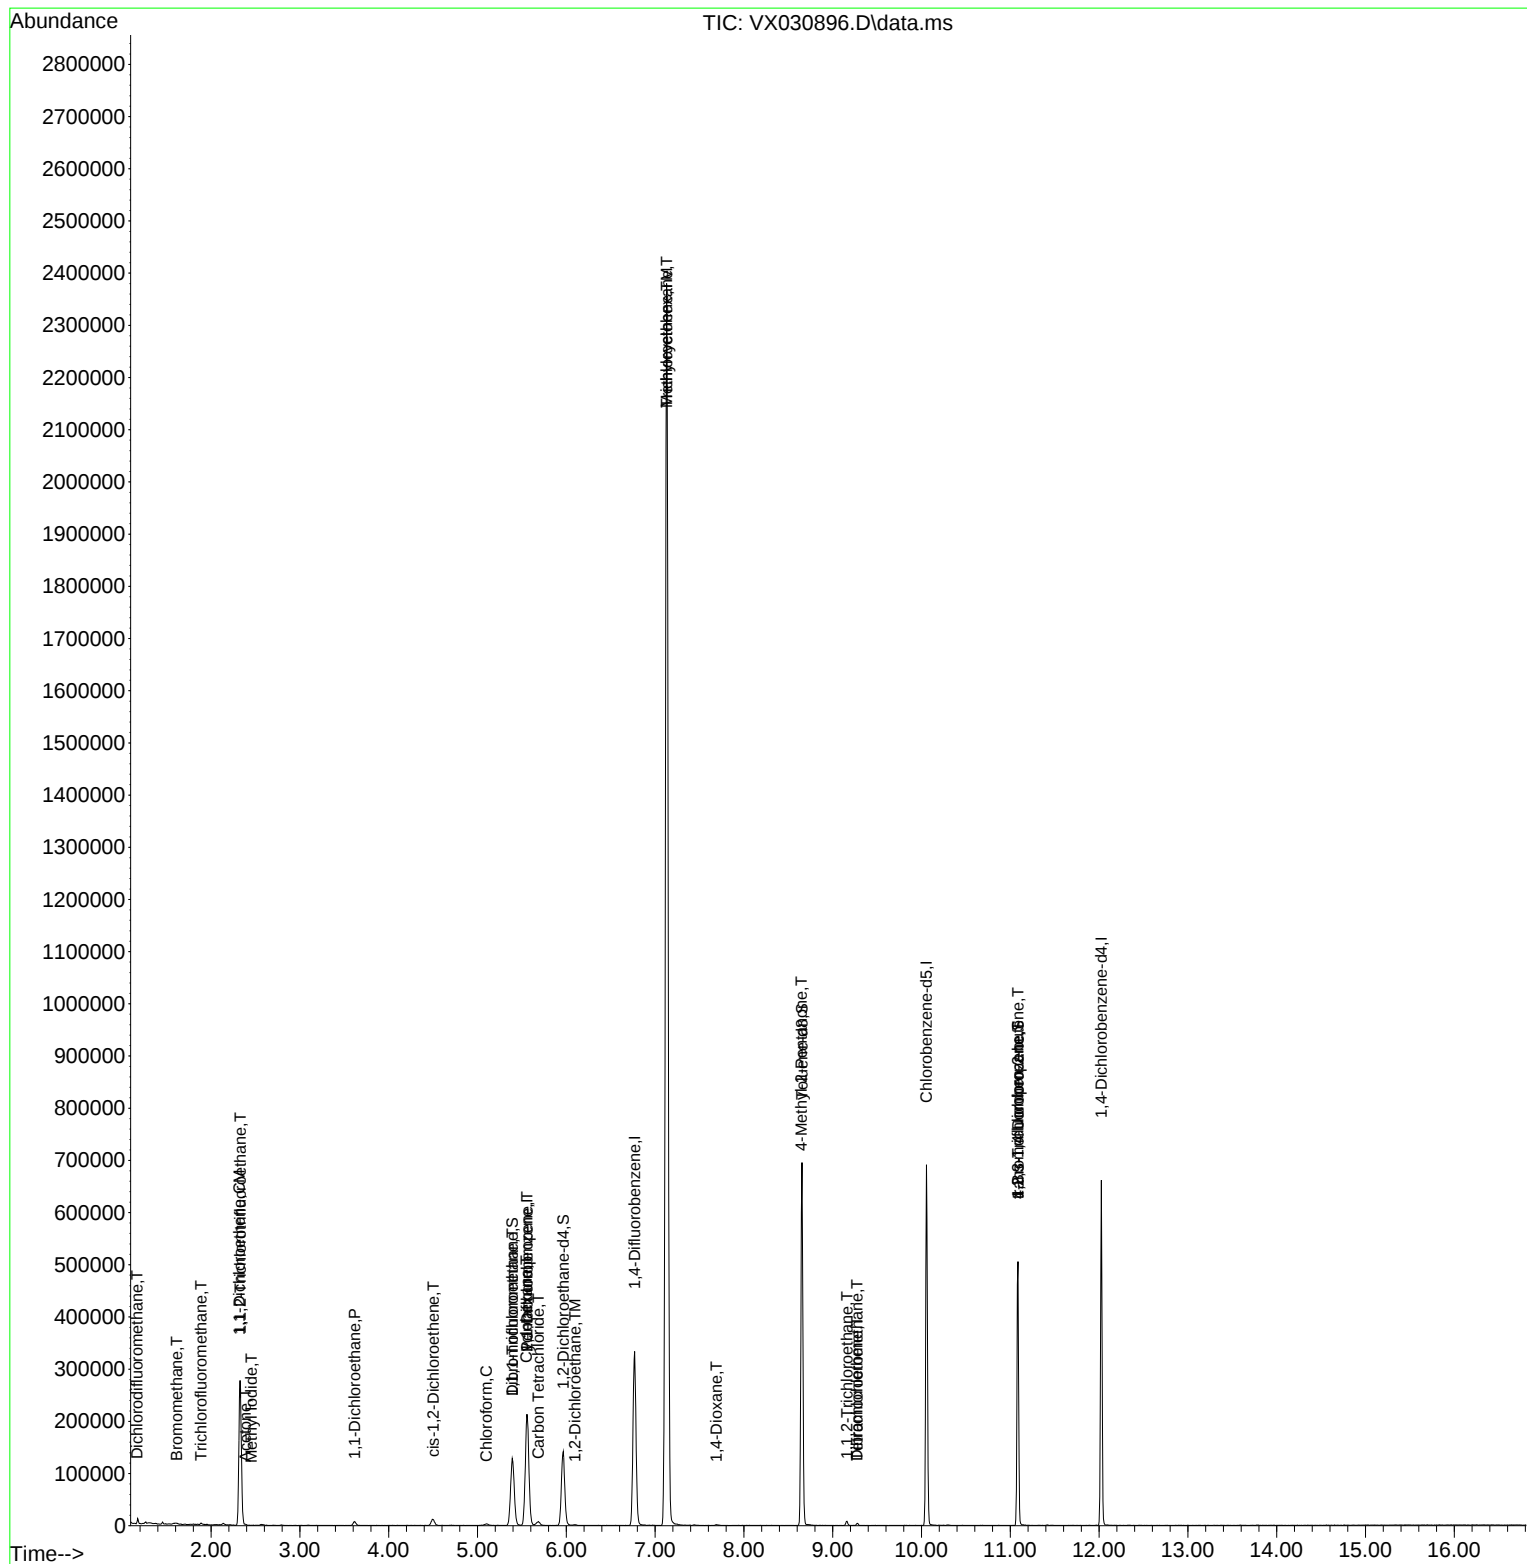




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27




Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823


Tgt Ion:168 Resp: 190877
Ion Ratio Lower Upper
168 100
99 61.0 44.0 66.0

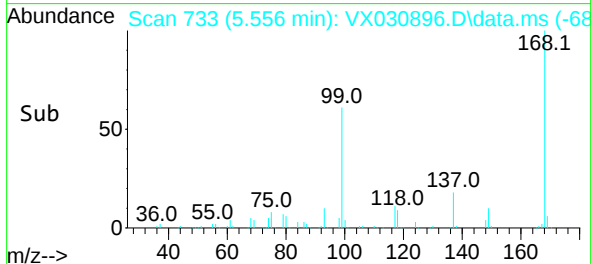

#2
Dichlorodifluoromethane
Concen: 0.544 ug/l
RT: 1.167 min Scan# 13
Delta R.T. -0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Tgt Ion: 85 Resp: 962
Ion Ratio Lower Upper
85 100
87 38.2 16.5 49.5


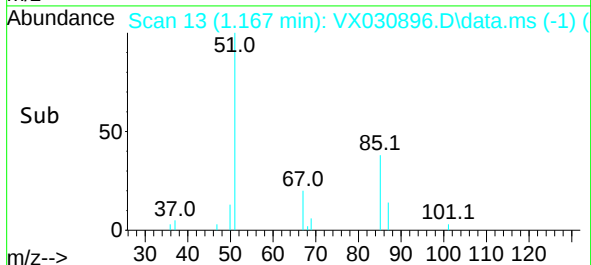

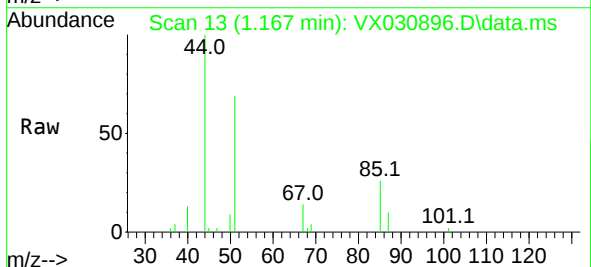


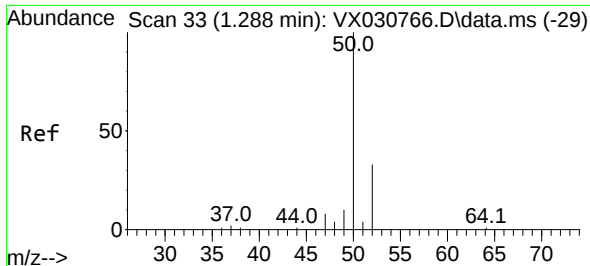

#3
Chloromethane
Concen: Below Cal
RT: 1.295 min Scan# 34
Delta R.T. 0.007 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27




Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823


Tgt Ion: 50 Resp: 413
Ion Ratio Lower Upper
50 100
52 18.0 26.3 39.5#

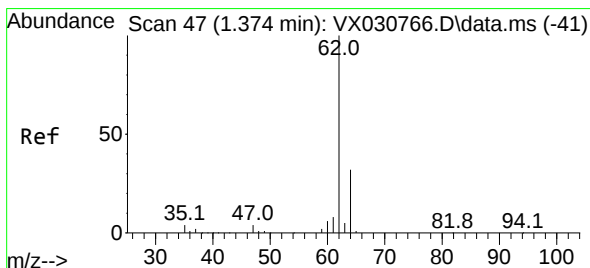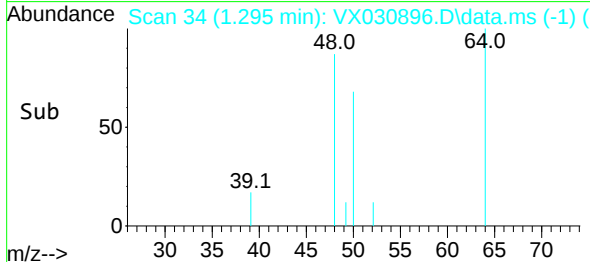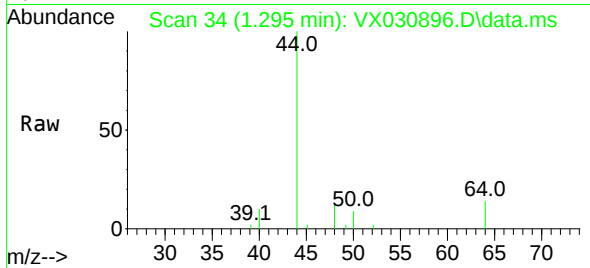

#4
Vinyl Chloride
Concen: Below Cal
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Tgt Ion: 62 Resp: 175
Ion Ratio Lower Upper
62 100
64 106.3 25.2 37.8#


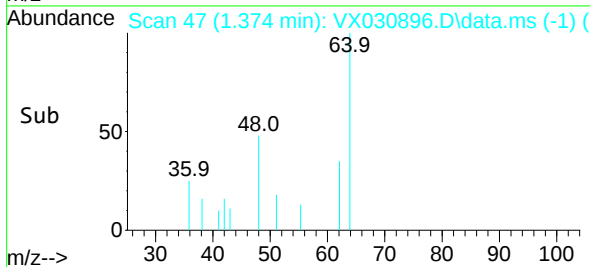

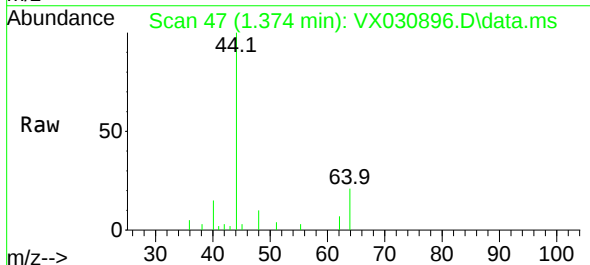


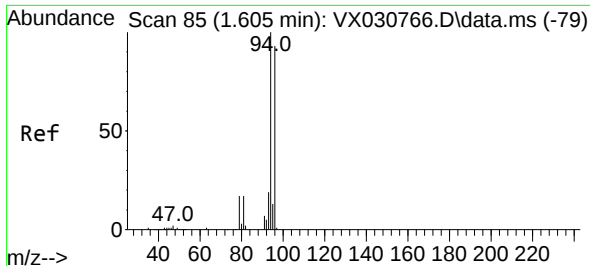

#5
Bromomethane
Concen: 0.242 ug/l
RT: 1.612 min Scan# 80
Delta R.T. 0.006 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27




Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823


Tgt Ion: 94 Resp: 215
Ion Ratio Lower Upper
94 100
96 59.3 76.9 115.3#

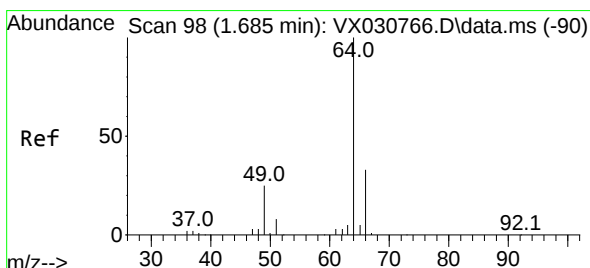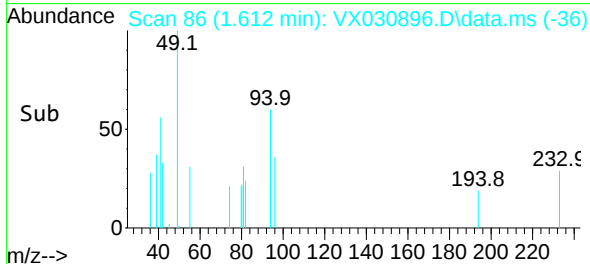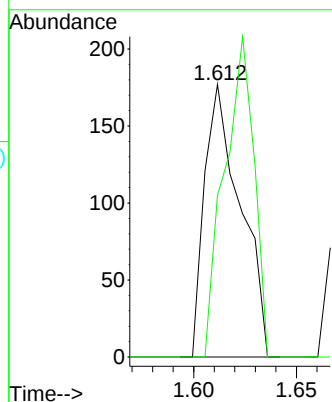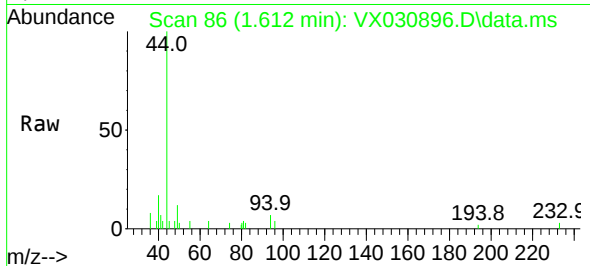

#6
Chloroethane
Concen: Below Cal
RT: 1.679 min Scan# 97
Delta R.T. -0.006 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Tgt Ion: 64 Resp: 216
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#


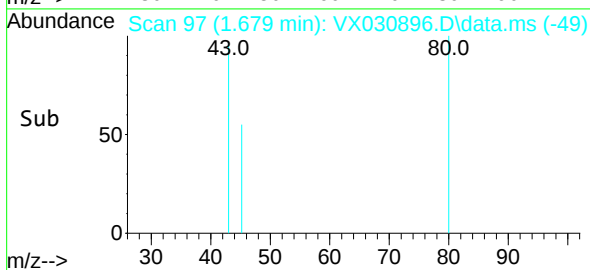
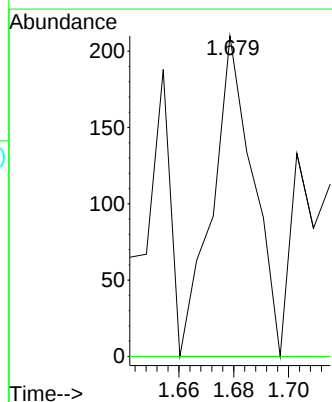
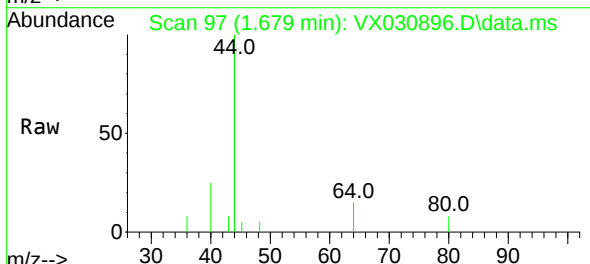




#7
 Trichlorofluoromethane
 Concen: 0.530 ug/l
 RT: 1.886 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX030896.D
 Acq: 28 Aug 2022 02:27




Instrument :
 MSVOA_X
 ClientSampleId :
 TT180D2-20220823


Tgt Ion:101 Resp: 1550
 Ion Ratio Lower Upper
 101 100
 103 51.0 49.7 74.5

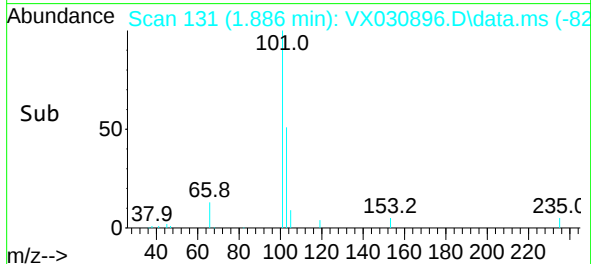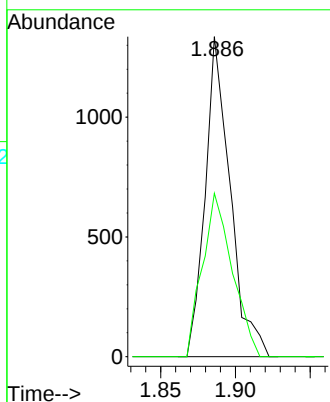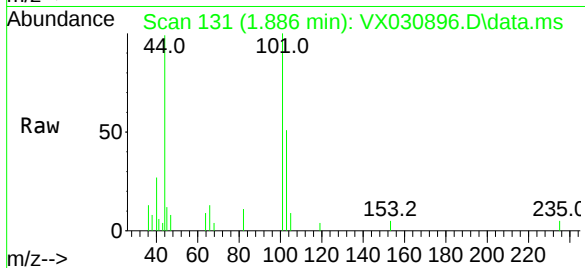

#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 37.579 ug/l
 RT: 2.331 min Scan# 204
 Delta R.T. 0.006 min
 Lab File: VX030896.D
 Acq: 28 Aug 2022 02:27

Tgt Ion:101 Resp: 69853
 Ion Ratio Lower Upper
 101 100
 85 46.4 34.0 51.0
 151 75.8 59.4 89.0


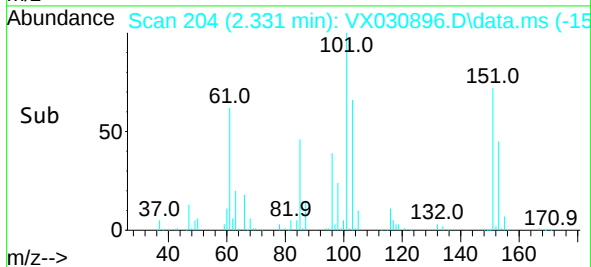
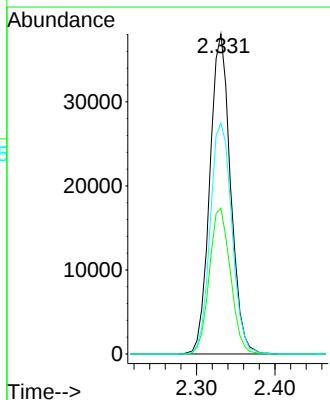
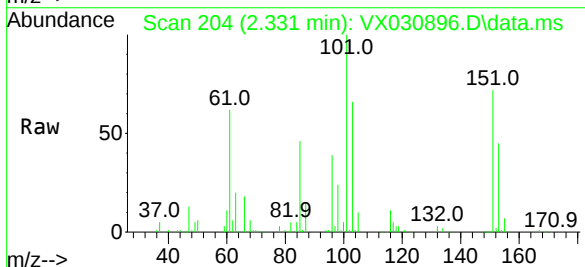




#10
Methyl Iodide
Concen: 4.195 ug/l
RT: 2.453 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27




Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823


Tgt Ion:142 Resp: 280
Ion Ratio Lower Upper
142 100
127 56.4 30.2 45.2#
141 6.8 11.3 16.9#

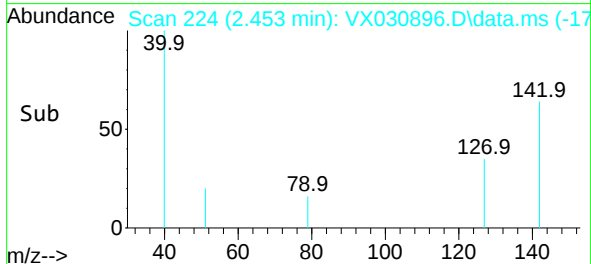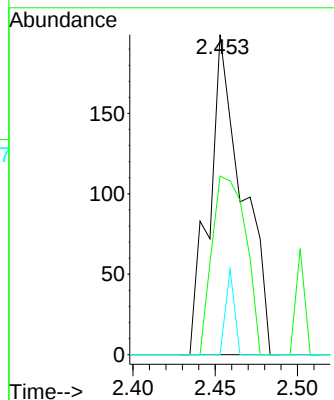

#12
1,1-Dichloroethene
Concen: 23.008 ug/l
RT: 2.319 min Scan# 202
Delta R.T. 0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Tgt Ion: 96 Resp: 39809
Ion Ratio Lower Upper
96 100
61 176.6 117.4 176.0#
98 66.6 52.2 78.4


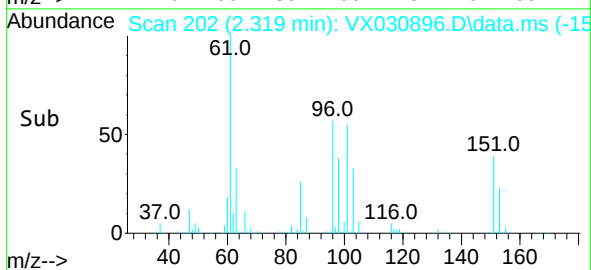
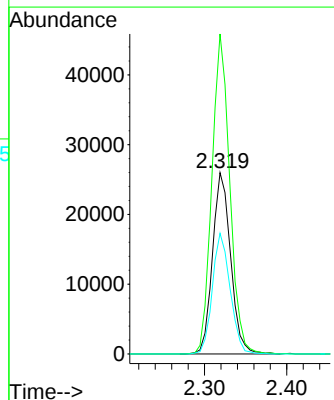
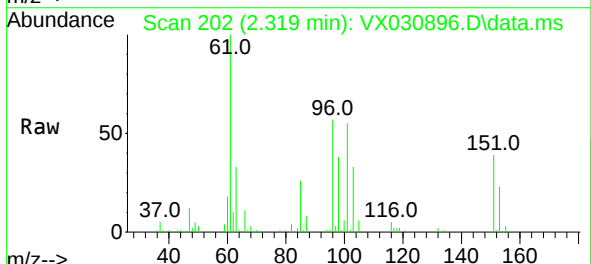


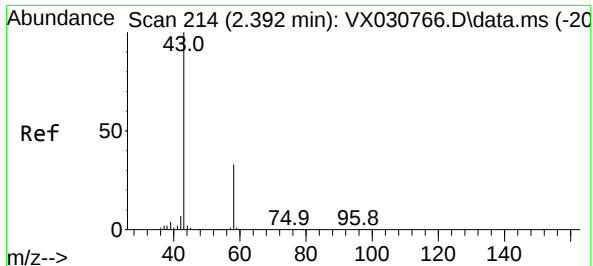

#16
Acetone
Concen: 1.263 ug/l
RT: 2.386 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27




Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823


Tgt Ion: 43 Resp: 1310
Ion Ratio Lower Upper
43 100
58 19.0 27.7 41.5#

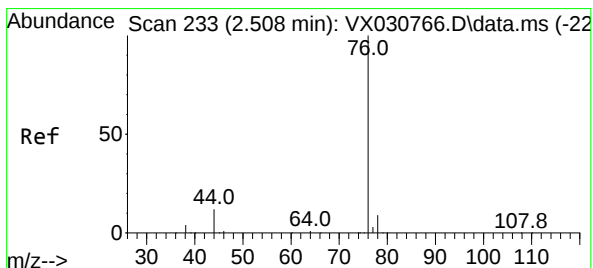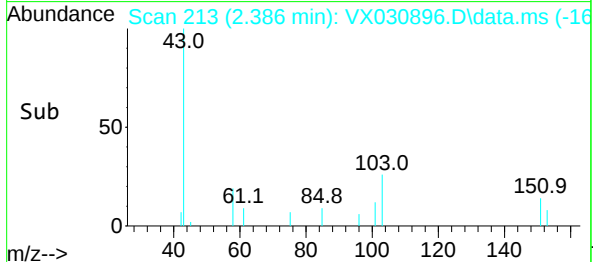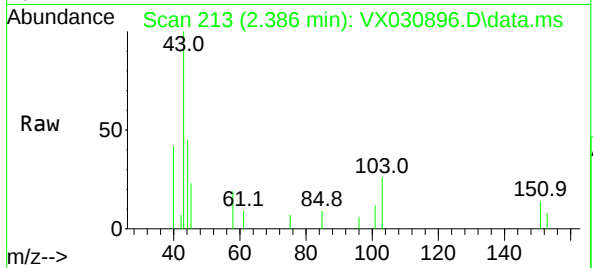

#17
Carbon Disulfide
Concen: Below Cal
RT: 2.520 min Scan# 235
Delta R.T. 0.012 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27


Tgt Ion: 76 Resp: 470
Ion Ratio Lower Upper
76 100
78 0.0 7.8 11.6#

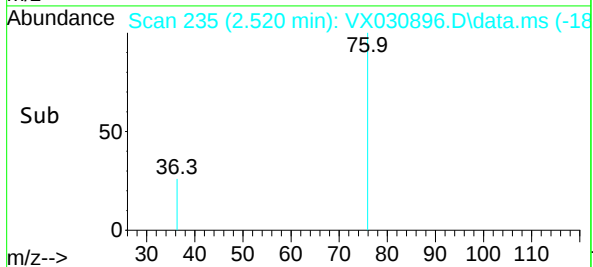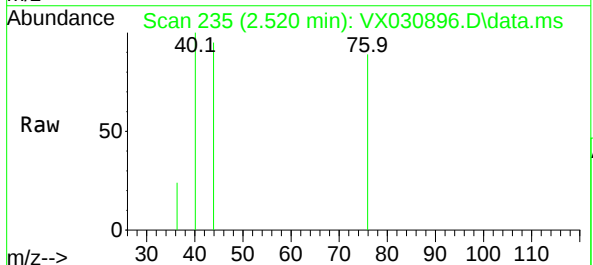






#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27


Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823

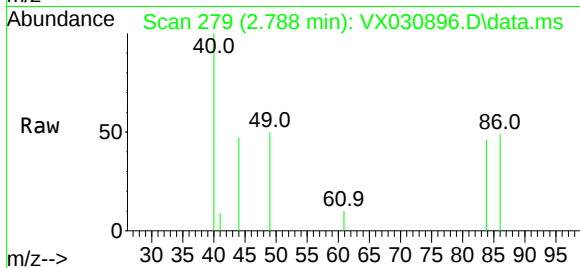



Tgt Ion:	84	Resp:	314
Ion	Ratio	Lower	Upper
84	100		
49	110.7	93.8	140.6
51	0.0	29.4	44.0#
86	108.4	51.0	76.4#




#24
1,1-Dichloroethane
Concen: 2.228 ug/l
RT: 3.617 min Scan# 415
Delta R.T. 0.006 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

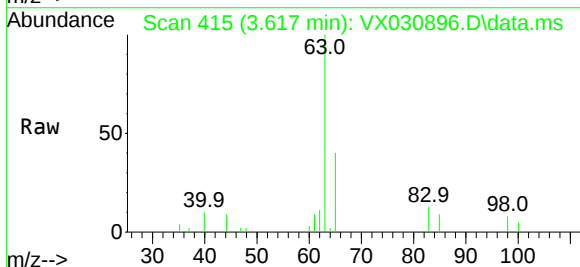

Tgt Ion:	63	Resp:	8120
Ion	Ratio	Lower	Upper
63	100		
98	7.8	3.5	10.5
100	5.4	2.3	6.9





#27

cis-1,2-Dichloroethene

Concen: 3.306 ug/l

RT: 4.501 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27

Instrument :

MSVOA_X

ClientSampleId :

TT180D2-20220823





Tgt Ion: 96 Resp: 7591

Ion Ratio Lower Upper

96 100

61 127.9 0.0 270.0

98 64.5 0.0 127.8

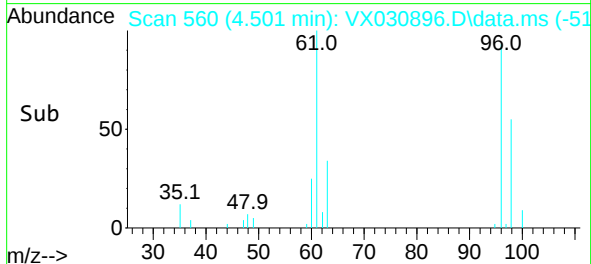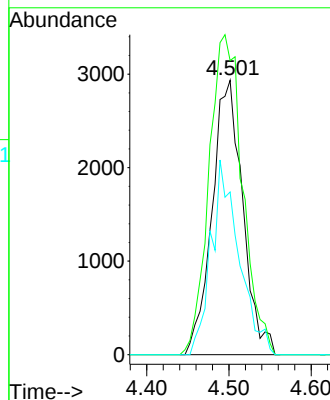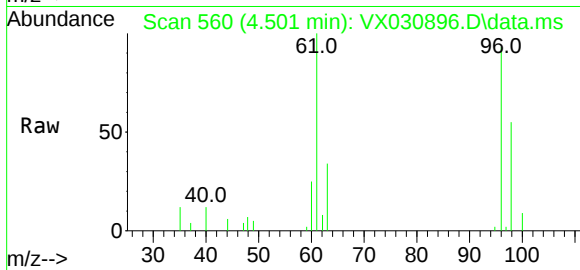

#30

Chloroform

Concen: 0.912 ug/l

RT: 5.099 min Scan# 658

Delta R.T. -0.000 min

Lab File: VX030896.D




Acq: 28 Aug 2022 02:27


Tgt Ion: 83 Resp: 3498

Ion Ratio Lower Upper

83 100


85 67.4 51.5 77.3

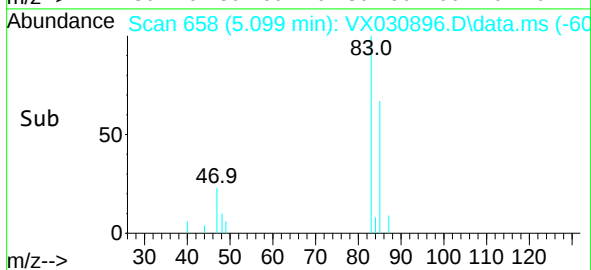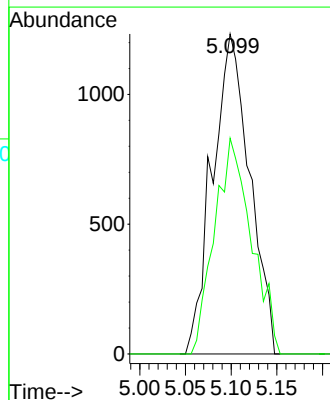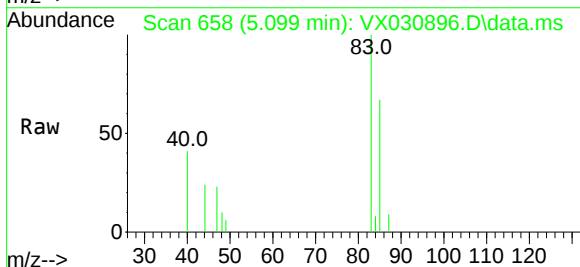



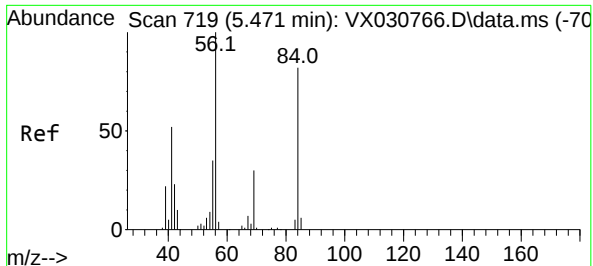


#31
Cyclohexane
Concen: 1.612 ug/l
RT: 5.550 min Scan# 719
Delta R.T. 0.079 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823



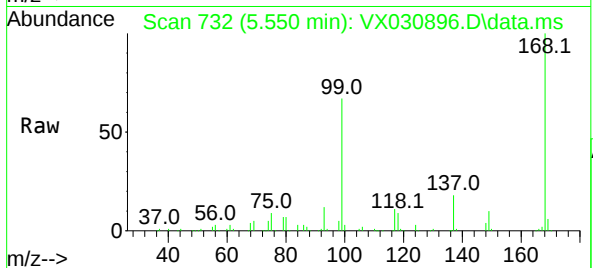



Tgt Ion: 56 Resp: 4627
Ion Ratio Lower Upper
56 100
69 186.6 25.4 38.0#
84 118.1 68.9 103.3#

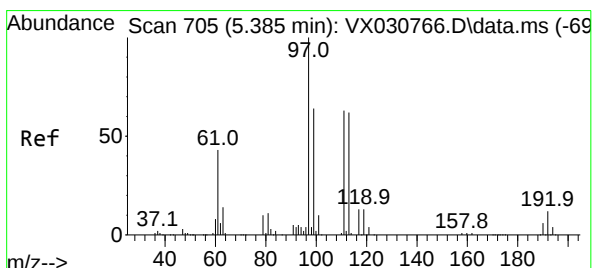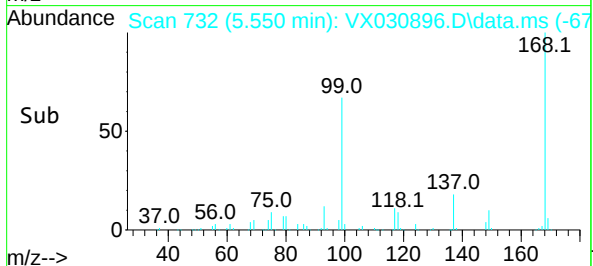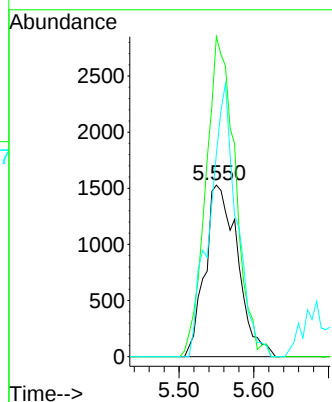

#32
1,1,1-Trichloroethane
Concen: 2.128 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Tgt Ion: 97 Resp: 6600
Ion Ratio Lower Upper
97 100
99 66.2 51.4 77.0
61 47.1 35.8 53.8

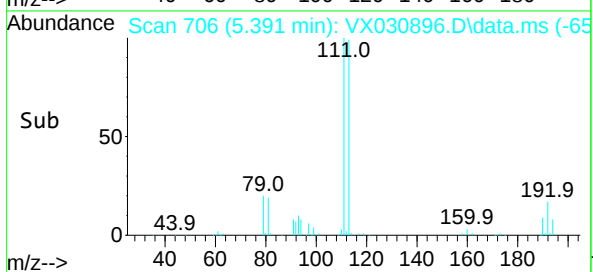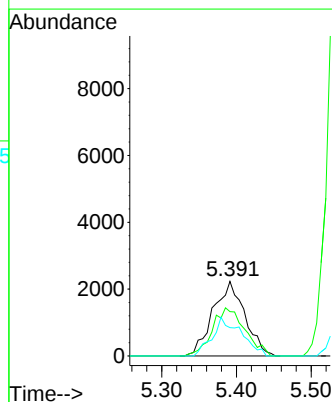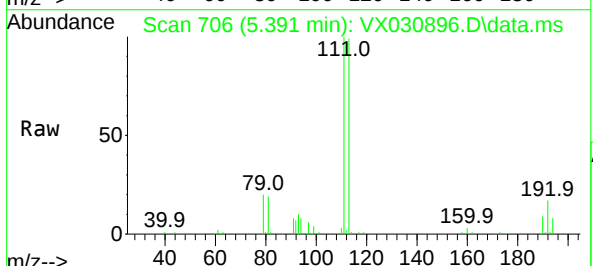



#33

1,2-Dichloroethane-d4

Concen: 61.251 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27

Instrument :

MSVOA_X

ClientSampleId :





TT180D2-20220823

Tgt Ion: 65 Resp: 137523

Ion Ratio Lower Upper

65 100

67 51.7 0.0 109.6

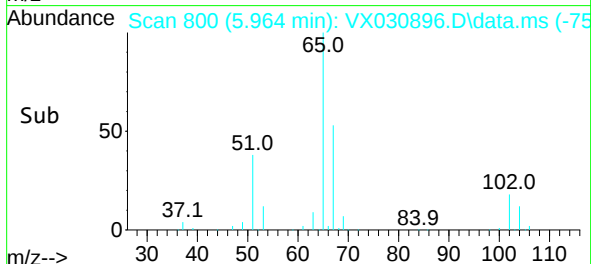

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27




Tgt Ion: 114 Resp: 332709


Ion Ratio Lower Upper

114 100

63 22.4 0.0 38.4

88 16.3 0.0 31.8

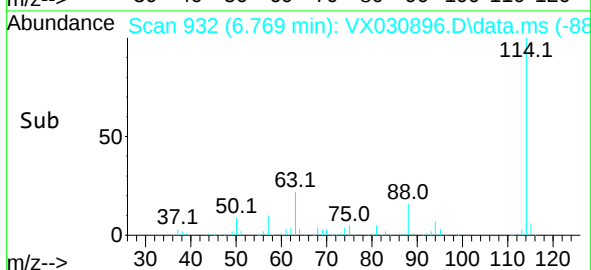

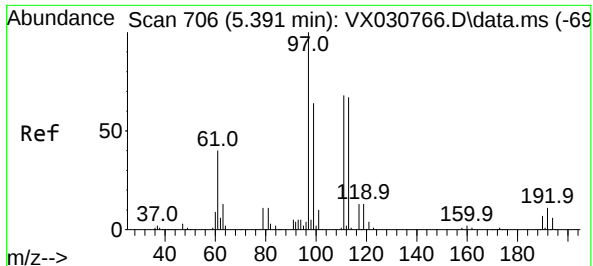

#35

Dibromofluoromethane

Concen: 51.667 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27

Instrument :

MSVOA_X

ClientSampleId :

TT180D2-20220823





Tgt Ion:113 Resp: 105648

Ion Ratio Lower Upper

113 100

111 103.0 83.2 124.8

192 17.9 14.8 22.2

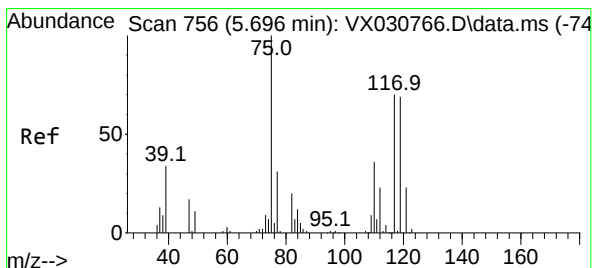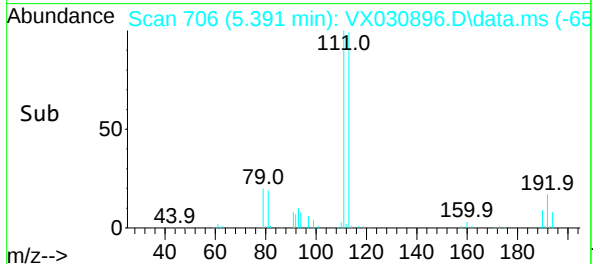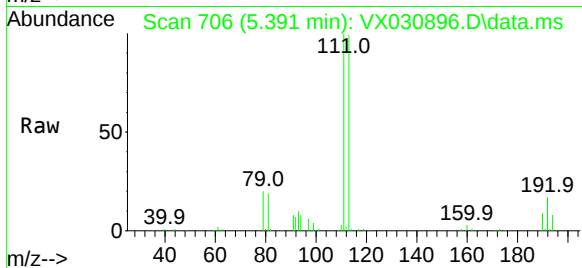

#36

1,1-Dichloropropene

Concen: 5.786 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27




Tgt Ion: 75 Resp: 16111


Ion Ratio Lower Upper

75 100

110 9.5 19.3 57.9#

77 0.0 24.4 36.6#

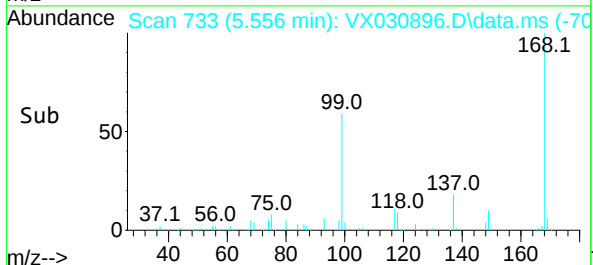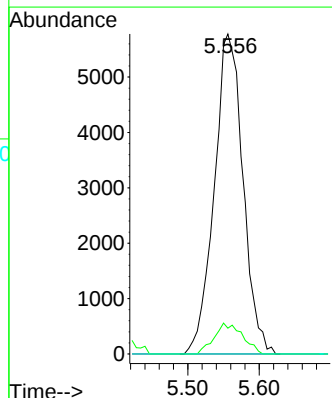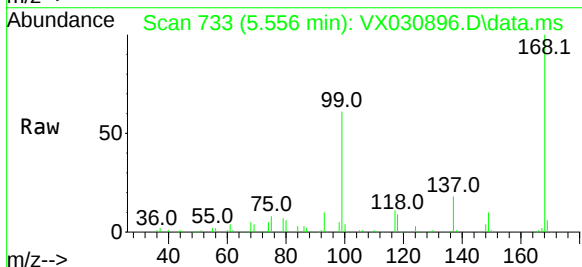



#38

Carbon Tetrachloride

Concen: 2.240 ug/l

RT: 5.684 min Scan# 71

Delta R.T. 0.006 min

Lab File: VX030896.D


Acq: 28 Aug 2022 02:27

Instrument :

MSVOA_X

ClientSampleId :

TT180D2-20220823

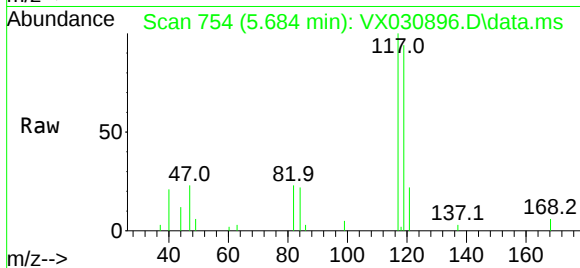




Tgt Ion:117 Resp: 6579

Ion Ratio Lower Upper

117 100

119 94.0 74.1 111.1

121 22.1 25.8 38.8#

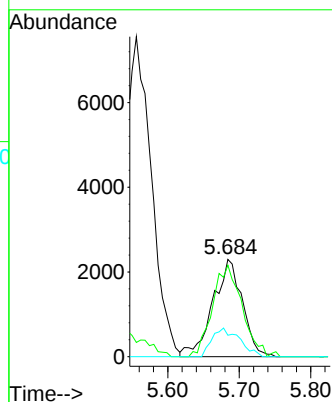

#39

Methylcyclohexane

Concen: 3.451 ug/l

RT: 7.129 min Scan# 991

Delta R.T. -0.256 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27




Tgt Ion: 83 Resp: 11501


Ion Ratio Lower Upper

83 100

55 0.0 57.7 86.5#

98 209.0 36.5 54.7#

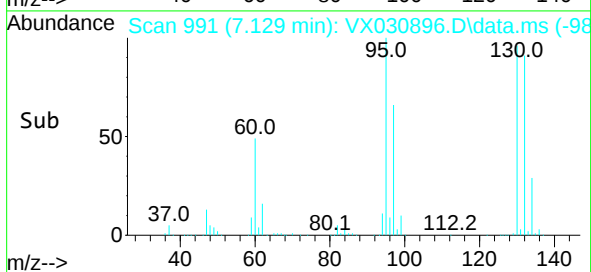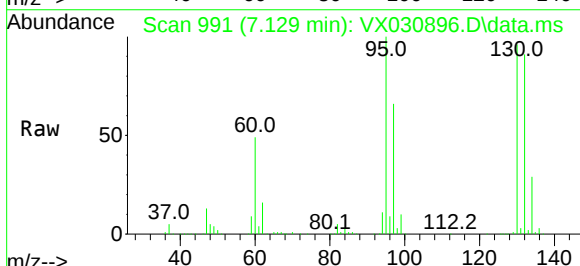



#42

1,2-Dichloroethane

Concen: 0.532 ug/l

RT: 6.099 min Scan# 81

Delta R.T. -0.000 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27

Instrument :

MSVOA_X

ClientSampleId :





TT180D2-20220823

Tgt Ion: 62 Resp: 1572

Ion Ratio Lower Upper

62 100

98 1.3 0.0 20.2

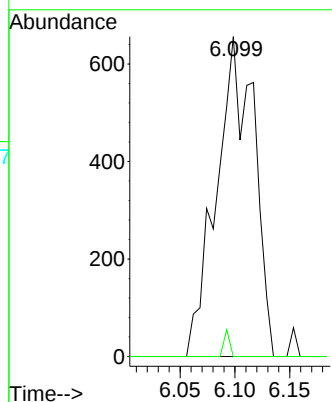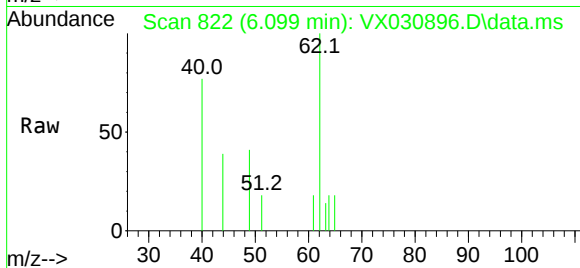

#44

Trichloroethene

Concen: 367.344 ug/l

RT: 7.129 min Scan# 991

Delta R.T. -0.000 min

Lab File: VX030896.D




Acq: 28 Aug 2022 02:27


Tgt Ion:130 Resp: 884106

Ion Ratio Lower Upper

130 100

95 104.0 0.0 194.8

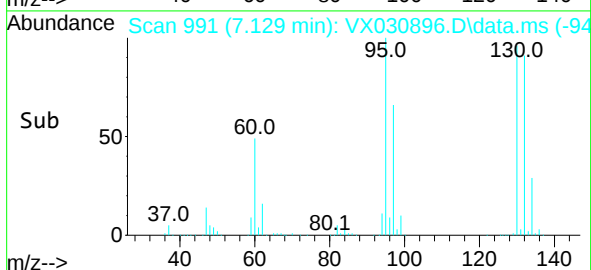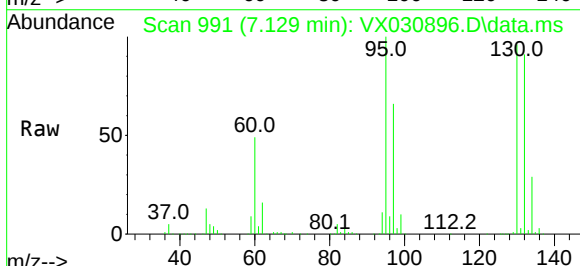

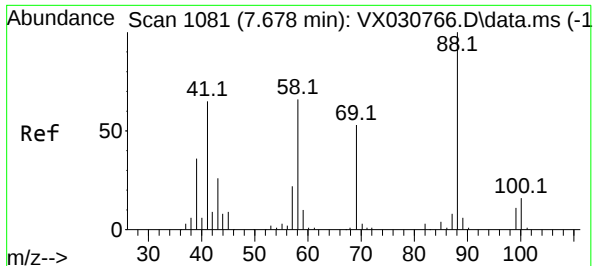

#49

1,4-Dioxane

Concen: 21.364 ug/l

RT: 7.690 min Scan# 1083

Delta R.T. 0.012 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27

Instrument :

MSVOA_X

ClientSampleId :

TT180D2-20220823





Tgt Ion: 88 Resp: 1306

Ion Ratio Lower Upper

88 100

43 34.8 23.8 35.8

58 42.8 53.8 80.6#

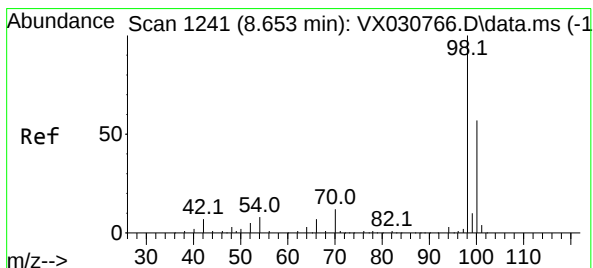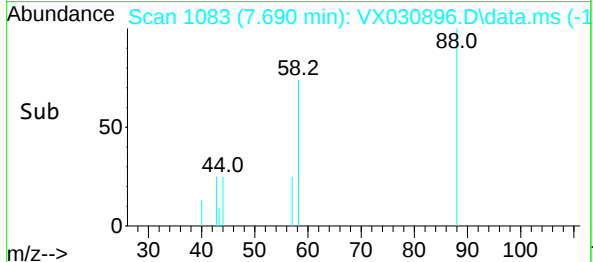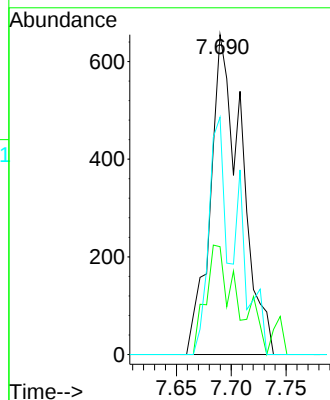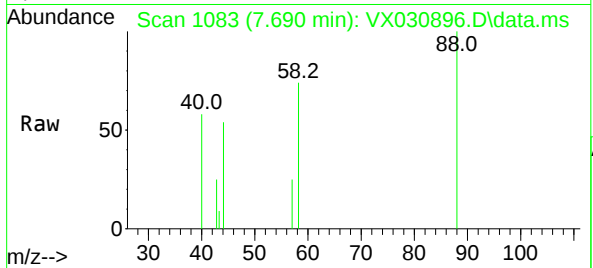

#50

Toluene-d8

Concen: 55.877 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.000 min

Lab File: VX030896.D




Acq: 28 Aug 2022 02:27


Tgt Ion: 98 Resp: 398144

Ion Ratio Lower Upper

98 100

100 62.8 52.3 78.5

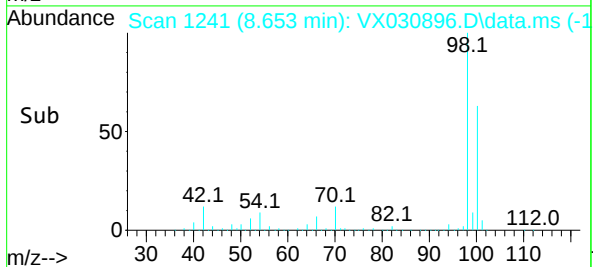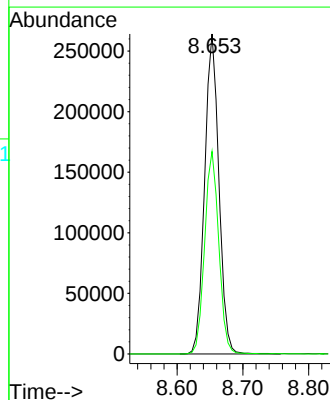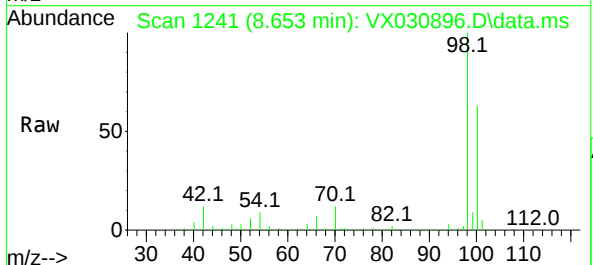

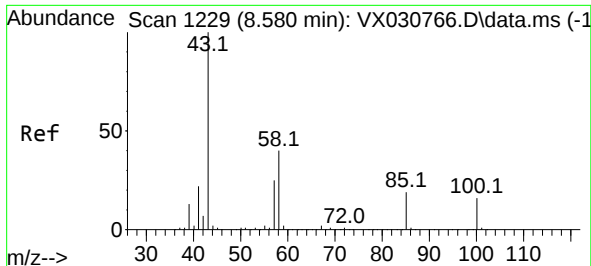

#51

4-Methyl-2-Pentanone

Concen: 0.534 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.067 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27

Instrument :

MSVOA_X

ClientSampleId :





TT180D2-20220823

Tgt Ion: 43 Resp: 1790

Ion Ratio Lower Upper

43 100

58 196.7 31.4 47.2#

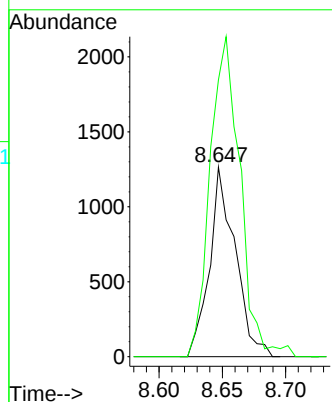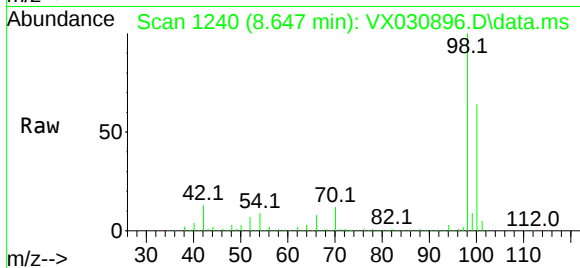

#55

1,1,2-Trichloroethane

Concen: 0.943 ug/l

RT: 9.159 min Scan# 1324

Delta R.T. 0.006 min

Lab File: VX030896.D

Acq: 28 Aug 2022 02:27

Tgt Ion: 97 Resp: 2179




Ion Ratio Lower Upper


97 100

83 84.1 68.9 103.3

85 57.7 44.0 66.0

99 64.4 48.3 72.5


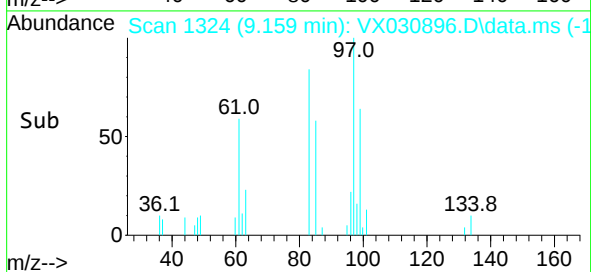

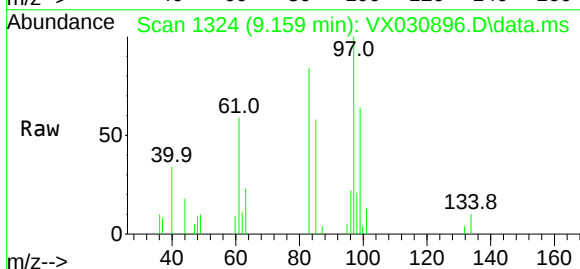


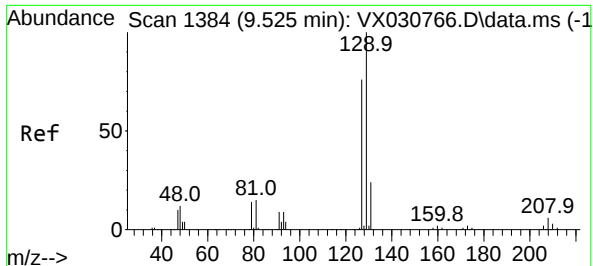

#60
Dibromochloromethane
Concen: 0.289 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27




Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823


Tgt Ion:129 Resp: 697
Ion Ratio Lower Upper
129 100
127 0.0 38.5 115.5#

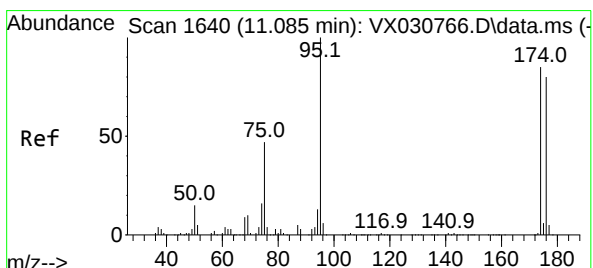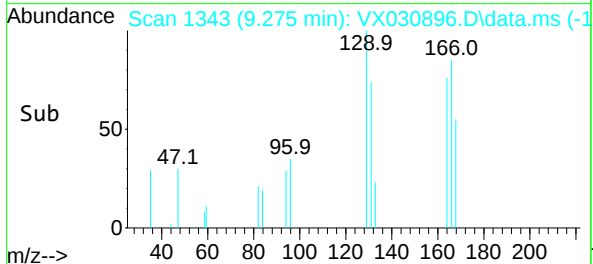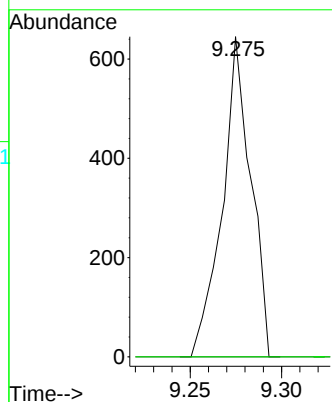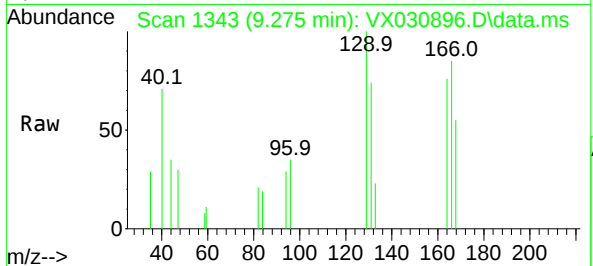

#62
4-Bromofluorobenzene
Concen: 50.345 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Tgt Ion: 95 Resp: 133553
Ion Ratio Lower Upper
95 100
174 73.4 0.0 149.0
176 70.8 0.0 146.0


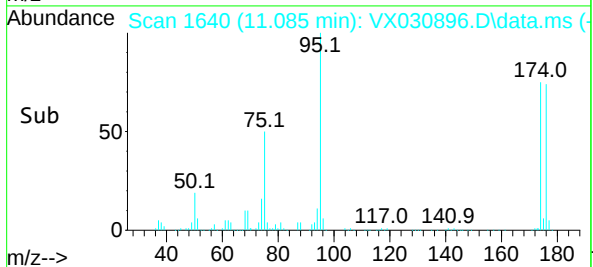
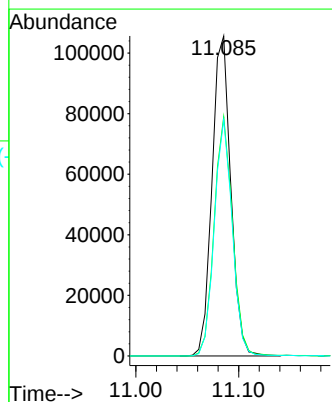
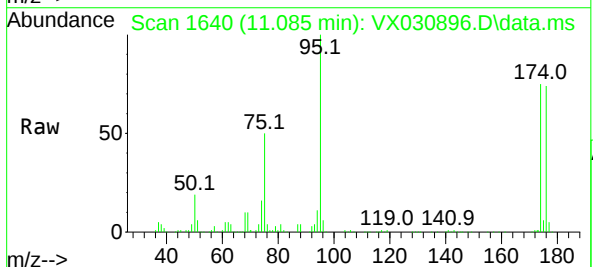




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27




Instrument :
MSVOA_X
ClientSampleId :
TT180D2-20220823


Tgt Ion:117 Resp: 293936
Ion Ratio Lower Upper
117 100
82 59.2 42.7 64.1
119 31.6 25.4 38.2

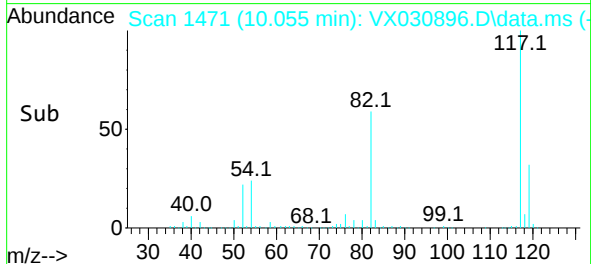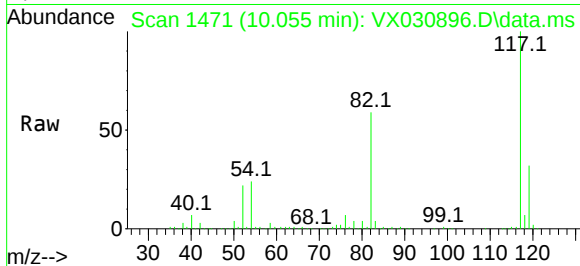

#64
Tetrachloroethene
Concen: 0.284 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX030896.D
Acq: 28 Aug 2022 02:27

Tgt Ion:164 Resp: 658
Ion Ratio Lower Upper
164 100
166 112.4 98.2 147.4
129 131.6 80.8 121.2#
131 97.6 75.5 113.3


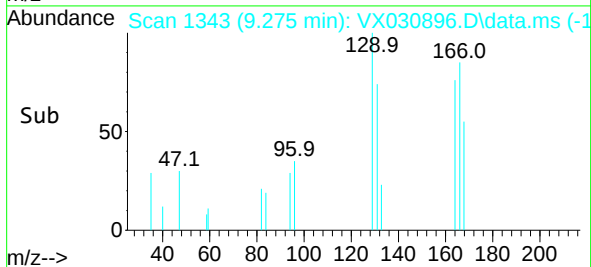

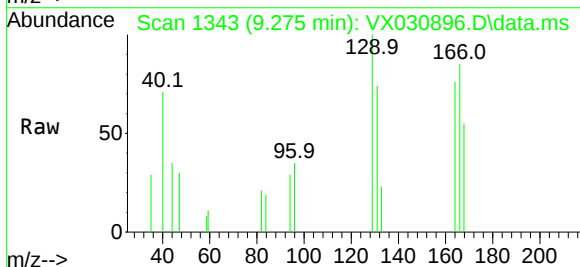




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX030896.D
 Acq: 28 Aug 2022 02:27




Instrument :
 MSVOA_X
 ClientSampleId :
 TT180D2-20220823


Tgt Ion:152 Resp: 125753
 Ion Ratio Lower Upper
 152 100
 115 62.1 40.5 121.5
 150 154.5 0.0 347.0

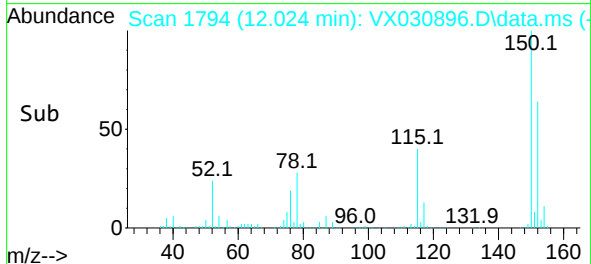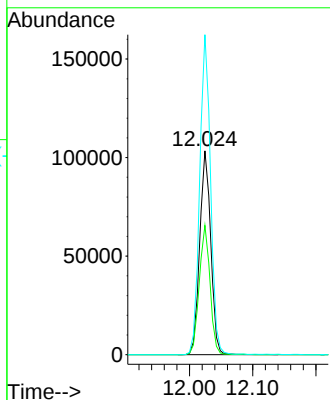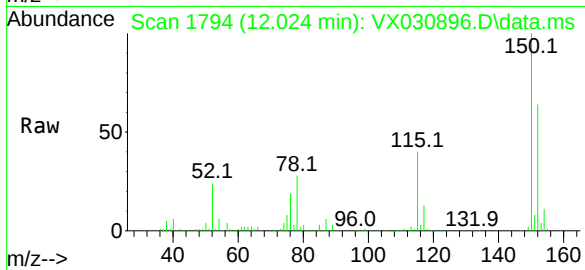

#76
 1,2,3-Trichloropropane
 Concen: 25.395 ug/l
 RT: 11.085 min Scan# 1640
 Delta R.T. -0.159 min
 Lab File: VX030896.D
 Acq: 28 Aug 2022 02:27


Tgt Ion: 75 Resp: 69965
 Ion Ratio Lower Upper
 75 100
 77 1.3 19.8 59.3#

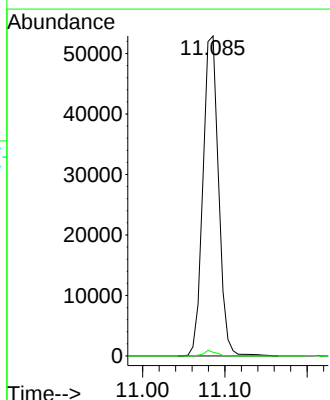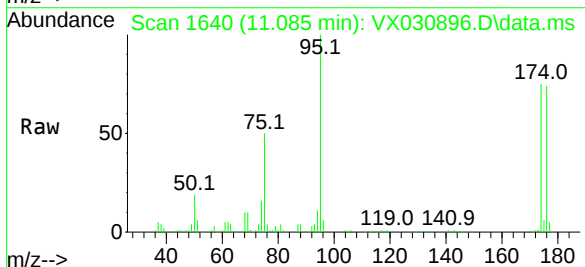



#81
 trans-1,4-Dichloro-2-butene
 Concen: 81.935 ug/l
 RT: 11.085 min Scan# 1
 Delta R.T. 0.067 min
 Lab File: VX030896.D
 Acq: 28 Aug 2022 02:27

Instrument :
 MSVOA_X
 ClientSampleId :
 TT180D2-20220823

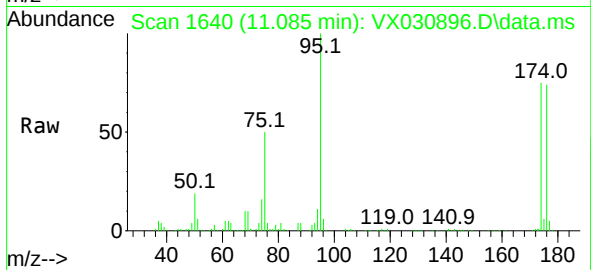

Tgt Ion: 75 Resp: 69965
 Ion Ratio Lower Upper
 75 100
 53 0.1 74.2 111.4#
 89 0.0 34.8 52.2#

