

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
 Data File : VX030904.D
 Acq On : 28 Aug 2022 05:35
 Operator : JC/MD
 Sample : N4360-9
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT101D1-20220824

Quant Time: Aug 29 01:16:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	159476	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	273951	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	246399	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	104686	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	125691	67.004	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 134.000%#	
35) Dibromofluoromethane	5.391	113	89946	53.423	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 106.840%	
50) Toluene-d8	8.653	98	339072	57.793	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 115.580%#	
62) 4-Bromofluorobenzene	11.085	95	111464	51.030	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 102.060%	
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.166	85	1737	1.175	ug/l	84
3) Chloromethane	1.295	50	345	Below Cal	#	81
4) Vinyl Chloride	1.453	62	40	Below Cal	#	43
5) Bromomethane	1.605	94	207	0.279	ug/l #	2
6) Chloroethane	1.715	64	167	Below Cal	#	41
7) Trichlorofluoromethane	1.892	101	627	0.257	ug/l	95
9) 1,1,2-Trichlorotrifluo...	2.331	101	26393	16.995	ug/l	96
12) 1,1-Dichloroethene	2.319	96	8695	6.015	ug/l	91
16) Acetone	2.392	43	1435	1.655	ug/l	91
17) Carbon Disulfide	2.520	76	139	Below Cal	#	74
20) Methylene Chloride	2.782	84	167	Below Cal	#	29
24) 1,1-Dichloroethane	3.617	63	3266	1.072	ug/l #	87
27) cis-1,2-Dichloroethene	4.489	96	4036	2.104	ug/l	85
29) Tetrahydrofuran	5.032	42	375	0.411	ug/l #	38
30) Chloroform	5.105	83	3353	1.046	ug/l	85
31) Cyclohexane	5.556	56	4184	1.744	ug/l #	26
32) 1,1,1-Trichloroethane	5.379	97	1131	0.436	ug/l #	24
36) 1,1-Dichloropropene	5.556	75	14628	6.380	ug/l #	48
38) Carbon Tetrachloride	5.678	117	2919	1.207	ug/l #	87
39) Methylcyclohexane	7.129	83	6630	2.416	ug/l #	1
42) 1,2-Dichloroethane	6.099	62	819	0.337	ug/l #	73
44) Trichloroethene	7.129	130	468224	236.273	ug/l	87
49) 1,4-Dioxane	7.690	88	1152	22.887	ug/l #	89
51) 4-Methyl-2-Pentanone	8.647	43	1791	0.649	ug/l #	1
55) 1,1,2-Trichloroethane	9.159	97	1095	0.576	ug/l	87
60) Dibromochloromethane	9.275	129	973	0.490	ug/l #	11
64) Tetrachloroethene	9.275	164	1133	0.584	ug/l #	79
76) 1,2,3-Trichloropropane	11.079	75	62465	27.235	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	62465	87.873	ug/l #	13

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
Data File : VX030904.D
Acq On : 28 Aug 2022 05:35
Operator : JC/MD
Sample : N4360-9
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824

Quant Time: Aug 29 01:16:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 26 02:03:28 2022
Response via : Initial Calibration




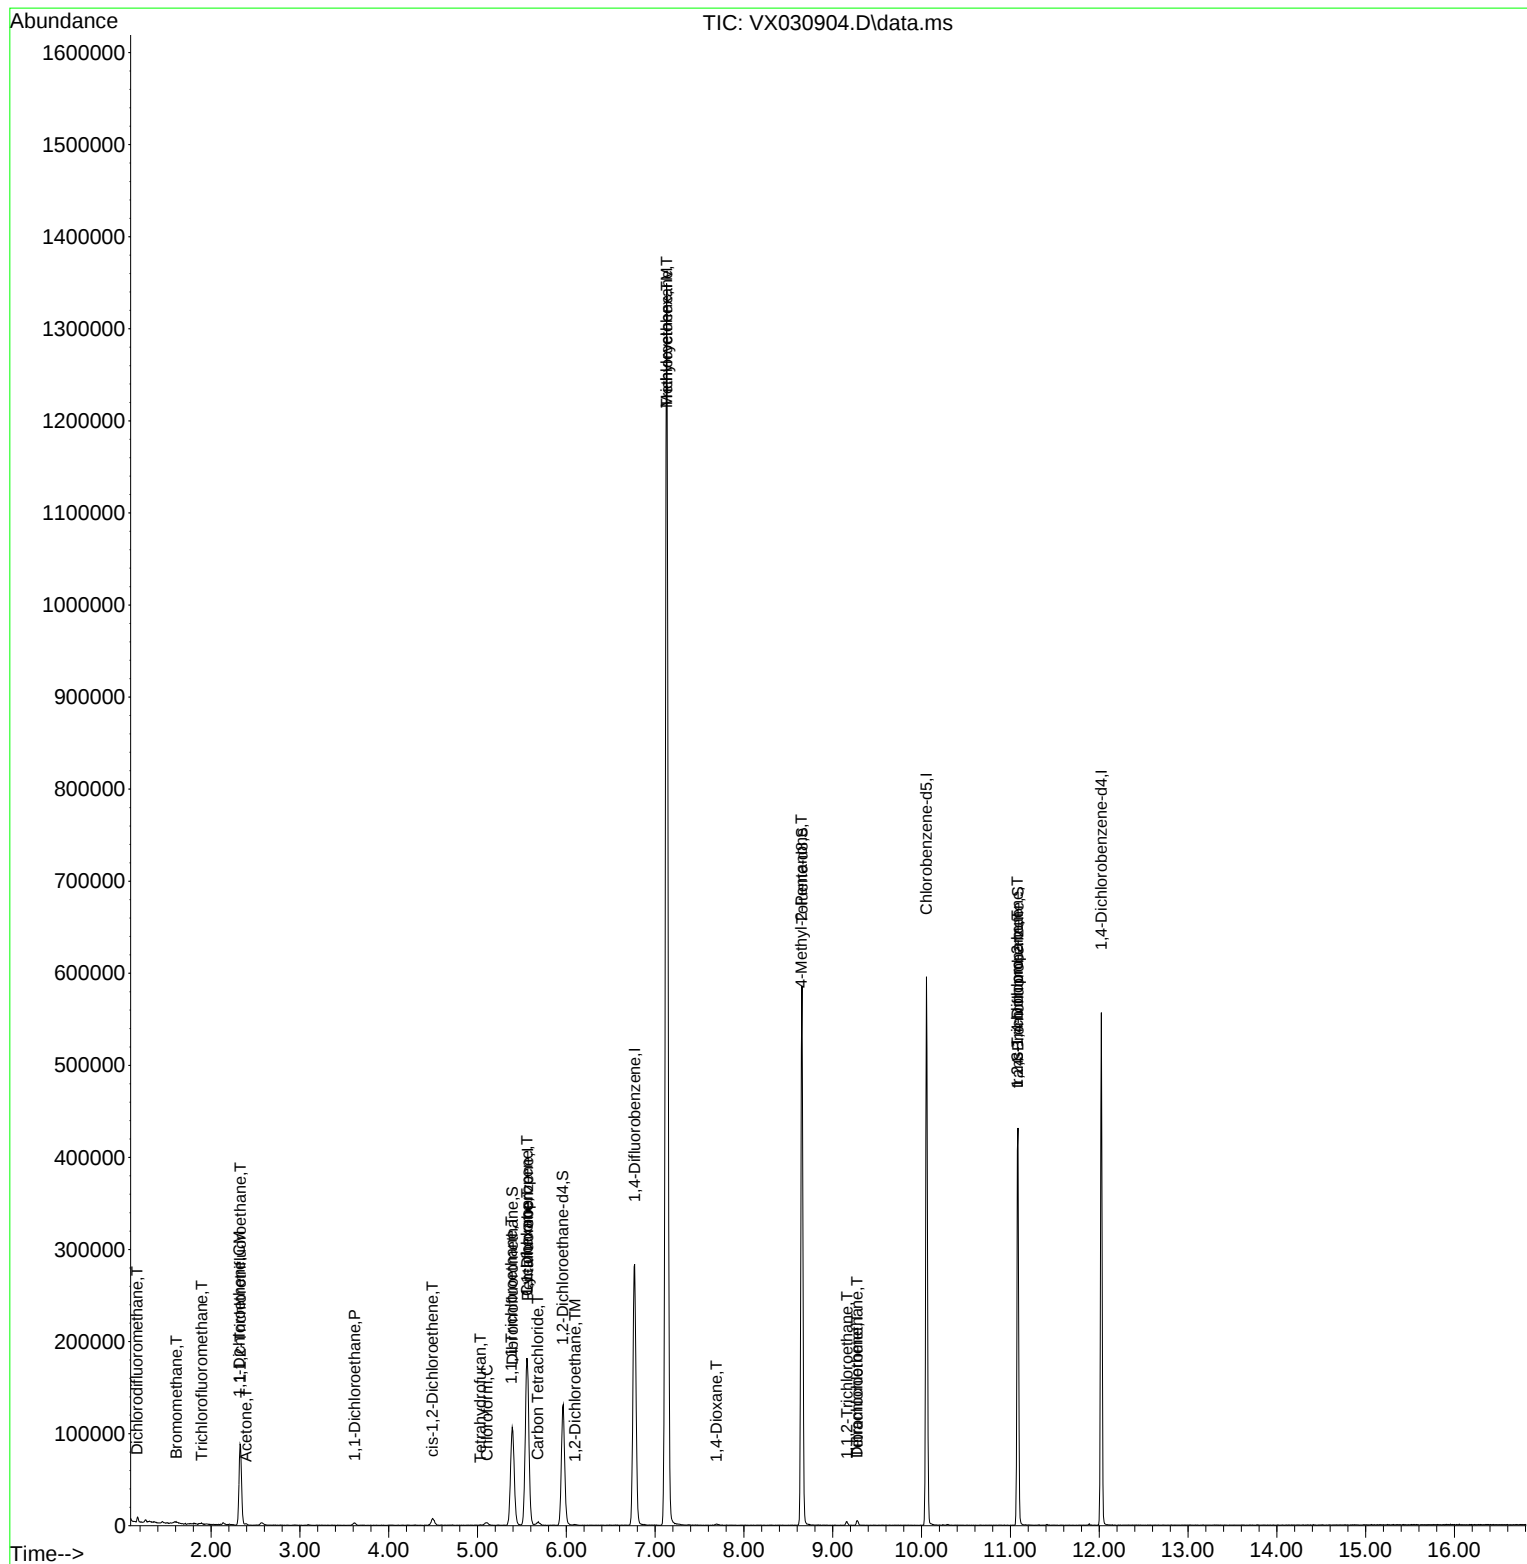




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion:168 Resp: 159476
Ion Ratio Lower Upper
168 100
99 61.4 44.0 66.0

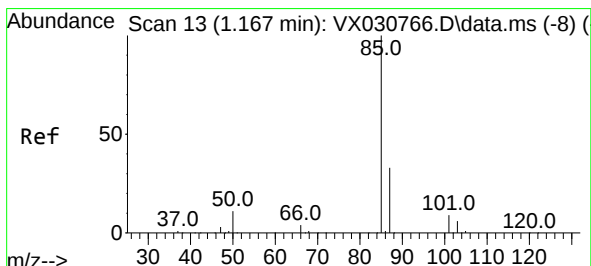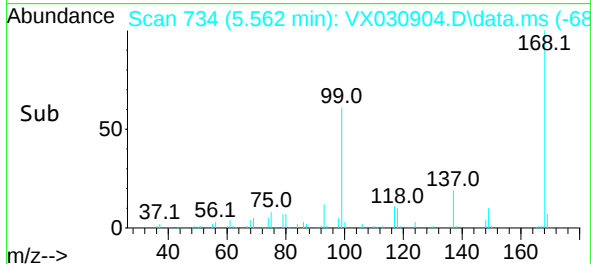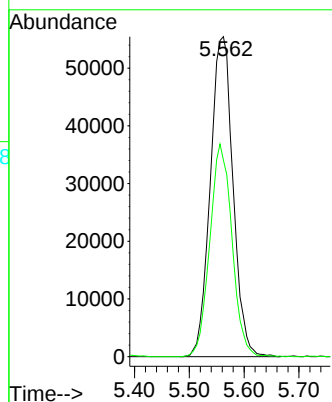

#2
Dichlorodifluoromethane
Concen: 1.175 ug/l
RT: 1.166 min Scan# 13
Delta R.T. -0.000 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 85 Resp: 1737
Ion Ratio Lower Upper
85 100
87 42.0 16.5 49.5




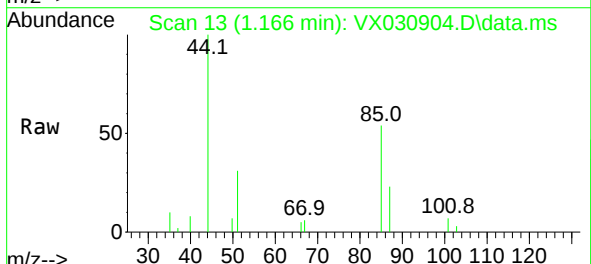


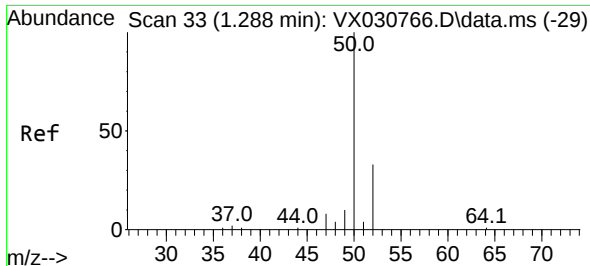

#3
Chloromethane
Concen: Below Cal
RT: 1.295 min Scan# 34
Delta R.T. 0.007 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion: 50 Resp: 345
Ion Ratio Lower Upper
50 100
52 22.0 26.3 39.5#

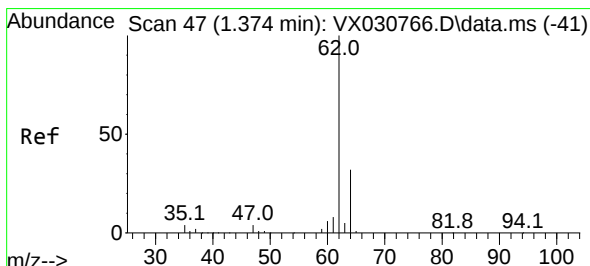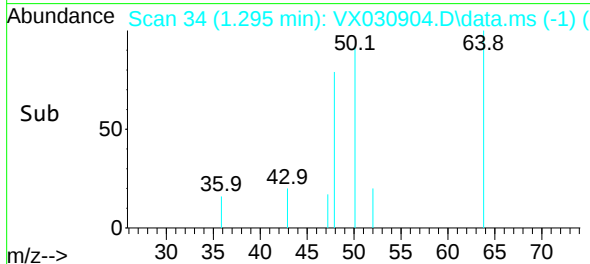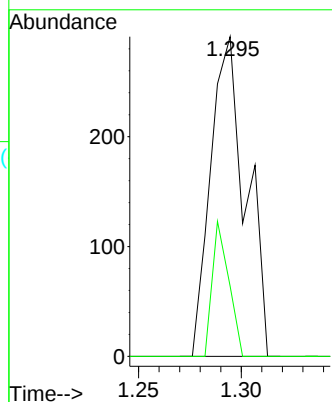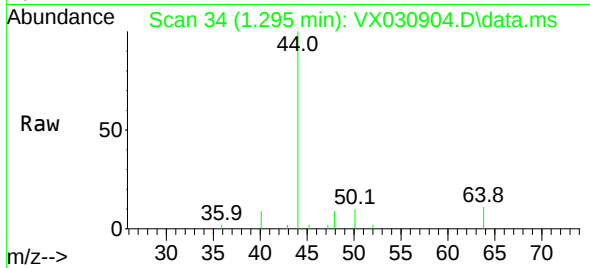

#4
Vinyl Chloride
Concen: Below Cal
RT: 1.453 min Scan# 60
Delta R.T. 0.079 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 62 Resp: 40
Ion Ratio Lower Upper
62 100
64 0.0 25.2 37.8#


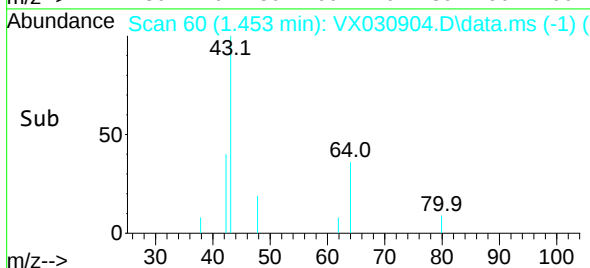

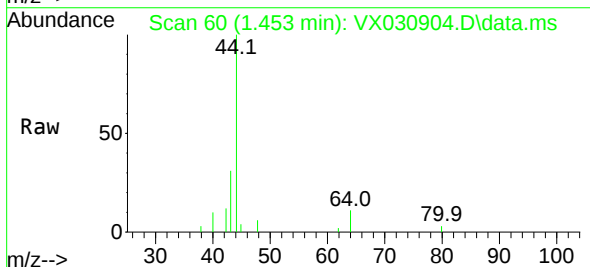


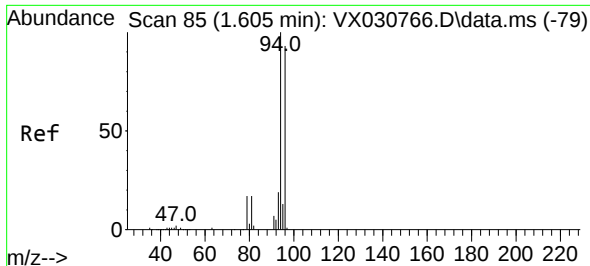

#5
Bromomethane
Concen: 0.279 ug/l
RT: 1.605 min Scan# 81
Delta R.T. -0.000 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion: 94 Resp: 207
Ion Ratio Lower Upper
94 100
96 0.0 76.9 115.3#

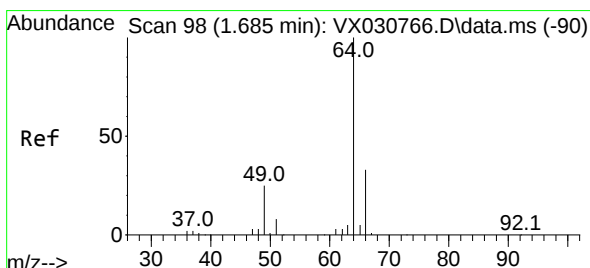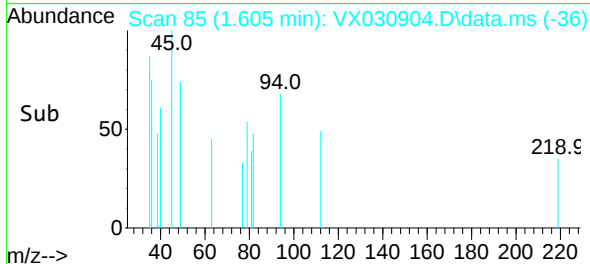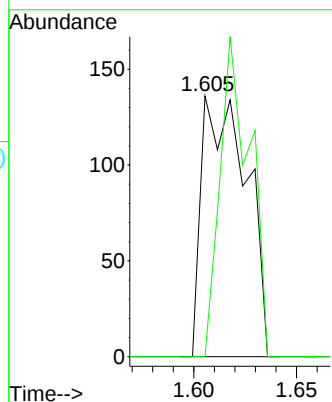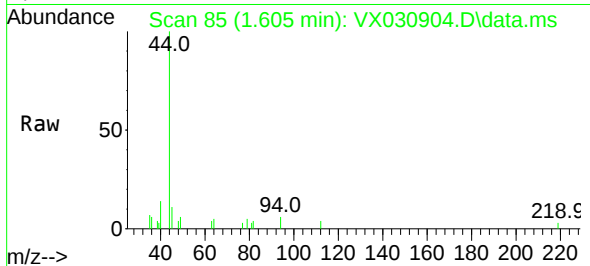

#6
Chloroethane
Concen: Below Cal
RT: 1.715 min Scan# 103
Delta R.T. 0.030 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 64 Resp: 167
Ion Ratio Lower Upper
64 100
66 0.0 27.2 40.8#


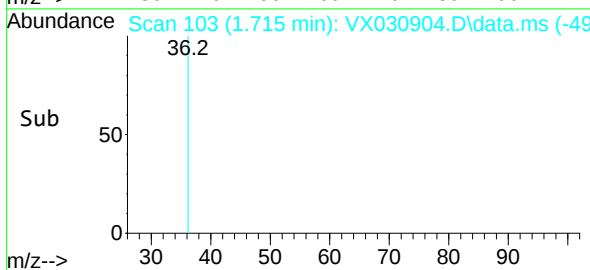
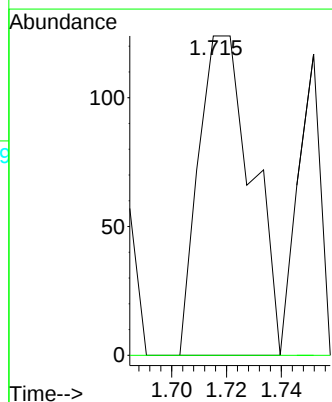
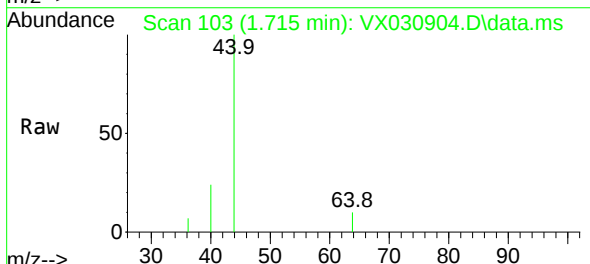


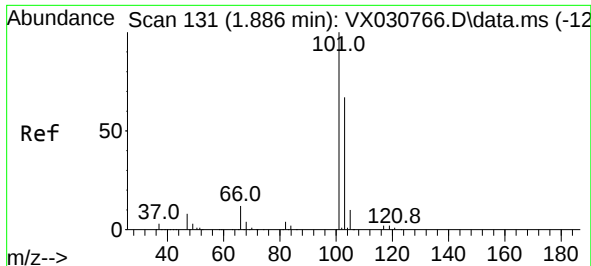

#7
Trichlorofluoromethane
Concen: 0.257 ug/l
RT: 1.892 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion:101 Resp: 627
Ion Ratio Lower Upper
101 100
103 65.7 49.7 74.5

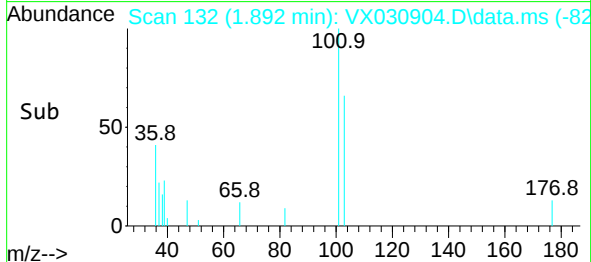

#9
1,1,2-Trichlorotrifluoroethane
Concen: 16.995 ug/l
RT: 2.331 min Scan# 204
Delta R.T. 0.006 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion:101 Resp: 26393
Ion Ratio Lower Upper
101 100
85 49.1 34.0 51.0
151 74.8 59.4 89.0

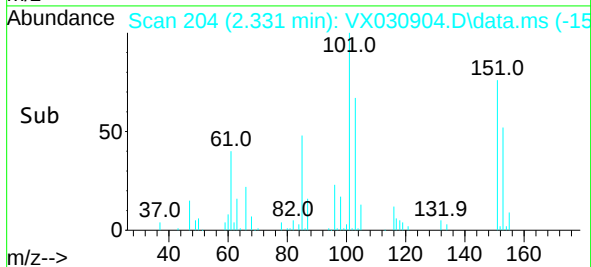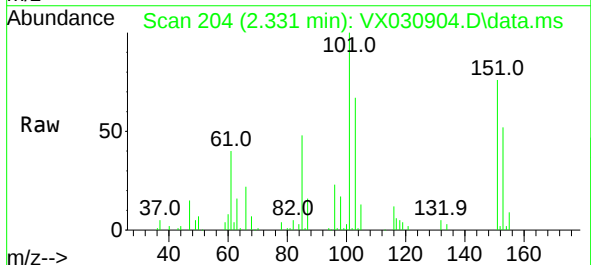



#12

1,1-Dichloroethene

Concen: 6.015 ug/l

RT: 2.319 min Scan# 20

Delta R.T. -0.000 min

Lab File: VX030904.D


Acq: 28 Aug 2022 05:35

Instrument :

MSVOA_X

ClientSampleId :

TT101D1-20220824

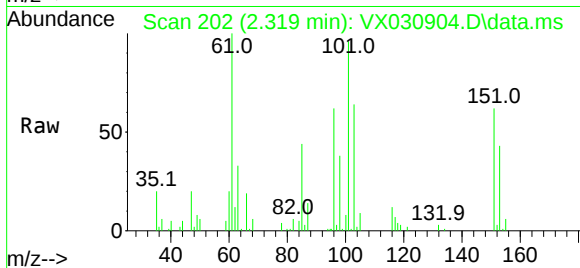




Tgt Ion: 96 Resp: 8695

Ion Ratio Lower Upper

96 100

61 160.7 117.4 176.0

98 61.2 52.2 78.4

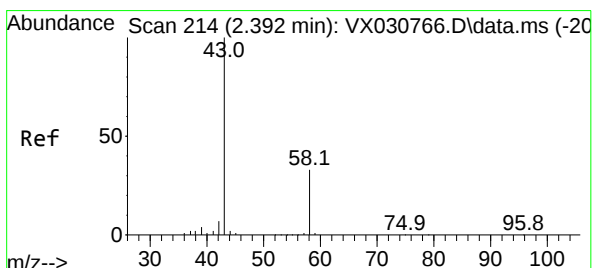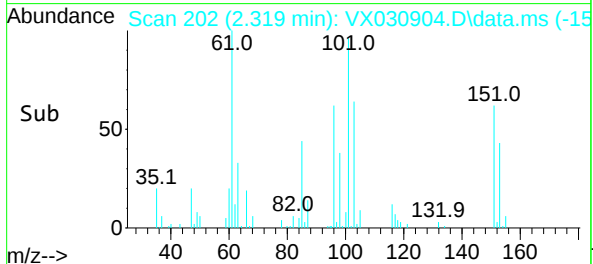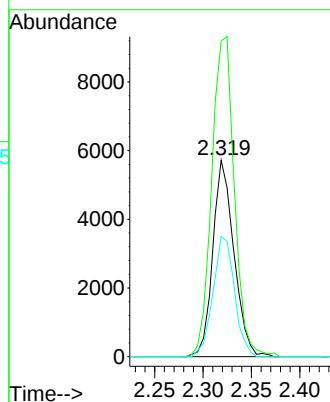

#16

Acetone

Concen: 1.655 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX030904.D




Acq: 28 Aug 2022 05:35


Tgt Ion: 43 Resp: 1435

Ion Ratio Lower Upper

43 100

58 29.5 27.7 41.5


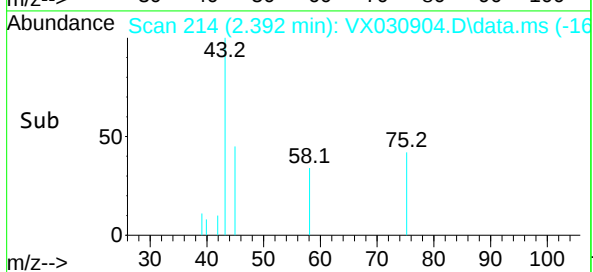
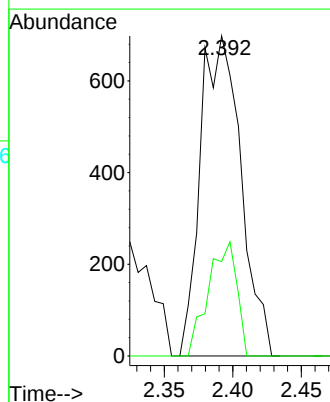
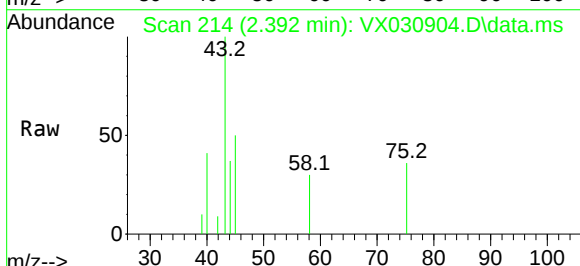




#17
Carbon Disulfide
Concen: Below Cal
RT: 2.520 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion: 76 Resp: 139
Ion Ratio Lower Upper
76 100
78 0.0 7.8 11.6#

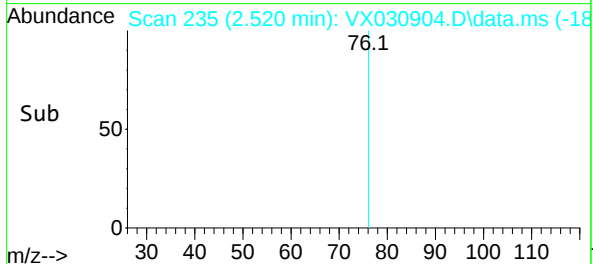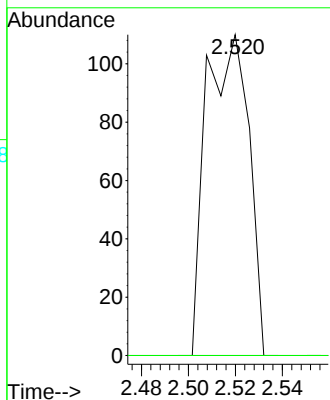

#20
Methylene Chloride
Concen: Below Cal
RT: 2.782 min Scan# 278
Delta R.T. -0.006 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 84 Resp: 167
Ion Ratio Lower Upper
84 100
49 192.7 93.8 140.6#
51 0.0 29.4 44.0#
86 0.0 51.0 76.4#


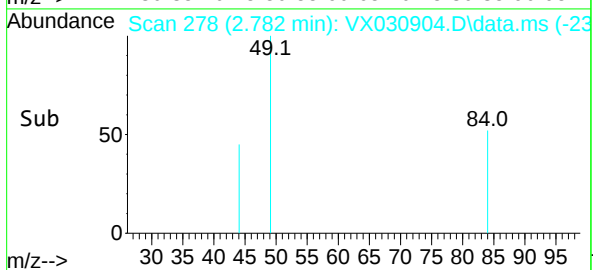
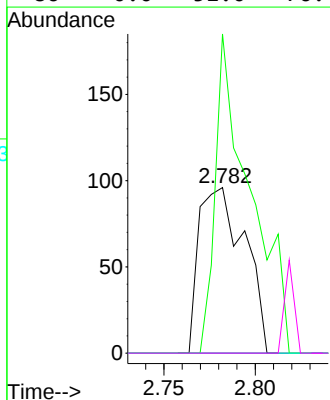
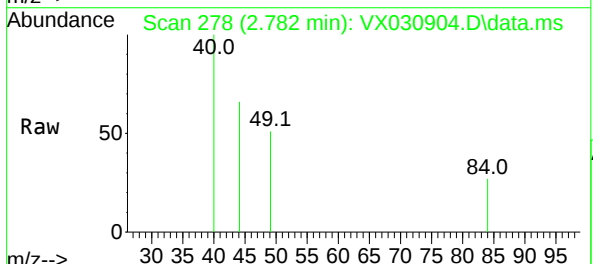




#24
1,1-Dichloroethane
Concen: 1.072 ug/l
RT: 3.617 min Scan# 414
Delta R.T. 0.006 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion: 63 Resp: 3266
Ion Ratio Lower Upper
63 100
98 0.0 3.5 10.5#
100 4.2 2.3 6.9

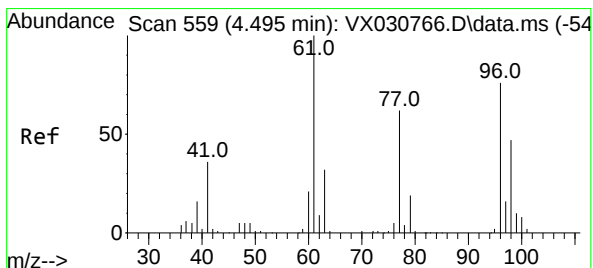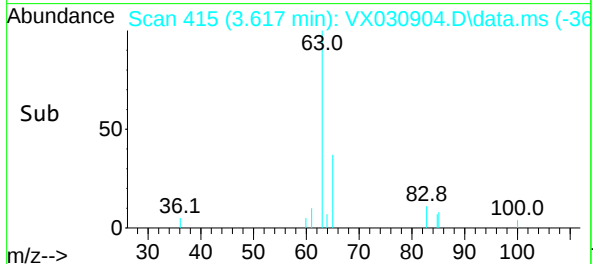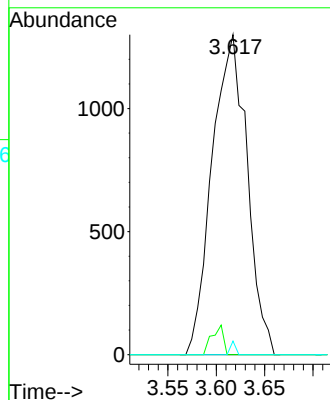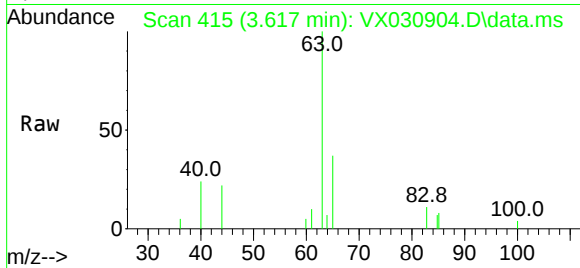

#27
cis-1,2-Dichloroethene
Concen: 2.104 ug/l
RT: 4.489 min Scan# 558
Delta R.T. -0.006 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 96 Resp: 4036
Ion Ratio Lower Upper
96 100
61 155.2 0.0 270.0
98 73.1 0.0 127.8

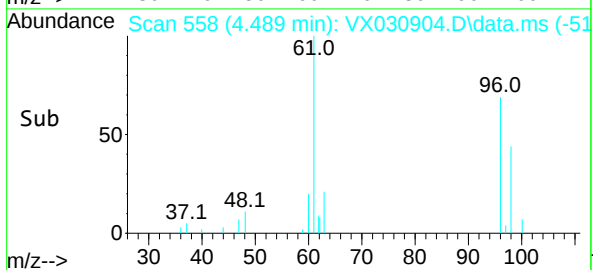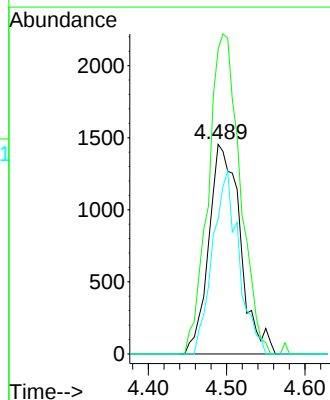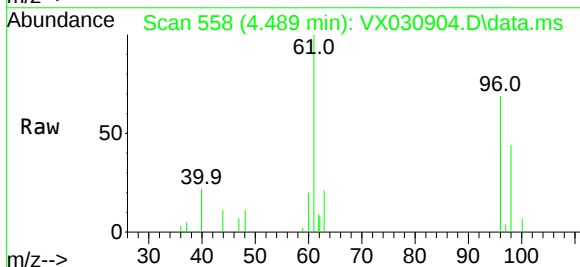



#29

Tetrahydrofuran

Concen: 0.411 ug/l

RT: 5.032 min Scan# 64

Delta R.T. 0.019 min

Lab File: VX030904.D


Acq: 28 Aug 2022 05:35

Instrument :




MSVOA_X

ClientSampleId :

TT101D1-20220824

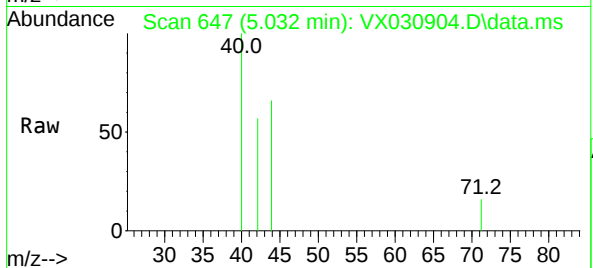

Tgt Ion:	42	Resp:	375
Ion Ratio	Lower	Upper	
42	100		
72	0.0	36.5	54.7#
71	7.7	33.9	50.9#

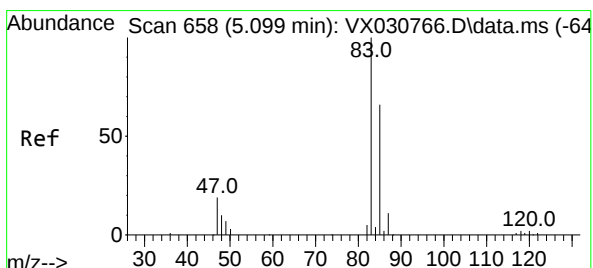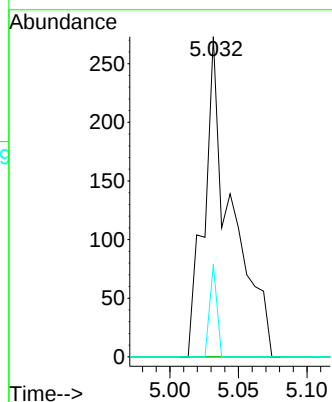

#30

Chloroform

Concen: 1.046 ug/l




RT: 5.105 min Scan# 659


Delta R.T. 0.006 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35


Tgt Ion:	83	Resp:	3353
Ion Ratio	Lower	Upper	
83	100		
85	52.5	51.5	77.3

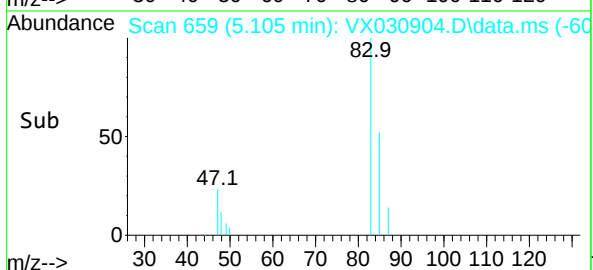






#31
Cyclohexane
Concen: 1.744 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.085 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824

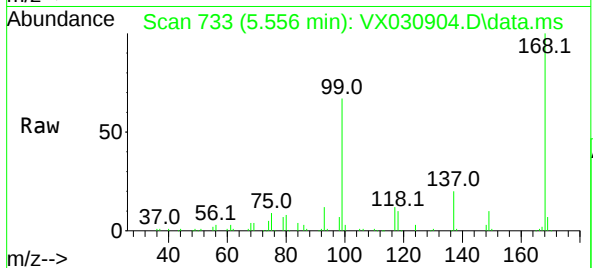

Tgt Ion: 56 Resp: 4184




Ion	Ratio	Lower	Upper
56	100		
69	128.0	25.4	38.0#
84	120.1	68.9	103.3#

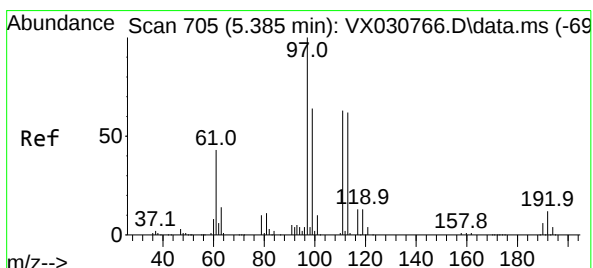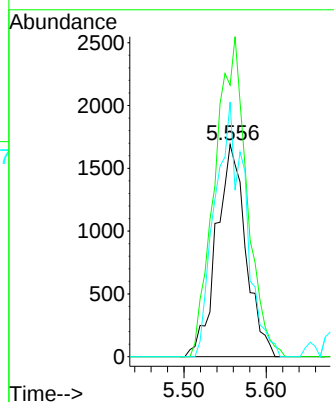


#32
1,1,1-Trichloroethane
Concen: 0.436 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 97 Resp: 1131

Ion	Ratio	Lower	Upper
97	100		
99	0.0	51.4	77.0#
61	0.0	35.8	53.8#

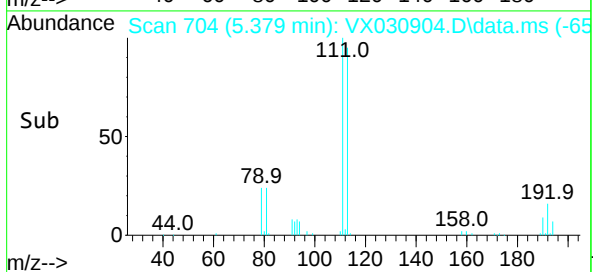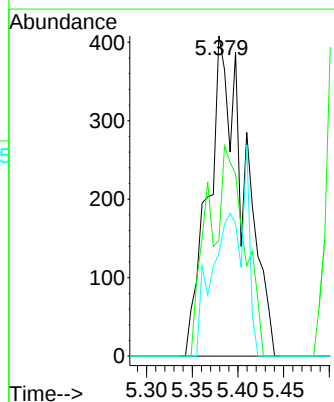

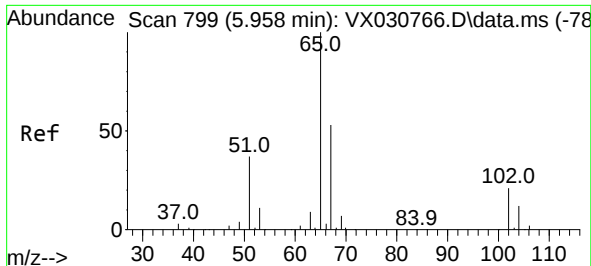

#33

1,2-Dichloroethane-d4

Concen: 67.004 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35

Instrument :

MSVOA_X

ClientSampleId :





TT101D1-20220824

Tgt Ion: 65 Resp: 125691

Ion Ratio Lower Upper

65 100

67 51.7 0.0 109.6

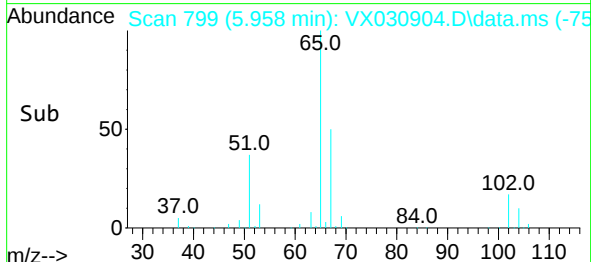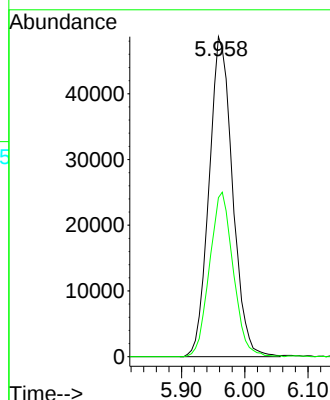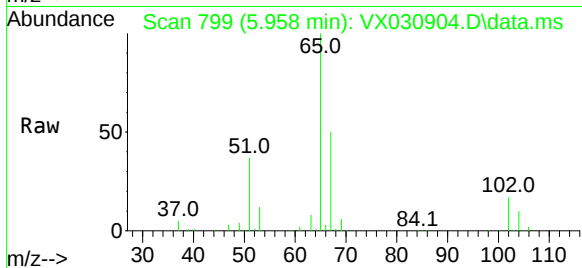

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35




Tgt Ion: 114 Resp: 273951


Ion Ratio Lower Upper

114 100

63 23.4 0.0 38.4

88 16.6 0.0 31.8

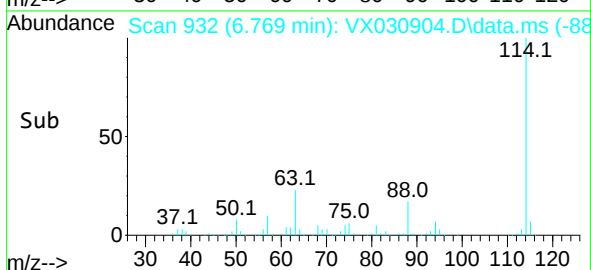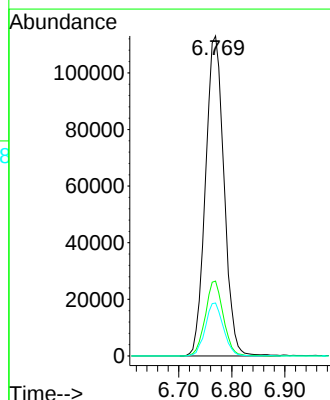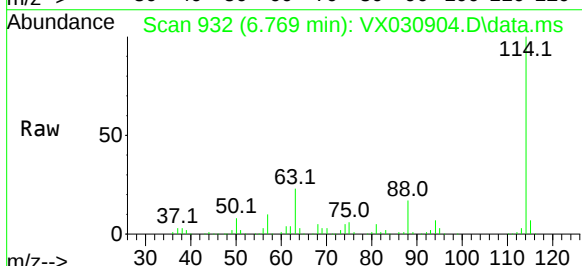



#35

Dibromofluoromethane

Concen: 53.423 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX030904.D


Acq: 28 Aug 2022 05:35

Instrument :

MSVOA_X

ClientSampleId :

TT101D1-20220824

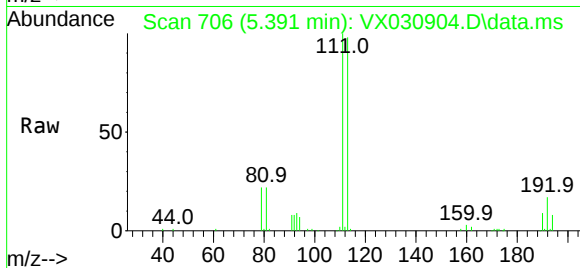




Tgt Ion:113 Resp: 89946

Ion Ratio Lower Upper

113 100

111 105.4 83.2 124.8

192 17.3 14.8 22.2

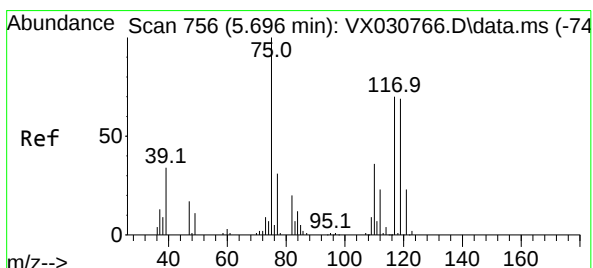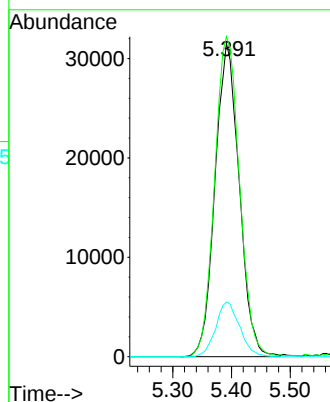

#36

1,1-Dichloropropene

Concen: 6.380 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35




Tgt Ion: 75 Resp: 14628


Ion Ratio Lower Upper

75 100

110 9.4 19.3 57.9#

77 0.0 24.4 36.6#


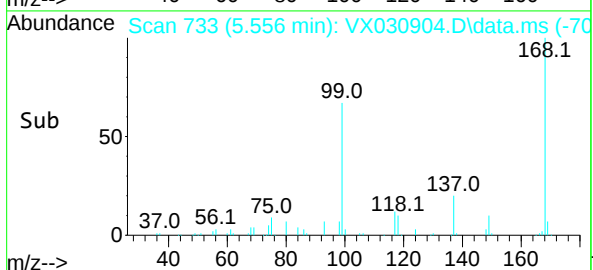
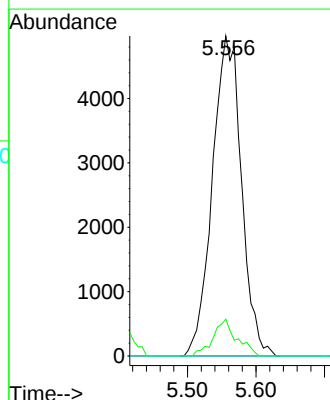
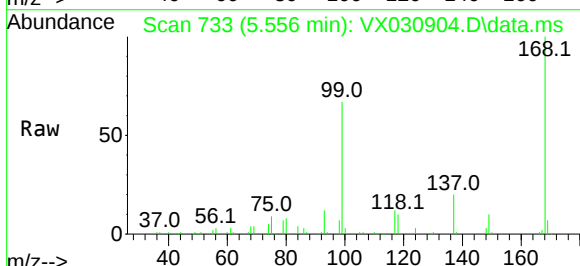


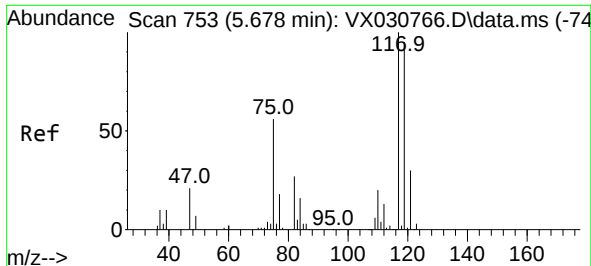

#38
Carbon Tetrachloride
Concen: 1.207 ug/l
RT: 5.678 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion:117 Resp: 2919
Ion Ratio Lower Upper
117 100
119 82.5 74.1 111.1
121 21.4 25.8 38.8#

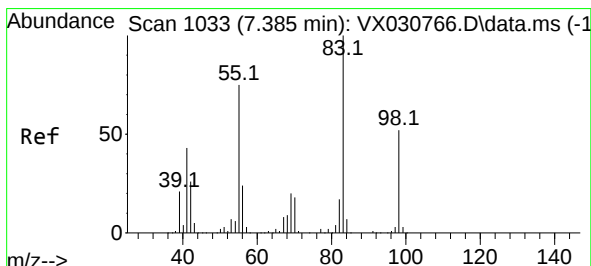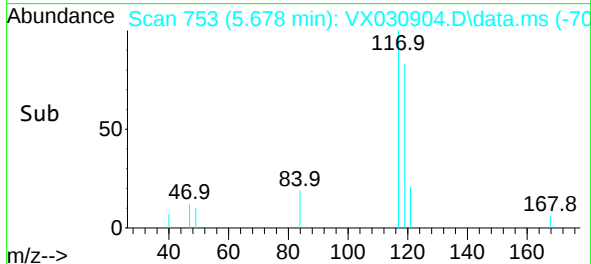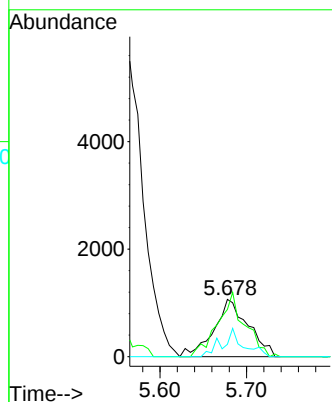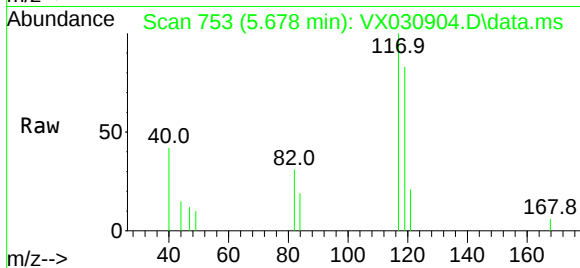

#39
Methylcyclohexane
Concen: 2.416 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.256 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 83 Resp: 6630
Ion Ratio Lower Upper
83 100
55 0.0 57.7 86.5#
98 182.4 36.5 54.7#

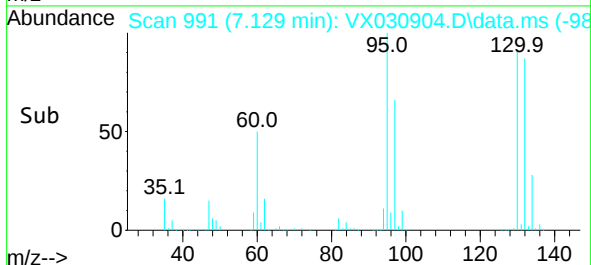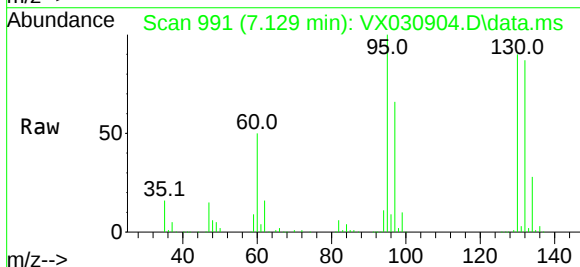



#42

1,2-Dichloroethane

Concen: 0.337 ug/l

RT: 6.099 min Scan# 81

Delta R.T. -0.000 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35

Instrument :

MSVOA_X

ClientSampleId :





TT101D1-20220824

Tgt Ion: 62 Resp: 819

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.2

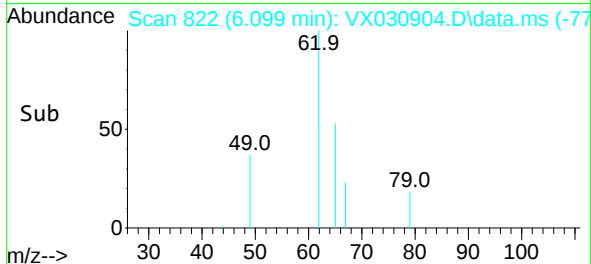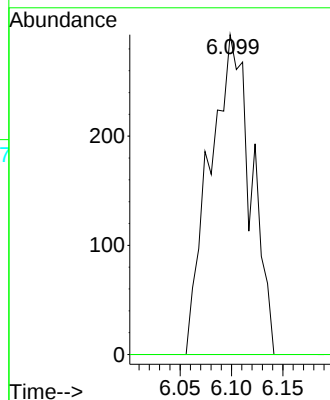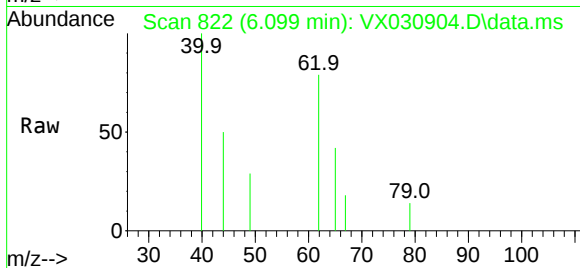

#44

Trichloroethene

Concen: 236.273 ug/l

RT: 7.129 min Scan# 991

Delta R.T. -0.000 min

Lab File: VX030904.D




Acq: 28 Aug 2022 05:35


Tgt Ion:130 Resp: 468224

Ion Ratio Lower Upper

130 100

95 110.5 0.0 194.8

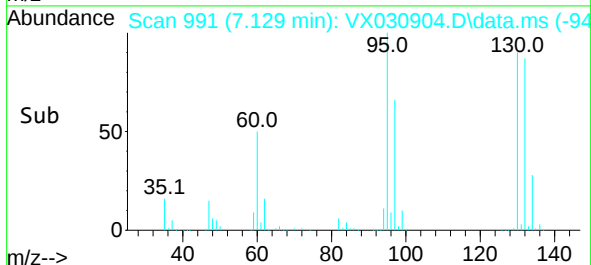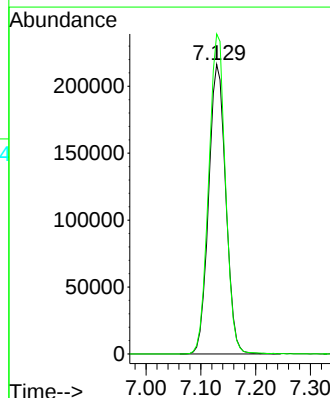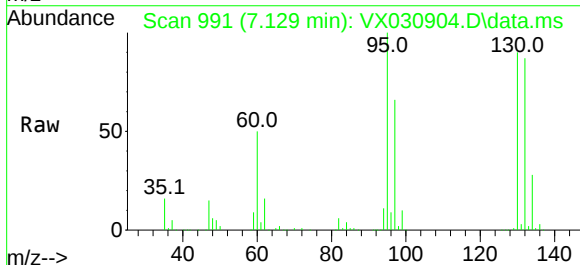

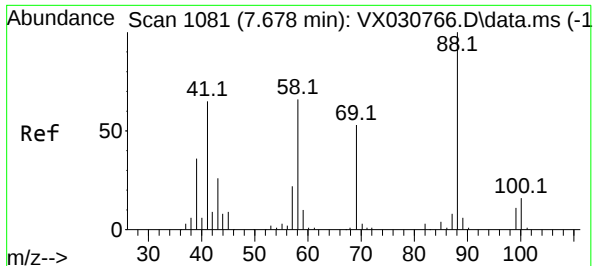

#49

1,4-Dioxane

Concen: 22.887 ug/l

RT: 7.690 min Scan# 110

Delta R.T. 0.012 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35

Instrument :

MSVOA_X

ClientSampleId :

TT101D1-20220824





Tgt Ion: 88 Resp: 1152

Ion Ratio Lower Upper

88 100

43 15.4 23.8 35.8#

58 70.0 53.8 80.6

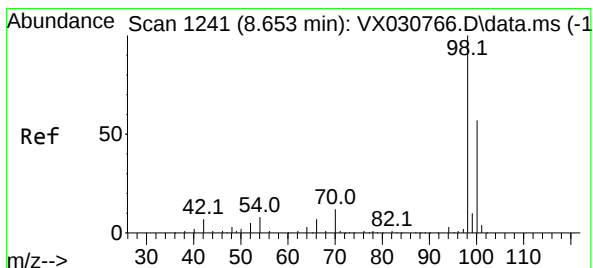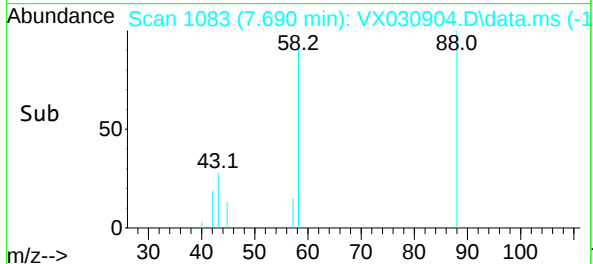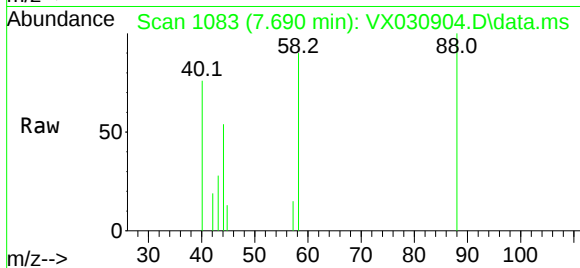

#50

Toluene-d8

Concen: 57.793 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX030904.D




Acq: 28 Aug 2022 05:35


Tgt Ion: 98 Resp: 339072

Ion Ratio Lower Upper

98 100

100 62.2 52.3 78.5

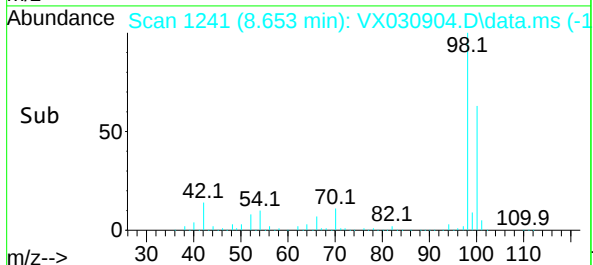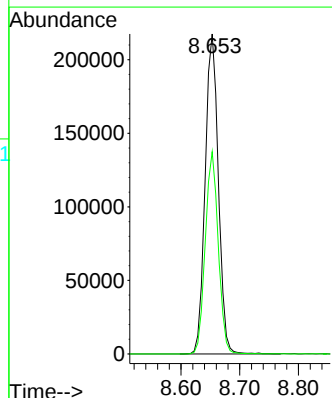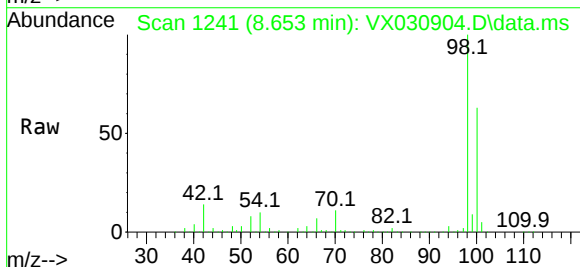

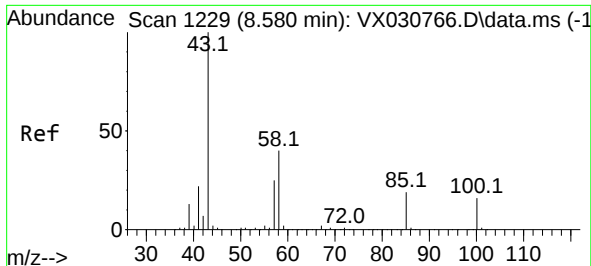

#51

4-Methyl-2-Pentanone

Concen: 0.649 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.067 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35

Instrument :

MSVOA_X

ClientSampleId :





TT101D1-20220824

Tgt Ion: 43 Resp: 1791

Ion Ratio Lower Upper

43 100

58 175.1 31.4 47.2#

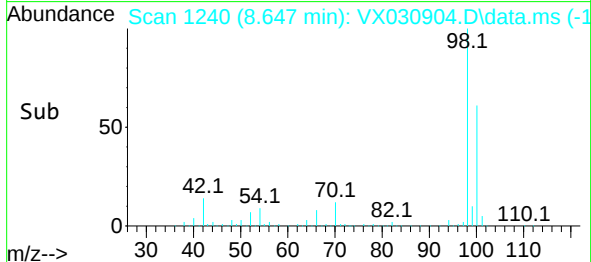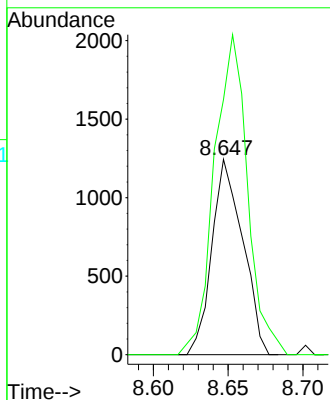

#55

1,1,2-Trichloroethane

Concen: 0.576 ug/l

RT: 9.159 min Scan# 1324

Delta R.T. 0.006 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35

Tgt Ion: 97 Resp: 1095




Ion Ratio Lower Upper


97 100

83 103.3 68.9 103.3

85 48.7 44.0 66.0

99 53.9 48.3 72.5

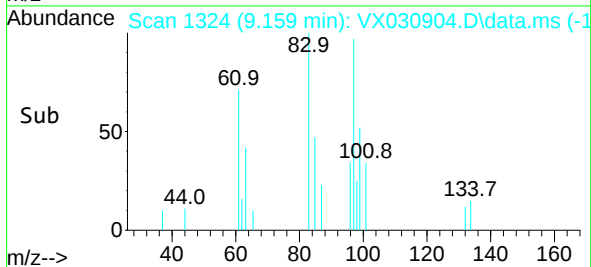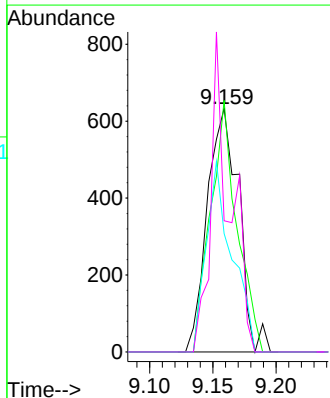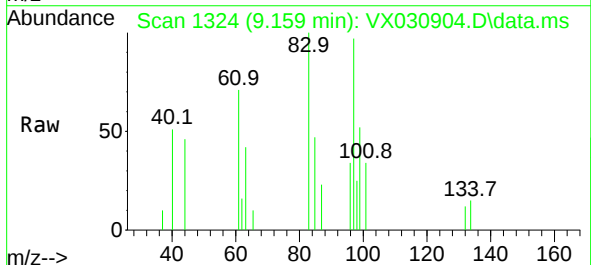



#60

Dibromochloromethane

Concen: 0.490 ug/l

RT: 9.275 min Scan# 11

Delta R.T. -0.250 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35

Instrument :

MSVOA_X

ClientSampleId :





TT101D1-20220824

Tgt Ion:129 Resp: 973

Ion Ratio Lower Upper

129 100

127 0.0 38.5 115.5#

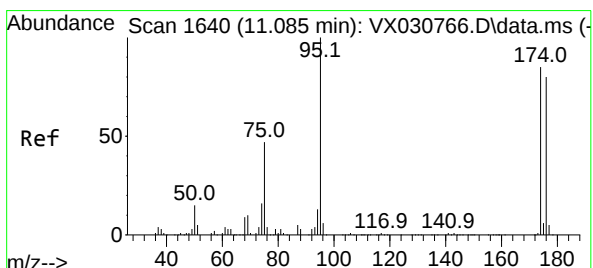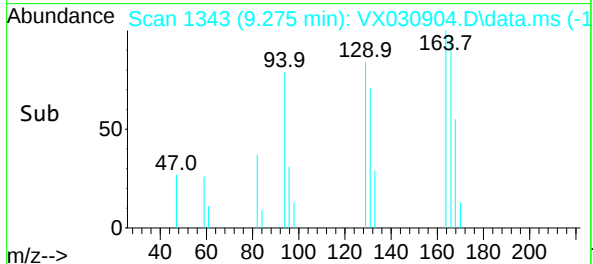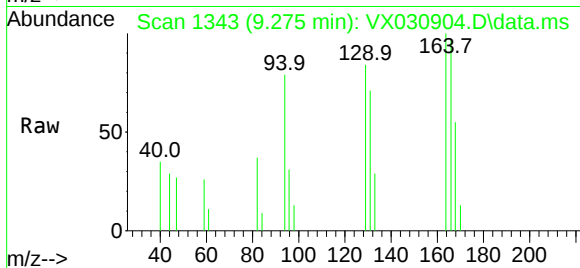

#62

4-Bromofluorobenzene

Concen: 51.030 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.000 min

Lab File: VX030904.D

Acq: 28 Aug 2022 05:35




Tgt Ion: 95 Resp: 111464


Ion Ratio Lower Upper

95 100

174 74.9 0.0 149.0

176 72.2 0.0 146.0


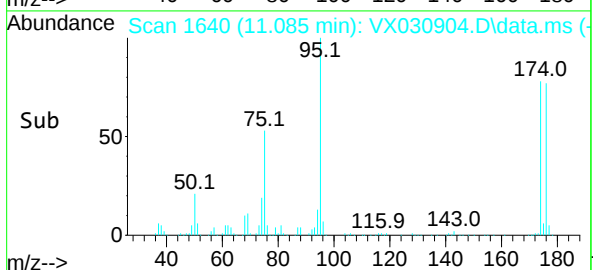

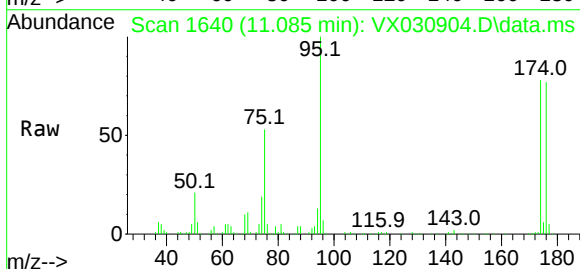


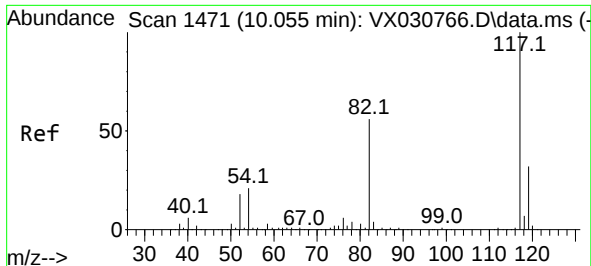

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion:117 Resp: 246399
Ion Ratio Lower Upper
117 100
82 59.8 42.7 64.1
119 32.1 25.4 38.2

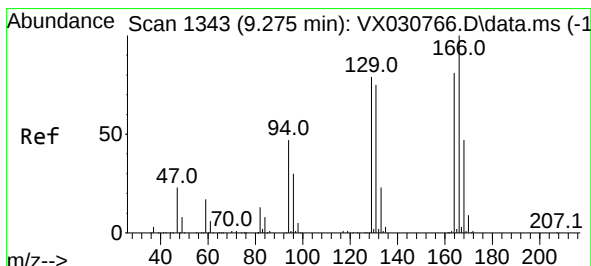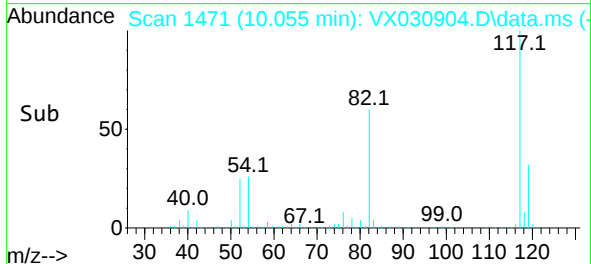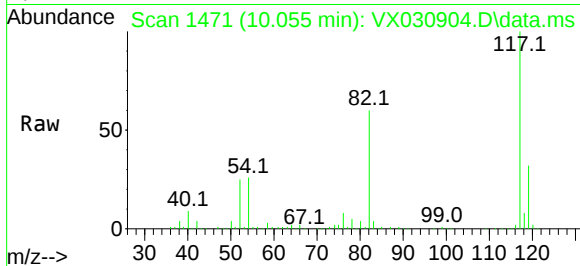

#64
Tetrachloroethene
Concen: 0.584 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion:164 Resp: 1133
Ion Ratio Lower Upper
164 100
166 96.6 98.2 147.4#
129 84.2 80.8 121.2
131 71.0 75.5 113.3#



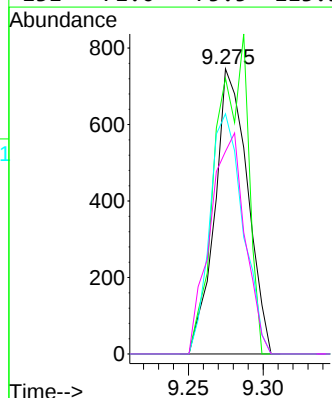
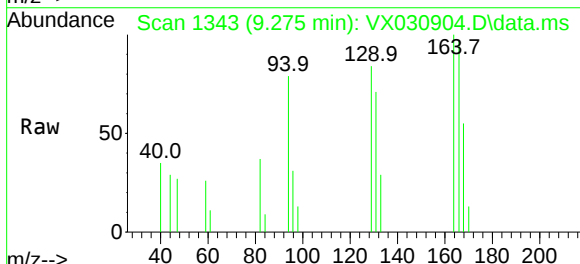




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35




Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824


Tgt Ion:152 Resp: 104686
Ion Ratio Lower Upper
152 100
115 63.3 40.5 121.5
150 157.7 0.0 347.0

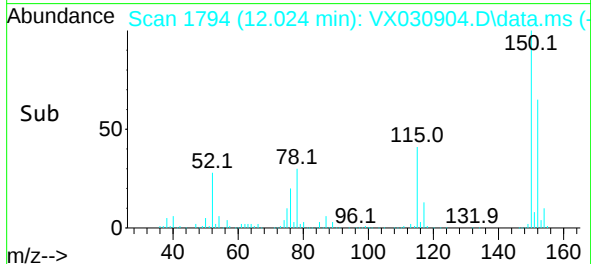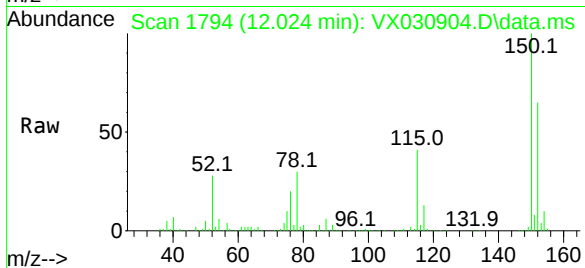

#76
1,2,3-Trichloropropane
Concen: 27.235 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Tgt Ion: 75 Resp: 62465
Ion Ratio Lower Upper
75 100
77 1.2 19.8 59.3#

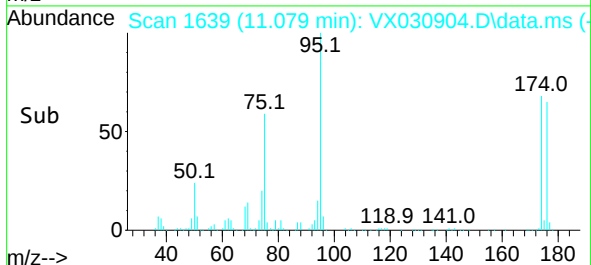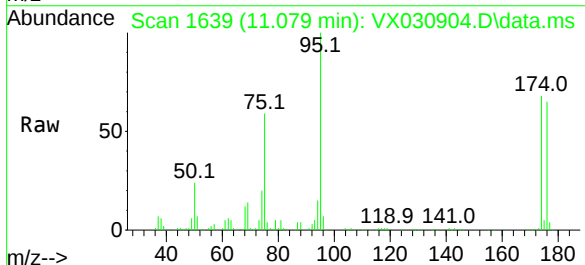

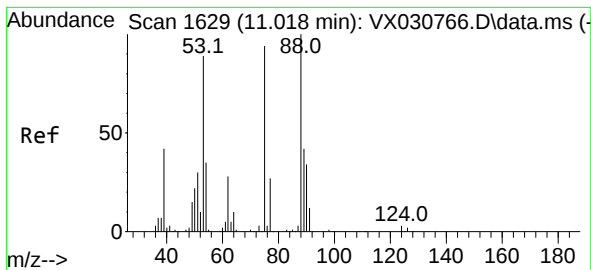

#81
trans-1,4-Dichloro-2-butene
Concen: 87.873 ug/l
RT: 11.079 min Scan# 10
Delta R.T. 0.061 min
Lab File: VX030904.D
Acq: 28 Aug 2022 05:35

Instrument :
MSVOA_X
ClientSampleId :
TT101D1-20220824

Tgt Ion: 75 Resp: 62465
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.8 52.2#

