

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
 Data File : VX030865.D
 Acq On : 27 Aug 2022 13:02
 Operator : JC/MD
 Sample : VX0827WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0827WBL01

Quant Time: Aug 29 01:08:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 26 02:03:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	216348	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	365543	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	323982	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	142099	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	140179	55.084	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	110.160%
35) Dibromofluoromethane	5.391	113	116075	51.668	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.340%
50) Toluene-d8	8.653	98	436394	55.744	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	111.480%
62) 4-Bromofluorobenzene	11.085	95	142630	48.937	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
Data File : VX030865.D
Acq On : 27 Aug 2022 13:02
Operator : JC/MD
Sample : VX0827WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL01

Quant Time: Aug 29 01:08:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 26 02:03:28 2022
Response via : Initial Calibration




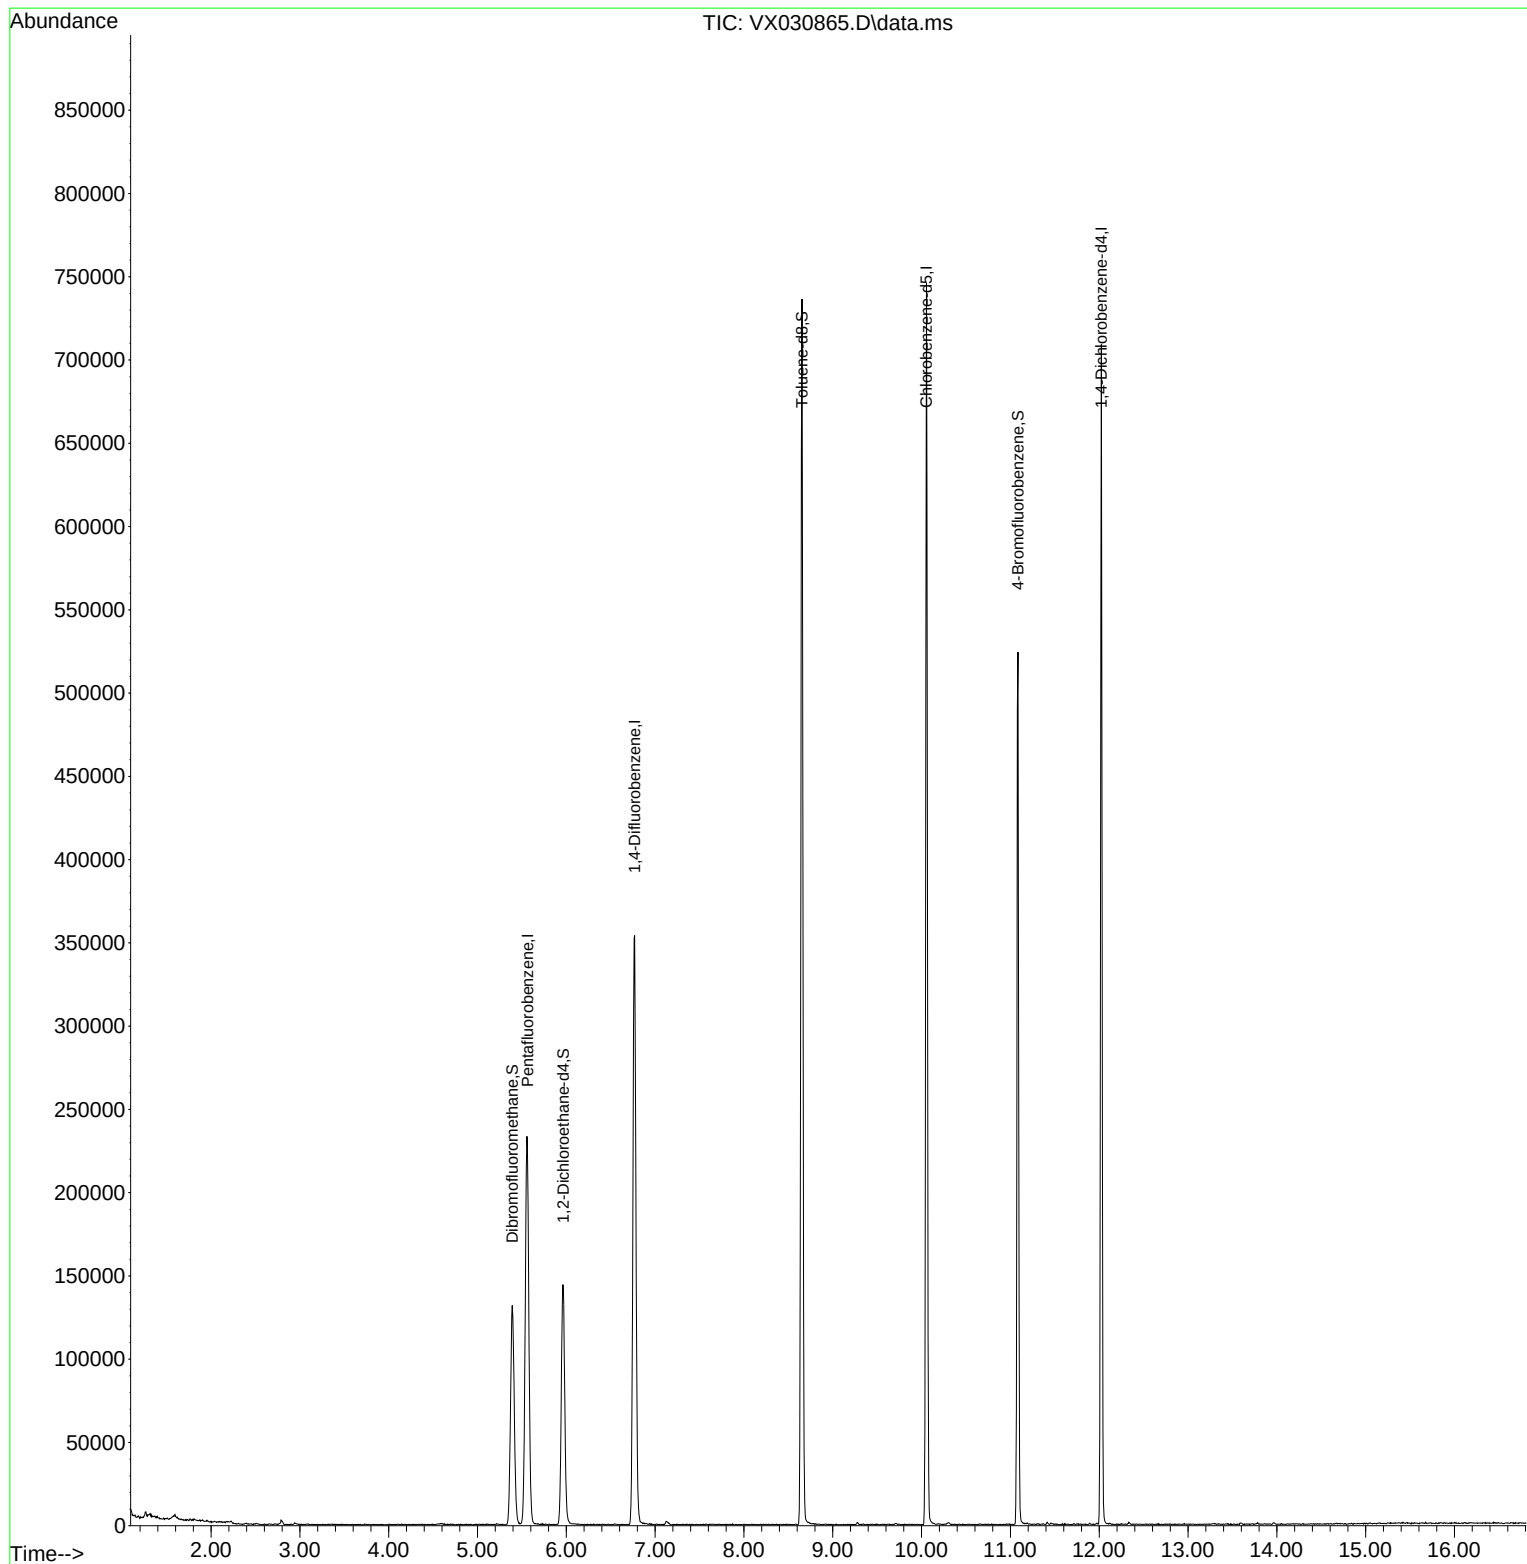


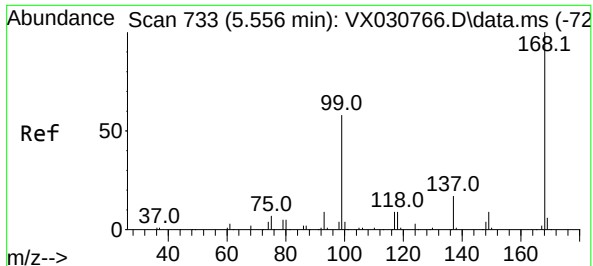

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL01


Tgt Ion:168 Resp: 216348
Ion Ratio Lower Upper
168 100
99 55.7 44.0 66.0

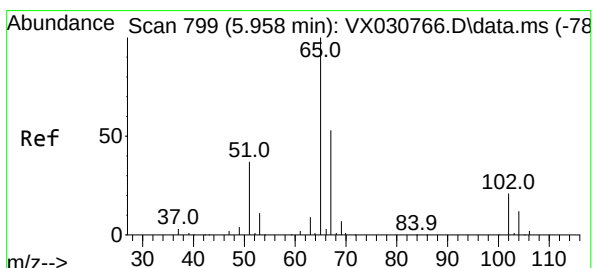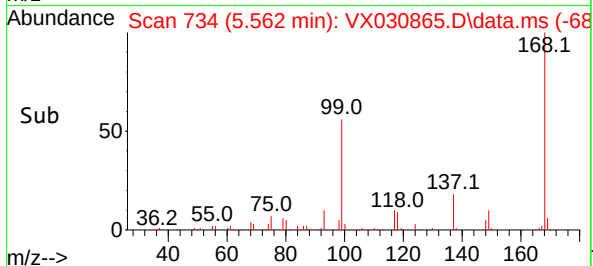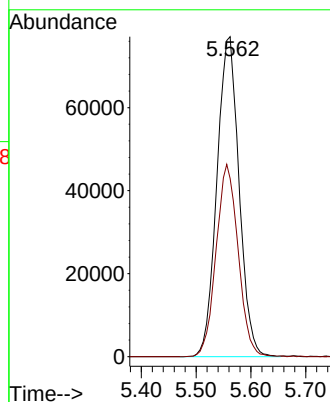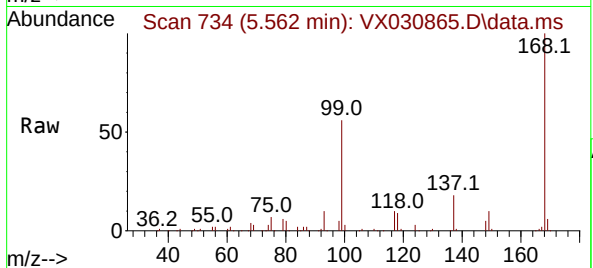

#33
1,2-Dichloroethane-d4
Concen: 55.084 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.006 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02

Tgt Ion: 65 Resp: 140179
Ion Ratio Lower Upper
65 100
67 54.2 0.0 109.6


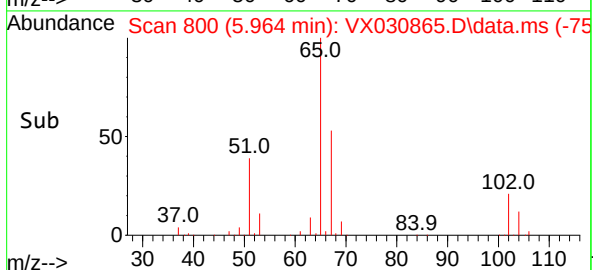
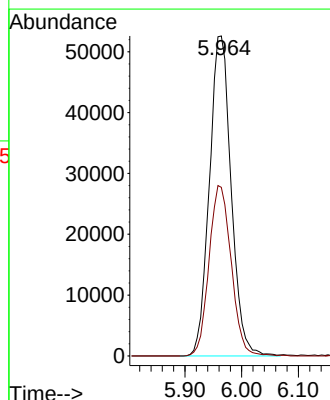
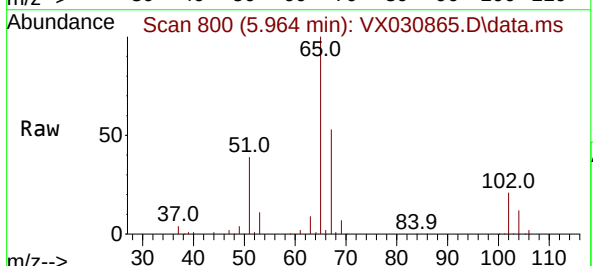


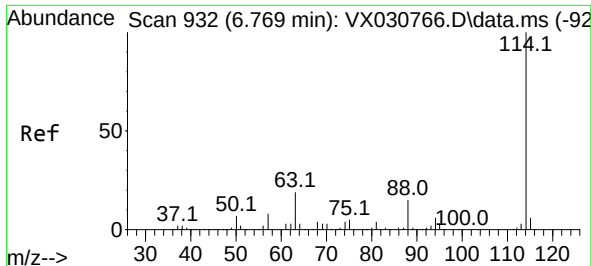

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL01


Tgt Ion:114 Resp: 365543
Ion Ratio Lower Upper
114 100
63 20.3 0.0 38.4
88 15.9 0.0 31.8

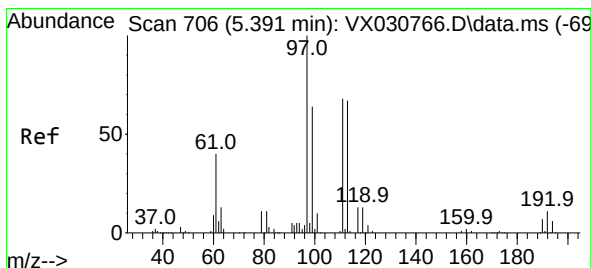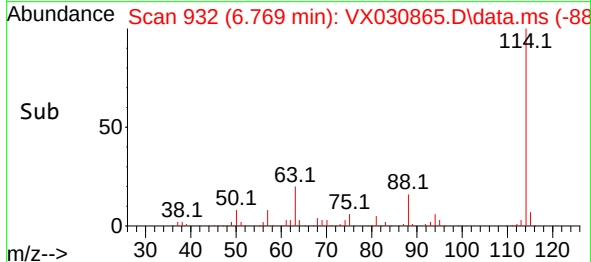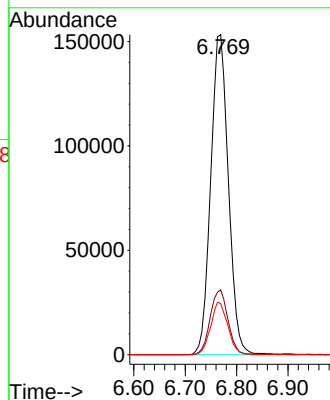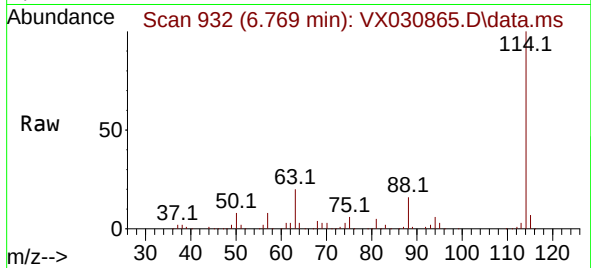

#35
Dibromofluoromethane
Concen: 51.668 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02

Tgt Ion:113 Resp: 116075
Ion Ratio Lower Upper
113 100
111 103.5 83.2 124.8
192 18.3 14.8 22.2


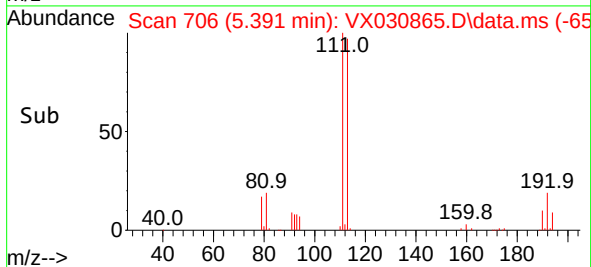
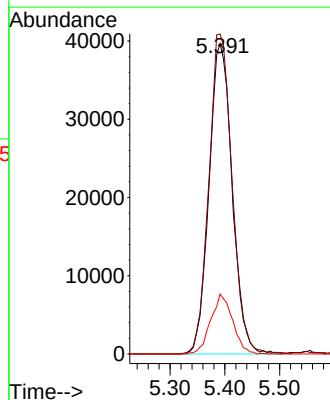
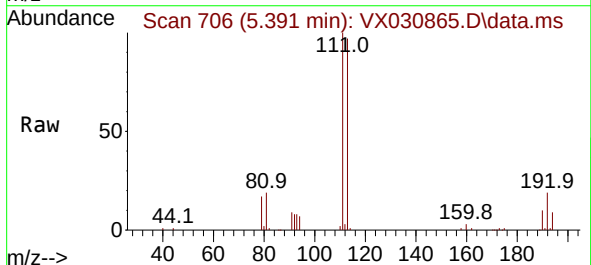


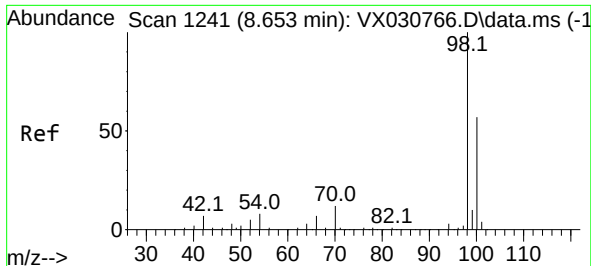

#50
Toluene-d8
Concen: 55.744 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02




Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL01


Tgt Ion: 98 Resp: 436394
Ion Ratio Lower Upper
98 100
100 63.8 52.3 78.5

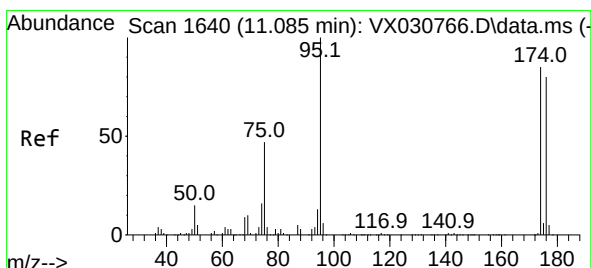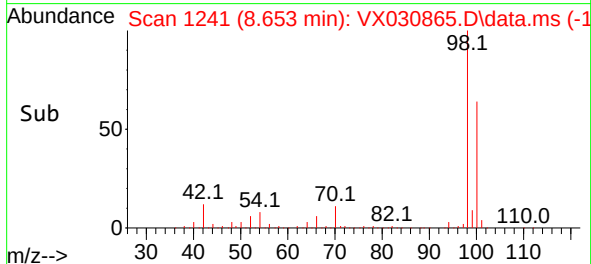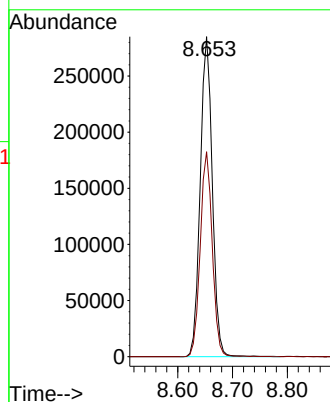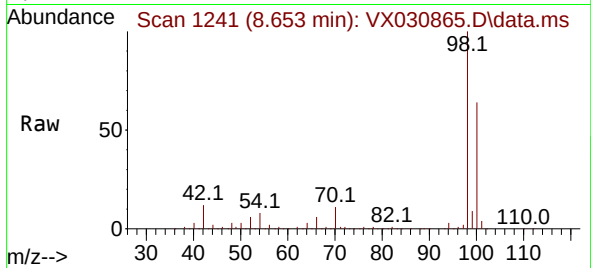

#62
4-Bromofluorobenzene
Concen: 48.937 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02

Tgt Ion: 95 Resp: 142630
Ion Ratio Lower Upper
95 100
174 77.6 0.0 149.0
176 73.7 0.0 146.0


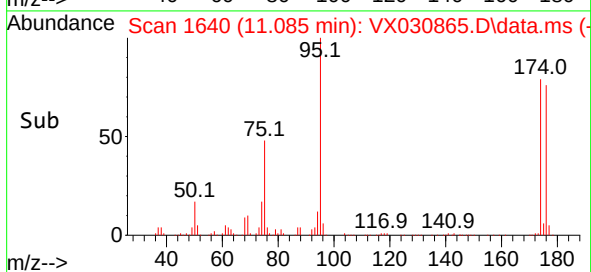
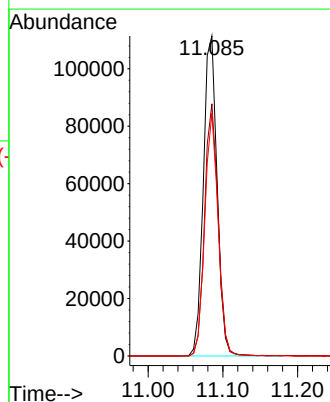
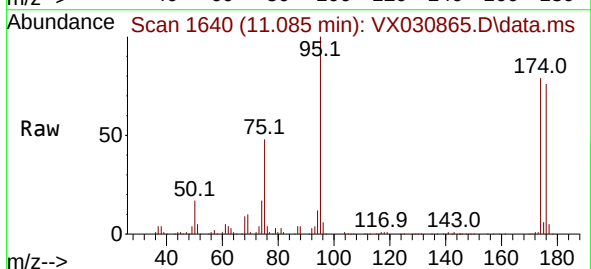


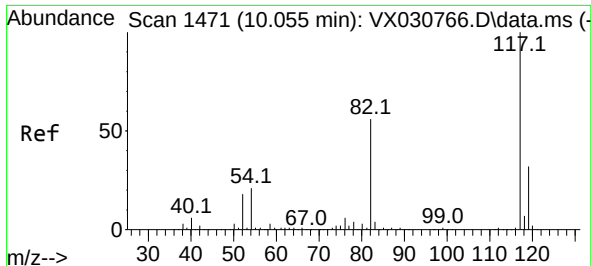

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02

Instrument :
MSVOA_X
ClientSampleId :
VX0827WBL01

Tgt Ion:117 Resp: 323982
Ion Ratio Lower Upper
117 100
82 57.4 42.7 64.1
119 33.0 25.4 38.2

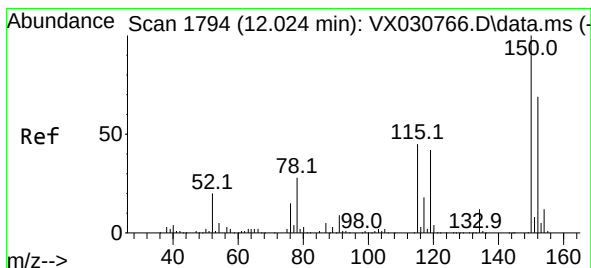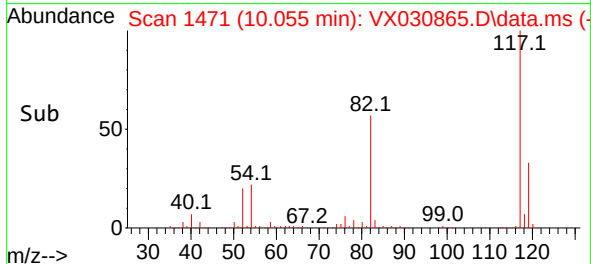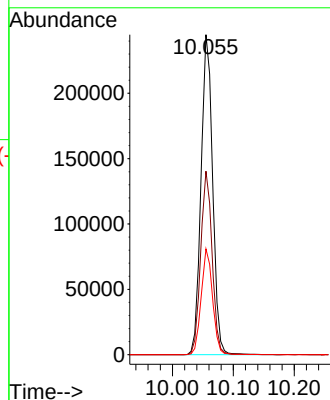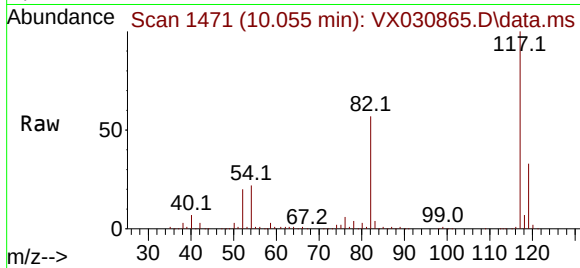

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX030865.D
Acq: 27 Aug 2022 13:02

Tgt Ion:152 Resp: 142099
Ion Ratio Lower Upper
152 100
115 59.3 40.5 121.5
150 157.4 0.0 347.0

