

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
 Data File : VX030898.D
 Acq On : 28 Aug 2022 03:14
 Operator : JC/MD
 Sample : N4360-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT172S1-20220823

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
 Title : SW846 8260

Signal : TIC: VX030898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	196	204	210	rBV4	8786	16493	1.62%	0.280%
2	5.391	690	706	722	rBV	118112	345954	34.04%	5.873%
3	5.556	722	733	747	rVV	208214	574821	56.56%	9.758%
4	5.958	789	799	814	rBV	136633	368655	36.28%	6.258%
5	6.763	922	931	952	rBV	324038	771530	75.92%	13.097%
6	7.129	982	991	1006	rBV2	239803	508454	50.03%	8.631%
7	8.653	1233	1241	1249	rBV	658125	1016270	100.00%	17.252%
8	9.275	1339	1343	1349	rBV2	14430	22797	2.24%	0.387%
9	10.055	1465	1471	1485	rBV	667953	889765	87.55%	15.104%
10	11.085	1634	1640	1648	rBV	480882	627321	61.73%	10.649%
11	12.024	1789	1794	1802	rBV	605557	748755	73.68%	12.711%




Sum of corrected areas: 5890815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
Data File : VX030898.D
Acq On : 28 Aug 2022 03:14
Operator : JC/MD
Sample : N4360-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT172S1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

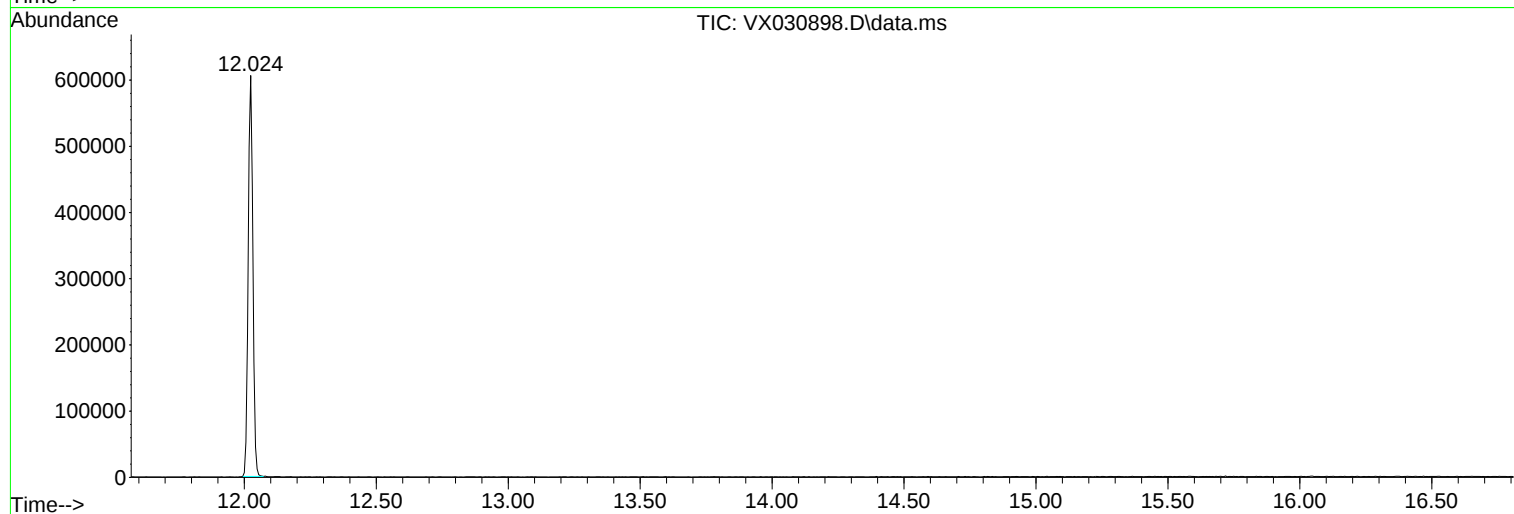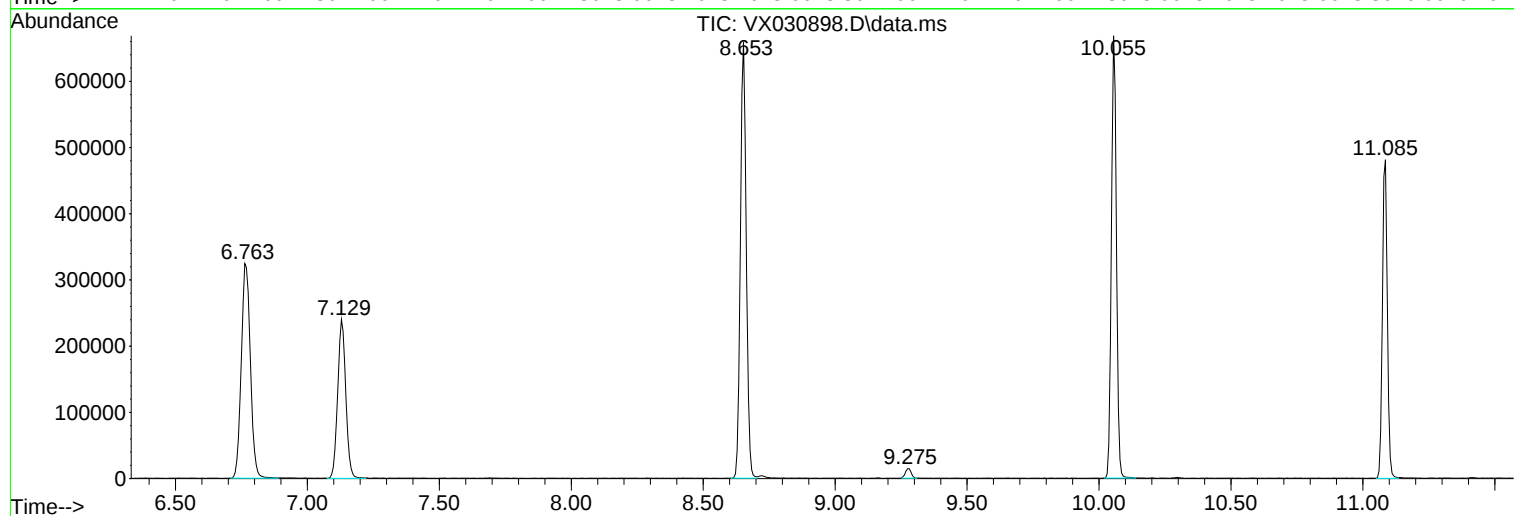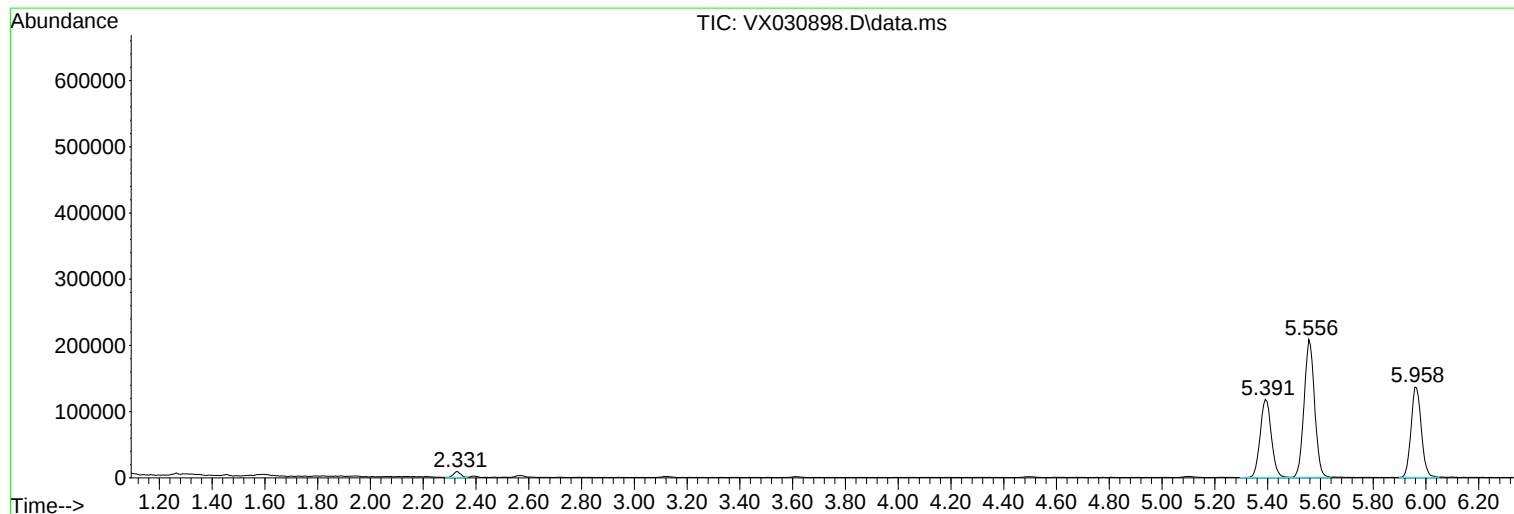

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
Data File : VX030898.D
Acq On : 28 Aug 2022 03:14
Operator : JC/MD
Sample : N4360-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT172S1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
Data File : VX030898.D
Acq On : 28 Aug 2022 03:14
Operator : JC/MD
Sample : N4360-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT172S1-20220823

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------