
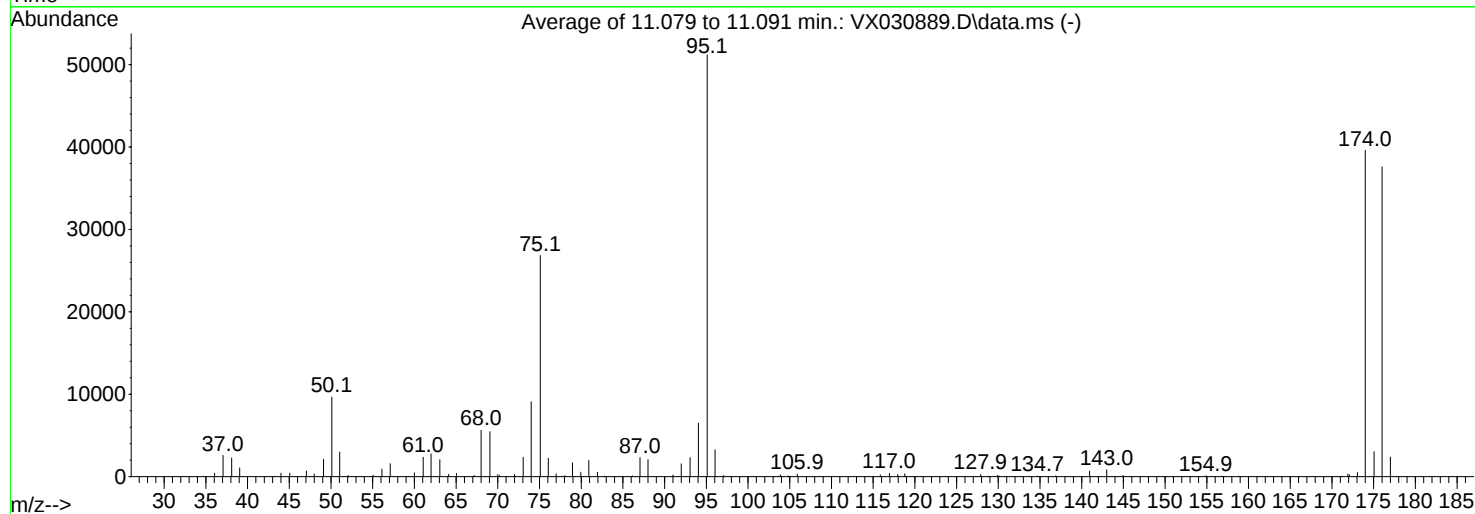


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082722\
Data File : VX030889.D
Acq On : 27 Aug 2022 22:56
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X082522W.M
Title : SW846 8260
Last Update : Fri Aug 26 02:03:28 2022

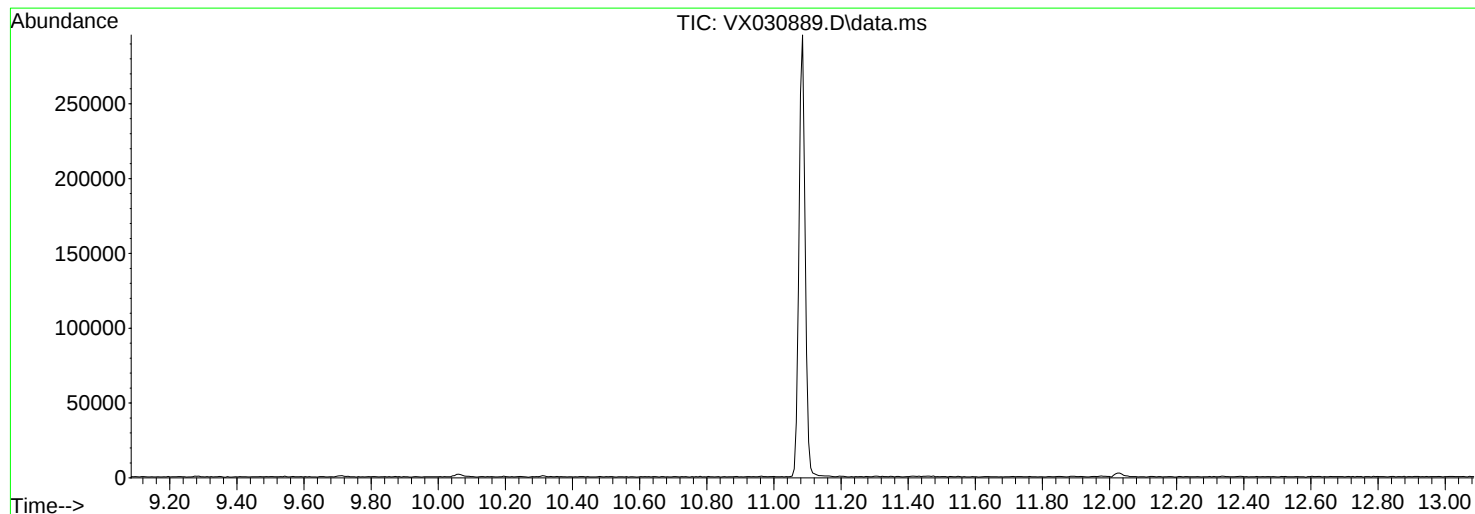

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	9659	PASS
75	95	30	60	52.4	26832	PASS
95	95	100	100	100.0	51179	PASS
96	95	5	9	6.4	3258	PASS
173	174	0.00	2	1.3	509	PASS
174	95	50	100	77.3	39584	PASS
175	174	5	9	7.6	3028	PASS
176	174	95	101	95.0	37587	PASS
177	176	5	9	6.3	2360	PASS