


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082818\
 Data File : VX004267.D
 Acq On : 28 Aug 2018 10:12
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
 Title : SW846 8260
 Last Update : Thu Aug 23 05:39:44 2018

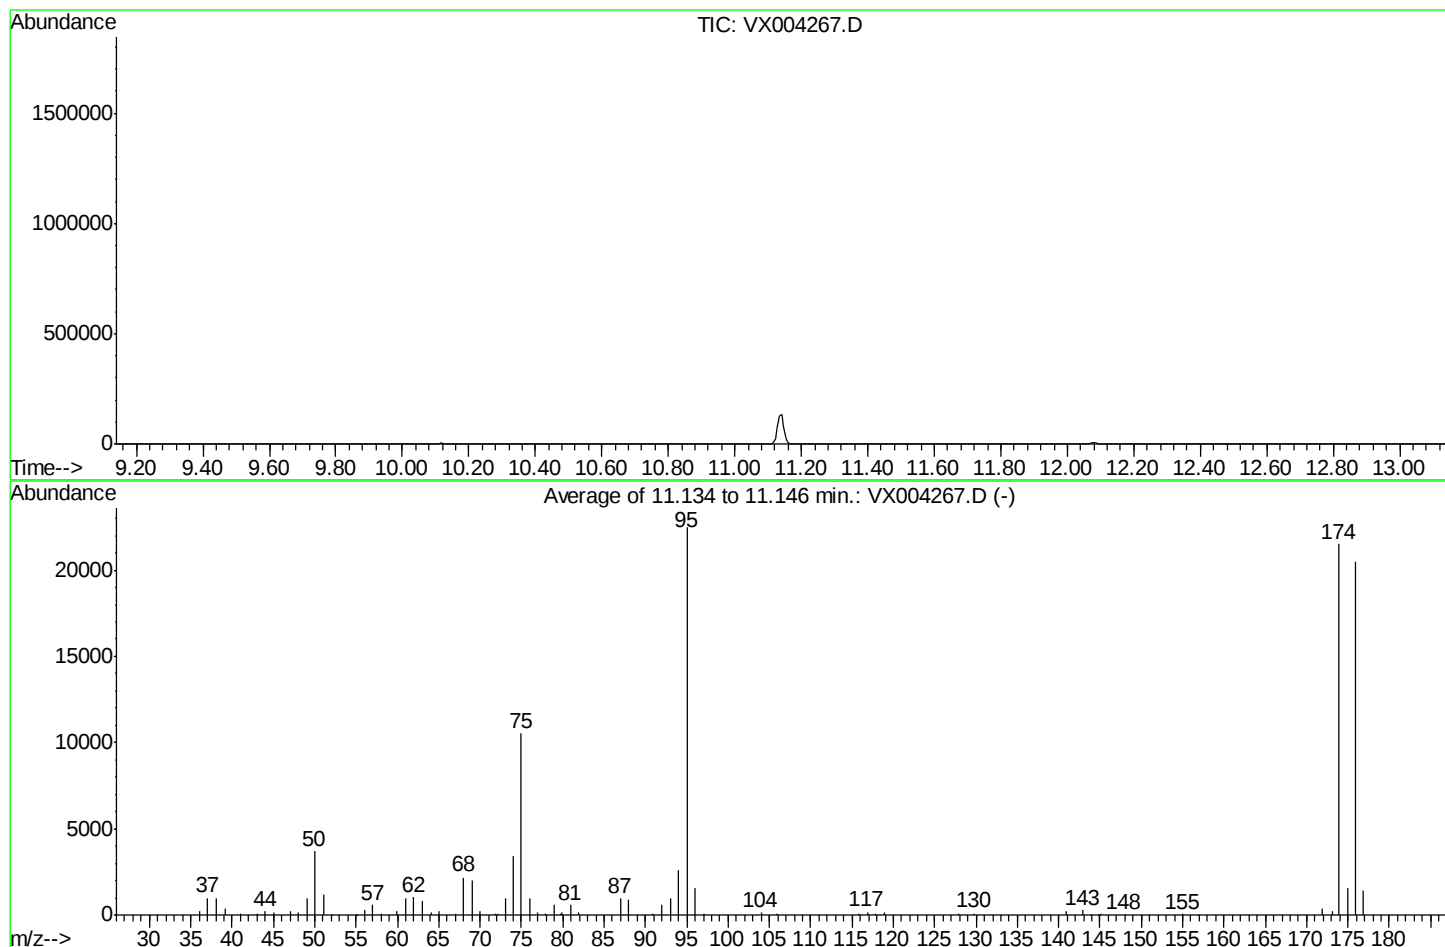

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	3678	PASS
75	95	30	60	46.9	10534	PASS
95	95	100	100	100.0	22481	PASS
96	95	5	9	6.9	1551	PASS
173	174	0.00	2	1.1	226	PASS
174	95	50	100	95.7	21520	PASS
175	174	5	9	7.3	1575	PASS
176	174	95	101	95.3	20498	PASS
177	176	5	9	6.9	1414	PASS