


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082819\
 Data File : VX011867.D
 Acq On : 28 Aug 2019 09:51
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_X/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082819S.M
 Title : SW846 8260
 Last Update : Wed Aug 28 10:09:52 2019

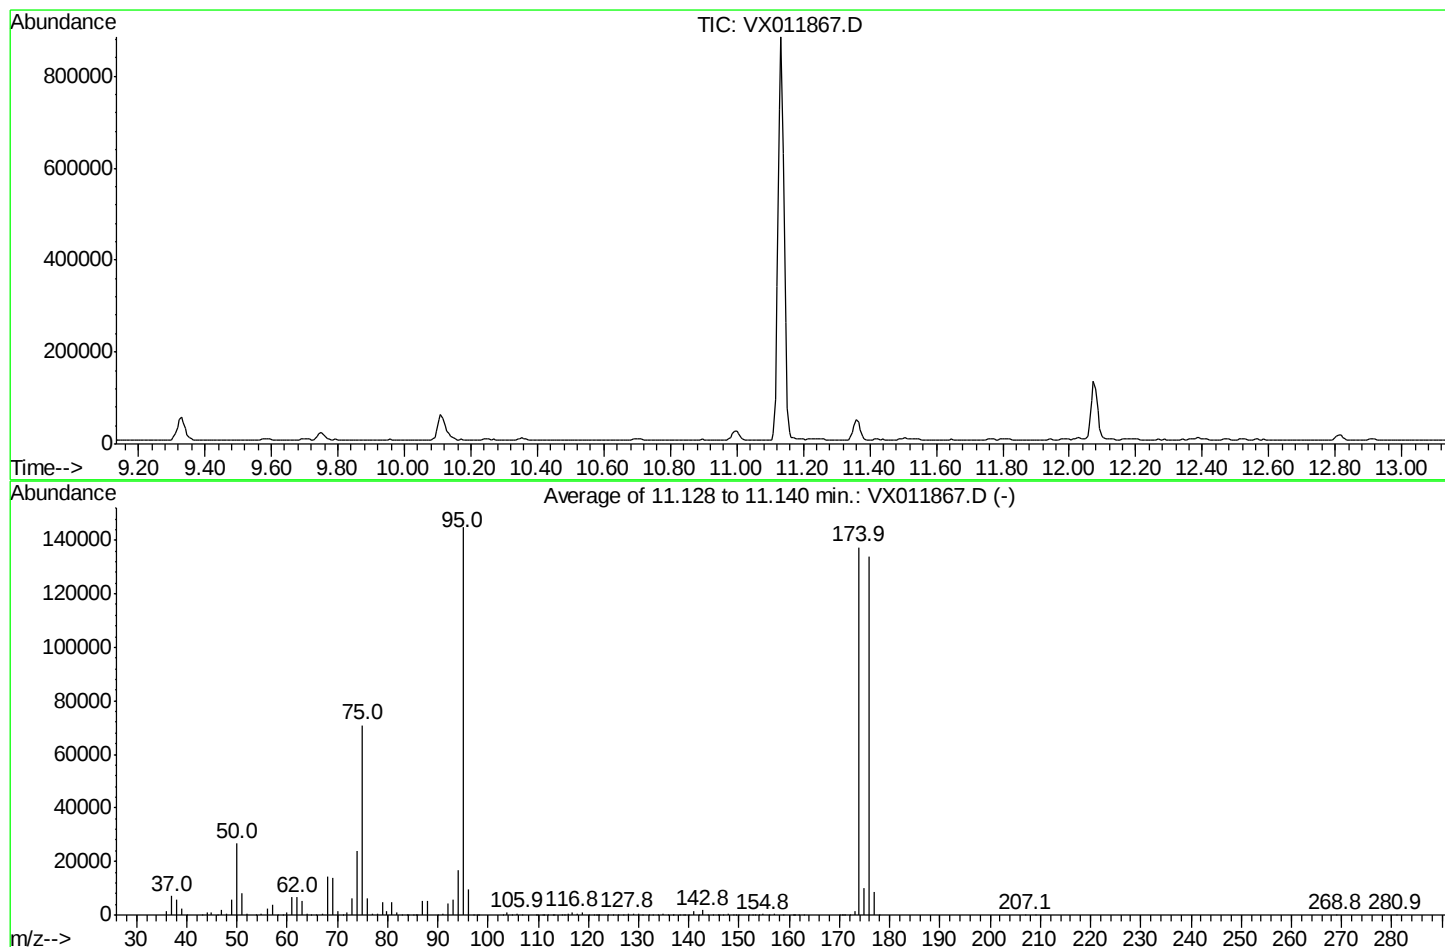

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	26703	PASS
75	95	30	60	48.9	70899	PASS
95	95	100	100	100.0	144847	PASS
96	95	5	9	6.5	9450	PASS
173	174	0.00	2	1.1	1496	PASS
174	95	50	100	94.9	137394	PASS
175	174	5	9	7.4	10099	PASS
176	174	95	101	97.7	134173	PASS
177	176	5	9	6.5	8668	PASS