


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX082823\
 Data File : VX037308.D
 Acq On : 28 Aug 2023 23:27
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081723W.M
 Title : SW846 8260
 Last Update : Fri Aug 18 09:30:38 2023

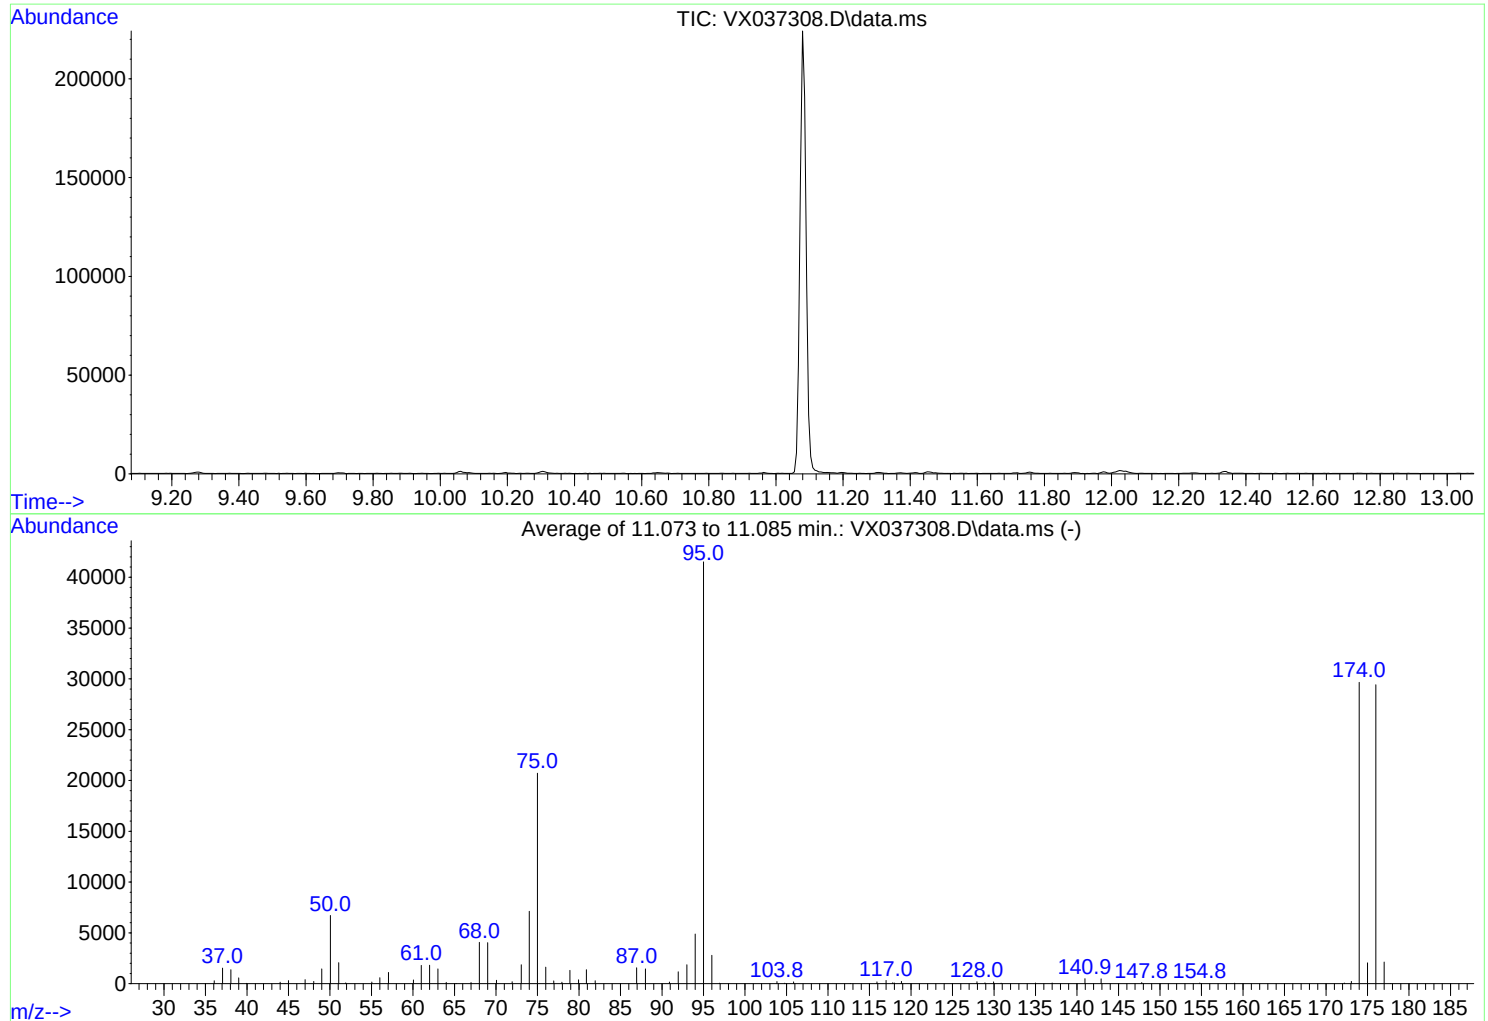

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	6710	PASS
75	95	30	60	49.9	20717	PASS
95	95	100	100	100.0	41515	PASS
96	95	5	9	6.7	2795	PASS
173	174	0.00	2	0.7	214	PASS
174	95	50	100	71.4	29661	PASS
175	174	5	9	6.9	2053	PASS
176	174	95	101	99.2	29413	PASS
177	176	5	9	7.2	2128	PASS