


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX082918\
Data File : VX004276.D
Acq On : 29 Aug 2018 07:35
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X082218W.M
Title : SW846 8260
Last Update : Thu Aug 23 05:39:44 2018

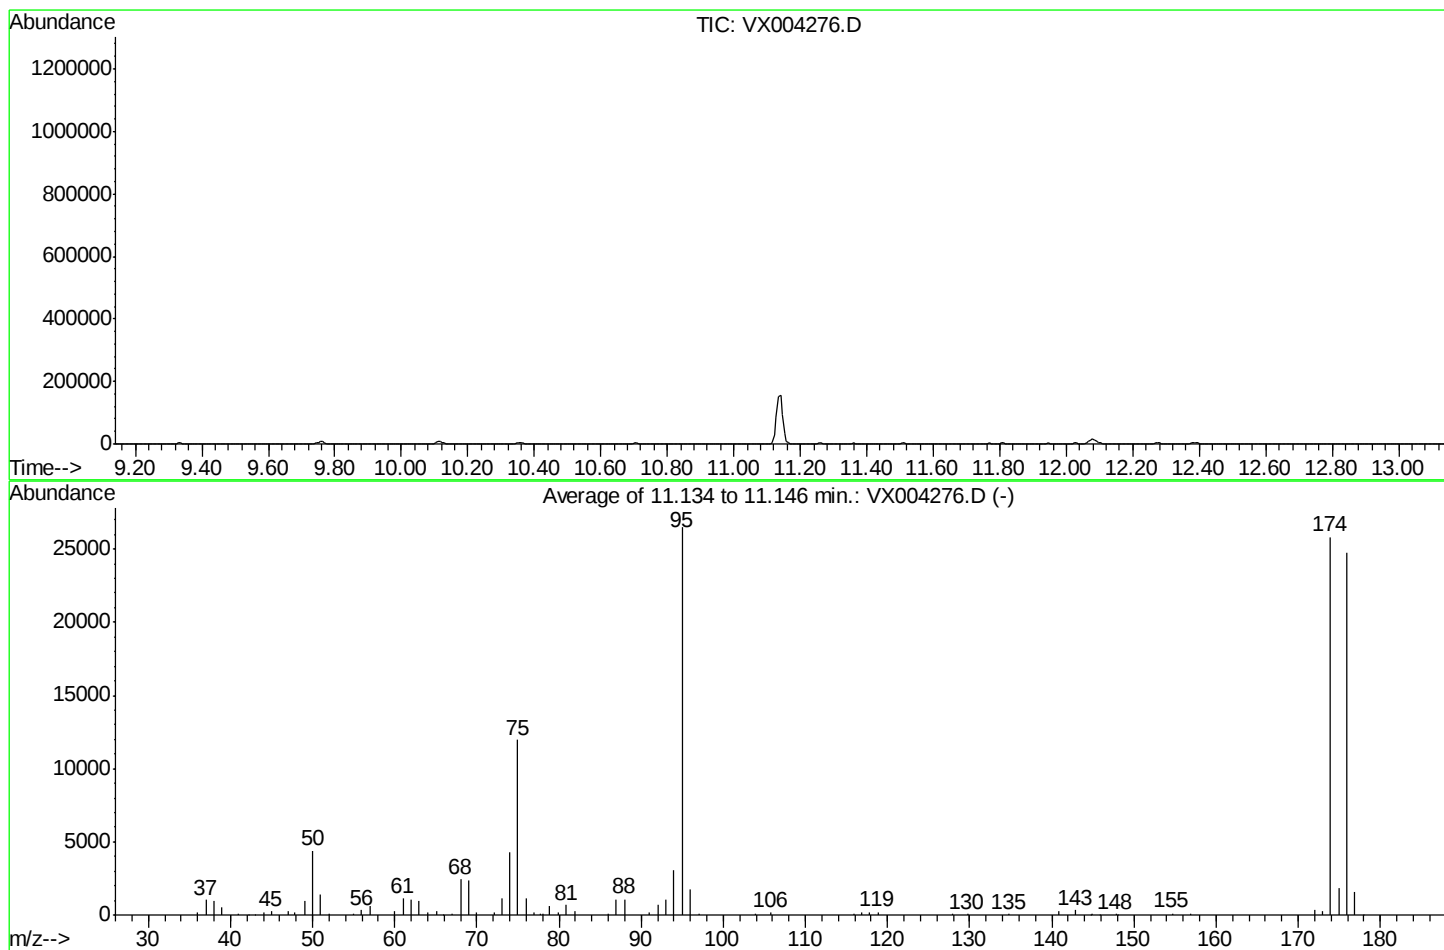

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	4386	PASS
75	95	30	60	45.1	11955	PASS
95	95	100	100	100.0	26485	PASS
96	95	5	9	6.5	1730	PASS
173	174	0.00	2	0.9	234	PASS
174	95	50	100	97.4	25805	PASS
175	174	5	9	7.0	1796	PASS
176	174	95	101	95.8	24709	PASS
177	176	5	9	6.5	1618	PASS